

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101223\
 Data File : VX038264.D
 Acq On : 12 Oct 2023 18:09
 Operator : JC/MD
 Sample : 04875-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GW-13-37-40

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038264.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.355	39	44	49	rBV2	3665	7188	1.10%	0.194%
2	5.025	638	646	655	rBV5	3599	11710	1.79%	0.316%
3	5.391	694	706	721	rBV	75413	220268	33.63%	5.935%
4	5.550	722	732	747	rVV	115231	328264	50.11%	8.845%
5	5.958	787	799	814	rBV	83136	223675	34.15%	6.027%
6	6.763	922	931	944	rBV	191396	452187	69.03%	12.184%
7	7.129	984	991	1001	rVB4	10138	23101	3.53%	0.622%
8	8.647	1234	1240	1259	rBV	402420	655064	100.00%	17.651%
9	9.275	1337	1343	1352	rVB2	16485	25794	3.94%	0.695%
10	10.055	1465	1471	1487	rBV	445081	623864	95.24%	16.810%
11	11.079	1634	1639	1650	rBV	365339	485691	74.14%	13.087%
12	12.024	1788	1794	1808	rVB	508972	654432	99.90%	17.634%




Sum of corrected areas: 3711238

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101223\
Data File : VX038264.D
Acq On : 12 Oct 2023 18:09
Operator : JC/MD
Sample : 04875-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-13-37-40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

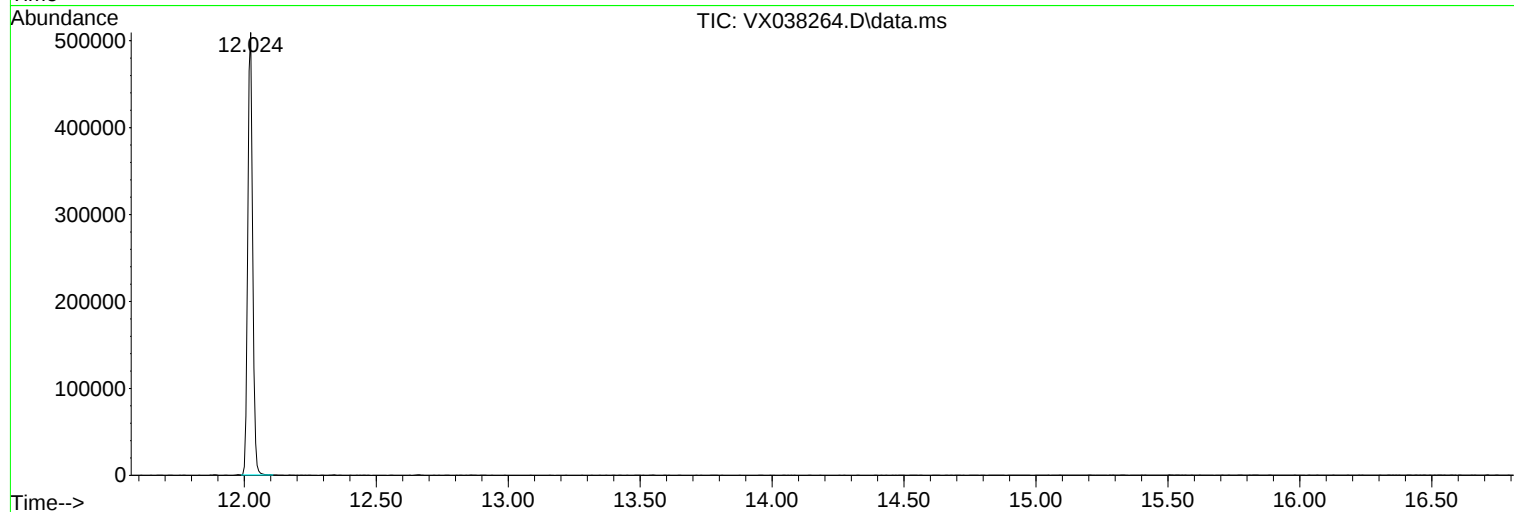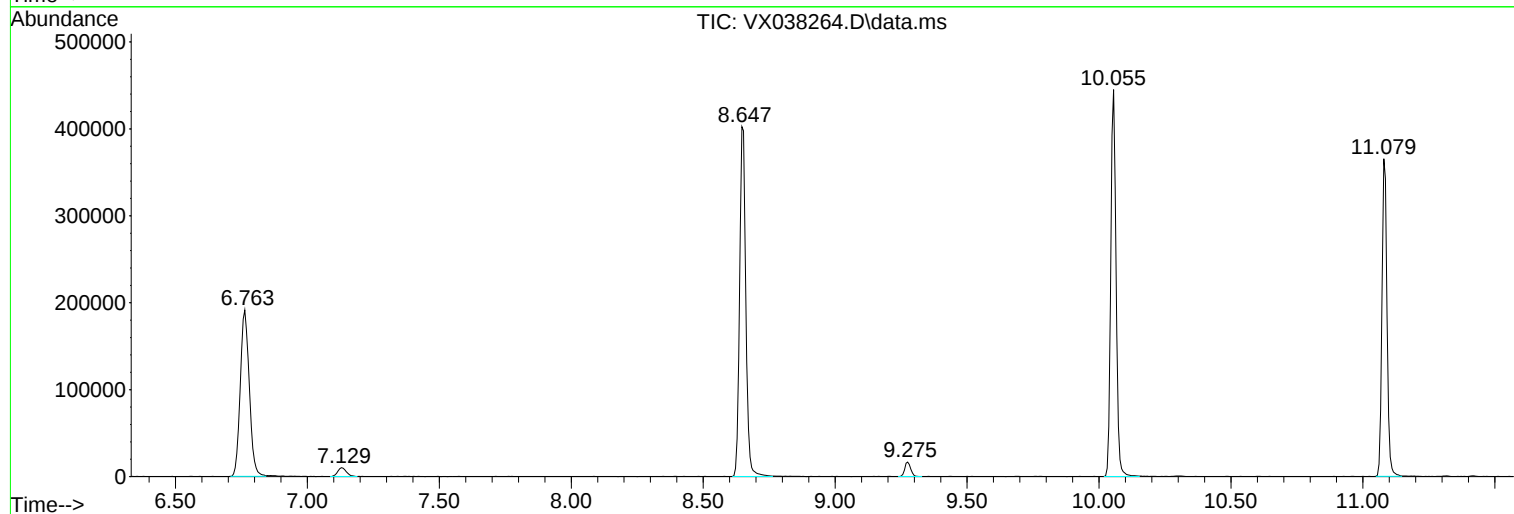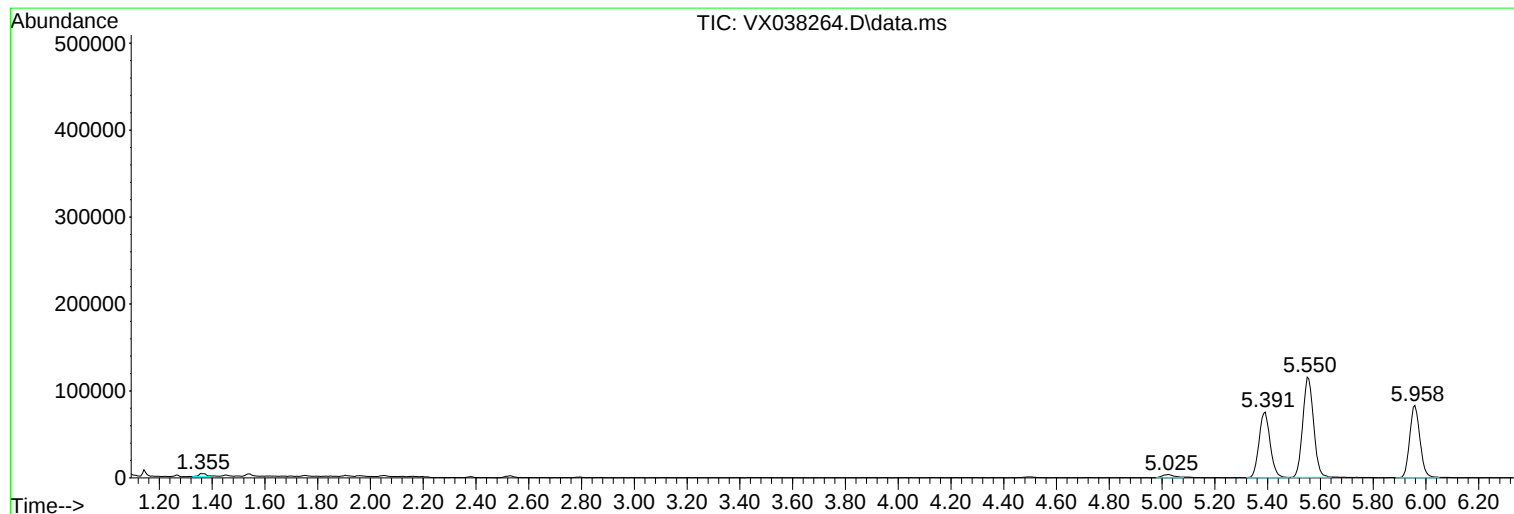

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101223\
Data File : VX038264.D
Acq On : 12 Oct 2023 18:09
Operator : JC/MD
Sample : 04875-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-13-37-40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101223\
Data File : VX038264.D
Acq On : 12 Oct 2023 18:09
Operator : JC/MD
Sample : 04875-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-13-37-40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------