



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101223\
Data File : VX038243.D
Acq On : 12 Oct 2023 08:46
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Title : SW846 8260
Last Update : Thu Oct 05 15:27:13 2023

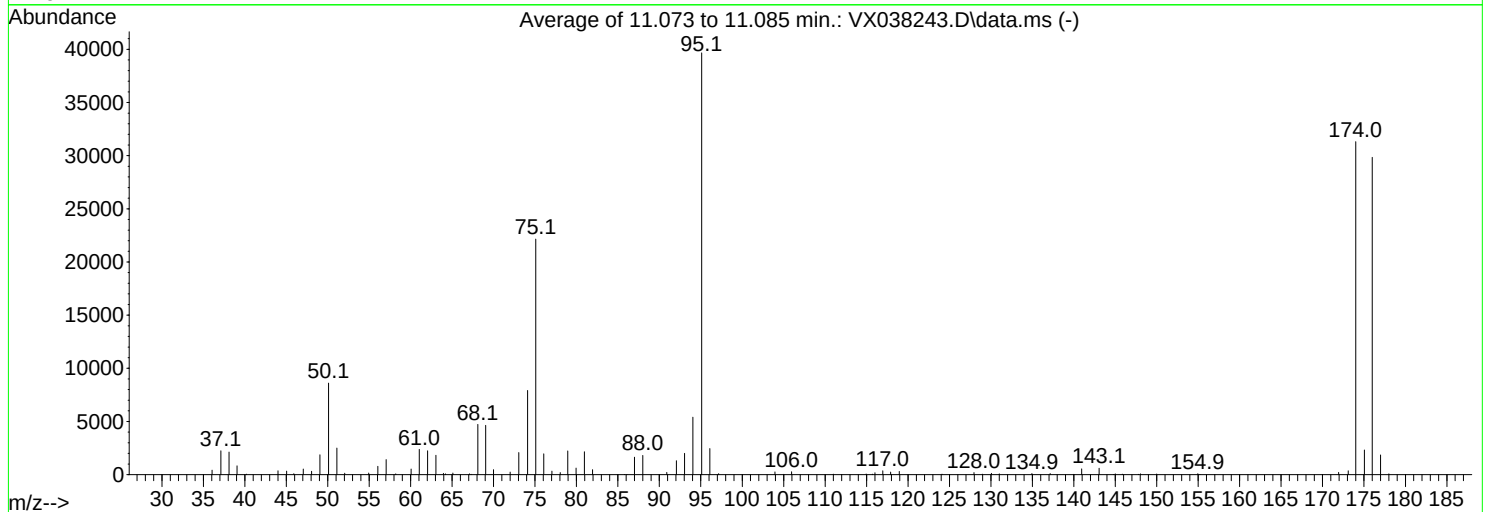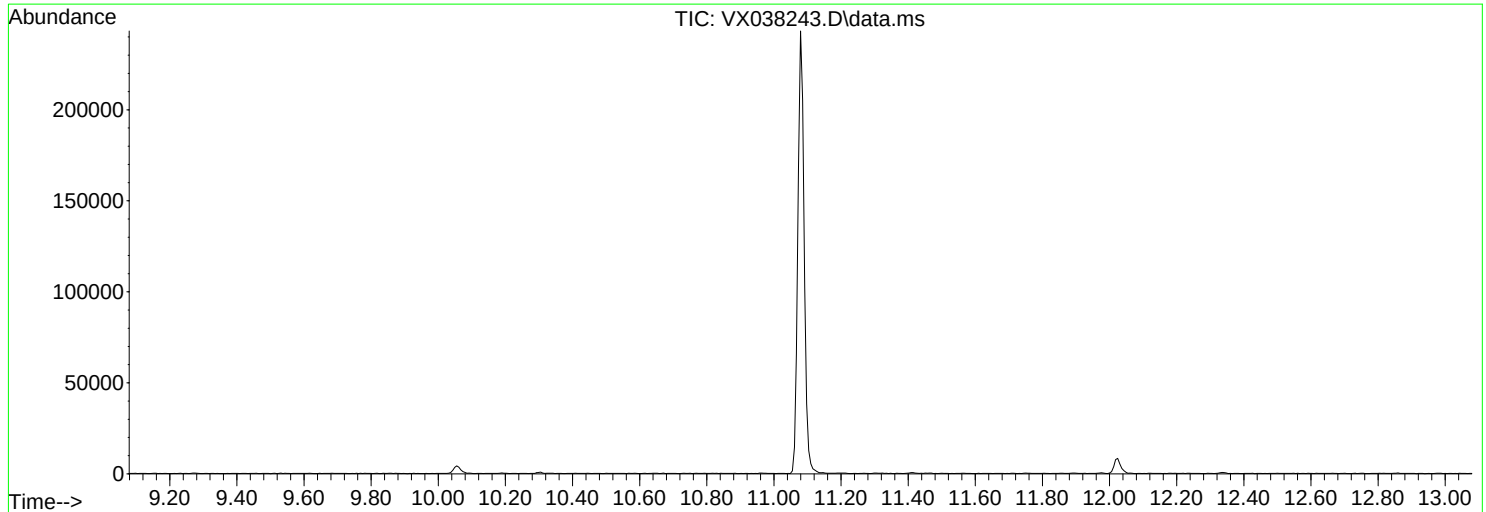

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	8603	PASS
75	95	30	60	55.9	22157	PASS
95	95	100	100	100.0	39669	PASS
96	95	5	9	6.2	2455	PASS
173	174	0.00	2	1.1	359	PASS
174	95	50	100	79.0	31323	PASS
175	174	5	9	7.4	2321	PASS
176	174	95	101	95.3	29840	PASS
177	176	5	9	6.2	1848	PASS