


Acetone

Response Ratio

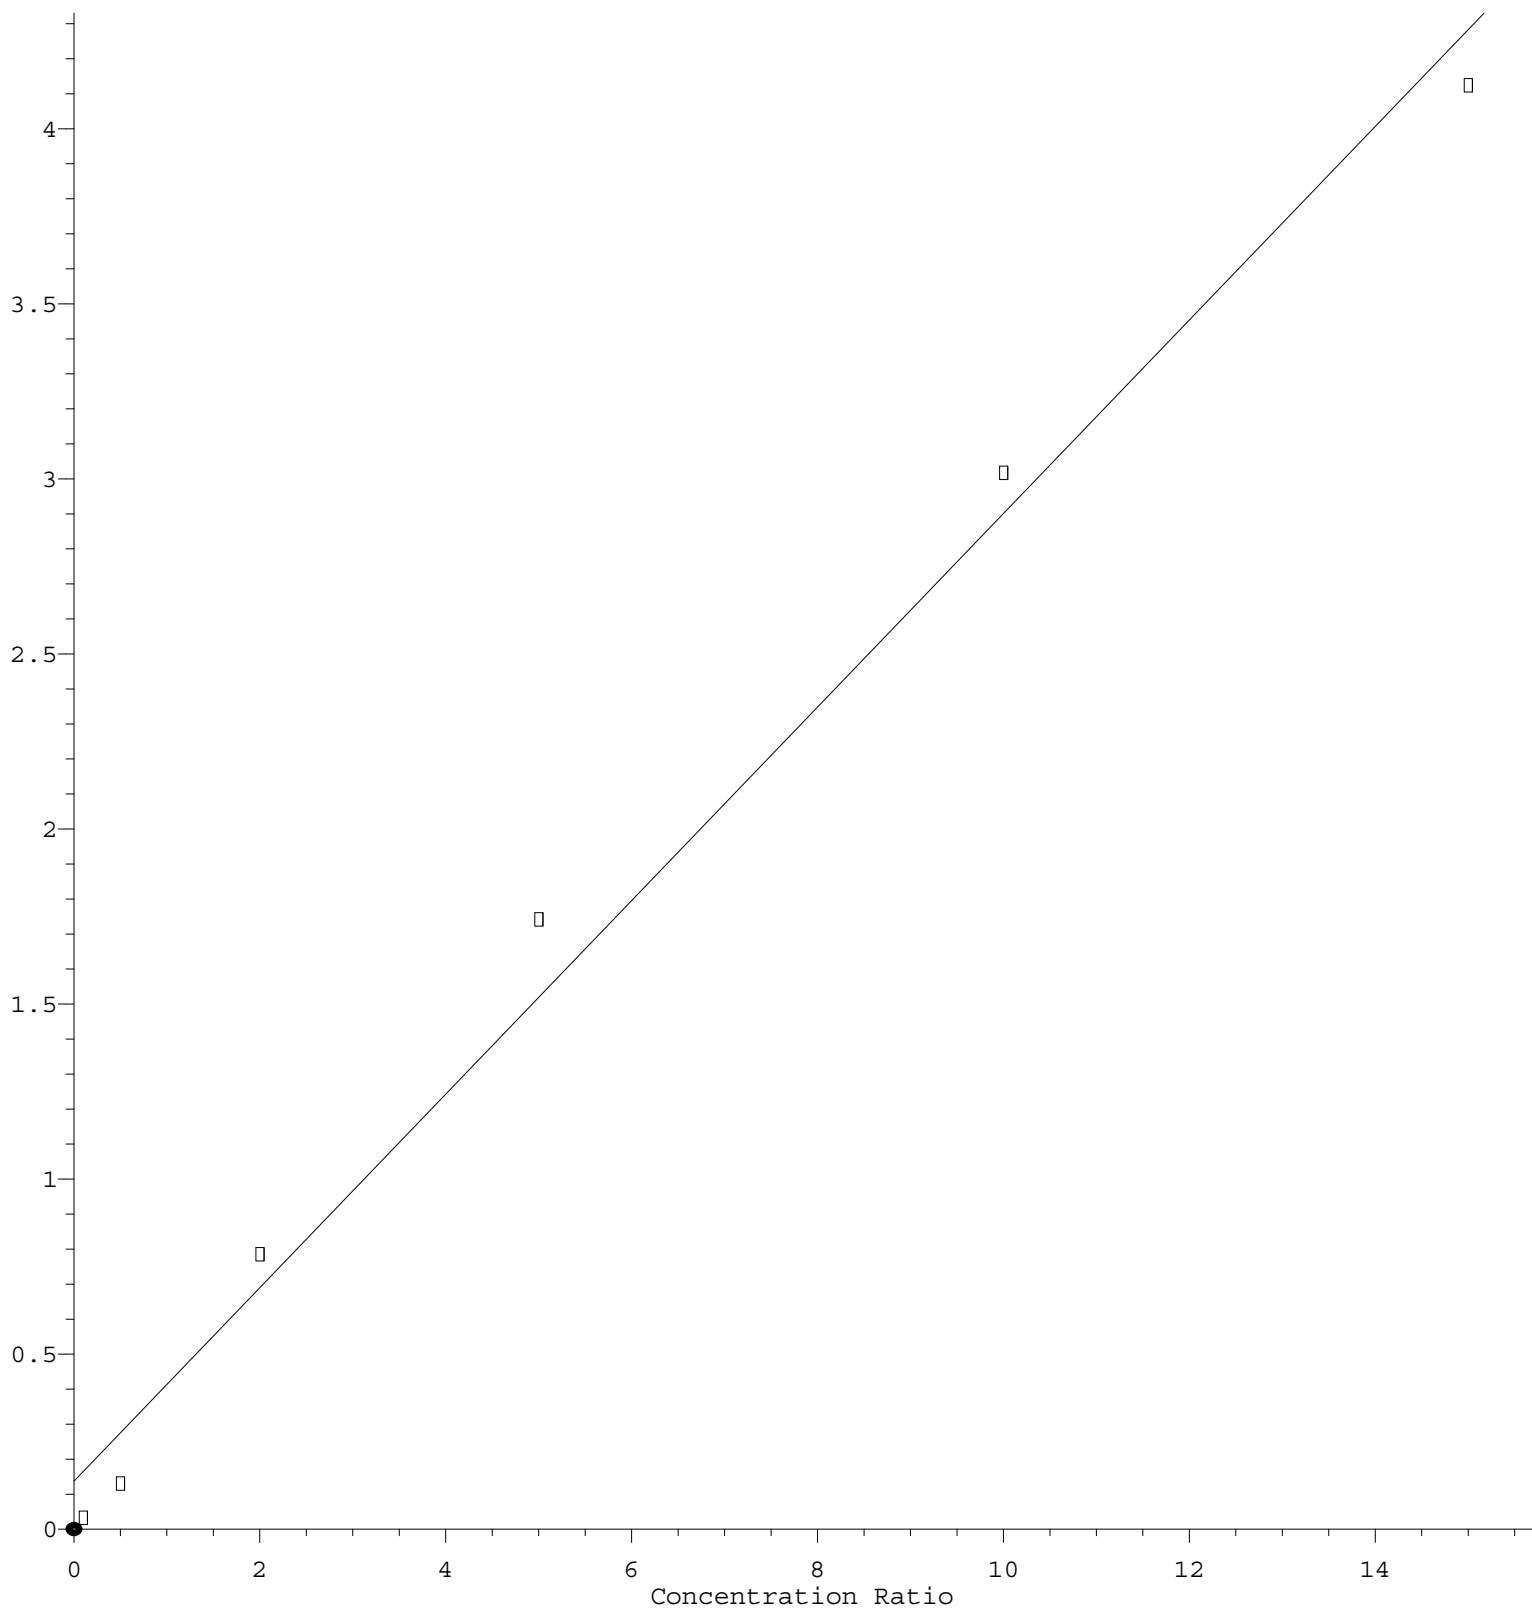

$$\text{Response} = 2.764\text{e-}001 * \text{Amt} + 1.365\text{e-}001$$


Coef of Det (r^2) = 0.990075 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X101321W.M

Calibration Table Last Updated: Thu Oct 14 03:51:38 2021

Ethyl methacrylate

Response Ratio

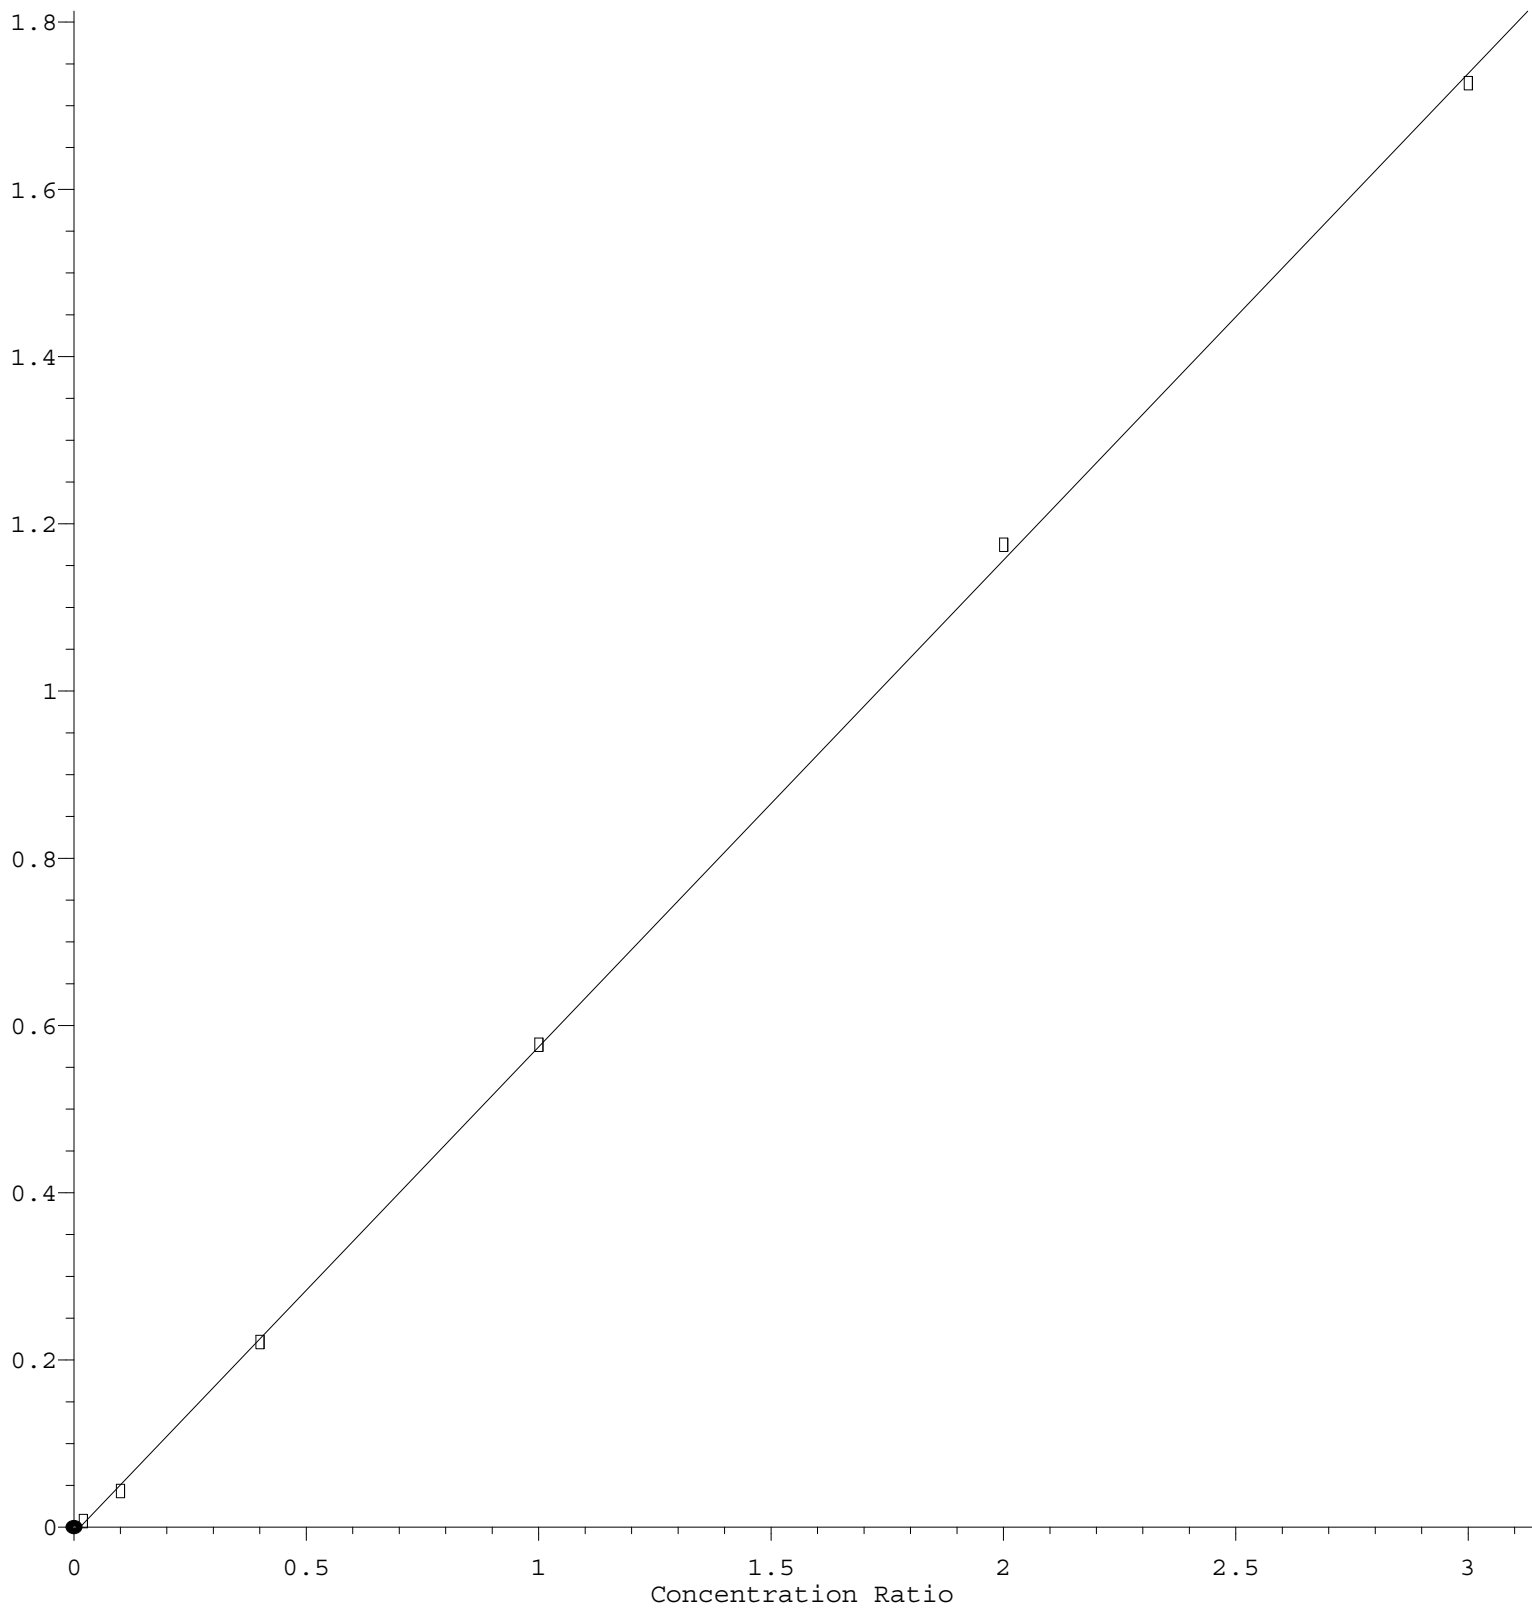

$$\text{Response} = 5.821\text{e-}001 * \text{Amt} - 7.438\text{e-}003$$


Coef of Det (r^2) = 0.999768 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X101321W.M

Calibration Table Last Updated: Thu Oct 14 03:51:38 2021

2-Hexanone

Response Ratio

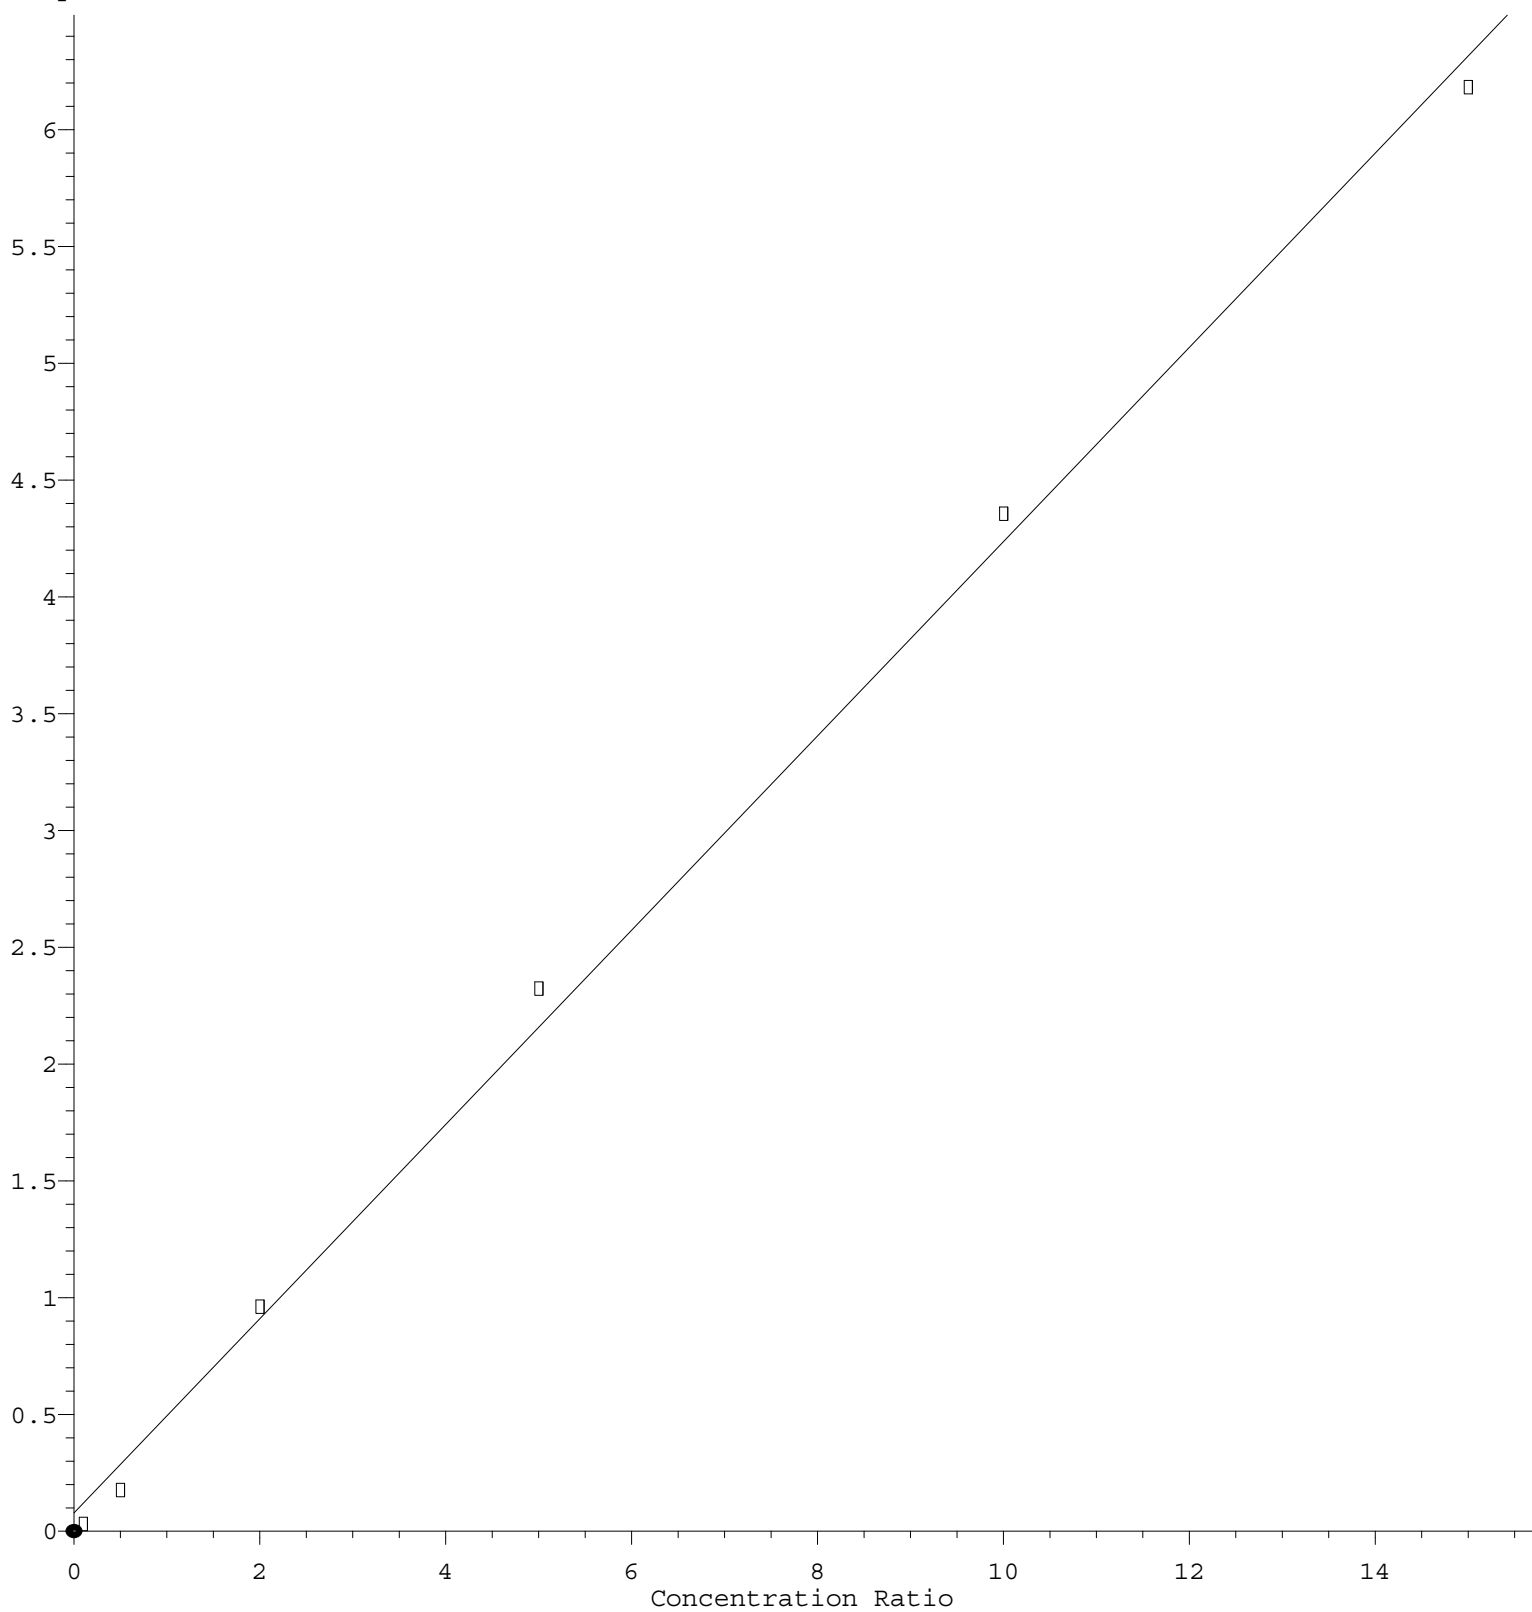

$$\text{Response} = 4.160\text{e-}001 * \text{Amt} + 7.768\text{e-}002$$


Coef of Det (r^2) = 0.997324 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X101321W.M

Calibration Table Last Updated: Thu Oct 14 03:51:38 2021

Dibromochloromethane

Response Ratio

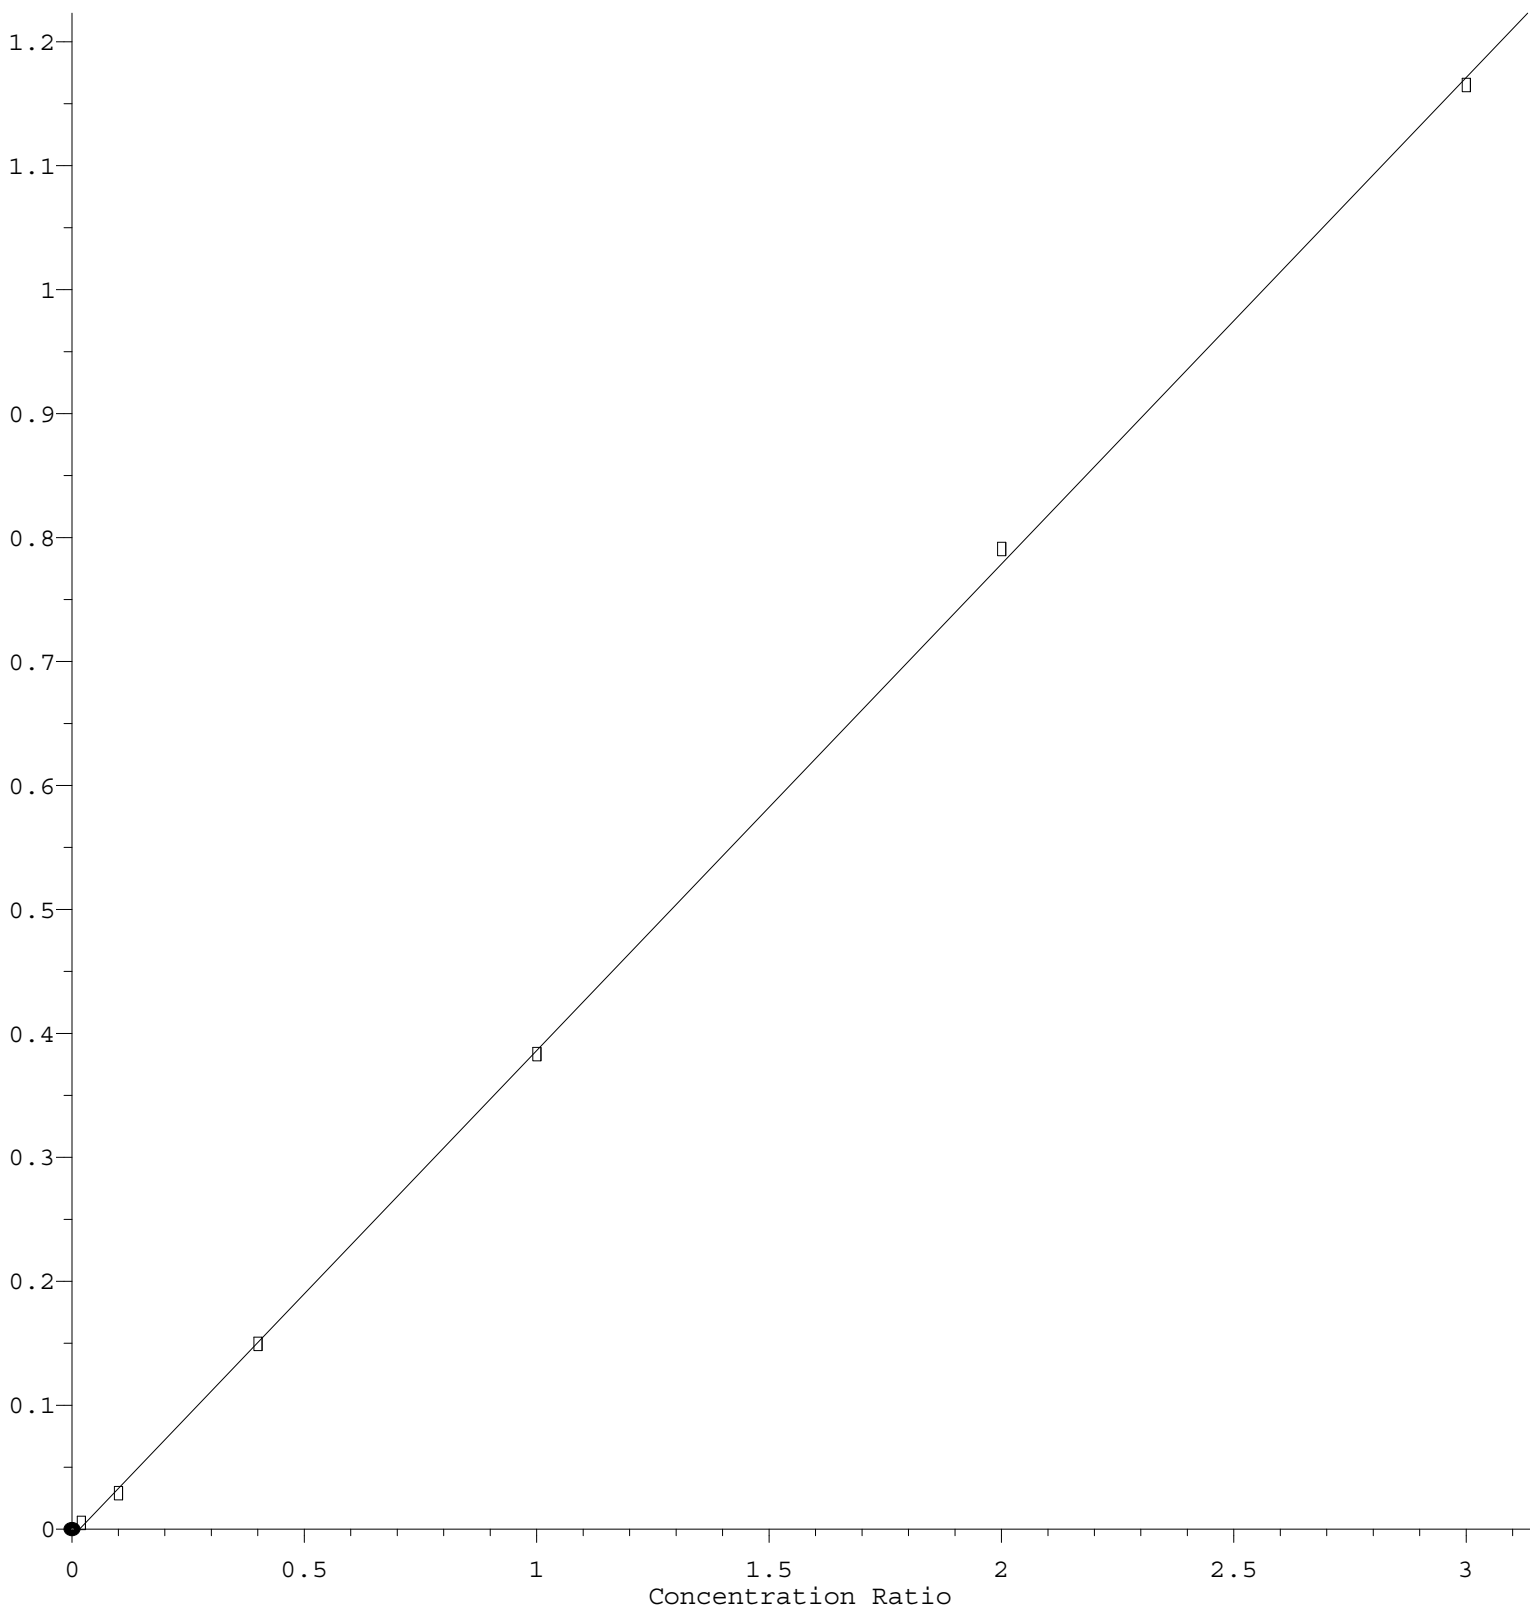

$$\text{Response} = 3.926\text{e-}001 * \text{Amt} - 6.173\text{e-}003$$


Coef of Det (r^2) = 0.999799 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X101321W.M

Calibration Table Last Updated: Thu Oct 14 03:51:38 2021

Styrene

Response Ratio

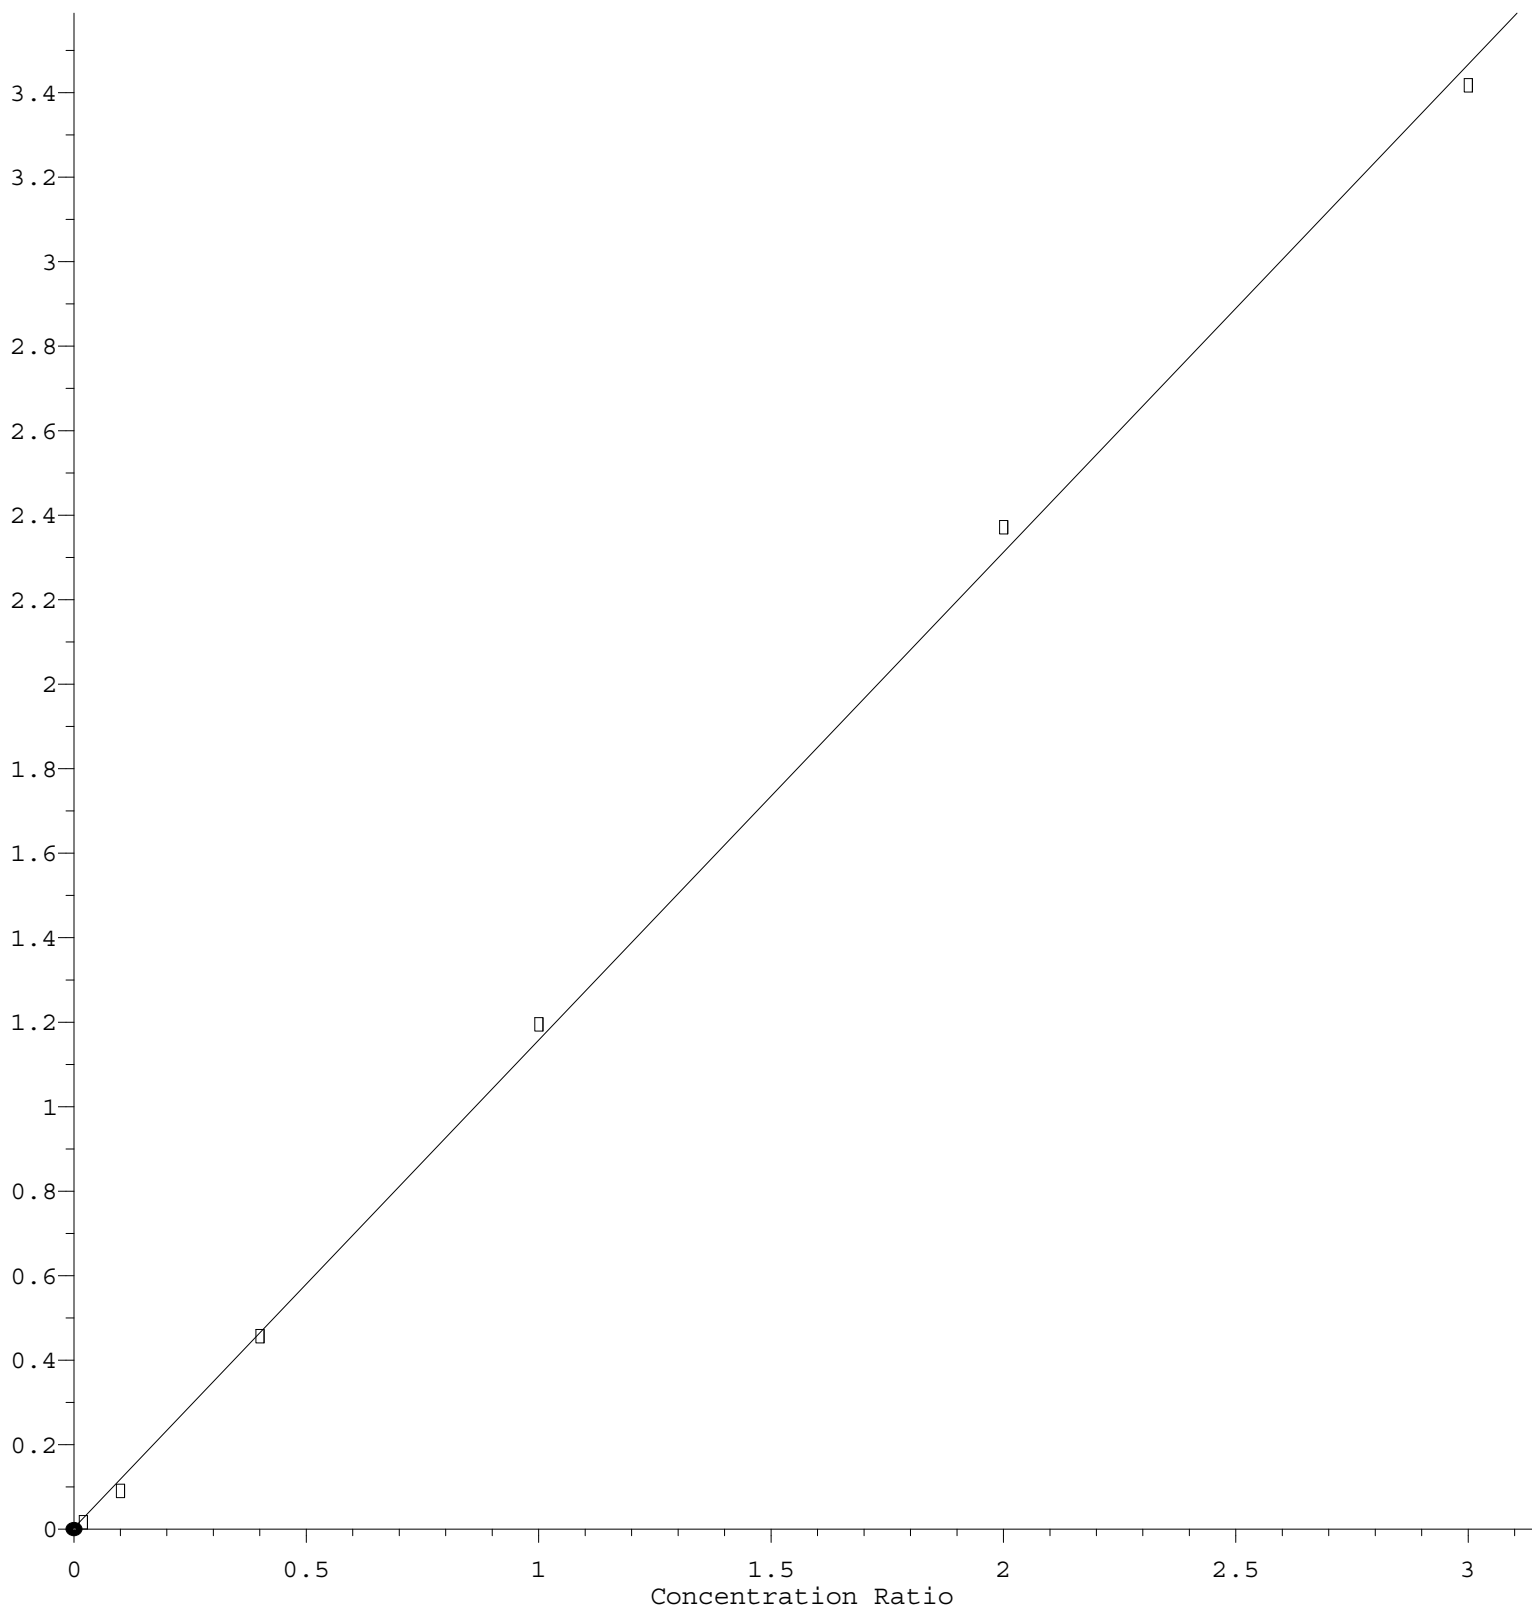

$$\text{Response} = 1.155\text{e}+000 * \text{Amt} + 3.277\text{e}-003$$


Coef of Det (r^2) = 0.999124 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X101321W.M

Calibration Table Last Updated: Thu Oct 14 03:51:38 2021

Bromoform

Response Ratio

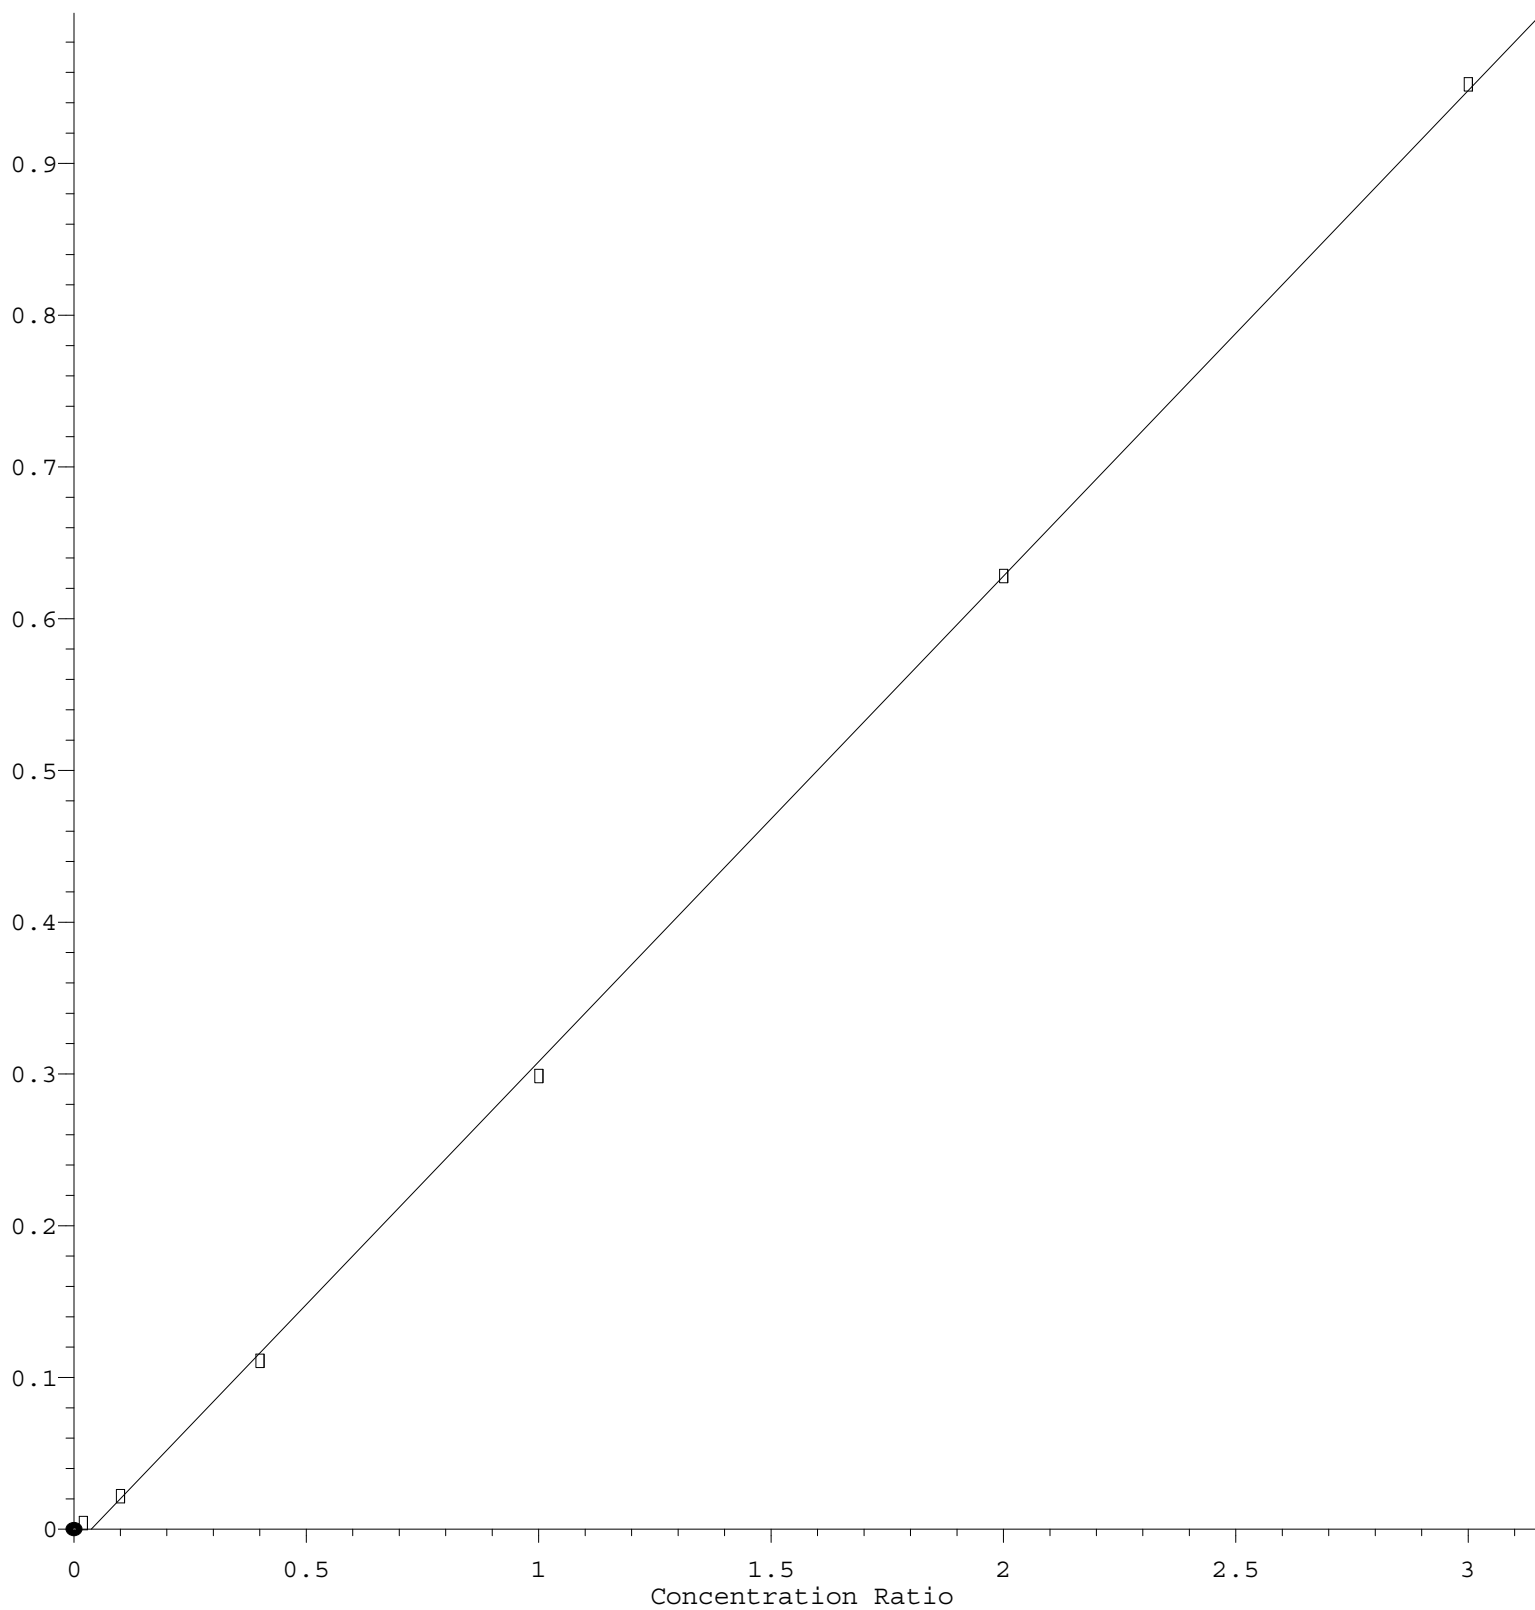

$$\text{Response} = 3.201\text{e-}001 * \text{Amt} - 1.190\text{e-}002$$


Coef of Det (r^2) = 0.999688 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X101321W.M

Calibration Table Last Updated: Thu Oct 14 03:51:38 2021

trans-1,4-Dichloro-2-butene

Response Ratio

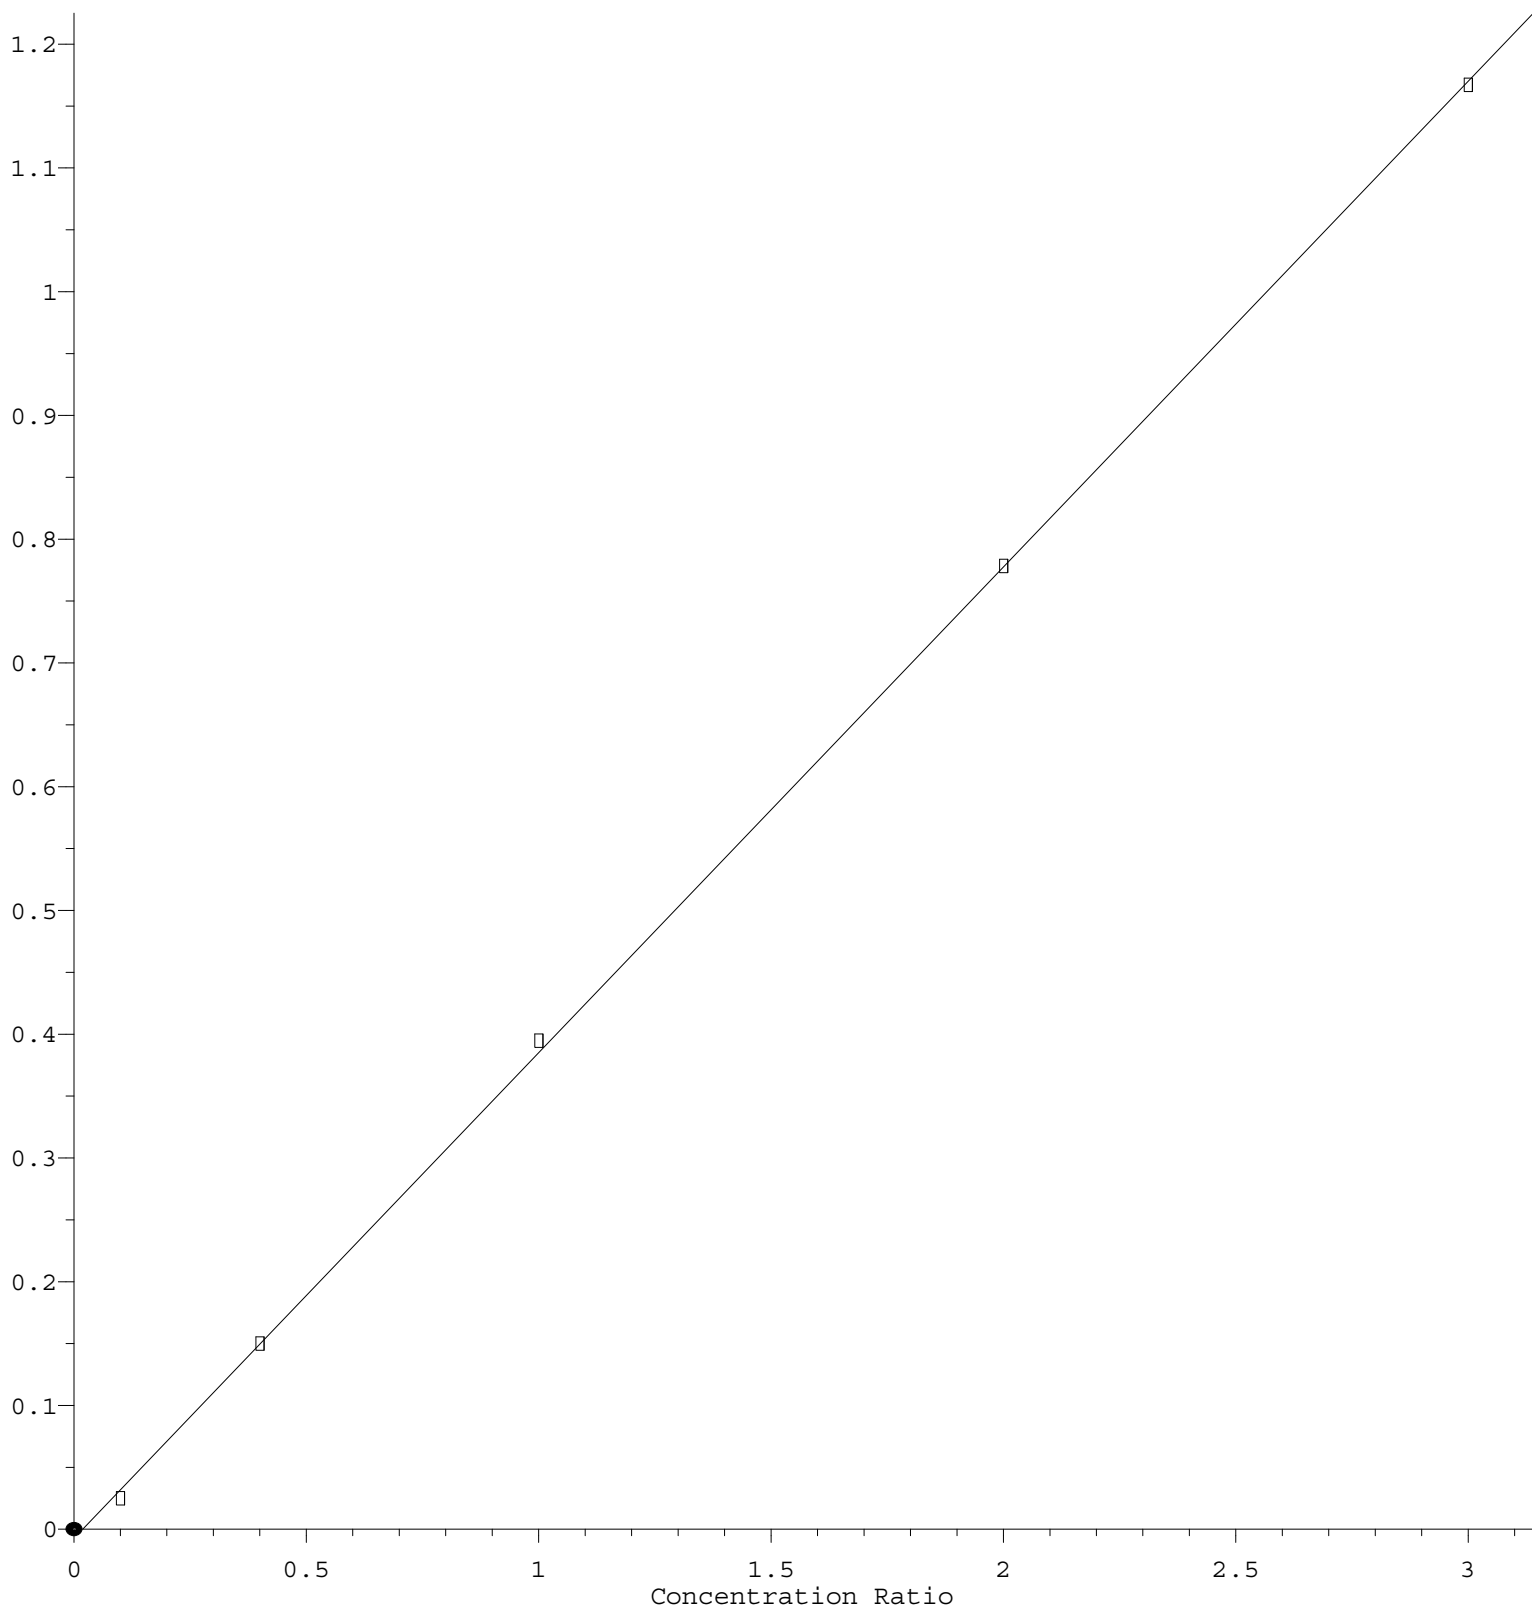

$$\text{Response} = 3.926\text{e-}001 * \text{Amt} - 7.312\text{e-}003$$

Coef of Det (r^2) = 0.999831 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X101321W.M

Calibration Table Last Updated: Thu Oct 14 03:51:38 2021

Naphthalene

Response Ratio

11
10
9
8
7
6
5
4
3
2
1
0

0

0.5

1

1.5

2


2.5

3

Concentration Ratio

Response = 3.542e+000 * Amt - 1.804e-002
 Coef of Det (r^2) = 0.999275 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X101321W.M
 Calibration Table Last Updated: Thu Oct 14 03:51:38 2021

Bromomethane

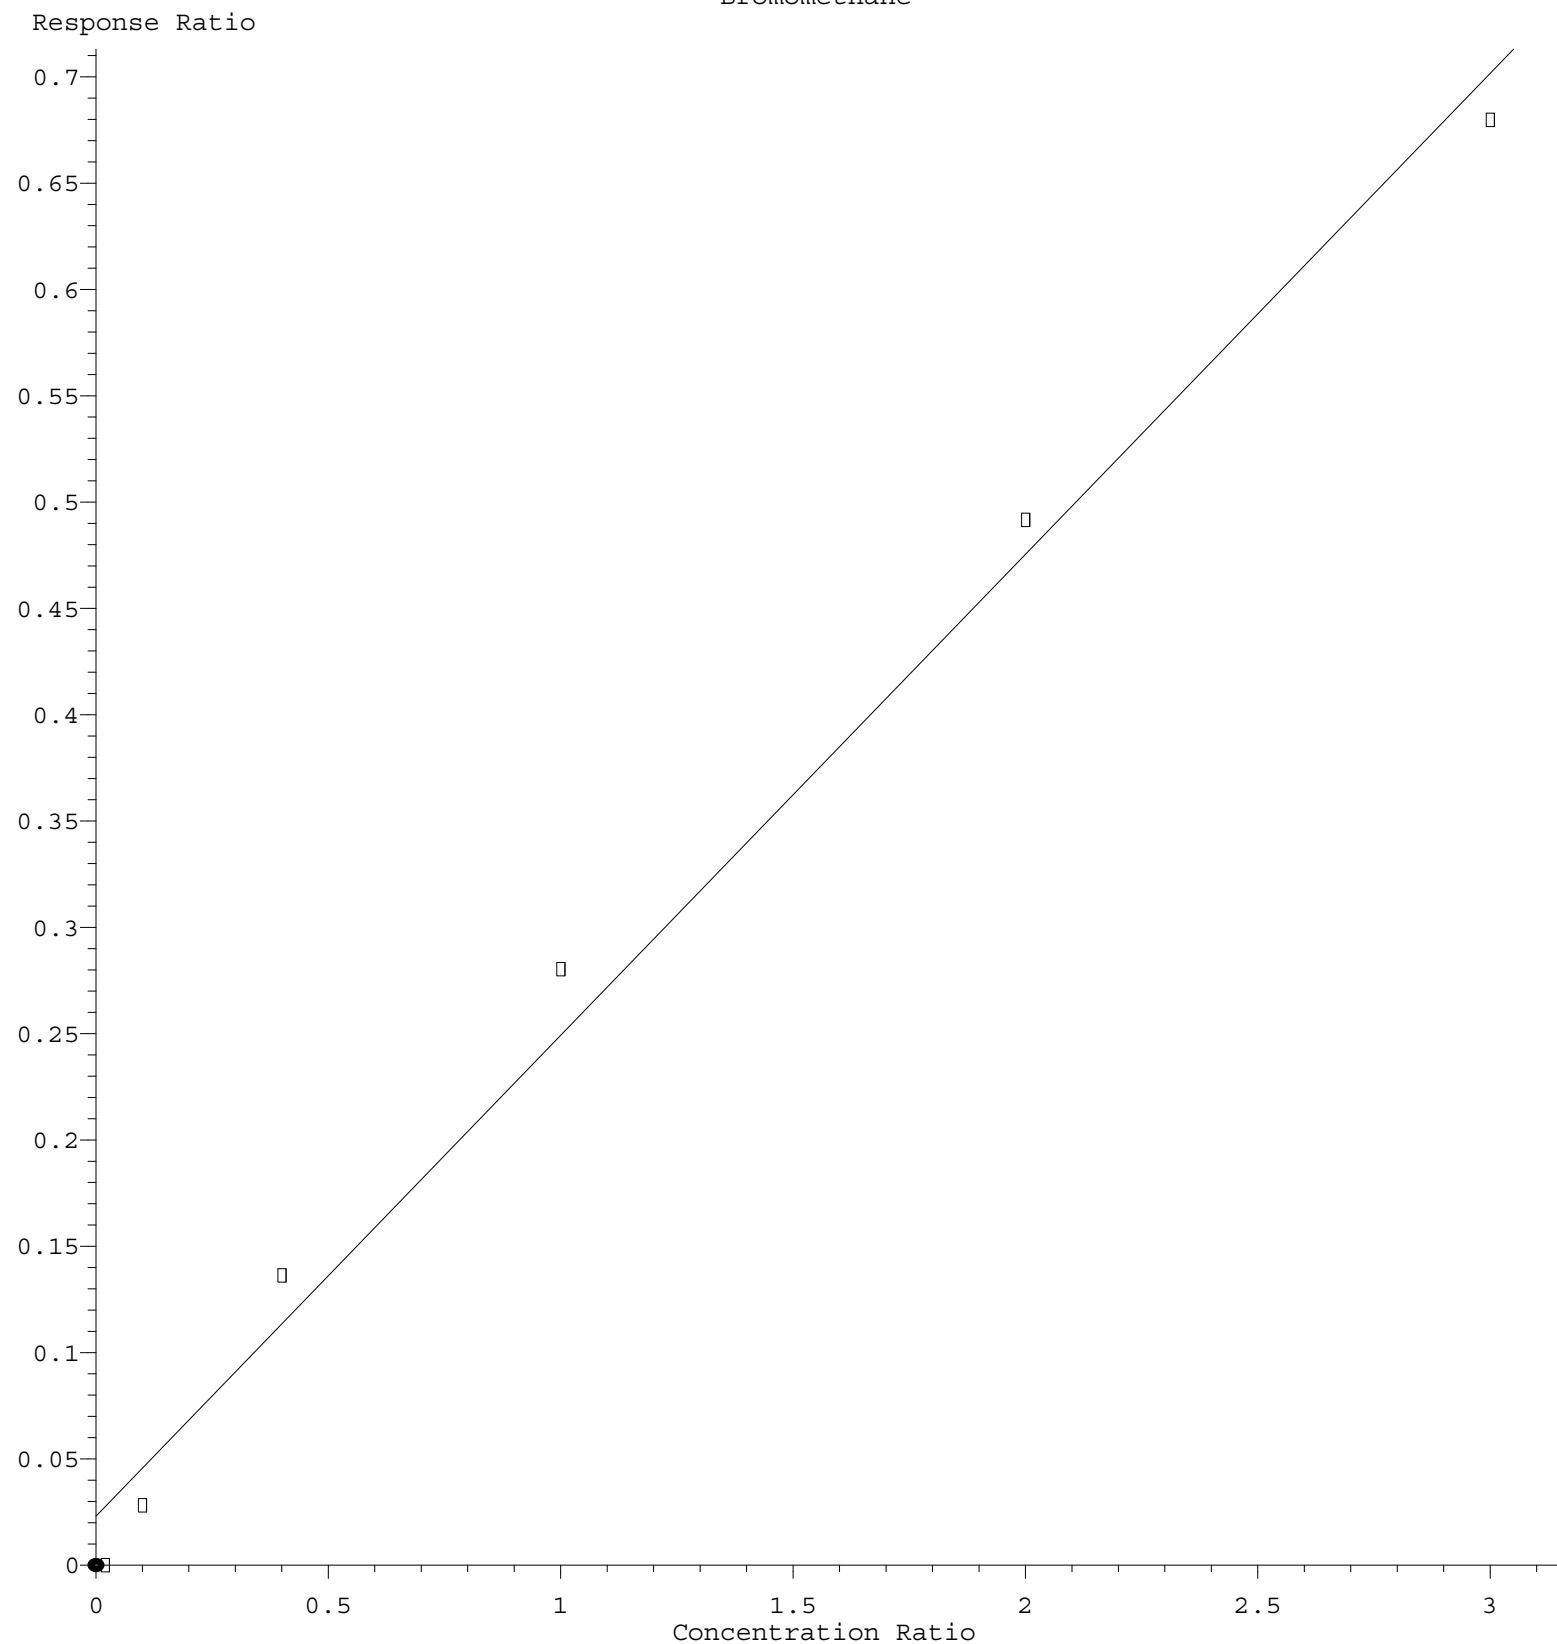

$\text{Response} = 2.264\text{e-}001 * \text{Amt} + 2.337\text{e-}002$
 Coef of Det (r^2) = 0.991013 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X101321W.M
 Calibration Table Last Updated: Thu Oct 14 03:51:38 2021