

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101321\
 Data File : VX024805.D
 Acq On : 13 Oct 2021 23:53
 Operator : JC/MD
 Sample : M4153-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-REF-5

Quant Time: Oct 14 03:59:39 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101321W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 14 03:51:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	122955	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	218914	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	214713	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	94179	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	96487	63.85	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 127.70%#	
35) Dibromofluoromethane	5.397	113	75349	57.82	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 115.64%	
50) Toluene-d8	8.653	98	271197	56.26	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 112.52%#	
62) 4-Bromofluorobenzene	11.085	95	101815	53.70	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 107.40%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101321\
Data File : VX024805.D
Acq On : 13 Oct 2021 23:53
Operator : JC/MD
Sample : M4153-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-REF-5

Quant Time: Oct 14 03:59:39 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101321W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 14 03:51:38 2021
Response via : Initial Calibration




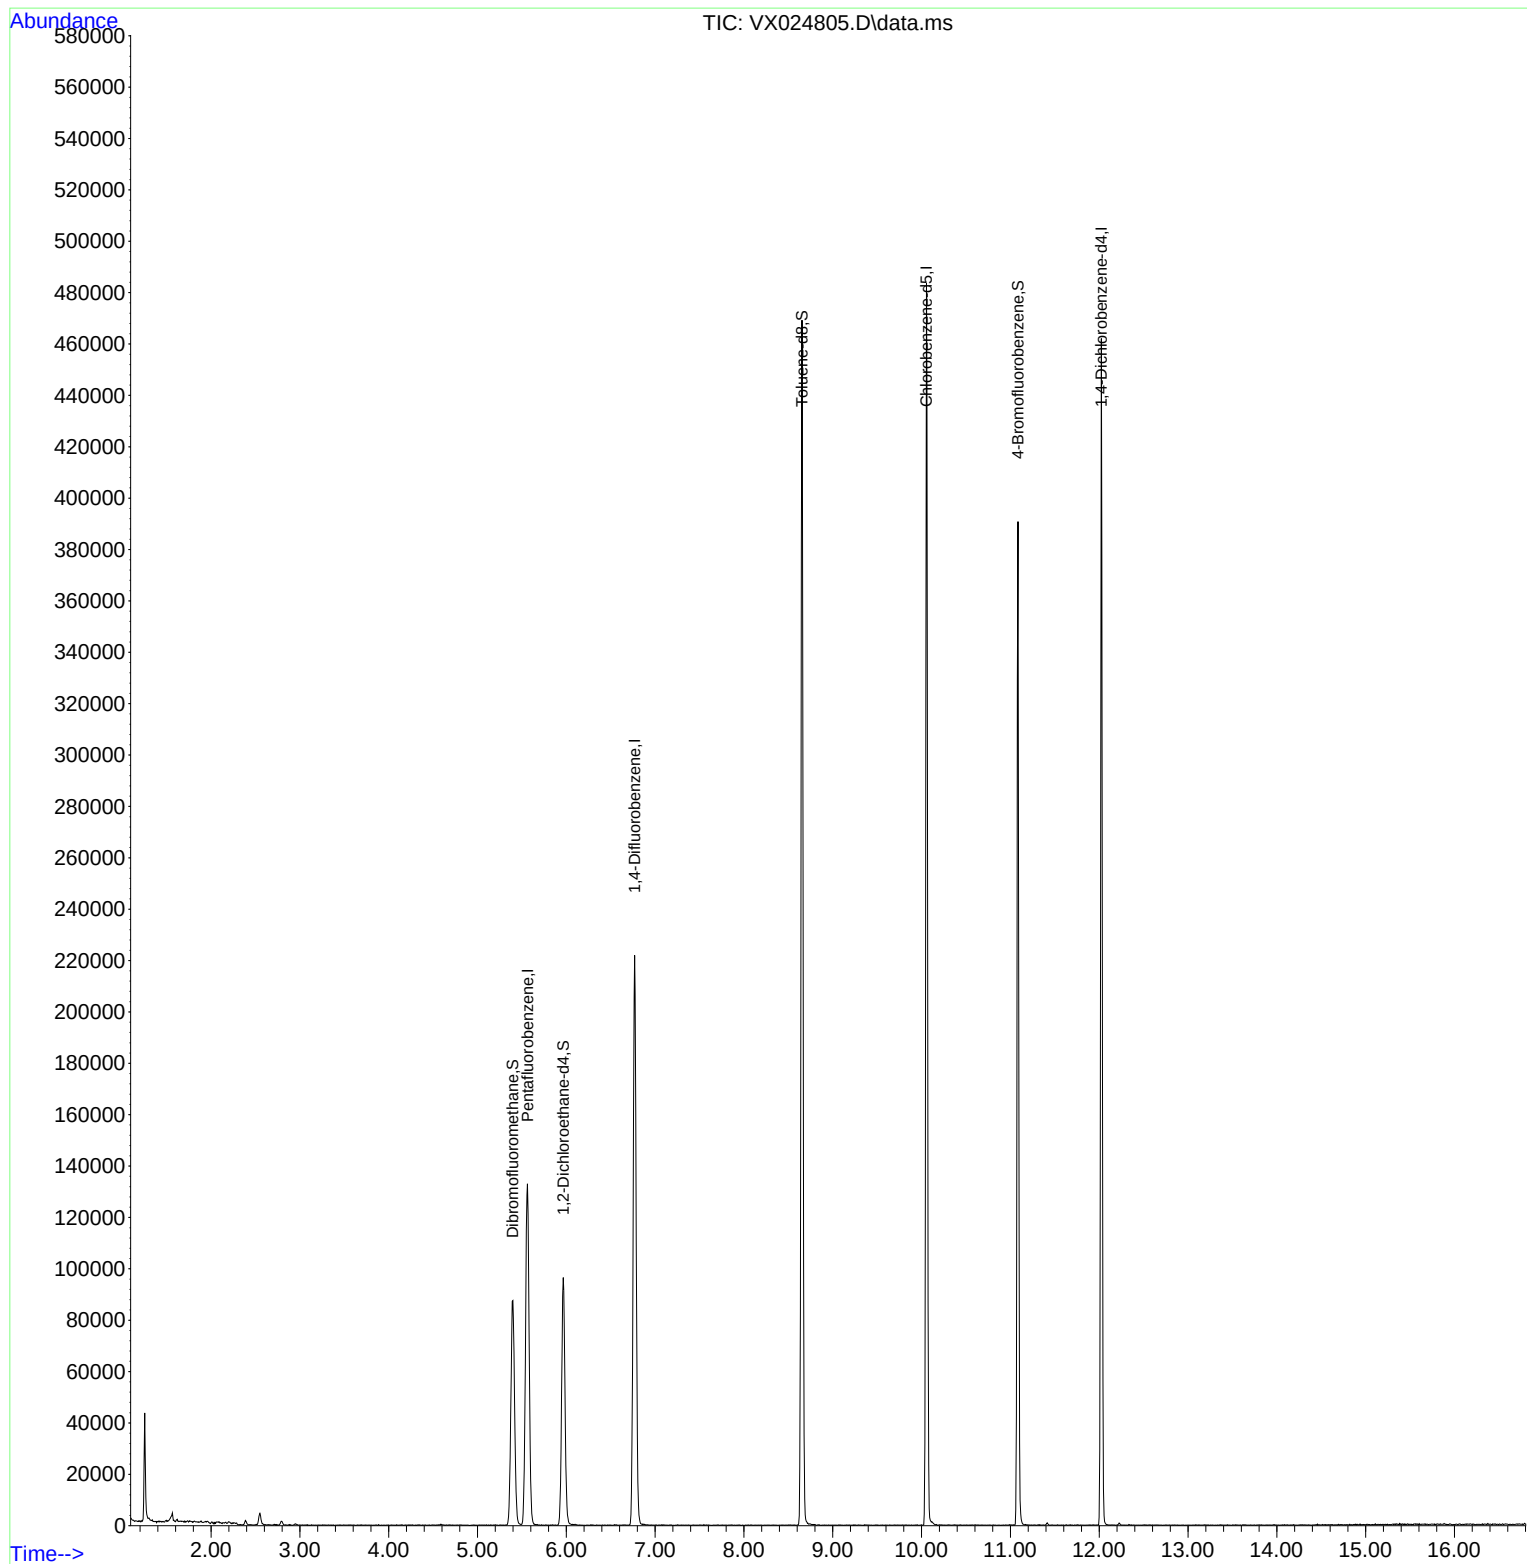


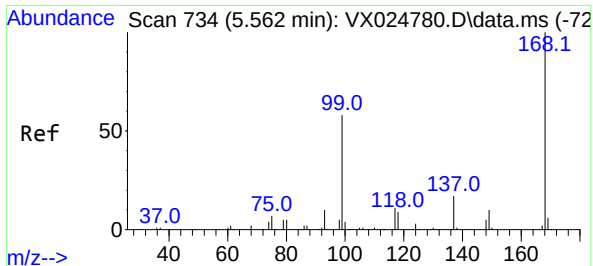

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.000 min
Lab File: VX024805.D
Acq: 13 Oct 2021 23:53




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-REF-5


Tgt Ion:168 Resp: 122955
Ion Ratio Lower Upper
168 100
99 59.9 46.4 69.6

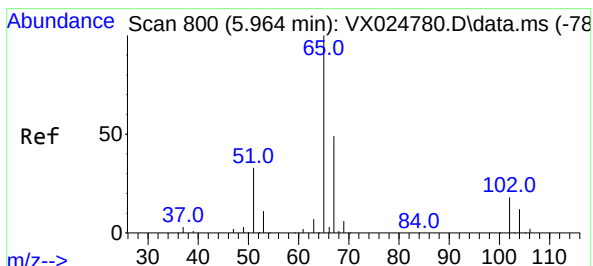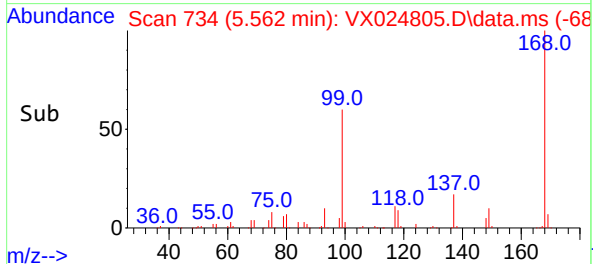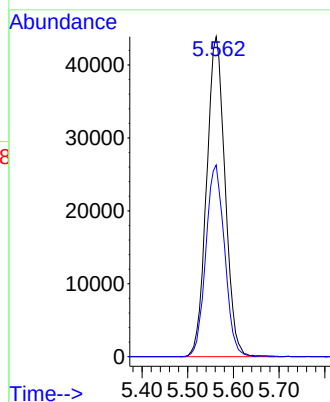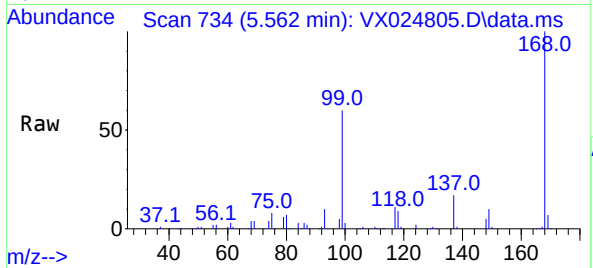

#33
1,2-Dichloroethane-d4
Concen: 63.85 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX024805.D
Acq: 13 Oct 2021 23:53

Tgt Ion: 65 Resp: 96487
Ion Ratio Lower Upper
65 100
67 51.0 0.0 101.0

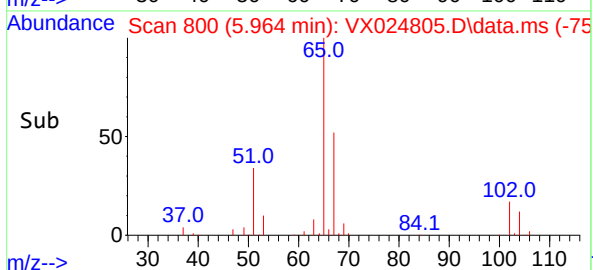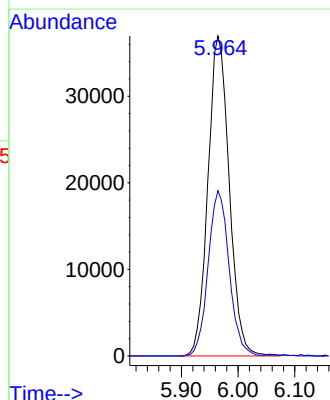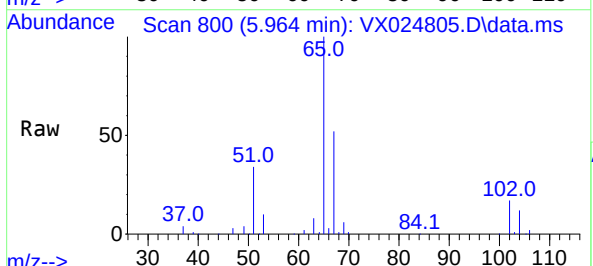




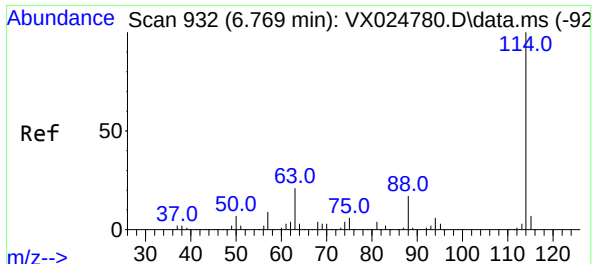


#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX024805.D
Acq: 13 Oct 2021 23:53

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-REF-5

Tgt Ion:114 Resp: 218914




Ion	Ratio	Lower	Upper
114	100		
63	19.5	0.0	41.0
88	16.1	0.0	34.8

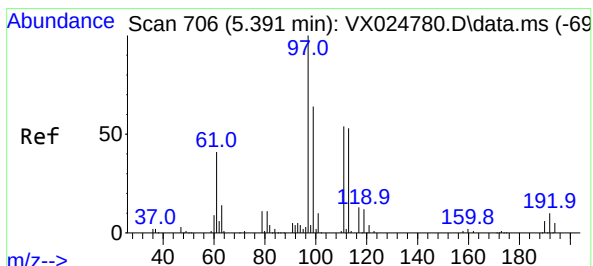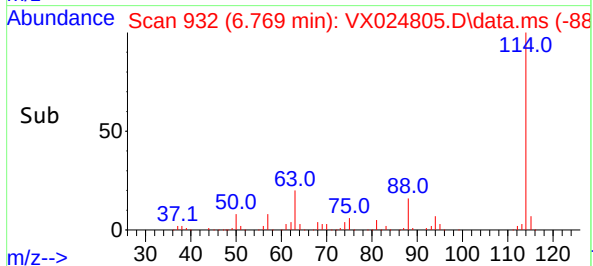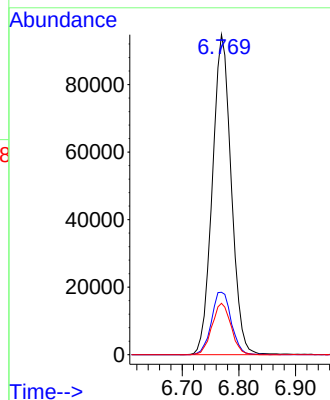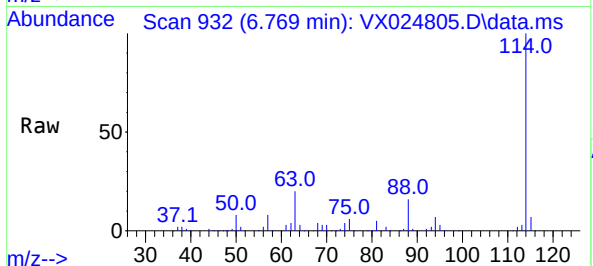


#35
Dibromofluoromethane
Concen: 57.82 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.006 min
Lab File: VX024805.D
Acq: 13 Oct 2021 23:53

Tgt Ion:113 Resp: 75349

Ion	Ratio	Lower	Upper
113	100		
111	102.4	82.1	123.1
192	19.1	15.6	23.4


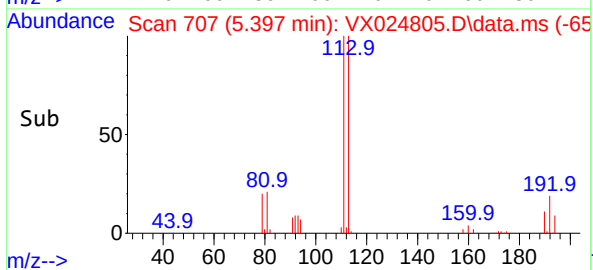
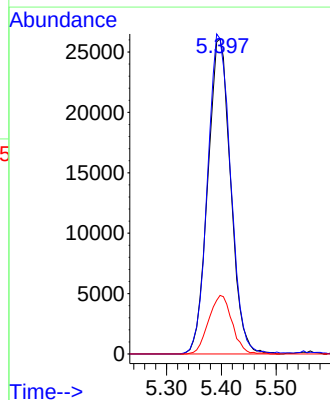
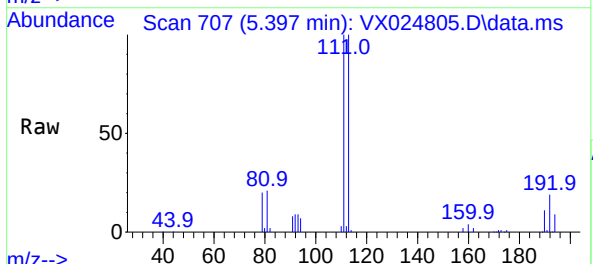


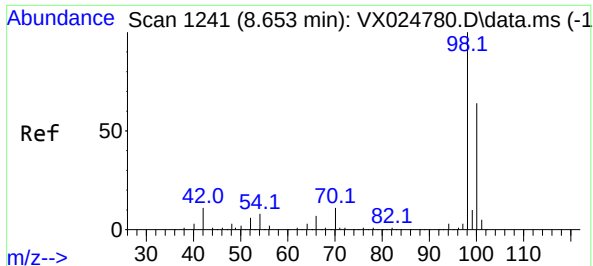

#50
Toluene-d8
Concen: 56.26 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX024805.D
Acq: 13 Oct 2021 23:53




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-REF-5


Tgt Ion: 98 Resp: 271197
Ion Ratio Lower Upper
98 100
100 63.6 51.4 77.0

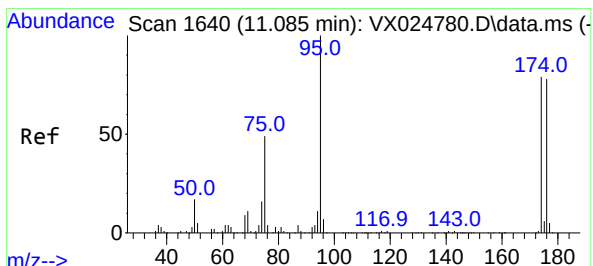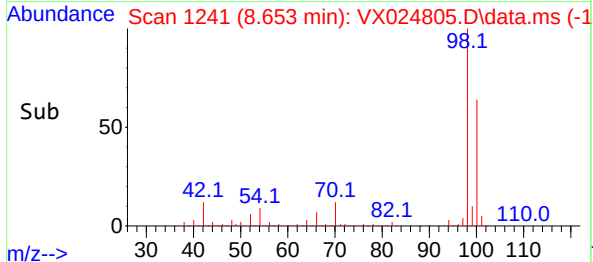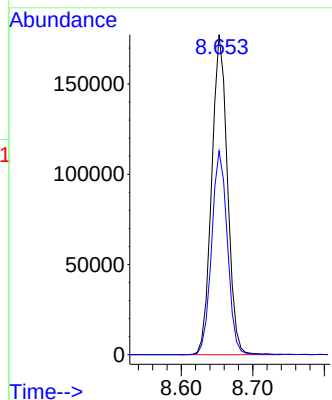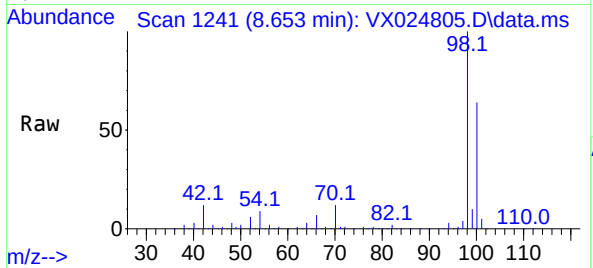

#62
4-Bromofluorobenzene
Concen: 53.70 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX024805.D
Acq: 13 Oct 2021 23:53

Tgt Ion: 95 Resp: 101815
Ion Ratio Lower Upper
95 100
174 79.6 0.0 158.0
176 76.3 0.0 153.6


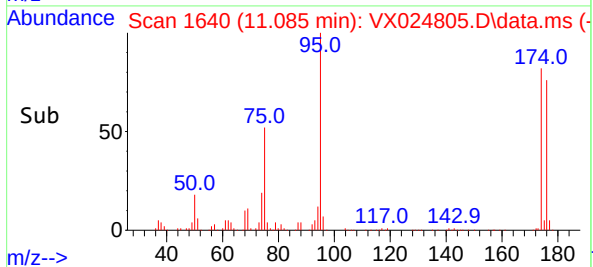
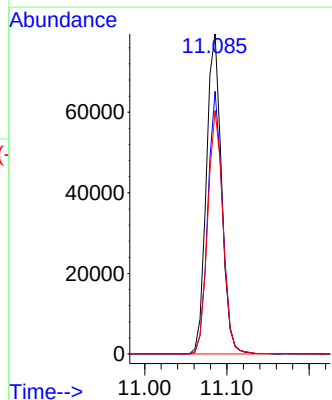
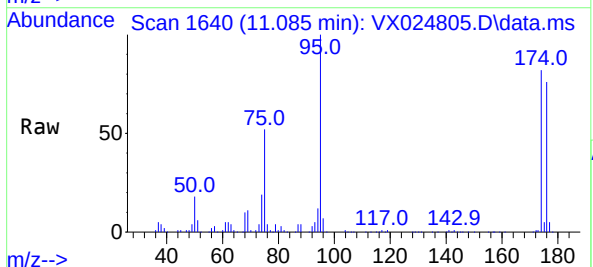


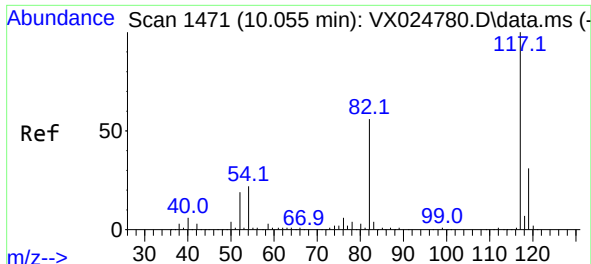

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX024805.D
Acq: 13 Oct 2021 23:53

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-REF-5

Tgt Ion:117 Resp: 214713
Ion Ratio Lower Upper
117 100
82 57.3 44.6 67.0
119 31.6 24.8 37.2

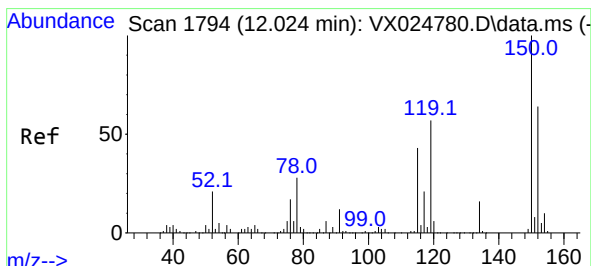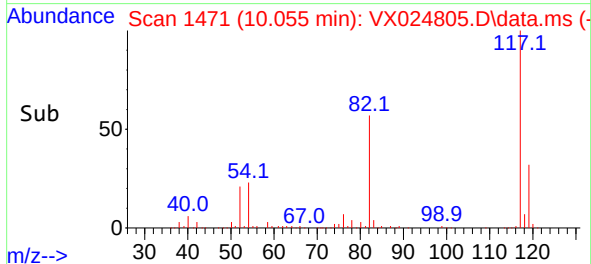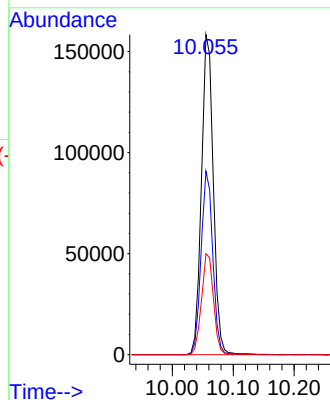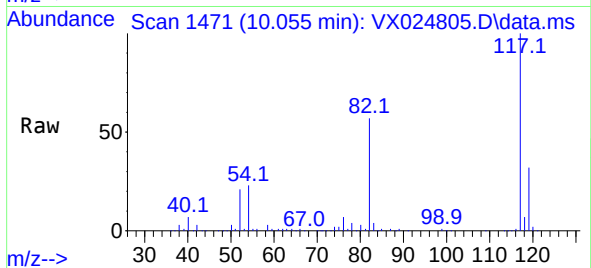

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX024805.D
Acq: 13 Oct 2021 23:53

Tgt Ion:152 Resp: 94179
Ion Ratio Lower Upper
152 100
115 60.3 43.3 129.8
150 159.1 0.0 351.2

