

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101321\
 Data File : VX024797.D
 Acq On : 13 Oct 2021 20:45
 Operator : JC/MD
 Sample : M4170-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SW-RR-03-(SA)RE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101321W.M

Title : SW846 8260

Signal : TIC: VX024797.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.251	23	27	36	rVB2	5168	8854	1.22%	0.229%
2	2.544	232	239	248	rBV	9300	17794	2.45%	0.461%
3	5.397	693	707	722	rBV2	87743	255880	35.27%	6.626%
4	5.562	722	734	747	rVB2	134815	381371	52.57%	9.875%
5	5.964	790	800	813	rBV2	94925	251047	34.61%	6.501%
6	6.769	922	932	946	rBV	224588	524125	72.25%	13.572%
7	8.653	1233	1241	1249	rBV	480238	725405	100.00%	18.784%
8	8.726	1249	1253	1263	rVB	6414	10311	1.42%	0.267%
9	10.055	1465	1471	1488	rBV	468940	650532	89.68%	16.845%
10	11.085	1634	1640	1651	rBV	389335	489445	67.47%	12.674%
11	12.024	1789	1794	1805	rBV	432964	547105	75.42%	14.167%




Sum of corrected areas: 3861869

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101321\
Data File : VX024797.D
Acq On : 13 Oct 2021 20:45
Operator : JC/MD
Sample : M4170-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-03-(SA)RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

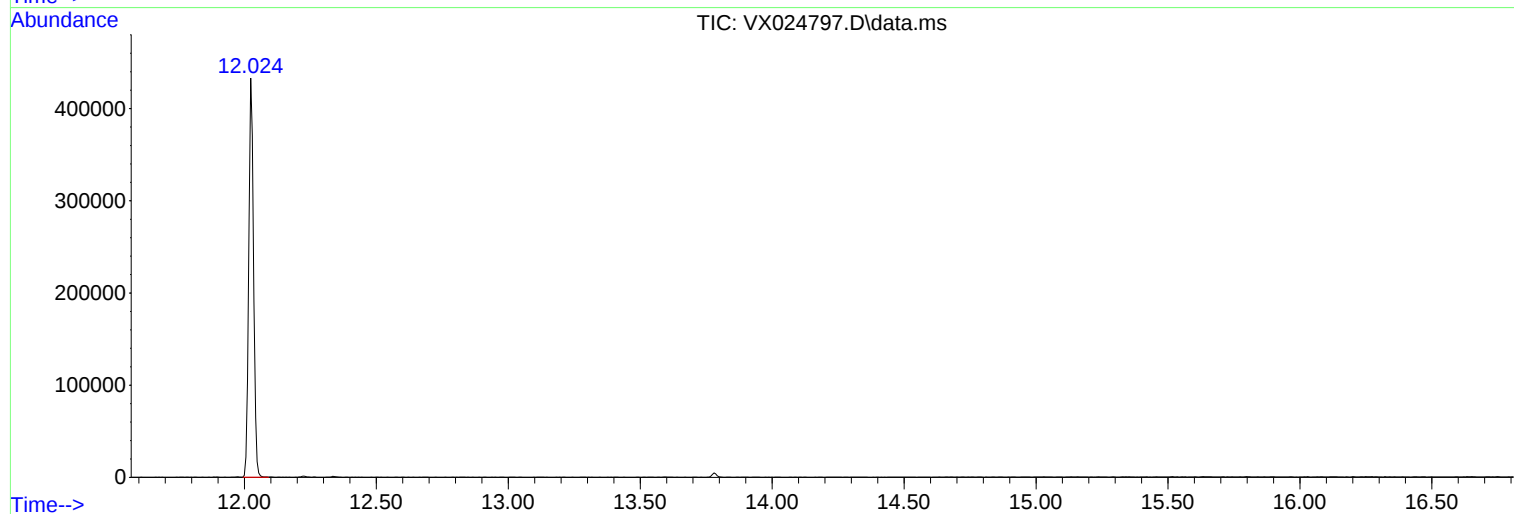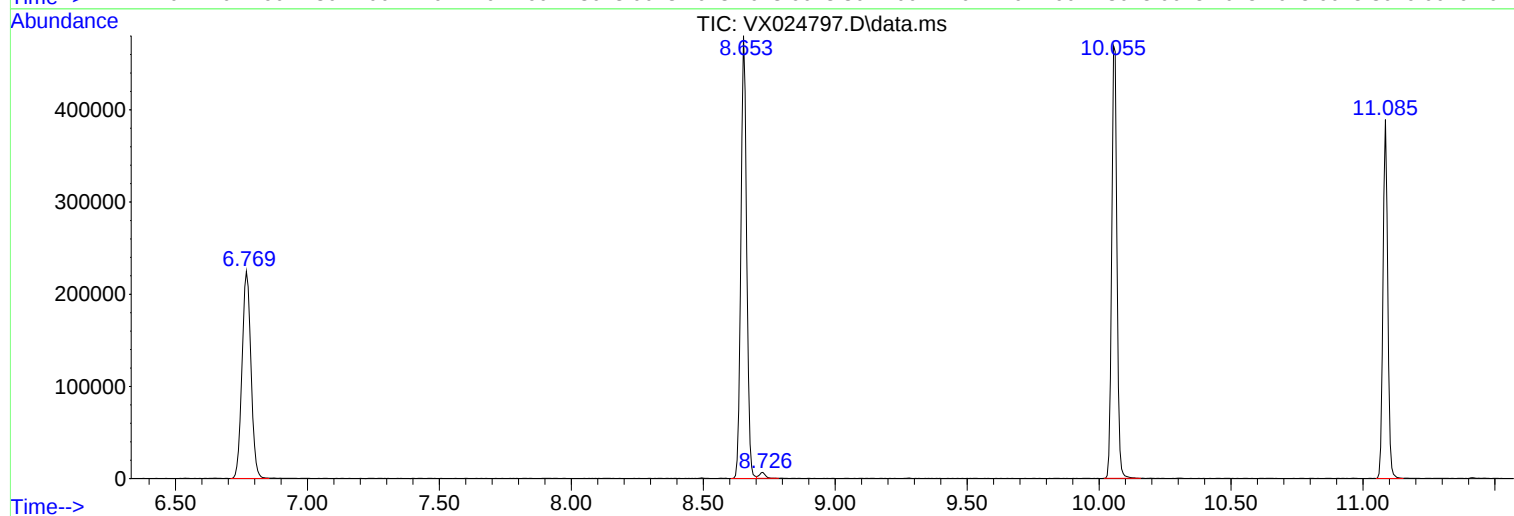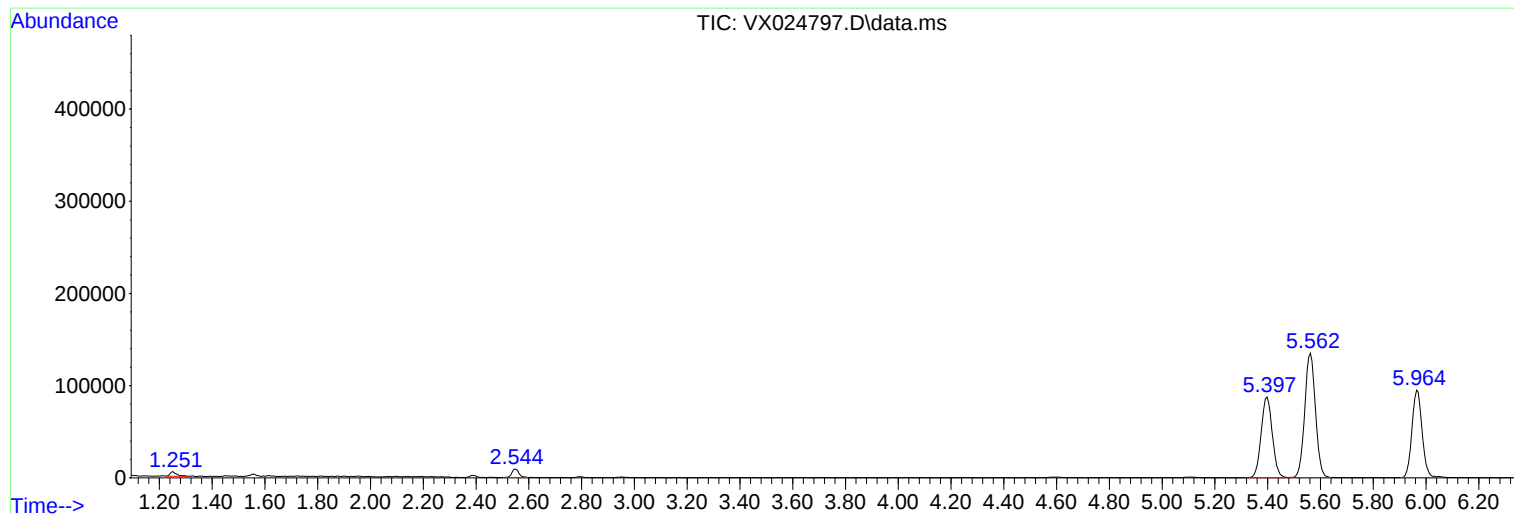

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101321\
Data File : VX024797.D
Acq On : 13 Oct 2021 20:45
Operator : JC/MD
Sample : M4170-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-03-(SA)RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101321\
Data File : VX024797.D
Acq On : 13 Oct 2021 20:45
Operator : JC/MD
Sample : M4170-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-03-(SA)RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
