
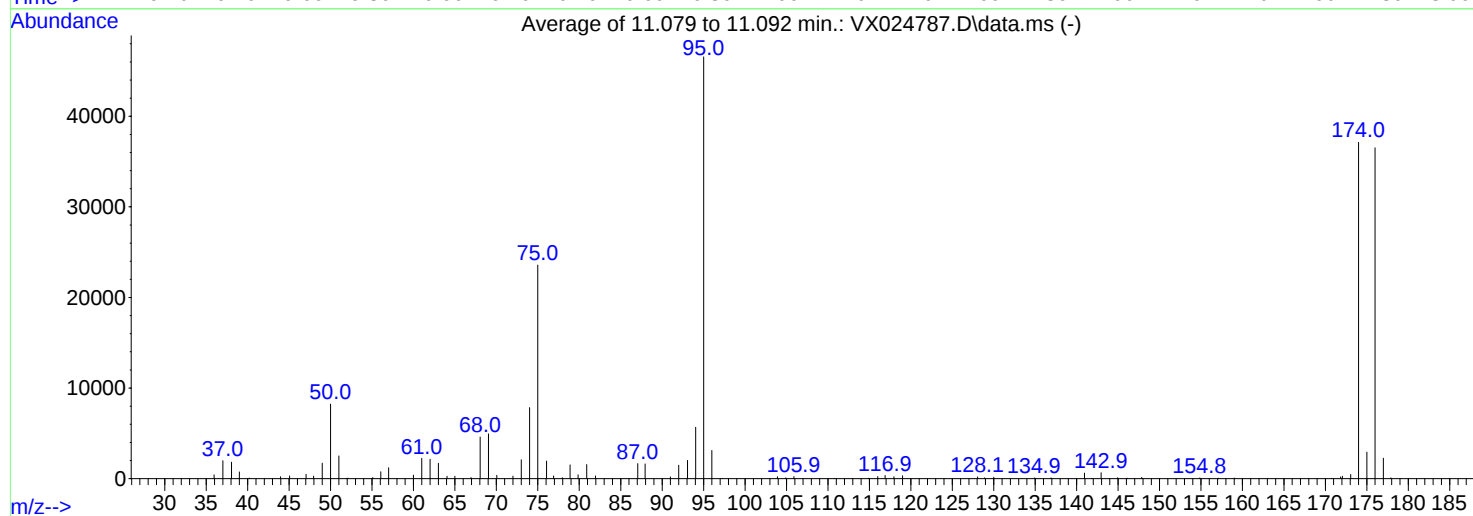


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101321\
Data File : VX024787.D
Acq On : 13 Oct 2021 15:53
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101321W.M
Title : SW846 8260
Last Update : Thu Oct 14 03:51:38 2021

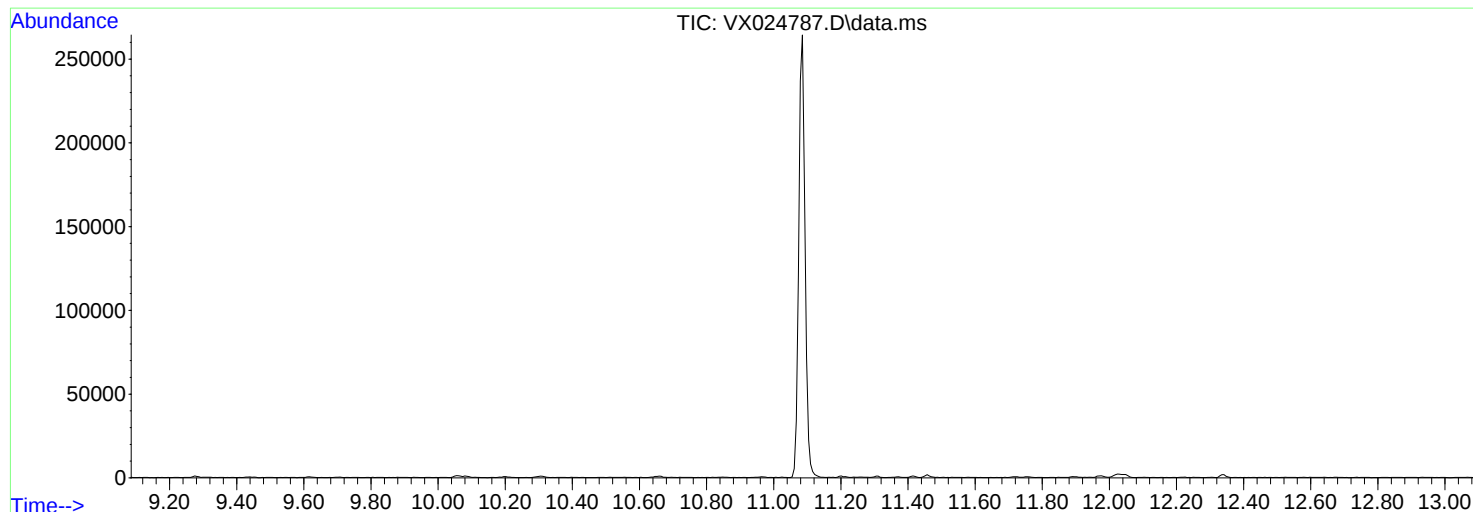

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.7	8230	PASS
75	95	30	60	50.7	23587	PASS
95	95	100	100	100.0	46560	PASS
96	95	5	9	6.7	3112	PASS
173	174	0.00	2	1.2	460	PASS
174	95	50	100	79.8	37133	PASS
175	174	5	9	7.9	2932	PASS
176	174	95	101	98.4	36531	PASS
177	176	5	9	6.2	2271	PASS