

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101322\
Data File : VX032118.D
Acq On : 13 Oct 2022 18:33
Operator : JC/MD
Sample : N5133-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
HAS-WATER-1013

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M

Title : SW846 8260

Signal : TIC: VX032118.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	694	705	721	rBV	80273	231713	33.92%	7.528%
2	5.556	722	733	745	rVB	92205	261088	38.22%	8.482%
3	5.958	788	799	816	rBV	93923	247124	36.18%	8.029%
4	6.763	922	931	946	rBV	126958	298583	43.71%	9.701%
5	8.653	1232	1241	1251	rBV	424700	683128	100.00%	22.194%
6	10.055	1464	1471	1481	rBV	307230	409274	59.91%	13.297%
7	11.079	1634	1639	1652	rBV	332778	441867	64.68%	14.356%
8	12.024	1788	1794	1805	rBV	408013	505238	73.96%	16.414%




Sum of corrected areas: 3078015

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101322\
Data File : VX032118.D
Acq On : 13 Oct 2022 18:33
Operator : JC/MD
Sample : N5133-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
HAS-WATER-1013

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

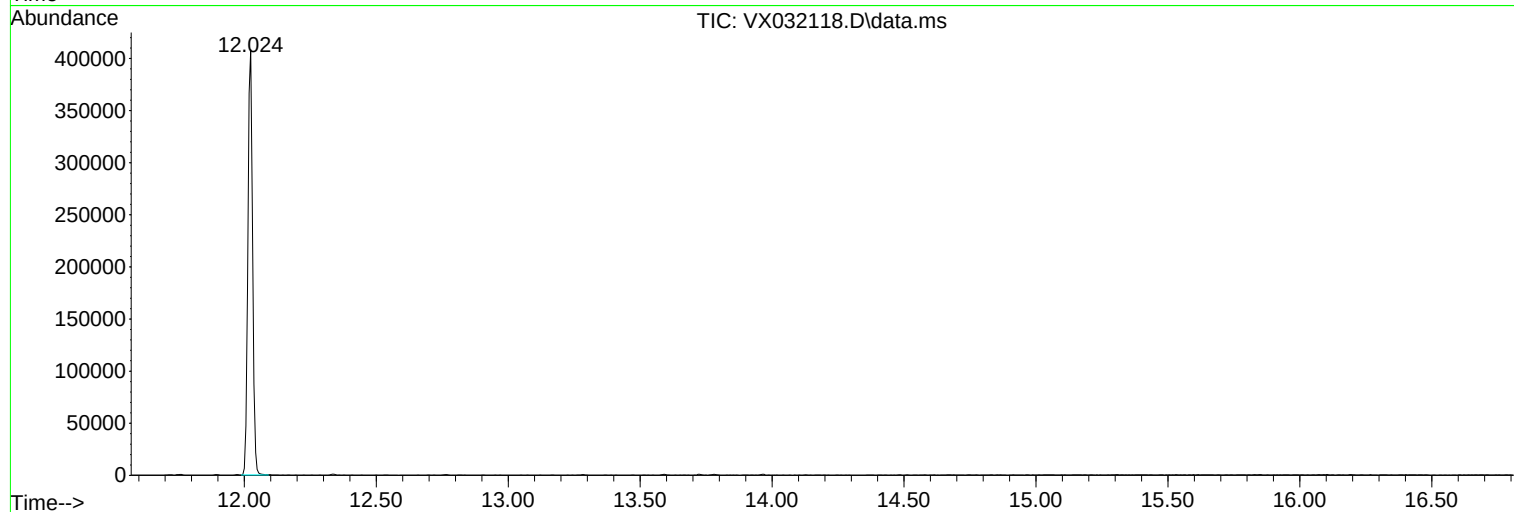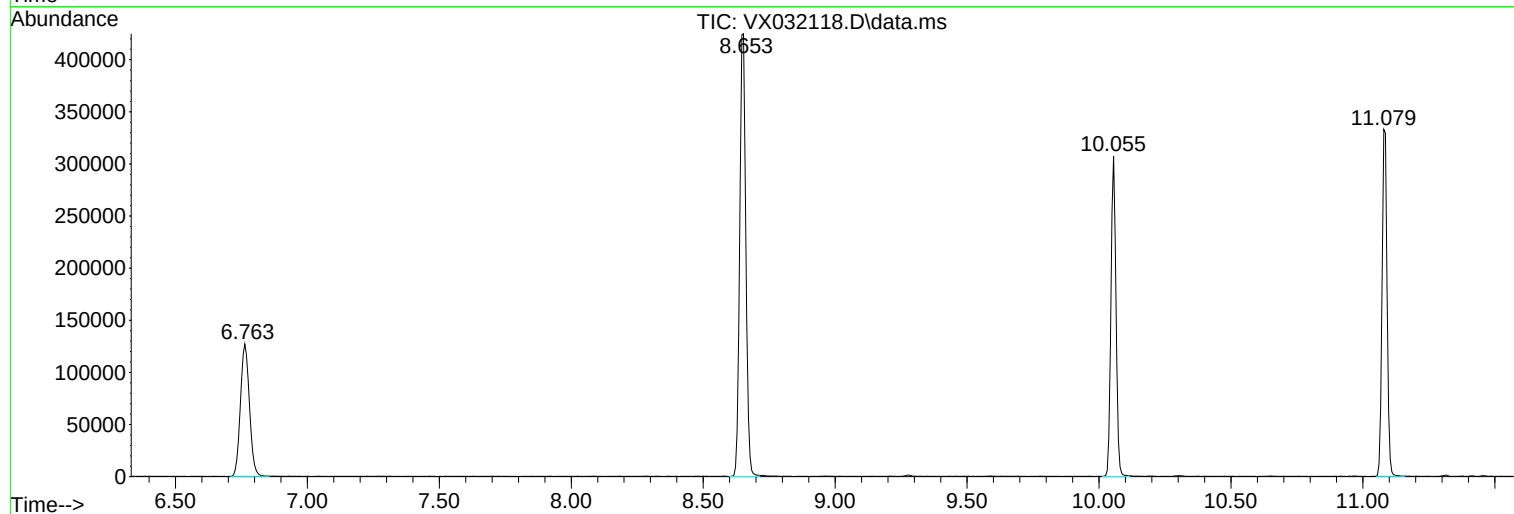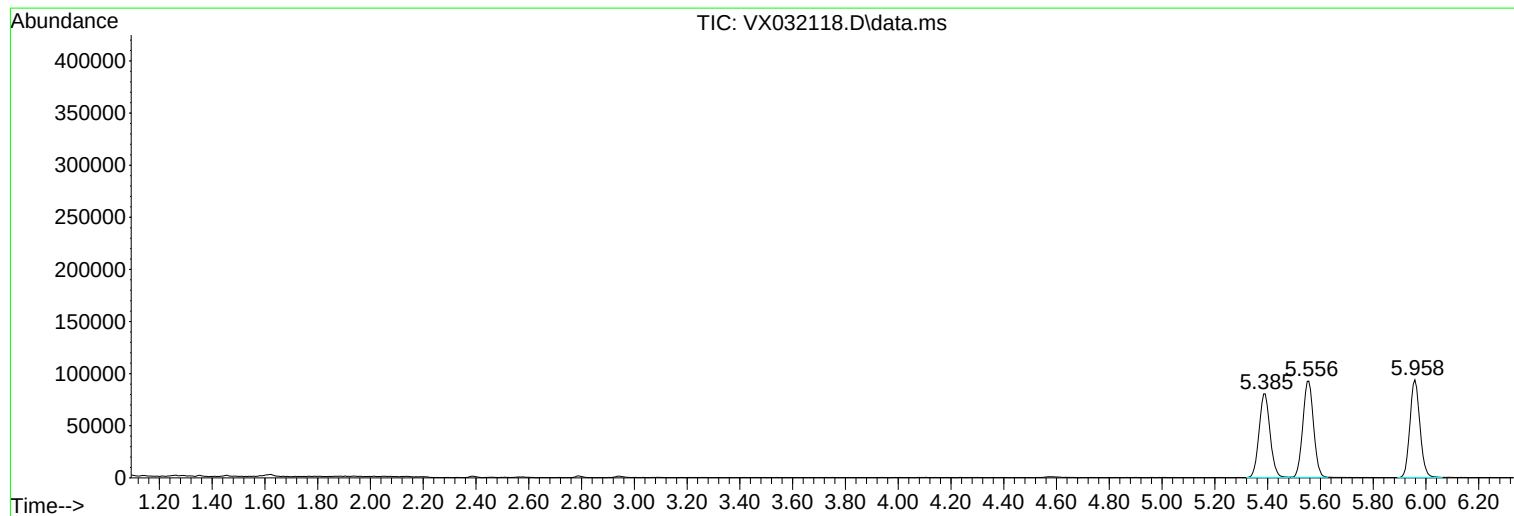

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101322\
Data File : VX032118.D
Acq On : 13 Oct 2022 18:33
Operator : JC/MD
Sample : N5133-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
HAS-WATER-1013

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101322\
Data File : VX032118.D
Acq On : 13 Oct 2022 18:33
Operator : JC/MD
Sample : N5133-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
HAS-WATER-1013

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------