

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101322\
 Data File : VX032121.D
 Acq On : 13 Oct 2022 19:40
 Operator : JC/MD
 Sample : N5116-04 5000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SWRN-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Title : SW846 8260

Signal : TIC: VX032121.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.617	81	87	96	rVB6	2132	5721	1.04%	0.225%
2	4.580	562	573	587	rBV2	2104	8357	1.52%	0.329%
3	5.391	694	706	720	rBV	59123	170664	31.09%	6.720%
4	5.556	723	733	744	rVB	66184	185228	33.74%	7.294%
5	5.958	785	799	813	rBV2	68375	181193	33.01%	7.135%
6	6.763	921	931	944	rBV	95752	224149	40.83%	8.826%
7	8.647	1234	1240	1252	rBV	345252	548942	100.00%	21.616%
8	10.055	1465	1471	1479	rBV	243040	321847	58.63%	12.673%
9	11.079	1634	1639	1649	rBV	267654	348994	63.58%	13.742%
10	12.024	1788	1794	1804	rBV	332214	415337	75.66%	16.355%
11	14.615	2216	2219	2220	rBV3	6066	6028	1.10%	0.237%
12	14.639	2220	2223	2226	rVB3	7087	8900	1.62%	0.350%
13	14.755	2237	2242	2245	rBV5	4105	7869	1.43%	0.310%
14	14.786	2245	2247	2252	rVB6	4475	6811	1.24%	0.268%
15	14.847	2252	2257	2266	rBV6	5439	15317	2.79%	0.603%
16	15.188	2308	2313	2314	rBV5	4510	6086	1.11%	0.240%
17	15.213	2314	2317	2321	rVB6	5320	7930	1.44%	0.312%
18	15.377	2340	2344	2346	rBV4	5769	8466	1.54%	0.333%
19	15.420	2347	2351	2357	rVB4	16180	25571	4.66%	1.007%
20	15.487	2358	2362	2364	rBV5	7210	12188	2.22%	0.480%
21	15.743	2401	2404	2409	rVB4	11842	16065	2.93%	0.633%
22	16.603	2543	2545	2550	rVB6	6670	7902	1.44%	0.311%




Sum of corrected areas: 2539565

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101322\
Data File : VX032121.D
Acq On : 13 Oct 2022 19:40
Operator : JC/MD
Sample : N5116-04 5000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SWRN-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

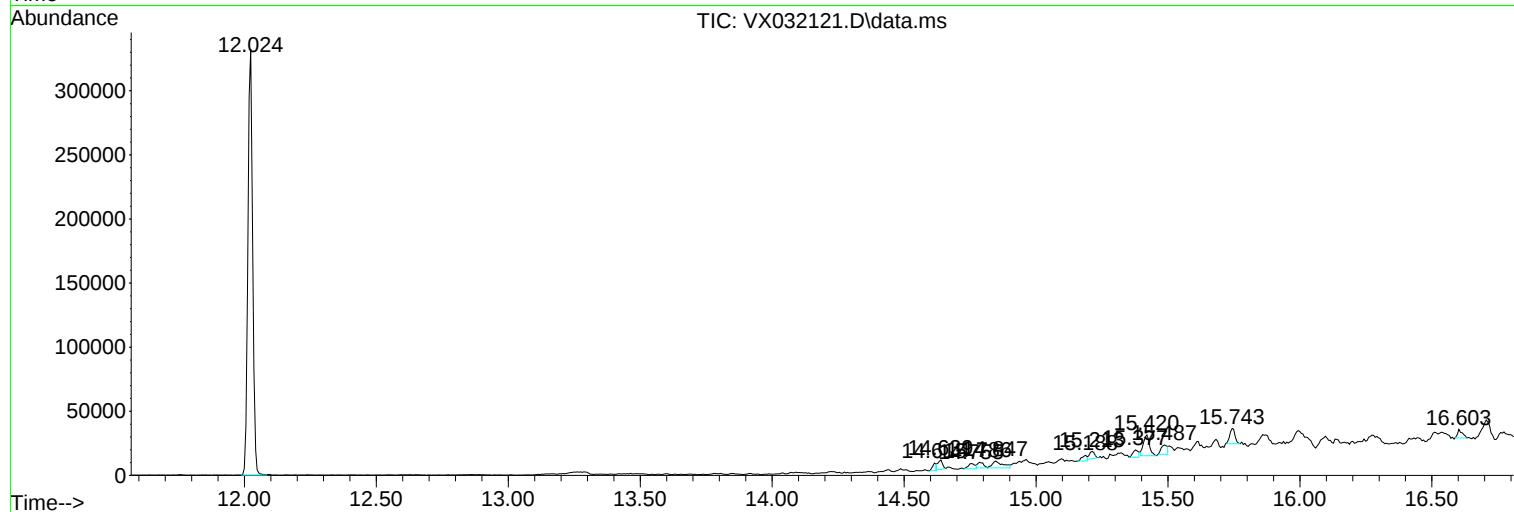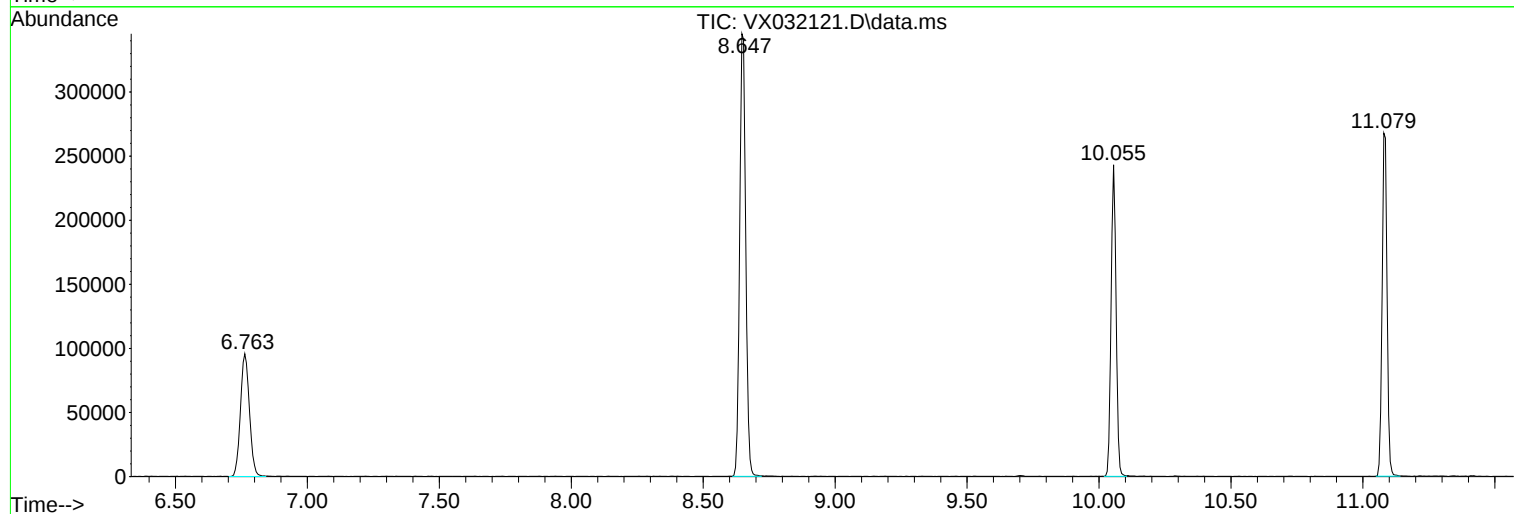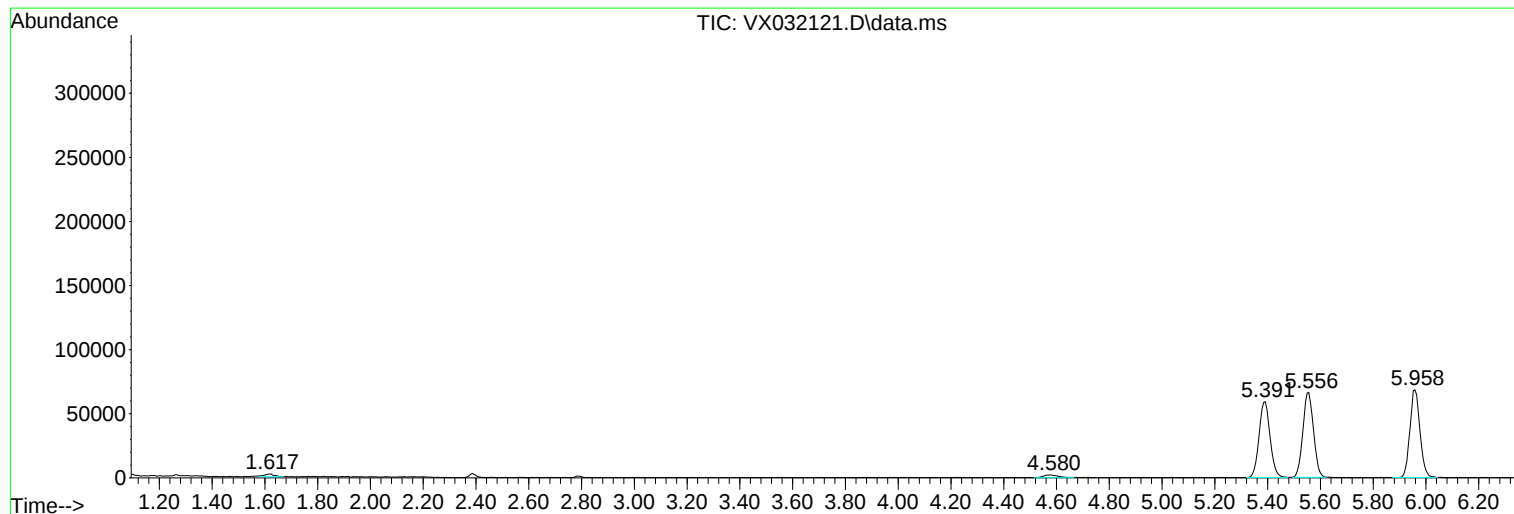

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101322\
Data File : VX032121.D
Acq On : 13 Oct 2022 19:40
Operator : JC/MD
Sample : N5116-04 5000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SWRN-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101322\
Data File : VX032121.D
Acq On : 13 Oct 2022 19:40
Operator : JC/MD
Sample : N5116-04 5000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SWRN-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------