

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101422\
 Data File : VX032139.D
 Acq On : 14 Oct 2022 17:00
 Operator : JC/MD
 Sample : N5141-01RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SV34211LRE

Quant Time: Oct 17 02:26:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 06 14:28:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	73789	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	100226	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	74914	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	51142	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	42369	27.803	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	55.600%#		
35) Dibromofluoromethane	5.397	113	30187	26.608	ug/l	0.01
Spiked Amount 50.000	Range 75 - 124		Recovery =	53.220%#		
50) Toluene-d8	8.653	98	194840	47.728	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	95.460%		
62) 4-Bromofluorobenzene	11.079	95	55946	38.765	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	77.520%#		
Target Compounds						
					Qvalue	
5) Bromomethane	1.624	94	267	Below Cal		99
11) Tert butyl alcohol	2.959	59	49	0.258 ug/l #		73
14) Allyl chloride	2.538	41	34835	21.782 ug/l #		64
16) Acetone	2.380	43	50779	98.045 ug/l		96
18) Methyl Acetate	2.538	43	96354	56.385 ug/l #		52
25) 2-Butanone	4.574	43	6778	8.372 ug/l		98
29) Tetrahydrofuran	5.019	42	998	1.910 ug/l #		24
36) 1,1-Dichloropropene	5.556	75	6275	4.171 ug/l #		51
37) Ethyl Acetate	4.666	43	287	0.203 ug/l #		68
38) Carbon Tetrachloride	5.556	117	8483	5.515 ug/l #		19
40) Benzene	6.056	78	1285	0.292 ug/l #		80
41) Methacrylonitrile	5.038	41	1524	2.069 ug/l #		41
49) 1,4-Dioxane	7.684	88	212	Below Cal #		40
51) 4-Methyl-2-Pentanone	8.586	43	716	0.503 ug/l		93
52) Toluene	8.720	92	12835	4.456 ug/l		99
53) t-1,3-Dichloropropene	8.720	75	133	1.291 ug/l #		1
67) Ethyl Benzene	10.195	91	24442	6.365 ug/l		100
68) m/p-Xylenes	10.305	106	56410	36.966 ug/l		100
69) o-Xylene	10.647	106	41278	27.830 ug/l		98
70) Styrene	10.647	104	2157	0.910 ug/l #		1
73) Isopropylbenzene	10.964	105	8594	2.228 ug/l		98
76) 1,2,3-Trichloropropane	11.378	75	2155	2.056 ug/l #		1
78) n-propylbenzene	11.305	91	28948	6.598 ug/l		98
79) 2-Chlorotoluene	11.378	91	29445	11.153 ug/l #		40
80) 1,3,5-Trimethylbenzene	11.451	105	76688	23.972 ug/l		99
81) trans-1,4-Dichloro-2-b...	11.079	75	32944	107.108 ug/l #		11
82) 4-Chlorotoluene	11.451	91	9372	3.099 ug/l #		44
83) tert-Butylbenzene	11.969	119	13988	4.418 ug/l		78
84) 1,2,4-Trimethylbenzene	11.750	105	349720	107.610 ug/l		98
85) sec-Butylbenzene	11.750	105	349720	89.215 ug/l #		56
86) p-Isopropyltoluene	12.012	119	7213	2.185 ug/l		94
89) n-Butylbenzene	12.323	91	21310	7.710 ug/l #		21
90) Hexachloroethane	12.530	117	6084	12.597 ug/l #		15
92) 1,2-Dibromo-3-Chloropr...	12.963	75	610	2.719 ug/l #		3
95) Naphthalene	13.774	128	156279	41.777 ug/l		98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101422\
Data File : VX032139.D
Acq On : 14 Oct 2022 17:00
Operator : JC/MD
Sample : N5141-01RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SV34211LRE

Quant Time: Oct 17 02:26:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 14:28:46 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101422\
Data File : VX032139.D
Acq On : 14 Oct 2022 17:00
Operator : JC/MD
Sample : N5141-01RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SV34211LRE

Quant Time: Oct 17 02:26:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 14:28:46 2022
Response via : Initial Calibration




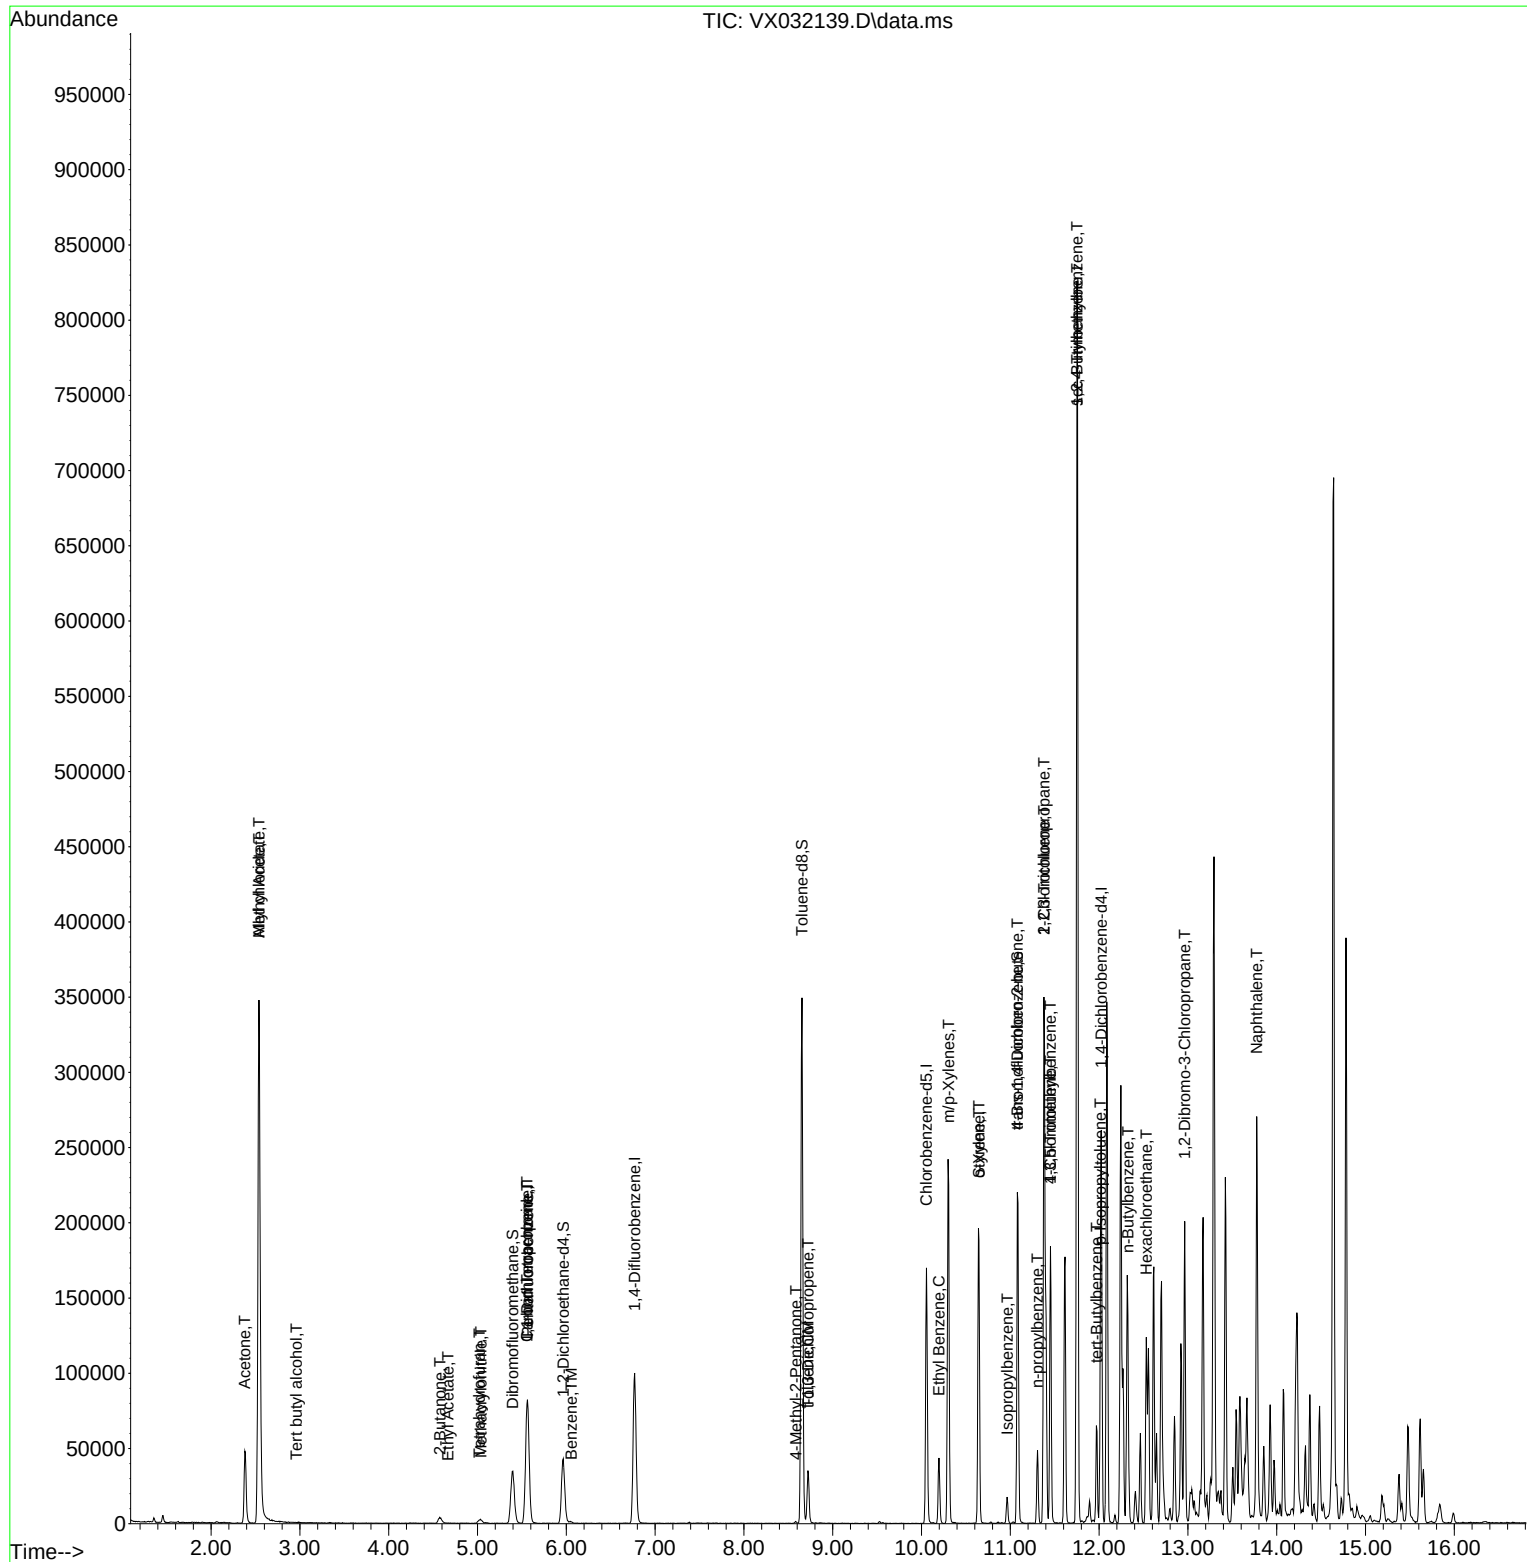


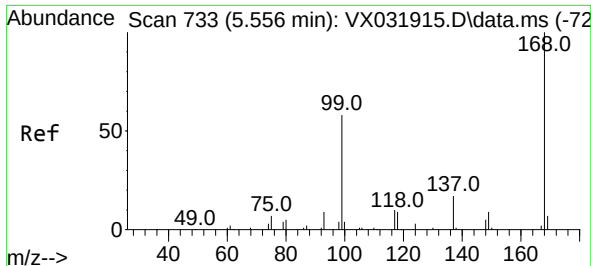

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00




Instrument :
MSVOA_X
ClientSampleId :
SV34211LRE


Tgt Ion:168 Resp: 73789
Ion Ratio Lower Upper
168 100
99 64.0 48.8 73.2

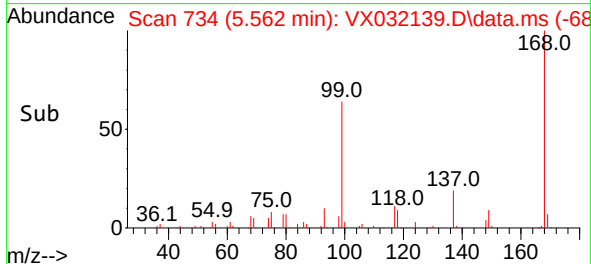

#5
Bromomethane
Concen: Below Cal
RT: 1.624 min Scan# 88
Delta R.T. 0.013 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00

Tgt Ion: 94 Resp: 267
Ion Ratio Lower Upper
94 100
96 94.3 74.4 111.6


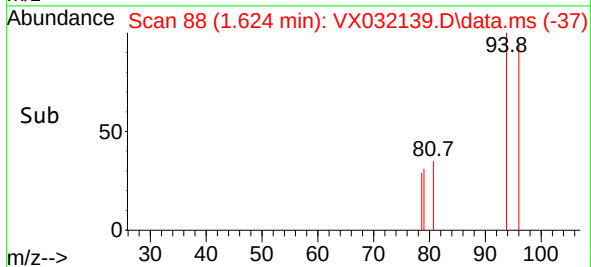

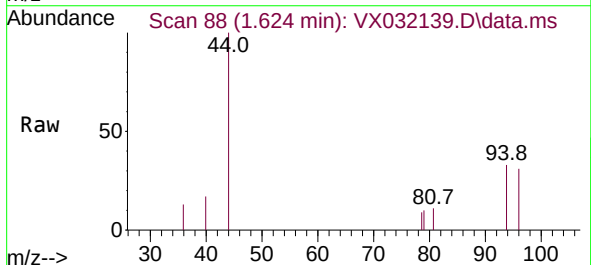




#11
Tert butyl alcohol
Concen: 0.258 ug/l
RT: 2.959 min Scan# 30
Delta R.T. -0.048 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00




Instrument :
MSVOA_X
ClientSampleId :
SV34211LRE


Tgt Ion: 59 Resp: 49
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#

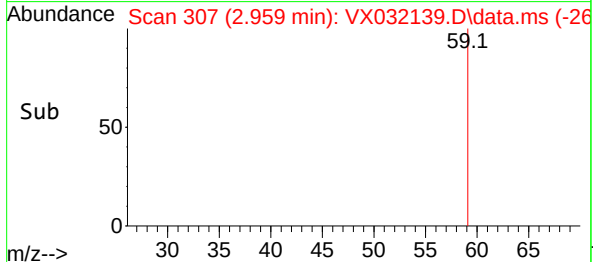

#14
Allyl chloride
Concen: 21.782 ug/l
RT: 2.538 min Scan# 238
Delta R.T. -0.128 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00

Tgt Ion: 41 Resp: 34835
Ion Ratio Lower Upper
41 100
39 94.3 58.2 87.4#
76 0.0 26.9 40.3#


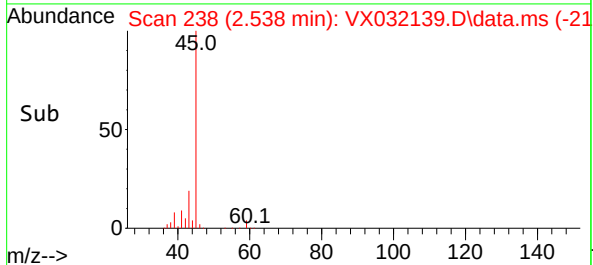

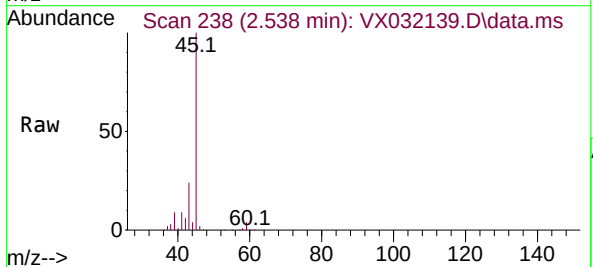




#16
Acetone
Concen: 98.045 ug/l
RT: 2.380 min Scan# 214
Delta R.T. -0.012 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00




Instrument :
MSVOA_X
ClientSampleId :
SV34211LRE


Tgt Ion: 43 Resp: 50779
Ion Ratio Lower Upper
43 100
58 27.8 23.8 35.8

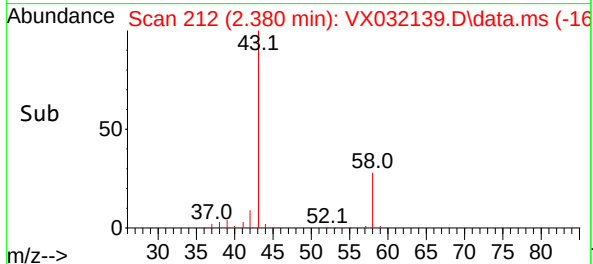

#18
Methyl Acetate
Concen: 56.385 ug/l
RT: 2.538 min Scan# 238
Delta R.T. -0.171 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00

Tgt Ion: 43 Resp: 96354
Ion Ratio Lower Upper
43 100
74 0.0 18.6 27.8#

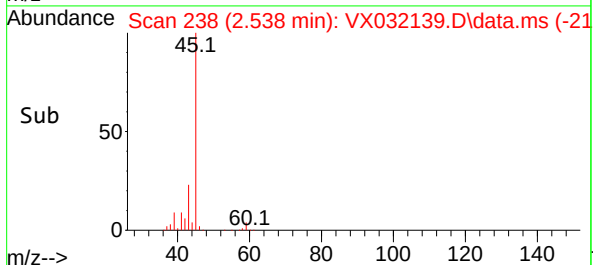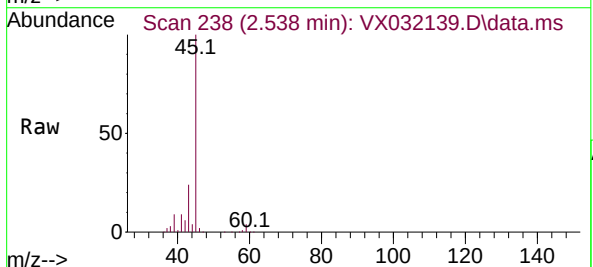



#25

2-Butanone

Concen: 8.372 ug/l

RT: 4.574 min Scan# 51

Delta R.T. 0.012 min

Lab File: VX032139.D

Acq: 14 Oct 2022 17:00

Instrument :

MSVOA_X

ClientSampleId :





SV34211LRE

Tgt Ion: 43 Resp: 6778

Ion Ratio Lower Upper

43 100

72 25.5 21.1 31.7



#29

Tetrahydrofuran

Concen: 1.910 ug/l

RT: 5.019 min Scan# 645

Delta R.T. 0.006 min

Lab File: VX032139.D

Acq: 14 Oct 2022 17:00




Tgt Ion: 42 Resp: 998


Ion Ratio Lower Upper

42 100

72 92.2 36.4 54.6#

71 93.3 33.5 50.3#

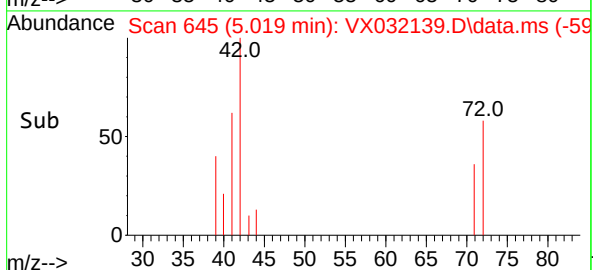



#33

1,2-Dichloroethane-d4

Concen: 27.803 ug/l

RT: 5.964 min Scan# 80

Delta R.T. 0.006 min

Lab File: VX032139.D

Acq: 14 Oct 2022 17:00

Instrument :

MSVOA_X

ClientSampleId :





SV34211LRE

Tgt Ion: 65 Resp: 42369

Ion Ratio Lower Upper

65 100

67 48.4 0.0 102.4

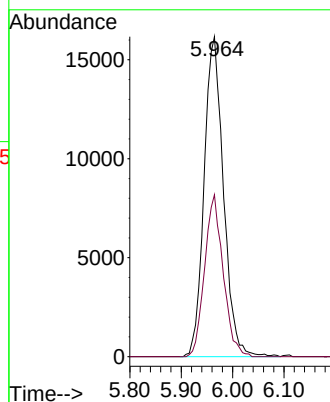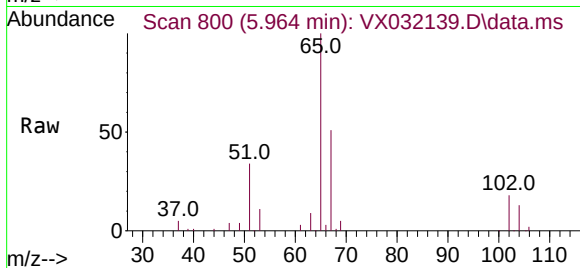

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.006 min

Lab File: VX032139.D

Acq: 14 Oct 2022 17:00




Tgt Ion: 114 Resp: 100226


Ion Ratio Lower Upper

114 100

63 19.6 0.0 42.6

88 15.1 0.0 33.0


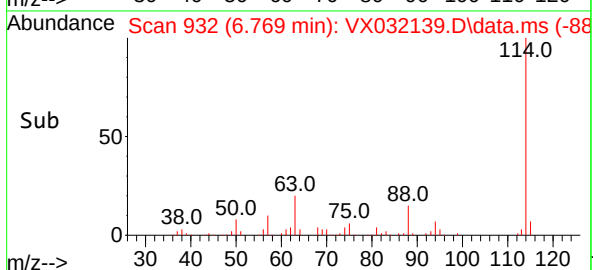

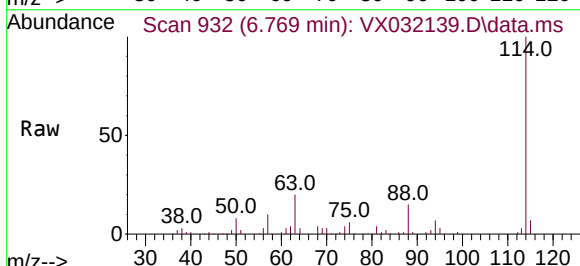




#35
Dibromofluoromethane
Concen: 26.608 ug/l
RT: 5.397 min Scan# 705
Delta R.T. 0.012 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00




Instrument :
MSVOA_X
ClientSampleId :
SV34211LRE


Tgt Ion:113 Resp: 30187
Ion Ratio Lower Upper
113 100
111 98.3 82.4 123.6
192 18.0 14.1 21.1

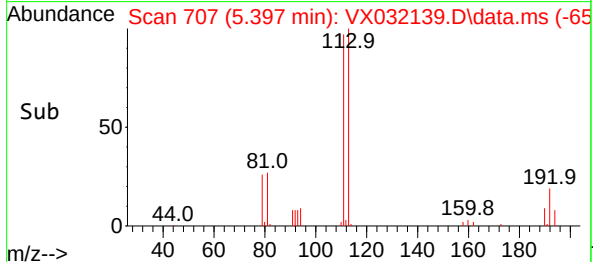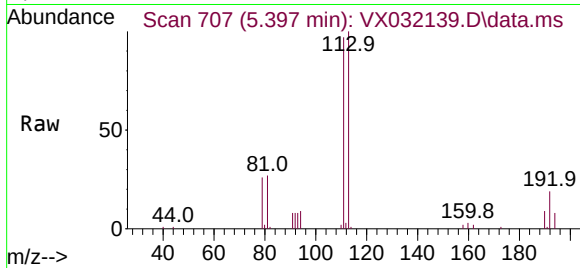

#36
1,1-Dichloropropene
Concen: 4.171 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.134 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00

Tgt Ion: 75 Resp: 6275
Ion Ratio Lower Upper
75 100
110 10.7 17.5 52.5#
77 0.0 24.9 37.3#

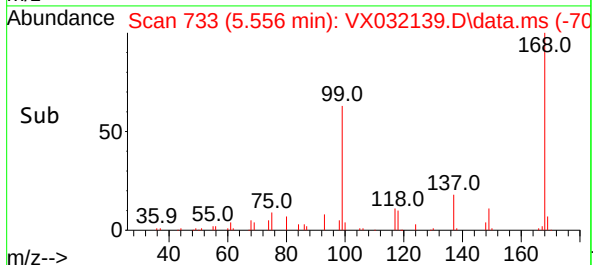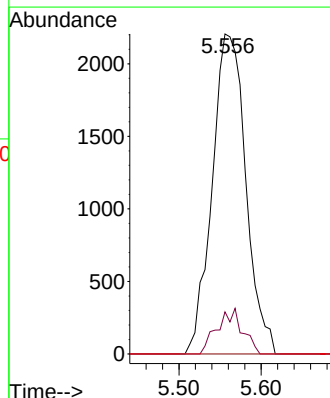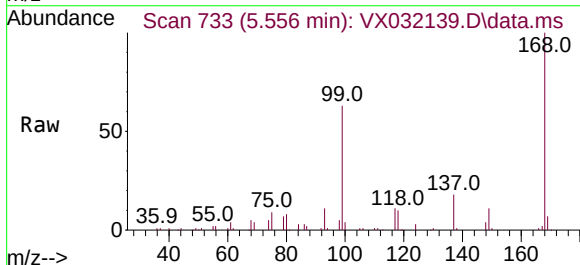



#37

Ethyl Acetate

Concen: 0.203 ug/l

RT: 4.666 min Scan# 51

Delta R.T. -0.048 min

Lab File: VX032139.D

Acq: 14 Oct 2022 17:00

Instrument :

MSVOA_X

ClientSampleId :

SV34211LRE





Tgt Ion: 43 Resp: 287

Ion Ratio Lower Upper

43 100

61 0.0 11.1 16.7#

70 0.0 8.6 13.0#

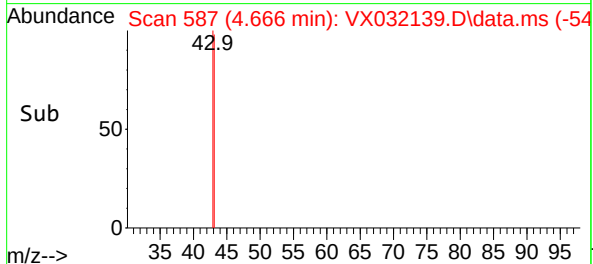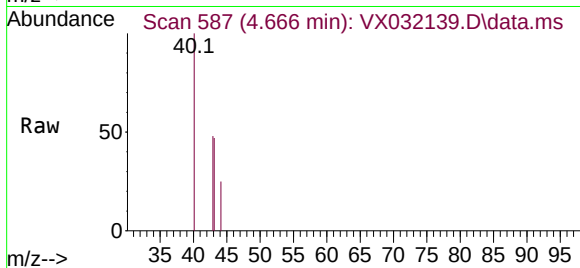

#38

Carbon Tetrachloride

Concen: 5.515 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.121 min

Lab File: VX032139.D

Acq: 14 Oct 2022 17:00




Tgt Ion: 117 Resp: 8483


Ion Ratio Lower Upper

117 100

119 7.2 74.6 112.0#

121 0.0 25.3 37.9#


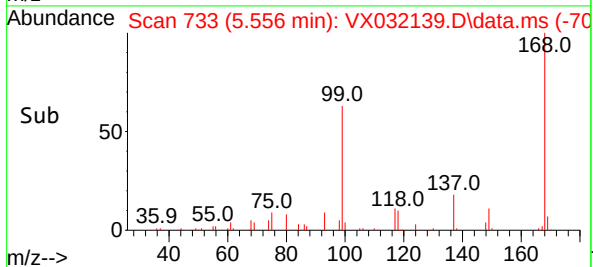

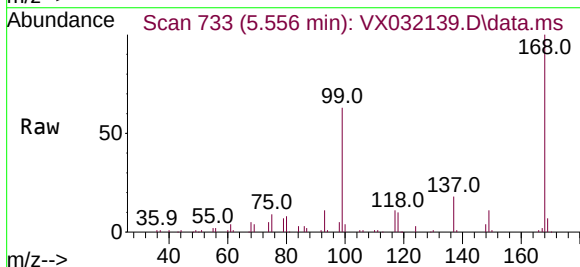




#40
Benzene
Concen: 0.292 ug/l
RT: 6.056 min Scan# 812
Delta R.T. 0.019 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00




Instrument :
MSVOA_X
ClientSampleId :
SV34211LRE


Tgt Ion: 78 Resp: 1285
Ion Ratio Lower Upper
78 100
77 13.5 18.7 28.1#

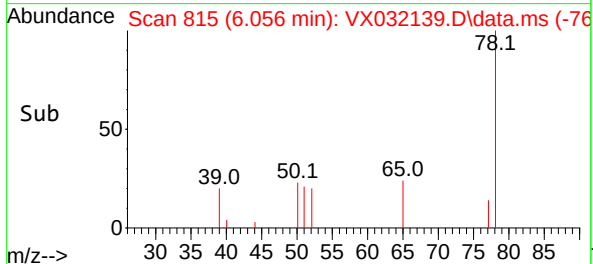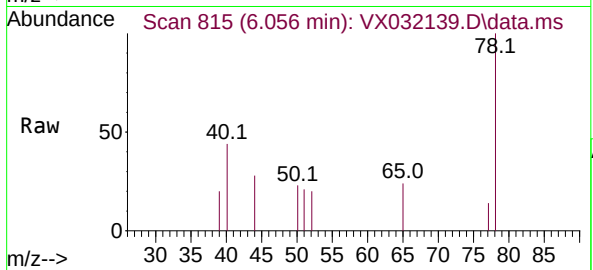

#41
Methacrylonitrile
Concen: 2.069 ug/l
RT: 5.038 min Scan# 648
Delta R.T. 0.116 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00

Tgt Ion: 41 Resp: 1524
Ion Ratio Lower Upper
41 100
39 37.5 45.0 67.6#
67 0.0 58.2 87.4#
52 0.0 25.0 37.6#

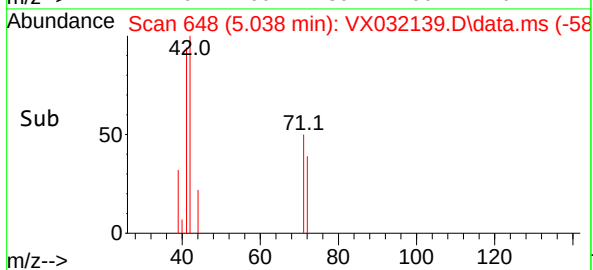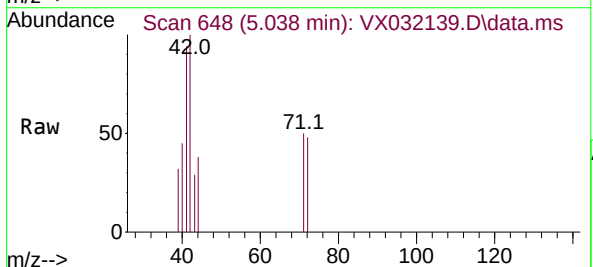



#49

1,4-Dioxane

Concen: Below Cal

RT: 7.684 min Scan# 1084

Delta R.T. -0.011 min

Lab File: VX032139.D

Acq: 14 Oct 2022 17:00

Instrument :

MSVOA_X

ClientSampleId :

SV34211LRE





Tgt Ion: 88 Resp: 212

Ion Ratio Lower Upper

88 100

43 25.9 27.1 40.7#

58 0.0 53.9 80.9#

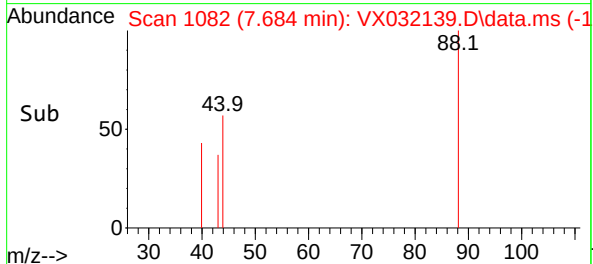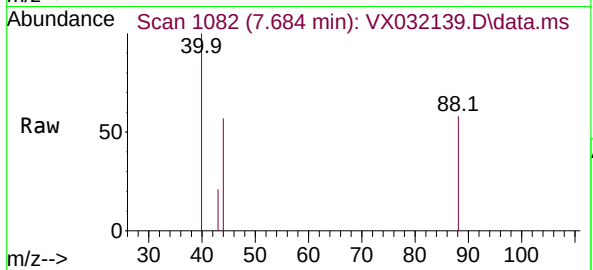

#50

Toluene-d8

Concen: 47.728 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX032139.D




Acq: 14 Oct 2022 17:00


Tgt Ion: 98 Resp: 194840

Ion Ratio Lower Upper

98 100

100 65.5 52.5 78.7

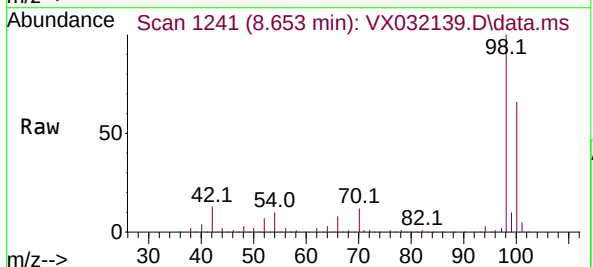

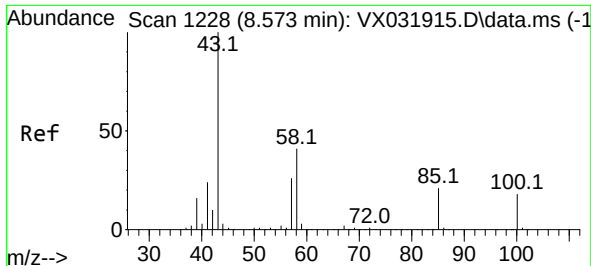

#51

4-Methyl-2-Pentanone

Concen: 0.503 ug/l

RT: 8.586 min Scan# 1230

Delta R.T. 0.013 min

Lab File: VX032139.D

Acq: 14 Oct 2022 17:00

Instrument :

MSVOA_X

ClientSampleId :





SV34211LRE

Tgt Ion: 43 Resp: 716

Ion Ratio Lower Upper

43 100

58 33.9 30.6 46.0

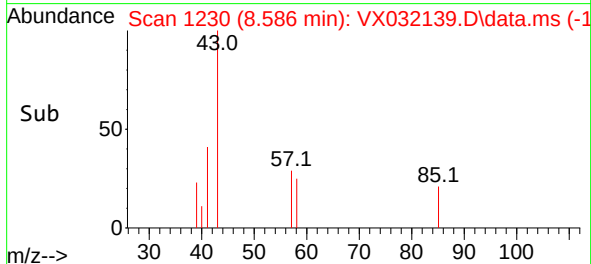

#52

Toluene

Concen: 4.456 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. 0.000 min

Lab File: VX032139.D




Acq: 14 Oct 2022 17:00


Tgt Ion: 92 Resp: 12835

Ion Ratio Lower Upper

92 100

91 170.5 137.1 205.7

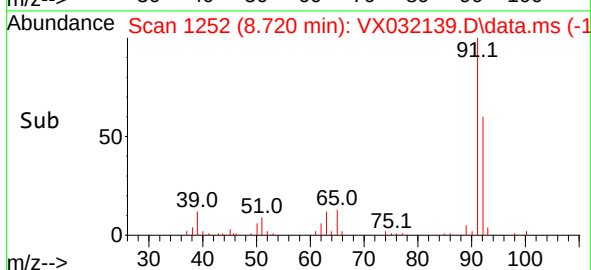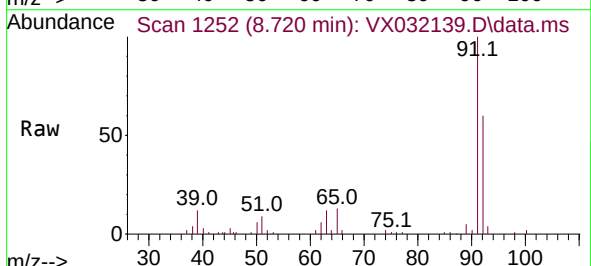



#53

t-1,3-Dichloropropene

Concen: 1.291 ug/l

RT: 8.720 min Scan# 11

Delta R.T. -0.262 min

Lab File: VX032139.D

Acq: 14 Oct 2022 17:00

Instrument :

MSVOA_X

ClientSampleId :





SV34211LRE

Tgt Ion: 75 Resp: 133

Ion Ratio Lower Upper

75 100

77 127.7 24.8 37.2#

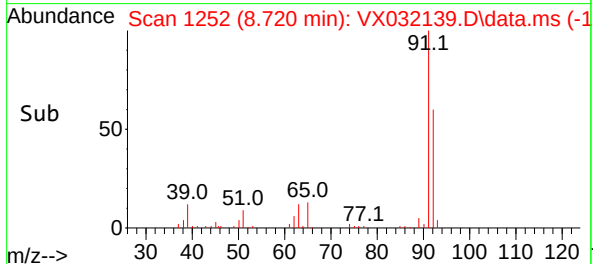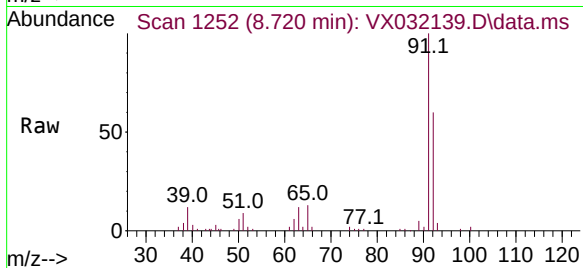

#62

4-Bromofluorobenzene

Concen: 38.765 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX032139.D

Acq: 14 Oct 2022 17:00




Tgt Ion: 95 Resp: 55946


Ion Ratio Lower Upper

95 100

174 77.2 0.0 153.2

176 71.8 0.0 144.0




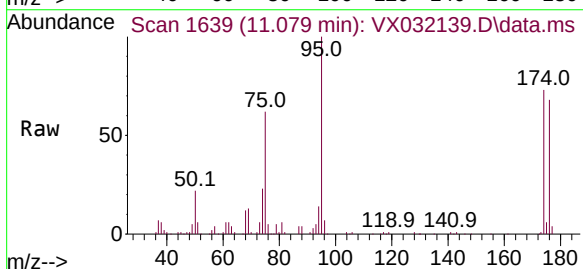




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00




Instrument :
MSVOA_X
ClientSampleId :
SV34211LRE


Tgt Ion:117 Resp: 74914
Ion Ratio Lower Upper
117 100
82 54.7 46.8 70.2
119 31.5 26.4 39.6

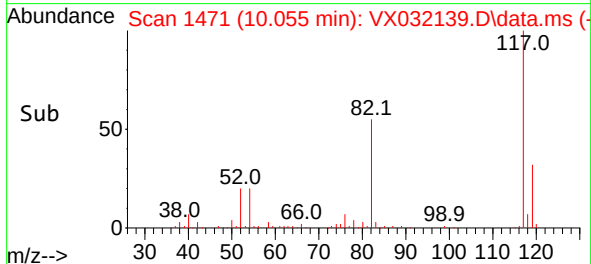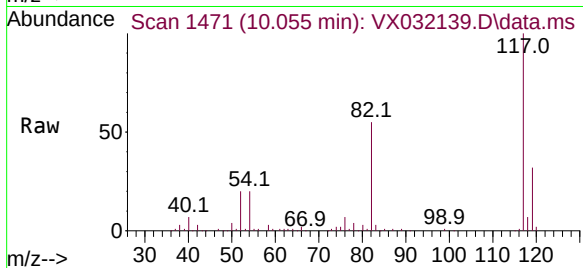

#67
Ethyl Benzene
Concen: 6.365 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00

Tgt Ion: 91 Resp: 24442
Ion Ratio Lower Upper
91 100
106 31.5 25.2 37.8


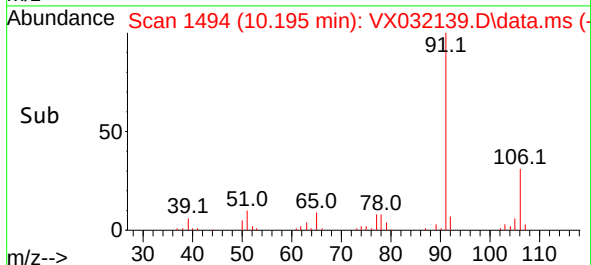
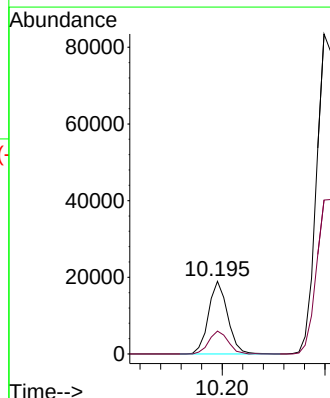
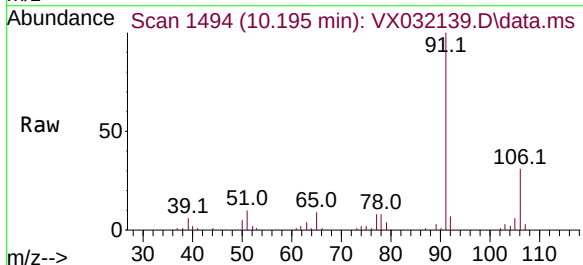


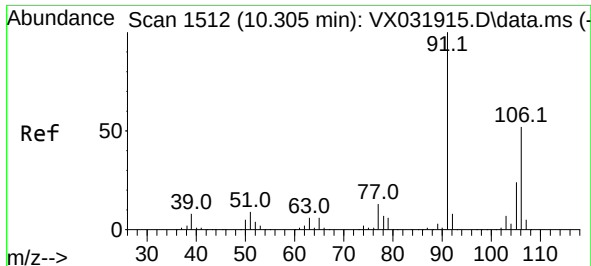

#68
m/p-Xylenes
Concen: 36.966 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00




Instrument :
MSVOA_X
ClientSampleId :
SV34211LRE


Tgt Ion:106 Resp: 56410
Ion Ratio Lower Upper
106 100
91 200.9 161.0 241.4

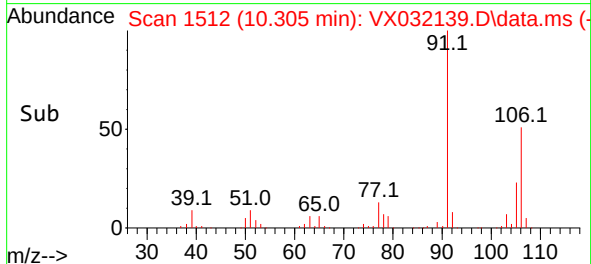

#69
o-Xylene
Concen: 27.830 ug/l
RT: 10.647 min Scan# 1568
Delta R.T. 0.007 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00

Tgt Ion:106 Resp: 41278
Ion Ratio Lower Upper
106 100
91 218.0 107.2 321.6

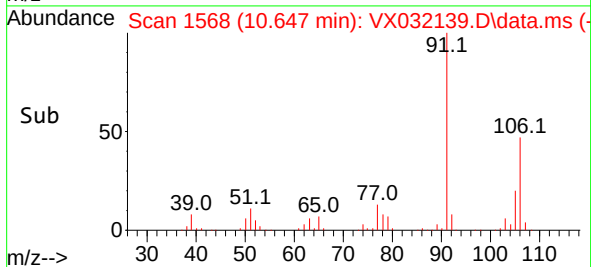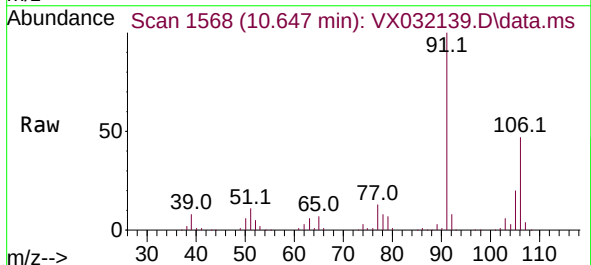



#70

Styrene

Concen: 0.910 ug/l

RT: 10.647 min Scan# 1

Delta R.T. -0.011 min

Lab File: VX032139.D

Acq: 14 Oct 2022 17:00

Instrument :

MSVOA_X

ClientSampleId :

SV34211LRE





Tgt Ion:104 Resp: 2157

Ion Ratio Lower Upper

104 100

78 323.0 41.4 62.2#

103 253.7 43.8 65.8#

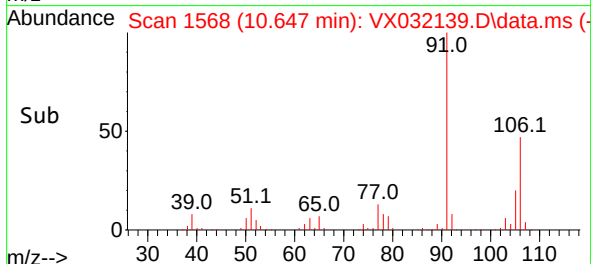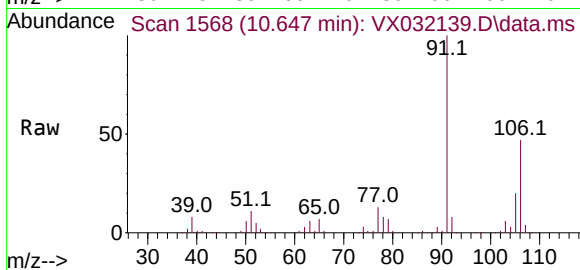

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX032139.D

Acq: 14 Oct 2022 17:00




Tgt Ion:152 Resp: 51142


Ion Ratio Lower Upper

152 100

115 65.0 43.4 130.1

150 156.6 0.0 346.8


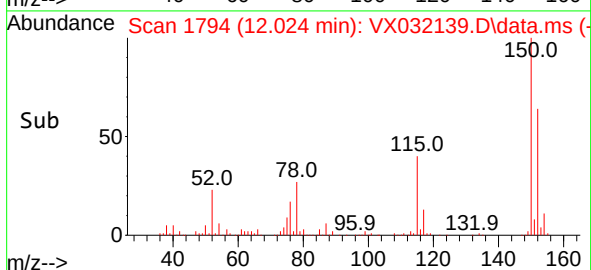

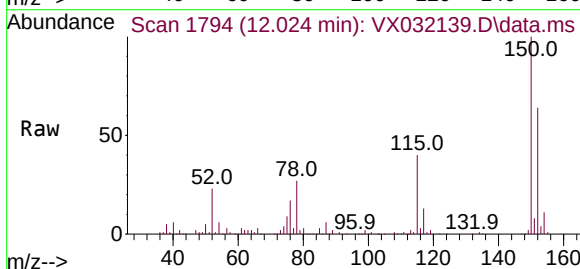




#73
Isopropylbenzene
Concen: 2.228 ug/l
RT: 10.964 min Scan# 1687
Delta R.T. 0.001 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00




Instrument :
MSVOA_X
ClientSampleId :
SV34211LRE


Tgt Ion:105 Resp: 8594
Ion Ratio Lower Upper
105 100
120 26.3 13.7 41.0

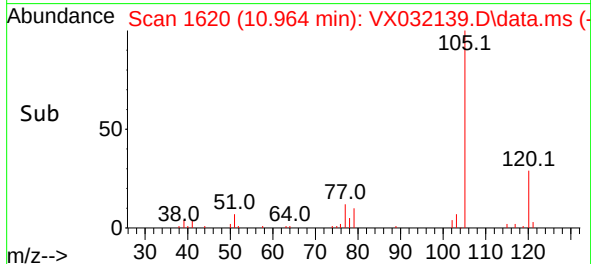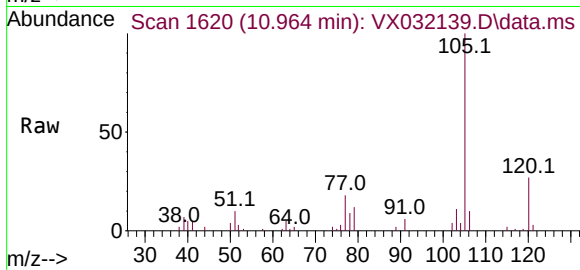

#76
1,2,3-Trichloropropane
Concen: 2.056 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.141 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00

Tgt Ion: 75 Resp: 2155
Ion Ratio Lower Upper
75 100
77 1267.9 20.3 60.9#


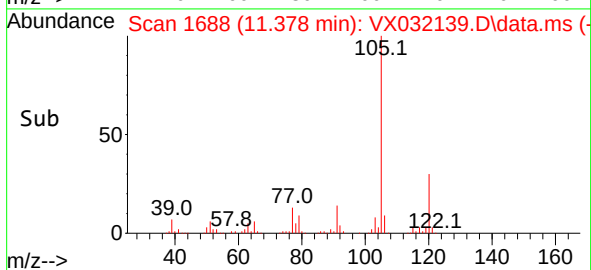

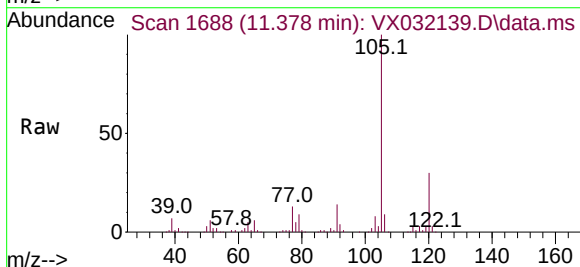


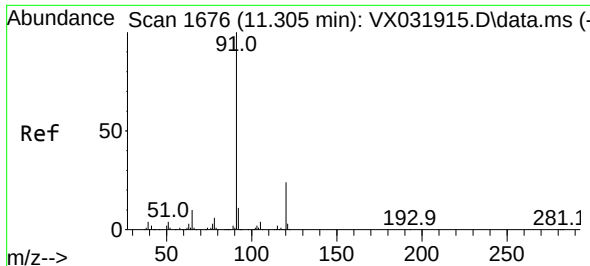

#78
n-propylbenzene
Concen: 6.598 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00




Instrument :
MSVOA_X
ClientSampleId :
SV34211LRE


Tgt Ion: 91 Resp: 28948
Ion Ratio Lower Upper
91 100
120 22.7 11.8 35.4

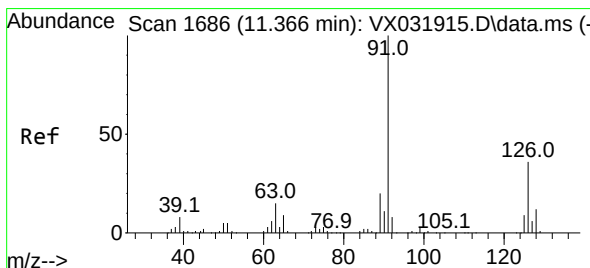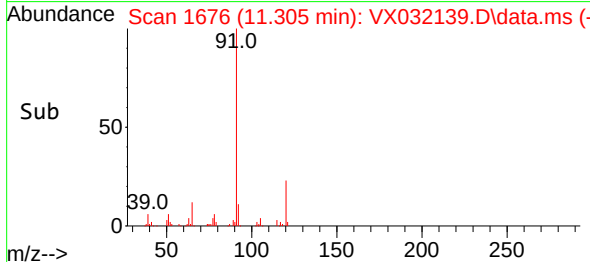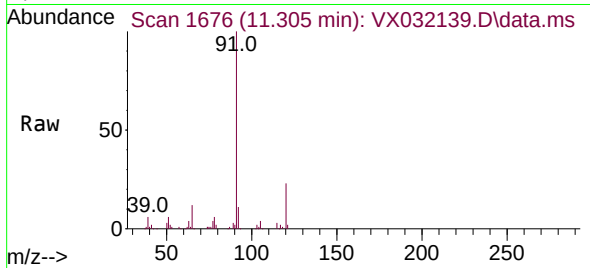

#79
2-Chlorotoluene
Concen: 11.153 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00

Tgt Ion: 91 Resp: 29445
Ion Ratio Lower Upper
91 100
126 0.0 17.4 52.3#

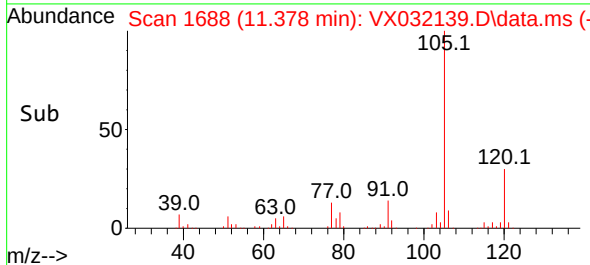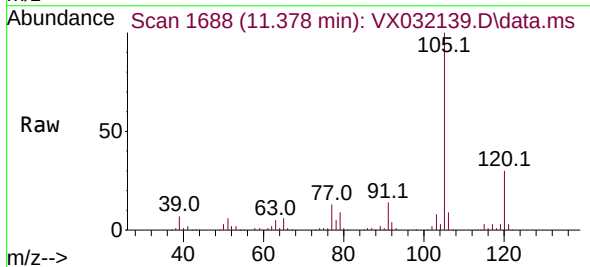



#80

1,3,5-Trimethylbenzene

Concen: 23.972 ug/l

RT: 11.451 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX032139.D

Acq: 14 Oct 2022 17:00

Instrument :

MSVOA_X

ClientSampleId :





SV34211LRE

Tgt Ion:105 Resp: 76688

Ion Ratio Lower Upper

105 100

120 48.1 24.5 73.5

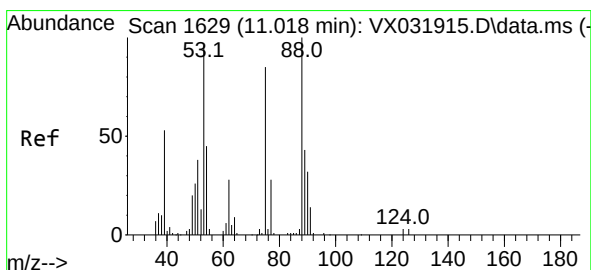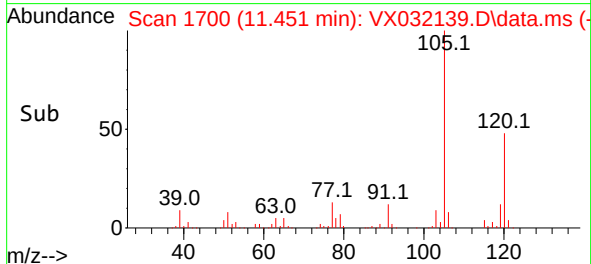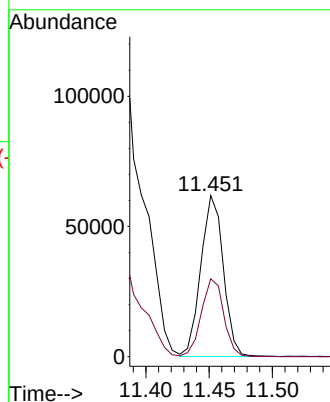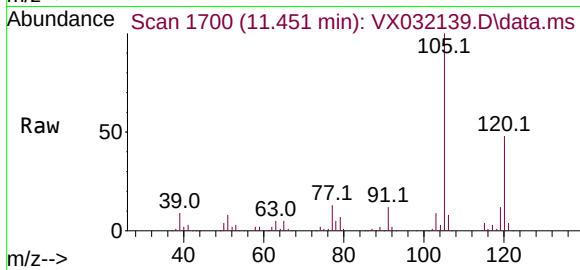

#81

trans-1,4-Dichloro-2-butene

Concen: 107.108 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX032139.D

Acq: 14 Oct 2022 17:00




Tgt Ion: 75 Resp: 32944


Ion Ratio Lower Upper

75 100

53 0.0 77.6 116.4#

89 0.0 37.4 56.0#




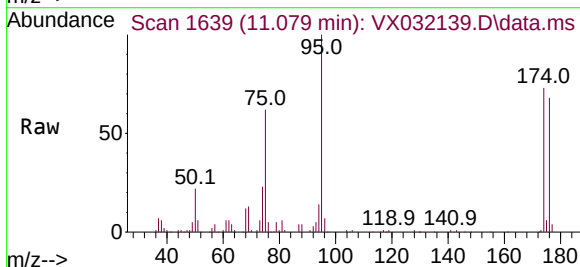




#82
4-Chlorotoluene
Concen: 3.099 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00




Instrument :
MSVOA_X
ClientSampleId :
SV34211LRE


Tgt Ion: 91 Resp: 9372
Ion Ratio Lower Upper
91 100
126 0.0 15.1 45.3#

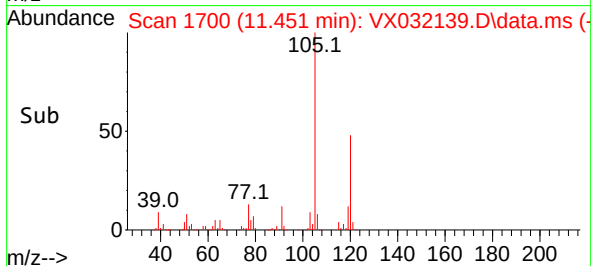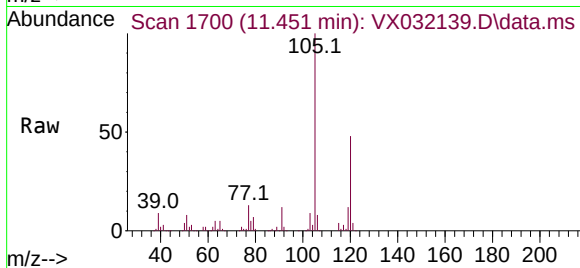

#83
tert-Butylbenzene
Concen: 4.418 ug/l
RT: 11.969 min Scan# 1785
Delta R.T. 0.256 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00

Tgt Ion: 119 Resp: 13988
Ion Ratio Lower Upper
119 100
91 37.6 29.2 87.6
134 27.4 11.6 34.8


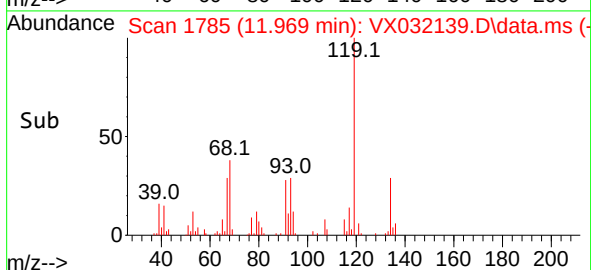

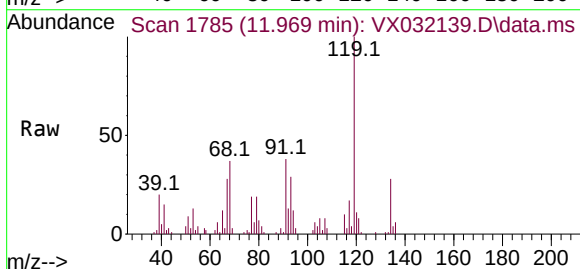


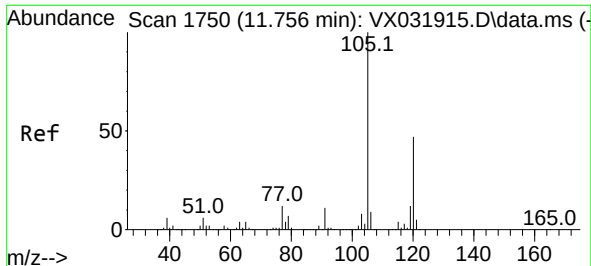

#84
1,2,4-Trimethylbenzene
Concen: 107.610 ug/l
RT: 11.750 min Scan# 1750
Delta R.T. -0.006 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00




Instrument :
MSVOA_X
ClientSampleId :
SV34211LRE


Tgt Ion:105 Resp: 349720
Ion Ratio Lower Upper
105 100
120 44.0 22.6 67.8

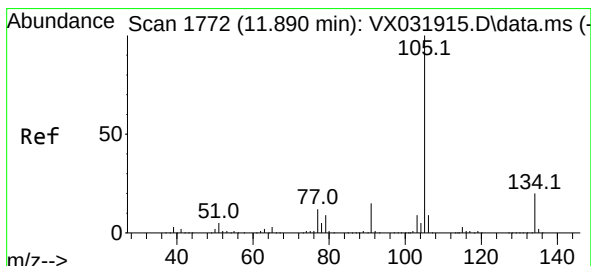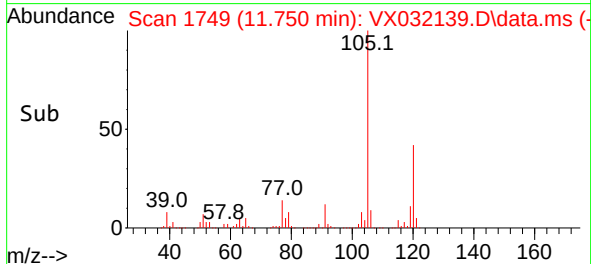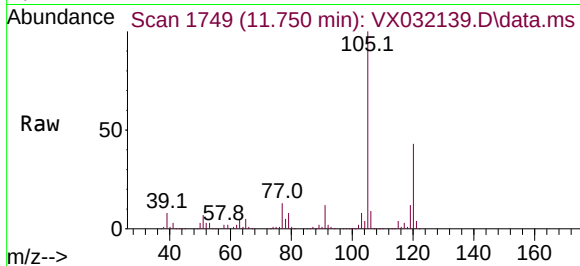

#85
sec-Butylbenzene
Concen: 89.215 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.140 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00

Tgt Ion:105 Resp: 349720
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#


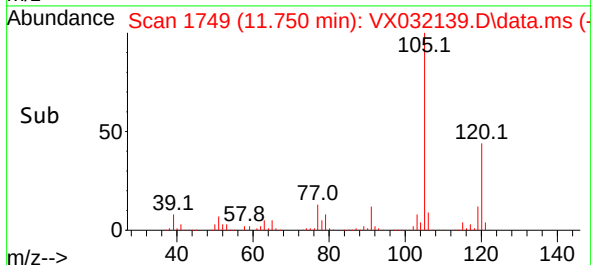

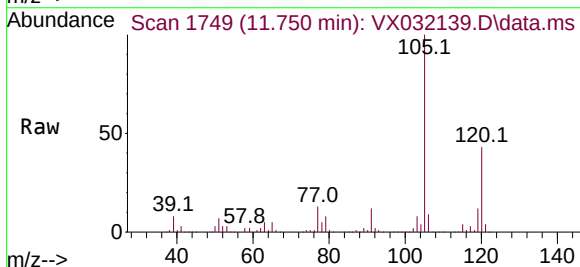


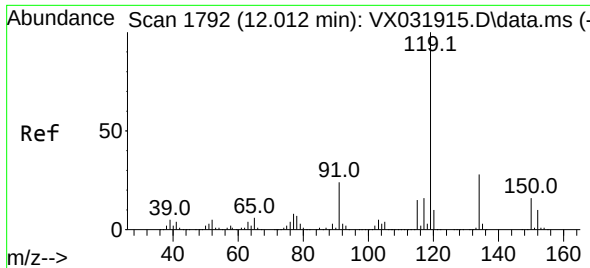

#86
p-Isopropyltoluene
Concen: 2.185 ug/l
RT: 12.012 min Scan# 119
Delta R.T. 0.000 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00




Instrument :
MSVOA_X
ClientSampleId :
SV34211LRE


Tgt Ion:119 Resp: 7213
Ion Ratio Lower Upper
119 100
134 25.6 13.4 40.2
91 29.7 12.4 37.2

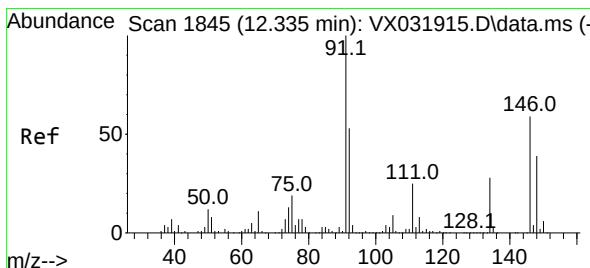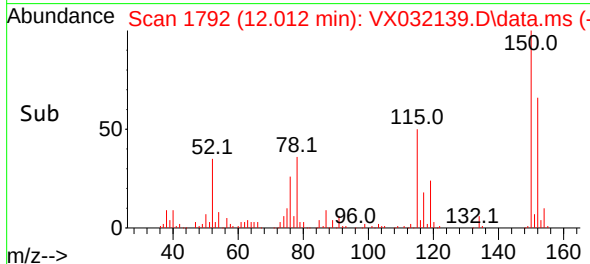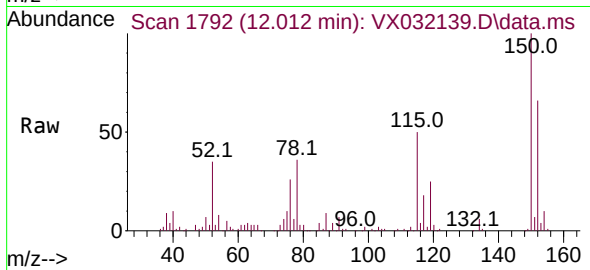

#89
n-Butylbenzene
Concen: 7.710 ug/l
RT: 12.323 min Scan# 1843
Delta R.T. -0.012 min
Lab File: VX032139.D
Acq: 14 Oct 2022 17:00

Tgt Ion: 91 Resp: 21310
Ion Ratio Lower Upper
91 100
92 27.6 27.0 81.0
134 111.8 13.3 39.9#

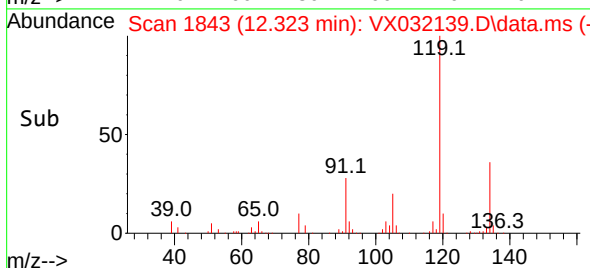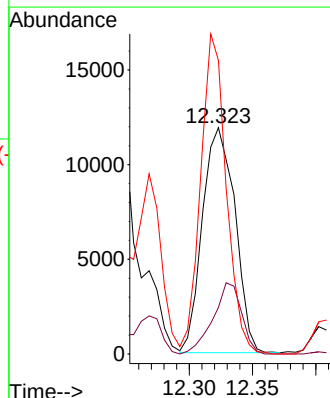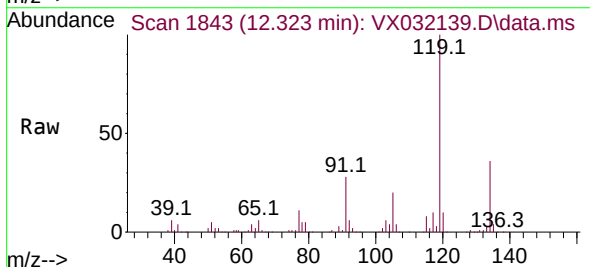



#90

Hexachloroethane

Concen: 12.597 ug/l

RT: 12.530 min Scan# 117

Delta R.T. -0.012 min

Lab File: VX032139.D

Acq: 14 Oct 2022 17:00

Instrument :

MSVOA_X

ClientSampleId :





SV34211LRE

Tgt Ion:117 Resp: 6084

Ion Ratio Lower Upper

117 100

201 0.0 34.8 104.4#

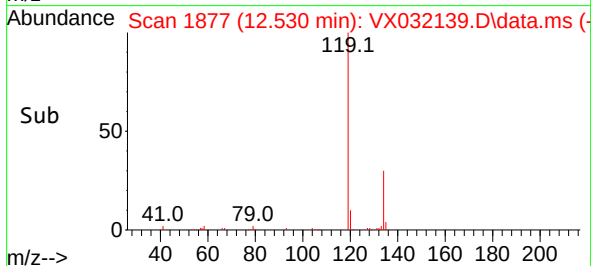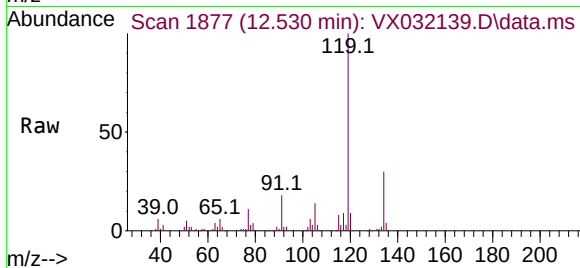

#92

1,2-Dibromo-3-Chloropropane

Concen: 2.719 ug/l

RT: 12.963 min Scan# 1948

Delta R.T. 0.019 min

Lab File: VX032139.D

Acq: 14 Oct 2022 17:00




Tgt Ion: 75 Resp: 610


Ion Ratio Lower Upper

75 100

155 0.0 40.3 120.8#

157 0.0 51.5 154.5#

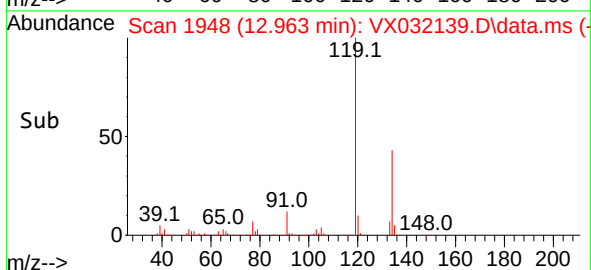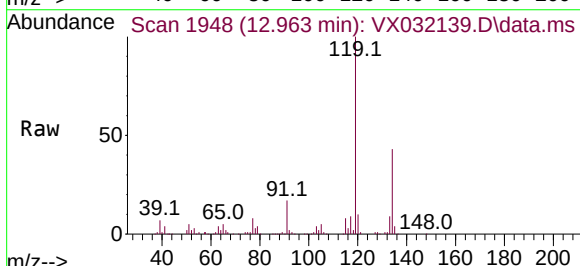

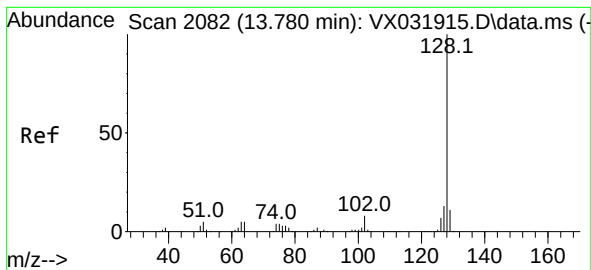

#95

Naphthalene

Concen: 41.777 ug/l

RT: 13.774 min Scan# 20

Delta R.T. -0.006 min

Lab File: VX032139.D


Acq: 14 Oct 2022 17:00

Instrument :

MSVOA_X

ClientSampleId :

SV34211LRE

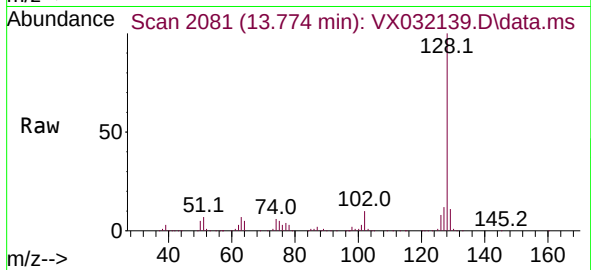

Tgt Ion:128 Resp: 156279

Ion Ratio Lower Upper

128 100

127 12.3 10.4 15.6

129 11.5 8.8 13.2

