

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101422\
 Data File : VX032131.D
 Acq On : 14 Oct 2022 13:57
 Operator : JC/MD
 Sample : N5151-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 256317-6

Quant Time: Oct 17 02:24:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 06 14:28:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	87340	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	131689	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	135204	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	66463	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	95676	53.043	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 106.080%	
35) Dibromofluoromethane	5.385	113	72280	48.489	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 96.980%	
50) Toluene-d8	8.647	98	267387	49.850	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 99.700%	
62) 4-Bromofluorobenzene	11.079	95	73802	38.920	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 77.840%#	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101422\
Data File : VX032131.D
Acq On : 14 Oct 2022 13:57
Operator : JC/MD
Sample : N5151-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
256317-6

Quant Time: Oct 17 02:24:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 14:28:46 2022
Response via : Initial Calibration




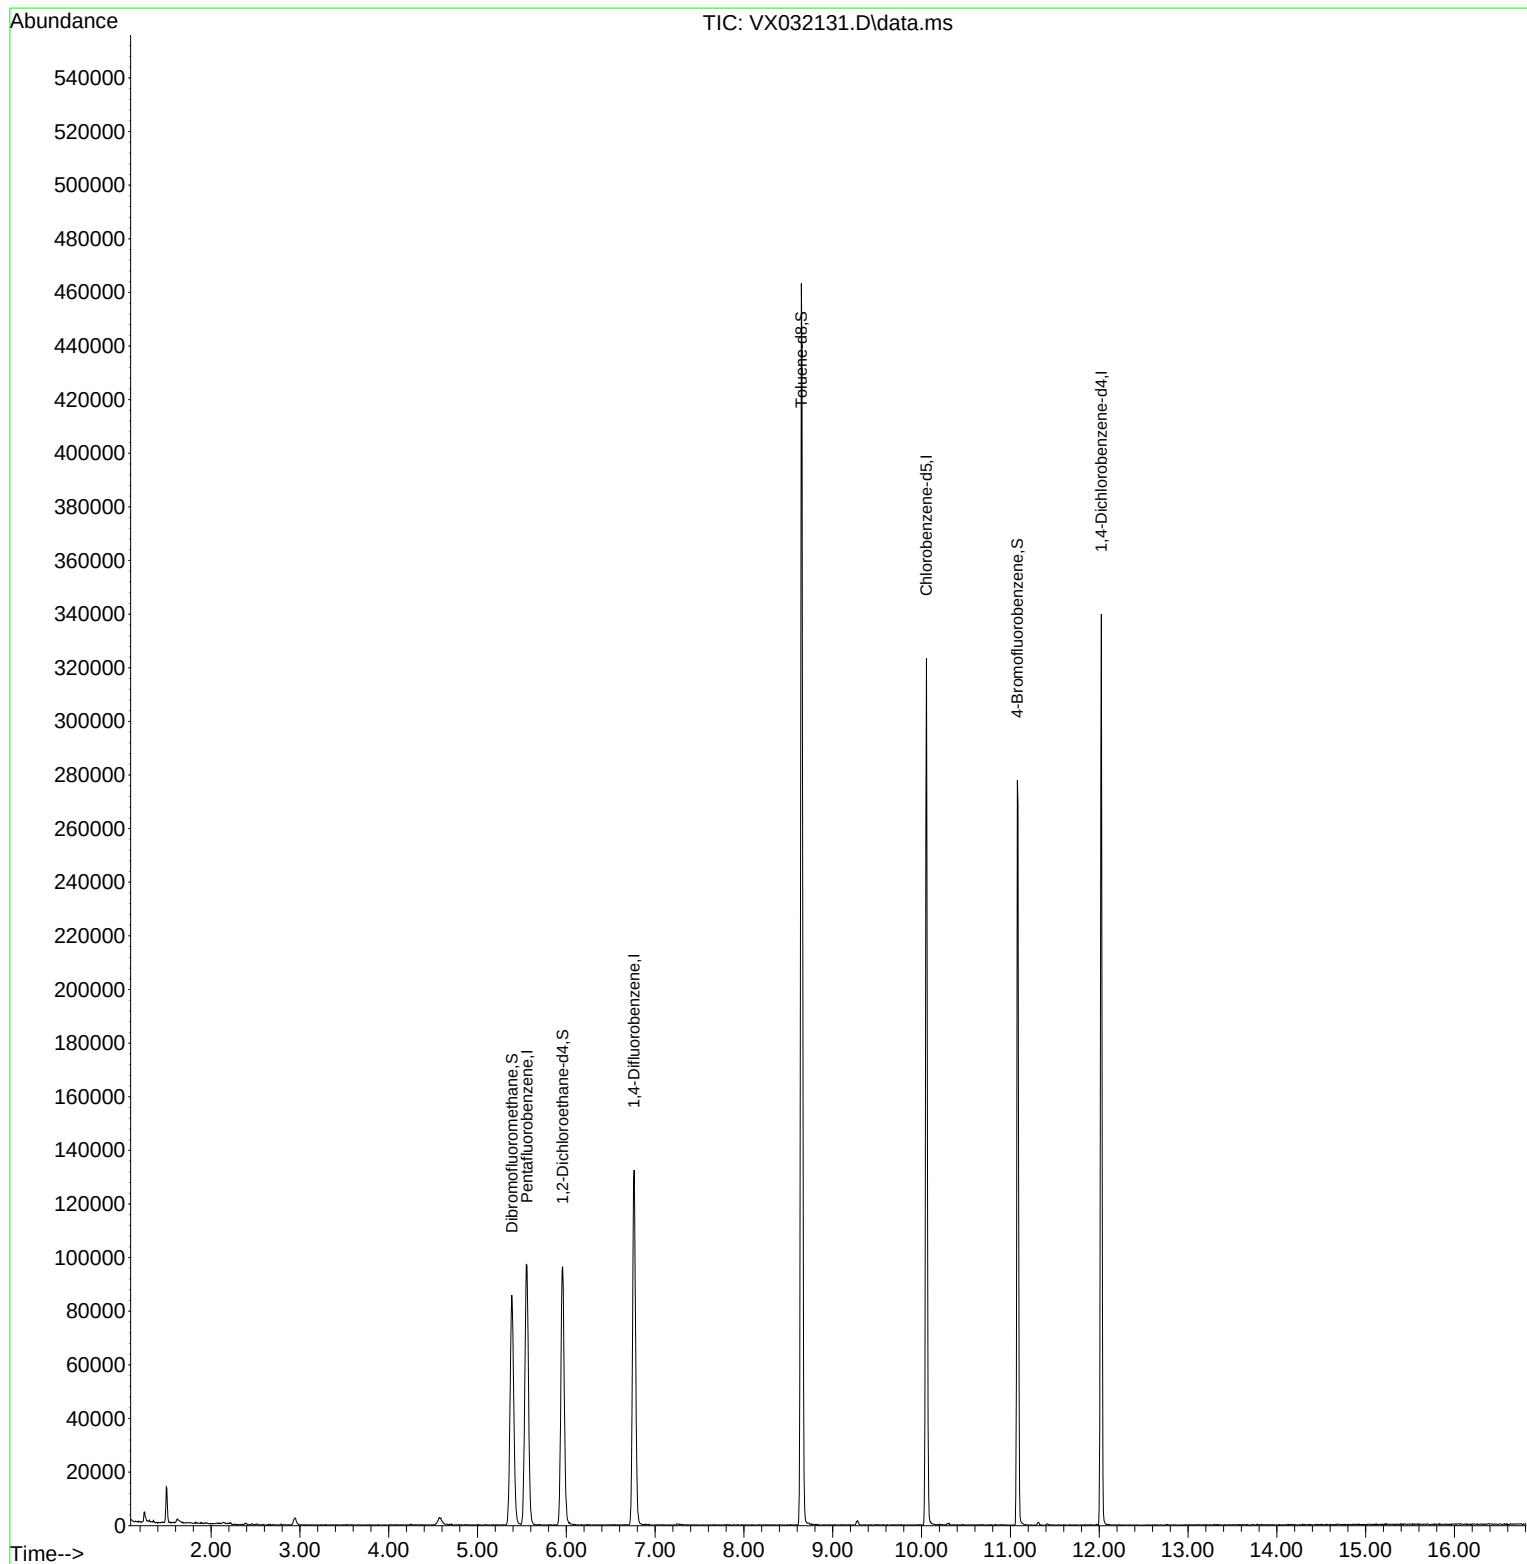


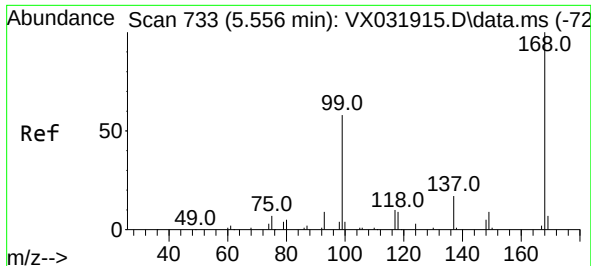

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.000 min
Lab File: VX032131.D
Acq: 14 Oct 2022 13:57




Instrument :
MSVOA_X
ClientSampleId :
256317-6


Tgt Ion:168 Resp: 87340
Ion Ratio Lower Upper
168 100
99 63.3 48.8 73.2

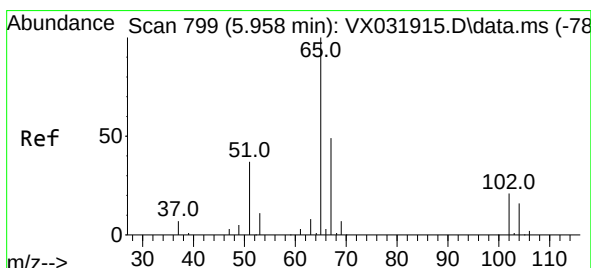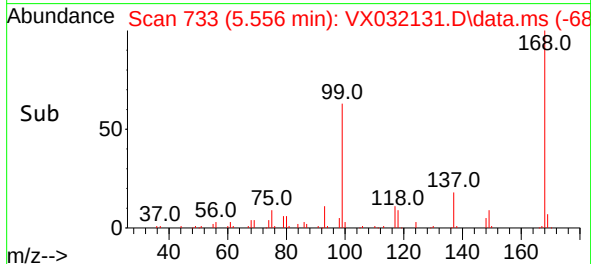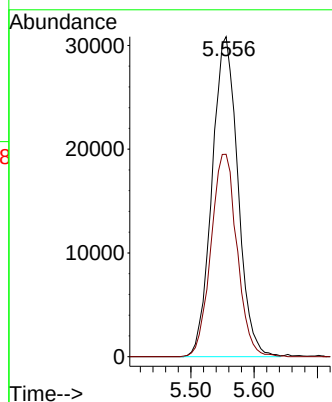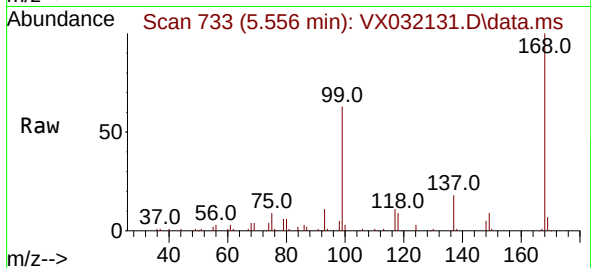

#33
1,2-Dichloroethane-d4
Concen: 53.043 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX032131.D
Acq: 14 Oct 2022 13:57

Tgt Ion: 65 Resp: 95676
Ion Ratio Lower Upper
65 100
67 49.6 0.0 102.4


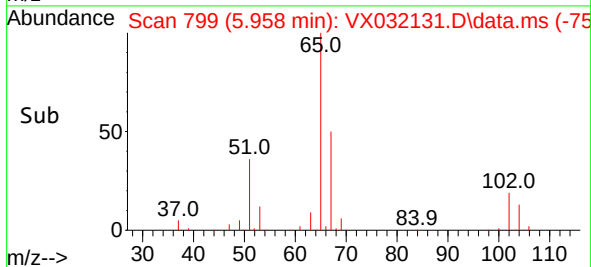
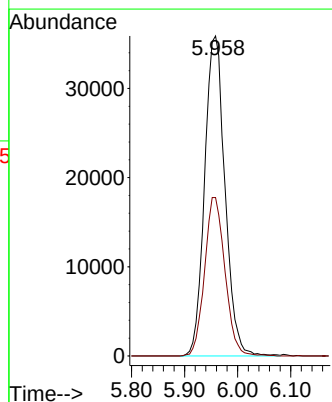
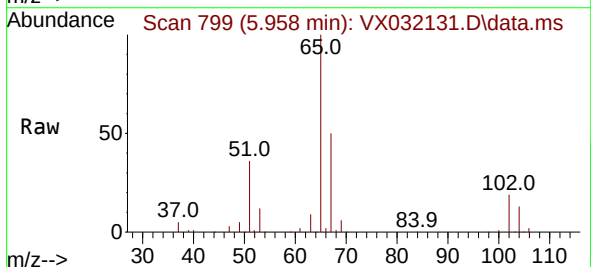


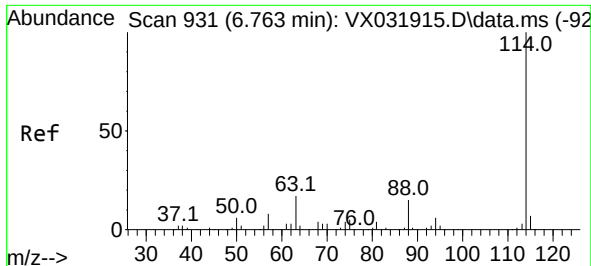

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX032131.D
Acq: 14 Oct 2022 13:57




Instrument :
MSVOA_X
ClientSampleId :
256317-6


Tgt Ion:114 Resp: 131689
Ion Ratio Lower Upper
114 100
63 21.1 0.0 42.6
88 15.1 0.0 33.0

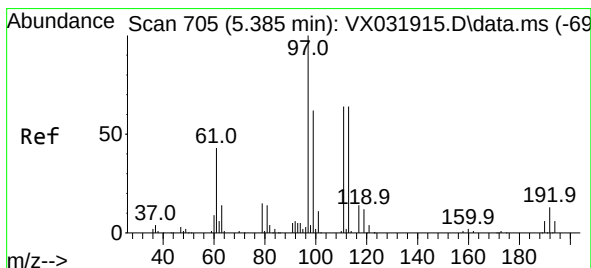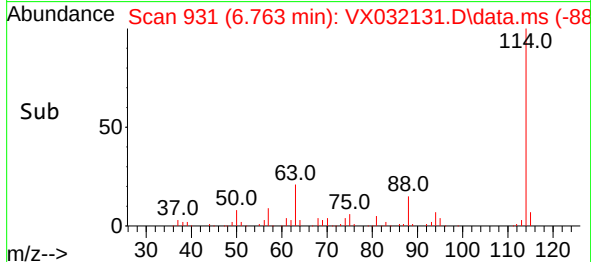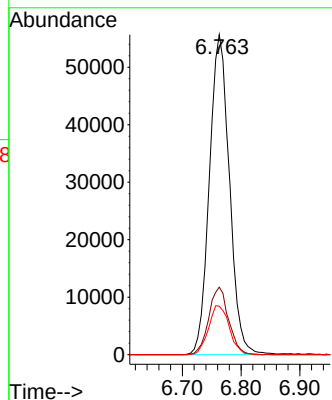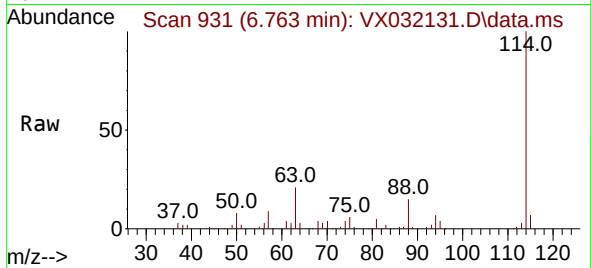

#35
Dibromofluoromethane
Concen: 48.489 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX032131.D
Acq: 14 Oct 2022 13:57

Tgt Ion:113 Resp: 72280
Ion Ratio Lower Upper
113 100
111 101.7 82.4 123.6
192 17.5 14.1 21.1


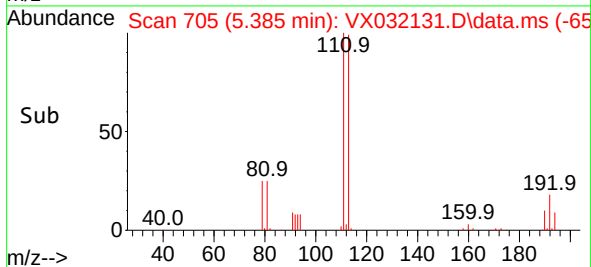
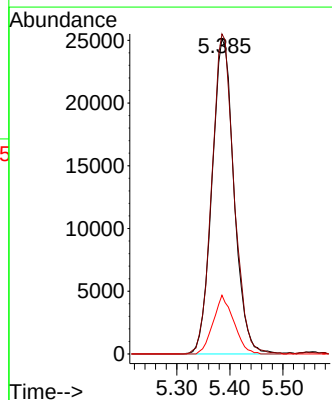
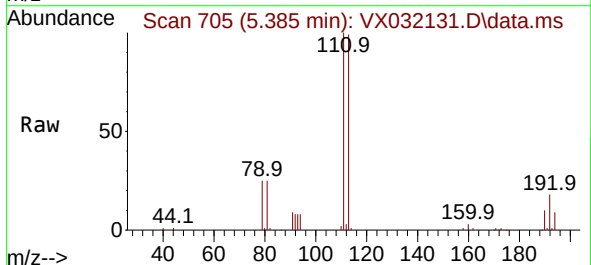


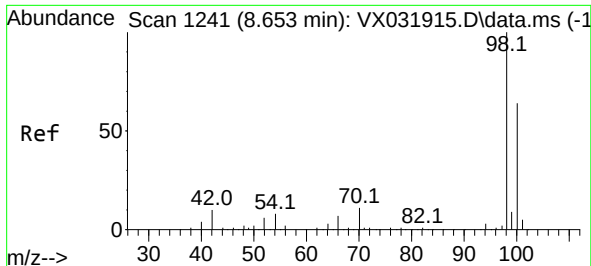

#50
Toluene-d8
Concen: 49.850 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX032131.D
Acq: 14 Oct 2022 13:57




Instrument :
MSVOA_X
ClientSampleId :
256317-6


Tgt Ion: 98 Resp: 267387
Ion Ratio Lower Upper
98 100
100 65.1 52.5 78.7

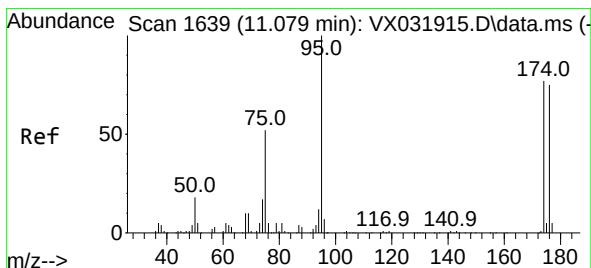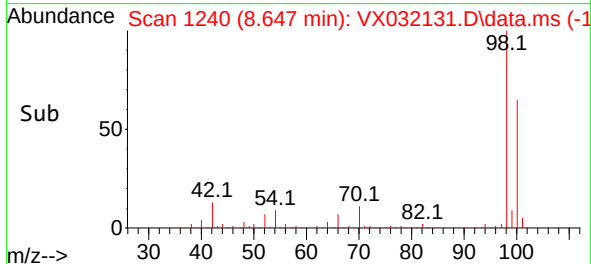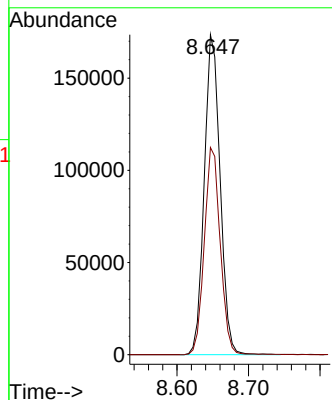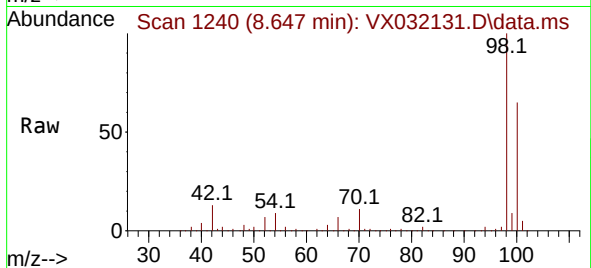

#62
4-Bromofluorobenzene
Concen: 38.920 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX032131.D
Acq: 14 Oct 2022 13:57

Tgt Ion: 95 Resp: 73802
Ion Ratio Lower Upper
95 100
174 78.1 0.0 153.2
176 75.3 0.0 144.0


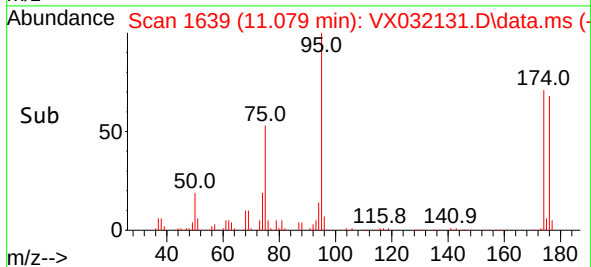
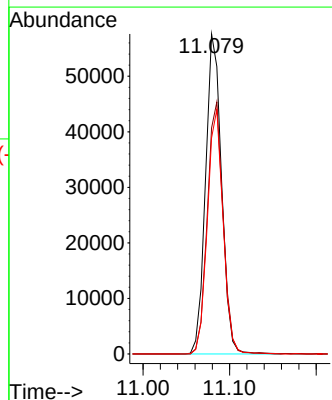
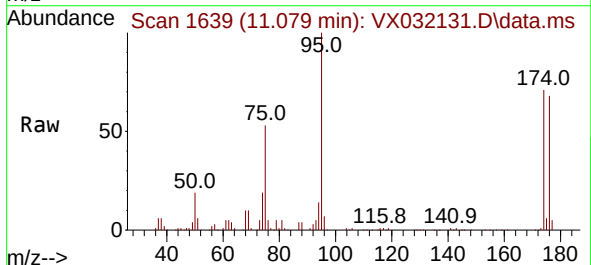


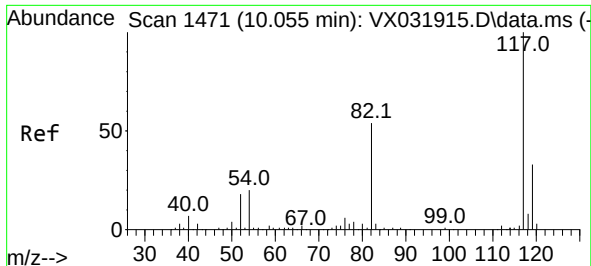

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX032131.D
Acq: 14 Oct 2022 13:57

Instrument :
MSVOA_X
ClientSampleId :
256317-6

Tgt Ion:117 Resp: 135204
Ion Ratio Lower Upper
117 100
82 58.2 46.8 70.2
119 32.7 26.4 39.6

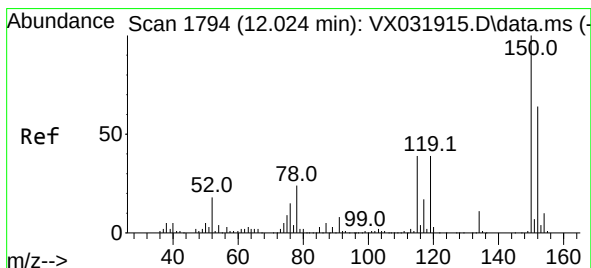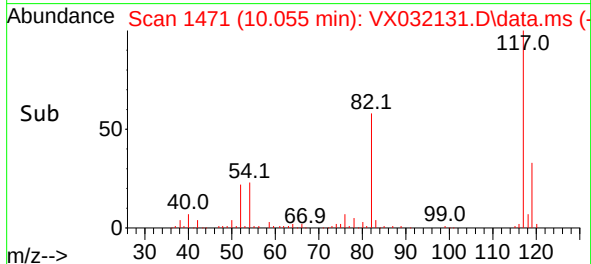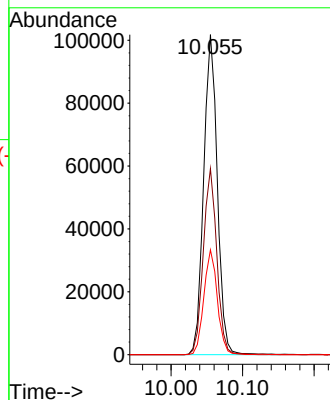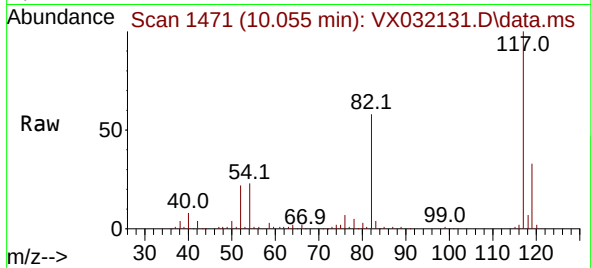

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX032131.D
Acq: 14 Oct 2022 13:57

Tgt Ion:152 Resp: 66463
Ion Ratio Lower Upper
152 100
115 61.5 43.4 130.1
150 157.9 0.0 346.8

