

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101422\
 Data File : VX032143.D
 Acq On : 14 Oct 2022 18:33
 Operator : JC/MD
 Sample : N5146-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SAMPLE-MANAG

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M

Title : SW846 8260

Signal : TIC: VX032143.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.788	273	279	287	rVB2	3263	5778	1.09%	0.196%
2	2.940	295	304	316	rBV	22595	52502	9.89%	1.783%
3	4.580	560	573	588	rBV	17784	65665	12.37%	2.230%
4	5.385	695	705	719	rBV	79300	228346	43.02%	7.756%
5	5.556	722	733	747	rVB	91998	259843	48.95%	8.826%
6	5.958	789	799	816	rBV	91908	242269	45.64%	8.229%
7	6.763	921	931	943	rBV	124938	293279	55.25%	9.962%
8	8.653	1232	1241	1255	rBV	332297	530843	100.00%	18.031%
9	10.055	1465	1471	1485	rBV	293902	388876	73.26%	13.209%
10	11.079	1634	1639	1649	rBV	345299	445630	83.95%	15.137%
11	12.024	1788	1794	1801	rBV	350393	430981	81.19%	14.639%




Sum of corrected areas: 2944012

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101422\
Data File : VX032143.D
Acq On : 14 Oct 2022 18:33
Operator : JC/MD
Sample : N5146-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

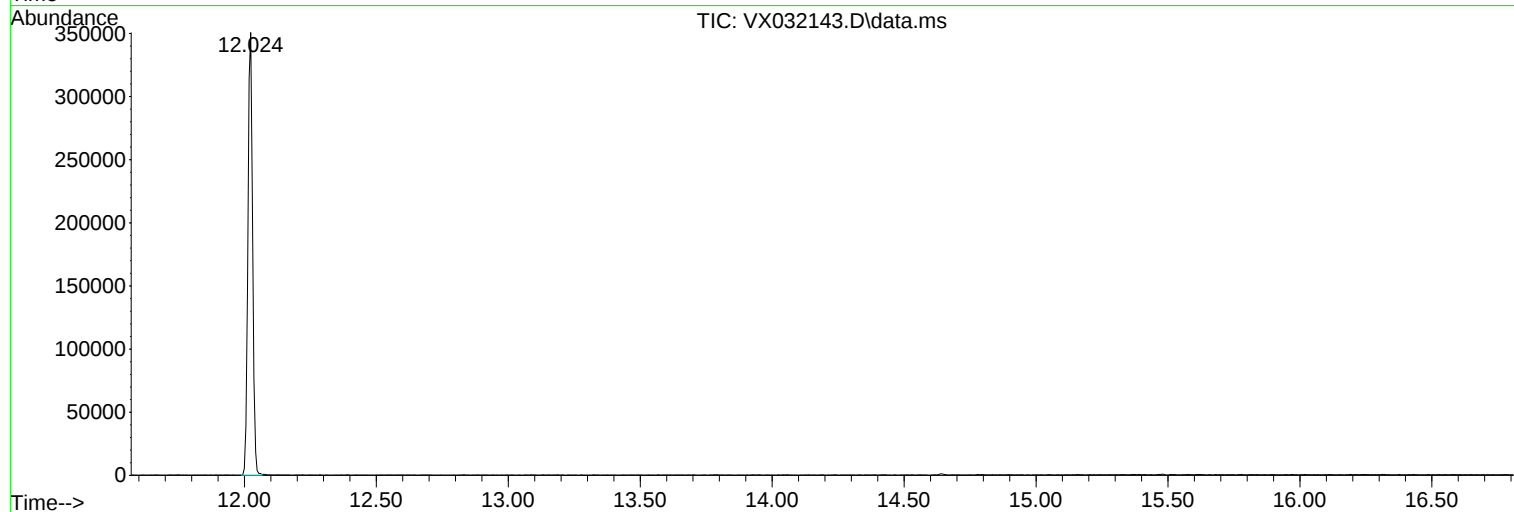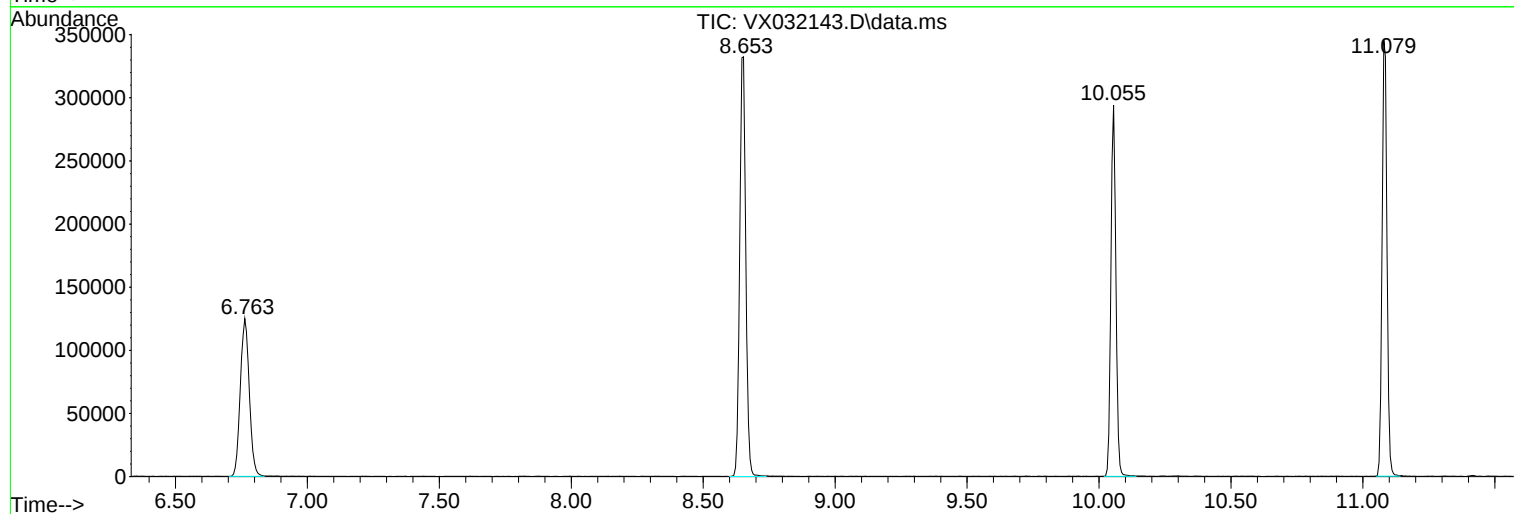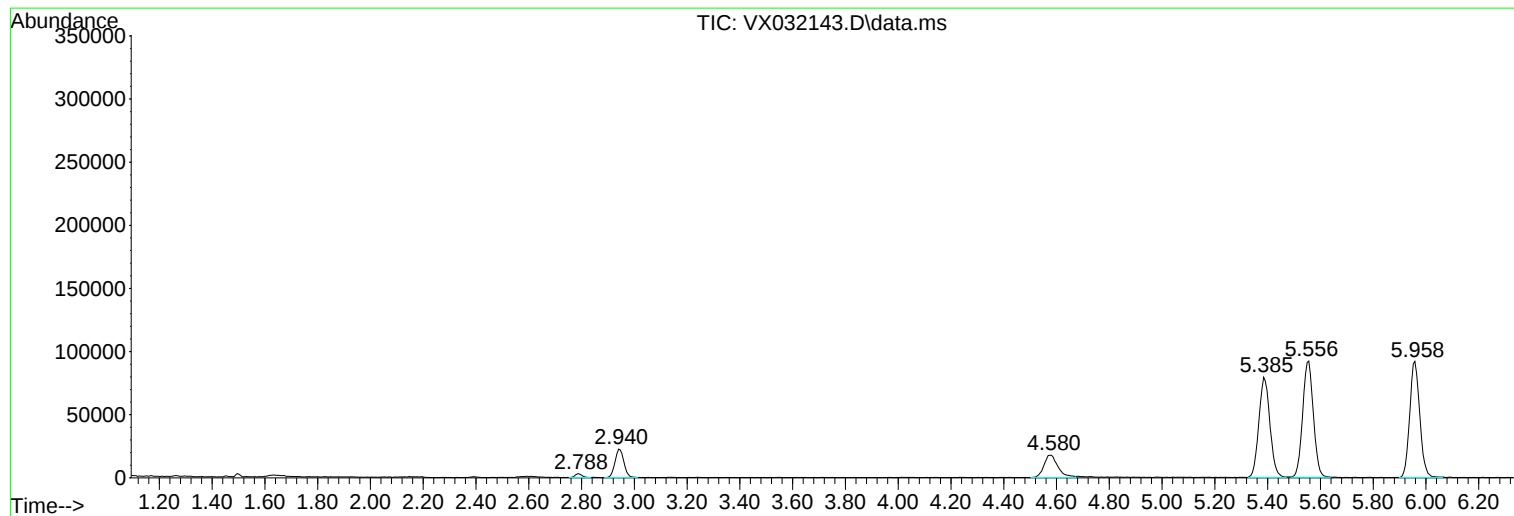

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101422\
Data File : VX032143.D
Acq On : 14 Oct 2022 18:33
Operator : JC/MD
Sample : N5146-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101422\
Data File : VX032143.D
Acq On : 14 Oct 2022 18:33
Operator : JC/MD
Sample : N5146-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc