
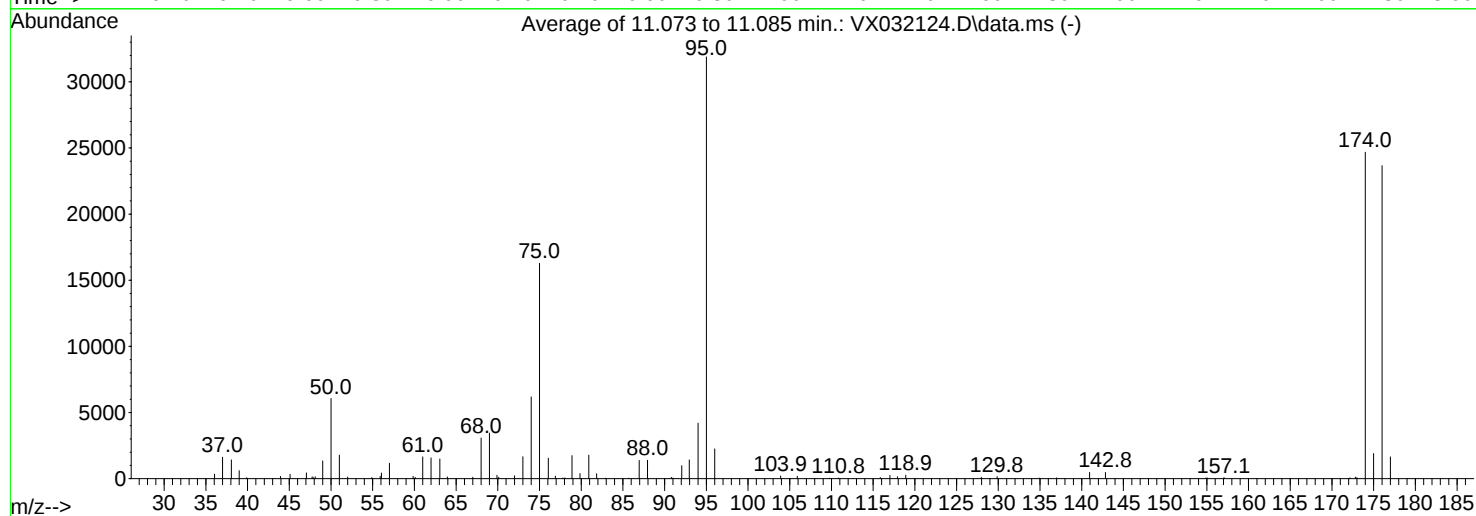


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101422\
 Data File : VX032124.D
 Acq On : 14 Oct 2022 09:38
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Title : SW846 8260
 Last Update : Thu Oct 06 14:28:46 2022

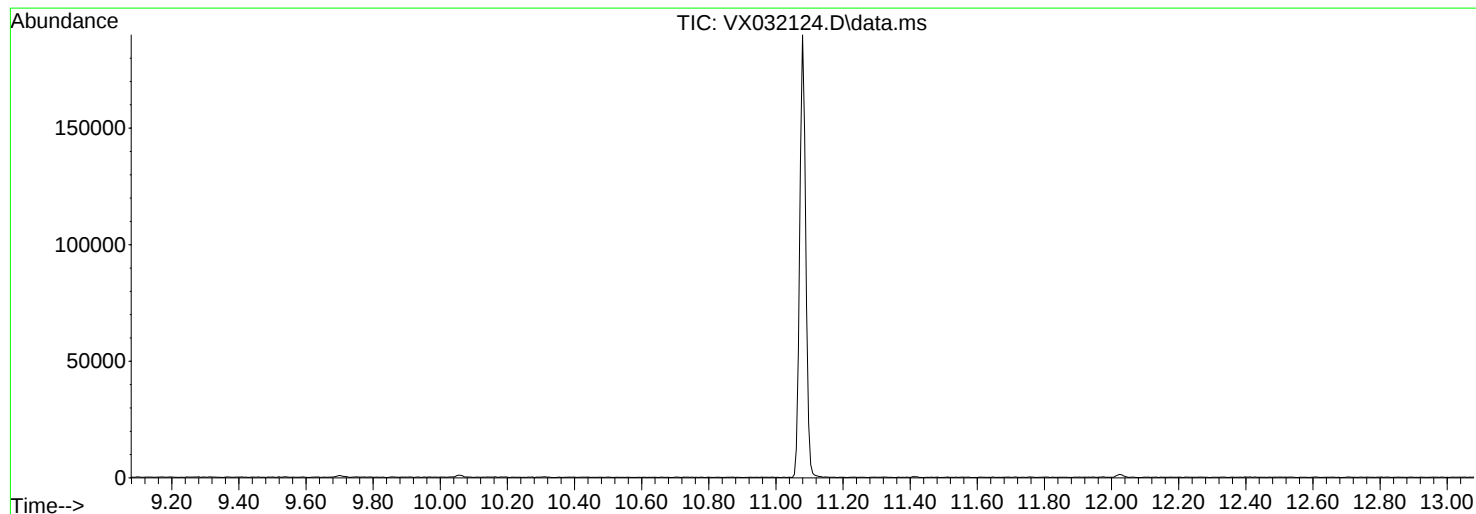

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	6063	PASS
75	95	30	60	51.1	16281	PASS
95	95	100	100	100.0	31891	PASS
96	95	5	9	7.1	2250	PASS
173	174	0.00	2	0.5	122	PASS
174	95	50	100	77.4	24680	PASS
175	174	5	9	7.7	1899	PASS
176	174	95	101	95.9	23669	PASS
177	176	5	9	7.0	1648	PASS