

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101424\
 Data File : VX043376.D
 Acq On : 14 Oct 2024 12:47
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
 Title : SW846 8260

Signal : TIC: VX043376.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.575	70	80	81	rBV4	4405	9560	2.04%	0.363%
2	1.617	81	87	89	rBV5	2490	5779	1.23%	0.219%
3	2.940	295	304	314	rBV	5406	12395	2.65%	0.471%
4	5.385	694	705	720	rBV	54161	160991	34.39%	6.114%
5	5.544	720	731	750	rVB2	86908	250960	53.61%	9.531%
6	5.952	788	798	815	rBV	65448	172777	36.91%	6.562%
7	6.757	920	930	948	rBV	144348	353026	75.42%	13.408%
8	8.647	1234	1240	1255	rBV	283319	468085	100.00%	17.778%
9	10.049	1465	1470	1481	rBV	279761	404643	86.45%	15.368%
10	11.079	1634	1639	1648	rBV	242269	316160	67.54%	12.008%
11	12.018	1788	1793	1801	rBV	298578	390061	83.33%	14.814%
12	15.420	2347	2351	2357	rVB6	7462	10693	2.28%	0.406%
13	15.743	2400	2404	2408	rVB4	7816	10591	2.26%	0.402%
14	16.091	2456	2461	2467	rBV2	23437	46841	10.01%	1.779%
15	16.279	2488	2492	2493	rBV3	5148	7586	1.62%	0.288%
16	16.706	2559	2562	2567	rVB7	5823	8080	1.73%	0.307%
17	16.767	2569	2572	2573	rBV3	4321	4777	1.02%	0.181%




Sum of corrected areas: 2633005

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101424\
Data File : VX043376.D
Acq On : 14 Oct 2024 12:47
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

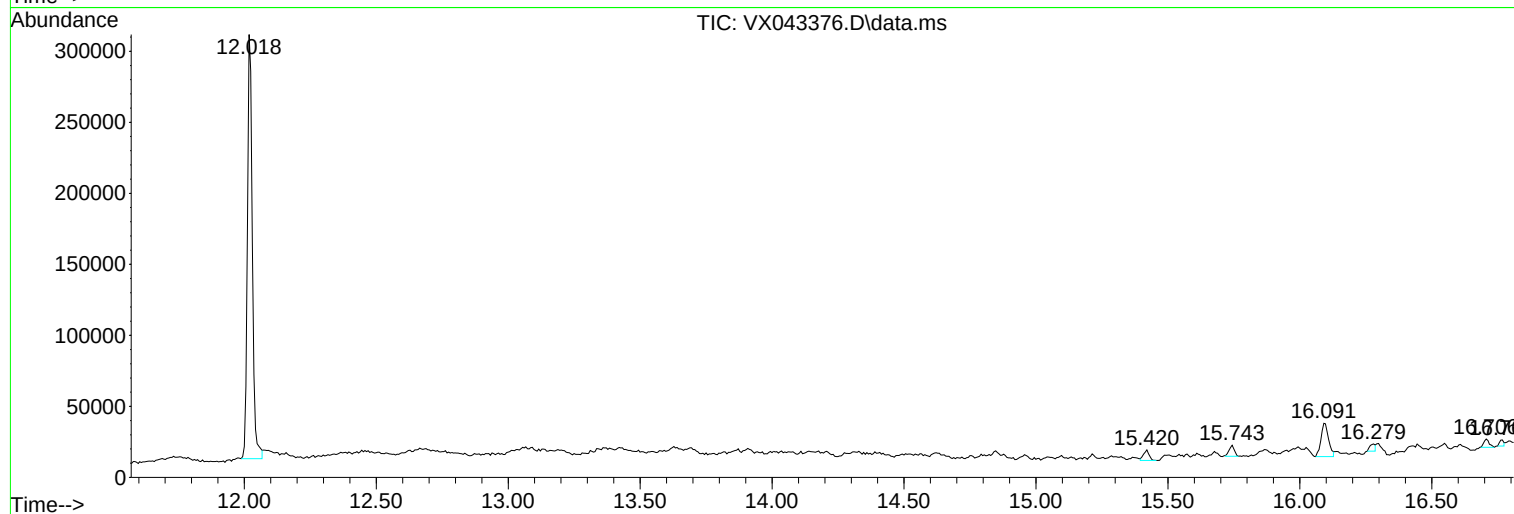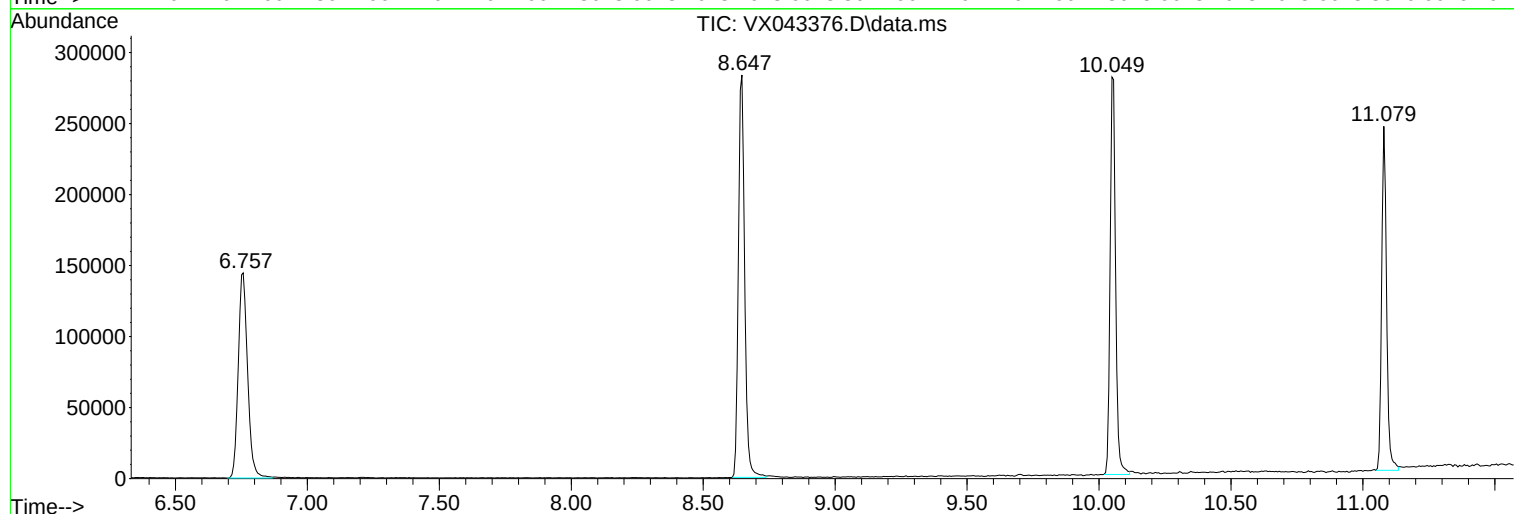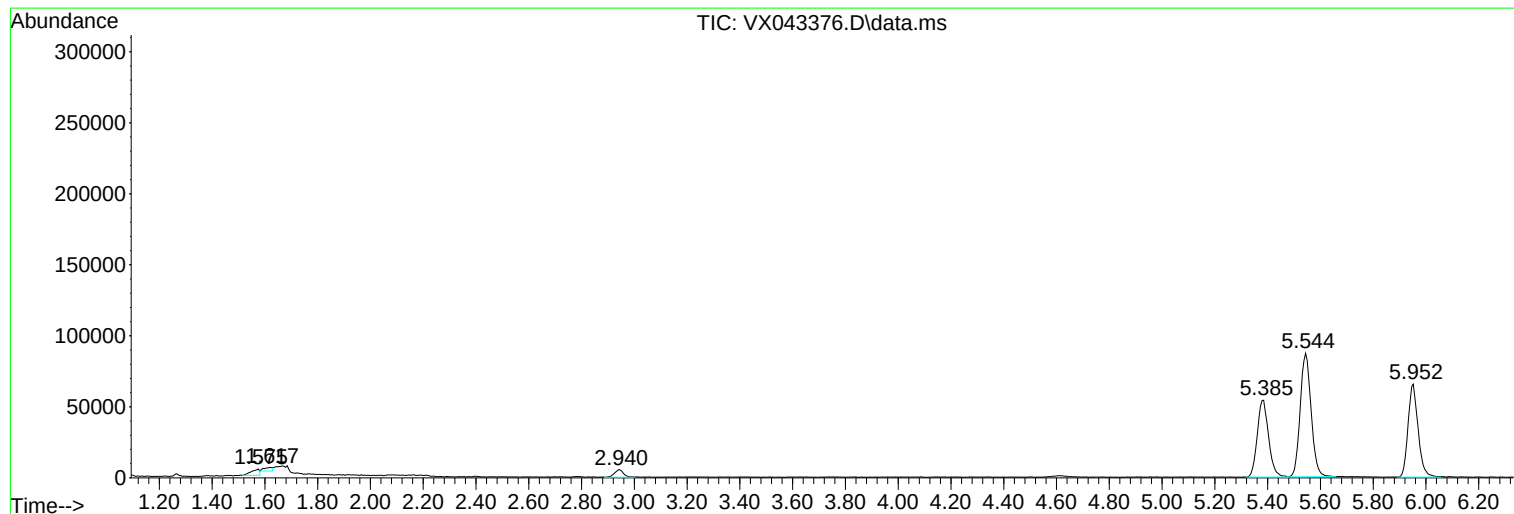

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101424\
Data File : VX043376.D
Acq On : 14 Oct 2024 12:47
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butylated Hydroxytoluene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.090	6.00 ug/l	46841	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butylated Hydroxytoluene	220	C15H24O	000128-37-0	91
2			Phenol, 2,4,6-tris(1-methylethyl)-	220	C15H24O	002934-07-8	70
3			Phenol, 4,6-di(1,1-dimethylethyl)-	220	C15H24O	000616-55-7	64
4			Phenol, 2,6-bis(1,1-dimethylethyl)-	277	C17H27NO2	001918-11-2	53
5			6-Methyl-1H,6H,7H-pyrrolo[2,3-c]-	220	C11H16N2OSi	1000504-47-6	52

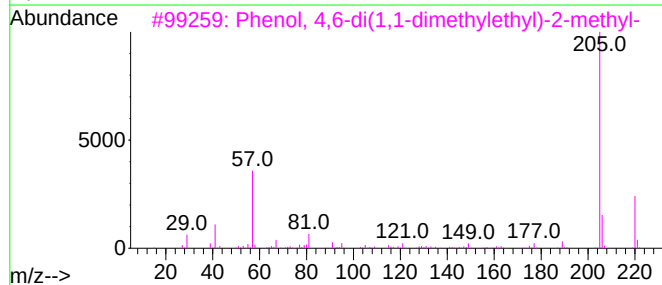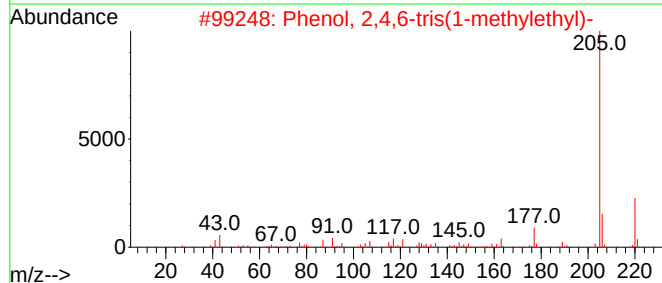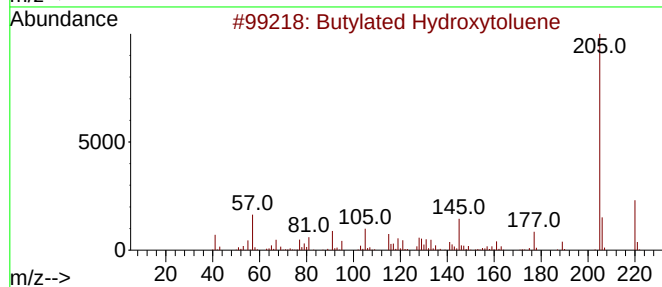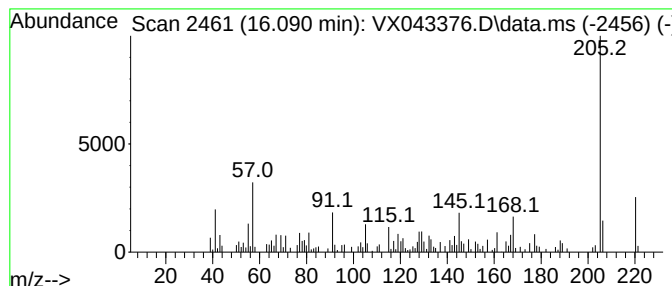

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101424\
Data File : VX043376.D
Acq On : 14 Oct 2024 12:47
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butylated Hydro...	16.090	6.0	ug/l	46841	4	12.024	390061	50.0