

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101425\
Data File : VX048170.D
Acq On : 14 Oct 2025 16:35
Operator : JC/MD
Sample : Q3345-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TANK-FARM-WATER

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M

Title : SW846 8260

Signal : TIC: VX048170.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.520	229	235	243	rBV	8639	17389	1.93%	0.348%
2	2.940	297	304	315	rVB3	4935	12156	1.35%	0.243%
3	4.544	559	567	580	rBV4	3239	13206	1.46%	0.264%
4	5.373	693	703	721	rBV2	92218	298844	33.10%	5.977%
5	5.543	721	731	754	rVB	127458	402185	44.55%	8.043%
6	5.940	787	796	816	rBV	101992	302598	33.52%	6.052%
7	6.751	918	929	950	rBV	247552	648268	71.80%	12.965%
8	8.634	1231	1238	1256	rBV	518591	851897	94.36%	17.037%
9	10.037	1463	1468	1486	rBV	623096	902449	99.96%	18.048%
10	11.067	1631	1637	1647	rBV	464994	648313	71.81%	12.966%
11	12.006	1785	1791	1801	rBV	685099	902831	100.00%	18.056%




Sum of corrected areas: 5000136

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101425\
Data File : VX048170.D
Acq On : 14 Oct 2025 16:35
Operator : JC/MD
Sample : Q3345-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TANK-FARM-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

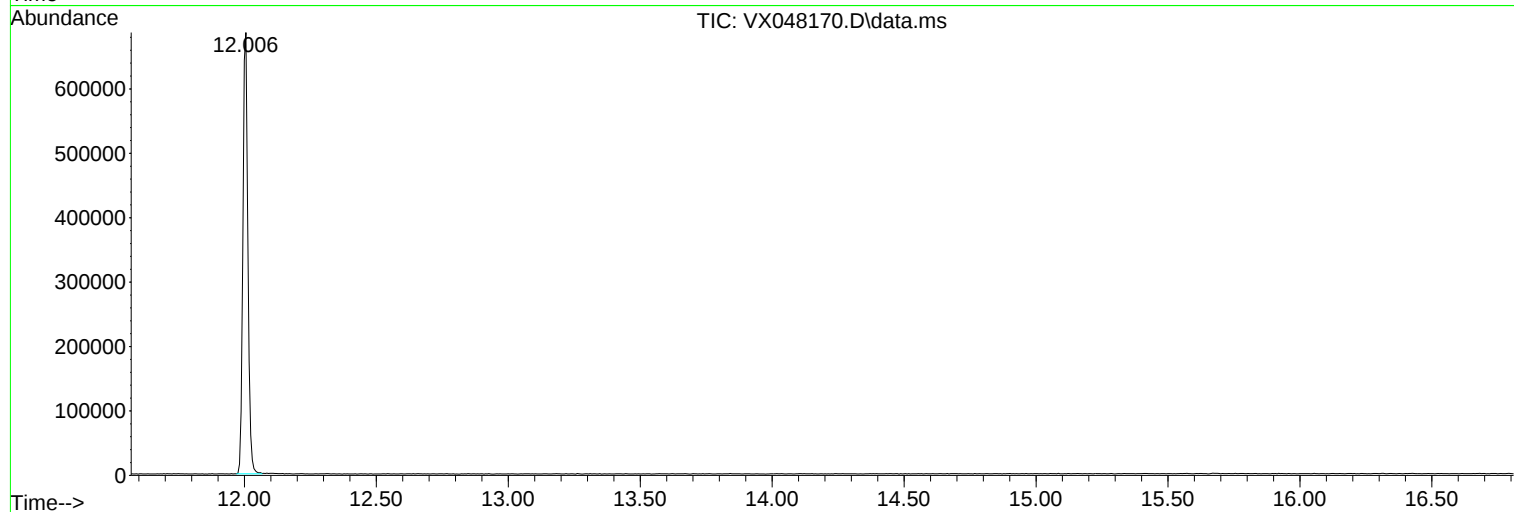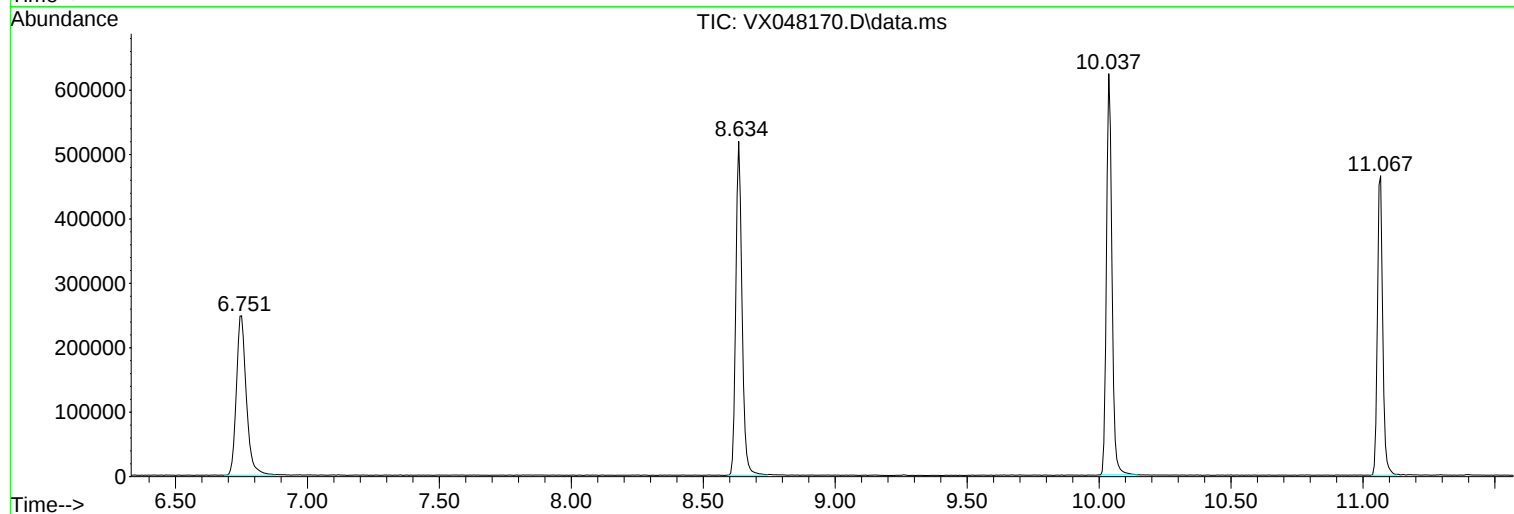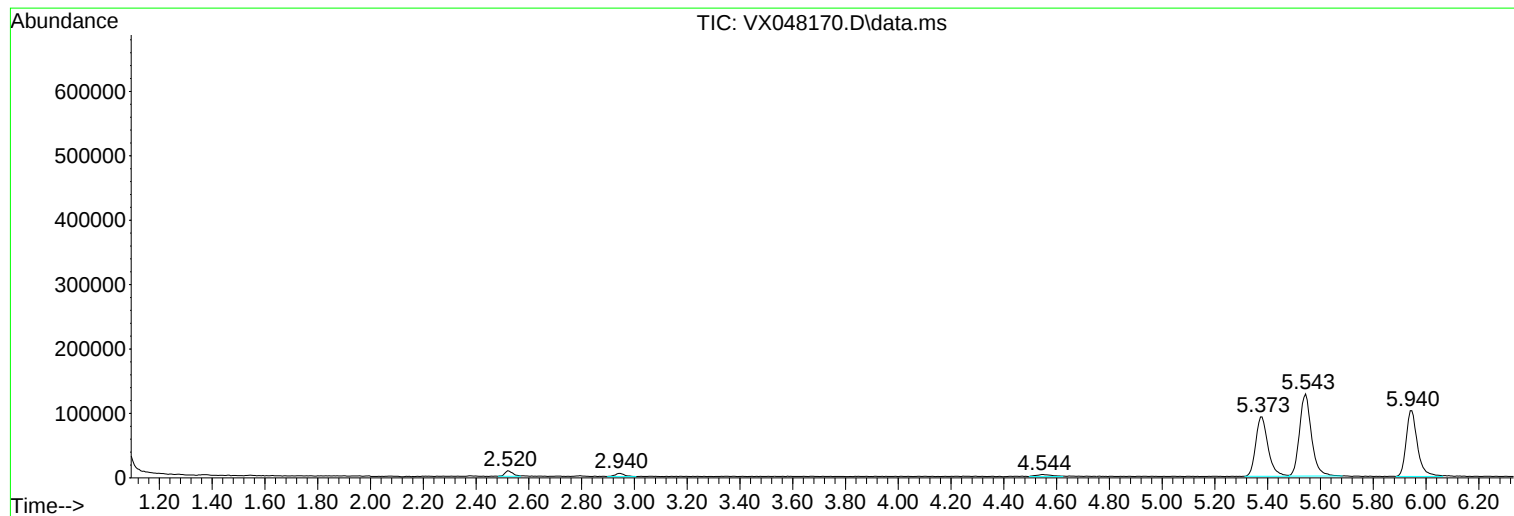

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101425\
Data File : VX048170.D
Acq On : 14 Oct 2025 16:35
Operator : JC/MD
Sample : Q3345-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TANK-FARM-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101425\
Data File : VX048170.D
Acq On : 14 Oct 2025 16:35
Operator : JC/MD
Sample : Q3345-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TANK-FARM-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc