
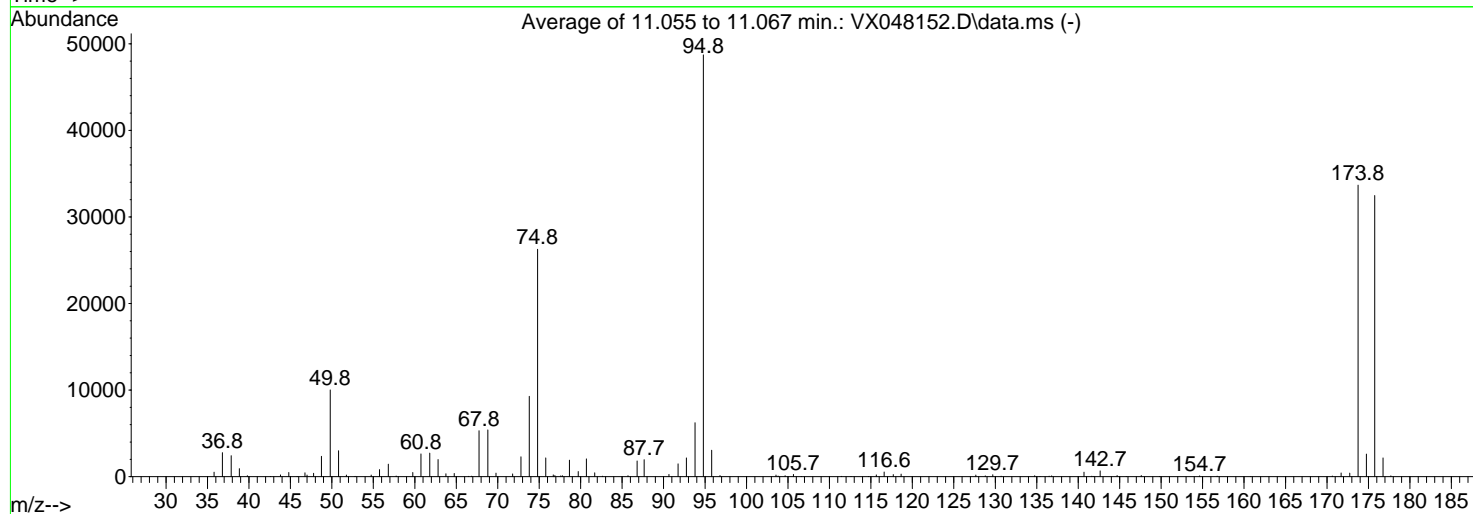


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX101425\  
 Data File : VX048152.D  
 Acq On : 14 Oct 2025 09:33  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091625W.M  
 Title : SW846 8260  
 Last Update : Wed Sep 17 06:39:58 2025

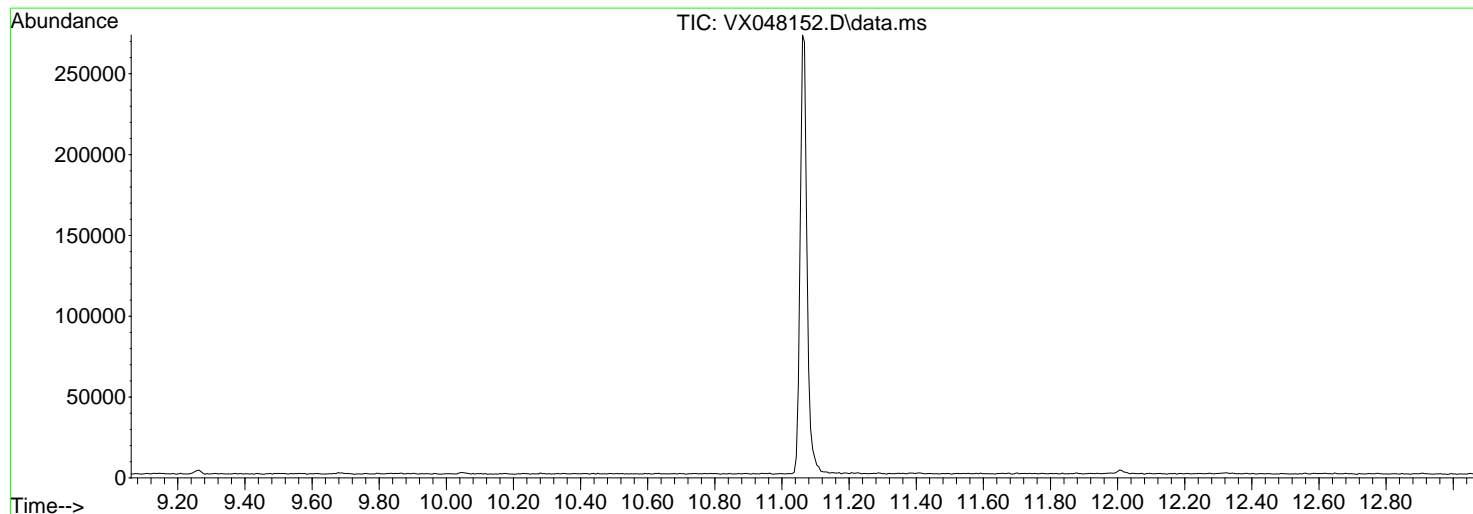

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result
50	95	15	40	20.6	10025	PASS
75	95	30	60	53.9	26259	PASS
95	95	100	100	100.0	48723	PASS
96	95	5	9	6.2	3044	PASS
173	174	0.00	2	1.2	399	PASS
174	95	50	100	69.1	33677	PASS
175	174	5	9	7.7	2598	PASS
176	174	95	101	96.5	32483	PASS
177	176	5	9	6.7	2171	PASS