

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX101518\
 Data File : VX005352.D
 Acq On : 15 Oct 2018 19:01
 Operator : JC/MD
 Sample : J5198-16
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampled :
 CL-02-101218-C

Quant Time: Oct 16 03:38:46 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X101218W.M
 Quant Title : SW846 8260
 QLast Update : Fri Oct 12 11:28:43 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	260147	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	392149	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	356351	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	168824	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	153884	53.30	ug/l	0.00
Spiked Amount				50.000		
Recovery						= 106.60%
35) Dibromofluoromethane	5.51	113	123139	47.41	ug/l	0.00
Spiked Amount				50.000		
Recovery						= 94.82%
50) Toluene-d8	8.71	98	461599	51.77	ug/l	0.00
Spiked Amount				50.000		
Recovery						= 103.54%
62) 4-Bromofluorobenzene	11.14	95	148045	44.20	ug/l	0.00
Spiked Amount				50.000		
Recovery						= 88.40%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Bromomethane	1.65	94	290	0.754	ug/l #	76
6) Chloroethane	1.70	64	48	0.359	ug/l #	44
11) Tert butyl alcohol	3.03	59	2155	2.646	ug/l #	72
13) Acrolein	2.29	56	59	Below Cal	#	1
14) Allyl chloride	2.85	41	36318	7.260	ug/l #	28
16) Acetone	2.45	43	19984	11.971	ug/l	99
18) Methyl Acetate	2.78	43	11086	2.334	ug/l	96
20) Methylene Chloride	2.85	84	831910	349.861	ug/l	96
25) 2-Butanone	4.71	43	2700	1.105	ug/l	98
29) Tetrahydrofuran	5.15	42	1387	0.890	ug/l #	40
30) Chloroform	5.21	83	1672	0.374	ug/l #	81
31) Cyclohexane	5.66	56	4717	1.188	ug/l #	1
36) 1,1-Dichloropropene	5.66	75	17039	4.486	ug/l #	50
38) Carbon Tetrachloride	5.66	117	23088	6.050	ug/l #	16
43) Isopropyl Acetate	6.46	43	155004	23.824	ug/l	97
44) Trichloroethene	7.21	130	121	Below Cal		4
47) Bromodichloromethane	7.90	83	868	0.254	ug/l #	75
48) Methyl methacrylate	7.68	41	6849	2.030	ug/l #	21
49) 1,4-Dioxane	7.88	88	29	0.373	ug/l #	1
51) 4-Methyl-2-Pentanone	8.62	43	2524	0.560	ug/l #	34
54) cis-1,3-Dichloropropene	8.62	75	1085	0.271	ug/l #	75
59) 2-Hexanone	9.54	43	8422	2.324	ug/l #	54
68) m/p-Xylenes	10.35	106	1882	0.393	ug/l	92
69) o-Xylene	10.70	106	1080	0.234	ug/l	95
76) 1,2,3-Trichloropropane	11.14	75	74074	22.620	ug/l #	37
80) 1,3,5-Trimethylbenzene	11.51	105	3081	0.358	ug/l	94
81) trans-1,4-Dichloro-2-buten	11.14	75	74074	68.731	ug/l #	10
84) 1,2,4-Trimethylbenzene	11.81	105	8232	0.931	ug/l	95
95) Naphthalene	13.83	128	321211	27.589	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX101518\
 Data File : VX005352.D
 Acq On : 15 Oct 2018 19:01
 Operator : JC/MD
 Sample : J5198-16
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 Client Sampled :
 CL-02-101218-C

Quant Time: Oct 16 03:38:46 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X101218W.M
 Quant Title : SW846 8260
 QLast Update : Fri Oct 12 11:28:43 2018
 Response via : Initial Calibration




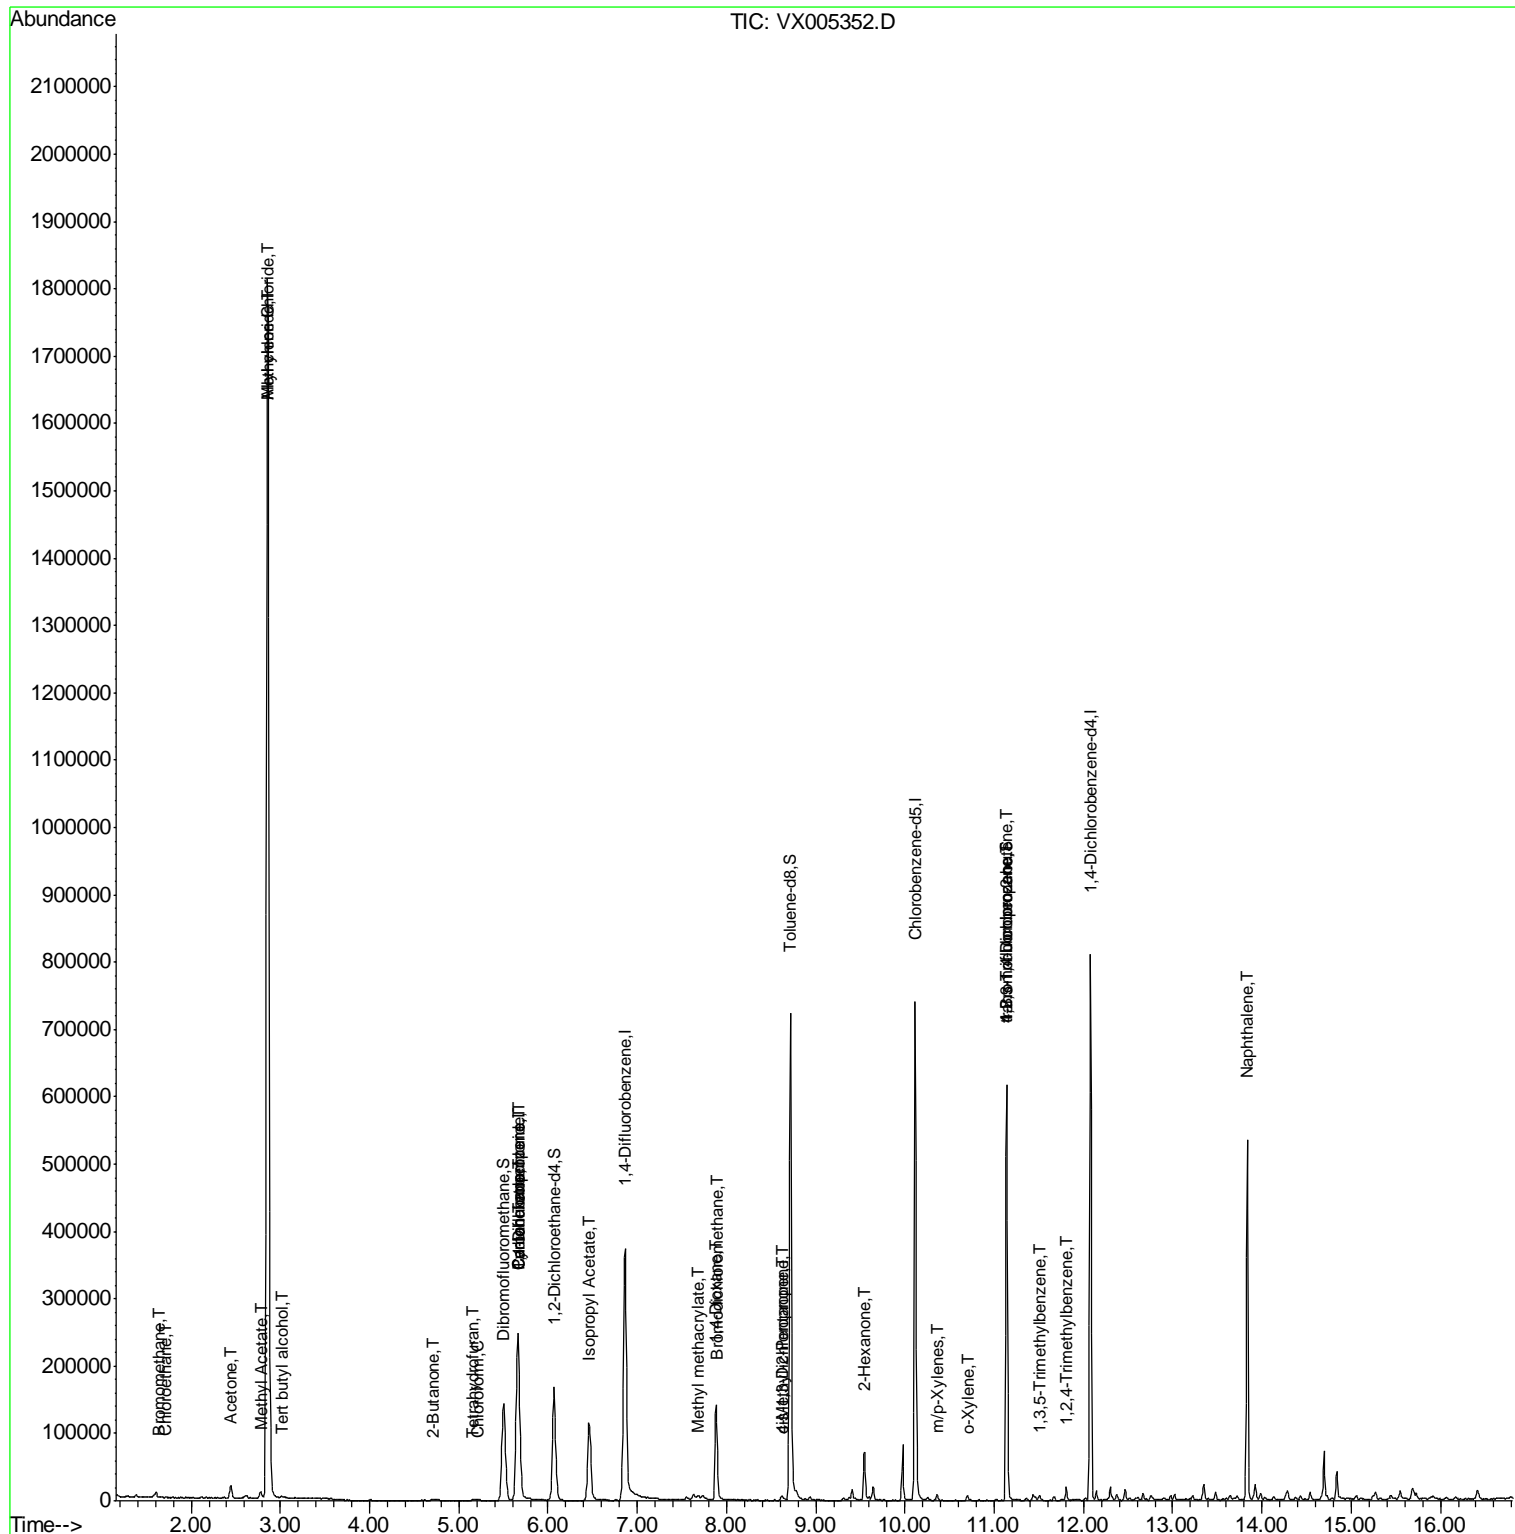




#1
 Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 5.67 min Scan# 740
 Delta R.T. 0.00 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01




Instrument :
 MSVOA_X
 ClientSampleId :
 CL-02-101218-C


Tgt Ion: 168 Resp: 260147
 Ion Ratio Lower Upper
 168 100
 99 49.2 39.9 59.9

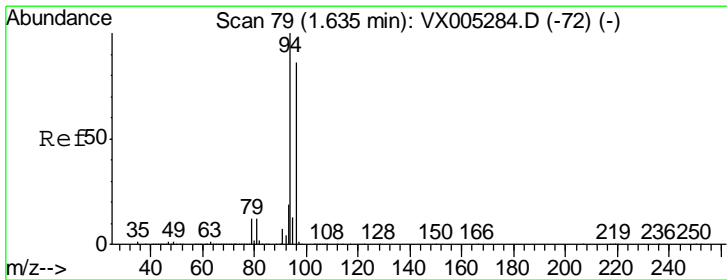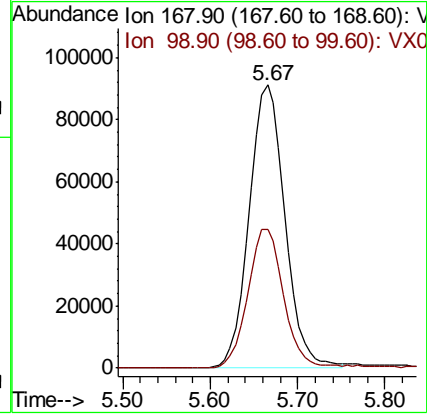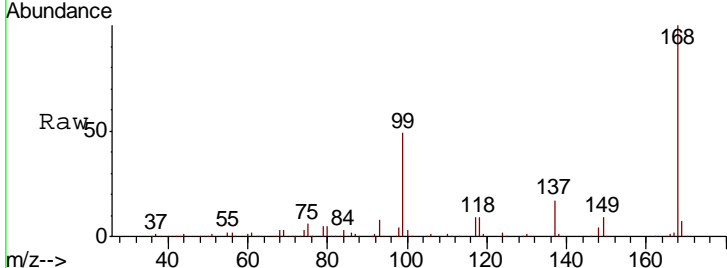

#5
 Bromomethane
 Concen: 0.754 ug/l
 RT: 1.65 min Scan# 82
 Delta R.T. 0.02 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01

Tgt Ion: 94 Resp: 290
 Ion Ratio Lower Upper
 94 100
 96 69.9 74.5 111.7#

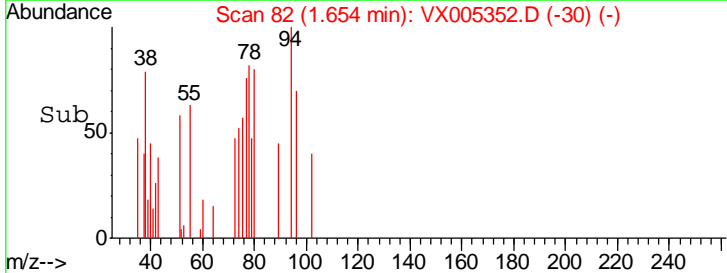
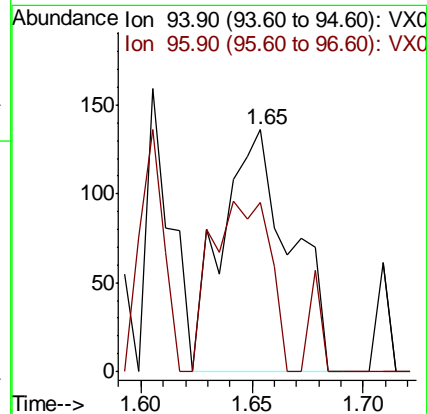





#6
 Chloroethane
 Concen: 0.359 ug/l
 RT: 1.70 min Scan# 90
 Delta R.T. -0.01 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01





Instrument : MSVOA_X
 ClientSampled : CL-02-101218-C


Tgt Ion	Resp	Lower	Upper
64	100		
66	0.0	24.6	36.8#

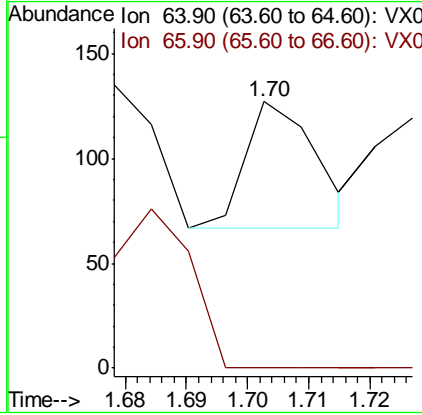

#11
 Tert butyl alcohol
 Concen: 2.646 ug/l
 RT: 3.03 min Scan# 307
 Delta R.T. -0.05 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01

Tgt Ion	Resp	Lower	Upper
59	100		
57	0.0	8.2	12.4#


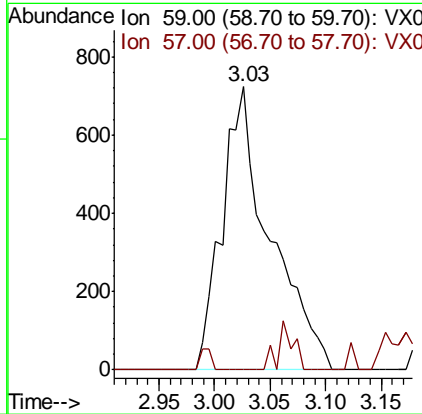





#13
 Acrolein
 Concen: Below Cal
 RT: 2.29 min Scan# 187
 Delta R.T. 0.00 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01





Instrument : MSVOA_X
 ClientSampled : CL-02-101218-C


Tgt Ion	Resp	Lower	Upper
56	100		
55	167.8	54.7	82.1#

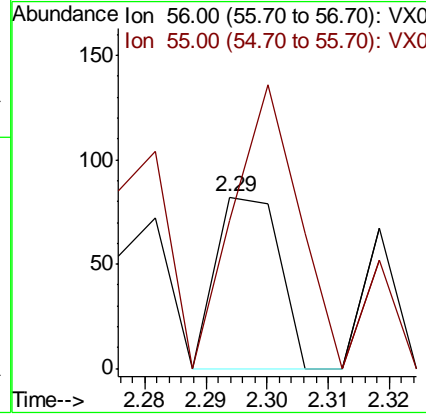

#14
 Allyl chloride
 Concen: 7.260 ug/l
 RT: 2.85 min Scan# 279
 Delta R.T. 0.13 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01

Tgt Ion	Resp	Lower	Upper
41	100		
39	0.7	48.9	73.3#
76	0.0	26.7	40.1#



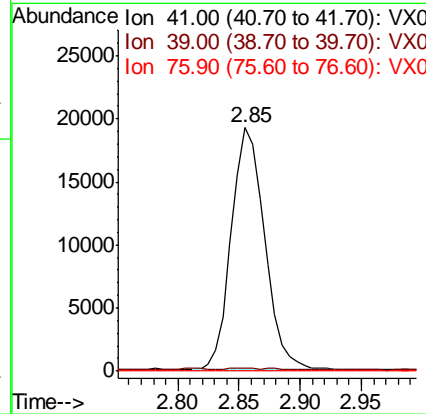



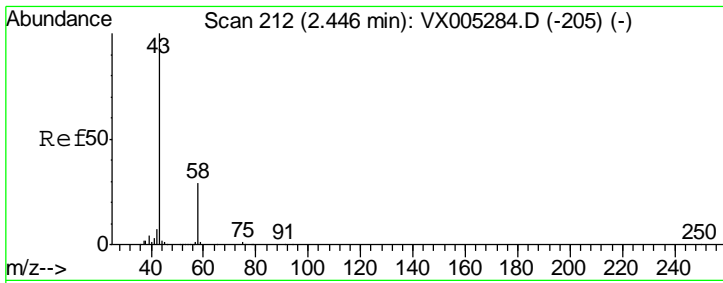

#16
 Acetone
 Concen: 11.971 ug/l
 RT: 2.45 min Scan# 212
 Delta R.T. 0.00 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01




Instrument :
 MSVOA_X
 ClientSampled :
 CL-02-101218-C


Tgt Ion	Resp	Lower	Upper
43	19984		
58	33.3	26.2	39.4

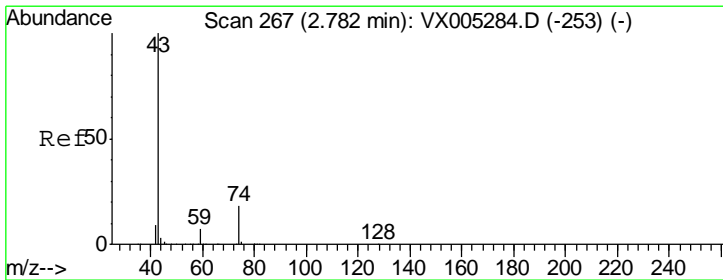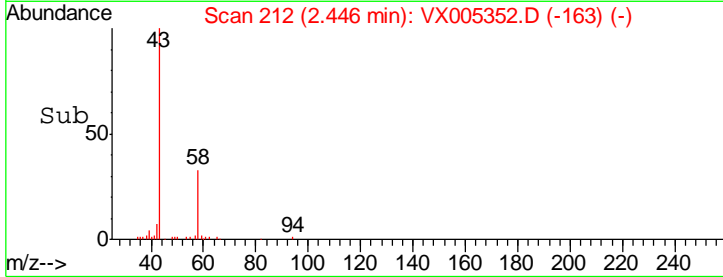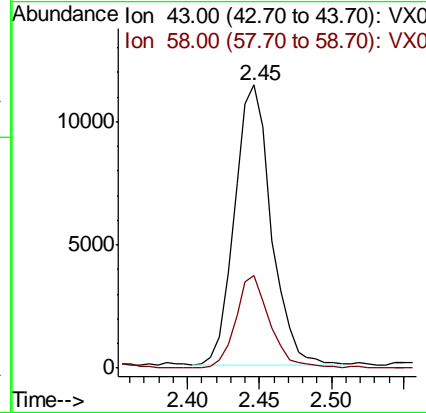

#18
 Methyl Acetate
 Concen: 2.334 ug/l
 RT: 2.78 min Scan# 267
 Delta R.T. 0.00 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01

Tgt Ion	Resp	Lower	Upper
43	11086		
74	22.5	19.4	29.2

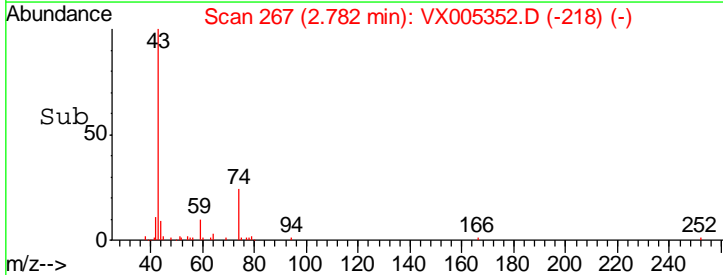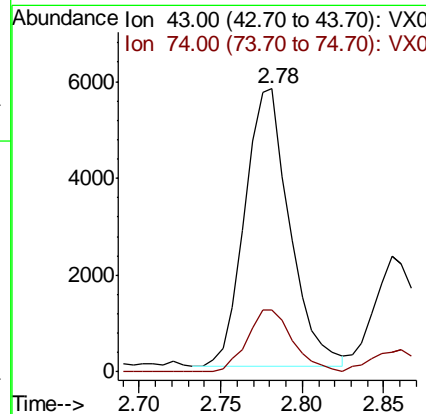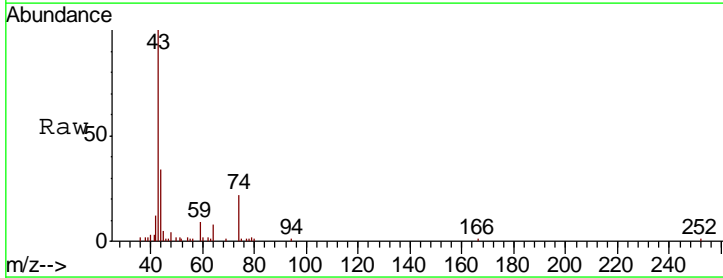







#20
Methylene Chloride
Concen: 349.861 ug/l
RT: 2.85 min Scan# 279
Delta R.T. 0.00 min
Lab File: VX005352.D
Acq: 15 Oct 2018 19:01

Instrument :
MSVOA_X
ClientSampled :
CL-02-101218-C

Tgt Ion: 84 Resp: 831910




Ion	Ratio	Lower	Upper
84	100		
49	132.4	101.2	151.8
51	40.4	29.5	44.3
86	64.1	52.3	78.5

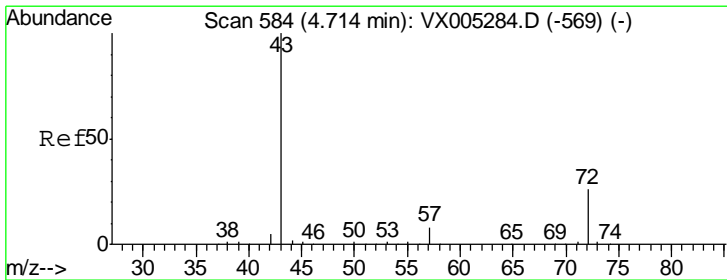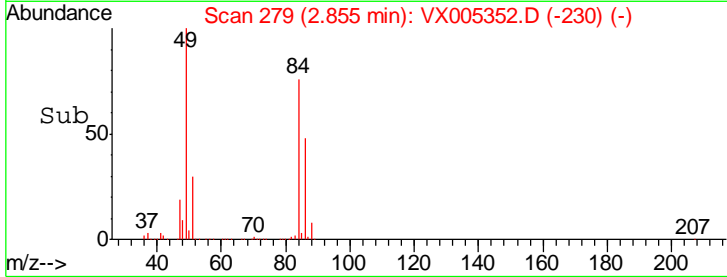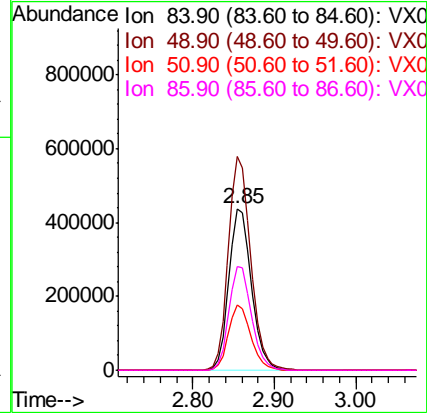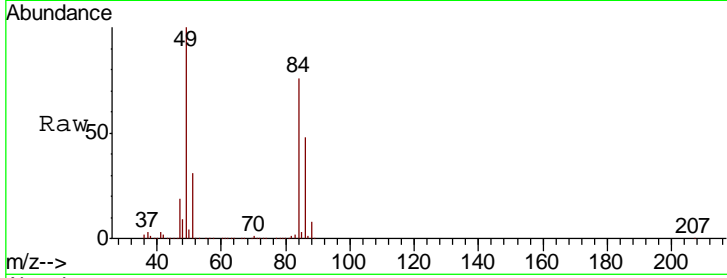


#25
2-Butanone
Concen: 1.105 ug/l
RT: 4.71 min Scan# 583
Delta R.T. -0.01 min
Lab File: VX005352.D
Acq: 15 Oct 2018 19:01

Tgt Ion: 43 Resp: 2700

Ion	Ratio	Lower	Upper
43	100		
72	26.2	22.0	33.0



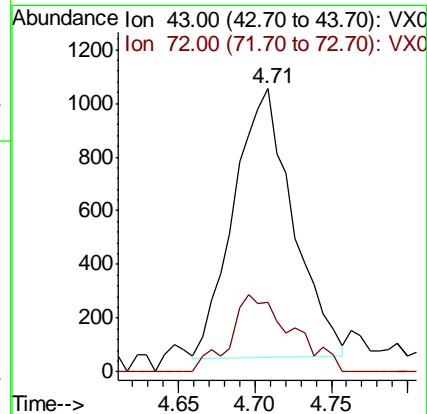
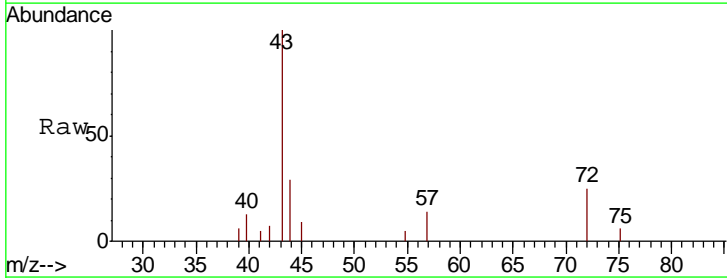


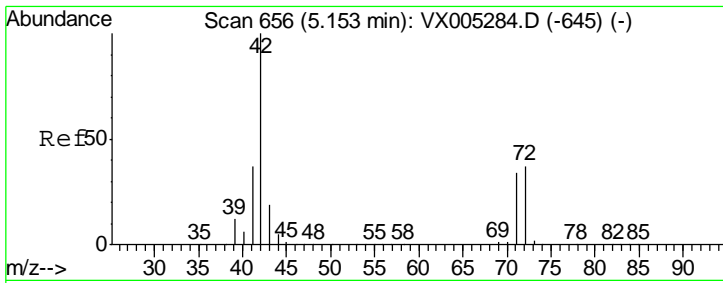

#29
 Tetrahydrofuran
 Concen: 0.890 ug/l
 RT: 5.15 min Scan# 656
 Delta R.T. 0.00 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01




Instrument :
 MSVOA_X
 ClientSampled :
 CL-02-101218-C


Tgt Ion	Resp	Lower	Upper
42	1387		
72	11.8	37.4	56.0#
71	0.0	34.5	51.7#

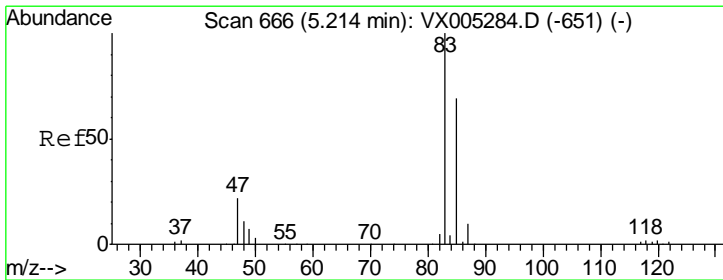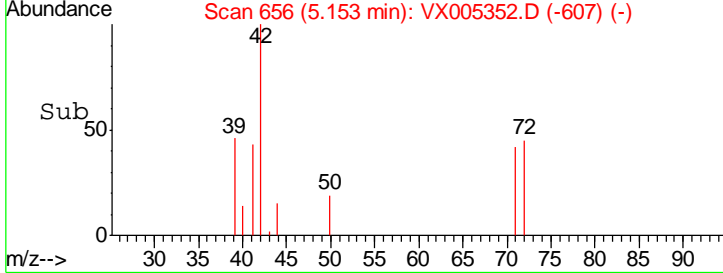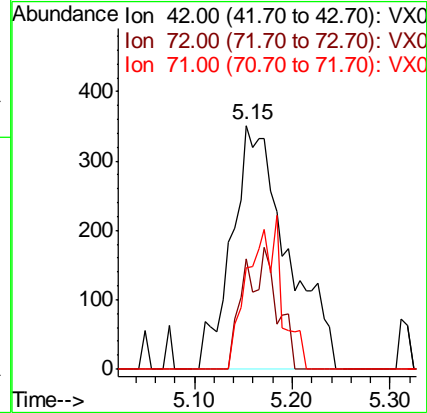

#30
 Chloroform
 Concen: 0.374 ug/l
 RT: 5.21 min Scan# 666
 Delta R.T. 0.00 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01

Tgt Ion	Resp	Lower	Upper
83	1672		
85	80.8	52.6	79.0#


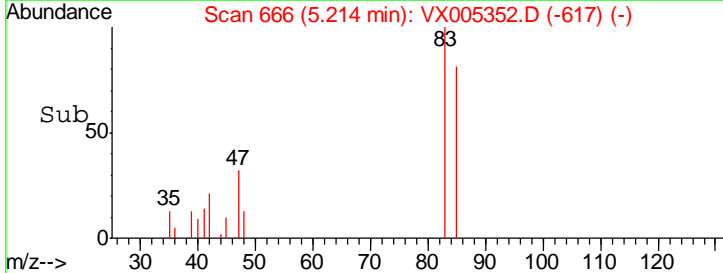
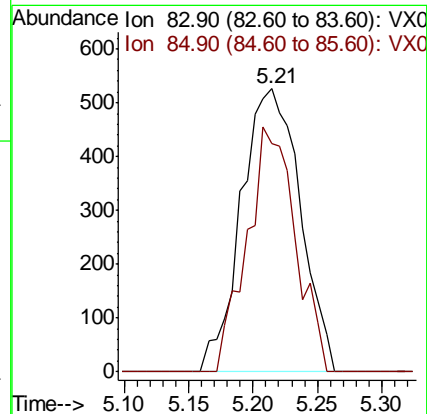



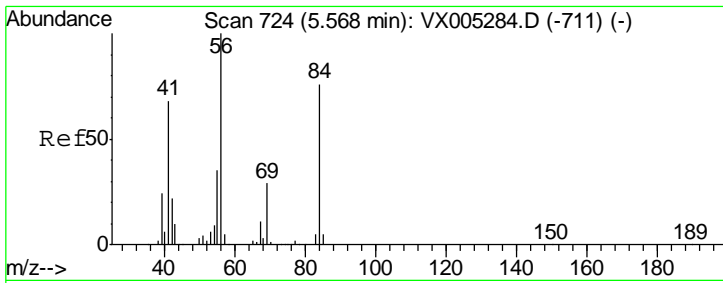

#31
 Cyclohexane
 Concen: 1.188 ug/l
 RT: 5.66 min Scan# 739
 Delta R.T. 0.09 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01




Instrument :
 MSVOA_X
 ClientSampled :
 CL-02-101218-C


Tgt Ion	Resp	Lower	Upper
56	4717		
69	190.3	25.4	38.2#
84	138.9	71.4	107.2#

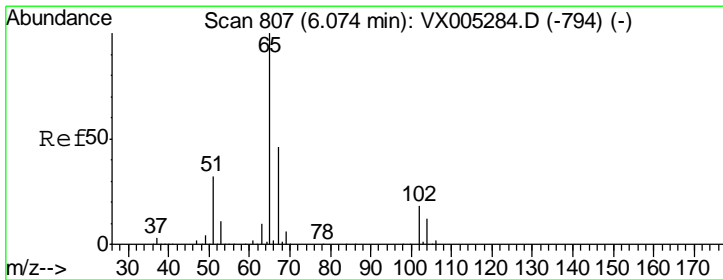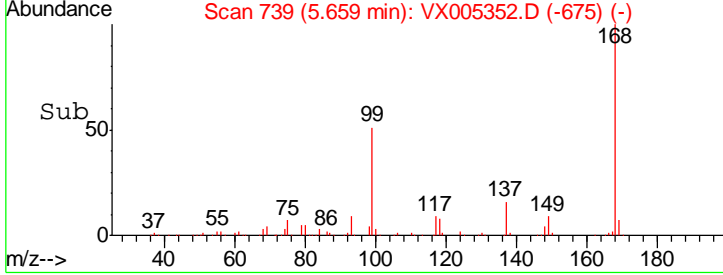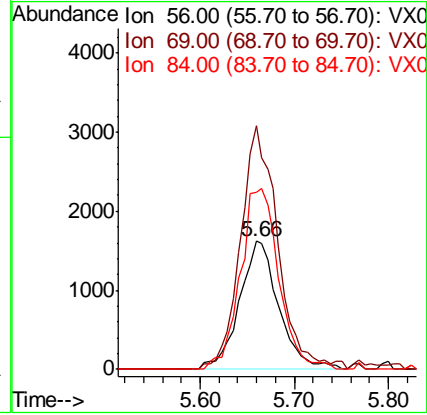

#33
 1,2-Dichloroethane-d4
 Concen: 53.298 ug/l
 RT: 6.07 min Scan# 806
 Delta R.T. -0.01 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01

Tgt Ion	Resp	Lower	Upper
65	153884		
67	53.2	0.0	106.8


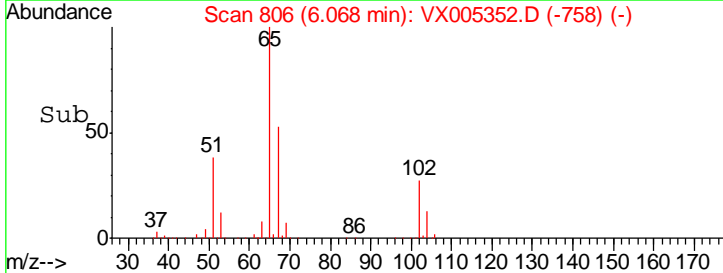
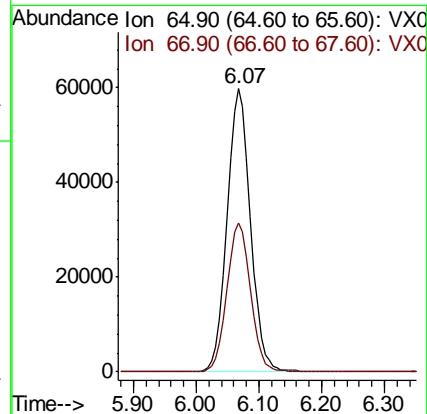





#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.87 min Scan# 937
 Delta R.T. 0.00 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01




Instrument :
 MSVOA_X
 ClientSampleId :
 CL-02-101218-C


Tgt Ion	Resp	Lower	Upper
114	392149		
63	16.9	0.0	39.0
88	13.1	0.0	30.4

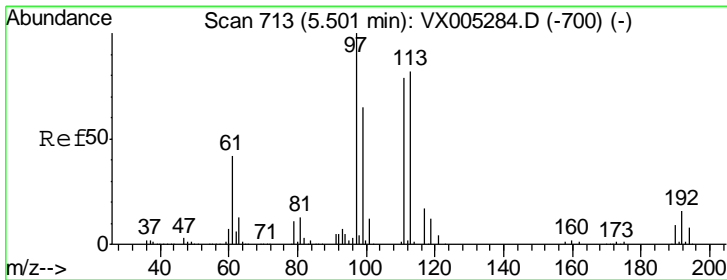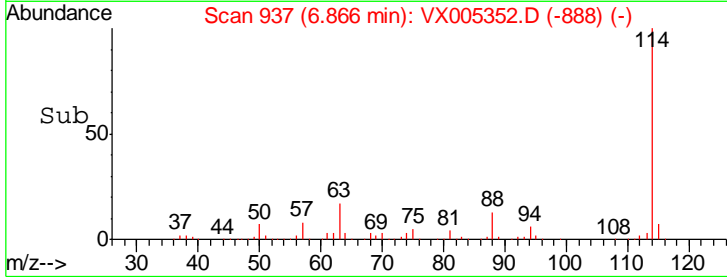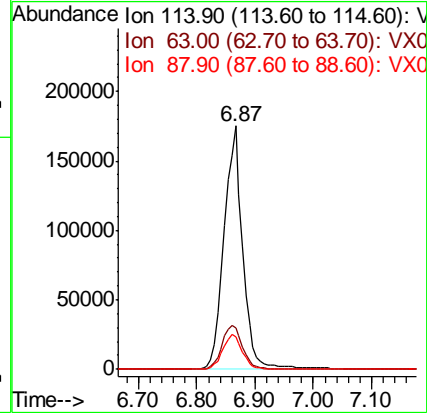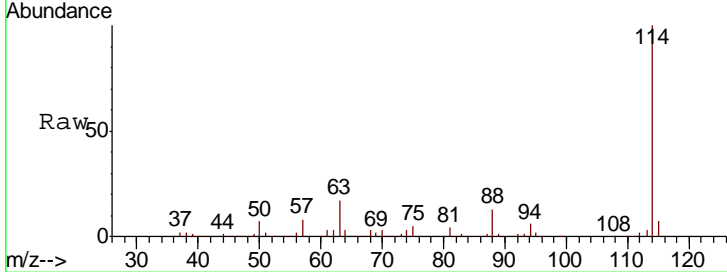

#35
 Dibromofluoromethane
 Concen: 47.410 ug/l
 RT: 5.51 min Scan# 714
 Delta R.T. 0.01 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01

Tgt Ion	Resp	Lower	Upper
113	123139		
111	102.2	82.4	123.6
192	24.1	19.4	29.2



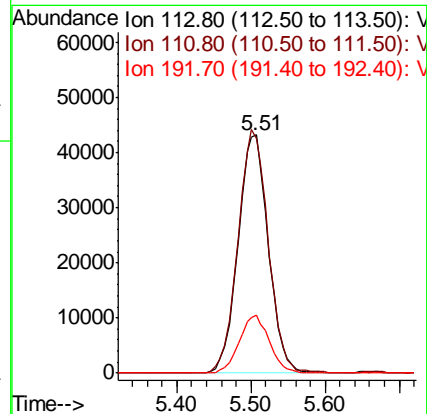
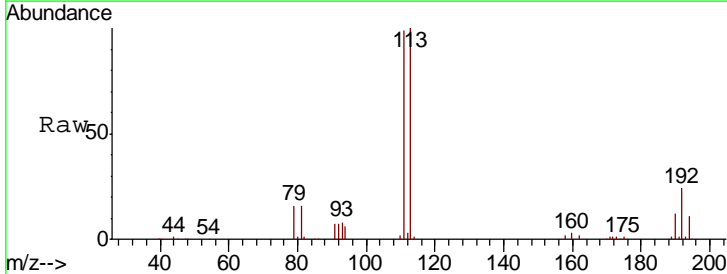


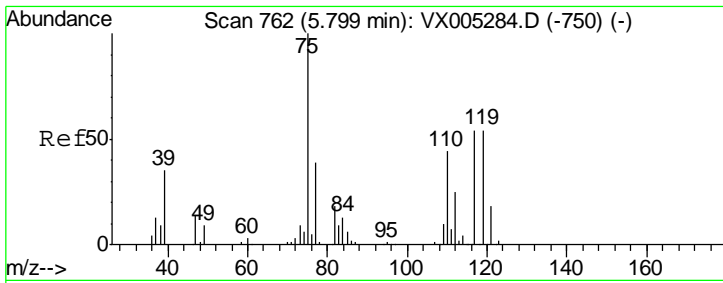

#36
 1,1-Dichloropropene
 Concen: 4.486 ug/l
 RT: 5.66 min Scan# 739
 Delta R.T. -0.14 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01




Instrument :
 MSVOA_X
 ClientSampled :
 CL-02-101218-C


Tgt Ion	Resp	Lower	Upper
75	17039		
110	9.2	18.0	54.0#
77	0.0	24.6	36.8#

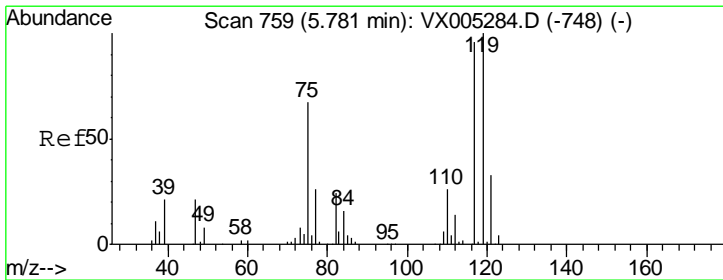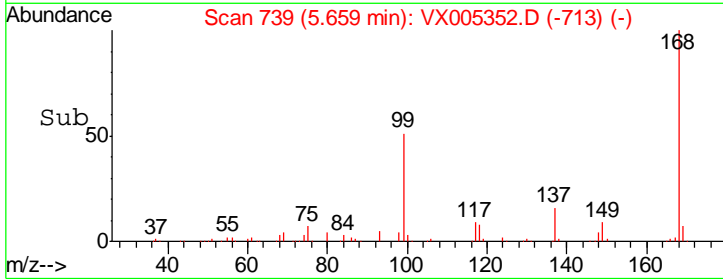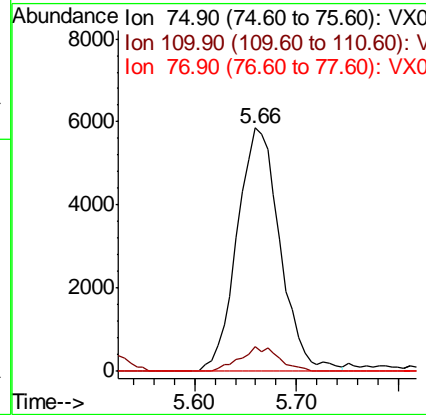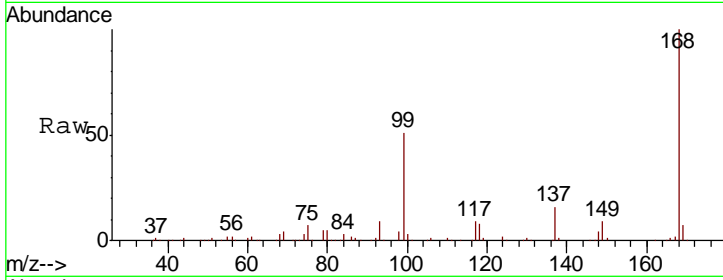

#38
 Carbon Tetrachloride
 Concen: 6.050 ug/l
 RT: 5.66 min Scan# 739
 Delta R.T. -0.12 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01

Tgt Ion	Resp	Lower	Upper
117	23088		
119	6.5	78.8	118.2#
121	0.0	24.9	37.3#


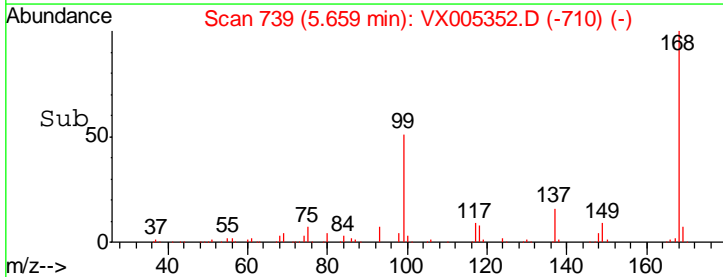
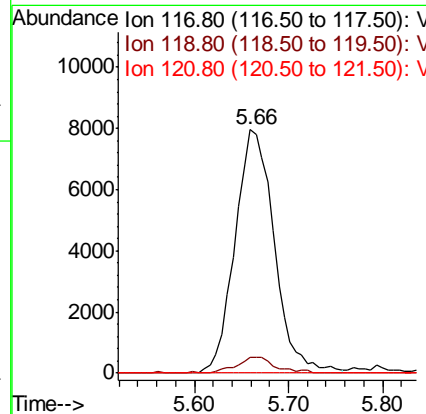
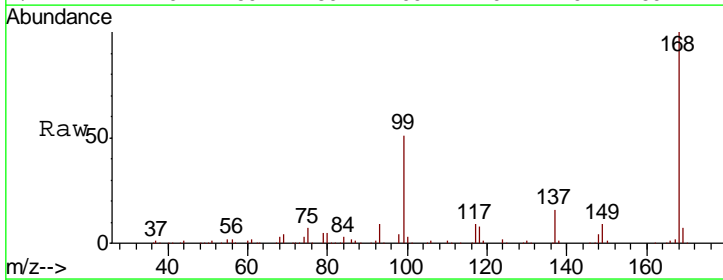




#43
 Isopropyl Acetate
 Concen: 23.824 ug/l
 RT: 6.46 min Scan# 870
 Delta R.T. -0.01 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01




Instrument :
 MSVOA_X
 ClientSampled :
 CL-02-101218-C


Tgt Ion	Resp	Lower	Upper
43	155004		
61	20.2	17.0	25.4
87	12.9	11.4	17.2

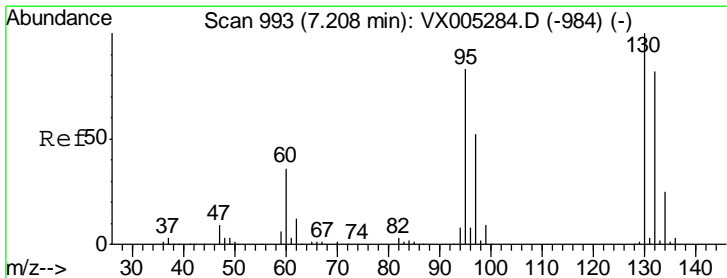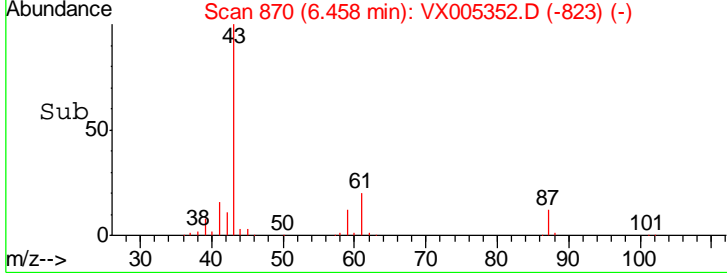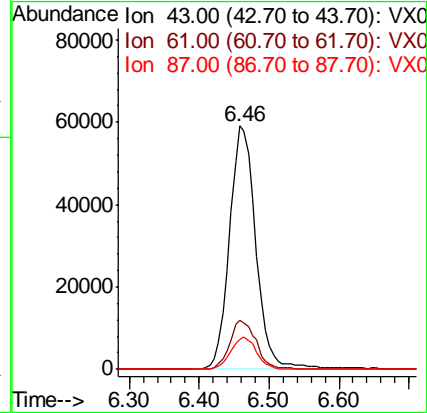

#44
 Trichloroethene
 Concen: Below Cal
 RT: 7.21 min Scan# 993
 Delta R.T. 0.00 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01

Tgt Ion	Resp	Lower	Upper
130	121		
95	0.0	0.0	181.6


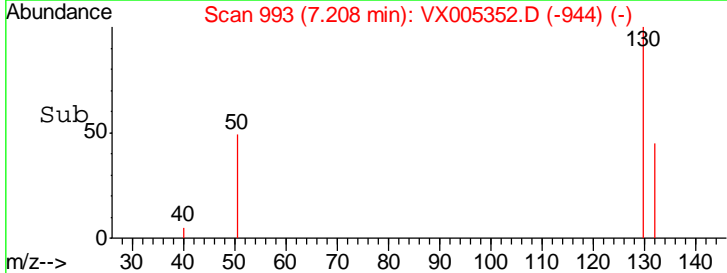
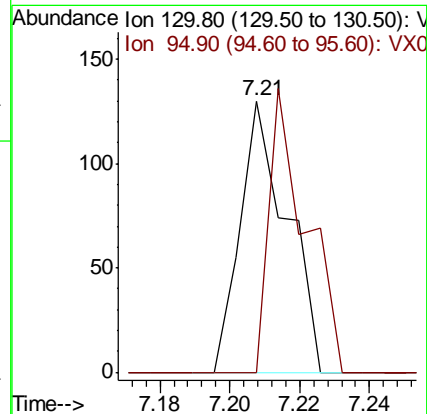
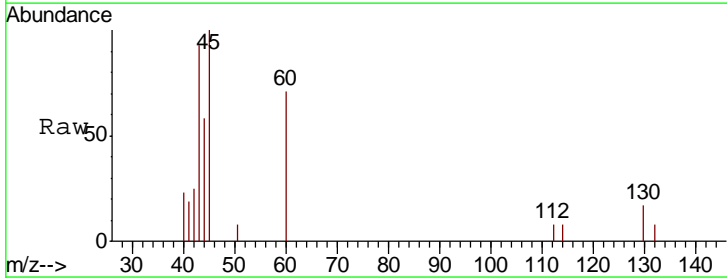


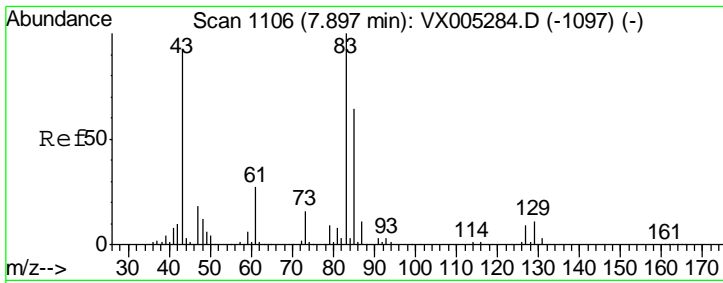

#47
 Bromodichloromethane
 Concen: 0.254 ug/l
 RT: 7.90 min Scan# 1106
 Delta R.T. 0.00 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01




Instrument : MSVOA_X
 ClientSampled : CL-02-101218-C


Tgt Ion	Resp	Lower	Upper
83	100		
85	44.2	50.9	76.3#
127	0.0	7.3	10.9#

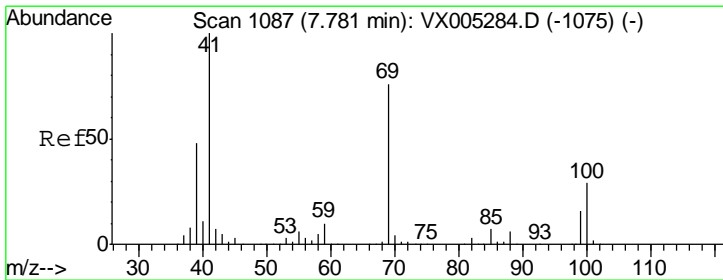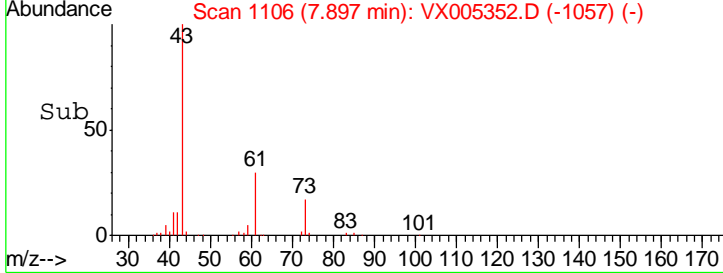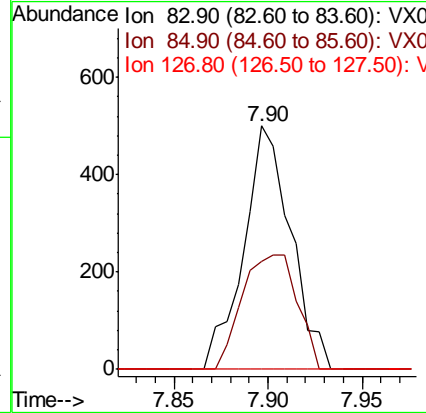

#48
 Methyl methacrylate
 Concen: 2.030 ug/l
 RT: 7.68 min Scan# 1071
 Delta R.T. -0.10 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01

Tgt Ion	Resp	Lower	Upper
41	100		
69	0.0	70.2	105.4#
39	15.5	42.7	64.1#


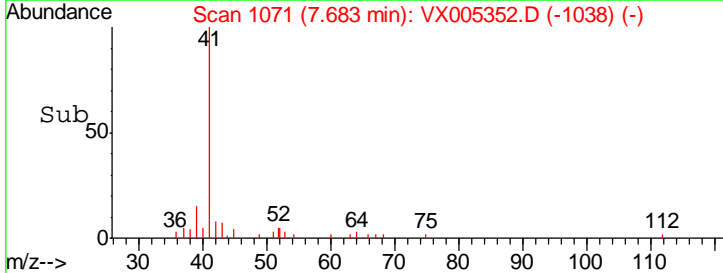
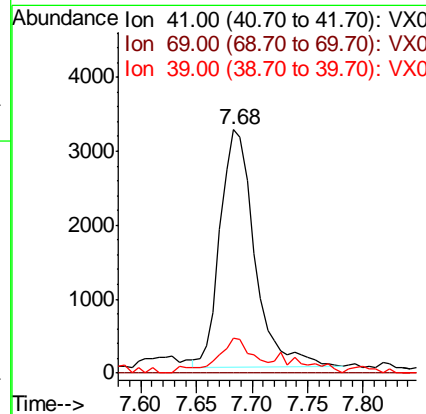



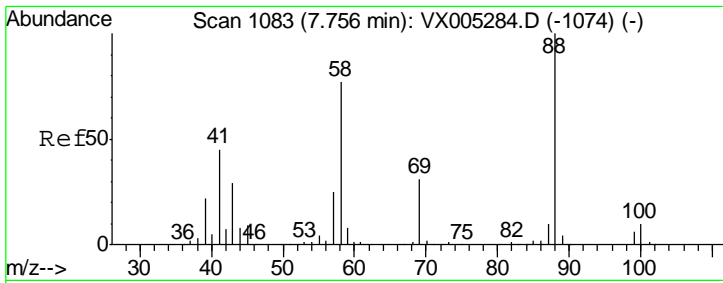

#49
 1,4-Dioxane
 Concen: 0.373 ug/l
 RT: 7.88 min Scan# 1103
 Delta R.T. 0.12 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01




Instrument : MSVOA_X
 ClientSampled : CL-02-101218-C


Tgt Ion	Resp	Lower	Upper
88	100		
43	454262.1	24.7	37.1#
58	4555.2	55.3	82.9#

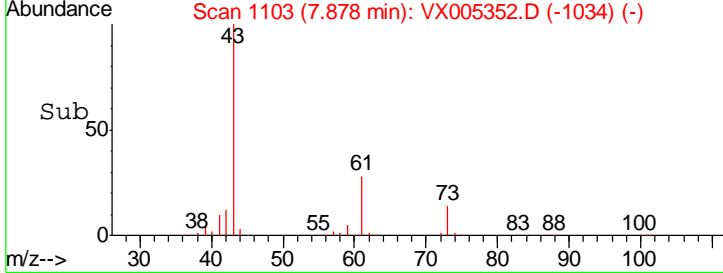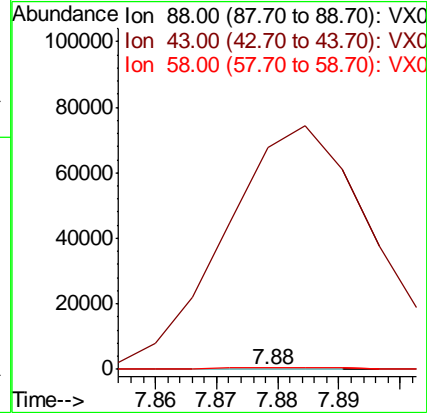

#50
 Toluene-d8
 Concen: 51.768 ug/l
 RT: 8.71 min Scan# 1240
 Delta R.T. 0.00 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01

Tgt Ion	Resp	Lower	Upper
98	100		
100	64.0	52.9	79.3


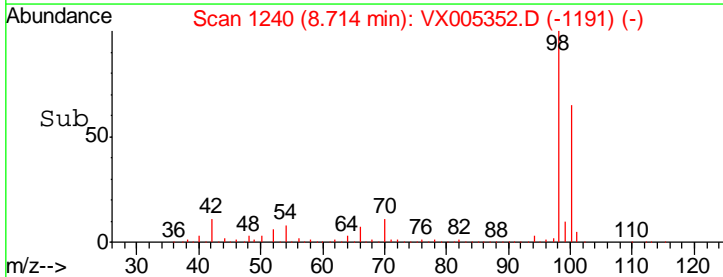
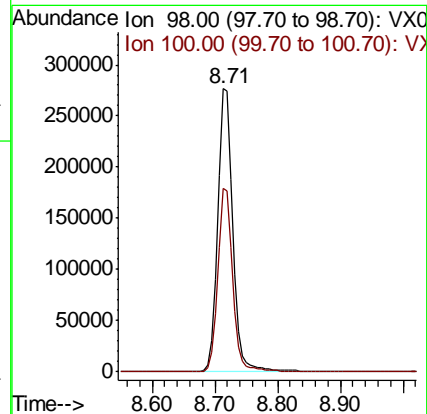





#51
 4-Methyl-2-Pentanone
 Concen: 0.560 ug/l
 RT: 8.62 min Scan# 1225
 Delta R.T. -0.03 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01




Instrument : MSVOA_X
 ClientSampled : CL-02-101218-C


Tgt Ion	Resp	Lower	Upper
43	100		
58	0.0	33.1	49.7#

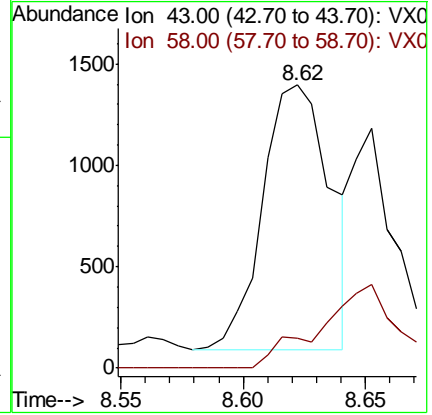

#54
 cis-1,3-Dichloropropene
 Concen: 0.271 ug/l
 RT: 8.62 min Scan# 1225
 Delta R.T. 0.18 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01

Tgt Ion	Resp	Lower	Upper
75	100		
77	0.0	26.2	39.2#
39	44.8	36.4	54.6


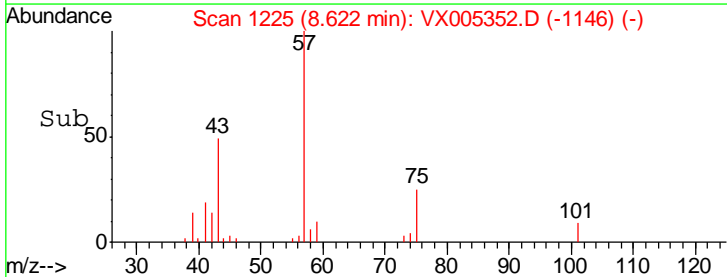
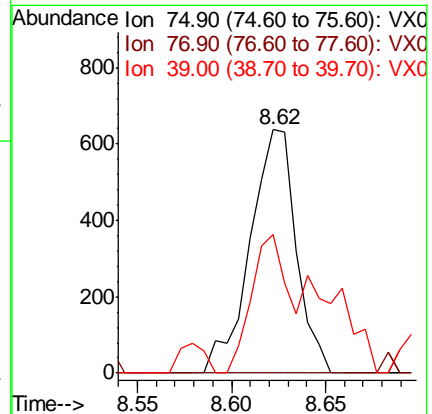





#59
 2-Hexanone
 Concen: 2.324 ug/l
 RT: 9.54 min Scan# 1376
 Delta R.T. 0.04 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01




Instrument :
 MSVOA_X
ClientSampled :
 CL-02-101218-C


Tgt Ion: 43 Resp: 8422
 Ion Ratio Lower Upper
 43 100
 58 24.2 29.0 87.0#

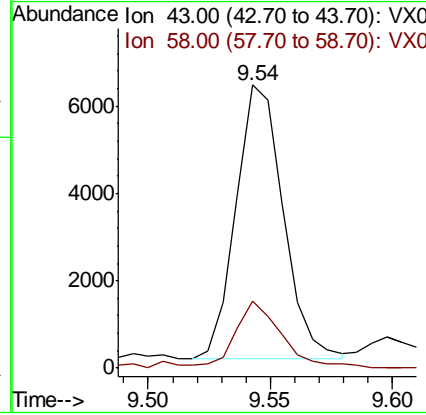

#62
 4-Bromofluorobenzene
 Concen: 44.197 ug/l
 RT: 11.14 min Scan# 1638
 Delta R.T. 0.00 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01

Tgt Ion: 95 Resp: 148045
 Ion Ratio Lower Upper
 95 100
 174 98.1 0.0 185.2
 176 94.2 0.0 178.6


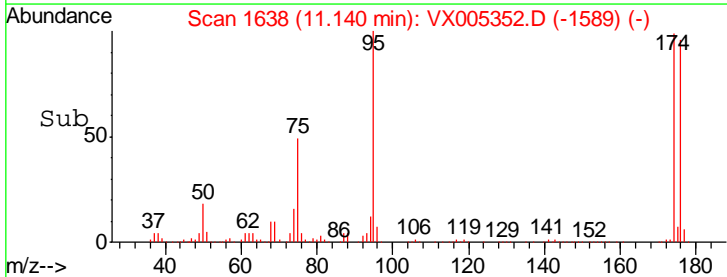
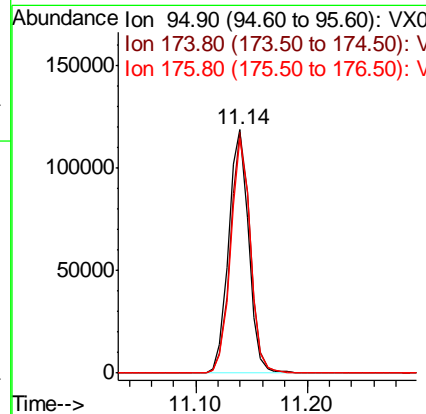





#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 10.12 min Scan# 1470
 Delta R.T. 0.00 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01




Instrument :
 MSVOA_X
 ClientSampled :
 CL-02-101218-C


Tgt Ion	Resp	Lower	Upper
117	356351		
82	52.1	47.8	71.6
119	32.3	29.3	43.9

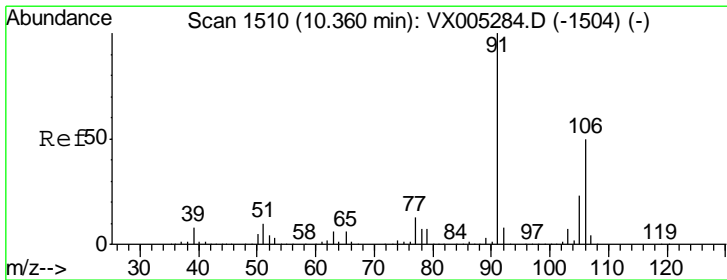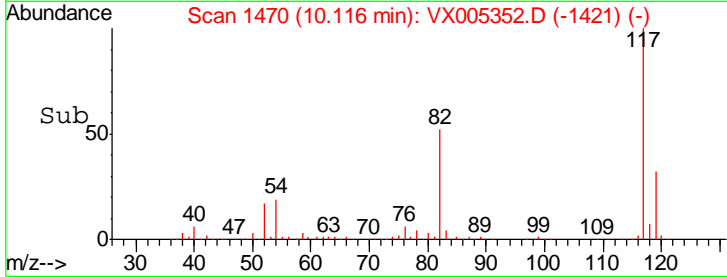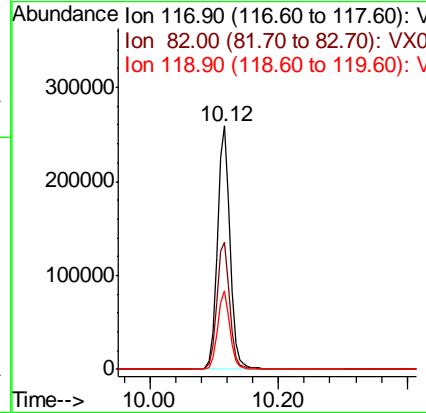

#68
 m/p-Xylenes
 Concen: 0.393 ug/l
 RT: 10.35 min Scan# 1509
 Delta R.T. -0.01 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01

Tgt Ion	Resp	Lower	Upper
106	1882		
91	208.8	157.1	235.7



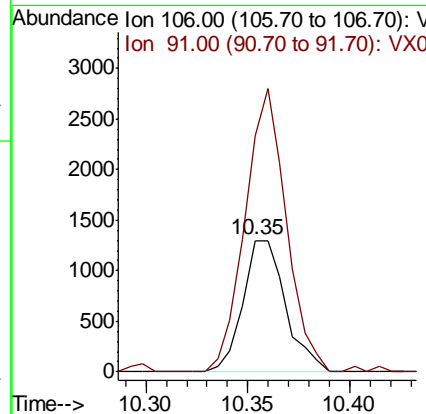
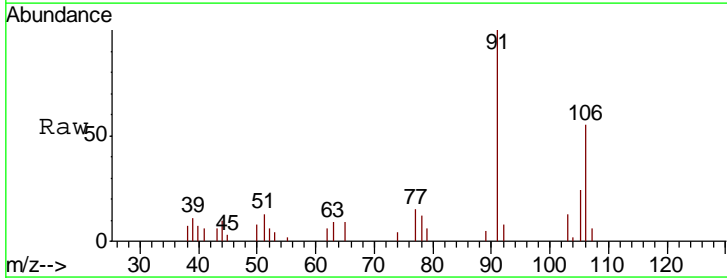




#69
 o-Xylene
 Concen: 0.234 ug/l
 RT: 10.70 min Scan# 1566
 Delta R.T. 0.00 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01




Instrument : MSVOA_X
 ClientSampled : CL-02-101218-C


Tgt Ion	Resp	Lower	Upper
106	1080		
91	202.8	105.1	315.1

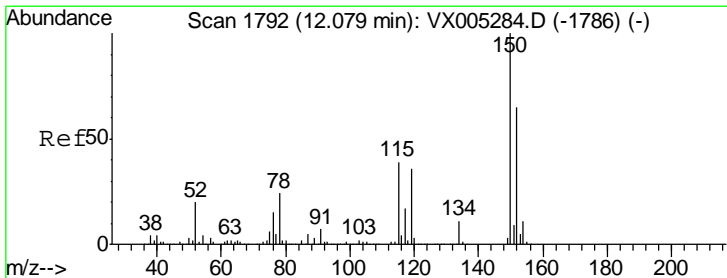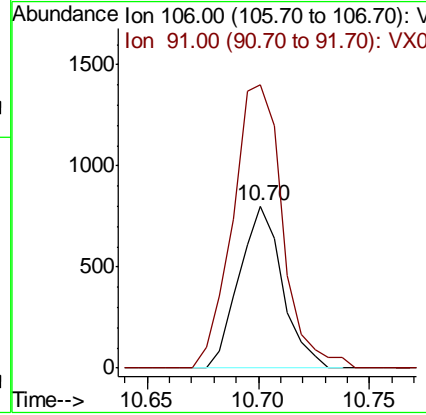

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.08 min Scan# 1792
 Delta R.T. 0.00 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01

Tgt Ion	Resp	Lower	Upper
152	168824		
115	54.6	39.0	117.0
150	155.8	0.0	351.0



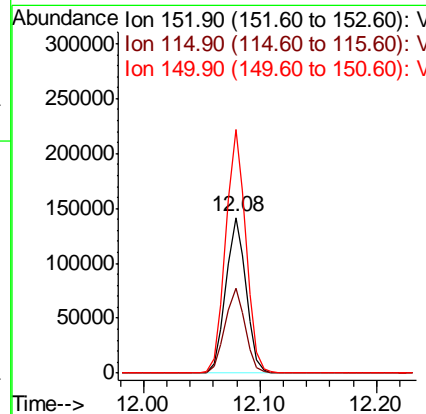



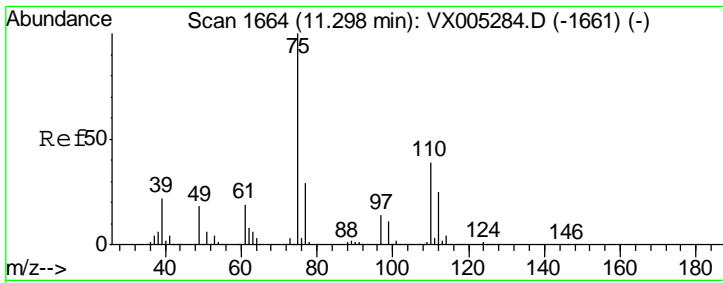

#76
 1,2,3-Trichloropropane
 Concen: 22.620 ug/l
 RT: 11.14 min Scan# 1638
 Delta R.T. -0.16 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01




Instrument :
 MSVOA_X
 ClientSampled :
 CL-02-101218-C


Tgt Ion: 75 Resp: 74074
 Ion Ratio Lower Upper
 75 100
 77 1.4 20.2 60.6#

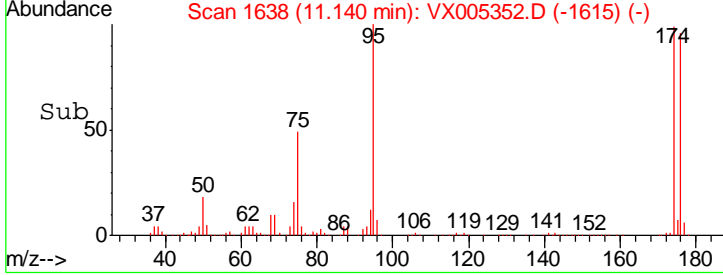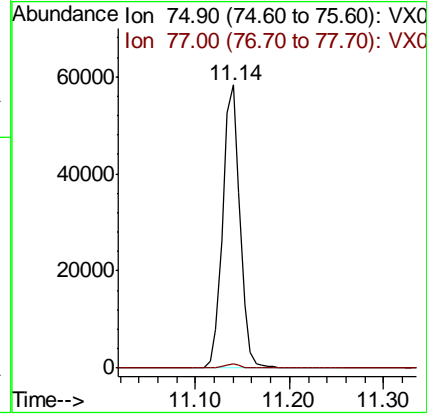

#80
 1,3,5-Trimethylbenzene
 Concen: 0.358 ug/l
 RT: 11.51 min Scan# 1698
 Delta R.T. 0.00 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01

Tgt Ion: 105 Resp: 3081
 Ion Ratio Lower Upper
 105 100
 120 47.0 25.6 76.8

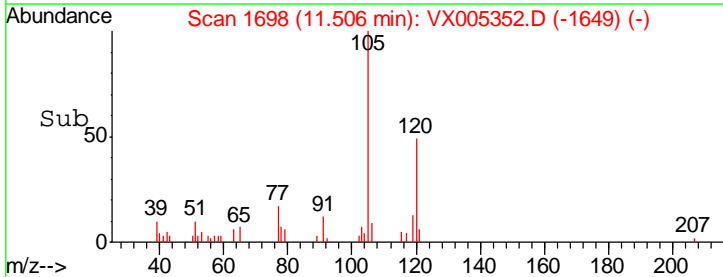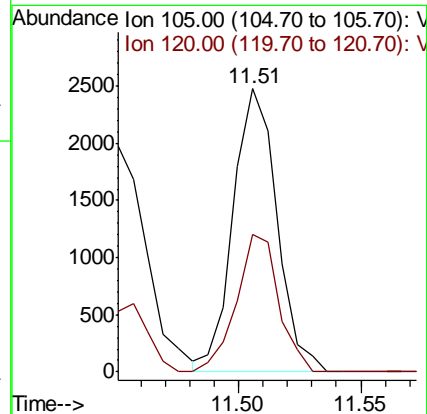


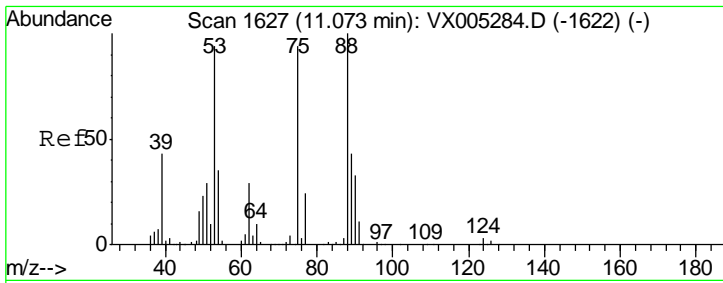




#81
 trans-1,4-Dichloro-2-butene
 Concen: 68.731 ug/l
 RT: 11.14 min Scan# 1638
 Delta R.T. 0.07 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01

Instrument :
 MSVOA_X
 ClientSampled :
 CL-02-101218-C

Tgt Ion	Resp	Lower	Upper
75	100		
53	0.2	80.1	120.1#
89	0.0	37.2	55.8#




Abundance Ion 74.90 (74.60 to 75.60): VX0
 Ion 53.00 (52.70 to 53.70): VX0
 Ion 88.90 (88.60 to 89.60): VX0

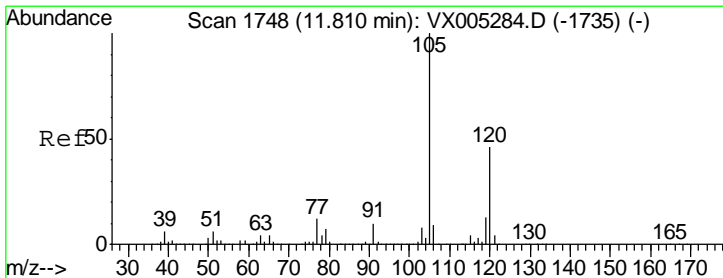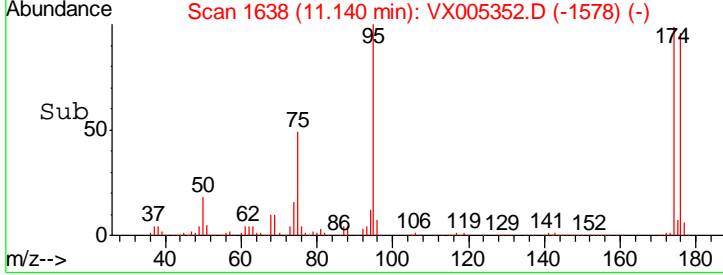
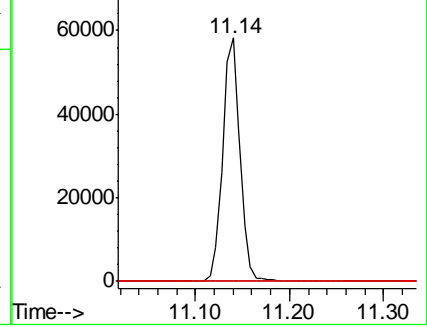



#84
 1,2,4-Trimethylbenzene
 Concen: 0.931 ug/l
 RT: 11.81 min Scan# 1748
 Delta R.T. 0.00 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01

Tgt Ion	Resp	Lower	Upper
105	100		
120	49.9	23.2	69.6

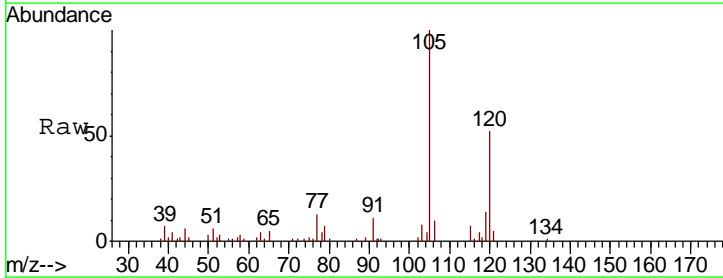

Abundance Ion 105.00 (104.70 to 105.70): V
 Ion 120.00 (119.70 to 120.70): V

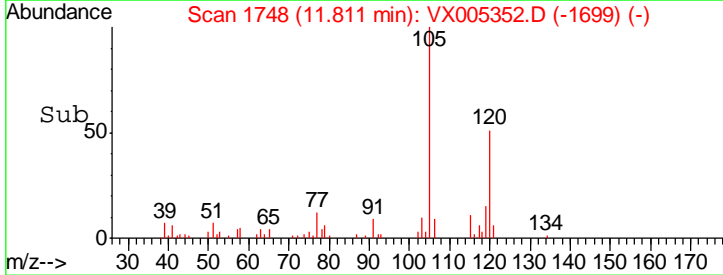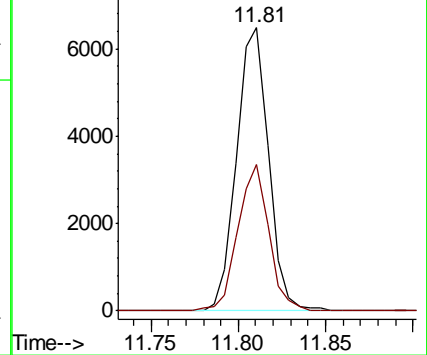

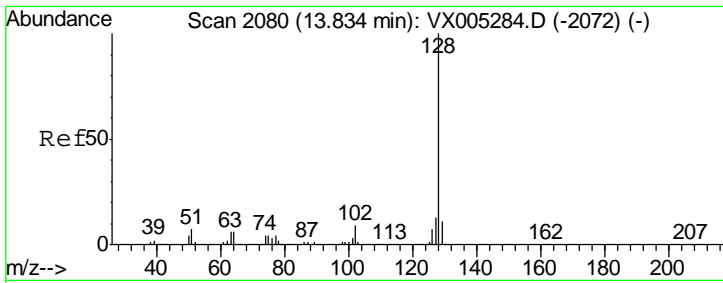

#95
 Naphthalene
 Concen: 27.589 ug/l
 RT: 13.83 min Scan# 2080
 Delta R.T. 0.00 min
 Lab File: VX005352.D
 Acq: 15 Oct 2018 19:01

Instrument : MSVOA_X
 ClientSampled : CL-02-101218-C

Tot Ion	128	Resp	321211
Ion	Ratio	Lower	Upper
128	100		
127	13.1	10.2	15.2
129	10.9	8.6	12.8

