


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX101519\
Data File : VX013066.D
Acq On : 15 Oct 2019 09:55
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Title : SW846 8260
Last Update : Wed Oct 16 07:26:22 2019

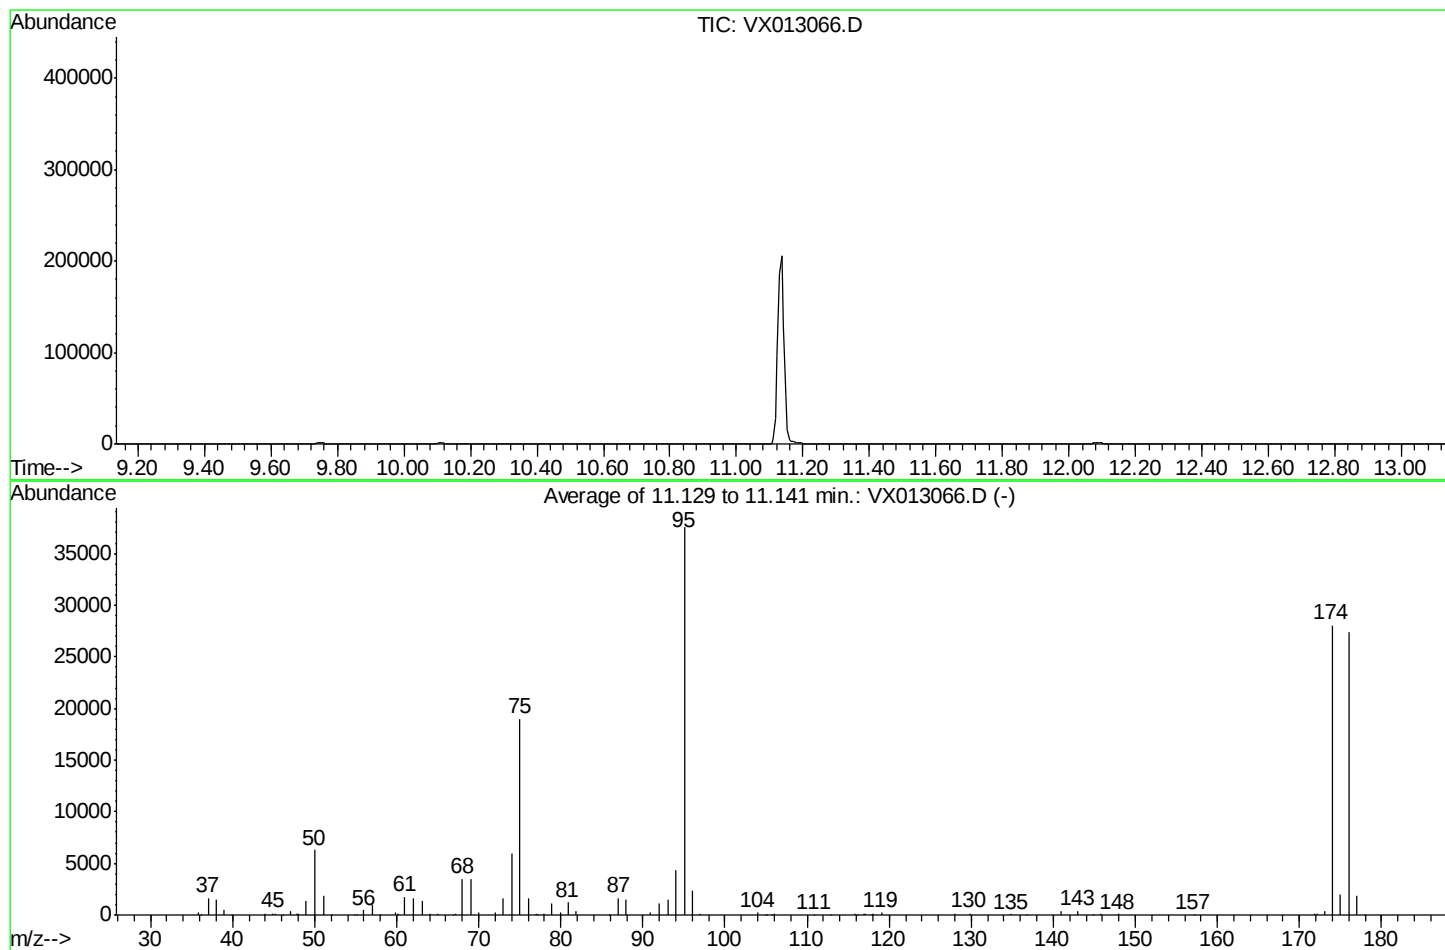

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	6308	PASS
75	95	30	60	50.7	19017	PASS
95	95	100	100	100.0	37536	PASS
96	95	5	9	6.4	2393	PASS
173	174	0.00	2	1.4	404	PASS
174	95	50	100	74.7	28056	PASS
175	174	5	9	7.0	1951	PASS
176	174	95	101	97.5	27354	PASS
177	176	5	9	6.7	1828	PASS