


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX101520\
 Data File : VX018932.D
 Acq On : 15 Oct 2020 12:59
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X101520W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Oct 15 15:32:58 2020

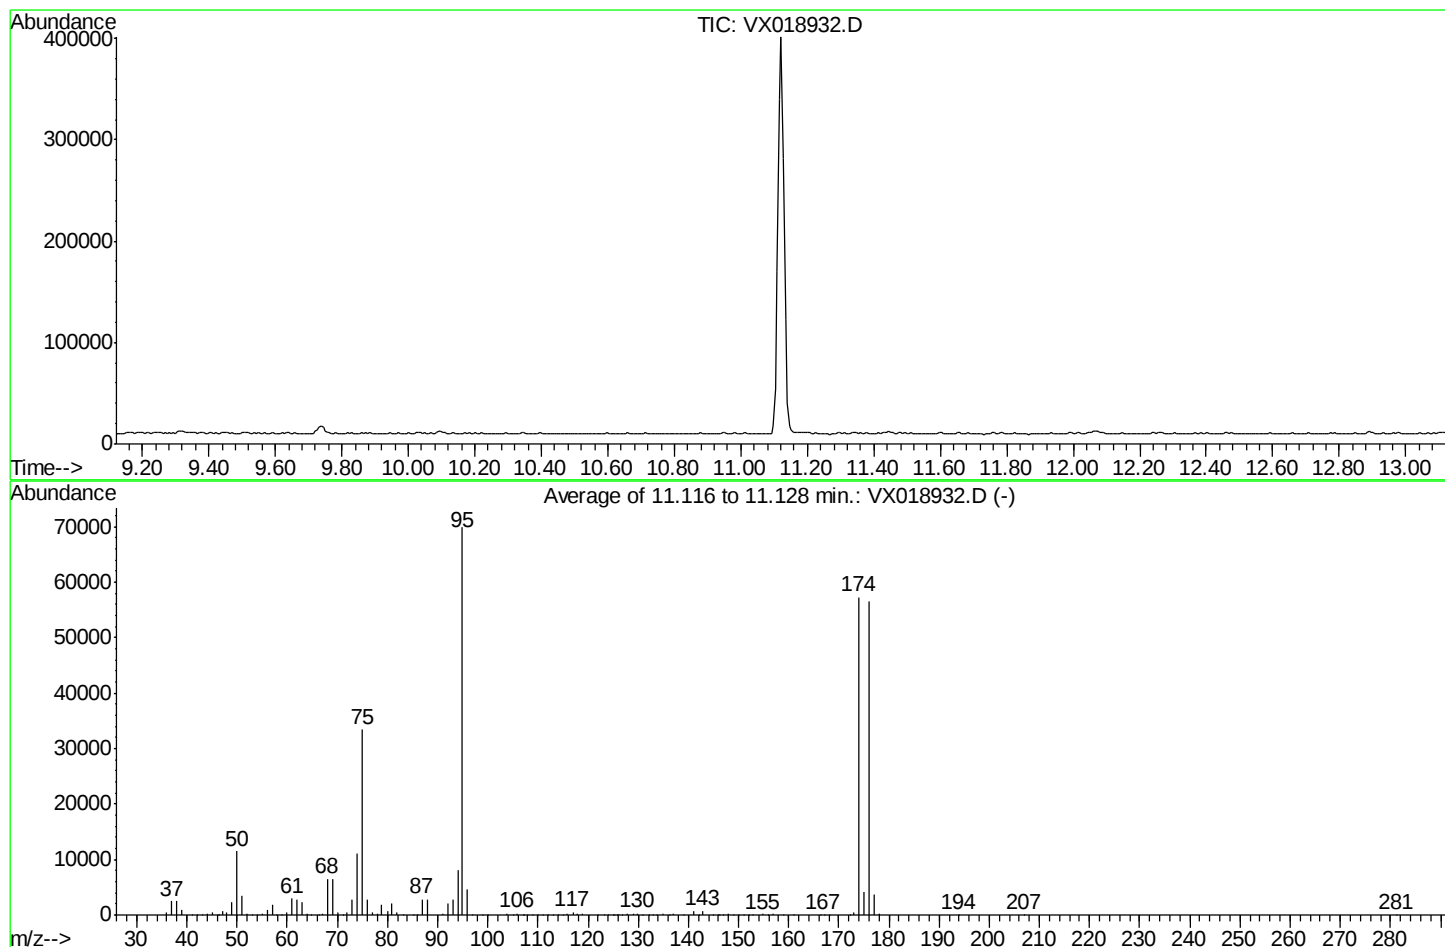

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1639

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	11441	PASS
75	95	30	60	47.8	33397	PASS
95	95	100	100	100.0	69916	PASS
96	95	5	9	6.6	4622	PASS
173	174	0.00	2	1.0	573	PASS
174	95	50	100	82.0	57317	PASS
175	174	5	9	7.4	4236	PASS
176	174	95	101	98.5	56482	PASS
177	176	5	9	6.6	3745	PASS