

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
 Data File : VX024827.D
 Acq On : 15 Oct 2021 13:17
 Operator : JC/MD
 Sample : VX1015WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK610

Quant Time: Oct 18 01:29:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 18 01:29:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	270301	50.00	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	252712	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	118017	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	60026	35.87	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	71.74%
7) Chloroethane-d5	1.666	69	49596	45.02	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.04%
11) 1,1-Dichloroethene-d2	2.306	63	103096	31.38	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.76%
21) 2-Butanone-d5	4.459	46	143405	104.23	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	104.23%
24) Chloroform-d	5.062	84	152842	45.09	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.18%
26) 1,2-Dichloroethane-d4	5.958	65	113928	47.53	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.06%
32) Benzene-d6	5.977	84	309323	43.45	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.90%
36) 1,2-Dichloropropane-d6	7.312	67	99493	44.69	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	89.38%
41) Toluene-d8	8.653	98	280692	40.47	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.94%
43) trans-1,3-Dichloroprop...	8.952	79	48555	44.01	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.02%
47) 2-Hexanone-d5	9.384	63	99823	95.50	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.50%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	144493	47.12	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.24%
66) 1,2-Dichlorobenzene-d4	12.323	152	110078	47.67	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.34%
Target Compounds						
25) Chloroform	5.099	83	12483	3.36	ug/L	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
Data File : VX024827.D
Acq On : 15 Oct 2021 13:17
Operator : JC/MD
Sample : VX1015WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK610

Quant Time: Oct 18 01:29:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM100721WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Oct 18 01:29:23 2021
Response via : Initial Calibration

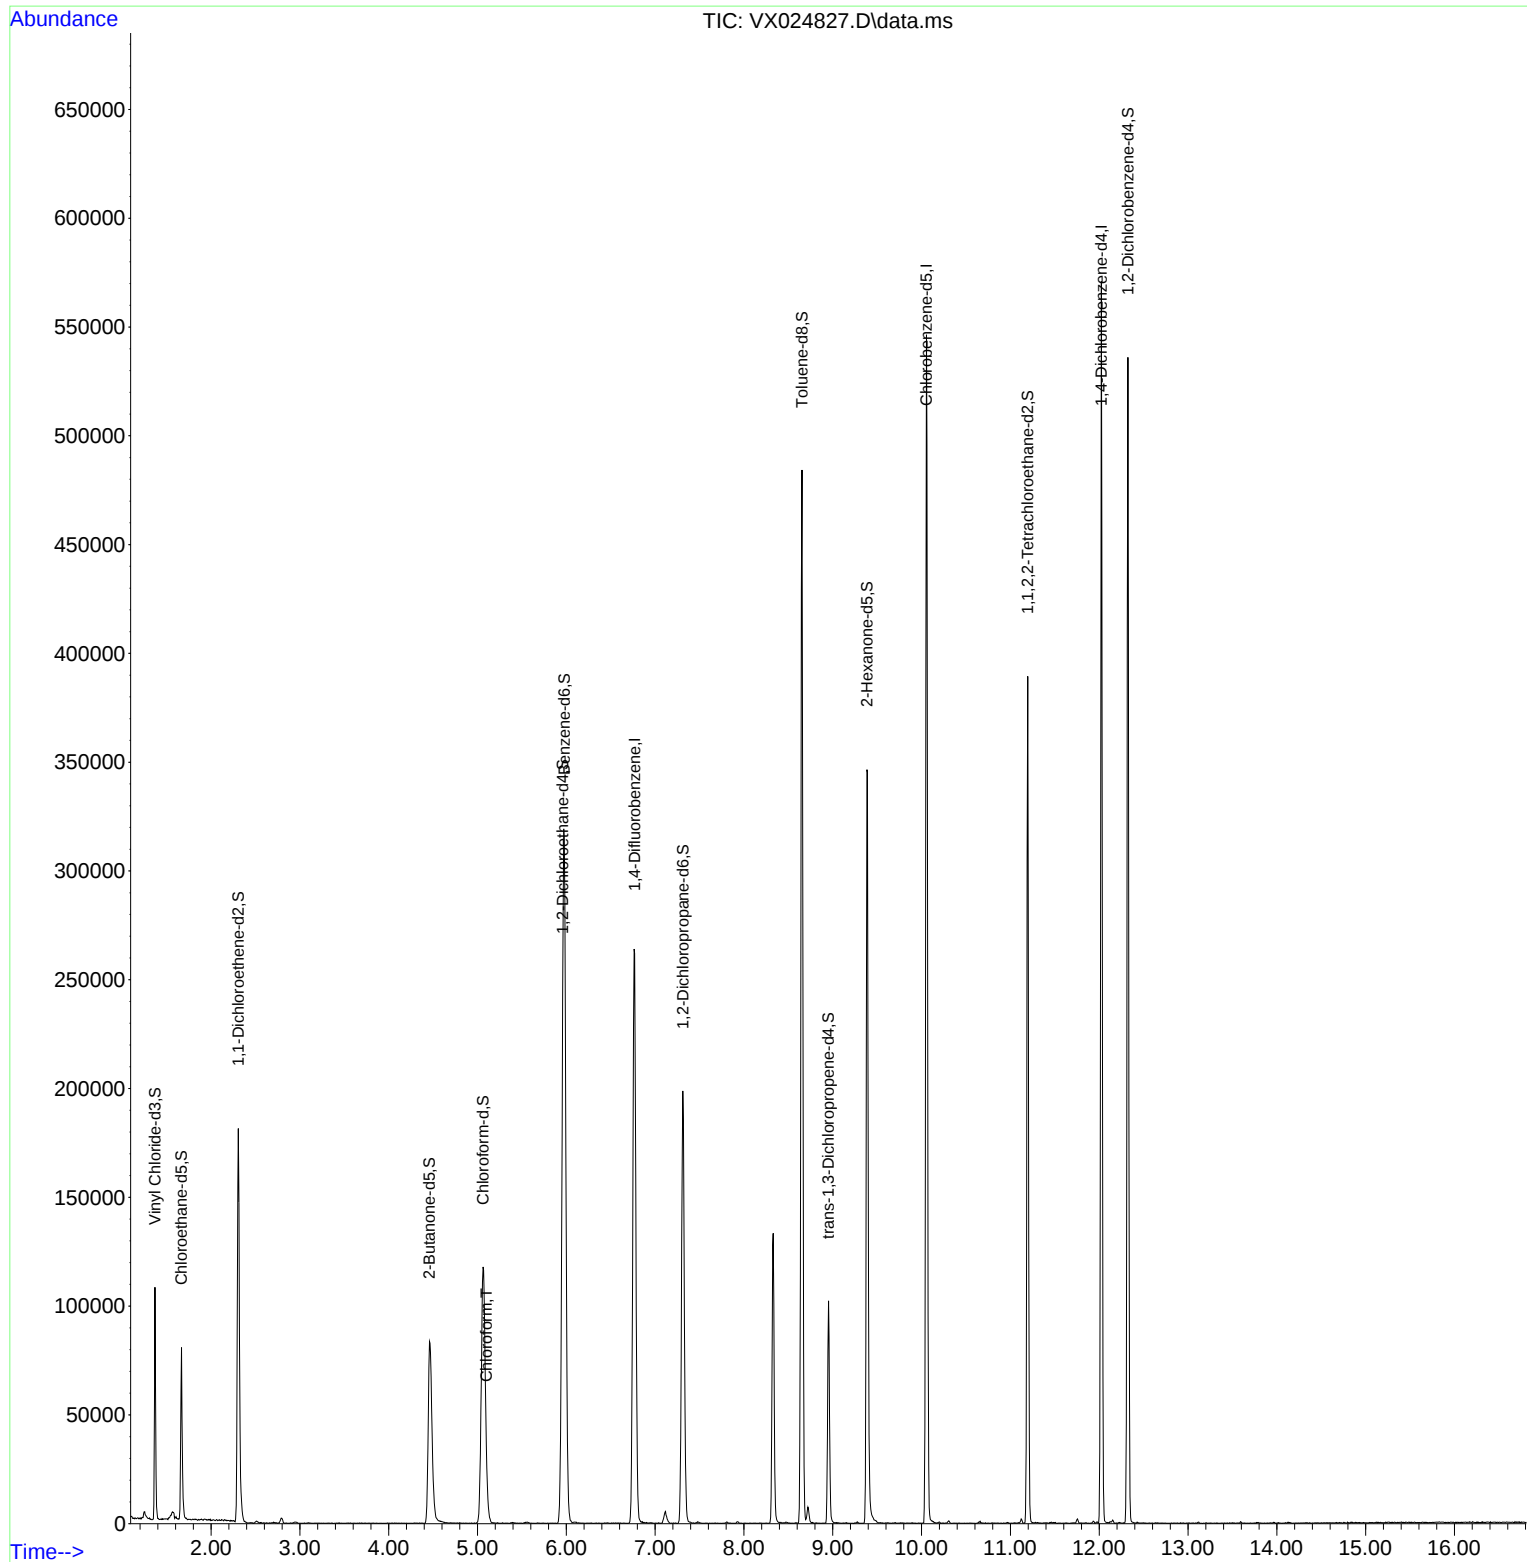

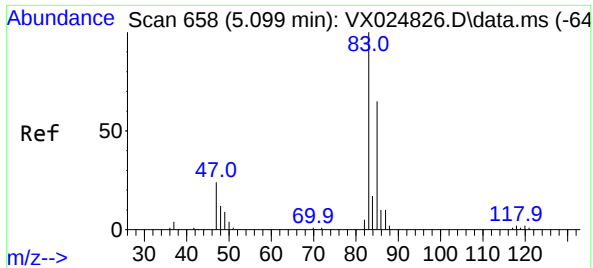

#25
Chloroform
Concen: 3.36 ug/L
RT: 5.099 min Scan# 658
Delta R.T. -0.000 min
Lab File: VX024827.D
Acq: 15 Oct 2021 13:17

Instrument :
MSVOA_X
ClientSampleId :
VBLK610

Tgt Ion: 83 Resp: 12483
Ion Ratio Lower Upper
83 100
85 66.1 46.3 85.9

