

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
 Data File : VX024821.D
 Acq On : 14 Oct 2021 18:56
 Operator : JC/MD
 Sample : VX1015WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK609

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M

Title : VOC Analysis

Signal : TIC: VX024821.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	33	rBV2	5305	7444	0.78%	0.100%
2	1.368	43	46	53	rBV	116168	104179	10.88%	1.402%
3	1.666	91	95	104	rVB	80259	99471	10.39%	1.339%
4	2.306	194	200	213	rVB	178920	288154	30.09%	3.879%
5	2.514	229	234	239	rBV2	772	1306	0.14%	0.018%
6	2.550	239	240	243	rVV2	334	225	0.02%	0.003%
7	2.697	263	264	266	rBV	305	290	0.03%	0.004%
8	2.788	274	279	286	rVB3	3174	5691	0.59%	0.077%
9	2.953	301	306	313	rVB3	529	1249	0.13%	0.017%
10	3.081	326	327	330	rBV3	192	213	0.02%	0.003%
11	3.166	339	341	342	rVB	325	187	0.02%	0.003%
12	3.184	342	344	346	rBV	222	267	0.03%	0.004%
13	3.300	361	363	365	rVV	206	158	0.02%	0.002%
14	3.361	371	373	376	rVB2	176	148	0.02%	0.002%
15	3.532	398	401	403	rBV	149	161	0.02%	0.002%
16	3.721	430	432	434	rVB2	228	163	0.02%	0.002%
17	3.934	464	467	469	rVB2	218	235	0.02%	0.003%
18	4.062	486	488	491	rVB	324	280	0.03%	0.004%
19	4.099	491	494	498	rBV2	237	417	0.04%	0.006%
20	4.465	544	554	576	rBV	89229	265731	27.75%	3.577%
21	5.068	640	653	671	rBV	121067	395446	41.29%	5.323%
22	5.391	704	706	710	rVB3	281	272	0.03%	0.004%
23	5.538	726	730	732	rBV2	341	441	0.05%	0.006%
24	5.556	732	733	734	rBV	355	162	0.02%	0.002%
25	5.976	790	802	818	rVV2	329040	957722	100.00%	12.891%
26	6.098	821	822	829	rVV3	642	856	0.09%	0.012%
27	6.178	832	835	837	rVB	267	217	0.02%	0.003%
28	6.214	839	841	845	rVB	247	233	0.02%	0.003%
29	6.263	847	849	851	rBV	156	158	0.02%	0.002%
30	6.391	868	870	872	rVB2	282	217	0.02%	0.003%
31	6.409	872	873	874	rBV	299	150	0.02%	0.002%
32	6.446	877	879	882	rBV2	221	270	0.03%	0.004%
33	6.531	891	893	895	rBV2	218	232	0.02%	0.003%
34	6.769	922	932	944	rBV	252878	596623	62.30%	8.030%
35	6.873	948	949	950	rVB	506	187	0.02%	0.003%
36	7.117	982	989	999	rVB2	5538	12550	1.31%	0.169%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
 Data File : VX024821.D
 Acq On : 14 Oct 2021 18:56
 Operator : JC/MD
 Sample : VX1015WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK609

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
 Title : VOC Analysis

37	7.312	1012	1021	1036	rBV	196805	434602	45.38%	5.850%
38	7.434	1039	1041	1043	rBV	222	166	0.02%	0.002%
39	7.476	1043	1048	1054	rBV4	534	1155	0.12%	0.016%
40	7.805	1097	1102	1110	rVB4	558	1005	0.10%	0.014%
41	7.885	1114	1115	1118	rVB	241	149	0.02%	0.002%
42	7.927	1118	1122	1129	rBV4	966	1562	0.16%	0.021%
43	8.141	1155	1157	1161	rBV2	196	335	0.03%	0.005%
44	8.263	1175	1177	1181	rBV2	188	249	0.03%	0.003%
45	8.330	1181	1188	1201	rBV	134445	219627	22.93%	2.956%
46	8.415	1201	1202	1204	rBV	392	189	0.02%	0.003%
47	8.476	1209	1212	1217	rVB4	565	764	0.08%	0.010%
48	8.586	1225	1230	1232	rBV2	274	326	0.03%	0.004%
49	8.653	1234	1241	1249	rBV	488804	751855	78.50%	10.120%
50	8.726	1249	1253	1259	rVB	6917	11278	1.18%	0.152%
51	8.952	1284	1290	1297	rBV	100655	148600	15.52%	2.000%
52	9.171	1324	1326	1328	rBV	243	160	0.02%	0.002%
53	9.275	1341	1343	1348	rVB3	625	797	0.08%	0.011%
54	9.330	1348	1352	1353	rVB2	213	180	0.02%	0.002%
55	9.391	1356	1362	1376	rBV	377477	556157	58.07%	7.486%
56	9.616	1397	1399	1401	rVB2	226	176	0.02%	0.002%
57	10.055	1465	1471	1484	rBV	524707	711470	74.29%	9.576%
58	10.201	1491	1495	1499	rVB3	408	631	0.07%	0.008%
59	10.305	1507	1512	1519	rBV4	1070	1814	0.19%	0.024%
60	10.451	1533	1536	1538	rBV2	139	168	0.02%	0.002%
61	10.500	1542	1544	1547	rBV	185	179	0.02%	0.002%
62	10.652	1565	1569	1574	rBV4	456	818	0.09%	0.011%
63	10.726	1579	1581	1585	rBV2	147	149	0.02%	0.002%
64	10.957	1617	1619	1620	rVV2	256	173	0.02%	0.002%
65	11.091	1638	1641	1643	rBV3	408	439	0.05%	0.006%
66	11.122	1643	1646	1649	rVB3	1631	1891	0.20%	0.025%
67	11.195	1652	1658	1668	rBV	402690	505113	52.74%	6.799%
68	11.457	1698	1701	1703	rBV3	580	771	0.08%	0.010%
69	11.482	1703	1705	1709	rVB3	640	640	0.07%	0.009%
70	11.610	1723	1726	1729	rBV2	155	244	0.03%	0.003%
71	11.689	1735	1739	1740	rBV	180	283	0.03%	0.004%
72	11.756	1746	1750	1754	rVB2	2093	2589	0.27%	0.035%
73	11.835	1762	1763	1765	rBV2	177	164	0.02%	0.002%
74	11.872	1767	1769	1772	rBV2	218	260	0.03%	0.003%
75	11.939	1776	1780	1782	rBV2	880	1030	0.11%	0.014%
76	11.975	1783	1786	1789	rBV	449	490	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
 Data File : VX024821.D
 Acq On : 14 Oct 2021 18:56
 Operator : JC/MD
 Sample : VX1015WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK609

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M

Title : VOC Analysis

77	12.024	1789	1794	1804	rBV	520388	646566	67.51%	8.703%
78	12.323	1837	1843	1849	rBV	543341	677162	70.71%	9.114%
79	12.488	1868	1870	1872	rVB	222	181	0.02%	0.002%
80	12.616	1888	1891	1894	rBV2	194	279	0.03%	0.004%
81	13.054	1962	1963	1967	rVB	317	319	0.03%	0.004%
82	13.115	1971	1973	1975	rVV2	269	259	0.03%	0.003%
83	13.207	1985	1988	1992	rVB2	182	289	0.03%	0.004%
84	13.250	1992	1995	1996	rBV2	188	200	0.02%	0.003%
85	13.280	1998	2000	2002	rVV2	181	221	0.02%	0.003%
86	13.323	2005	2007	2010	rVV	308	241	0.03%	0.003%
87	13.439	2023	2026	2027	rBV2	200	148	0.02%	0.002%
88	13.524	2039	2040	2046	rBV	204	328	0.03%	0.004%
89	13.774	2079	2081	2082	rBV	215	229	0.02%	0.003%
90	13.963	2110	2112	2113	rBV	280	277	0.03%	0.004%
91	14.030	2121	2123	2126	rBV2	149	152	0.02%	0.002%
92	14.073	2127	2130	2131	rVB	306	214	0.02%	0.003%
93	14.329	2168	2172	2173	rBV2	250	278	0.03%	0.004%
94	14.402	2182	2184	2187	rVB2	329	225	0.02%	0.003%
95	15.085	2294	2296	2298	rVB2	413	300	0.03%	0.004%
96	15.109	2298	2300	2301	rBV2	365	268	0.03%	0.004%
97	15.389	2343	2346	2348	rBV2	347	435	0.05%	0.006%
98	15.414	2348	2350	2352	rVB2	448	208	0.02%	0.003%
99	15.542	2369	2371	2373	rBV3	274	230	0.02%	0.003%
100	15.645	2387	2388	2390	rBV	249	147	0.02%	0.002%




Sum of corrected areas: 7429509

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
Data File : VX024821.D
Acq On : 14 Oct 2021 18:56
Operator : JC/MD
Sample : VX1015WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK609

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

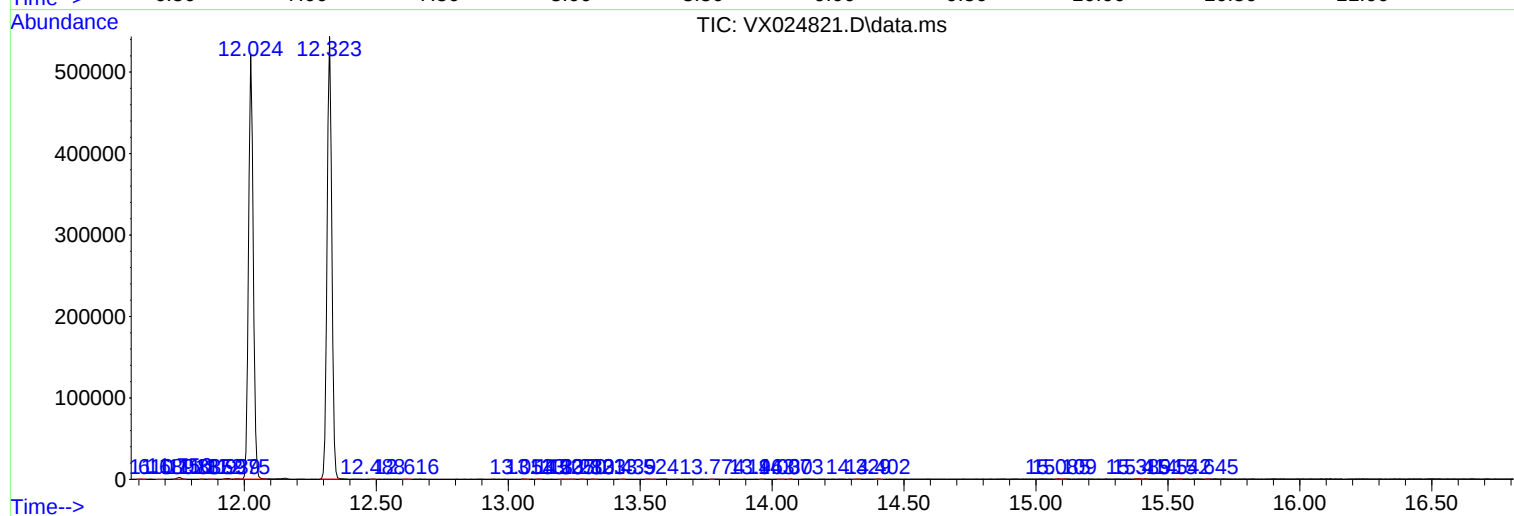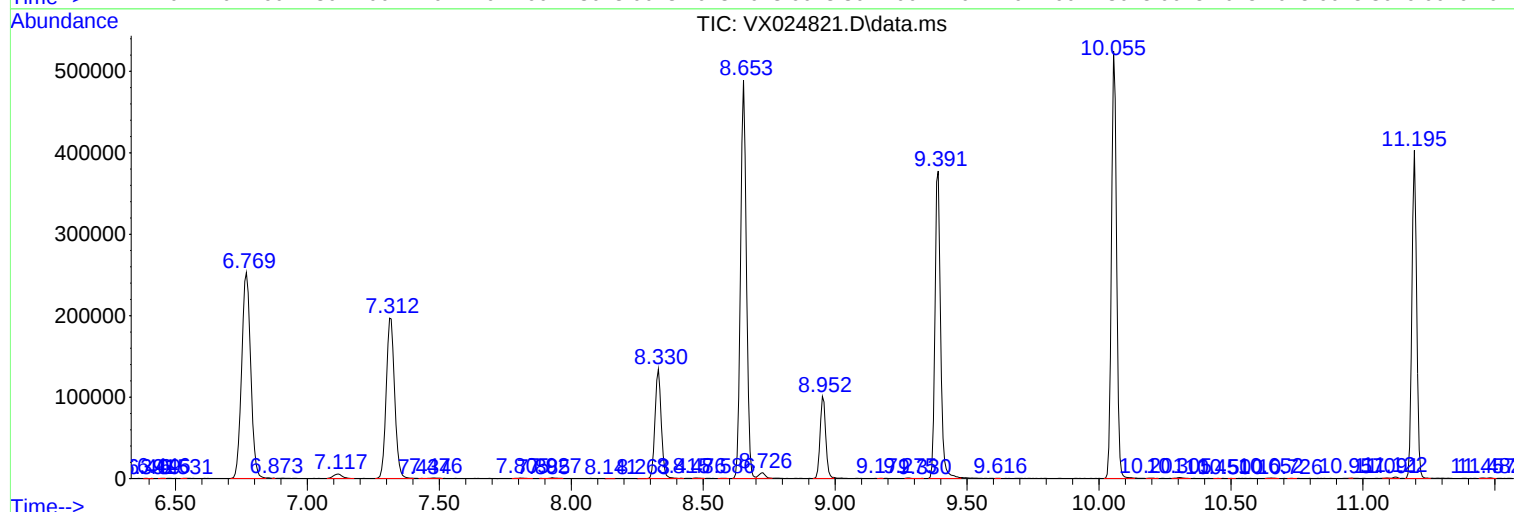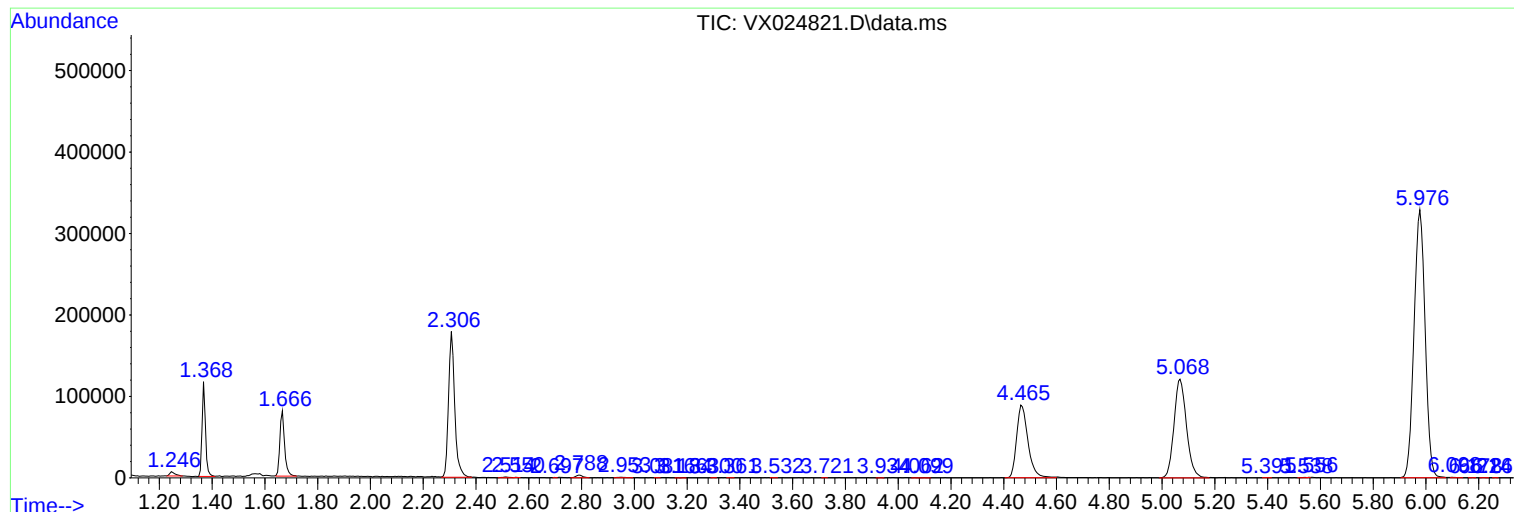

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
Data File : VX024821.D
Acq On : 14 Oct 2021 18:56
Operator : JC/MD
Sample : VX1015WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK609

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM100721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
Data File : VX024821.D
Acq On : 14 Oct 2021 18:56
Operator : JC/MD
Sample : VX1015WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK609

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
