

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
 Data File : VX024823.D
 Acq On : 14 Oct 2021 19:43
 Operator : JC/MD
 Sample : M4103-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M

Title : VOC Analysis

Signal : TIC: VX024823.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	32	rBV	6009	8107	0.89%	0.114%
2	1.367	43	46	56	rVB	105302	96709	10.61%	1.364%
3	1.666	91	95	103	rVB	77454	92310	10.13%	1.302%
4	2.306	194	200	210	rBV	173076	274978	30.17%	3.878%
5	2.428	218	220	223	rBV3	345	341	0.04%	0.005%
6	2.788	275	279	284	rBV4	783	1294	0.14%	0.018%
7	2.946	301	305	306	rBV2	515	700	0.08%	0.010%
8	3.026	316	318	320	rBV	161	160	0.02%	0.002%
9	3.081	325	327	328	rVB2	378	180	0.02%	0.003%
10	3.093	328	329	331	rBV	242	226	0.02%	0.003%
11	3.172	340	342	346	rVB	260	284	0.03%	0.004%
12	3.300	361	363	367	rVB	279	283	0.03%	0.004%
13	3.331	367	368	370	rBV	204	170	0.02%	0.002%
14	3.751	433	437	439	rVB2	167	210	0.02%	0.003%
15	3.861	454	455	457	rBV	257	158	0.02%	0.002%
16	3.995	475	477	481	rVB2	172	168	0.02%	0.002%
17	4.471	543	555	570	rBV	82864	251564	27.60%	3.548%
18	4.733	597	598	601	rBV2	181	225	0.02%	0.003%
19	5.068	641	653	671	rVB	119646	375495	41.20%	5.296%
20	5.239	680	681	685	rVV	169	141	0.02%	0.002%
21	5.428	710	712	714	rBV	153	199	0.02%	0.003%
22	5.562	730	734	742	rBV3	503	1077	0.12%	0.015%
23	5.653	746	749	750	rVB	273	222	0.02%	0.003%
24	5.678	750	753	754	rBV	264	202	0.02%	0.003%
25	5.976	790	802	819	rBV2	312277	911357	100.00%	12.854%
26	6.165	829	833	837	rVB3	337	442	0.05%	0.006%
27	6.226	841	843	844	rVB	246	152	0.02%	0.002%
28	6.245	844	846	848	rBV	185	238	0.03%	0.003%
29	6.403	871	872	874	rBV	193	154	0.02%	0.002%
30	6.440	876	878	879	rVV	217	149	0.02%	0.002%
31	6.470	881	883	886	rVB3	242	251	0.03%	0.004%
32	6.769	923	932	948	rVV	236632	560953	61.55%	7.912%
33	7.019	971	973	974	rBV	243	227	0.02%	0.003%
34	7.123	982	990	998	rBV2	4968	11827	1.30%	0.167%
35	7.220	1004	1006	1008	rVB2	215	164	0.02%	0.002%
36	7.318	1011	1022	1033	rBV	187925	416633	45.72%	5.876%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
 Data File : VX024823.D
 Acq On : 14 Oct 2021 19:43
 Operator : JC/MD
 Sample : M4103-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM100721WMA.M
 Title : VOC Analysis

37	7.476	1046	1048	1049	rBV2	515	473	0.05%	0.007%
38	7.659	1076	1078	1081	rVB	229	160	0.02%	0.002%
39	7.811	1099	1103	1107	rVV	542	894	0.10%	0.013%
40	7.933	1118	1123	1129	rVB4	933	1624	0.18%	0.023%
41	8.031	1137	1139	1142	rBV	160	145	0.02%	0.002%
42	8.092	1145	1149	1153	rVB2	152	262	0.03%	0.004%
43	8.330	1181	1188	1196	rBV	127530	205354	22.53%	2.896%
44	8.476	1207	1212	1217	rBV	638	874	0.10%	0.012%
45	8.580	1227	1229	1231	rVB2	272	271	0.03%	0.004%
46	8.653	1234	1241	1250	rBV	458521	711843	78.11%	10.040%
47	8.726	1250	1253	1259	rVB	6558	9120	1.00%	0.129%
48	8.854	1273	1274	1276	rBV	196	178	0.02%	0.003%
49	8.951	1284	1290	1305	rBV	95450	144183	15.82%	2.034%
50	9.122	1317	1318	1321	rBV	279	262	0.03%	0.004%
51	9.171	1324	1326	1331	rVV2	346	452	0.05%	0.006%
52	9.220	1332	1334	1335	rVV	343	172	0.02%	0.002%
53	9.281	1339	1344	1349	rBV3	841	1321	0.14%	0.019%
54	9.348	1352	1355	1356	rBV2	182	215	0.02%	0.003%
55	9.390	1356	1362	1382	rBV	363348	533096	58.49%	7.519%
56	9.896	1443	1445	1448	rVB	196	198	0.02%	0.003%
57	9.927	1448	1450	1452	rBV	151	161	0.02%	0.002%
58	10.055	1466	1471	1488	rVB	496615	678516	74.45%	9.570%
59	10.305	1508	1512	1518	rVV3	1016	1572	0.17%	0.022%
60	10.360	1520	1521	1523	rBV3	257	214	0.02%	0.003%
61	10.591	1557	1559	1563	rVB2	172	162	0.02%	0.002%
62	10.793	1589	1592	1593	rBV	200	243	0.03%	0.003%
63	11.024	1629	1630	1636	rVB2	338	348	0.04%	0.005%
64	11.091	1636	1641	1642	rBV2	338	483	0.05%	0.007%
65	11.122	1642	1646	1652	rVV3	1628	2108	0.23%	0.030%
66	11.195	1652	1658	1669	rVB	386625	485687	53.29%	6.850%
67	11.463	1698	1702	1703	rBV2	293	358	0.04%	0.005%
68	11.664	1733	1735	1737	rBV	291	193	0.02%	0.003%
69	11.683	1737	1738	1741	rBV	132	141	0.02%	0.002%
70	11.750	1746	1749	1754	rVV2	1977	2322	0.25%	0.033%
71	11.890	1771	1772	1775	rVB	274	193	0.02%	0.003%
72	11.939	1776	1780	1783	rBV3	627	743	0.08%	0.010%
73	12.024	1789	1794	1803	rBV	503445	610965	67.04%	8.617%
74	12.122	1808	1810	1813	rVV2	481	495	0.05%	0.007%
75	12.225	1821	1827	1837	rBV	18622	28678	3.15%	0.404%
76	12.323	1838	1843	1852	rVB	521376	650610	71.39%	9.176%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
 Data File : VX024823.D
 Acq On : 14 Oct 2021 19:43
 Operator : JC/MD
 Sample : M4103-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AC6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M

Title : VOC Analysis

77	12.426	1858	1860	1861	rBV2	421	285	0.03%	0.004%
78	12.445	1861	1863	1867	rVB2	824	1011	0.11%	0.014%
79	12.481	1867	1869	1876	rVB	339	506	0.06%	0.007%
80	12.634	1893	1894	1896	rBV2	243	147	0.02%	0.002%
81	12.768	1914	1916	1918	rBV2	245	207	0.02%	0.003%
82	12.823	1921	1925	1926	rBV2	131	143	0.02%	0.002%
83	13.280	1998	2000	2001	rVB	301	135	0.01%	0.002%
84	13.457	2027	2029	2033	rBV	268	299	0.03%	0.004%
85	13.591	2050	2051	2053	rBV2	248	170	0.02%	0.002%
86	13.786	2079	2083	2087	rVB3	422	585	0.06%	0.008%
87	13.944	2107	2109	2111	rVB	267	150	0.02%	0.002%
88	13.963	2111	2112	2115	rVB	238	183	0.02%	0.003%
89	13.999	2115	2118	2121	rBV	262	359	0.04%	0.005%
90	14.030	2121	2123	2125	rBV	185	175	0.02%	0.002%
91	14.073	2128	2130	2131	rBV	294	208	0.02%	0.003%
92	14.371	2177	2179	2181	rVB3	239	208	0.02%	0.003%
93	14.835	2253	2255	2259	rBV3	234	280	0.03%	0.004%
94	14.993	2279	2281	2283	rBV2	524	434	0.05%	0.006%
95	15.292	2329	2330	2333	rBV	358	225	0.02%	0.003%
96	15.542	2370	2371	2372	rBV	323	213	0.02%	0.003%
97	15.956	2438	2439	2443	rBV3	424	354	0.04%	0.005%
98	16.371	2505	2507	2508	rBV	359	268	0.03%	0.004%
99	16.407	2511	2513	2514	rBV2	305	195	0.02%	0.003%
100	16.584	2540	2542	2543	rBV	333	181	0.02%	0.003%




Sum of corrected areas: 7090160

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
Data File : VX024823.D
Acq On : 14 Oct 2021 19:43
Operator : JC/MD
Sample : M4103-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
C0AC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM100721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

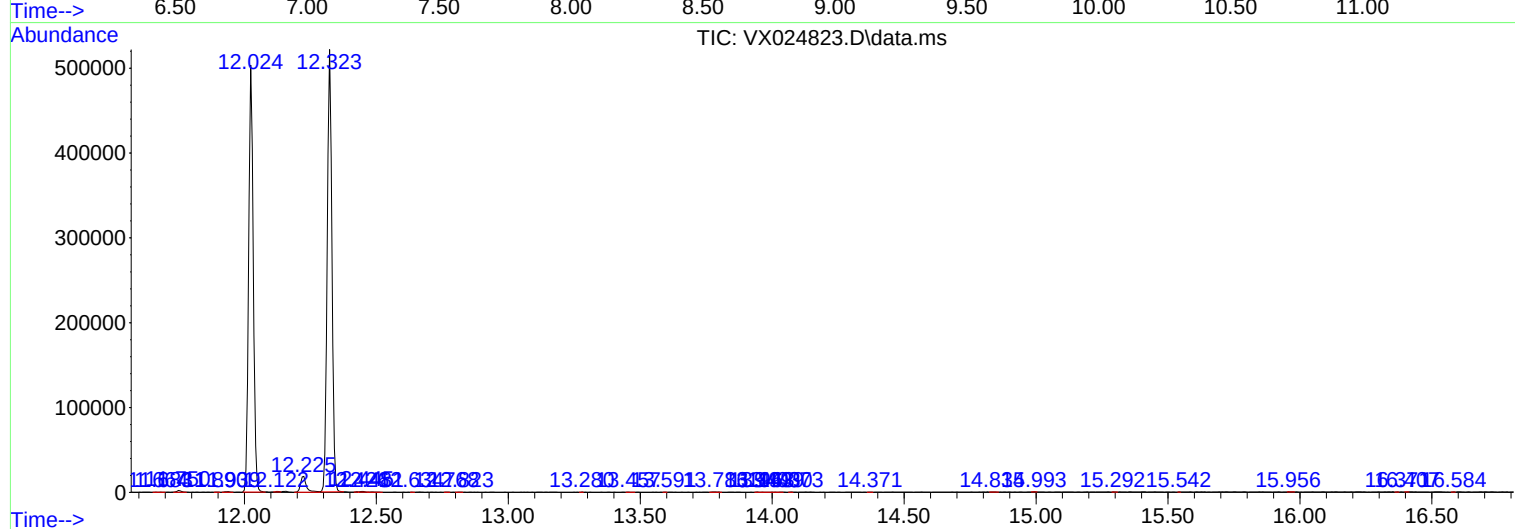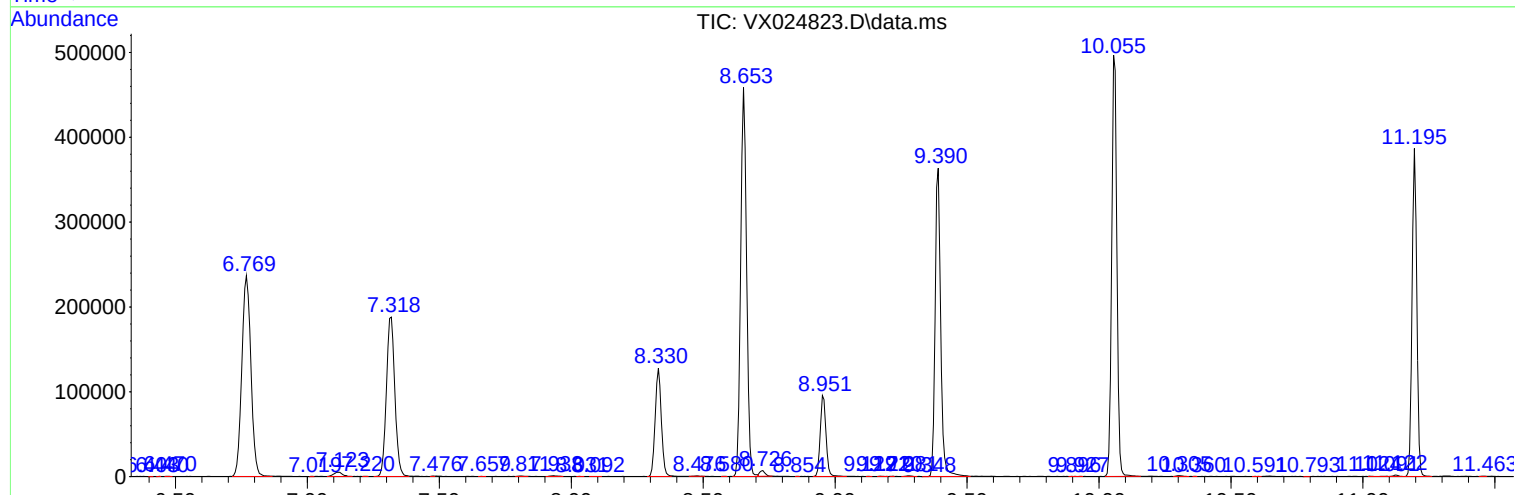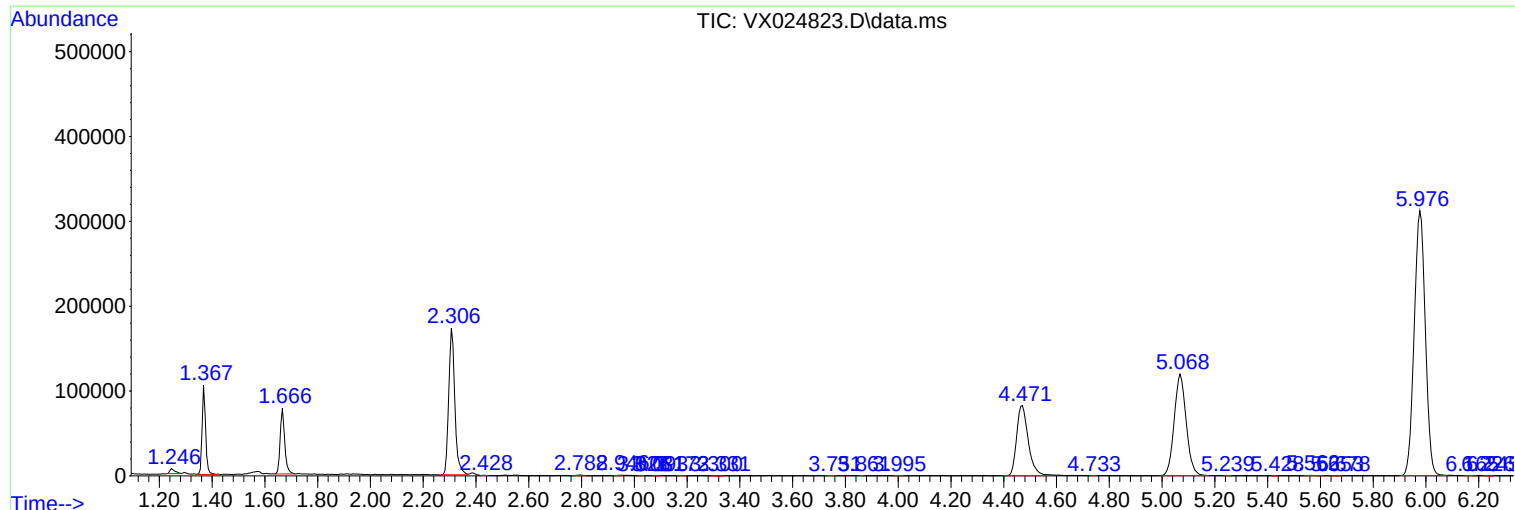

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
Data File : VX024823.D
Acq On : 14 Oct 2021 19:43
Operator : JC/MD
Sample : M4103-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM100721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
Data File : VX024823.D
Acq On : 14 Oct 2021 19:43
Operator : JC/MD
Sample : M4103-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AC6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
