

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
 Data File : VX024827.D
 Acq On : 15 Oct 2021 13:17
 Operator : JC/MD
 Sample : VX1015WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK610

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M

Title : VOC Analysis

Signal : TIC: VX024827.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	54	rVB	106756	96487	10.29%	1.296%
2	1.666	90	95	106	rVB	79106	95224	10.16%	1.279%
3	2.306	194	200	218	rVB	181305	295160	31.49%	3.965%
4	2.514	227	234	239	rBV3	1027	2340	0.25%	0.031%
5	2.563	239	242	244	rVV3	398	460	0.05%	0.006%
6	2.587	244	246	247	rVV	265	197	0.02%	0.003%
7	2.623	250	252	255	rBV2	244	241	0.03%	0.003%
8	2.703	263	265	269	rVB2	377	428	0.05%	0.006%
9	2.794	273	280	286	rBV2	2356	4348	0.46%	0.058%
10	4.221	513	514	518	rBV2	141	217	0.02%	0.003%
11	4.288	522	525	526	rBV	224	223	0.02%	0.003%
12	4.373	536	539	543	rVB2	145	197	0.02%	0.003%
13	4.459	544	553	571	rBV	83483	249621	26.63%	3.353%
14	5.062	638	652	671	rVV	117831	386292	41.21%	5.189%
15	5.221	676	678	680	rVB	238	188	0.02%	0.003%
16	5.282	686	688	691	rVB	246	188	0.02%	0.003%
17	5.379	701	704	705	rBV2	284	290	0.03%	0.004%
18	5.525	725	728	729	rBV	329	303	0.03%	0.004%
19	5.538	729	730	731	rBV	334	220	0.02%	0.003%
20	5.672	750	752	754	rBV2	184	180	0.02%	0.002%
21	5.970	788	801	817	rBV2	319194	937290	100.00%	12.591%
22	6.507	887	889	891	rBV2	228	193	0.02%	0.003%
23	6.531	891	893	895	rVV2	227	224	0.02%	0.003%
24	6.550	895	896	900	rVV2	216	263	0.03%	0.004%
25	6.763	921	931	945	rBV	263916	628748	67.08%	8.446%
26	6.903	953	954	959	rVB2	311	169	0.02%	0.002%
27	7.037	975	976	980	rVB2	264	206	0.02%	0.003%
28	7.117	980	989	999	rBV	5508	12334	1.32%	0.166%
29	7.312	1011	1021	1033	rBV	198703	427318	45.59%	5.740%
30	7.428	1038	1040	1043	rVB2	284	249	0.03%	0.003%
31	7.476	1043	1048	1056	rBV3	701	1505	0.16%	0.020%
32	7.610	1068	1070	1071	rBV	198	188	0.02%	0.003%
33	7.805	1099	1102	1107	rVB2	560	743	0.08%	0.010%
34	7.934	1118	1123	1127	rBV3	736	1259	0.13%	0.017%
35	8.330	1181	1188	1198	rBV	133155	217791	23.24%	2.926%
36	8.470	1209	1211	1217	rVB3	566	950	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
 Data File : VX024827.D
 Acq On : 15 Oct 2021 13:17
 Operator : JC/MD
 Sample : VX1015WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK610

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
 Title : VOC Analysis

37	8.586	1228	1230	1234	rVB2	271	207	0.02%	0.003%
38	8.653	1234	1241	1248	rBV	484088	742533	79.22%	9.974%
39	8.720	1248	1252	1259	rVB	7306	12348	1.32%	0.166%
40	8.811	1264	1267	1268	rBV	269	208	0.02%	0.003%
41	8.952	1284	1290	1301	rVV	102167	148865	15.88%	2.000%
42	9.153	1321	1323	1324	rVB	296	164	0.02%	0.002%
43	9.250	1337	1339	1340	rBV	366	311	0.03%	0.004%
44	9.275	1341	1343	1347	rVB2	679	688	0.07%	0.009%
45	9.384	1356	1361	1383	rVB	346168	524140	55.92%	7.041%
46	9.762	1422	1423	1425	rBV	240	177	0.02%	0.002%
47	10.055	1465	1471	1489	rVB	546169	750808	80.10%	10.086%
48	10.244	1500	1502	1503	rVB2	286	201	0.02%	0.003%
49	10.275	1503	1507	1508	rBV2	240	342	0.04%	0.005%
50	10.305	1508	1512	1517	rVB2	1156	1682	0.18%	0.023%
51	10.421	1529	1531	1536	rVB2	182	187	0.02%	0.003%
52	10.640	1565	1567	1568	rVV	595	461	0.05%	0.006%
53	10.659	1568	1570	1574	rVB2	877	856	0.09%	0.011%
54	10.720	1579	1580	1583	rVB	334	171	0.02%	0.002%
55	10.756	1583	1586	1587	rBV2	174	197	0.02%	0.003%
56	10.793	1591	1592	1594	rBV2	239	175	0.02%	0.002%
57	10.927	1611	1614	1616	rBV	202	194	0.02%	0.003%
58	10.970	1616	1621	1624	rVV3	403	613	0.07%	0.008%
59	11.049	1631	1634	1635	rBV2	237	203	0.02%	0.003%
60	11.091	1639	1641	1642	rVV	215	164	0.02%	0.002%
61	11.122	1642	1646	1650	rVB2	1996	2380	0.25%	0.032%
62	11.195	1652	1658	1666	rBV	389213	491095	52.40%	6.597%
63	11.280	1670	1672	1675	rBV	293	252	0.03%	0.003%
64	11.378	1686	1688	1689	rBV2	237	189	0.02%	0.003%
65	11.463	1698	1702	1704	rBV2	511	738	0.08%	0.010%
66	11.695	1735	1740	1742	rBV2	247	353	0.04%	0.005%
67	11.756	1746	1750	1754	rVV2	2001	2600	0.28%	0.035%
68	11.933	1775	1779	1782	rVB3	959	1164	0.12%	0.016%
69	11.975	1782	1786	1789	rBV3	678	787	0.08%	0.011%
70	12.024	1789	1794	1805	rVV	570698	700889	74.78%	9.415%
71	12.122	1809	1810	1812	rVV3	719	696	0.07%	0.009%
72	12.152	1813	1815	1818	rVB2	1501	1546	0.16%	0.021%
73	12.232	1823	1828	1832	rVV2	363	527	0.06%	0.007%
74	12.323	1837	1843	1858	rVB	535815	685318	73.12%	9.206%
75	12.427	1858	1860	1866	rBV4	534	688	0.07%	0.009%
76	12.567	1879	1883	1885	rBV2	152	172	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
 Data File : VX024827.D
 Acq On : 15 Oct 2021 13:17
 Operator : JC/MD
 Sample : VX1015WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK610

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
 Title : VOC Analysis

77	12.658	1897	1898	1902	rBV2	185	176	0.02%	0.002%
78	13.116	1970	1973	1976	rBV3	555	674	0.07%	0.009%
79	13.176	1981	1983	1986	rBV2	170	268	0.03%	0.004%
80	13.207	1986	1988	1990	rVB	257	217	0.02%	0.003%
81	13.469	2029	2031	2034	rBV	227	218	0.02%	0.003%
82	13.567	2042	2047	2049	rVB2	197	278	0.03%	0.004%
83	13.591	2049	2051	2054	rBV3	817	789	0.08%	0.011%
84	13.774	2080	2081	2082	rBV	303	217	0.02%	0.003%
85	13.963	2110	2112	2116	rVB2	526	682	0.07%	0.009%
86	14.079	2128	2131	2132	rBV2	183	246	0.03%	0.003%
87	14.097	2132	2134	2136	rVV	301	219	0.02%	0.003%
88	14.237	2156	2157	2160	rBV	181	190	0.02%	0.003%
89	14.365	2177	2178	2182	rVB	202	177	0.02%	0.002%
90	14.457	2191	2193	2195	rBV2	211	213	0.02%	0.003%
91	14.499	2198	2200	2202	rBV2	322	253	0.03%	0.003%
92	14.755	2240	2242	2244	rBV	316	240	0.03%	0.003%
93	14.847	2253	2257	2258	rBV2	385	455	0.05%	0.006%
94	14.883	2261	2263	2265	rBV2	283	170	0.02%	0.002%
95	16.017	2447	2449	2450	rBV	322	203	0.02%	0.003%
96	16.255	2487	2488	2490	rVB	418	176	0.02%	0.002%
97	16.273	2490	2491	2493	rBV2	304	162	0.02%	0.002%
98	16.310	2495	2497	2498	rBV	433	275	0.03%	0.004%
99	16.408	2512	2513	2515	rVB2	346	166	0.02%	0.002%
100	16.682	2557	2558	2560	rBV	404	202	0.02%	0.003%


Sum of corrected areas: 7444389

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
Data File : VX024827.D
Acq On : 15 Oct 2021 13:17
Operator : JC/MD
Sample : VX1015WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK610

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM100721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

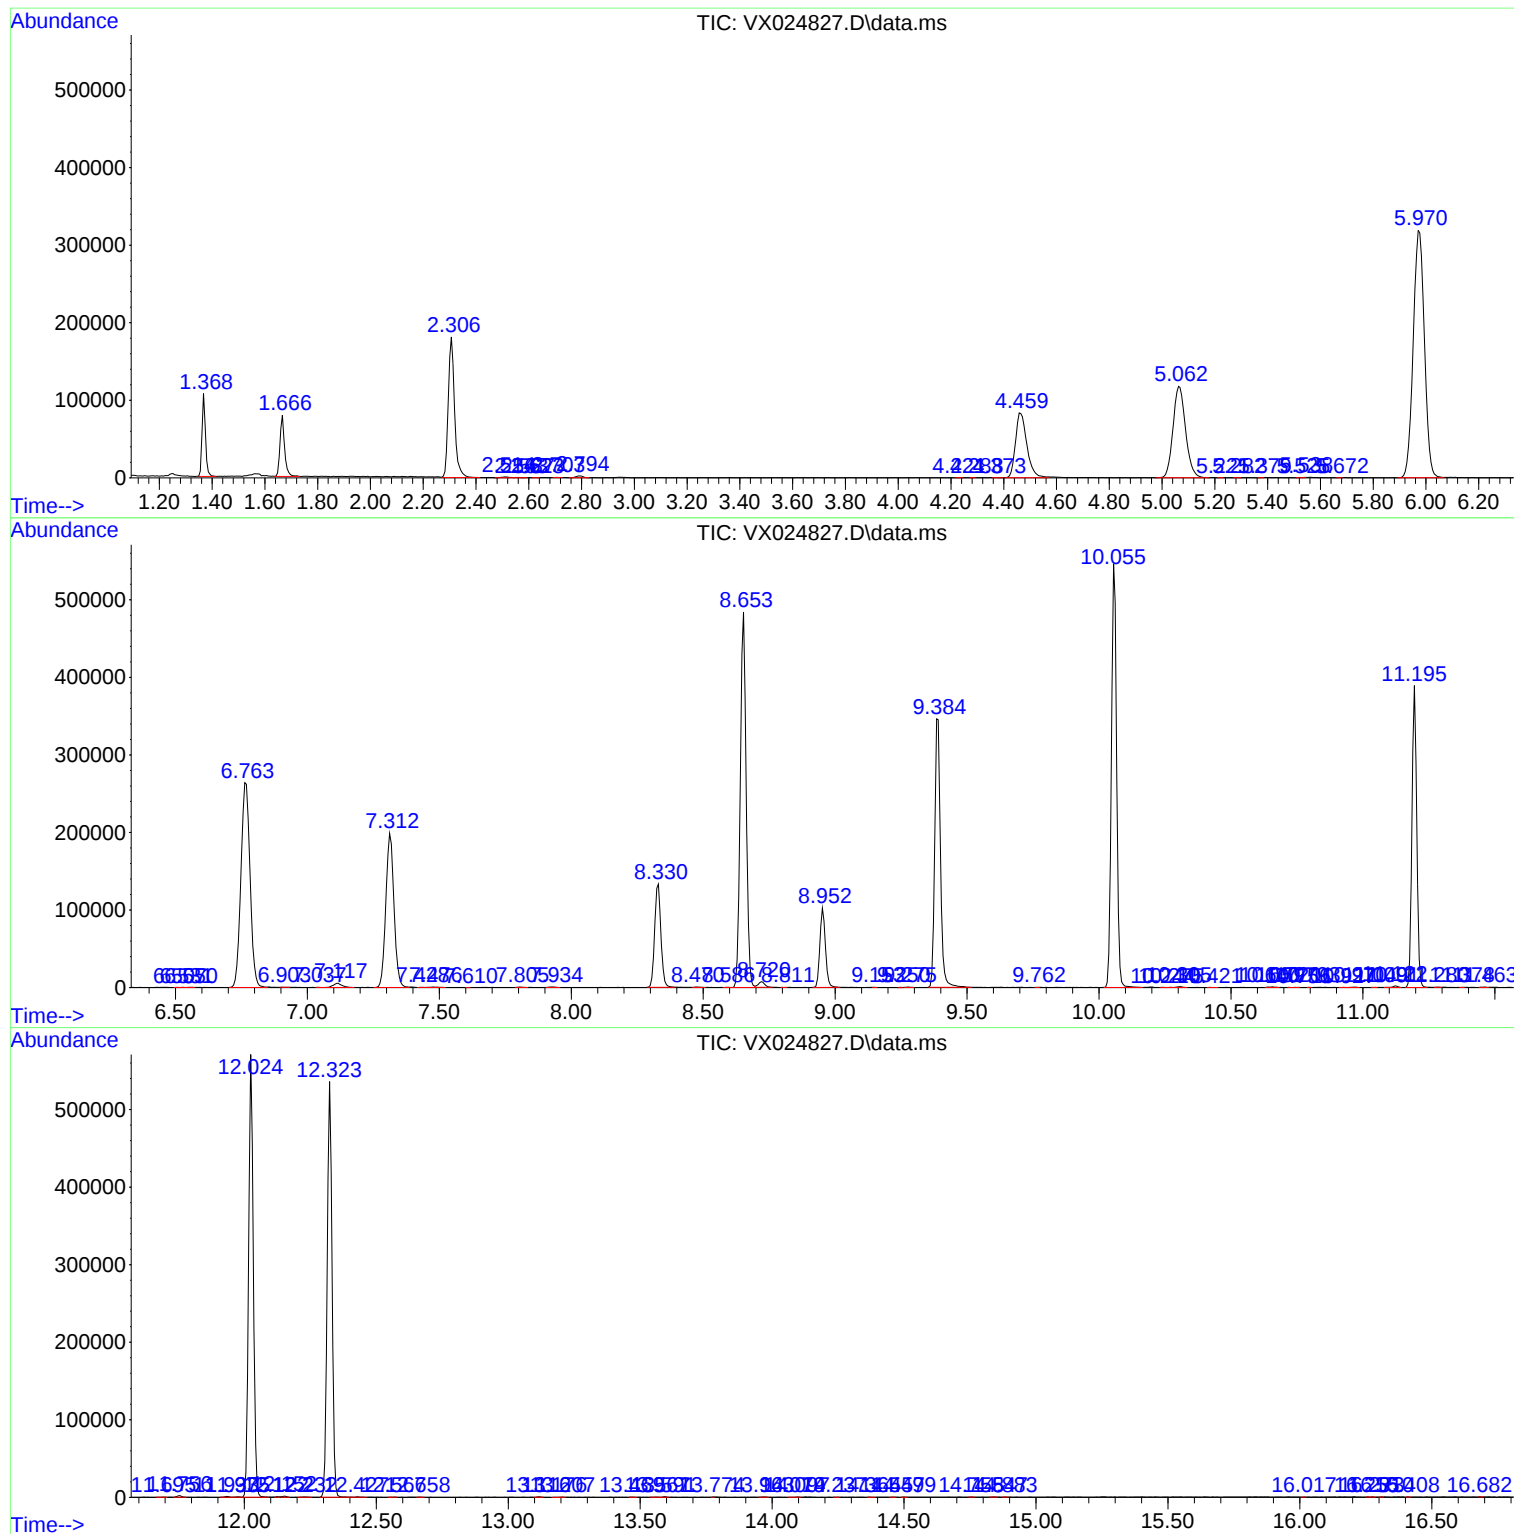

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
Data File : VX024827.D
Acq On : 15 Oct 2021 13:17
Operator : JC/MD
Sample : VX1015WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK610

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM100721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
Data File : VX024827.D
Acq On : 15 Oct 2021 13:17
Operator : JC/MD
Sample : VX1015WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK610

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
