

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
 Data File : VX024828.D
 Acq On : 15 Oct 2021 13:43
 Operator : JC/MD
 Sample : M4103-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
 Title : VOC Analysis

Signal : TIC: VX024828.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	24	26	32	rVB3	3434	5074	0.55%	0.071%
2	1.368	43	46	55	rVB	100206	91552	9.94%	1.275%
3	1.666	91	95	103	rVB	72467	88793	9.64%	1.237%
4	2.307	194	200	211	rBV	167819	269783	29.28%	3.758%
5	2.508	231	233	238	rVB3	511	642	0.07%	0.009%
6	2.709	264	266	272	rVB	557	730	0.08%	0.010%
7	2.794	275	280	285	rVB2	2457	4220	0.46%	0.059%
8	2.855	289	290	293	rVB	286	128	0.01%	0.002%
9	2.953	301	306	310	rVB4	552	1104	0.12%	0.015%
10	3.020	315	317	319	rBV2	227	179	0.02%	0.002%
11	3.099	327	330	331	rVB2	388	349	0.04%	0.005%
12	3.123	331	334	335	rBV2	267	329	0.04%	0.005%
13	3.337	367	369	371	rBV2	177	157	0.02%	0.002%
14	3.422	381	383	385	rVB2	201	143	0.02%	0.002%
15	3.453	385	388	390	rBV	160	168	0.02%	0.002%
16	3.733	432	434	437	rVB	206	162	0.02%	0.002%
17	3.886	458	459	464	rVV	170	241	0.03%	0.003%
18	4.062	486	488	490	rBV2	142	142	0.02%	0.002%
19	4.294	523	526	528	rBV2	192	267	0.03%	0.004%
20	4.465	544	554	569	rBV	86003	258101	28.02%	3.595%
21	5.062	641	652	671	rBV	116361	376356	40.85%	5.242%
22	5.294	688	690	692	rVB2	237	161	0.02%	0.002%
23	5.391	704	706	714	rVB3	342	636	0.07%	0.009%
24	5.464	714	718	720	rBV2	158	207	0.02%	0.003%
25	5.489	720	722	726	rVB2	182	150	0.02%	0.002%
26	5.562	729	734	739	rVB3	540	1142	0.12%	0.016%
27	5.611	739	742	743	rVB	265	218	0.02%	0.003%
28	5.635	743	746	747	rBV	243	317	0.03%	0.004%
29	5.678	752	753	757	rBV	228	158	0.02%	0.002%
30	5.830	776	778	780	rBV	232	246	0.03%	0.003%
31	5.977	789	802	819	rBV2	312511	921254	100.00%	12.832%
32	6.172	833	834	836	rBV	228	172	0.02%	0.002%
33	6.330	857	860	862	rVB	210	246	0.03%	0.003%
34	6.348	862	863	865	rBV	163	164	0.02%	0.002%
35	6.537	893	894	899	rVB3	246	310	0.03%	0.004%
36	6.763	922	931	947	rBV	235794	565888	61.43%	7.882%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
 Data File : VX024828.D
 Acq On : 15 Oct 2021 13:43
 Operator : JC/MD
 Sample : M4103-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM100721WMA.M
 Title : VOC Analysis

37	7.111	982	988	998	rVB3	5251	12742	1.38%	0.177%
38	7.312	1012	1021	1034	rBV	195472	422578	45.87%	5.886%
39	7.434	1039	1041	1043	rBV3	215	217	0.02%	0.003%
40	7.580	1063	1065	1068	rBV2	151	183	0.02%	0.003%
41	7.665	1077	1079	1080	rBV	160	136	0.01%	0.002%
42	7.714	1085	1087	1089	rVV2	205	164	0.02%	0.002%
43	7.738	1089	1091	1093	rVB2	194	183	0.02%	0.003%
44	7.806	1098	1102	1107	rVB3	359	662	0.07%	0.009%
45	7.927	1118	1122	1128	rBV3	1006	1613	0.18%	0.022%
46	8.001	1131	1134	1137	rBV2	212	173	0.02%	0.002%
47	8.330	1181	1188	1197	rBV	129985	213389	23.16%	2.972%
48	8.470	1207	1211	1216	rVB4	629	902	0.10%	0.013%
49	8.653	1234	1241	1248	rVV	466378	721537	78.32%	10.050%
50	8.720	1249	1252	1259	rVB	6758	10381	1.13%	0.145%
51	8.952	1284	1290	1305	rBV	101715	149510	16.23%	2.082%
52	9.275	1341	1343	1346	rVB3	575	574	0.06%	0.008%
53	9.391	1356	1362	1383	rBV	360190	544222	59.07%	7.580%
54	9.708	1411	1414	1417	rBV3	275	313	0.03%	0.004%
55	9.976	1456	1458	1460	rVB2	175	138	0.01%	0.002%
56	10.000	1460	1462	1465	rBV	208	259	0.03%	0.004%
57	10.055	1465	1471	1485	rVV	510043	687661	74.64%	9.578%
58	10.208	1493	1496	1498	rVB2	502	491	0.05%	0.007%
59	10.305	1508	1512	1517	rBV3	1085	1418	0.15%	0.020%
60	10.384	1523	1525	1527	rBV	172	164	0.02%	0.002%
61	10.573	1554	1556	1558	rBV	345	232	0.03%	0.003%
62	10.653	1562	1569	1575	rBV3	561	1034	0.11%	0.014%
63	10.714	1577	1579	1581	rVB	215	132	0.01%	0.002%
64	10.963	1618	1620	1626	rVB3	296	418	0.05%	0.006%
65	11.085	1638	1640	1642	rVB2	233	222	0.02%	0.003%
66	11.122	1642	1646	1650	rBV3	1514	1850	0.20%	0.026%
67	11.195	1652	1658	1668	rBV	401361	499287	54.20%	6.954%
68	11.463	1697	1702	1703	rBV	557	593	0.06%	0.008%
69	11.598	1723	1724	1726	rBV	202	143	0.02%	0.002%
70	11.683	1736	1738	1741	rVB2	207	162	0.02%	0.002%
71	11.713	1741	1743	1744	rBV	230	130	0.01%	0.002%
72	11.750	1745	1749	1754	rVB4	1613	2338	0.25%	0.033%
73	11.933	1776	1779	1784	rBV3	535	740	0.08%	0.010%
74	11.976	1784	1786	1789	rVV	575	418	0.05%	0.006%
75	12.024	1789	1794	1804	rVV	517219	631982	68.60%	8.803%
76	12.128	1806	1811	1813	rVV4	767	1172	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
 Data File : VX024828.D
 Acq On : 15 Oct 2021 13:43
 Operator : JC/MD
 Sample : M4103-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
 Title : VOC Analysis

77	12.152	1813	1815	1819	rVB2	1231	1169	0.13%	0.016%
78	12.225	1824	1827	1830	rVB2	363	500	0.05%	0.007%
79	12.323	1837	1843	1852	rBV	547178	671696	72.91%	9.356%
80	12.475	1867	1868	1875	rVB3	323	517	0.06%	0.007%
81	12.542	1875	1879	1880	rBV2	191	274	0.03%	0.004%
82	12.634	1892	1894	1895	rBV	224	156	0.02%	0.002%
83	12.664	1896	1899	1904	rVB4	460	689	0.07%	0.010%
84	12.701	1904	1905	1908	rBV	145	126	0.01%	0.002%
85	12.859	1928	1931	1934	rVB2	231	233	0.03%	0.003%
86	13.378	2014	2016	2019	rVB	137	164	0.02%	0.002%
87	13.414	2019	2022	2024	rBV2	224	294	0.03%	0.004%
88	13.439	2024	2026	2031	rVV2	152	187	0.02%	0.003%
89	13.500	2034	2036	2039	rBV	158	155	0.02%	0.002%
90	13.591	2049	2051	2054	rBV2	475	527	0.06%	0.007%
91	13.615	2054	2055	2056	rVB	431	158	0.02%	0.002%
92	13.628	2056	2057	2060	rBV2	129	125	0.01%	0.002%
93	13.780	2079	2082	2084	rVV2	495	527	0.06%	0.007%
94	13.804	2084	2086	2090	rVB2	163	210	0.02%	0.003%
95	13.963	2110	2112	2115	rVB	400	302	0.03%	0.004%
96	14.390	2180	2182	2185	rVB2	260	261	0.03%	0.004%
97	14.420	2185	2187	2188	rBV	209	129	0.01%	0.002%
98	14.609	2215	2218	2220	rBV2	250	275	0.03%	0.004%
99	15.048	2288	2290	2292	rVB	335	191	0.02%	0.003%
100	15.268	2324	2326	2328	rBV2	233	199	0.02%	0.003%




Sum of corrected areas: 7179416

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
Data File : VX024828.D
Acq On : 15 Oct 2021 13:43
Operator : JC/MD
Sample : M4103-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM100721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

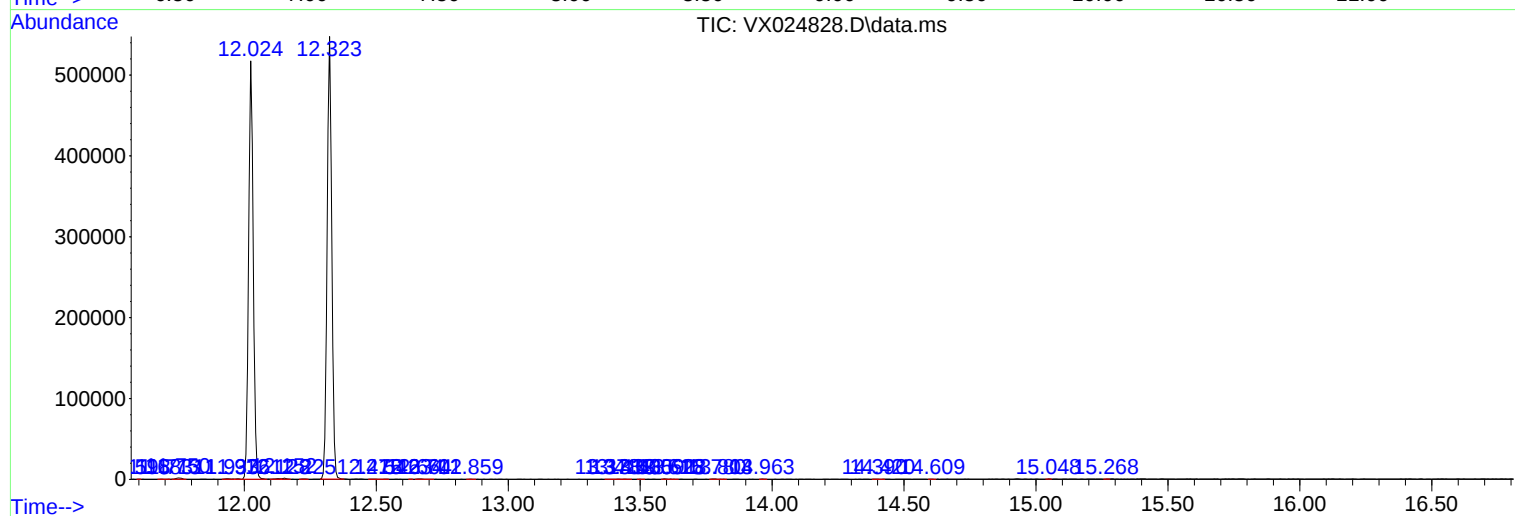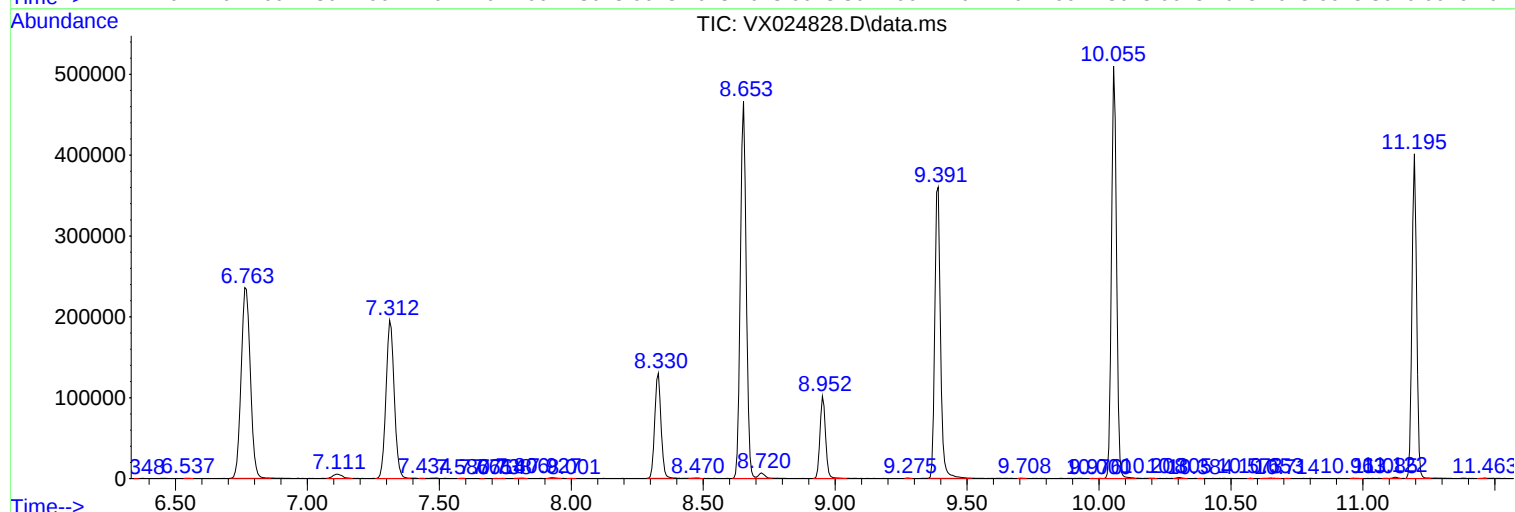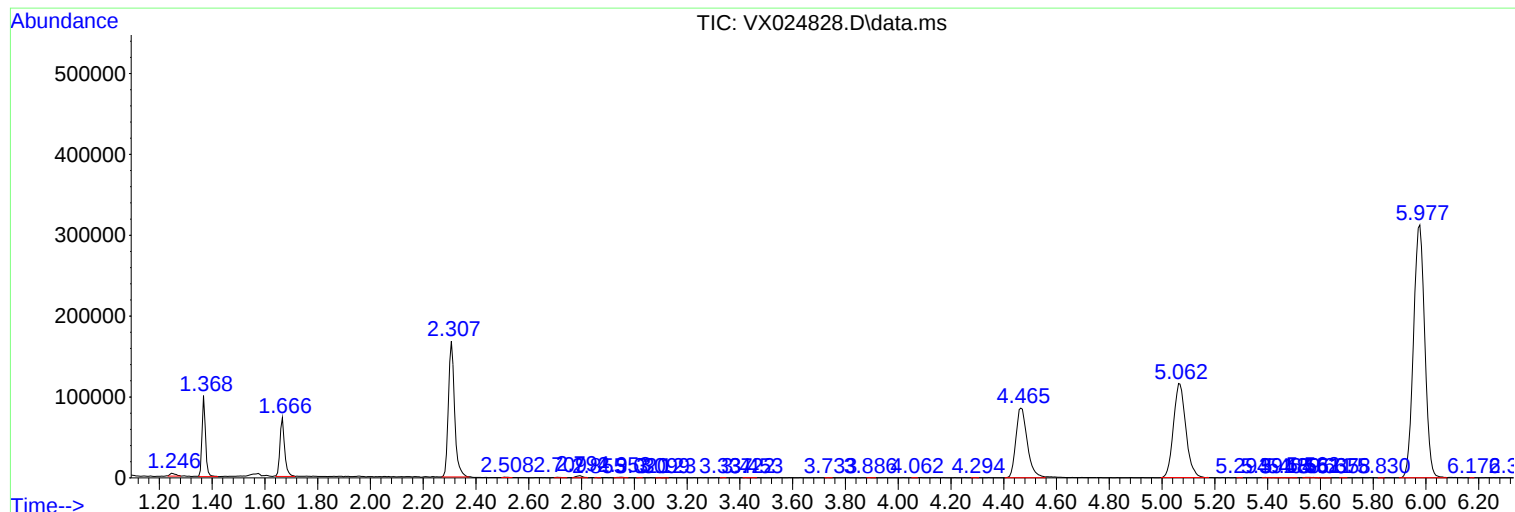

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
Data File : VX024828.D
Acq On : 15 Oct 2021 13:43
Operator : JC/MD
Sample : M4103-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
Data File : VX024828.D
Acq On : 15 Oct 2021 13:43
Operator : JC/MD
Sample : M4103-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
