
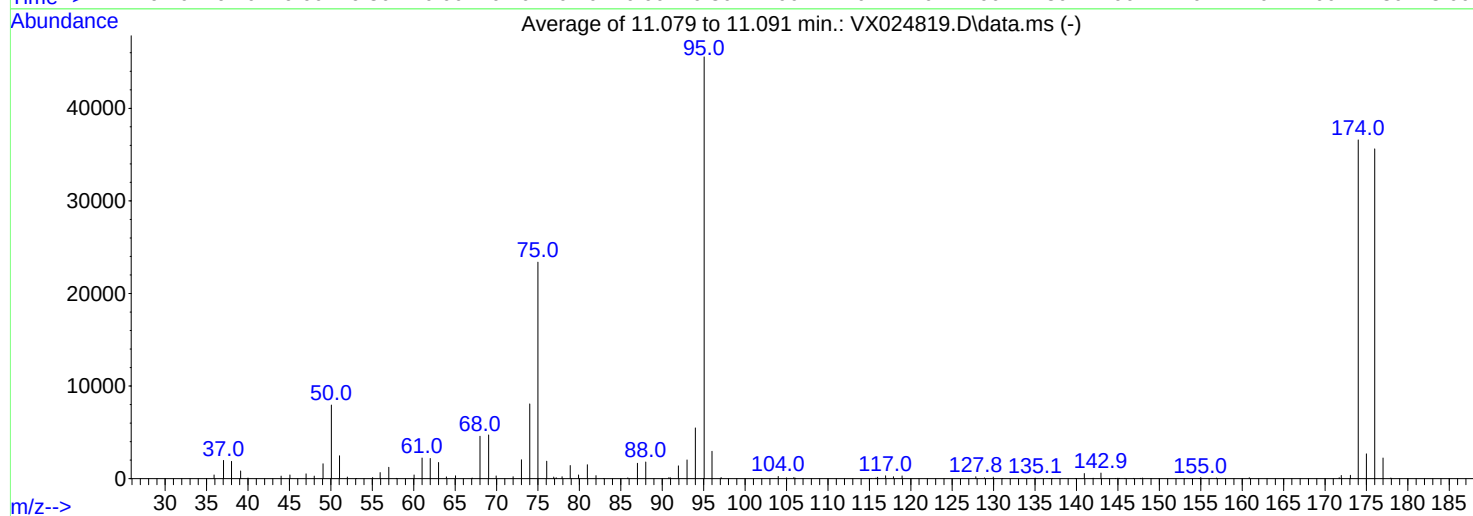


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX101521\  
 Data File : VX024819.D  
 Acq On : 14 Oct 2021 17:30  
 Operator : JC/MD  
 Sample : BFB604  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB604

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXLM100721WMA.M  
 Title : VOC Analysis  
 Last Update : Wed Oct 20 14:52:57 2021

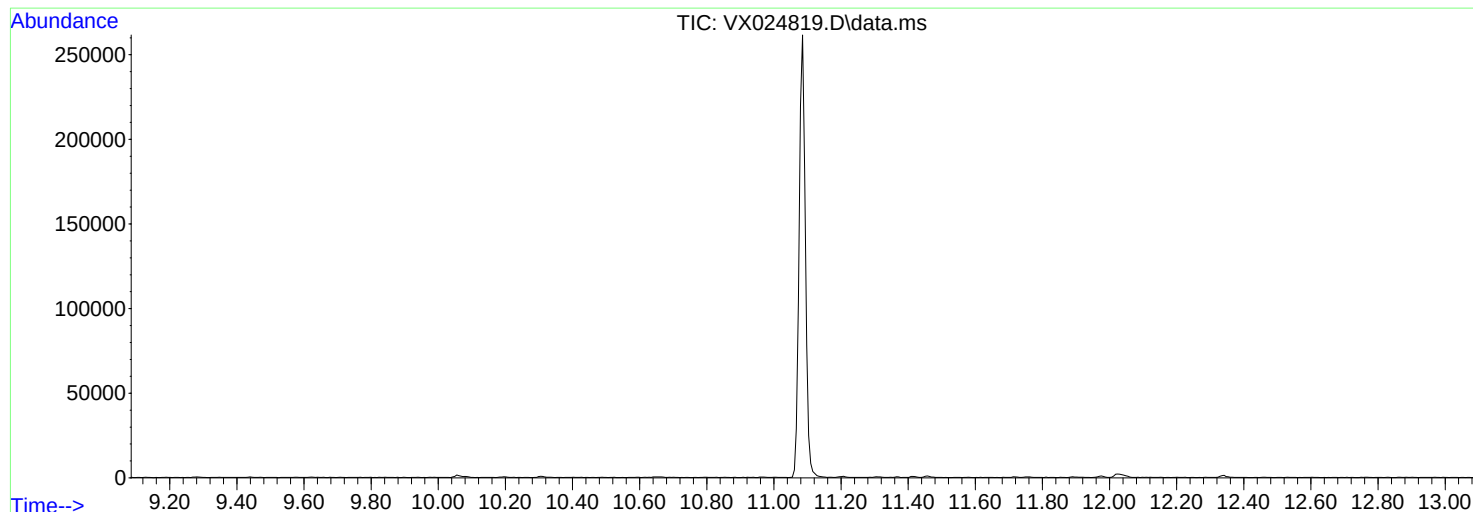

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 17.4         | 7949       | PASS                |
| 75             | 95              | 30              | 80              | 51.3         | 23392      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 45560      | PASS                |
| 96             | 95              | 5               | 9               | 6.5          | 2960       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.0          | 370        | PASS                |
| 174            | 95              | 50              | 120             | 80.3         | 36597      | PASS                |
| 175            | 174             | 5               | 9               | 7.3          | 2686       | PASS                |
| 176            | 174             | 95              | 101             | 97.3         | 35627      | PASS                |
| 177            | 176             | 5               | 9               | 6.3          | 2237       | PASS                |

| m/z   | Abundance |
|-------|-----------|
| 40.10 | 80.0      |
| 44.10 | 116.0     |

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB604

| m/z    | Abundance |
|--------|-----------|
| 35.90  | 473.0     |
| 37.10  | 2327.0    |
| 38.00  | 2033.0    |
| 39.10  | 907.0     |
| 40.00  | 130.0     |
| 44.00  | 444.0     |
| 45.10  | 545.0     |
| 47.00  | 569.0     |
| 48.00  | 320.0     |
| 49.10  | 1732.0    |
| 50.10  | 9153.0    |
| 51.00  | 2782.0    |
| 52.00  | 178.0     |
| 55.00  | 154.0     |
| 55.90  | 780.0     |
| 57.00  | 1419.0    |
| 60.00  | 433.0     |
| 61.00  | 2310.0    |
| 62.00  | 2307.0    |
| 63.00  | 2051.0    |
| 63.90  | 232.0     |
| 65.00  | 300.0     |
| 68.00  | 5158.0    |
| 69.00  | 5196.0    |
| 69.90  | 286.0     |
| 72.00  | 209.0     |
| 73.00  | 2143.0    |
| 74.00  | 8229.0    |
| 75.00  | 24744.0   |
| 76.00  | 2121.0    |
| 77.20  | 336.0     |
| 77.90  | 134.0     |
| 78.90  | 1590.0    |
| 79.90  | 394.0     |
| 81.00  | 1577.0    |
| 82.00  | 303.0     |
| 82.90  | 50.0      |
| 85.80  | 88.0      |
| 87.10  | 1741.0    |
| 88.00  | 2024.0    |
| 90.80  | 214.0     |
| 92.00  | 1519.0    |
| 93.00  | 2098.0    |
| 94.00  | 5500.0    |
| 95.10  | 46512.0   |
| 96.00  | 3200.0    |
| 97.00  | 72.0      |
| 104.10 | 207.0     |
| 105.00 | 71.0      |
| 106.00 | 204.0     |
| 115.80 | 237.0     |
| 116.90 | 341.0     |
| 117.90 | 256.0     |
| 118.90 | 272.0     |
| 127.80 | 178.0     |
| 128.90 | 74.0      |
| 130.00 | 127.0     |
| 131.10 | 58.0      |
| 134.90 | 114.0     |
| 137.10 | 64.0      |
| 141.00 | 624.0     |
| 142.00 | 60.0      |
| 142.90 | 625.0     |
| 145.00 | 150.0     |
| 148.00 | 59.0      |
| 153.00 | 51.0      |
| 154.80 | 76.0      |
| 156.90 | 87.0      |
| 160.80 | 67.0      |
| 171.90 | 275.0     |
| 173.10 | 371.0     |
| 174.00 | 32208.0   |
| 175.00 | 2227.0    |
| 176.00 | 31568.0   |
| 177.00 | 1802.0    |
| 177.90 | 60.0      |

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB604

| m/z    | Abundance |
|--------|-----------|
| 35.90  | 413.0     |
| 37.00  | 2253.0    |
| 38.00  | 2231.0    |
| 39.10  | 990.0     |
| 40.10  | 135.0     |
| 44.00  | 437.0     |
| 45.00  | 412.0     |
| 47.10  | 599.0     |
| 48.00  | 335.0     |
| 49.10  | 1877.0    |
| 50.00  | 8864.0    |
| 51.10  | 2861.0    |
| 52.00  | 244.0     |
| 53.10  | 59.0      |
| 55.10  | 129.0     |
| 56.00  | 636.0     |
| 57.00  | 1415.0    |
| 57.90  | 58.0      |
| 60.00  | 398.0     |
| 61.00  | 2849.0    |
| 62.00  | 2629.0    |
| 63.00  | 1901.0    |
| 64.00  | 233.0     |
| 65.10  | 360.0     |
| 67.00  | 124.0     |
| 68.00  | 5231.0    |
| 69.00  | 5367.0    |
| 70.00  | 346.0     |
| 72.10  | 250.0     |
| 73.00  | 2609.0    |
| 74.00  | 9961.0    |
| 75.00  | 27128.0   |
| 76.10  | 2107.0    |
| 76.90  | 351.0     |
| 78.00  | 270.0     |
| 78.90  | 1577.0    |
| 79.90  | 538.0     |
| 80.90  | 1762.0    |
| 82.00  | 437.0     |
| 85.80  | 86.0      |
| 86.90  | 1761.0    |
| 88.00  | 2214.0    |
| 91.00  | 260.0     |
| 91.90  | 1655.0    |
| 93.00  | 2377.0    |
| 94.00  | 6812.0    |
| 95.00  | 53240.0   |
| 96.00  | 3411.0    |
| 97.10  | 216.0     |
| 104.00 | 296.0     |
| 105.00 | 94.0      |
| 105.80 | 228.0     |
| 107.00 | 63.0      |
| 115.20 | 62.0      |
| 116.00 | 294.0     |
| 116.90 | 354.0     |
| 117.80 | 182.0     |
| 119.00 | 390.0     |
| 127.90 | 253.0     |
| 128.90 | 96.0      |
| 130.00 | 193.0     |
| 135.10 | 99.0      |
| 136.80 | 73.0      |
| 140.90 | 664.0     |
| 142.00 | 109.0     |
| 143.00 | 671.0     |
| 144.70 | 82.0      |
| 145.20 | 105.0     |
| 145.80 | 64.0      |
| 146.90 | 56.0      |
| 147.80 | 87.0      |
| 148.10 | 90.0      |
| 155.00 | 234.0     |
| 156.90 | 101.0     |
| 160.90 | 123.0     |
| 172.00 | 424.0     |
| 172.90 | 385.0     |
| 174.00 | 44056.0   |
| 175.00 | 3459.0    |
| 176.00 | 42736.0   |
| 177.00 | 3031.0    |
| 177.90 | 88.0      |

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB604

| m/z    | Abundance |
|--------|-----------|
| 36.00  | 283.0     |
| 37.00  | 1314.0    |
| 38.00  | 1336.0    |
| 39.00  | 593.0     |
| 39.90  | 169.0     |
| 44.00  | 289.0     |
| 45.00  | 236.0     |
| 46.90  | 384.0     |
| 47.90  | 161.0     |
| 49.00  | 1234.0    |
| 50.00  | 5829.0    |
| 51.00  | 1792.0    |
| 51.90  | 101.0     |
| 55.10  | 103.0     |
| 56.00  | 568.0     |
| 57.00  | 873.0     |
| 57.90  | 56.0      |
| 60.10  | 361.0     |
| 60.90  | 1508.0    |
| 62.10  | 1599.0    |
| 63.00  | 1289.0    |
| 63.90  | 112.0     |
| 65.00  | 295.0     |
| 67.10  | 87.0      |
| 68.00  | 3365.0    |
| 69.10  | 3604.0    |
| 69.90  | 237.0     |
| 71.90  | 181.0     |
| 73.00  | 1346.0    |
| 74.00  | 6054.0    |
| 75.00  | 18304.0   |
| 76.00  | 1449.0    |
| 76.90  | 189.0     |
| 77.80  | 196.0     |
| 78.90  | 1096.0    |
| 80.00  | 238.0     |
| 80.90  | 1155.0    |
| 81.90  | 237.0     |
| 85.90  | 71.0      |
| 87.00  | 1503.0    |
| 88.00  | 1170.0    |
| 90.80  | 178.0     |
| 92.00  | 1000.0    |
| 93.00  | 1613.0    |
| 94.00  | 4125.0    |
| 95.00  | 36928.0   |
| 96.00  | 2270.0    |
| 97.10  | 97.0      |
| 103.90 | 229.0     |
| 105.00 | 80.0      |
| 106.10 | 151.0     |
| 116.00 | 165.0     |
| 117.00 | 261.0     |
| 118.00 | 178.0     |
| 118.90 | 220.0     |
| 127.90 | 168.0     |
| 128.90 | 101.0     |
| 129.90 | 204.0     |
| 135.00 | 83.0      |
| 139.90 | 64.0      |
| 141.00 | 370.0     |
| 143.00 | 543.0     |
| 145.90 | 50.0      |
| 146.90 | 62.0      |
| 147.70 | 94.0      |
| 149.00 | 64.0      |
| 155.00 | 119.0     |
| 160.90 | 110.0     |
| 171.70 | 318.0     |
| 172.00 | 335.0     |
| 173.10 | 353.0     |
| 174.00 | 33528.0   |
| 175.00 | 2371.0    |
| 176.00 | 32576.0   |
| 177.00 | 1879.0    |
| 178.00 | 77.0      |

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB604