
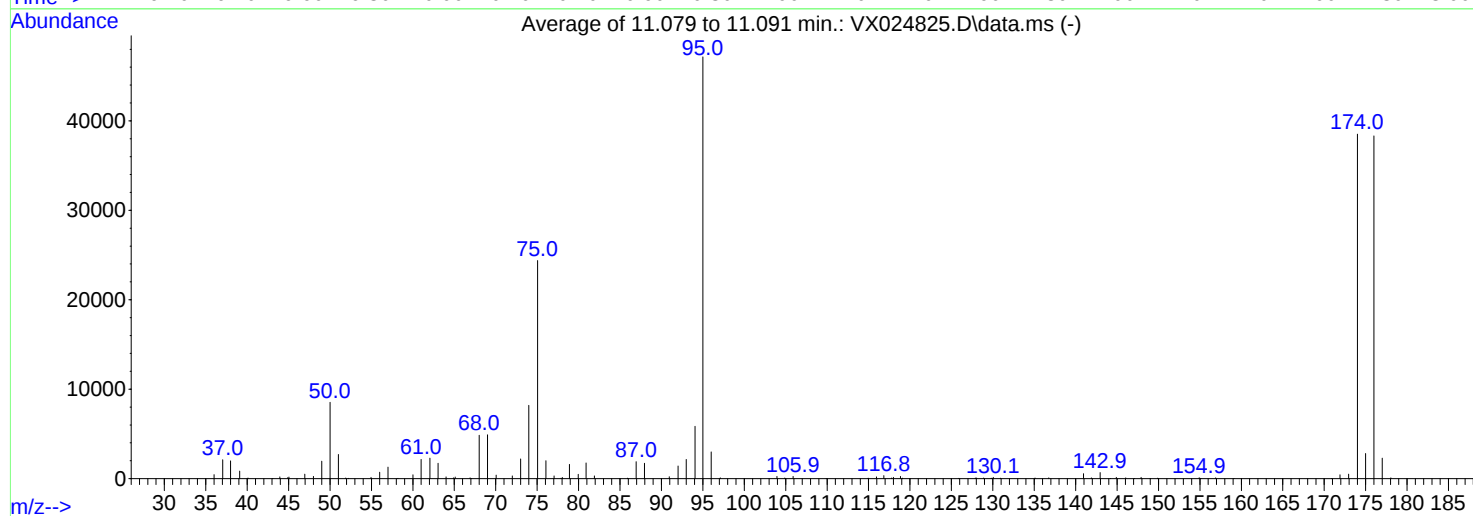


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101521\
 Data File : VX024825.D
 Acq On : 15 Oct 2021 09:58
 Operator : JC/MD
 Sample : BFB605
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB605

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM100721WMA.M
 Title : VOC Analysis
 Last Update : Wed Oct 20 14:52:57 2021

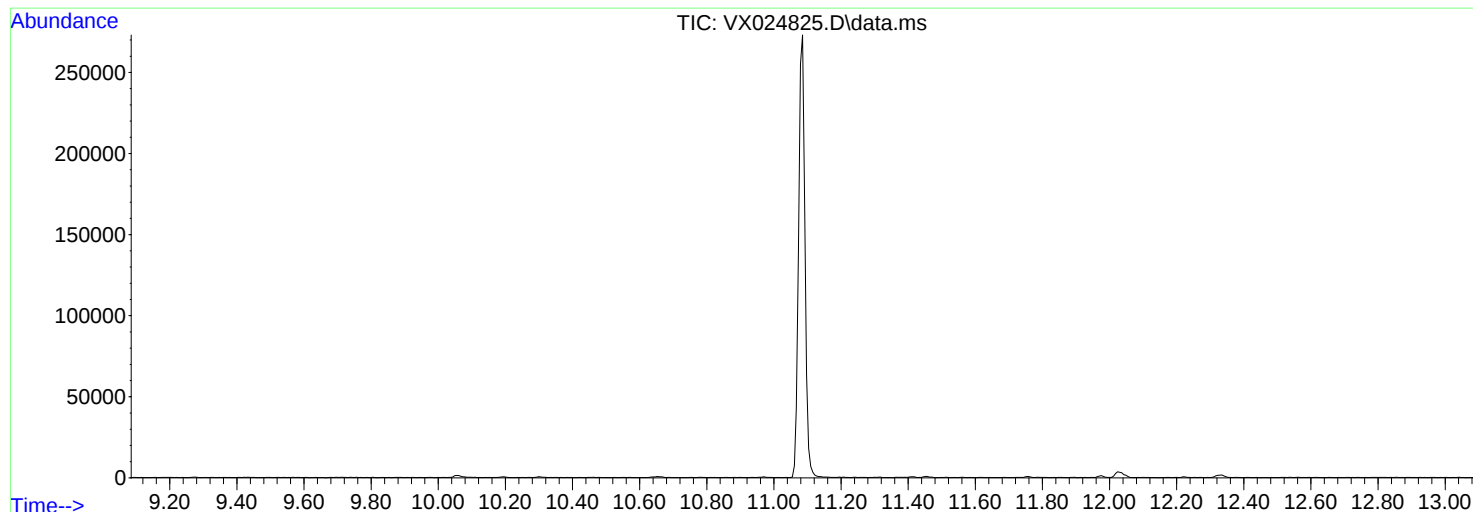

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	8526	PASS
75	95	30	80	51.7	24384	PASS
95	95	100	100	100.0	47157	PASS
96	95	5	9	6.3	2990	PASS
173	174	0.00	2	1.3	510	PASS
174	95	50	120	81.7	38517	PASS
175	174	5	9	7.3	2813	PASS
176	174	95	101	99.5	38312	PASS
177	176	5	9	6.0	2289	PASS

m/z	Abundance
39.90	84.0
44.10	137.0

Instrument :
MSVOA_X
ClientSampleId :
BFB605

m/z	Abundance
36.00	585.0
37.10	2575.0
38.00	2450.0
39.10	1047.0
39.90	61.0
43.10	64.0
44.00	366.0
44.90	404.0
47.00	636.0
48.10	311.0
49.00	2302.0
50.00	10193.0
51.00	3364.0
51.90	134.0
55.00	172.0
56.00	839.0
57.00	1587.0
60.00	477.0
61.00	2455.0
62.10	2811.0
63.00	2334.0
64.00	296.0
64.90	258.0
66.90	98.0
68.00	5386.0
69.00	5395.0
70.00	460.0
72.00	269.0
73.00	2616.0
74.00	9810.0
75.00	28808.0
76.00	2454.0
77.00	295.0
77.90	137.0
78.90	1754.0
79.90	627.0
80.90	2228.0
81.80	282.0
86.90	2282.0
88.00	1996.0
90.90	244.0
92.10	1774.0
93.00	2628.0
94.00	6328.0
95.00	53968.0
96.00	3405.0
97.10	110.0
104.00	286.0
104.80	68.0
105.90	347.0
109.90	65.0
114.90	67.0
116.10	275.0
116.90	431.0
117.80	215.0
119.00	275.0
127.90	219.0
129.00	92.0
129.80	189.0
135.10	84.0
136.70	69.0
141.10	654.0
141.90	120.0
143.00	709.0
144.90	188.0
146.10	80.0
147.10	51.0
148.00	151.0
149.00	67.0
149.90	83.0
155.00	137.0
170.90	53.0
171.90	431.0
172.90	440.0
174.00	37816.0
175.00	3007.0
176.00	37208.0
177.00	2094.0
178.00	110.0

Instrument :
MSVOA_X
ClientSampleId :
BFB605

m/z	Abundance
36.00	575.0
37.00	2690.0
38.00	2053.0
39.10	973.0
40.10	137.0
43.90	362.0
45.10	302.0
47.00	588.0
47.90	289.0
49.00	2116.0
50.00	10242.0
51.00	3140.0
51.90	104.0
54.90	146.0
56.00	765.0
57.00	1615.0
60.00	440.0
61.00	2500.0
62.00	2622.0
63.10	1752.0
64.00	162.0
65.10	356.0
66.90	188.0
68.00	5830.0
69.00	5915.0
70.10	531.0
72.00	427.0
73.00	2502.0
74.00	9499.0
75.10	27944.0
76.10	2339.0
77.10	301.0
78.10	275.0
78.90	1962.0
80.00	455.0
80.90	1916.0
81.90	415.0
85.90	83.0
87.00	2254.0
87.90	1951.0
90.90	205.0
92.00	1612.0
93.00	2242.0
94.10	6669.0
95.00	55480.0
96.00	3744.0
97.10	91.0
103.90	277.0
104.90	91.0
105.90	227.0
115.00	78.0
115.90	202.0
116.80	341.0
118.00	211.0
118.80	503.0
125.90	96.0
128.10	131.0
128.80	107.0
130.00	292.0
130.90	79.0
135.10	121.0
136.80	104.0
140.90	541.0
141.90	77.0
142.90	727.0
144.20	69.0
144.90	134.0
146.00	118.0
147.90	182.0
149.90	79.0
154.80	199.0
156.90	120.0
159.10	52.0
172.00	523.0
173.00	672.0
174.00	46656.0
175.00	3342.0
176.00	44960.0
177.00	2905.0
178.10	106.0

Instrument :
MSVOA_X
ClientSampleId :
BFB605

m/z	Abundance
36.00	190.0
37.10	1074.0
38.10	1436.0
39.00	513.0
40.10	101.0
44.00	289.0
45.00	263.0
46.80	280.0
48.00	144.0
49.00	1414.0
50.00	5142.0
51.10	1601.0
52.20	99.0
55.00	122.0
56.00	525.0
57.10	682.0
58.20	86.0
60.00	366.0
61.10	1504.0
62.00	1447.0
63.00	1065.0
64.00	135.0
65.10	194.0
67.10	78.0
68.00	3328.0
69.00	3405.0
70.10	204.0
71.90	209.0
73.00	1502.0
74.00	5292.0
75.00	16400.0
76.00	1239.0
77.10	320.0
78.00	125.0
79.00	1087.0
79.90	390.0
80.90	1101.0
82.00	226.0
85.90	57.0
87.00	1155.0
88.00	1229.0
91.00	219.0
91.90	867.0
93.00	1591.0
94.00	4557.0
95.00	32024.0
96.00	1821.0
97.10	75.0
104.00	187.0
105.00	50.0
106.00	178.0
115.80	141.0
116.80	276.0
118.00	203.0
119.10	152.0
128.00	111.0
130.10	136.0
131.00	68.0
136.80	74.0
140.80	483.0
141.80	59.0
143.00	596.0
144.90	85.0
146.00	50.0
147.80	113.0
155.10	86.0
156.90	129.0
171.80	320.0
173.00	418.0
174.00	31080.0
175.10	2090.0
176.00	32768.0
177.00	1867.0
178.10	78.0

Instrument :
MSVOA_X
ClientSampleId :
BFB605