
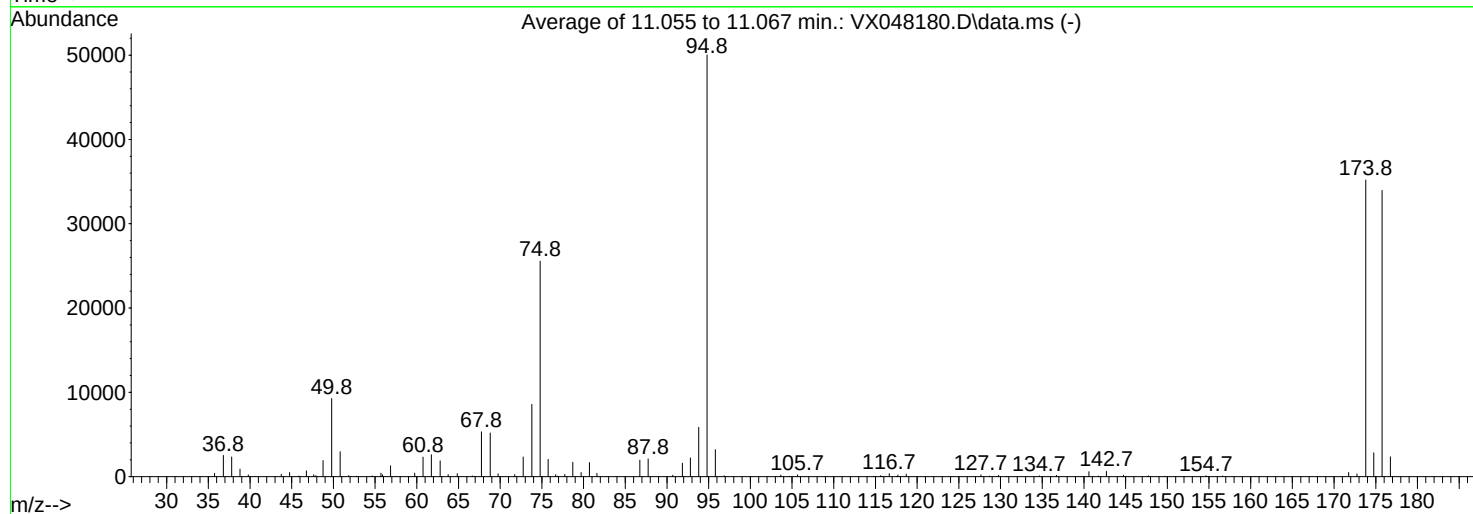


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101525\
Data File : VX048180.D
Acq On : 15 Oct 2025 08:41
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Title : SW846 8260
Last Update : Wed Sep 17 06:39:58 2025

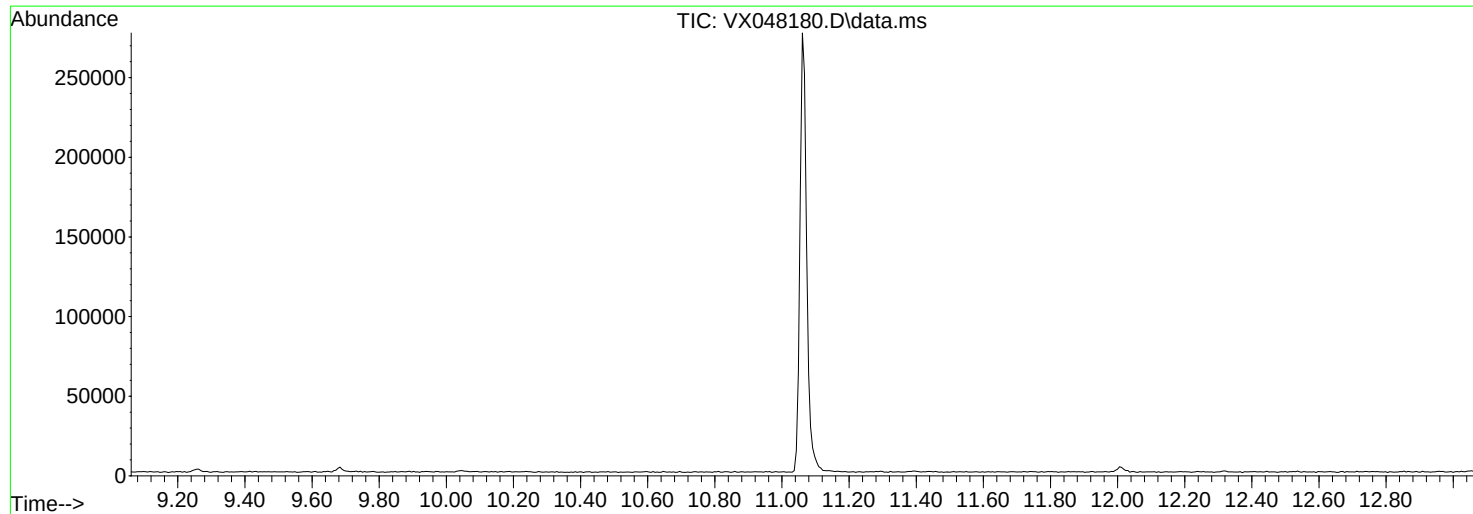

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	9261	PASS
75	95	30	60	51.1	25563	PASS
95	95	100	100	100.0	50037	PASS
96	95	5	9	6.4	3211	PASS
173	174	0.00	2	0.9	318	PASS
174	95	50	100	70.3	35184	PASS
175	174	5	9	8.0	2829	PASS
176	174	95	101	96.5	33955	PASS
177	176	5	9	6.9	2359	PASS