


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX101619\
Data File : VX013084.D
Acq On : 16 Oct 2019 09:26
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X101619W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Oct 17 03:05:35 2019

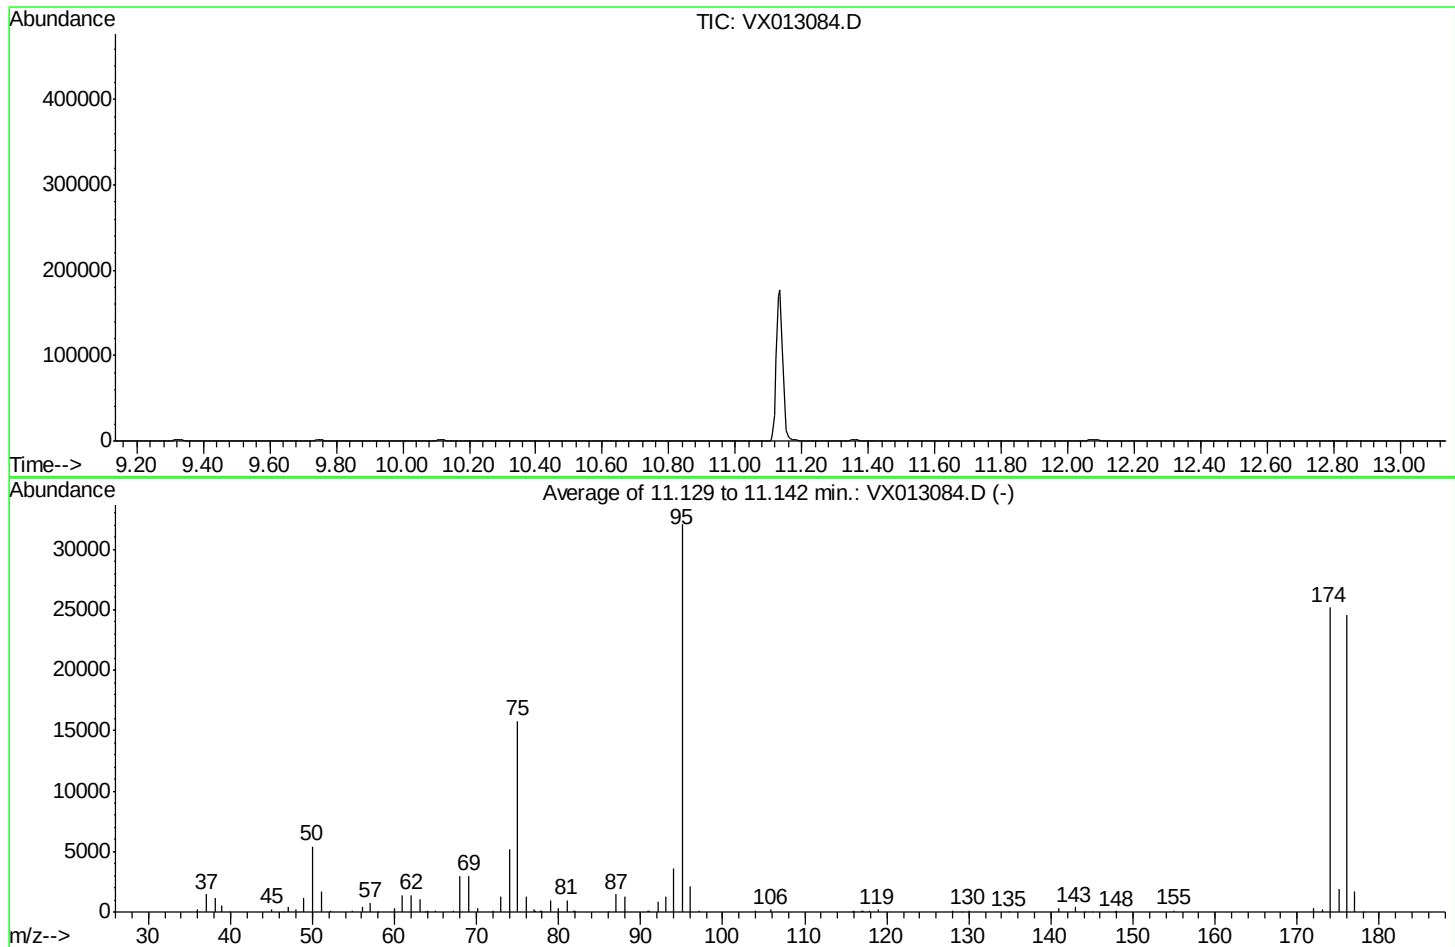

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1674

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	5444	PASS
75	95	30	60	49.3	15803	PASS
95	95	100	100	100.0	32069	PASS
96	95	5	9	6.5	2072	PASS
173	174	0.00	2	1.0	241	PASS
174	95	50	100	78.5	25189	PASS
175	174	5	9	7.4	1861	PASS
176	174	95	101	97.5	24568	PASS
177	176	5	9	6.8	1667	PASS