
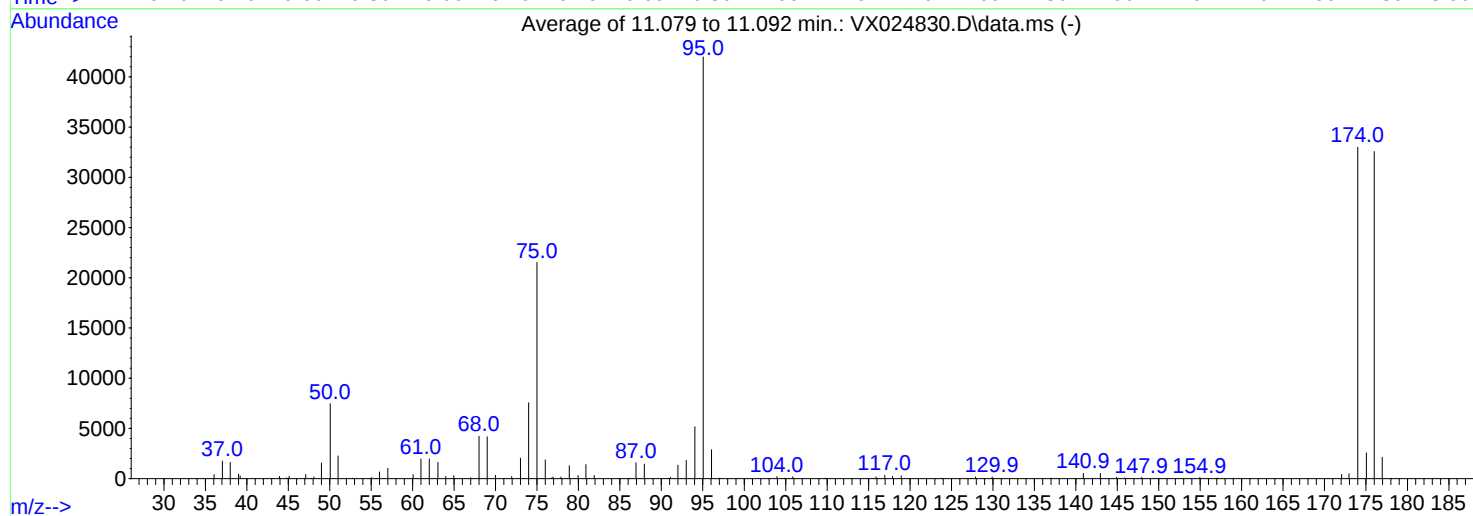


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101621\
 Data File : VX024830.D
 Acq On : 15 Oct 2021 15:18
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101321W.M
 Title : SW846 8260
 Last Update : Thu Oct 14 03:51:38 2021

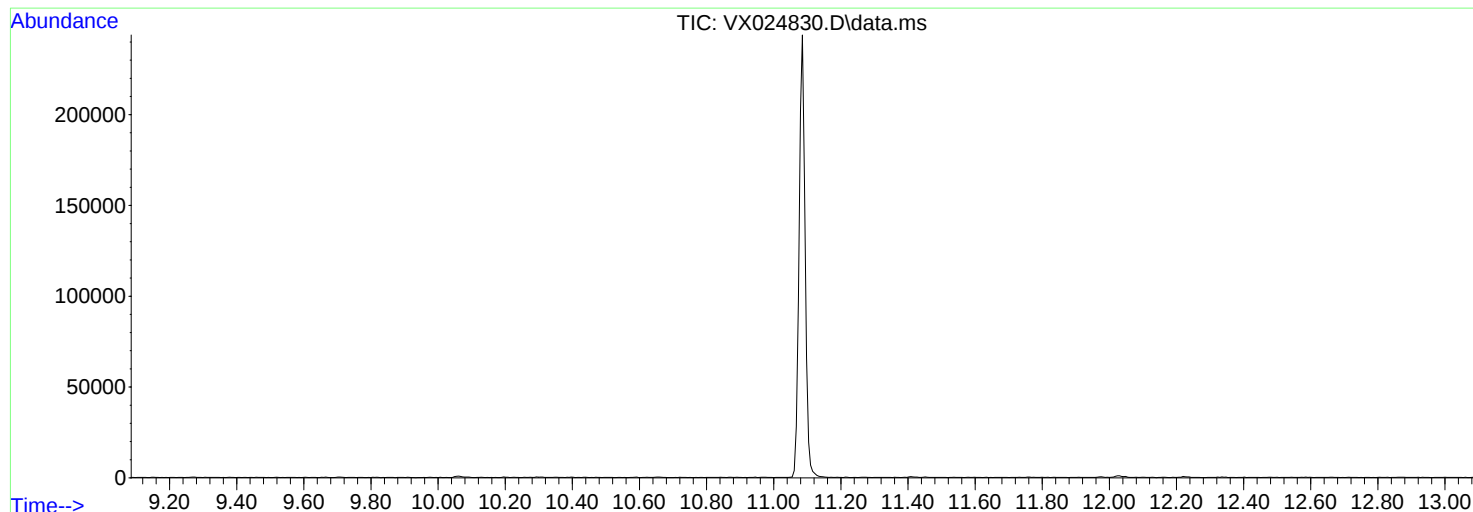

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	7459	PASS
75	95	30	60	51.2	21522	PASS
95	95	100	100	100.0	41995	PASS
96	95	5	9	6.9	2882	PASS
173	174	0.00	2	1.5	483	PASS
174	95	50	100	78.6	32995	PASS
175	174	5	9	7.8	2572	PASS
176	174	95	101	98.7	32565	PASS
177	176	5	9	6.5	2121	PASS