


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX101718\  
Data File : VX005377.D  
Acq On : 17 Oct 2018 07:32  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X101218W.M  
Title : SW846 8260  
Last Update : Fri Oct 12 11:28:43 2018

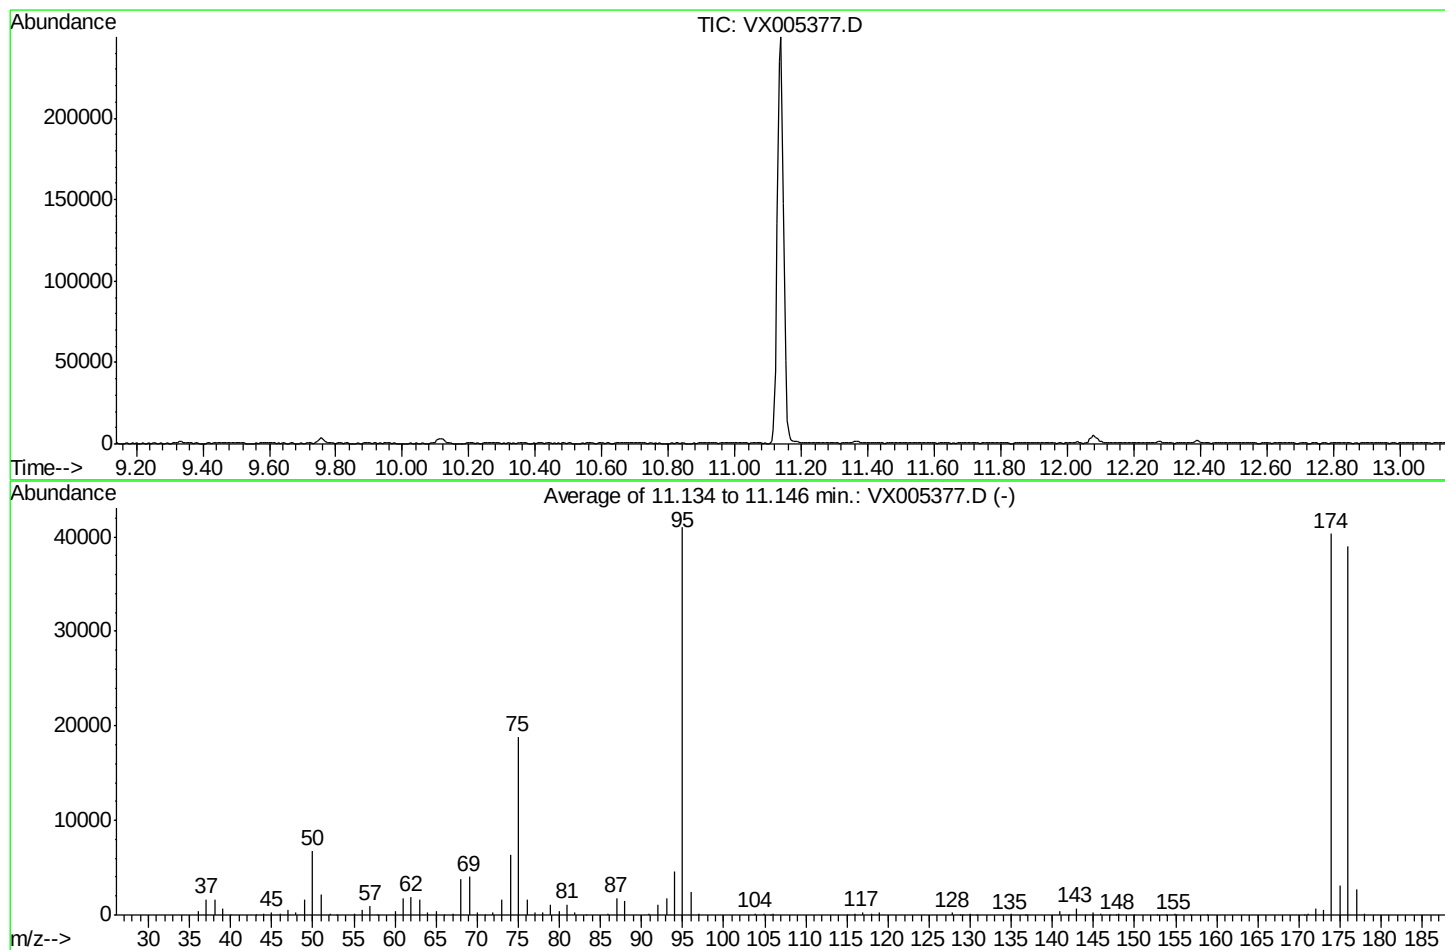

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1630

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 16.6      | 6803    | PASS             |
| 75          | 95           | 30           | 60           | 45.9      | 18821   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 41002   | PASS             |
| 96          | 95           | 5            | 9            | 6.1       | 2494    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.3       | 524     | PASS             |
| 174         | 95           | 50           | 100          | 98.3      | 40320   | PASS             |
| 175         | 174          | 5            | 9            | 7.6       | 3065    | PASS             |
| 176         | 174          | 95           | 101          | 96.8      | 39029   | PASS             |
| 177         | 176          | 5            | 9            | 7.0       | 2715    | PASS             |