

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101722\
 Data File : VX032166.D
 Acq On : 17 Oct 2022 20:09
 Operator : JC/MD
 Sample : PB148361TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB148361TB

Quant Time: Oct 18 04:24:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 18 04:18:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	101589	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	222684	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	202953	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	91862	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	106779	65.994	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 131.980%#			
35) Dibromofluoromethane	5.385	113	57506	37.847	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 75.700%			
50) Toluene-d8	8.647	98	279663	52.475	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 104.960%			
62) 4-Bromofluorobenzene	11.079	95	102624	50.576	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 101.160%			
Target Compounds					Qvalue	
3) Chloromethane	1.295	50	223	0.206	ug/l	96
5) Bromomethane	1.618	94	670	0.752	ug/l	91
6) Chloroethane	1.697	64	213	0.238	ug/l #	43
10) Methyl Iodide	2.459	142	385	0.358	ug/l #	81
11) Tert butyl alcohol	2.947	59	3178	14.281	ug/l #	73
16) Acetone	2.386	43	11496	29.550	ug/l	93
17) Carbon Disulfide	2.514	76	810	0.389	ug/l #	75
18) Methyl Acetate	2.715	43	687	0.434	ug/l	98
20) Methylene Chloride	2.788	84	4085	3.415	ug/l	93
25) 2-Butanone	4.580	43	1215	1.462	ug/l	93
29) Tetrahydrofuran	5.038	42	494	0.991	ug/l #	56
31) Cyclohexane	5.556	56	2422	1.343	ug/l #	22
36) 1,1-Dichloropropene	5.550	75	7927	3.606	ug/l #	50
37) Ethyl Acetate	4.727	43	14201	6.438	ug/l	99
38) Carbon Tetrachloride	5.550	117	10648	4.574	ug/l #	17
43) Isopropyl Acetate	6.342	43	87147	26.216	ug/l	99
48) Methyl methacrylate	7.799	41	86084	51.097	ug/l #	45
49) 1,4-Dioxane	7.799	88	97	2.808	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	76597	37.576	ug/l #	49
53) t-1,3-Dichloropropene	8.952	75	700	0.358	ug/l #	44
54) cis-1,3-Dichloropropene	8.549	75	33032	14.385	ug/l #	68
57) 1,3-Dichloropropane	9.482	76	4466	1.713	ug/l #	43
59) 2-Hexanone	9.482	43	62359	41.293	ug/l #	51
74) N-amyl acetate	10.640	43	22490	9.249	ug/l #	52
76) 1,2,3-Trichloropropane	11.079	75	57143	28.689	ug/l #	36
81) trans-1,4-Dichloro-2-b...	11.079	75	57143	110.443	ug/l #	11
93) 1,2,4-Trichlorobenzene	13.597	180	503	0.290	ug/l	93
94) Hexachlorobutadiene	13.719	225	316	0.435	ug/l	78
95) Naphthalene	13.780	128	1309	0.226	ug/l #	96
96) 1,2,3-Trichlorobenzene	13.963	180	477	0.275	ug/l	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101722\
Data File : VX032166.D
Acq On : 17 Oct 2022 20:09
Operator : JC/MD
Sample : PB148361TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB148361TB

Quant Time: Oct 18 04:24:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101722W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 18 04:18:35 2022
Response via : Initial Calibration




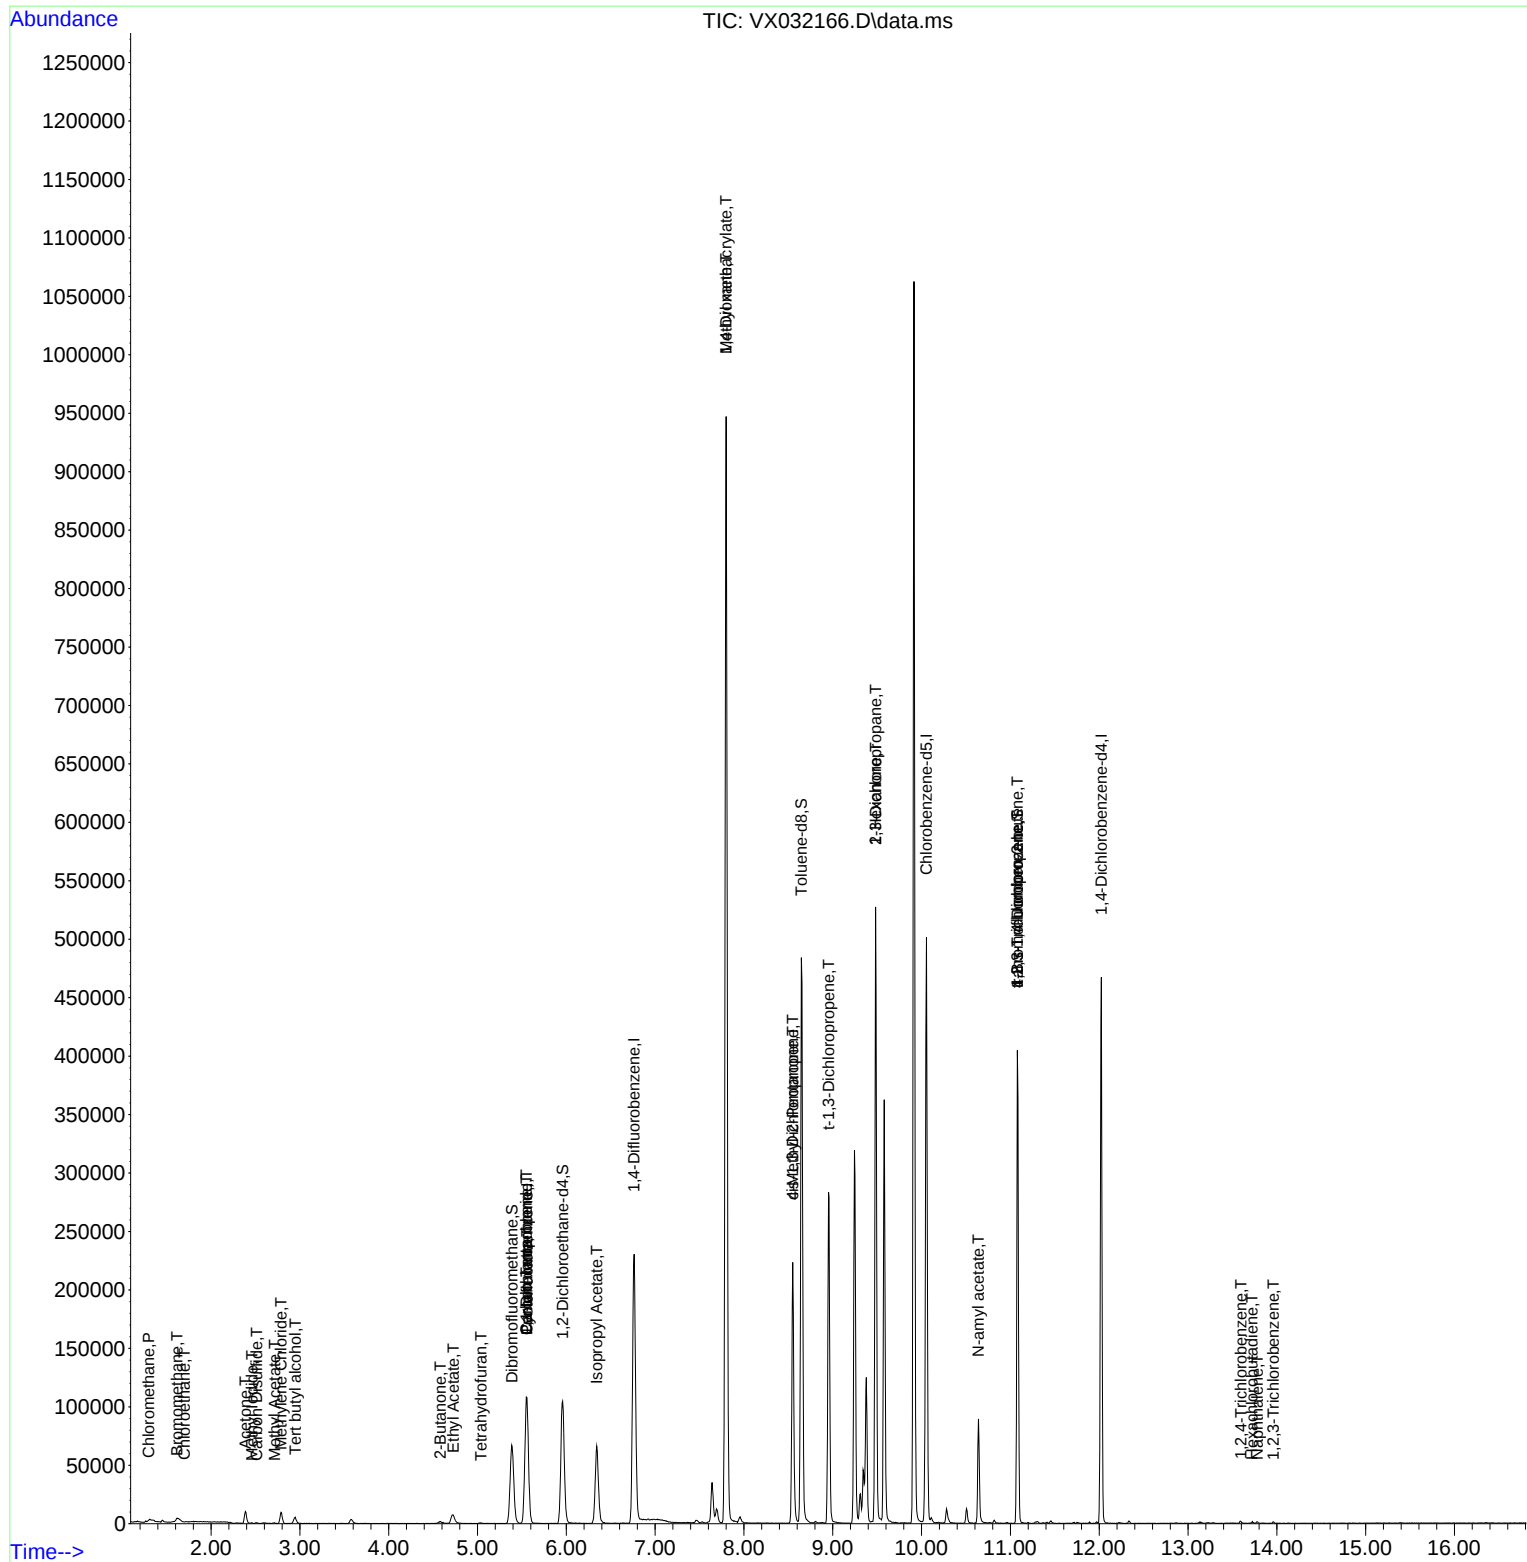




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09




Instrument :
MSVOA_X
ClientSampleId :
PB148361TB

Tgt Ion:168 Resp: 101589
Ion Ratio Lower Upper
168 100
99 57.2 48.8 73.2


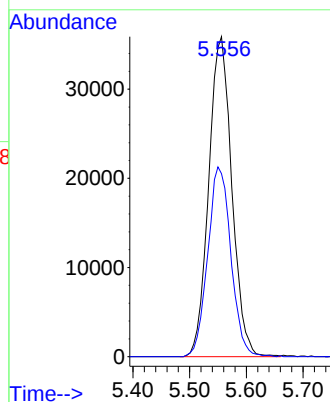
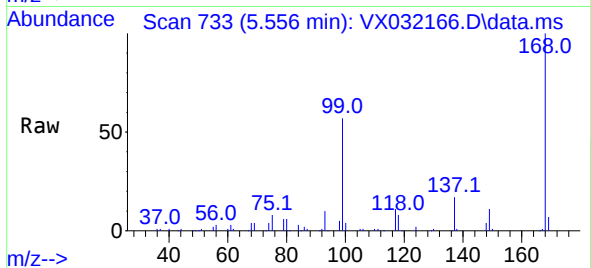


#3
Chloromethane
Concen: 0.206 ug/l
RT: 1.295 min Scan# 34
Delta R.T. 0.006 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09

Tgt Ion: 50 Resp: 223
Ion Ratio Lower Upper
50 100
52 35.8 26.9 40.3

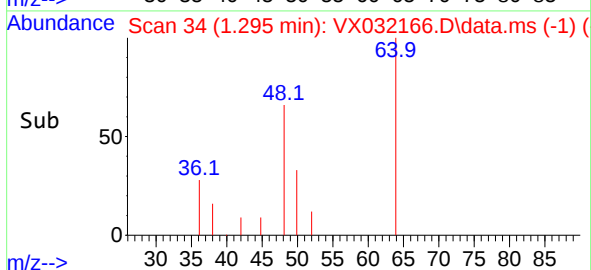

Abundance Scan 86 (1.612 min): VX032159.D\data.ms (-80)

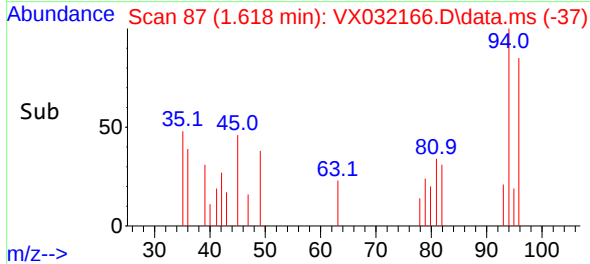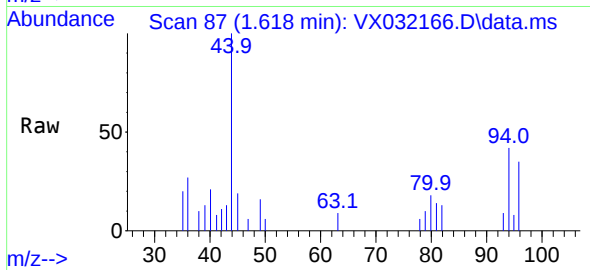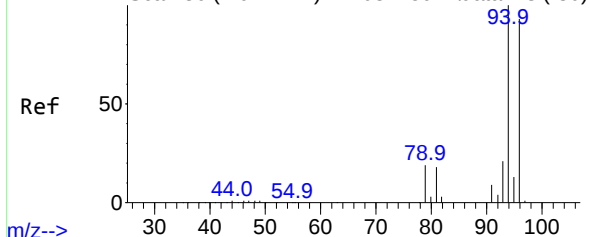

#5

Bromomethane

Concen: 0.752 ug/l

RT: 1.618 min Scan# 81

Delta R.T. 0.006 min

Lab File: VX032166.D

Acq: 17 Oct 2022 20:09

Instrument :

MSVOA_X

ClientSampleId :


PB148361TB

Tgt Ion: 94 Resp: 670




Ion Ratio Lower Upper

94 100

96 84.6 74.4 111.6



Abundance Scan 98 (1.685 min): VX032159.D\data.ms (-92)

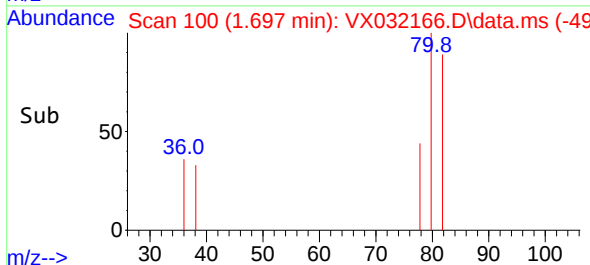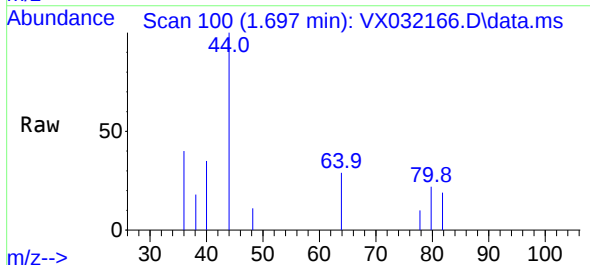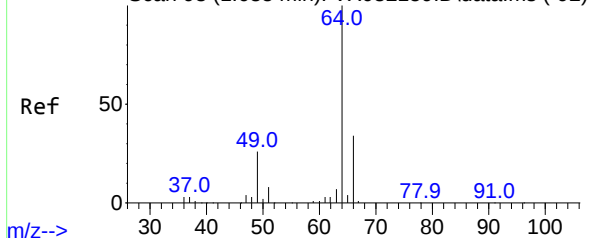

#6

Chloroethane

Concen: 0.238 ug/l

RT: 1.697 min Scan# 100

Delta R.T. 0.012 min

Lab File: VX032166.D


Acq: 17 Oct 2022 20:09


Tgt Ion: 64 Resp: 213

Ion Ratio Lower Upper

64 100

66 0.0 25.0 37.4#




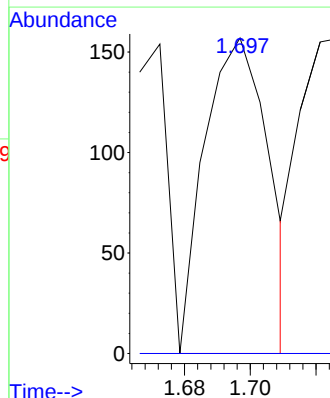




#10
Methyl Iodide
Concen: 0.358 ug/l
RT: 2.459 min Scan# 21
Delta R.T. 0.012 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09




Instrument :
MSVOA_X
ClientSampleId :
PB148361TB


Tgt Ion:142 Resp: 385
Ion Ratio Lower Upper
142 100
127 55.6 37.4 56.0
141 0.0 11.6 17.4#

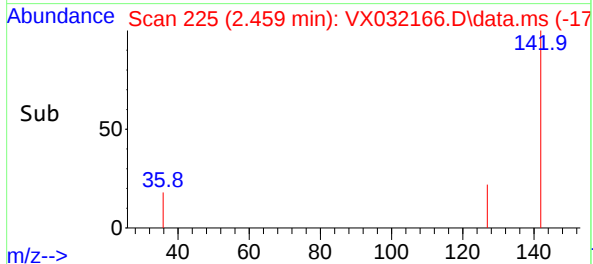

#11
Tert butyl alcohol
Concen: 14.281 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.048 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09

Tgt Ion: 59 Resp: 3178
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#




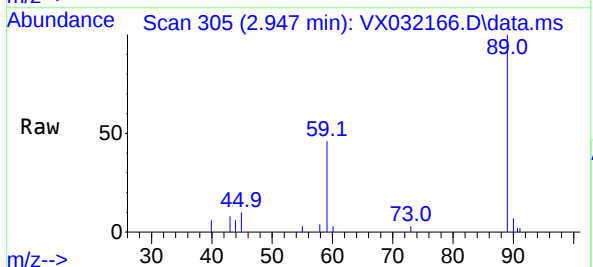




#16
Acetone
Concen: 29.550 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09




Instrument :
MSVOA_X
ClientSampleId :
PB148361TB


Tgt Ion: 43 Resp: 11496
Ion Ratio Lower Upper
43 100
58 33.7 23.8 35.8

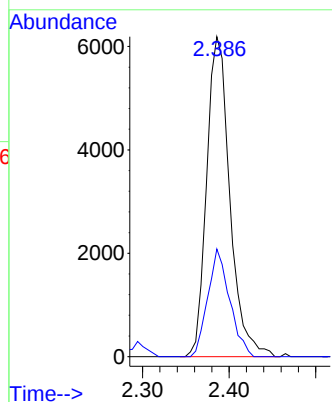

#17
Carbon Disulfide
Concen: 0.389 ug/l
RT: 2.514 min Scan# 234
Delta R.T. 0.006 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09

Tgt Ion: 76 Resp: 810
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#


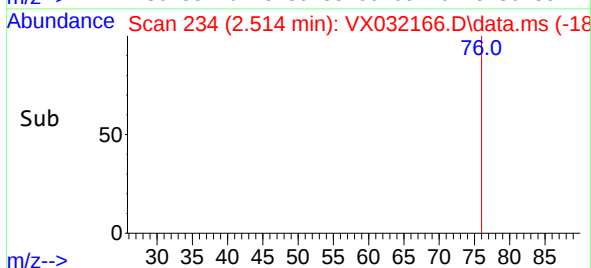
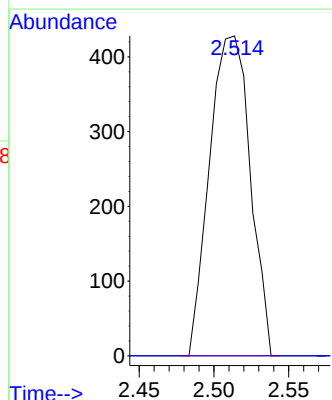



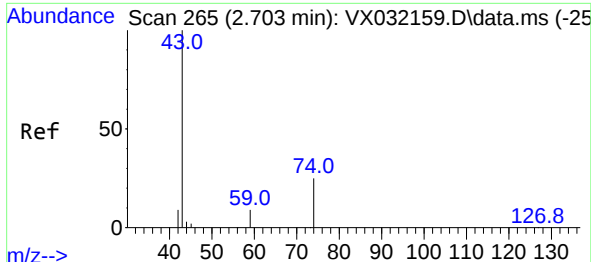

#18
Methyl Acetate
Concen: 0.434 ug/l
RT: 2.715 min Scan# 20
Delta R.T. 0.012 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09




Instrument :
MSVOA_X
ClientSampleId :
PB148361TB


Tgt Ion: 43 Resp: 687
Ion Ratio Lower Upper
43 100
74 24.2 18.6 27.8



#20
Methylene Chloride
Concen: 3.415 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.006 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09

Tgt Ion: 84 Resp: 4085
Ion Ratio Lower Upper
84 100
49 122.2 105.9 158.9
51 34.2 32.2 48.2
86 66.1 50.8 76.2

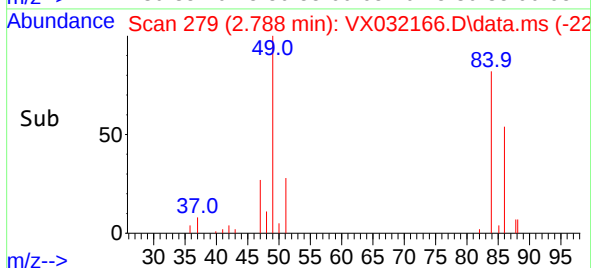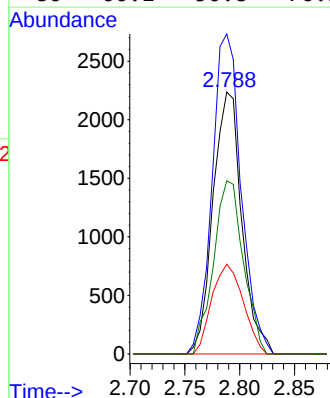



#25

2-Butanone

Concen: 1.462 ug/l

RT: 4.580 min Scan# 51

Delta R.T. 0.024 min

Lab File: VX032166.D

Acq: 17 Oct 2022 20:09

Instrument :

MSVOA_X

ClientSampleId :





PB148361TB

Tgt Ion: 43 Resp: 1215

Ion Ratio Lower Upper

43 100

72 22.9 21.1 31.7

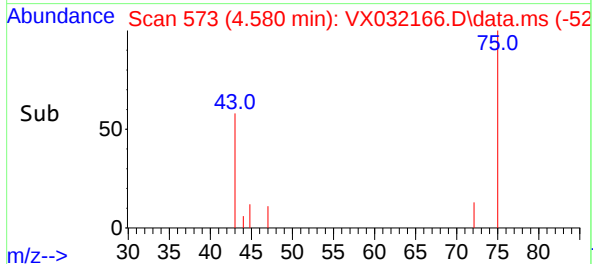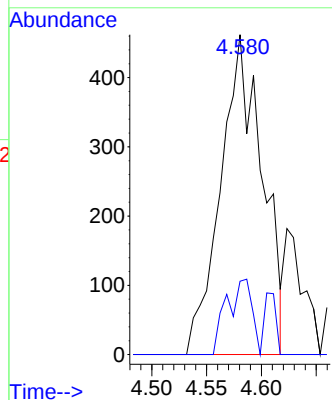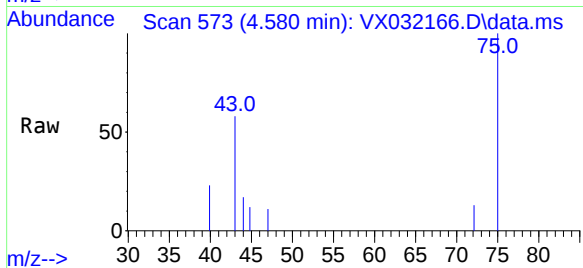

#29

Tetrahydrofuran

Concen: 0.991 ug/l

RT: 5.038 min Scan# 648

Delta R.T. 0.037 min

Lab File: VX032166.D

Acq: 17 Oct 2022 20:09




Tgt Ion: 42 Resp: 494


Ion Ratio Lower Upper

42 100

72 5.3 36.4 54.6#


71 25.7 33.5 50.3#

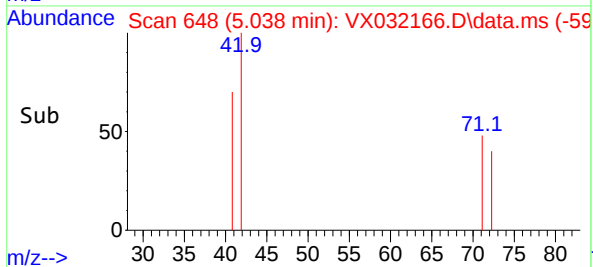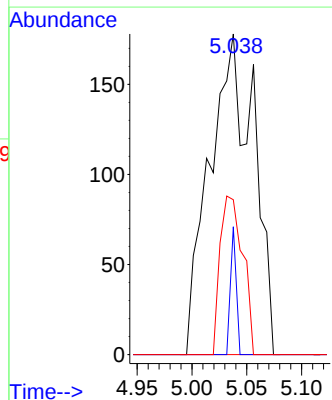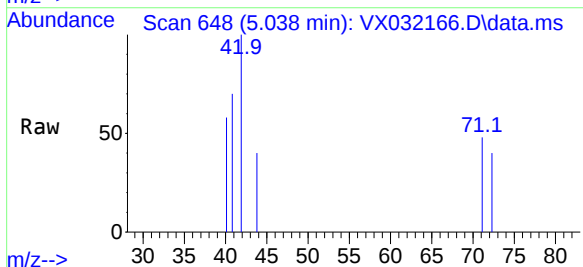



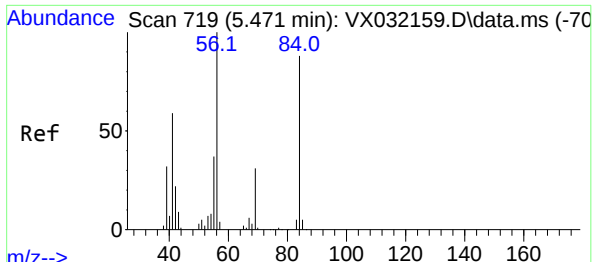


#31
Cyclohexane
Concen: 1.343 ug/l
RT: 5.556 min Scan# 719
Delta R.T. 0.085 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09

Instrument :
MSVOA_X
ClientSampleId :
PB148361TB



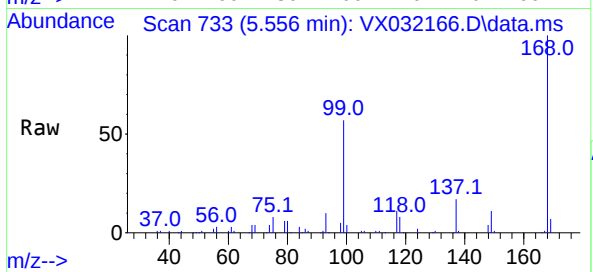



Tgt Ion: 56 Resp: 2422
Ion Ratio Lower Upper
56 100
69 139.0 25.1 37.7#
84 122.2 70.2 105.4#

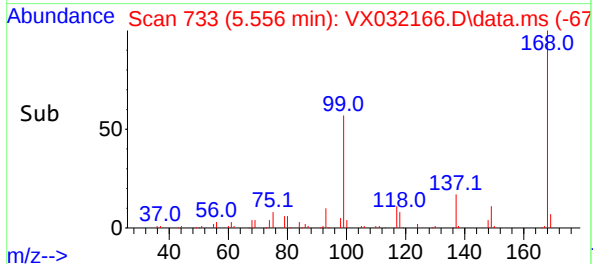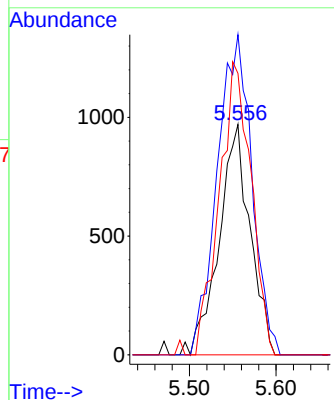

#33
1,2-Dichloroethane-d4
Concen: 65.994 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.006 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09

Tgt Ion: 65 Resp: 106779
Ion Ratio Lower Upper
65 100
67 49.1 0.0 102.4


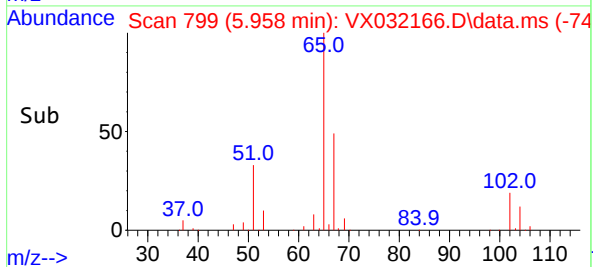
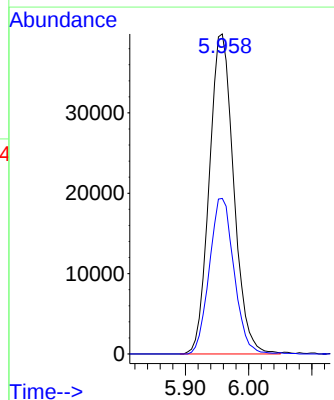
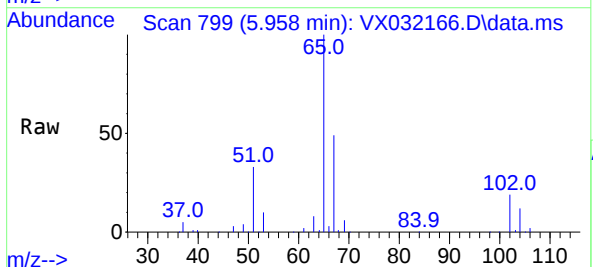


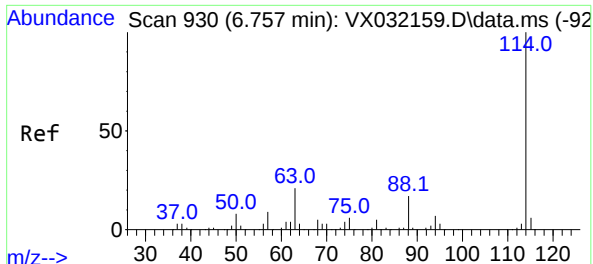

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09




Instrument :
MSVOA_X
ClientSampleId :
PB148361TB


Tgt Ion:114 Resp: 222684
Ion Ratio Lower Upper
114 100
63 20.3 0.0 42.6
88 16.7 0.0 33.0

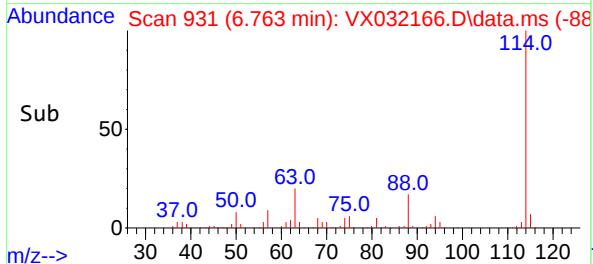

#35
Dibromofluoromethane
Concen: 37.847 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09

Tgt Ion:113 Resp: 57506
Ion Ratio Lower Upper
113 100
111 102.6 82.4 123.6
192 18.3 14.1 21.1


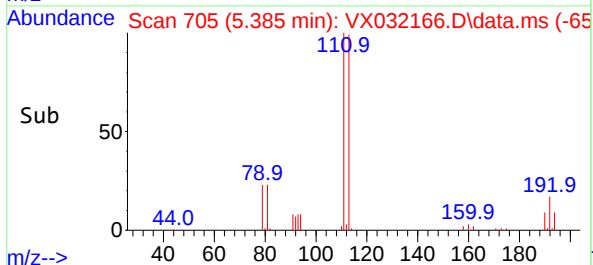
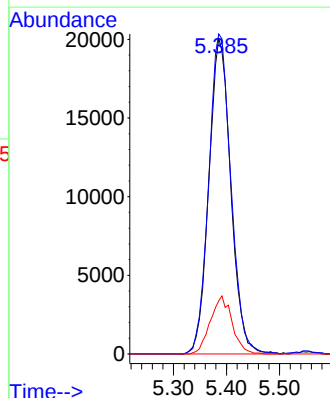
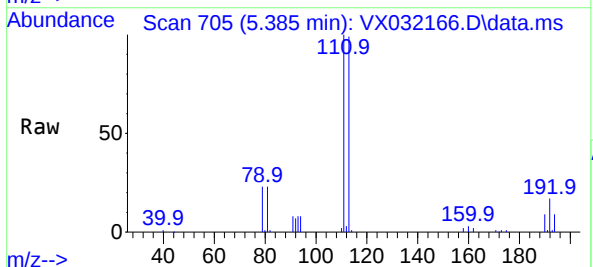




#36
1,1-Dichloropropene
Concen: 3.606 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.140 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09




Instrument :
MSVOA_X
ClientSampleId :
PB148361TB


Tgt Ion: 75 Resp: 7927
Ion Ratio Lower Upper
75 100
110 9.3 17.5 52.5#
77 0.0 24.9 37.3#

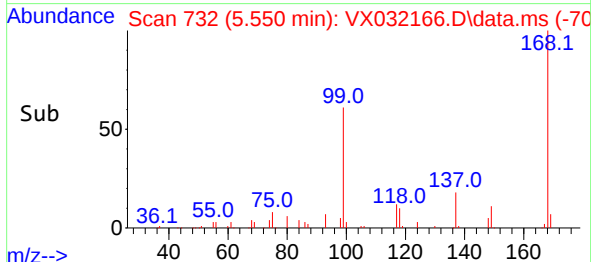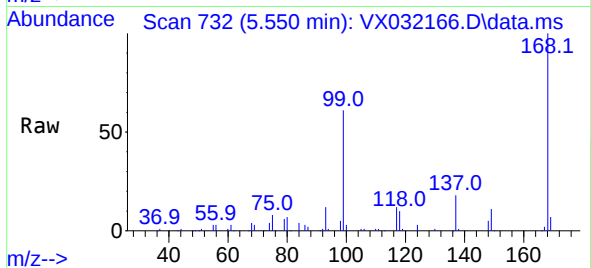

#37
Ethyl Acetate
Concen: 6.438 ug/l
RT: 4.727 min Scan# 597
Delta R.T. 0.018 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09


Tgt Ion: 43 Resp: 14201
Ion Ratio Lower Upper
43 100
61 13.3 11.1 16.7
70 10.9 8.6 13.0

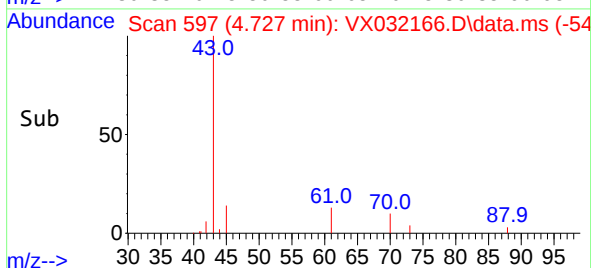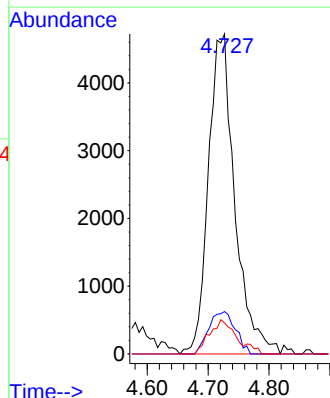



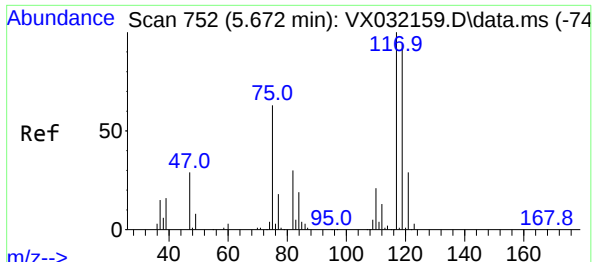


#38
Carbon Tetrachloride
Concen: 4.574 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09

Instrument :
MSVOA_X
ClientSampleId :
PB148361TB



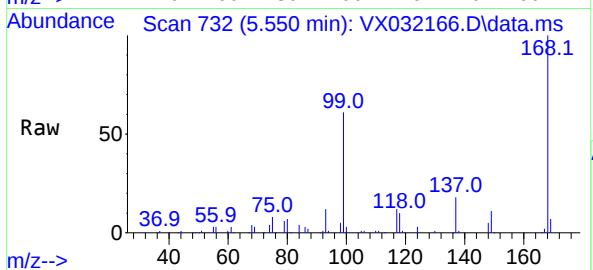



Tgt Ion:117 Resp: 10648
Ion Ratio Lower Upper
117 100
119 5.3 74.6 112.0#
121 0.0 25.3 37.9#

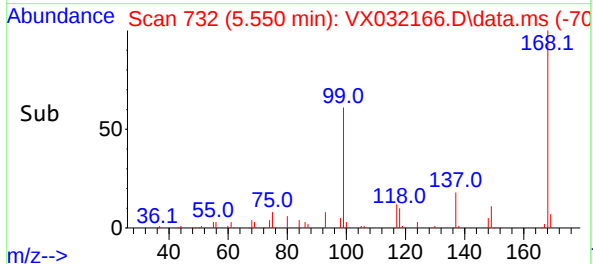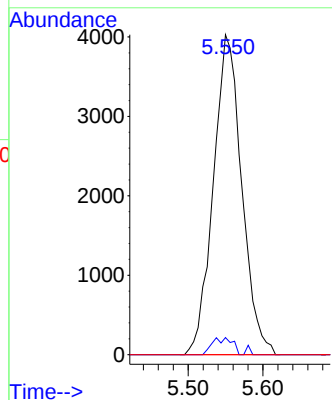

#43
Isopropyl Acetate
Concen: 26.216 ug/l
RT: 6.342 min Scan# 862
Delta R.T. 0.006 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09

Tgt Ion: 43 Resp: 87147
Ion Ratio Lower Upper
43 100
61 18.8 15.3 22.9
87 13.8 10.6 15.8


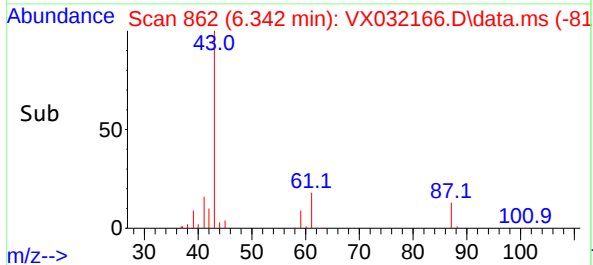
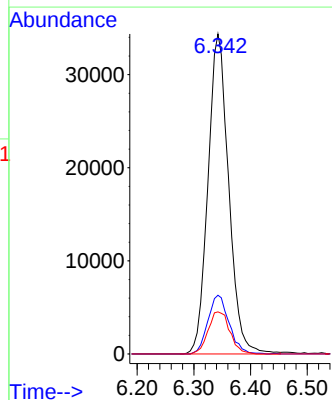
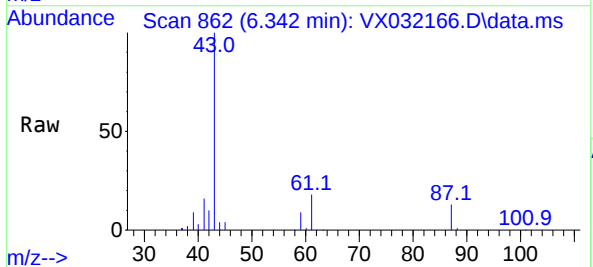




#48
Methyl methacrylate
Concen: 51.097 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.109 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09




Instrument :
MSVOA_X
ClientSampleId :
PB148361TB


Tgt Ion: 41 Resp: 86084
Ion Ratio Lower Upper
41 100
69 0.1 64.6 96.8#
39 57.4 51.4 77.0

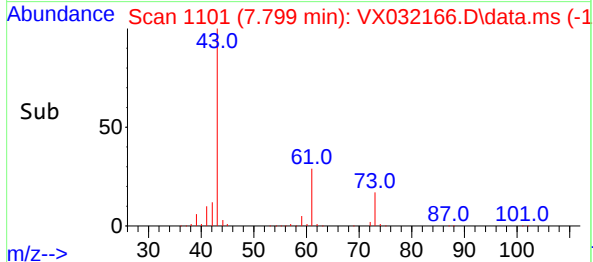

#49
1,4-Dioxane
Concen: 2.808 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.115 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09

Tgt Ion: 88 Resp: 97
Ion Ratio Lower Upper
88 100
43 859199.0 27.1 40.7#
58 3754.6 53.9 80.9#


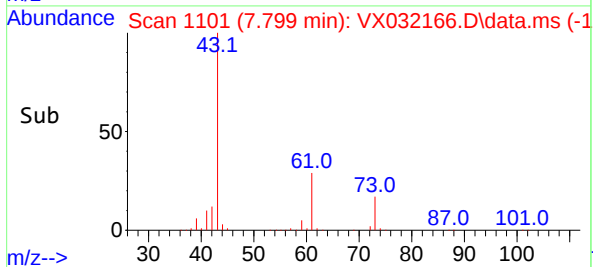

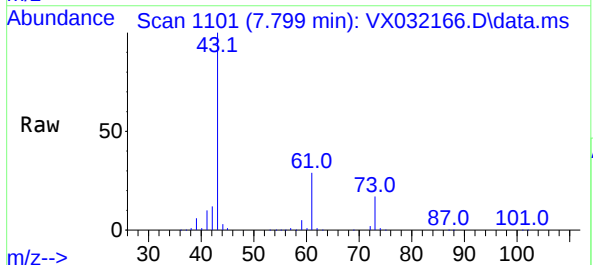




#50
Toluene-d8
Concen: 52.475 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09




Instrument :
MSVOA_X
ClientSampleId :
PB148361TB


Tgt Ion: 98 Resp: 279663
Ion Ratio Lower Upper
98 100
100 65.1 52.5 78.7

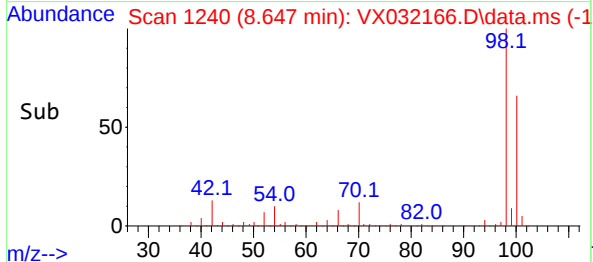

#51
4-Methyl-2-Pentanone
Concen: 37.576 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.025 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09

Tgt Ion: 43 Resp: 76597
Ion Ratio Lower Upper
43 100
58 7.5 30.6 46.0#

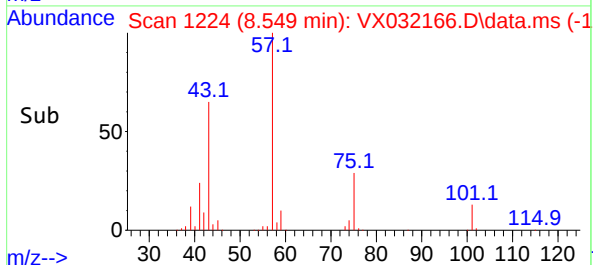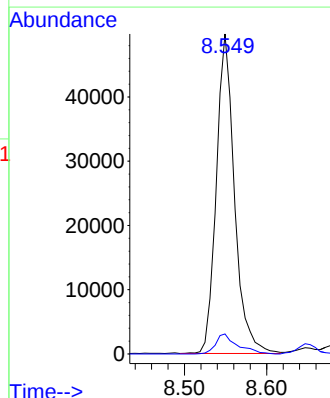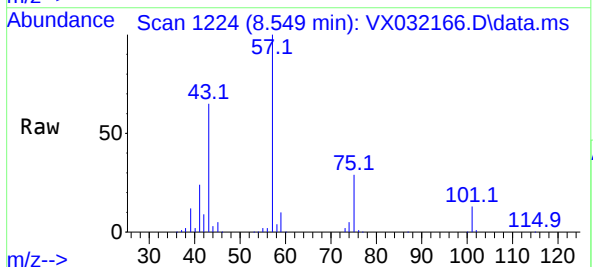



#53

t-1,3-Dichloropropene

Concen: 0.358 ug/l

RT: 8.952 min Scan# 11

Delta R.T. -0.024 min

Lab File: VX032166.D

Acq: 17 Oct 2022 20:09

Instrument :

MSVOA_X

ClientSampleId :





PB148361TB

Tgt Ion: 75 Resp: 700

Ion Ratio Lower Upper

75 100

77 0.0 24.8 37.2#

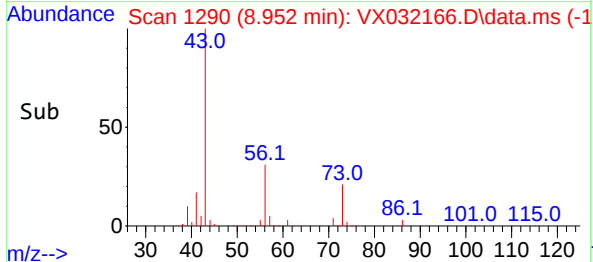

#54

cis-1,3-Dichloropropene

Concen: 14.385 ug/l

RT: 8.549 min Scan# 1224

Delta R.T. 0.183 min

Lab File: VX032166.D

Acq: 17 Oct 2022 20:09




Tgt Ion: 75 Resp: 33032


Ion Ratio Lower Upper

75 100

77 0.6 24.4 36.6#

39 40.9 43.7 65.5#

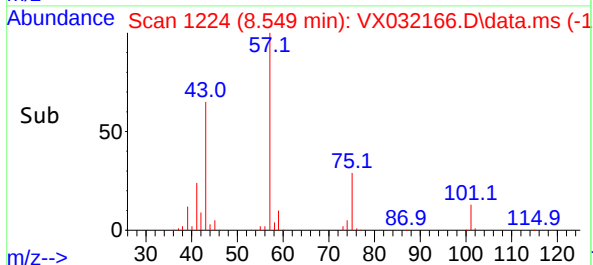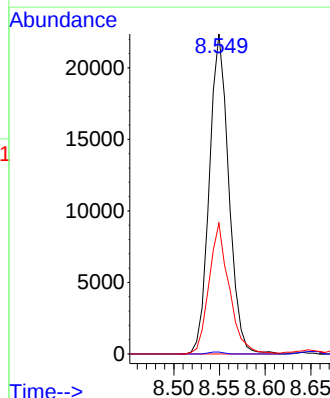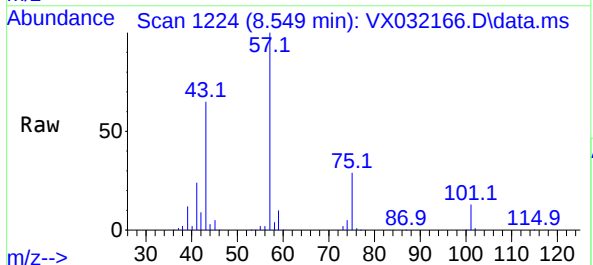

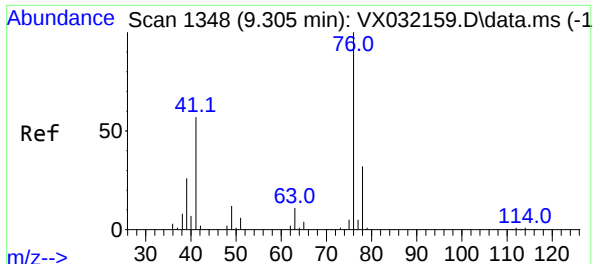

#57

1,3-Dichloropropane

Concen: 1.713 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.177 min

Lab File: VX032166.D

Acq: 17 Oct 2022 20:09

Instrument :

MSVOA_X

ClientSampleId :





PB148361TB

Tgt Ion: 76 Resp: 4466

Ion Ratio Lower Upper

76 100

78 0.0 25.5 38.3#

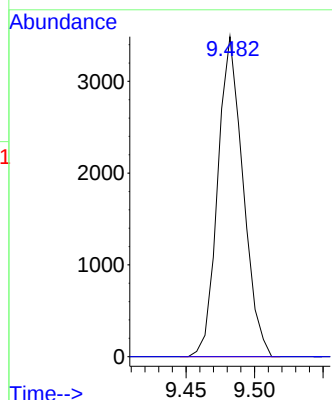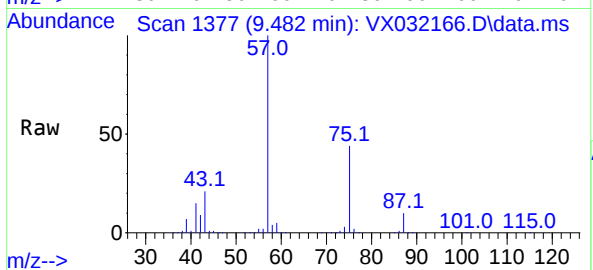

#59

2-Hexanone

Concen: 41.293 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.055 min

Lab File: VX032166.D




Acq: 17 Oct 2022 20:09


Tgt Ion: 43 Resp: 62359

Ion Ratio Lower Upper

43 100

58 18.6 26.7 80.0#


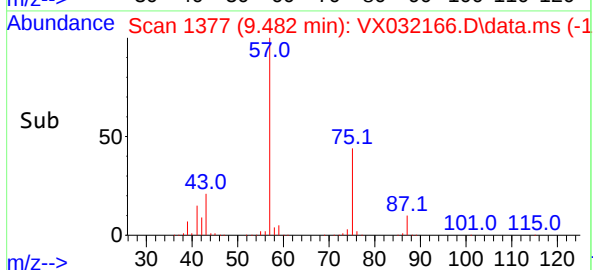
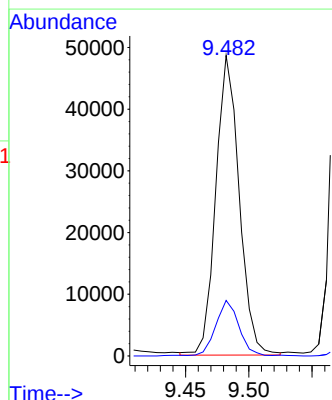





#62
4-Bromofluorobenzene
Concen: 50.576 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09




Instrument :
MSVOA_X
ClientSampleId :
PB148361TB


Tgt Ion: 95 Resp: 102624
Ion Ratio Lower Upper
95 100
174 72.4 0.0 153.2
176 70.5 0.0 144.0



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09

Tgt Ion: 117 Resp: 202953
Ion Ratio Lower Upper
117 100
82 58.3 46.8 70.2
119 31.7 26.4 39.6


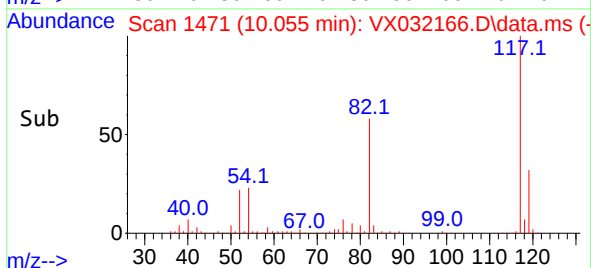
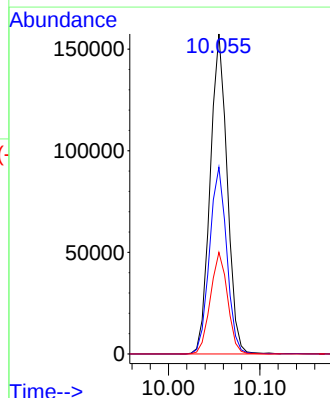





#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09




Instrument :
MSVOA_X
ClientSampleId :
PB148361TB


Tgt Ion:152 Resp: 91862
Ion Ratio Lower Upper
152 100
115 63.2 43.4 130.1
150 155.5 0.0 346.8

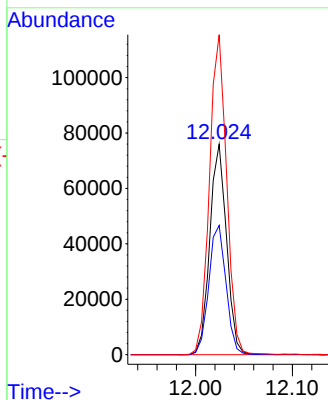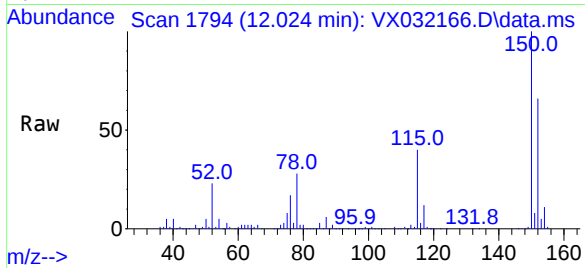

#74
N-ethyl acetate
Concen: 9.249 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.202 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09

Tgt Ion: 43 Resp: 22490
Ion Ratio Lower Upper
43 100
70 1.8 33.4 50.2#
55 4.1 18.2 27.2#
61 9.6 19.3 28.9#


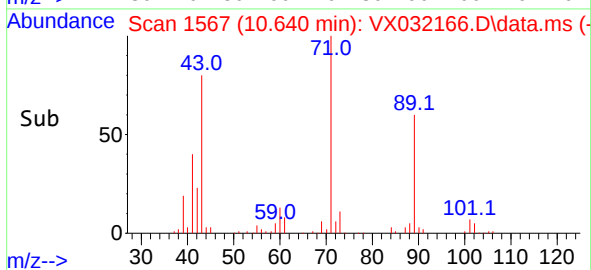
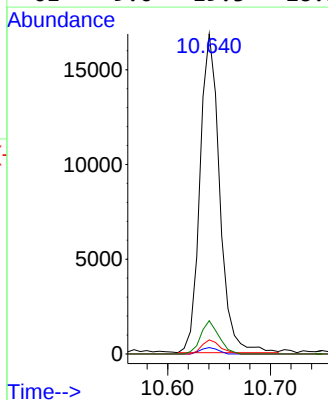
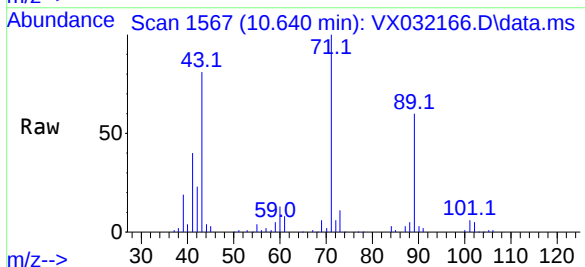




#76
1,2,3-Trichloropropane
Concen: 28.689 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09




Instrument :
MSVOA_X
ClientSampleId :
PB148361TB


Tgt Ion: 75 Resp: 57143
Ion Ratio Lower Upper
75 100
77 1.1 20.3 60.9#

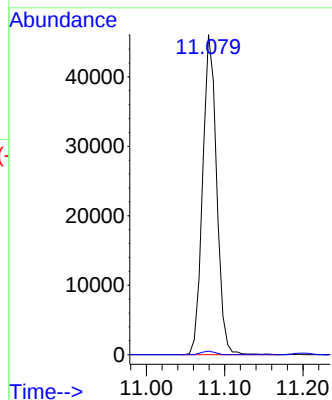

#81
trans-1,4-Dichloro-2-butene
Concen: 110.443 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09

Tgt Ion: 75 Resp: 57143
Ion Ratio Lower Upper
75 100
53 0.0 77.6 116.4#
89 0.0 37.4 56.0#


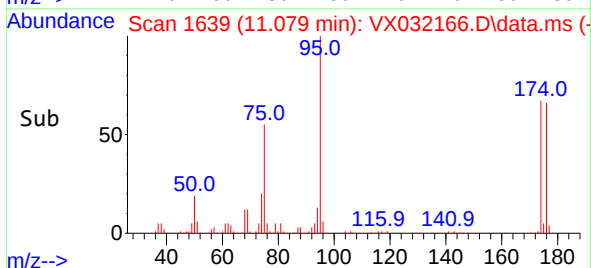
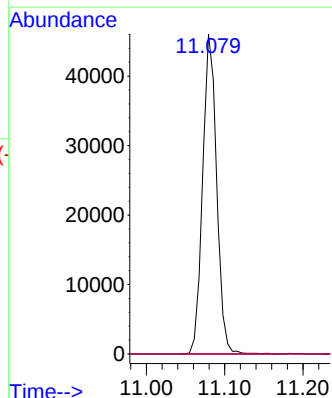





#93
1,2,4-Trichlorobenzene
Concen: 0.290 ug/l
RT: 13.597 min Scan# 2051
Delta R.T. 0.006 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09




Instrument :
MSVOA_X
ClientSampleId :
PB148361TB


Tgt Ion:180 Resp: 503
Ion Ratio Lower Upper
180 100
182 88.9 46.9 140.6
145 25.2 16.7 50.1

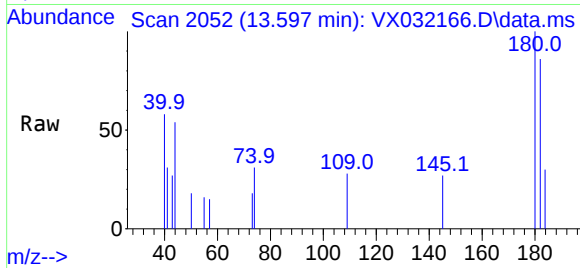

#94
Hexachlorobutadiene
Concen: 0.435 ug/l
RT: 13.719 min Scan# 2072
Delta R.T. -0.006 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09

Tgt Ion:225 Resp: 316
Ion Ratio Lower Upper
225 100
223 38.6 30.8 92.4
227 52.5 32.3 96.9


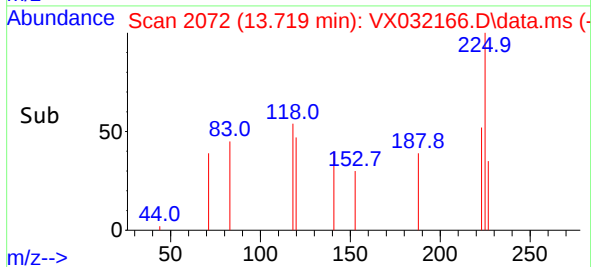

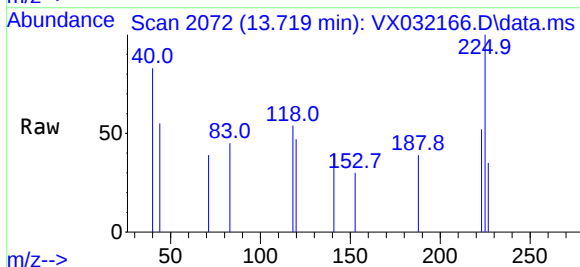




#95
Naphthalene
Concen: 0.226 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09

Instrument :
MSVOA_X
ClientSampleId :
PB148361TB

Tgt Ion:128 Resp: 1309
Ion Ratio Lower Upper
128 100
127 11.8 10.4 15.6
129 13.4 8.8 13.2#

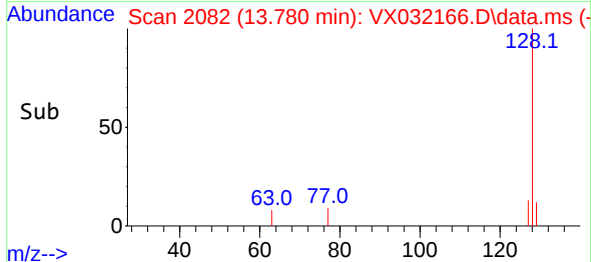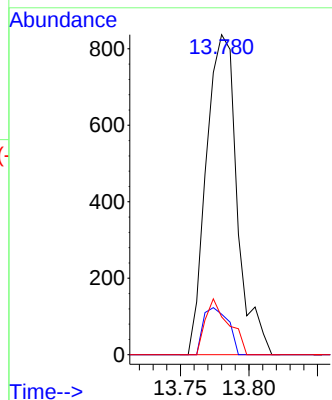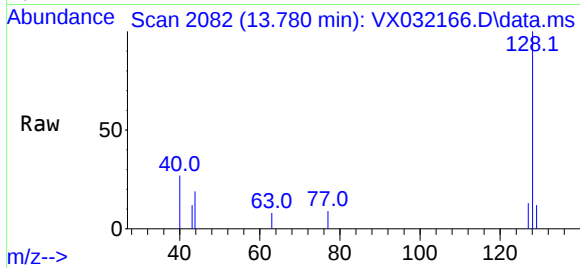

#96
1,2,3-Trichlorobenzene
Concen: 0.275 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. -0.000 min
Lab File: VX032166.D
Acq: 17 Oct 2022 20:09

Tgt Ion:180 Resp: 477
Ion Ratio Lower Upper
180 100
182 88.9 47.9 143.8
145 39.4 17.6 52.8

