

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101722\
 Data File : VX032168.D
 Acq On : 17 Oct 2022 20:55
 Operator : JC/MD
 Sample : N5159-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-32

Quant Time: Oct 18 04:25:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 18 04:18:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	124648	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	217583	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	206228	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	93434	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	103334	52.051	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 104.100%			
35) Dibromofluoromethane	5.385	113	73584	49.564	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 99.120%			
50) Toluene-d8	8.647	98	232825	44.711	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 89.420%			
62) 4-Bromofluorobenzene	11.079	95	104698	52.808	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 105.620%			
Target Compounds						Qvalue
3) Chloromethane	1.295	50	363	0.274	ug/l #	41
5) Bromomethane	1.618	94	398	0.364	ug/l #	43
11) Tert butyl alcohol	2.953	59	3752	13.741	ug/l #	73
13) Acrolein	2.233	56	213	0.927	ug/l #	81
16) Acetone	2.386	43	21367	44.762	ug/l	98
17) Carbon Disulfide	2.508	76	1033	0.405	ug/l #	75
18) Methyl Acetate	2.709	43	1293	0.665	ug/l	93
20) Methylene Chloride	2.782	84	6431	4.382	ug/l #	87
25) 2-Butanone	4.587	43	2891	2.835	ug/l	91
29) Tetrahydrofuran	5.032	42	674	1.102	ug/l #	65
31) Cyclohexane	5.556	56	3300	1.492	ug/l #	9
36) 1,1-Dichloropropene	5.550	75	11130	5.182	ug/l #	50
37) Ethyl Acetate	4.715	43	20246	9.393	ug/l	98
38) Carbon Tetrachloride	5.556	117	14053	6.178	ug/l #	17
40) Benzene	6.044	78	9455	1.574	ug/l	91
41) Methacrylonitrile	5.032	41	278	0.250	ug/l #	23
43) Isopropyl Acetate	6.342	43	87760	27.019	ug/l	100
48) Methyl methacrylate	7.598	41	2006	1.219	ug/l #	13
51) 4-Methyl-2-Pentanone	8.549	43	58316	29.279	ug/l #	47
52) Toluene	8.720	92	5939	1.552	ug/l	100
53) t-1,3-Dichloropropene	8.958	75	500	0.262	ug/l #	44
54) cis-1,3-Dichloropropene	8.549	75	25397	11.320	ug/l #	64
57) 1,3-Dichloropropane	9.482	76	3232	1.269	ug/l #	43
59) 2-Hexanone	9.482	43	44786	30.352	ug/l #	55
68) m/p-Xylenes	10.305	106	2220	0.727	ug/l	89
69) o-Xylene	10.640	106	1733	0.577	ug/l	92
70) Styrene	10.659	104	1750	0.360	ug/l	96
74) N-amyl acetate	10.781	43	596	0.241	ug/l #	43
76) 1,2,3-Trichloropropane	11.079	75	59004	29.125	ug/l #	37
81) trans-1,4-Dichloro-2-b...	11.079	75	59004	112.121	ug/l #	11
84) 1,2,4-Trimethylbenzene	11.756	105	4332	0.690	ug/l #	52
90) Hexachloroethane	12.414	117	328	0.370	ug/l #	15
95) Naphthalene	13.780	128	30059	5.099	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
SB-32

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101722\
Data File : VX032168.D
Acq On : 17 Oct 2022 20:55
Operator : JC/MD
Sample : N5159-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-32

Quant Time: Oct 18 04:25:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101722W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 18 04:18:35 2022
Response via : Initial Calibration




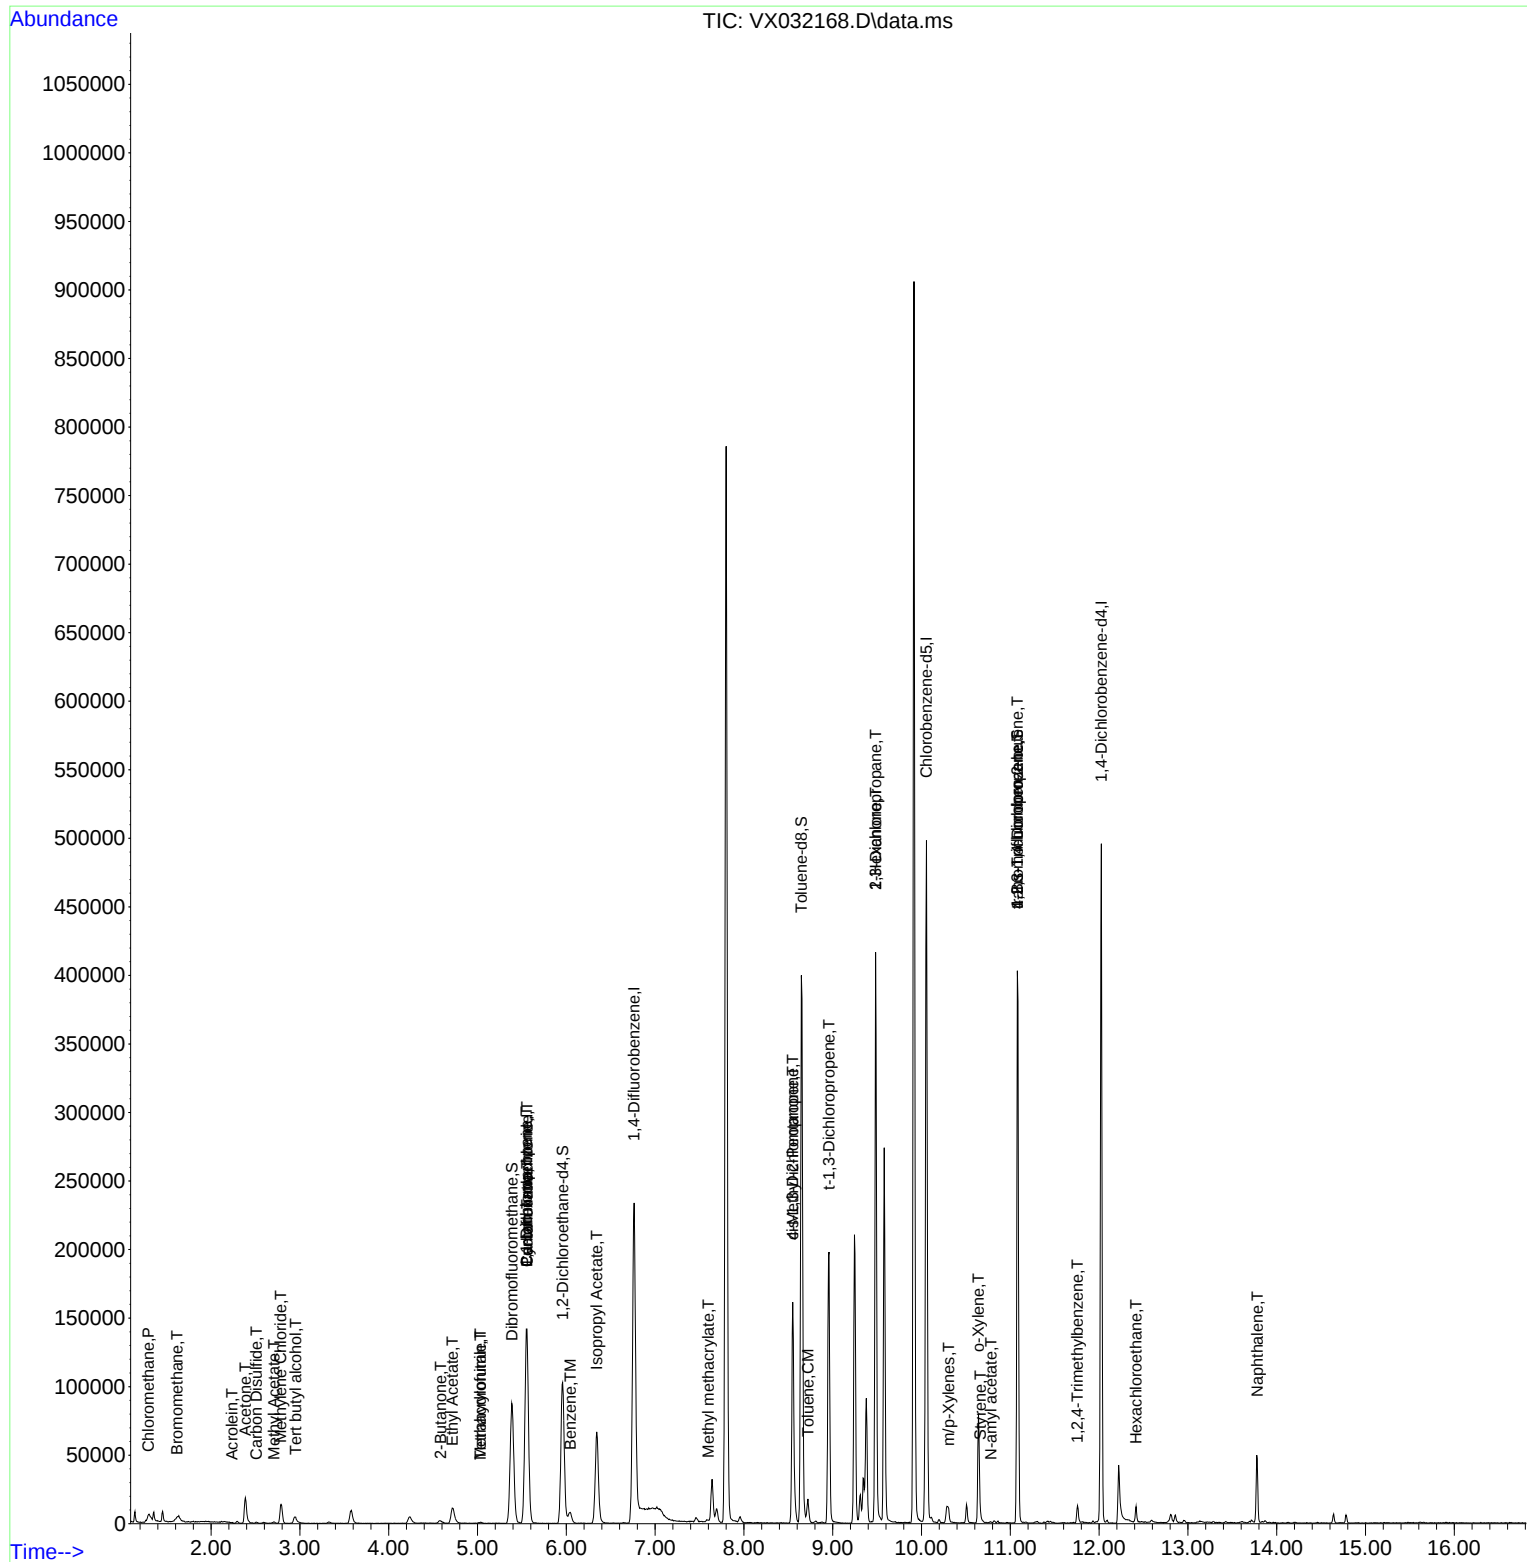




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55




Instrument :
MSVOA_X
ClientSampleId :
SB-32

Tgt Ion:168 Resp: 124648
Ion Ratio Lower Upper
168 100
99 63.8 48.8 73.2

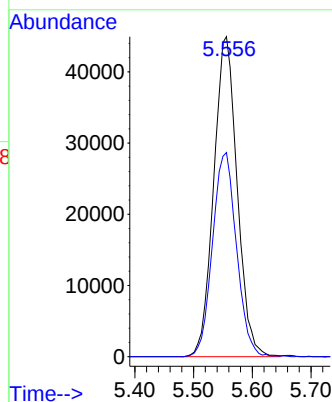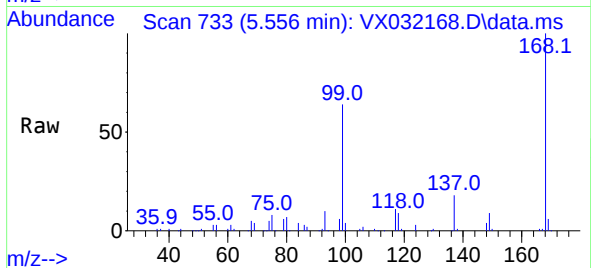


#3
Chloromethane
Concen: 0.274 ug/l
RT: 1.295 min Scan# 34
Delta R.T. 0.007 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55

Tgt Ion: 50 Resp: 363
Ion Ratio Lower Upper
50 100
52 0.0 26.9 40.3#

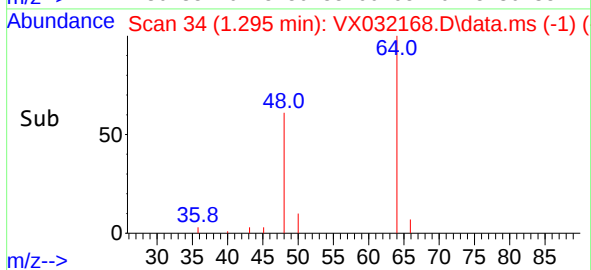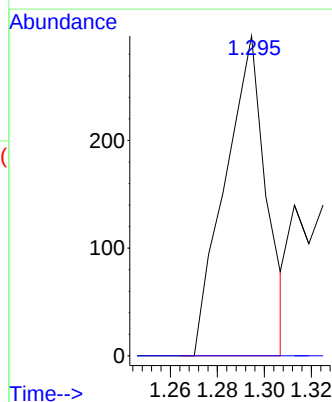

Abundance Scan 86 (1.612 min): VX032159.D\data.ms (-80)

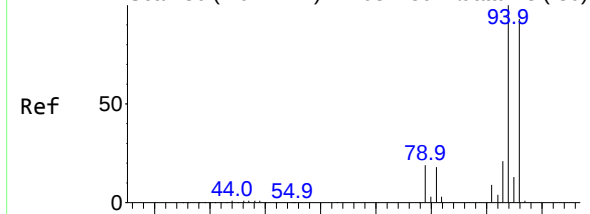

#5

Bromomethane

Concen: 0.364 ug/l

RT: 1.618 min Scan# 81

Delta R.T. 0.006 min

Lab File: VX032168.D

Acq: 17 Oct 2022 20:55

Instrument :

MSVOA_X

ClientSampleId :

SB-32


Tgt Ion: 94 Resp: 398

Ion Ratio Lower Upper


94 100

96 147.3 74.4 111.6#


Abundance Scan 87 (1.618 min): VX032168.D\data.ms

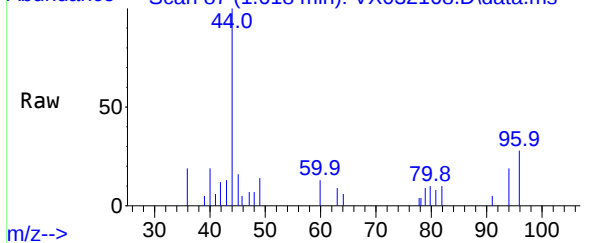


Abundance

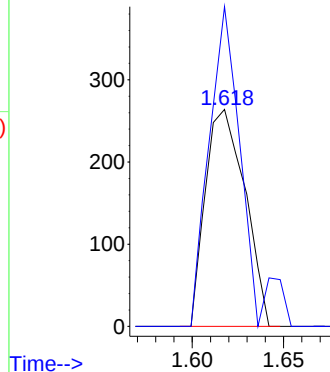

Abundance Scan 87 (1.618 min): VX032168.D\data.ms (-37)

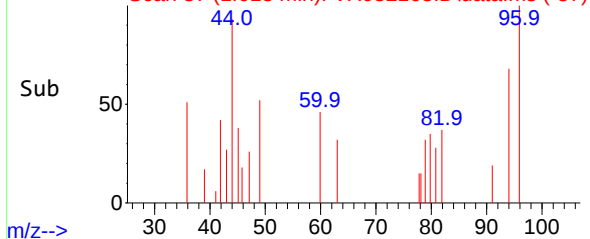

Abundance Scan 313 (2.995 min): VX032159.D\data.ms (-29)

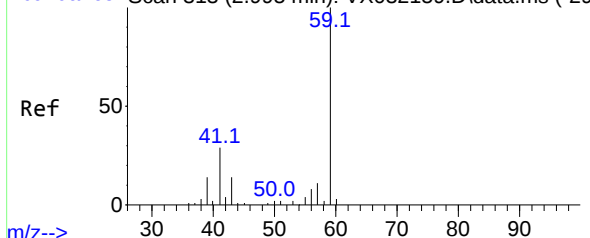

#11

Tert butyl alcohol

Concen: 13.741 ug/l

RT: 2.953 min Scan# 306

Delta R.T. -0.042 min

Lab File: VX032168.D

Acq: 17 Oct 2022 20:55


Tgt Ion: 59 Resp: 3752

Ion Ratio Lower Upper


59 100

57 0.0 8.2 12.2#


Abundance Scan 306 (2.953 min): VX032168.D\data.ms

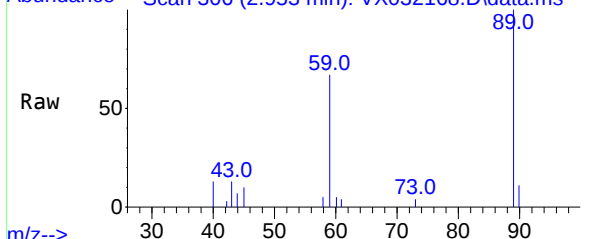


Abundance

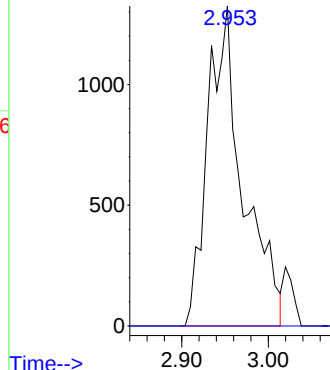

Abundance Scan 306 (2.953 min): VX032168.D\data.ms (-26)




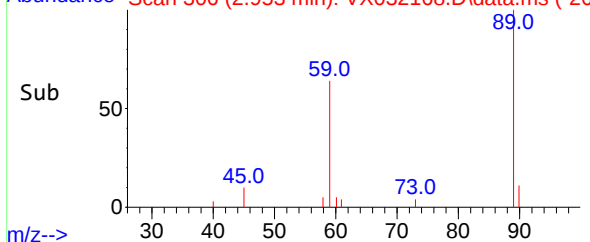




#13
Acrolein
Concen: 0.927 ug/l
RT: 2.233 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55




Instrument :
MSVOA_X
ClientSampleId :
SB-32


Tgt Ion: 56 Resp: 213
Ion Ratio Lower Upper
56 100
55 85.4 56.0 84.0#

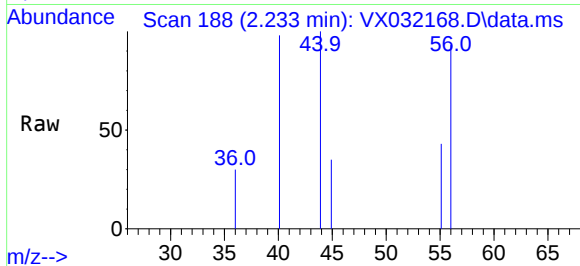

#16
Acetone
Concen: 44.762 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55

Tgt Ion: 43 Resp: 21367
Ion Ratio Lower Upper
43 100
58 28.5 23.8 35.8


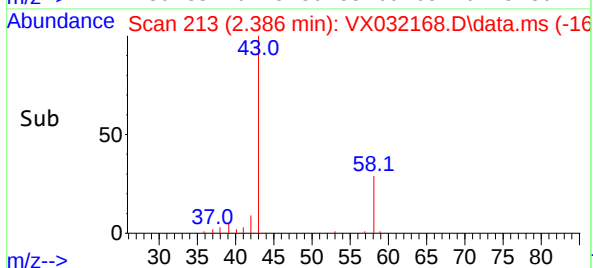

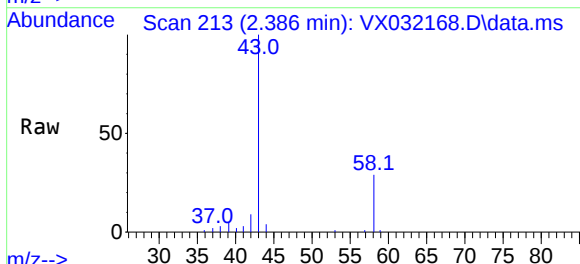




#17
Carbon Disulfide
Concen: 0.405 ug/l
RT: 2.508 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55




Instrument :
MSVOA_X
ClientSampleId :
SB-32


Tgt Ion: 76 Resp: 1033
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#



#18
Methyl Acetate
Concen: 0.665 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.006 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55

Tgt Ion: 43 Resp: 1293
Ion Ratio Lower Upper
43 100
74 20.0 18.6 27.8


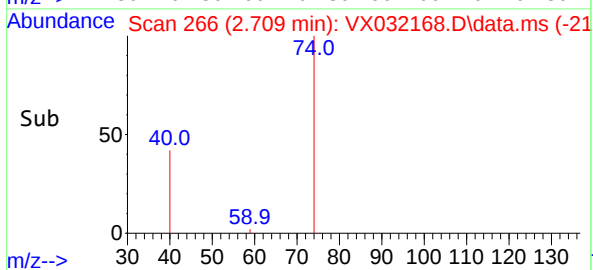






#20
Methylene Chloride
Concen: 4.382 ug/l
RT: 2.782 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55




Instrument :
MSVOA_X
ClientSampleId :
SB-32


Tgt Ion: 84	Resp: 6431
Ion Ratio	Lower Upper
84 100	
49 114.6	105.9 158.9
51 31.8	32.2 48.2#
86 58.2	50.8 76.2

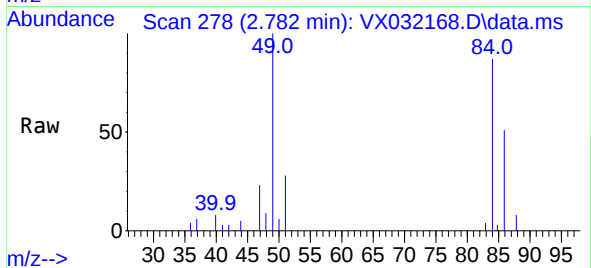

#25
2-Butanone
Concen: 2.835 ug/l
RT: 4.587 min Scan# 574
Delta R.T. 0.031 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55

Tgt Ion: 43	Resp: 2891		
Ion Ratio	Lower	Upper	
43 100			
72 21.8	21.1	31.7	

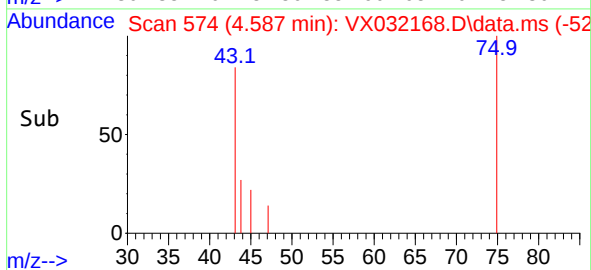



#29

Tetrahydrofuran

Concen: 1.102 ug/l

RT: 5.032 min Scan# 64

Delta R.T. 0.031 min

Lab File: VX032168.D

Acq: 17 Oct 2022 20:55

Instrument :

MSVOA_X

ClientSampleId :

SB-32





Tgt Ion: 42 Resp: 674

Ion Ratio Lower Upper

42 100

72 22.3 36.4 54.6#

71 19.7 33.5 50.3#

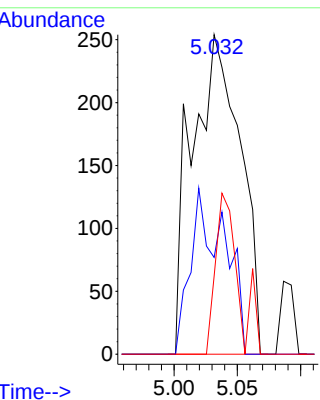

#31

Cyclohexane

Concen: 1.492 ug/l

RT: 5.556 min Scan# 733

Delta R.T. 0.085 min

Lab File: VX032168.D

Acq: 17 Oct 2022 20:55




Tgt Ion: 56 Resp: 3300


Ion Ratio Lower Upper

56 100

69 144.1 25.1 37.7#

84 135.5 70.2 105.4#

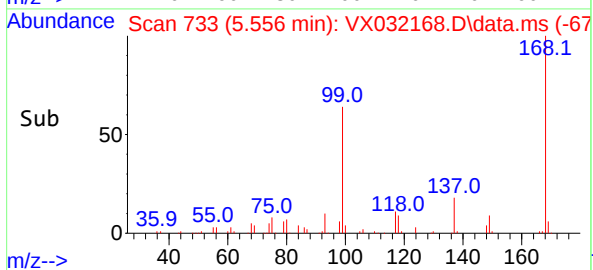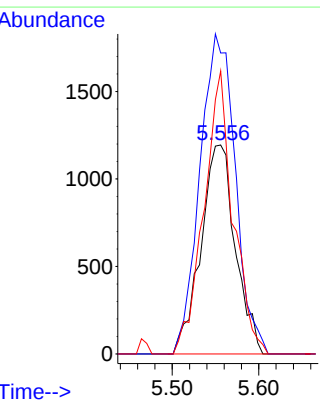



#33

1,2-Dichloroethane-d4

Concen: 52.051 ug/l

RT: 5.958 min Scan# 798

Delta R.T. 0.006 min

Lab File: VX032168.D

Acq: 17 Oct 2022 20:55

Instrument :

MSVOA_X

ClientSampleId :





SB-32

Tgt Ion: 65 Resp: 103334

Ion Ratio Lower Upper

65 100

67 49.2 0.0 102.4

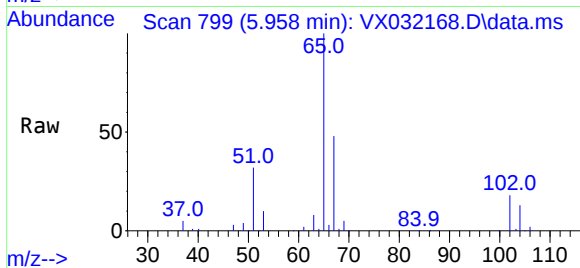

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.006 min

Lab File: VX032168.D

Acq: 17 Oct 2022 20:55




Tgt Ion: 114 Resp: 217583


Ion Ratio Lower Upper

114 100

63 20.7 0.0 42.6

88 16.7 0.0 33.0

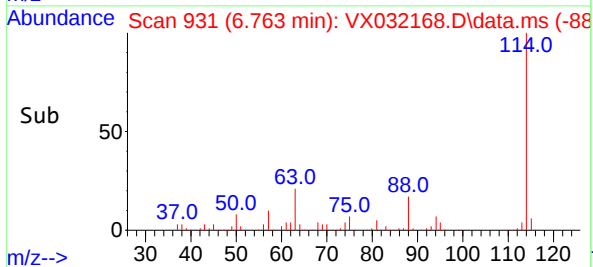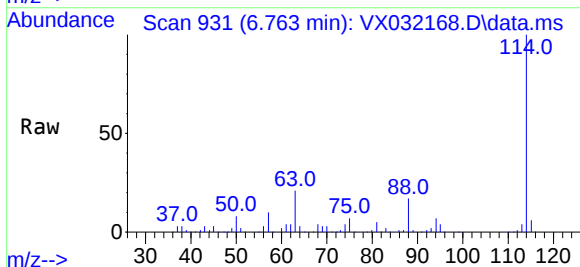

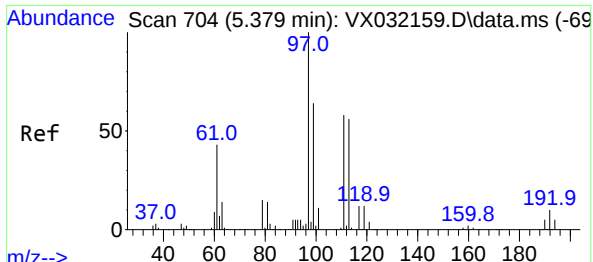

#35

Dibromofluoromethane

Concen: 49.564 ug/l

RT: 5.385 min Scan# 704

Delta R.T. 0.006 min

Lab File: VX032168.D

Acq: 17 Oct 2022 20:55

Instrument :

MSVOA_X

ClientSampleId :

SB-32





Tgt Ion:113 Resp: 73584

Ion Ratio Lower Upper

113 100

111 103.0 82.4 123.6

192 18.0 14.1 21.1

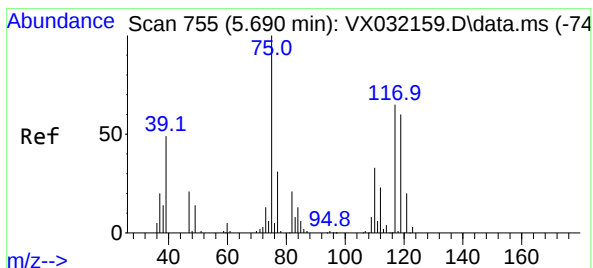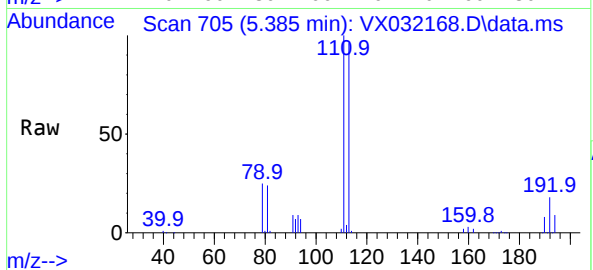

#36

1,1-Dichloropropene

Concen: 5.182 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.140 min

Lab File: VX032168.D

Acq: 17 Oct 2022 20:55




Tgt Ion: 75 Resp: 11130


Ion Ratio Lower Upper

75 100

110 9.7 17.5 52.5#

77 0.0 24.9 37.3#

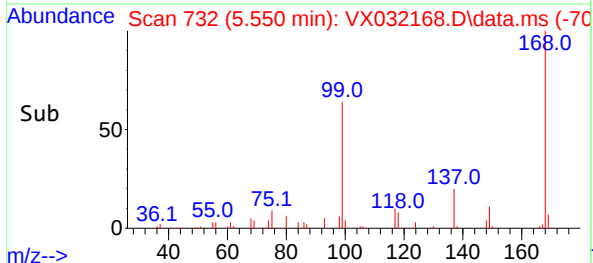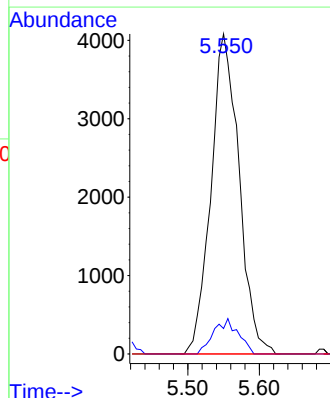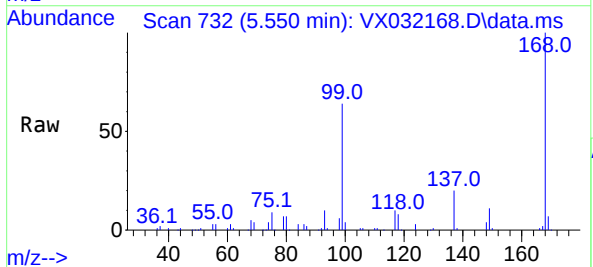



#37

Ethyl Acetate

Concen: 9.393 ug/l

RT: 4.715 min Scan# 594

Delta R.T. 0.006 min

Lab File: VX032168.D

Acq: 17 Oct 2022 20:55

Instrument :

MSVOA_X

ClientSampleId :

SB-32





Tgt Ion: 43 Resp: 20246

Ion Ratio Lower Upper

43 100

61 12.6 11.1 16.7

70 11.1 8.6 13.0

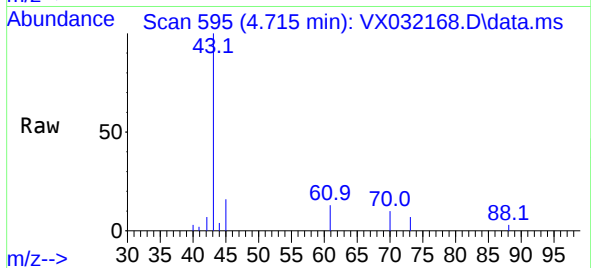

#38

Carbon Tetrachloride

Concen: 6.178 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.116 min

Lab File: VX032168.D

Acq: 17 Oct 2022 20:55




Tgt Ion: 117 Resp: 14053


Ion Ratio Lower Upper

117 100

119 4.9 74.6 112.0#

121 0.0 25.3 37.9#


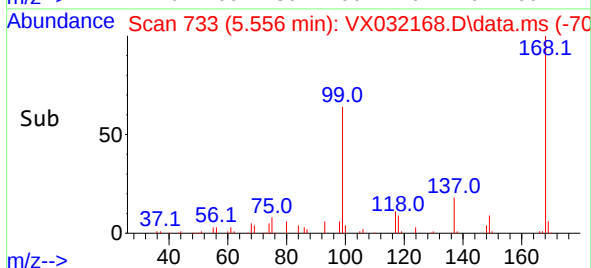
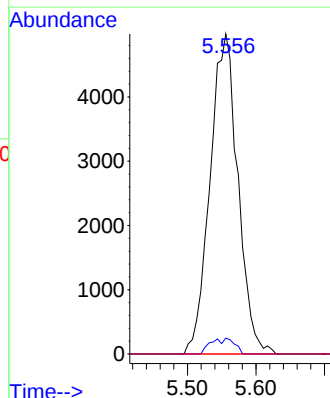





#40
Benzene
Concen: 1.574 ug/l
RT: 6.044 min Scan# 812
Delta R.T. 0.006 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55




Instrument :
MSVOA_X
ClientSampleId :
SB-32


Tgt Ion: 78 Resp: 9455
Ion Ratio Lower Upper
78 100
77 19.0 18.7 28.1

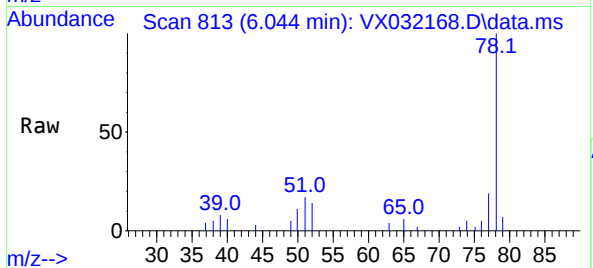

#41
Methacrylonitrile
Concen: 0.250 ug/l
RT: 5.032 min Scan# 647
Delta R.T. 0.116 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55

Tgt Ion: 41 Resp: 278
Ion Ratio Lower Upper
41 100
39 0.0 45.0 67.6#
67 0.0 58.2 87.4#
52 0.0 25.0 37.6#

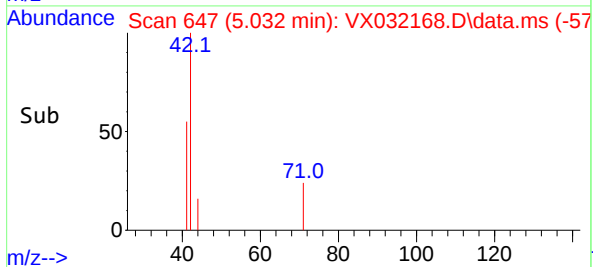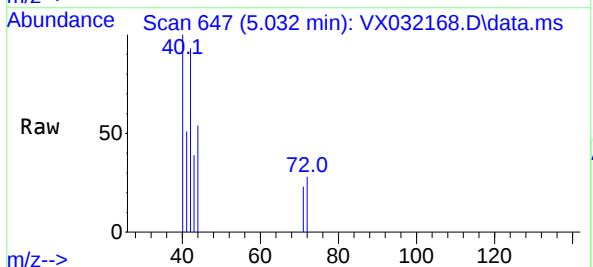



#43

Isopropyl Acetate

Concen: 27.019 ug/l

RT: 6.342 min Scan# 8

Delta R.T. 0.006 min

Lab File: VX032168.D

Acq: 17 Oct 2022 20:55

Instrument :

MSVOA_X

ClientSampleId :

SB-32





Tgt Ion: 43 Resp: 87760

Ion Ratio Lower Upper

43 100

61 19.4 15.3 22.9

87 13.3 10.6 15.8

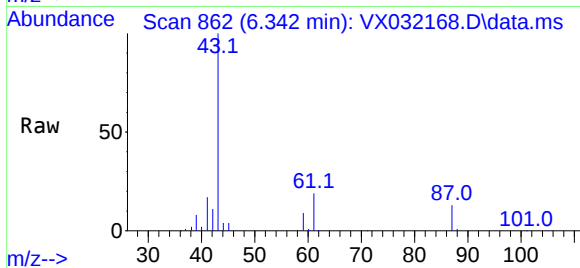

#48

Methyl methacrylate

Concen: 1.219 ug/l

RT: 7.598 min Scan# 1068

Delta R.T. -0.092 min

Lab File: VX032168.D

Acq: 17 Oct 2022 20:55




Tgt Ion: 41 Resp: 2006


Ion Ratio Lower Upper

41 100

69 0.0 64.6 96.8#

39 0.0 51.4 77.0#

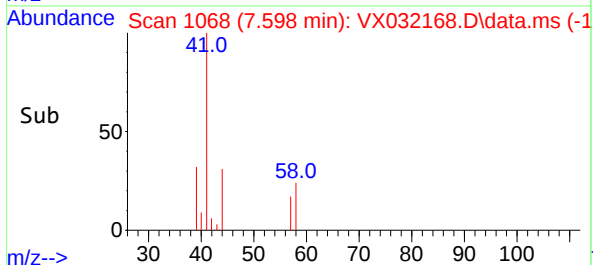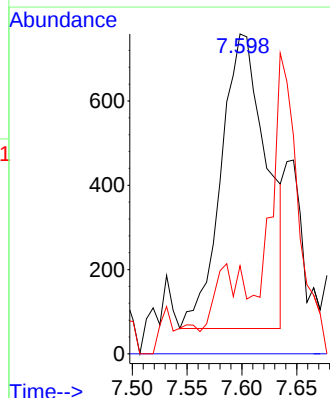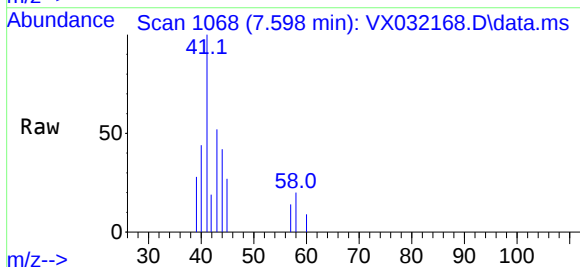



#50

Toluene-d8

Concen: 44.711 ug/l

RT: 8.647 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX032168.D

Acq: 17 Oct 2022 20:55

Instrument :

MSVOA_X

ClientSampleId :





SB-32

Tgt Ion: 98 Resp: 232825

Ion Ratio Lower Upper

98 100

100 66.3 52.5 78.7

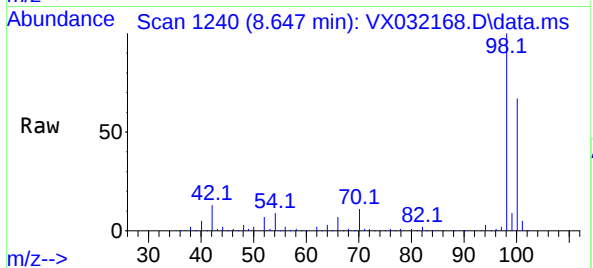

#51

4-Methyl-2-Pentanone

Concen: 29.279 ug/l

RT: 8.549 min Scan# 1224

Delta R.T. -0.025 min

Lab File: VX032168.D




Acq: 17 Oct 2022 20:55


Tgt Ion: 43 Resp: 58316

Ion Ratio Lower Upper

43 100

58 6.4 30.6 46.0#

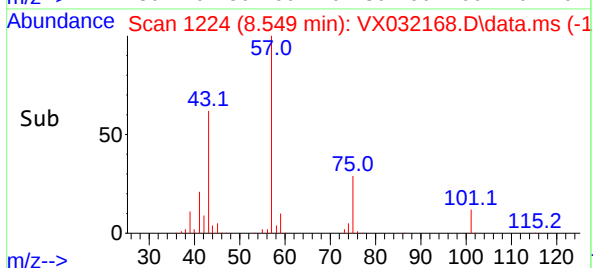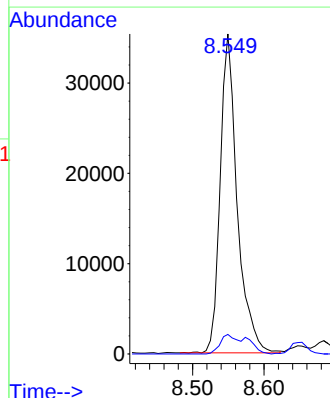



#52

Toluene

Concen: 1.552 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. 0.000 min

Lab File: VX032168.D

Acq: 17 Oct 2022 20:55

Instrument :

MSVOA_X

ClientSampleId :


SB-32

Tgt Ion: 92 Resp: 5939




Ion Ratio Lower Upper

92 100

91 171.4 137.1 205.7

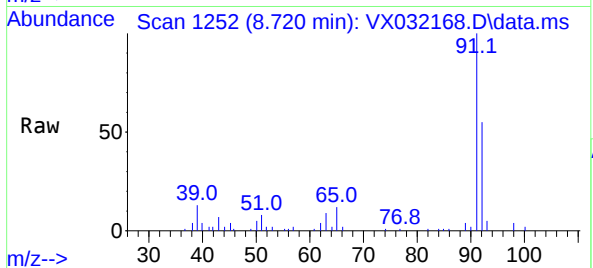

Abundance

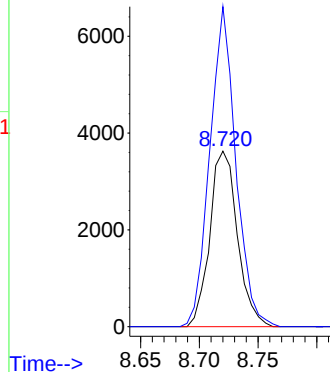

#53

t-1,3-Dichloropropene

Concen: 0.262 ug/l

RT: 8.958 min Scan# 1291

Delta R.T. -0.018 min

Lab File: VX032168.D


Acq: 17 Oct 2022 20:55

Tgt Ion: 75 Resp: 500



Ion Ratio Lower Upper


75 100

77 0.0 24.8 37.2#



Abundance



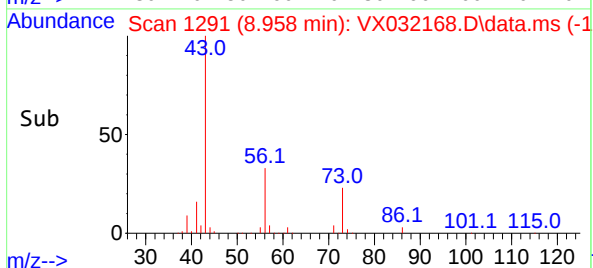
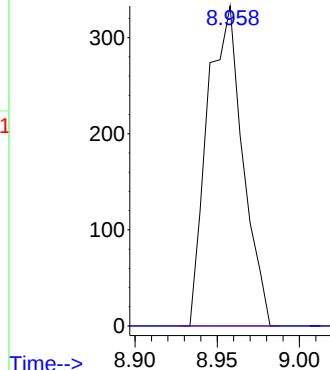




#54
 cis-1,3-Dichloropropene
 Concen: 11.320 ug/l
 RT: 8.549 min Scan# 1194
 Delta R.T. 0.183 min
 Lab File: VX032168.D
 Acq: 17 Oct 2022 20:55




Instrument :
 MSVOA_X
 ClientSampleId :
 SB-32


Tgt Ion: 75 Resp: 25397
 Ion Ratio Lower Upper
 75 100
 77 0.6 24.4 36.6#
 39 36.6 43.7 65.5#

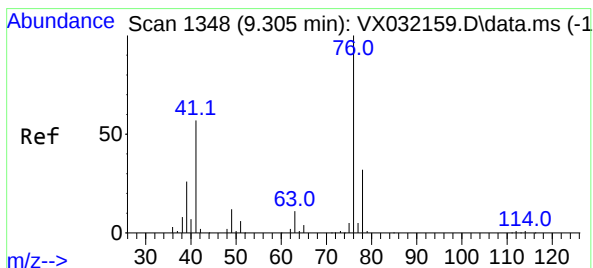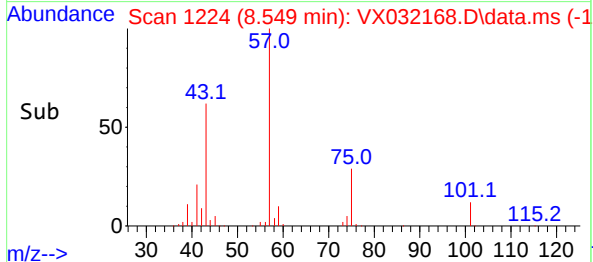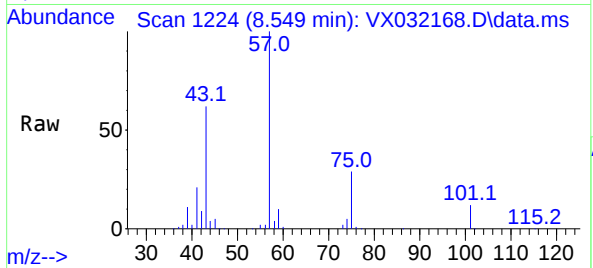

#57
 1,3-Dichloropropane
 Concen: 1.269 ug/l
 RT: 9.482 min Scan# 1377
 Delta R.T. 0.177 min
 Lab File: VX032168.D
 Acq: 17 Oct 2022 20:55

Tgt Ion: 76 Resp: 3232
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.5 38.3#

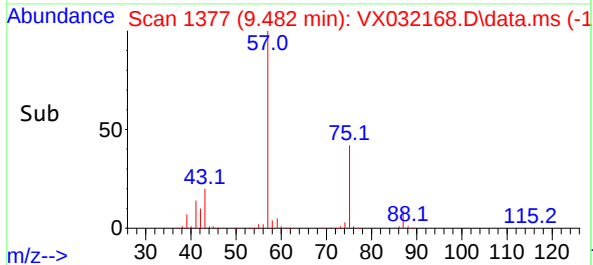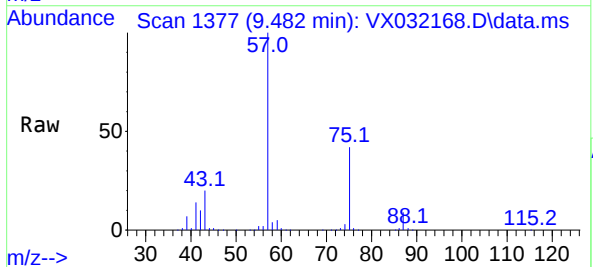



#59

2-Hexanone

Concen: 30.352 ug/l

RT: 9.482 min Scan# 1

Delta R.T. 0.055 min

Lab File: VX032168.D

Acq: 17 Oct 2022 20:55

Instrument :

MSVOA_X

ClientSampleId :





SB-32

Tgt Ion: 43 Resp: 44786

Ion Ratio Lower Upper

43 100

58 21.5 26.7 80.0#

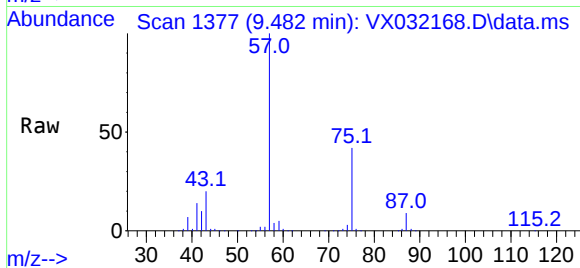

#62

4-Bromofluorobenzene

Concen: 52.808 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX032168.D

Acq: 17 Oct 2022 20:55




Tgt Ion: 95 Resp: 104698


Ion Ratio Lower Upper

95 100

174 73.4 0.0 153.2

176 70.9 0.0 144.0


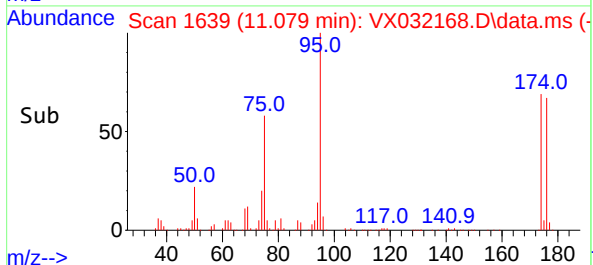
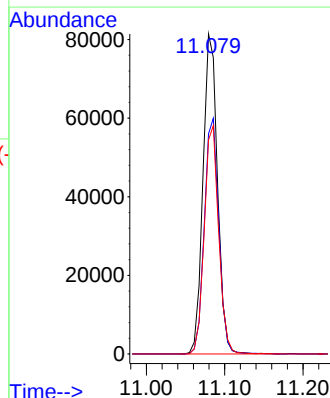
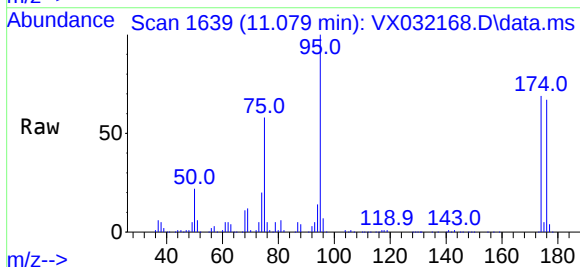




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55




Instrument :
MSVOA_X
ClientSampleId :
SB-32


Tgt Ion:117 Resp: 206228
Ion Ratio Lower Upper
117 100
82 57.1 46.8 70.2
119 31.8 26.4 39.6

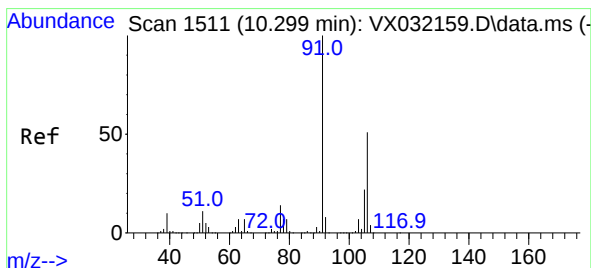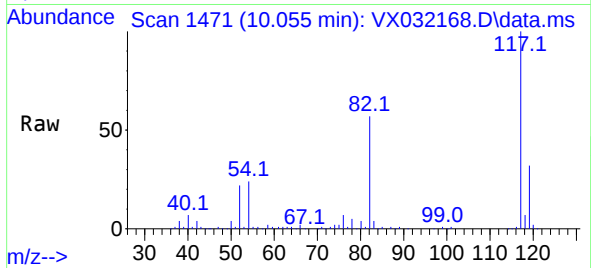

#68
m/p-Xylenes
Concen: 0.727 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55

Tgt Ion:106 Resp: 2220
Ion Ratio Lower Upper
106 100
91 218.1 161.0 241.4


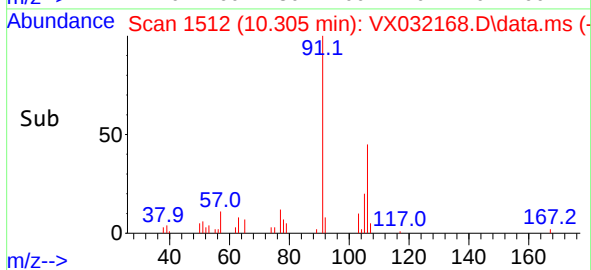

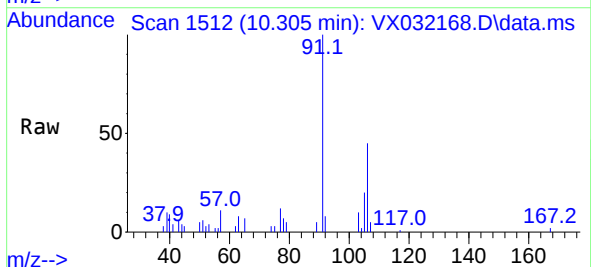




#69
o-Xylene
Concen: 0.577 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55




Instrument :
MSVOA_X
ClientSampleId :
SB-32


Tgt Ion:106 Resp: 1733
Ion Ratio Lower Upper
106 100
91 202.3 107.2 321.6

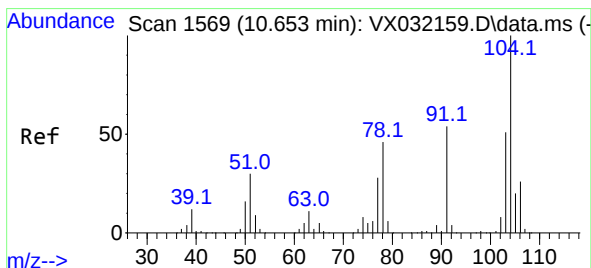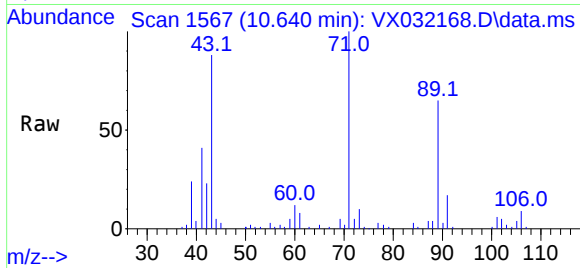

#70
Styrene
Concen: 0.360 ug/l
RT: 10.659 min Scan# 1570
Delta R.T. 0.006 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55

Tgt Ion:104 Resp: 1750
Ion Ratio Lower Upper
104 100
78 55.8 41.4 62.2
103 52.7 43.8 65.8


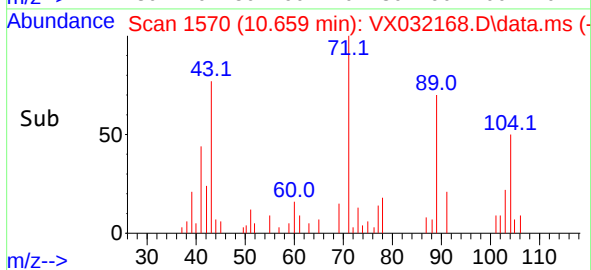

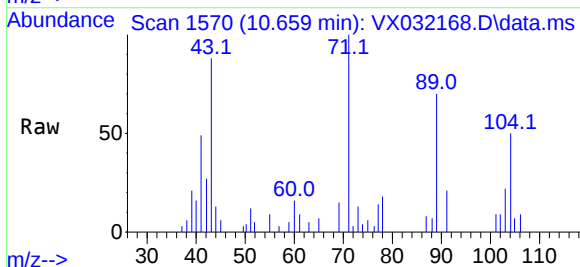




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55




Instrument :
MSVOA_X
ClientSampleId :
SB-32


Tgt Ion:152 Resp: 93434
Ion Ratio Lower Upper
152 100
115 63.9 43.4 130.1
150 156.6 0.0 346.8

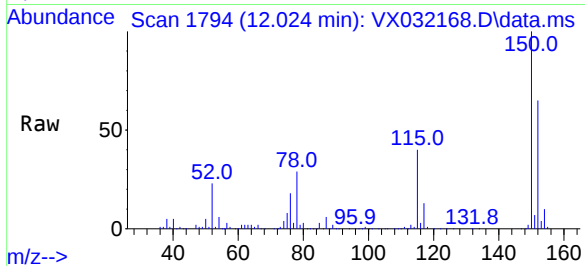

#74
N-ethyl acetate
Concen: 0.241 ug/l
RT: 10.781 min Scan# 1590
Delta R.T. -0.061 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55

Tgt Ion: 43 Resp: 596
Ion Ratio Lower Upper
43 100
70 0.0 33.4 50.2#
55 0.0 18.2 27.2#
61 0.0 19.3 28.9#


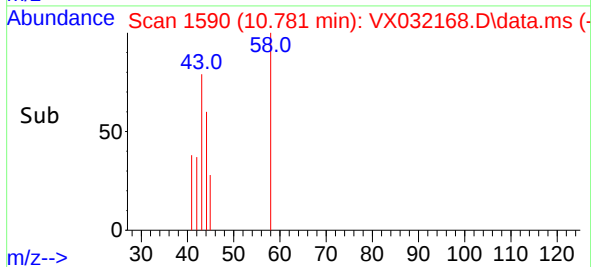

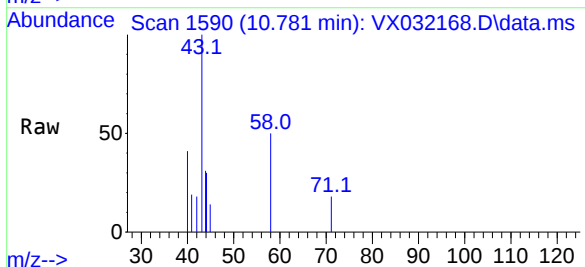




#76
1,2,3-Trichloropropane
Concen: 29.125 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55




Instrument :
MSVOA_X
ClientSampleId :
SB-32


Tgt Ion: 75 Resp: 59004
Ion Ratio Lower Upper
75 100
77 1.1 20.3 60.9#

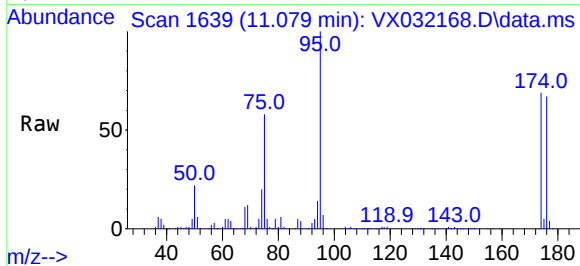

#81
trans-1,4-Dichloro-2-butene
Concen: 112.121 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55

Tgt Ion: 75 Resp: 59004
Ion Ratio Lower Upper
75 100
53 0.0 77.6 116.4#
89 0.1 37.4 56.0#


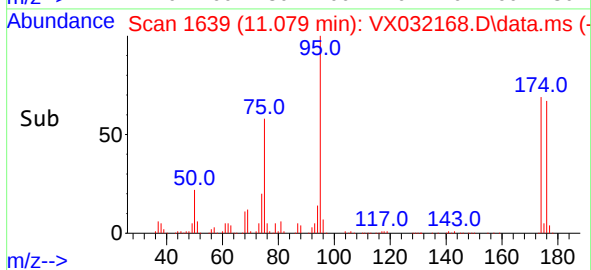

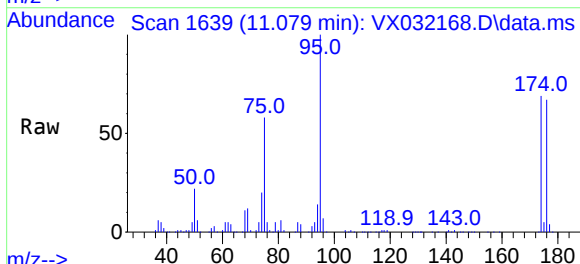




#84
1,2,4-Trimethylbenzene
Concen: 0.690 ug/l
RT: 11.756 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55




Instrument :
MSVOA_X
ClientSampleId :
SB-32


Tgt Ion:105 Resp: 4332
Ion Ratio Lower Upper
105 100
120 13.7 22.6 67.8#

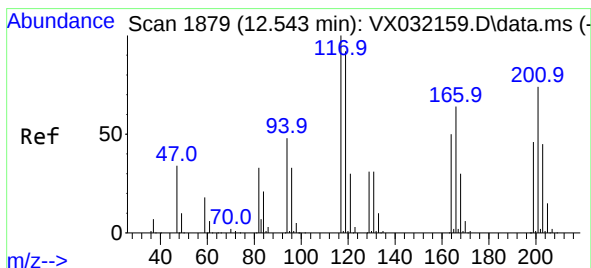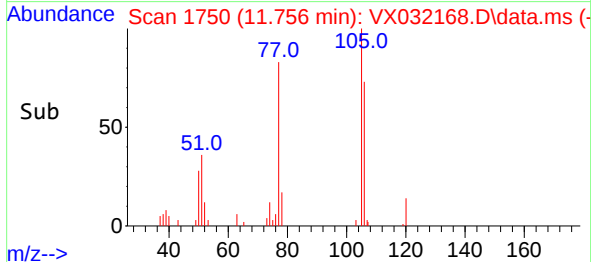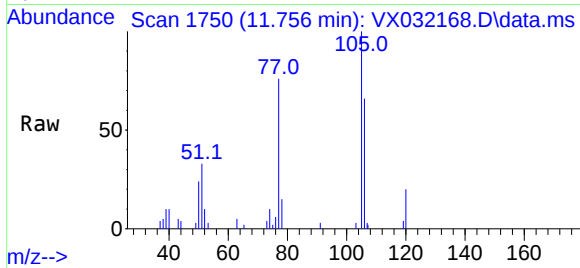

#90
Hexachloroethane
Concen: 0.370 ug/l
RT: 12.414 min Scan# 1858
Delta R.T. -0.129 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55


Tgt Ion:117 Resp: 328
Ion Ratio Lower Upper
117 100
201 0.0 34.8 104.4#

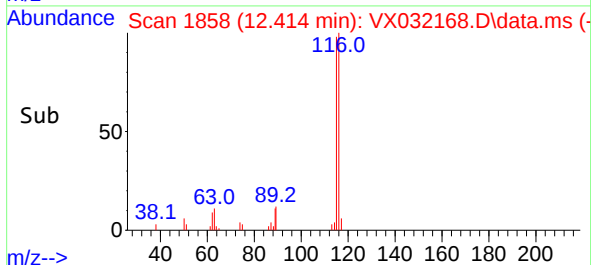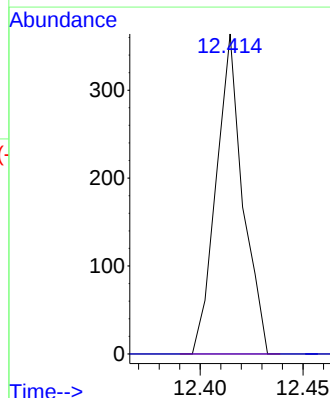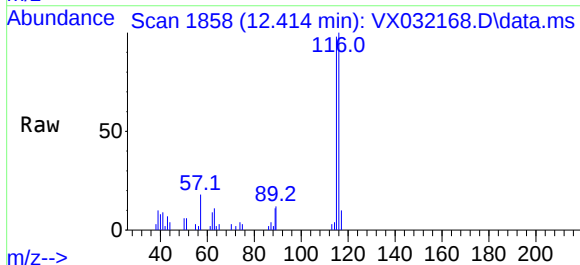



#95
Naphthalene
Concen: 5.099 ug/l
RT: 13.780 min Scan# 20
Delta R.T. 0.000 min
Lab File: VX032168.D
Acq: 17 Oct 2022 20:55

Instrument :
MSVOA_X
ClientSampleId :
SB-32

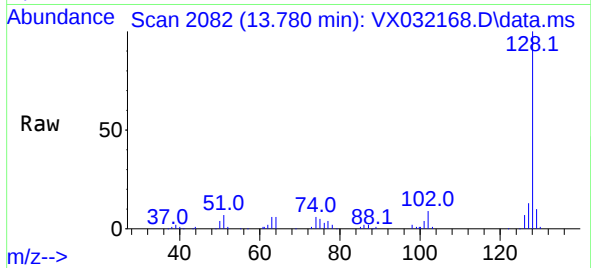

Tgt Ion:128 Resp: 30059
Ion Ratio Lower Upper
128 100
127 14.4 10.4 15.6
129 10.9 8.8 13.2

