

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101722\
 Data File : VX032172.D
 Acq On : 17 Oct 2022 22:28
 Operator : JC/MD
 Sample : N5159-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-36

Quant Time: Oct 18 04:28:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 18 04:18:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	122433	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	216075	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	163374	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	87848	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	105686	54.198	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 108.400%			
35) Dibromofluoromethane	5.385	113	75701	51.346	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 102.700%			
50) Toluene-d8	8.647	98	226966	43.890	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 87.780%			
62) 4-Bromofluorobenzene	11.079	95	102642	52.132	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 104.260%			
Target Compounds					Qvalue	
5) Bromomethane	1.618	94	476	0.443	ug/l #	72
11) Tert butyl alcohol	2.947	59	2513	9.370	ug/l #	73
13) Acrolein	2.240	56	147	0.651	ug/l	87
16) Acetone	2.386	43	18202	38.822	ug/l	99
18) Methyl Acetate	2.709	43	1773	0.929	ug/l #	87
20) Methylene Chloride	2.788	84	6612	4.587	ug/l #	94
25) 2-Butanone	4.581	43	2417	2.413	ug/l #	76
29) Tetrahydrofuran	5.026	42	658	1.095	ug/l #	55
31) Cyclohexane	5.544	56	3274	1.507	ug/l #	37
36) 1,1-Dichloropropene	5.556	75	11389	5.339	ug/l #	50
37) Ethyl Acetate	4.715	43	19970	9.330	ug/l	99
38) Carbon Tetrachloride	5.556	117	13968	6.184	ug/l #	18
40) Benzene	6.044	78	4982	0.835	ug/l #	86
43) Isopropyl Acetate	6.342	43	89556	27.765	ug/l	99
48) Methyl methacrylate	7.799	41	66049	40.404	ug/l #	45
49) 1,4-Dioxane	7.793	88	42	1.253	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	57245	28.942	ug/l #	51
52) Toluene	8.720	92	3423	0.900	ug/l	94
53) t-1,3-Dichloropropene	8.958	75	532	0.280	ug/l #	44
54) cis-1,3-Dichloropropene	8.549	75	26058	11.695	ug/l #	62
56) Ethyl methacrylate	9.244	69	600	0.291	ug/l #	1
57) 1,3-Dichloropropane	9.488	76	3541	1.400	ug/l #	43
59) 2-Hexanone	9.482	43	46361	31.638	ug/l #	52
68) m/p-Xylenes	10.299	106	1492	0.617	ug/l	95
69) o-Xylene	10.647	106	890	0.374	ug/l	79
70) Styrene	10.659	104	853	0.222	ug/l #	73
74) N-amyl acetate	10.640	43	18995	8.168	ug/l #	53
76) 1,2,3-Trichloropropane	11.079	75	56878	29.861	ug/l #	37
81) trans-1,4-Dichloro-2-b...	11.079	75	56878	114.954	ug/l #	11
84) 1,2,4-Trimethylbenzene	11.756	105	1537	0.261	ug/l	70
95) Naphthalene	13.780	128	8936	1.612	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101722\
Data File : VX032172.D
Acq On : 17 Oct 2022 22:28
Operator : JC/MD
Sample : N5159-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-36

Quant Time: Oct 18 04:28:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101722W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 18 04:18:35 2022
Response via : Initial Calibration




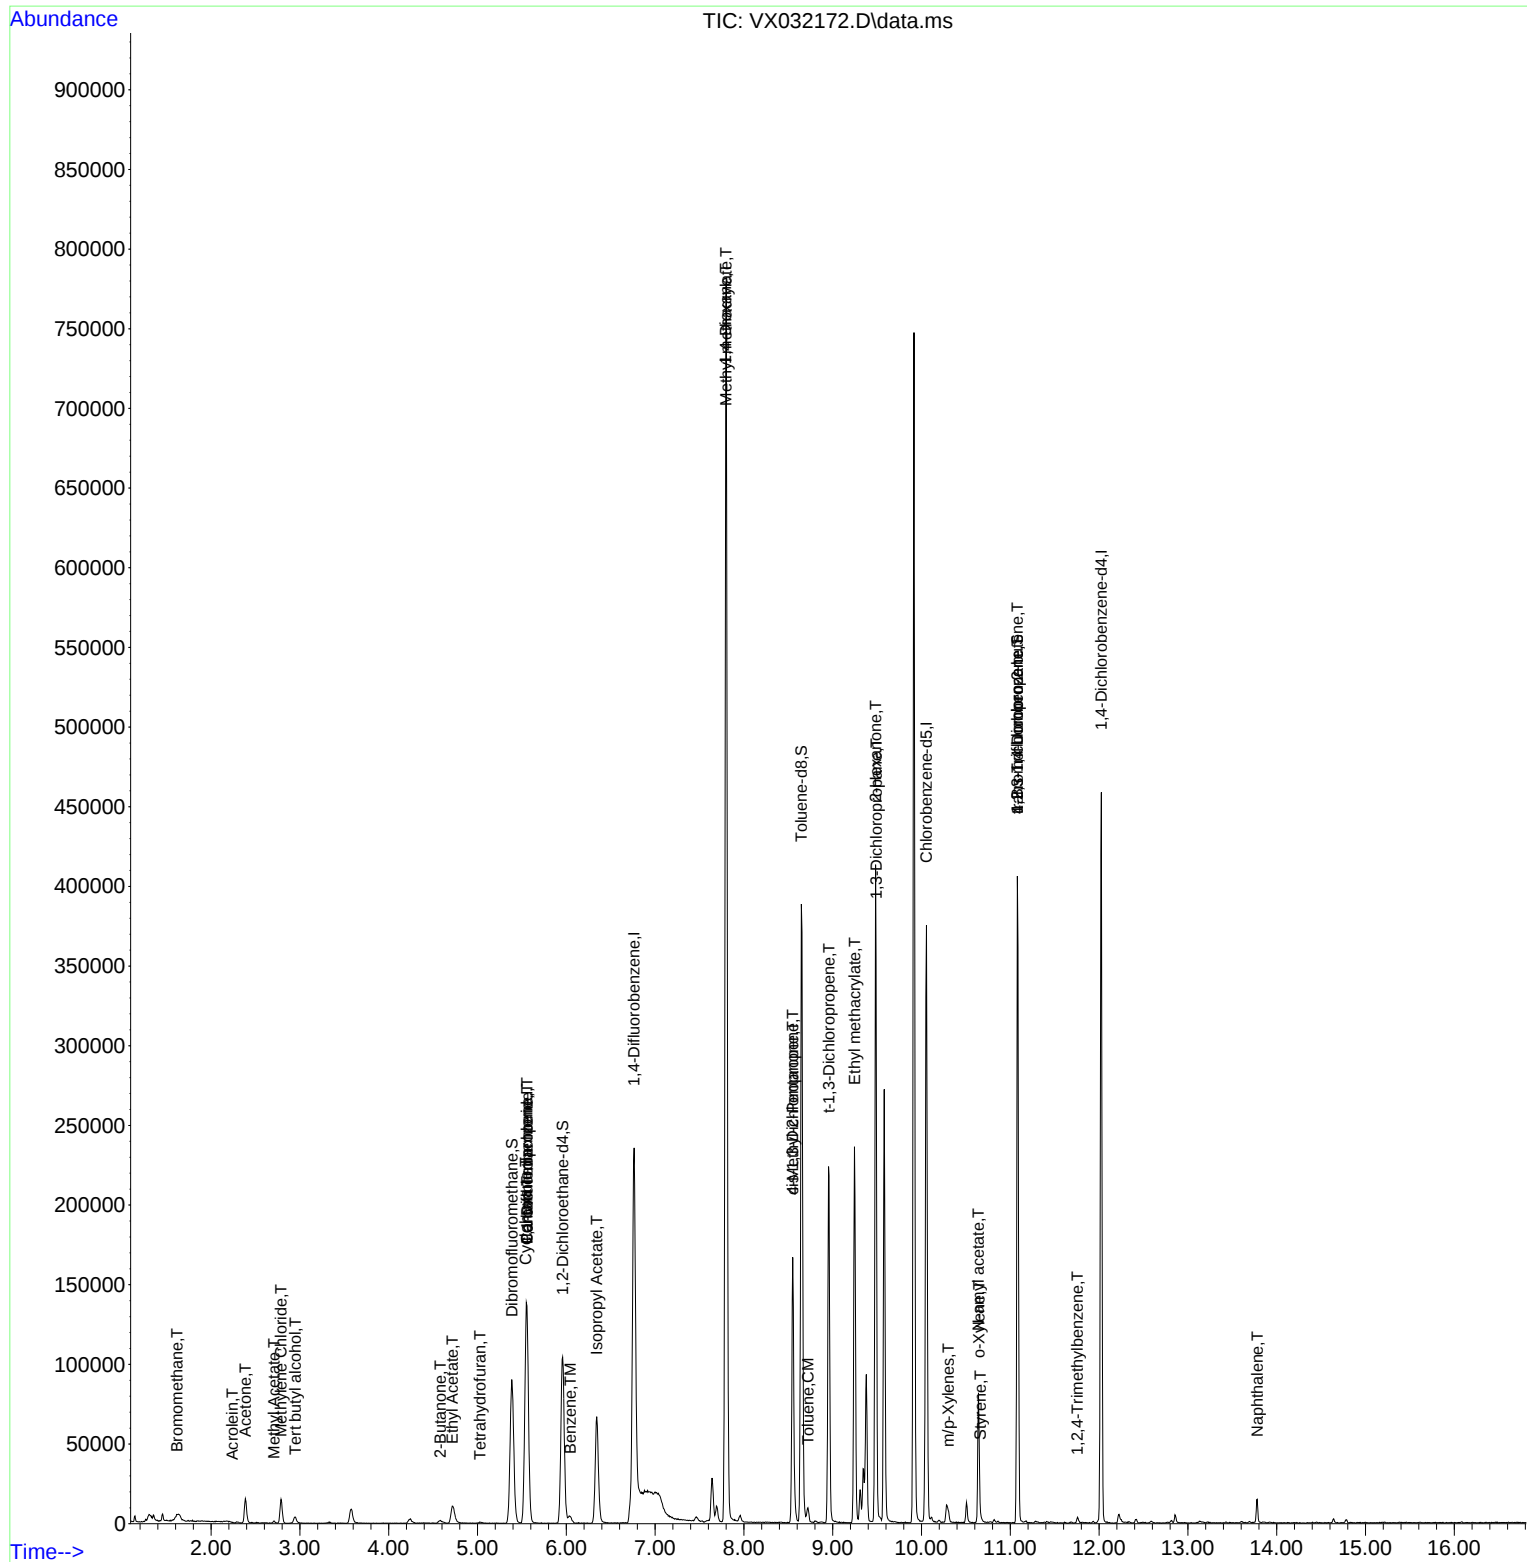




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28




Instrument :
MSVOA_X
ClientSampleId :
SB-36


Tgt Ion:168 Resp: 122433
Ion Ratio Lower Upper
168 100
99 61.2 48.8 73.2

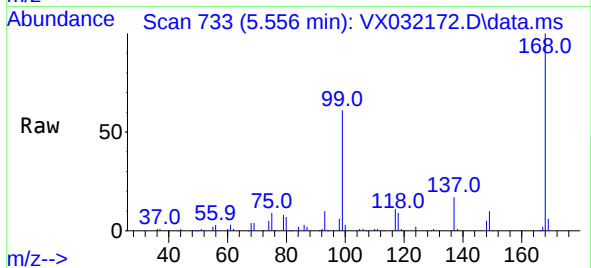

#5
Bromomethane
Concen: 0.443 ug/l
RT: 1.618 min Scan# 87
Delta R.T. 0.006 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28

Tgt Ion: 94 Resp: 476
Ion Ratio Lower Upper
94 100
96 65.7 74.4 111.6#


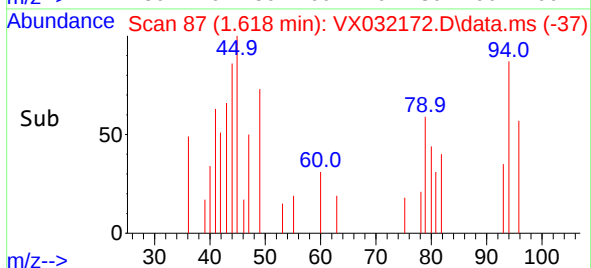
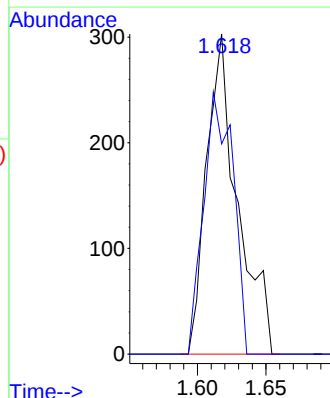





#11
Tert butyl alcohol
Concen: 9.370 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.048 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28




Instrument :
MSVOA_X
ClientSampleId :
SB-36


Tgt Ion: 59 Resp: 2513
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#

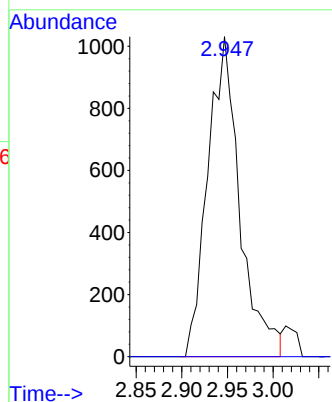

#13
Acrolein
Concen: 0.651 ug/l
RT: 2.240 min Scan# 189
Delta R.T. 0.006 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28

Tgt Ion: 56 Resp: 147
Ion Ratio Lower Upper
56 100
55 59.2 56.0 84.0



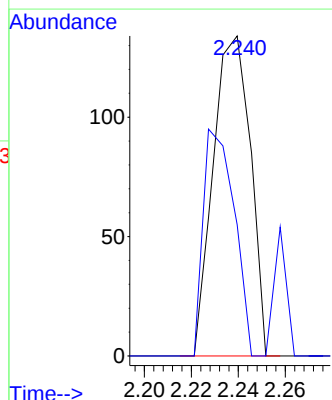





#16
Acetone
Concen: 38.822 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28




Instrument :
MSVOA_X
ClientSampleId :
SB-36


Tgt Ion: 43 Resp: 18202
Ion Ratio Lower Upper
43 100
58 30.4 23.8 35.8

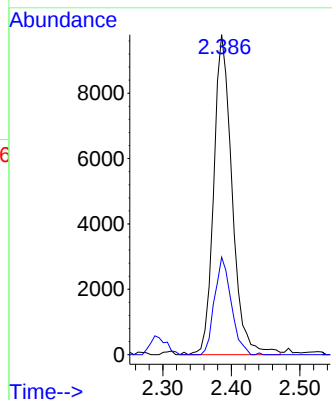

#18
Methyl Acetate
Concen: 0.929 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.006 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28

Tgt Ion: 43 Resp: 1773
Ion Ratio Lower Upper
43 100
74 16.9 18.6 27.8#


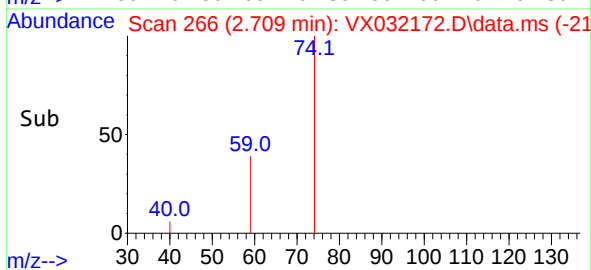
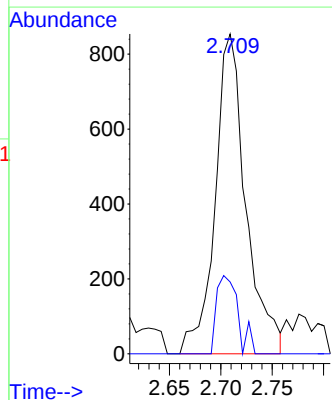





#20
Methylene Chloride
Concen: 4.587 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28




Instrument :
MSVOA_X
ClientSampleId :
SB-36


Tgt Ion: 84 Resp: 6612
Ion Ratio Lower Upper
84 100
49 129.0 105.9 158.9
51 29.5 32.2 48.2#
86 59.5 50.8 76.2

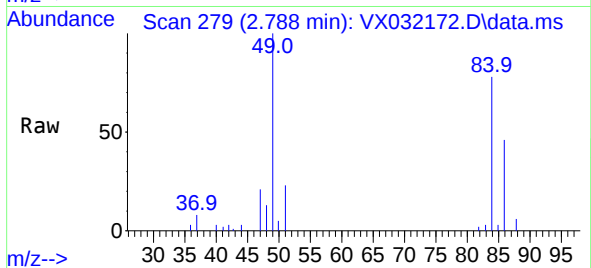

#25
2-Butanone
Concen: 2.413 ug/l
RT: 4.581 min Scan# 573
Delta R.T. 0.025 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28

Tgt Ion: 43 Resp: 2417
Ion Ratio Lower Upper
43 100
72 38.5 21.1 31.7#

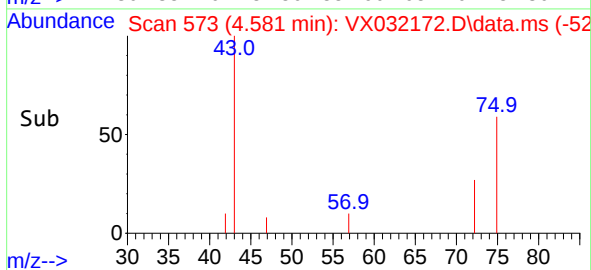







#29
Tetrahydrofuran
Concen: 1.095 ug/l
RT: 5.026 min Scan# 642
Delta R.T. 0.025 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28

Instrument :
MSVOA_X
ClientSampleId :
SB-36

Tgt Ion: 42 Resp: 658




Ion	Ratio	Lower	Upper
42	100		
72	12.6	36.4	54.6#
71	16.9	33.5	50.3#

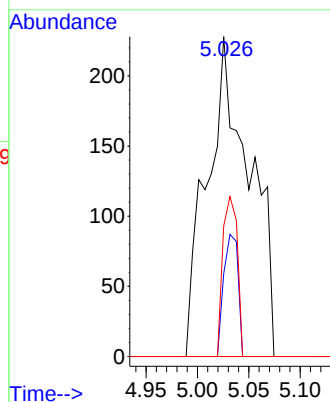


#31
Cyclohexane
Concen: 1.507 ug/l
RT: 5.544 min Scan# 731
Delta R.T. 0.073 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28

Tgt Ion: 56 Resp: 3274

Ion	Ratio	Lower	Upper
56	100		
69	133.6	25.1	37.7#
84	105.4	70.2	105.4

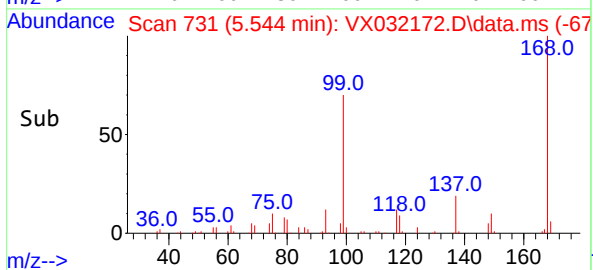



#33

1,2-Dichloroethane-d4

Concen: 54.198 ug/l

RT: 5.958 min Scan# 798

Delta R.T. 0.006 min

Lab File: VX032172.D

Acq: 17 Oct 2022 22:28

Instrument :

MSVOA_X

ClientSampleId :





SB-36

Tgt Ion: 65 Resp: 105686

Ion Ratio Lower Upper

65 100

67 50.4 0.0 102.4

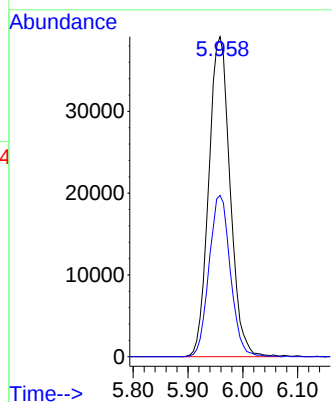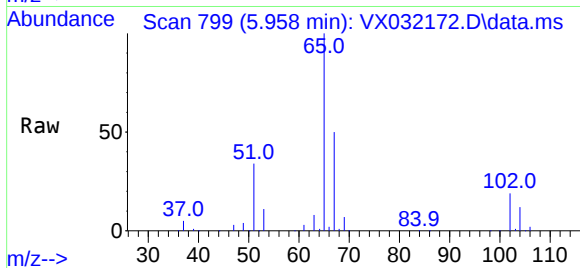

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.006 min

Lab File: VX032172.D

Acq: 17 Oct 2022 22:28




Tgt Ion: 114 Resp: 216075


Ion Ratio Lower Upper

114 100

63 20.2 0.0 42.6

88 16.2 0.0 33.0

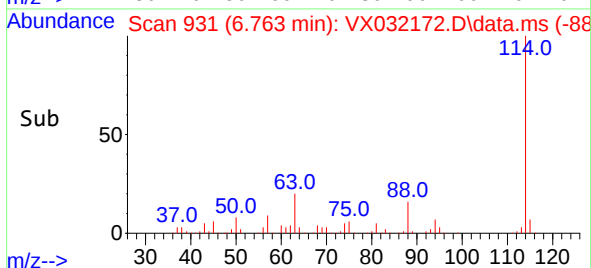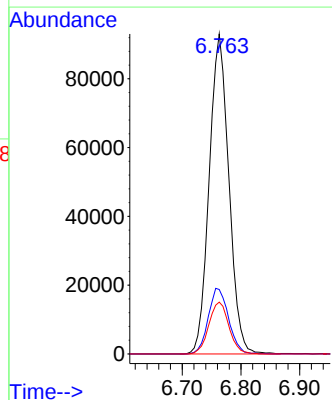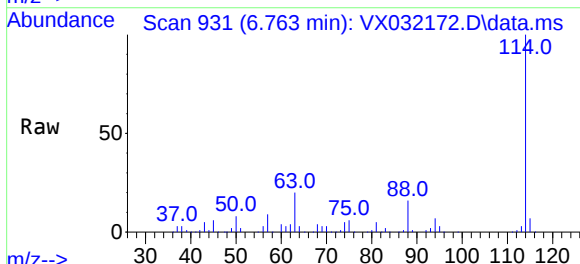

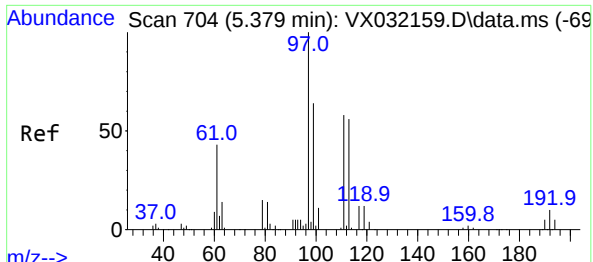

#35

Dibromofluoromethane

Concen: 51.346 ug/l

RT: 5.385 min Scan# 704

Delta R.T. 0.006 min

Lab File: VX032172.D

Acq: 17 Oct 2022 22:28

Instrument :

MSVOA_X

ClientSampleId :

SB-36





Tgt Ion:113 Resp: 75701

Ion Ratio Lower Upper

113 100

111 102.2 82.4 123.6

192 17.7 14.1 21.1

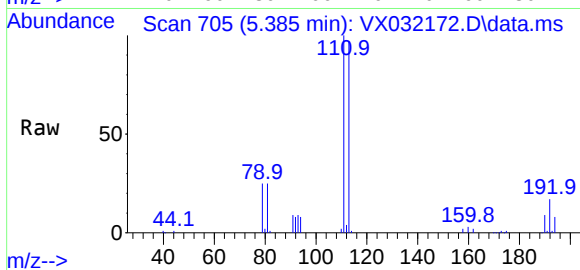

#36

1,1-Dichloropropene

Concen: 5.339 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.134 min

Lab File: VX032172.D

Acq: 17 Oct 2022 22:28




Tgt Ion: 75 Resp: 11389


Ion Ratio Lower Upper

75 100

110 9.8 17.5 52.5#

77 0.0 24.9 37.3#


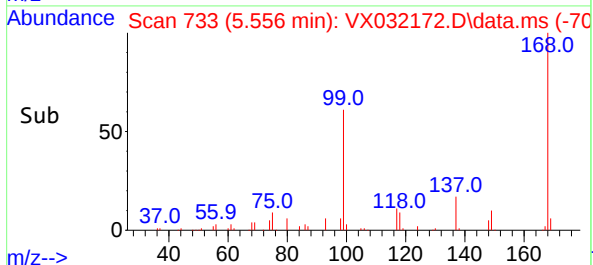
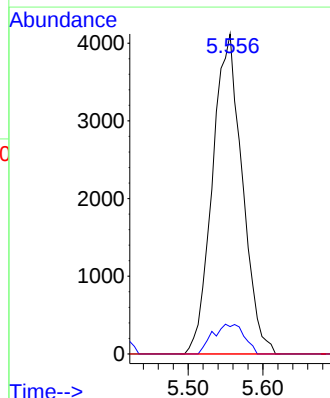
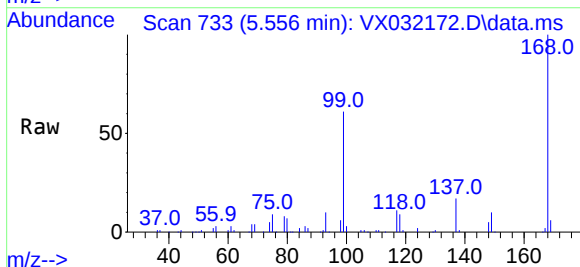




#37
Ethyl Acetate
Concen: 9.330 ug/l
RT: 4.715 min Scan# 51
Delta R.T. 0.006 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28




Instrument :
MSVOA_X
ClientSampleId :
SB-36


Tgt Ion: 43	Resp: 19970
Ion Ratio	Lower Upper
43 100	
61 13.4	11.1 16.7
70 11.4	8.6 13.0



#38
Carbon Tetrachloride
Concen: 6.184 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.116 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28

Tgt Ion: 117	Resp: 13968
Ion Ratio	Lower Upper
117 100	
119 5.8	74.6 112.0#
121 0.0	25.3 37.9#


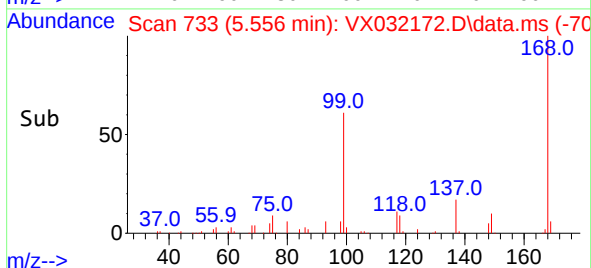
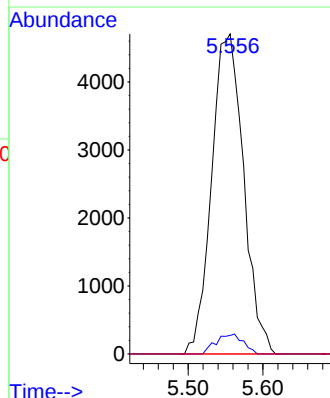





#40
Benzene
Concen: 0.835 ug/l
RT: 6.044 min Scan# 812
Delta R.T. 0.006 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28




Instrument :
MSVOA_X
ClientSampleId :
SB-36


Tgt Ion: 78 Resp: 4982
Ion Ratio Lower Upper
78 100
77 16.8 18.7 28.1#

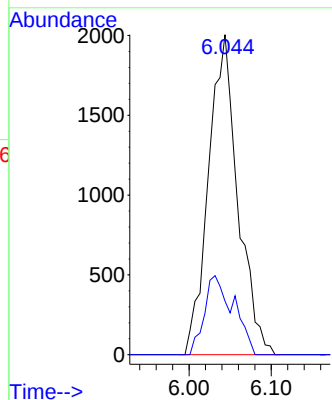

#43
Isopropyl Acetate
Concen: 27.765 ug/l
RT: 6.342 min Scan# 862
Delta R.T. 0.006 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28

Tgt Ion: 43 Resp: 89556
Ion Ratio Lower Upper
43 100
61 18.4 15.3 22.9
87 13.0 10.6 15.8


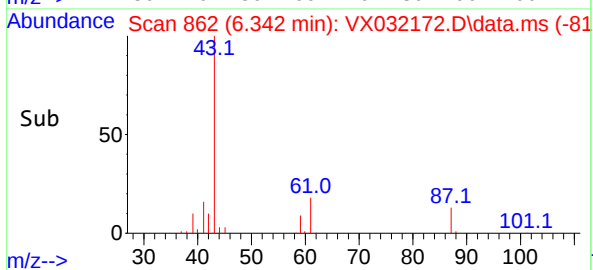
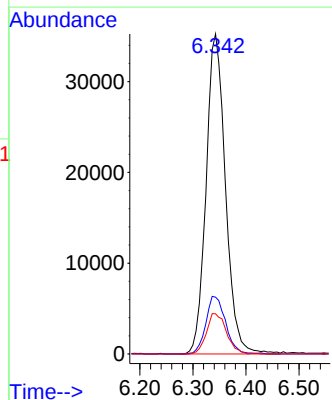
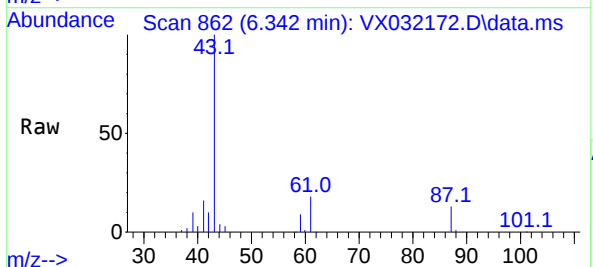




#48
Methyl methacrylate
Concen: 40.404 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.109 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28




Instrument :
MSVOA_X
ClientSampleId :
SB-36


Tgt Ion: 41 Resp: 66049
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 57.2 51.4 77.0

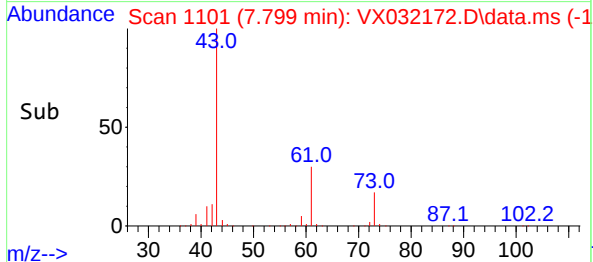

#49
1,4-Dioxane
Concen: 1.253 ug/l
RT: 7.793 min Scan# 1100
Delta R.T. 0.109 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28

Tgt Ion: 88 Resp: 42
Ion Ratio Lower Upper
88 100
43 1627114.3 27.1 40.7#
58 7526.2 53.9 80.9#

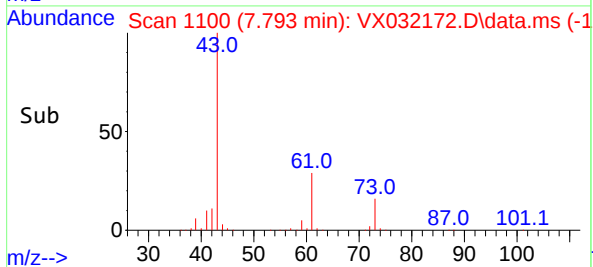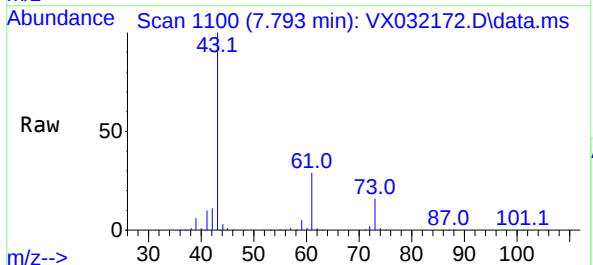



#50

Toluene-d8

Concen: 43.890 ug/l

RT: 8.647 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX032172.D

Acq: 17 Oct 2022 22:28

Instrument :

MSVOA_X

ClientSampleId :





SB-36

Tgt Ion: 98 Resp: 226966

Ion Ratio Lower Upper

98 100

100 66.1 52.5 78.7



#51

4-Methyl-2-Pentanone

Concen: 28.942 ug/l

RT: 8.549 min Scan# 1224

Delta R.T. -0.025 min

Lab File: VX032172.D




Acq: 17 Oct 2022 22:28


Tgt Ion: 43 Resp: 57245

Ion Ratio Lower Upper

43 100

58 8.8 30.6 46.0#


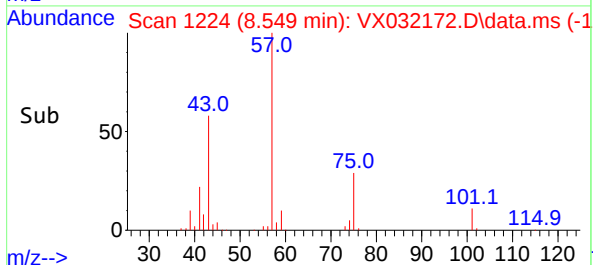
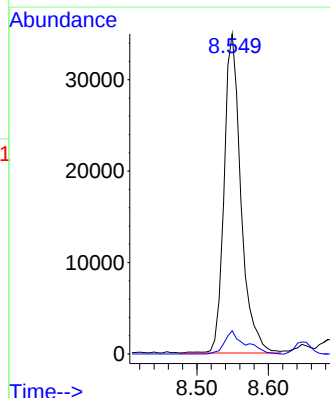
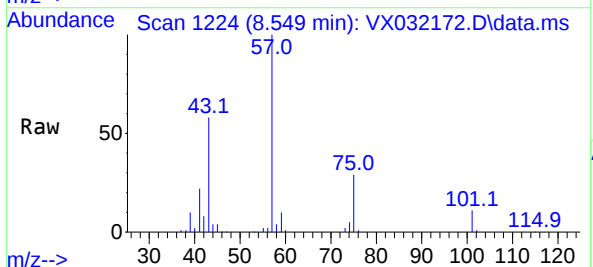




#52
Toluene
Concen: 0.900 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.000 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28




Instrument :
MSVOA_X
ClientSampleId :
SB-36


Tgt Ion: 92 Resp: 3423
Ion Ratio Lower Upper
92 100
91 163.3 137.1 205.7



#53
t-1,3-Dichloropropene
Concen: 0.280 ug/l
RT: 8.958 min Scan# 1291
Delta R.T. -0.018 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28

Tgt Ion: 75 Resp: 532
Ion Ratio Lower Upper
75 100
77 0.0 24.8 37.2#


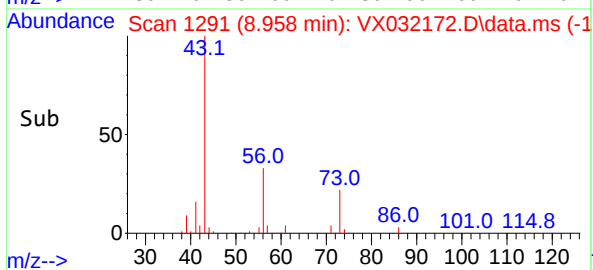






#54
cis-1,3-Dichloropropene
Concen: 11.695 ug/l
RT: 8.549 min Scan# 11
Delta R.T. 0.183 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28




Instrument :
MSVOA_X
ClientSampleId :
SB-36


Tgt Ion: 75 Resp: 26058
Ion Ratio Lower Upper
75 100
77 0.0 24.4 36.6#
39 34.9 43.7 65.5#

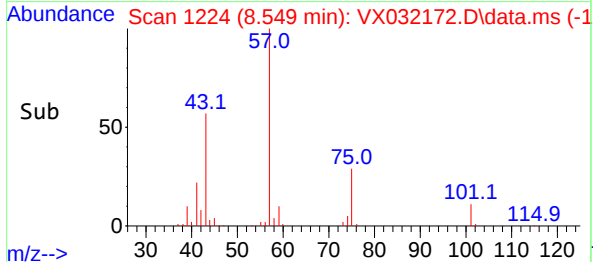

#56
Ethyl methacrylate
Concen: 0.291 ug/l
RT: 9.244 min Scan# 1338
Delta R.T. 0.128 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28

Tgt Ion: 69 Resp: 600
Ion Ratio Lower Upper
69 100
41 6125.3 54.2 81.4#
39 2838.2 34.2 51.2#


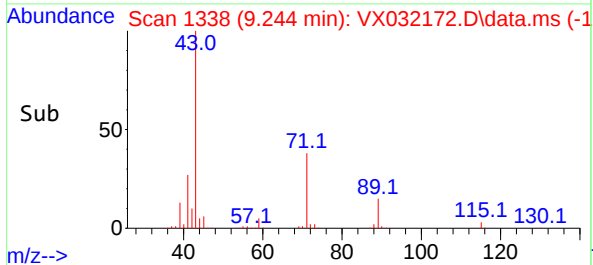

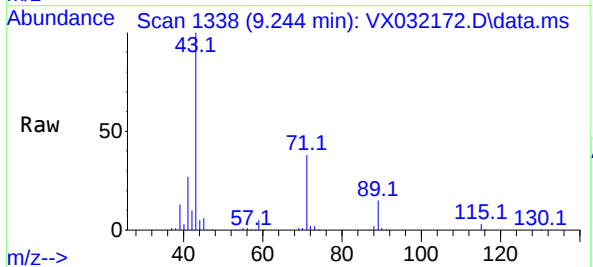




#57
1,3-Dichloropropane
Concen: 1.400 ug/l
RT: 9.488 min Scan# 11
Delta R.T. 0.183 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28




Instrument :
MSVOA_X
ClientSampleId :
SB-36


Tgt Ion: 76 Resp: 3541
Ion Ratio Lower Upper
76 100
78 0.0 25.5 38.3#

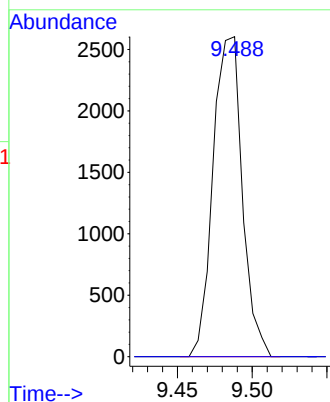

#59
2-Hexanone
Concen: 31.638 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.055 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28

Tgt Ion: 43 Resp: 46361
Ion Ratio Lower Upper
43 100
58 19.5 26.7 80.0#









#62
4-Bromofluorobenzene
Concen: 52.132 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28




Instrument :
MSVOA_X
ClientSampleId :
SB-36


Tgt Ion: 95 Resp: 102642
Ion Ratio Lower Upper
95 100
174 74.1 0.0 153.2
176 70.5 0.0 144.0

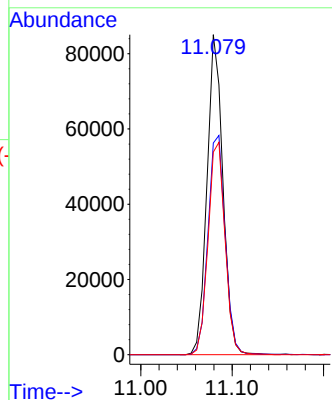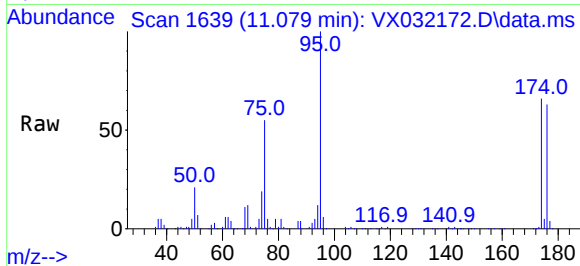

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28

Tgt Ion: 117 Resp: 163374
Ion Ratio Lower Upper
117 100
82 53.5 46.8 70.2
119 31.7 26.4 39.6


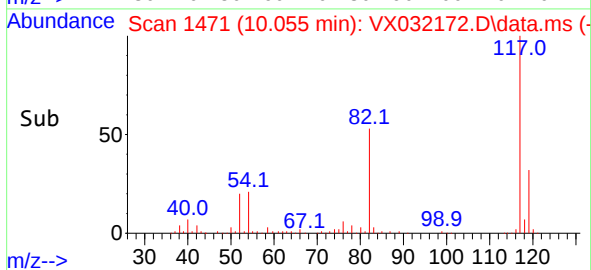
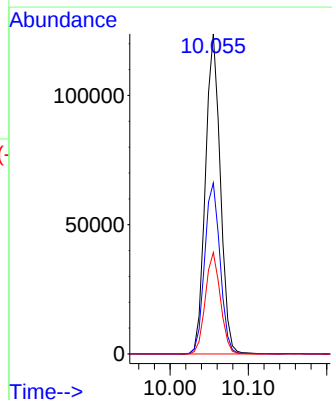
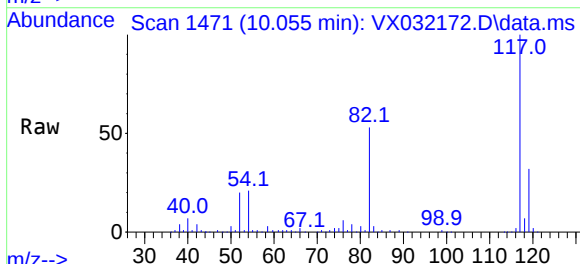




#68
m/p-Xylenes
Concen: 0.617 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. 0.000 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28




Instrument :
MSVOA_X
ClientSampleId :
SB-36


Tgt Ion:106 Resp: 1492
Ion Ratio Lower Upper
106 100
91 208.1 161.0 241.4

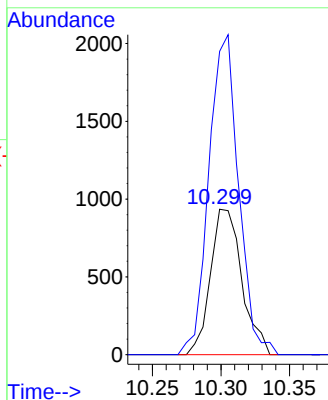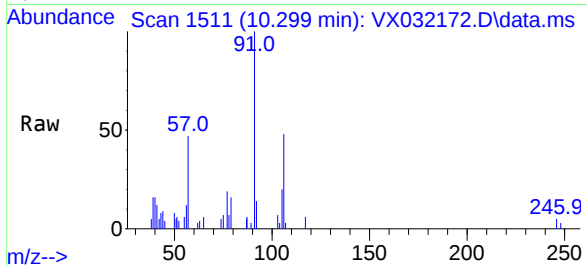

#69
o-Xylene
Concen: 0.374 ug/l
RT: 10.647 min Scan# 1568
Delta R.T. 0.007 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28

Tgt Ion:106 Resp: 890
Ion Ratio Lower Upper
106 100
91 248.3 107.2 321.6


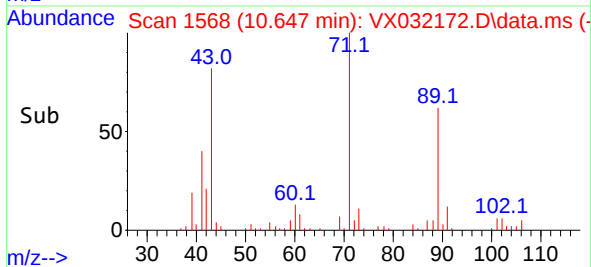
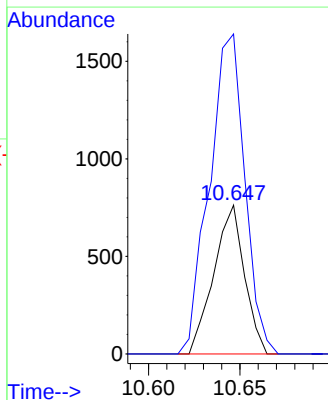
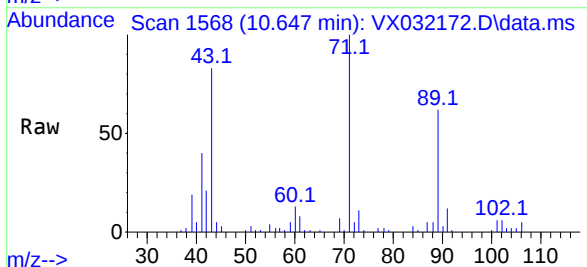




#70
Styrene
Concen: 0.222 ug/l
RT: 10.659 min Scan# 1569
Delta R.T. 0.006 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28




Instrument :
MSVOA_X
ClientSampleId :
SB-36


Tgt Ion:104 Resp: 853
Ion Ratio Lower Upper
104 100
78 71.5 41.4 62.2#
103 73.6 43.8 65.8#

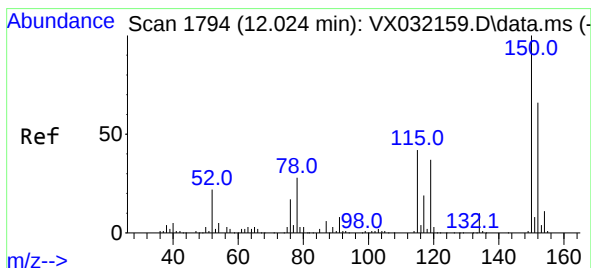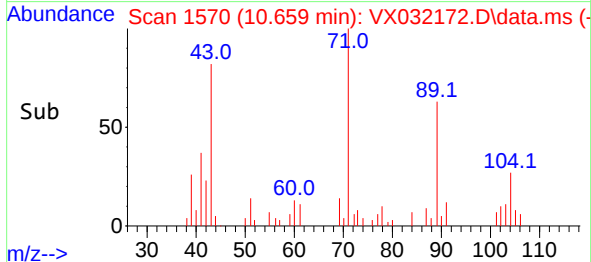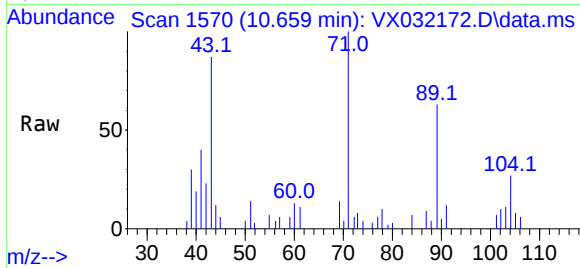

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28

Tgt Ion:152 Resp: 87848
Ion Ratio Lower Upper
152 100
115 64.2 43.4 130.1
150 159.3 0.0 346.8


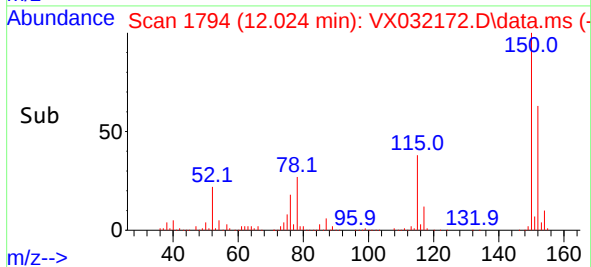

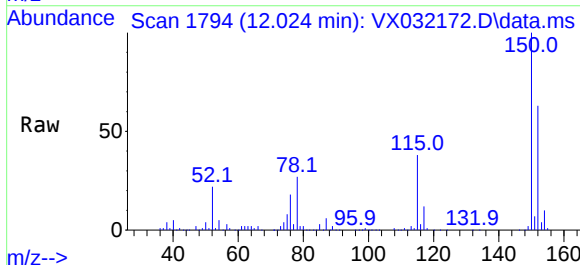




#74
N-amy1 acetate
Concen: 8.168 ug/l
RT: 10.640 min Scan# 1639
Delta R.T. -0.202 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28




Instrument :
MSVOA_X
ClientSampleId :
SB-36


Tgt Ion: 43	Resp: 18995
Ion Ratio	Lower Upper
43 100	
70 1.7	33.4 50.2#
55 4.9	18.2 27.2#
61 10.1	19.3 28.9#



#76
1,2,3-Trichloropropane
Concen: 29.861 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28

Tgt Ion: 75	Resp: 56878
Ion Ratio	Lower Upper
75 100	
77 1.1	20.3 60.9#


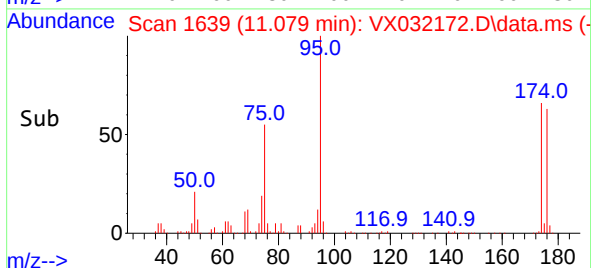
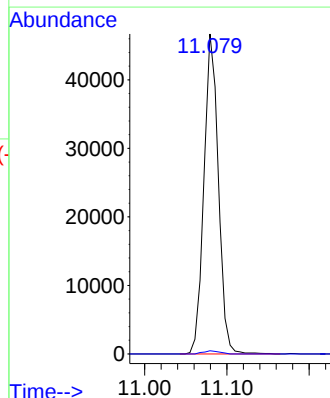





#81
 trans-1,4-Dichloro-2-butene
 Concen: 114.954 ug/l
 RT: 11.079 min Scan# 1
 Delta R.T. 0.061 min
 Lab File: VX032172.D
 Acq: 17 Oct 2022 22:28




Instrument :
 MSVOA_X
 ClientSampleId :
 SB-36


Tgt Ion: 75 Resp: 56878
 Ion Ratio Lower Upper
 75 100
 53 0.0 77.6 116.4#
 89 0.0 37.4 56.0#

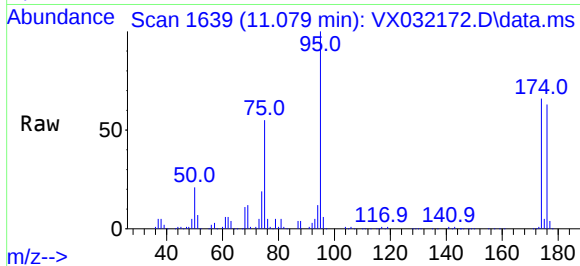

#84
 1,2,4-Trimethylbenzene
 Concen: 0.261 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. 0.006 min
 Lab File: VX032172.D
 Acq: 17 Oct 2022 22:28


Tgt Ion: 105 Resp: 1537
 Ion Ratio Lower Upper
 105 100
 120 25.6 22.6 67.8

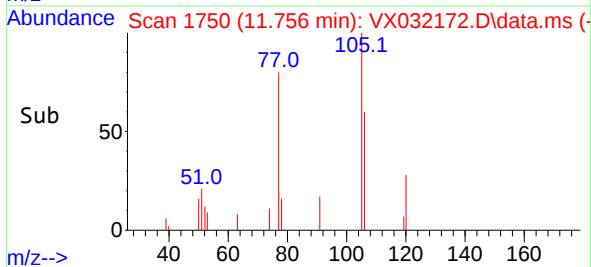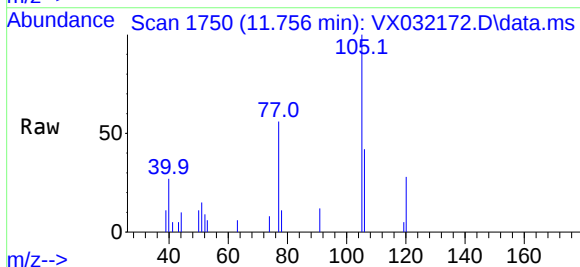

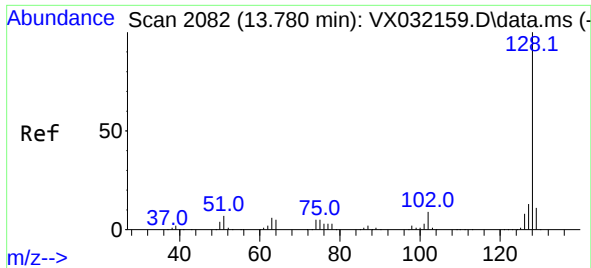

#95
Naphthalene
Concen: 1.612 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX032172.D
Acq: 17 Oct 2022 22:28

Instrument :
MSVOA_X
ClientSampleId :
SB-36

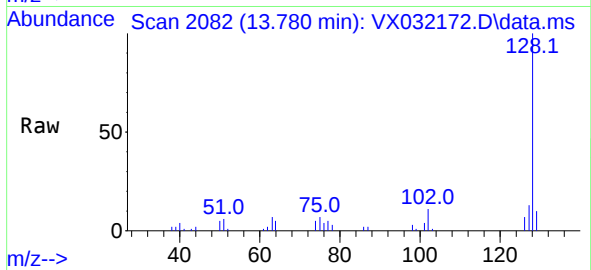

Tgt Ion:	128	Resp:	8936
Ion	Ratio	Lower	Upper
128	100		
127	12.9	10.4	15.6
129	10.6	8.8	13.2

