

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101722\
 Data File : VX032179.D
 Acq On : 18 Oct 2022 01:11
 Operator : JC/MD
 Sample : N5159-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-43

Quant Time: Oct 18 04:34:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 18 04:18:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	123232	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	176548	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	202901	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	91483	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	84031	42.814	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	85.620%
35) Dibromofluoromethane	5.385	113	71721	59.538	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	119.080%
50) Toluene-d8	8.647	98	270353	63.985	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	127.980%#
62) 4-Bromofluorobenzene	11.079	95	100643	62.561	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	125.120%#


Target Compounds				Qvalue		
5) Bromomethane	1.618	94	360	0.333	ug/l #	80
11) Tert butyl alcohol	2.947	59	3668	13.588	ug/l #	73
13) Acrolein	2.239	56	167	0.735	ug/l	85
16) Acetone	2.386	43	17930	37.994	ug/l	95
18) Methyl Acetate	2.709	43	1917	0.997	ug/l	99
20) Methylene Chloride	2.794	84	7206	4.966	ug/l	89
25) 2-Butanone	4.587	43	2043	2.026	ug/l #	85
29) Tetrahydrofuran	5.013	42	226	0.374	ug/l #	67
31) Cyclohexane	5.556	56	3278	1.499	ug/l #	40
36) 1,1-Dichloropropene	5.550	75	11155	6.401	ug/l #	50
37) Ethyl Acetate	4.715	43	19782	11.311	ug/l	99
38) Carbon Tetrachloride	5.556	117	13847	7.502	ug/l #	16
40) Benzene	6.050	78	3882	0.796	ug/l #	88
43) Isopropyl Acetate	6.342	43	69449	26.351	ug/l	98
48) Methyl methacrylate	7.799	41	67151	50.275	ug/l #	46
49) 1,4-Dioxane	7.793	88	73	2.666	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	77401	47.893	ug/l #	47
52) Toluene	8.720	92	4103	1.321	ug/l	98
53) t-1,3-Dichloropropene	8.952	75	538	0.347	ug/l #	44
54) cis-1,3-Dichloropropene	8.549	75	31984	17.569	ug/l #	69
56) Ethyl methacrylate	9.244	69	719	0.427	ug/l #	1
57) 1,3-Dichloropropane	9.482	76	4466	2.160	ug/l #	43
59) 2-Hexanone	9.482	43	60433	50.475	ug/l #	52
68) m/p-Xylenes	10.305	106	1708	0.568	ug/l	93
69) o-Xylene	10.646	106	1087	0.368	ug/l	83
70) Styrene	10.659	104	1456	0.305	ug/l	91
74) N-amyl acetate	10.640	43	18721	7.731	ug/l #	53
76) 1,2,3-Trichloropropane	11.079	75	57186	28.829	ug/l #	37
81) trans-1,4-Dichloro-2-b...	11.079	75	57186	110.984	ug/l #	11
84) 1,2,4-Trimethylbenzene	11.756	105	1602	0.261	ug/l #	60
85) sec-Butylbenzene	11.756	105	1602	0.213	ug/l #	56
95) Naphthalene	13.780	128	12918	2.238	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101722\
Data File : VX032179.D
Acq On : 18 Oct 2022 01:11
Operator : JC/MD
Sample : N5159-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-43


Quant Time: Oct 18 04:34:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101722W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 18 04:18:35 2022
Response via : Initial Calibration

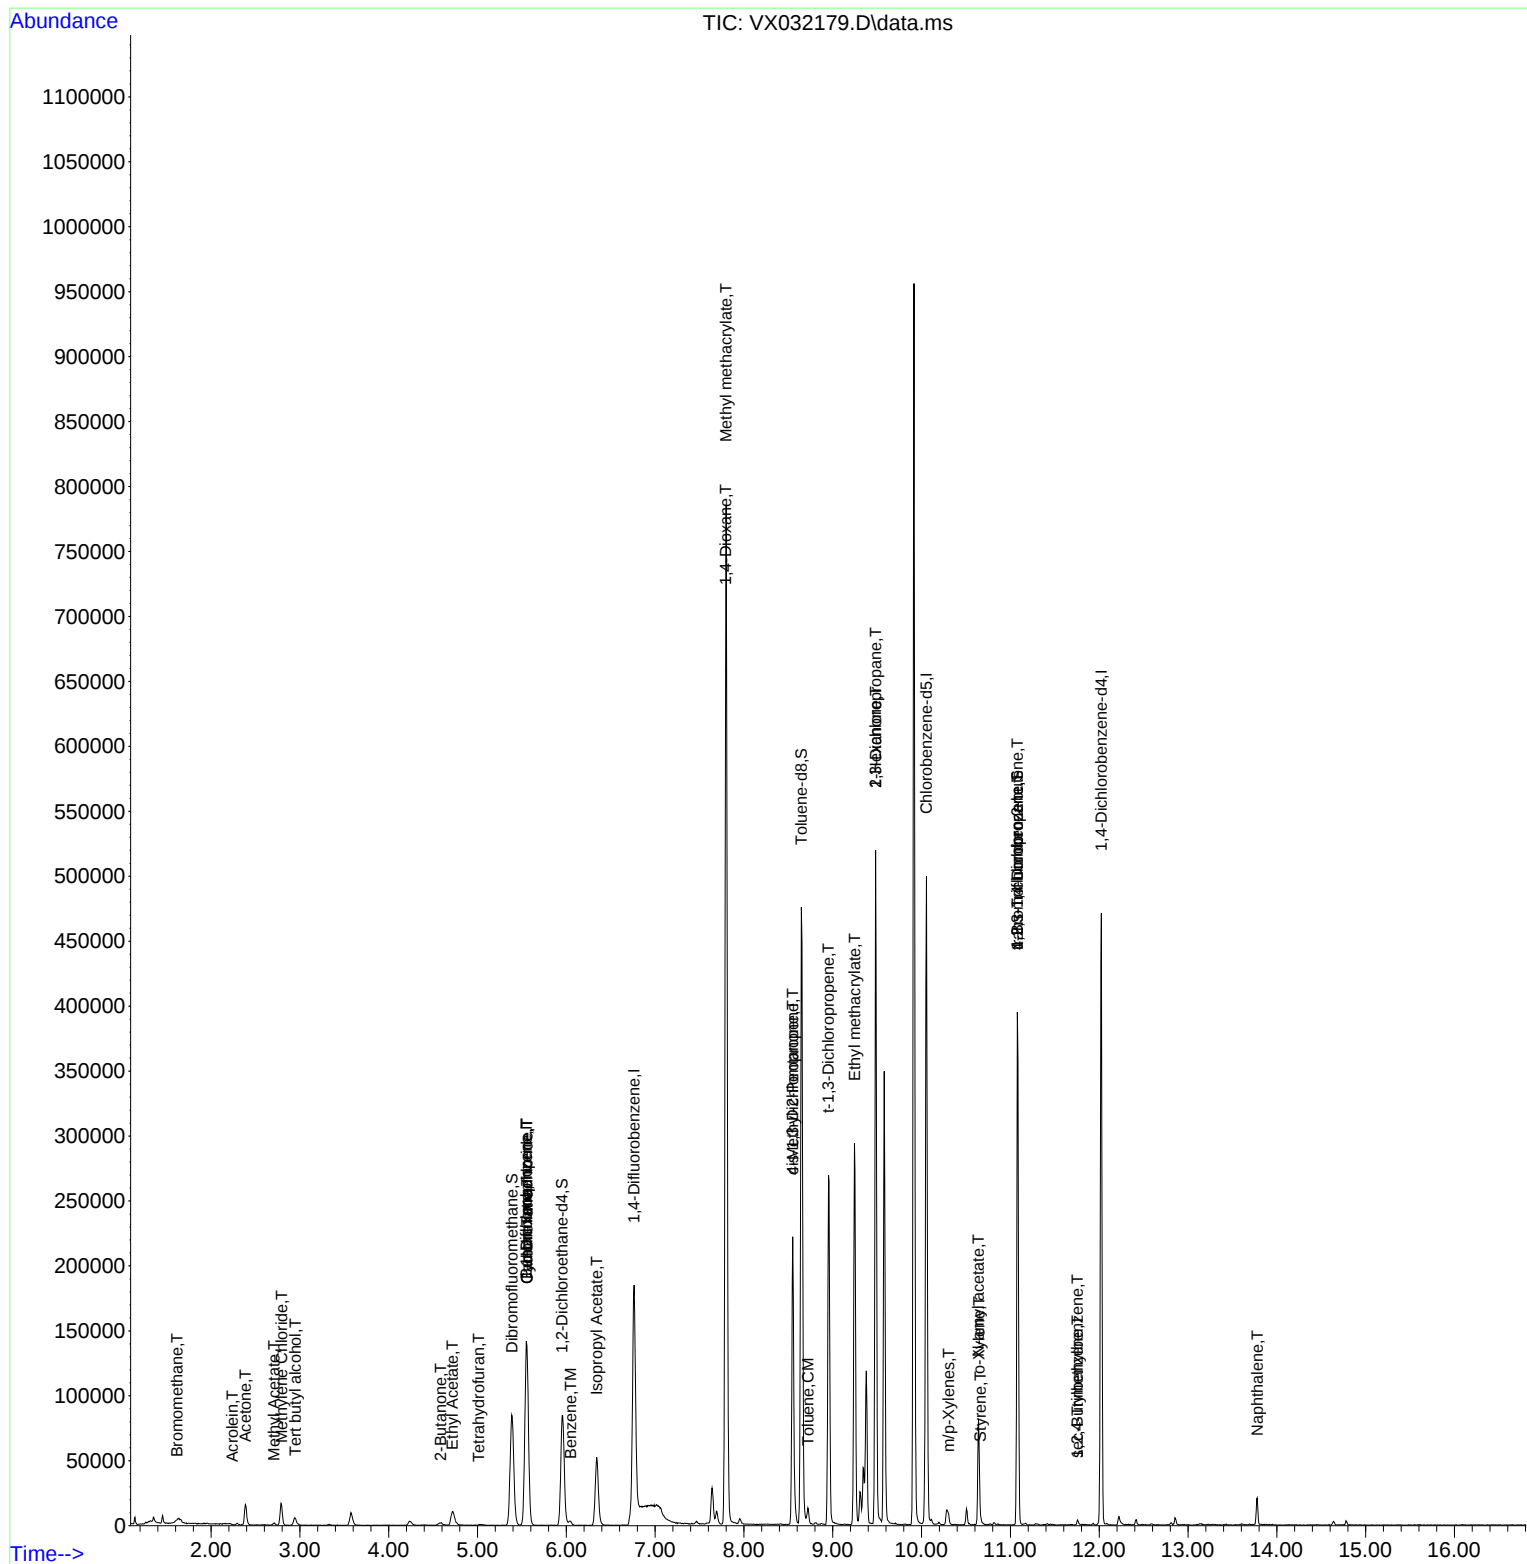






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11

Instrument :
MSVOA_X
ClientSampleId :
SB-43







Tgt Ion:168 Resp: 123232
Ion Ratio Lower Upper
168 100
99 67.1 48.8 73.2

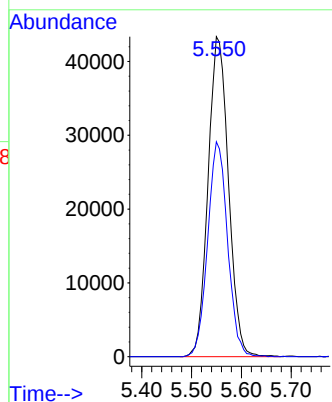

#5
Bromomethane
Concen: 0.333 ug/l
RT: 1.618 min Scan# 87
Delta R.T. 0.006 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11

Tgt Ion: 94 Resp: 360
Ion Ratio Lower Upper
94 100
96 73.8 74.4 111.6#

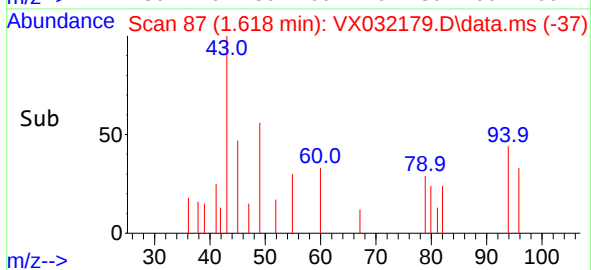



#11

Tert butyl alcohol

Concen: 13.588 ug/l

RT: 2.947 min Scan# 305

Delta R.T. -0.048 min

Lab File: VX032179.D

Acq: 18 Oct 2022 01:11

Instrument :

MSVOA_X

ClientSampleId :





SB-43

Tgt Ion: 59 Resp: 3668

Ion Ratio Lower Upper

59 100

57 0.0 8.2 12.2#

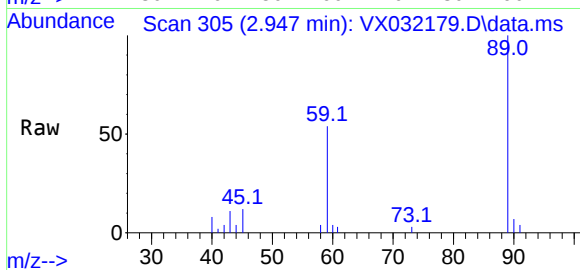

#13

Acrolein

Concen: 0.735 ug/l

RT: 2.239 min Scan# 189

Delta R.T. 0.006 min

Lab File: VX032179.D




Acq: 18 Oct 2022 01:11


Tgt Ion: 56 Resp: 167

Ion Ratio Lower Upper

56 100

55 82.6 56.0 84.0


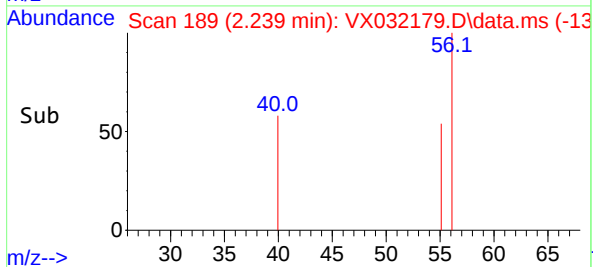

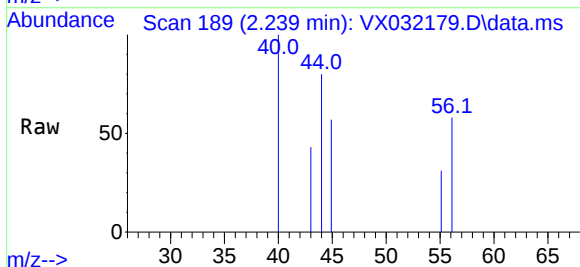




#16
Acetone
Concen: 37.994 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11




Instrument : MSVOA_X
ClientSampleId : SB-43


Tgt Ion: 43 Resp: 17930
Ion Ratio Lower Upper
43 100
58 27.2 23.8 35.8



#18
Methyl Acetate
Concen: 0.997 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.006 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11

Tgt Ion: 43 Resp: 1917
Ion Ratio Lower Upper
43 100
74 23.7 18.6 27.8

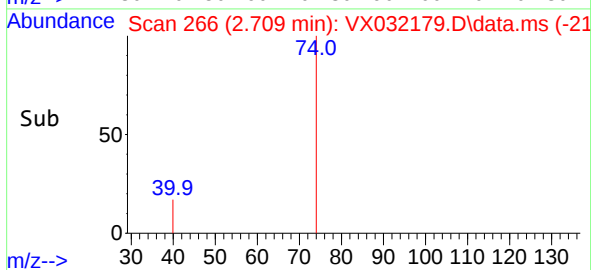







#20
Methylene Chloride
Concen: 4.966 ug/l
RT: 2.794 min Scan# 21
Delta R.T. 0.012 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11

Instrument :
MSVOA_X
ClientSampleId :
SB-43

Tgt Ion: 84 Resp: 7206




Ion	Ratio	Lower	Upper
84	100		
49	113.6	105.9	158.9
51	37.2	32.2	48.2
86	59.4	50.8	76.2




#25
2-Butanone
Concen: 2.026 ug/l
RT: 4.587 min Scan# 574
Delta R.T. 0.030 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11

Tgt Ion: 43 Resp: 2043

Ion	Ratio	Lower	Upper
43	100		
72	18.5	21.1	31.7#









#29
Tetrahydrofuran
Concen: 0.374 ug/l
RT: 5.013 min Scan# 642
Delta R.T. 0.012 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11




Instrument :
MSVOA_X
ClientSampleId :
SB-43


Tgt Ion:	42	Resp:	226
Ion	Ratio	Lower	Upper
42	100		
72	46.9	36.4	54.6
71	0.0	33.5	50.3#

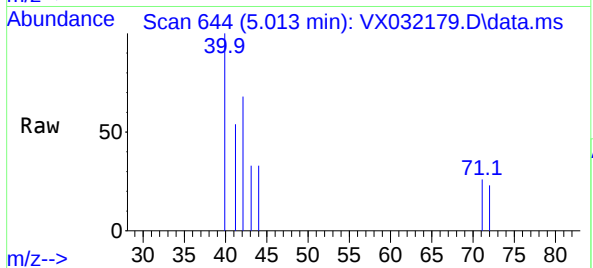

#31
Cyclohexane
Concen: 1.499 ug/l
RT: 5.556 min Scan# 733
Delta R.T. 0.085 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11

Tgt Ion:	56	Resp:	3278
Ion	Ratio	Lower	Upper
56	100		
69	128.4	25.1	37.7#
84	105.2	70.2	105.4


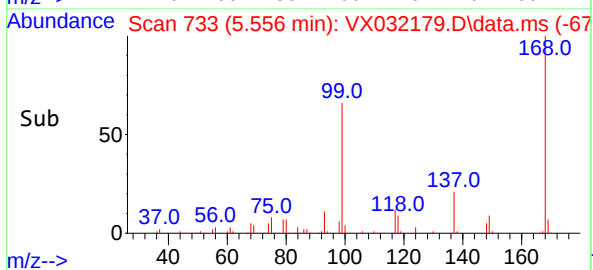






#33
 1,2-Dichloroethane-d4
 Concen: 42.814 ug/l
 RT: 5.952 min Scan# 798
 Delta R.T. 0.000 min
 Lab File: VX032179.D
 Acq: 18 Oct 2022 01:11




Instrument :
 MSVOA_X
 ClientSampleId :
 SB-43


Tgt Ion: 65 Resp: 84031
 Ion Ratio Lower Upper
 65 100
 67 50.0 0.0 102.4

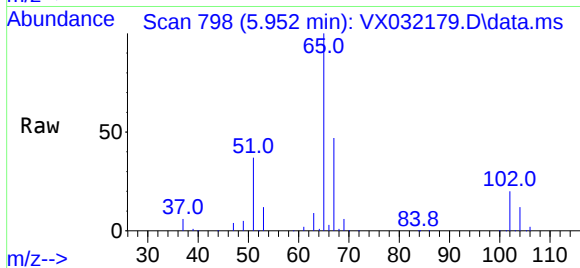

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.763 min Scan# 931
 Delta R.T. 0.006 min
 Lab File: VX032179.D
 Acq: 18 Oct 2022 01:11

Tgt Ion: 114 Resp: 176548
 Ion Ratio Lower Upper
 114 100
 63 18.6 0.0 42.6
 88 15.3 0.0 33.0


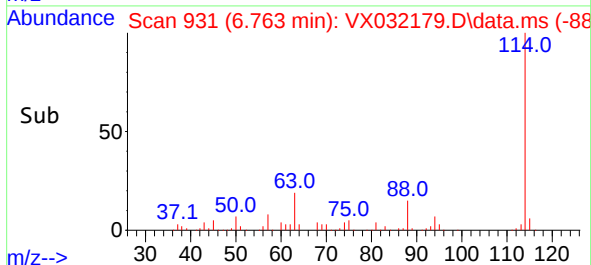
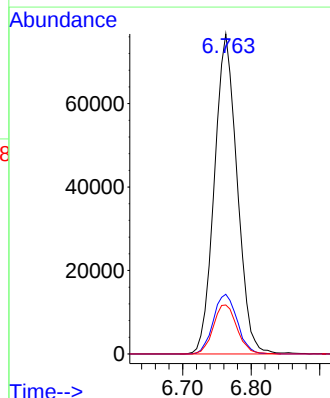
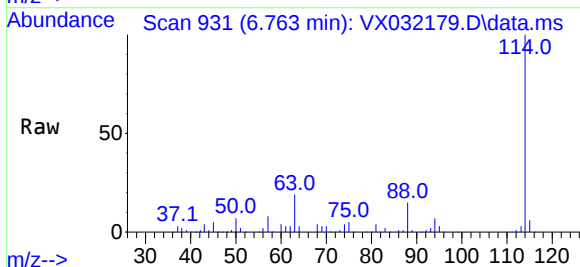


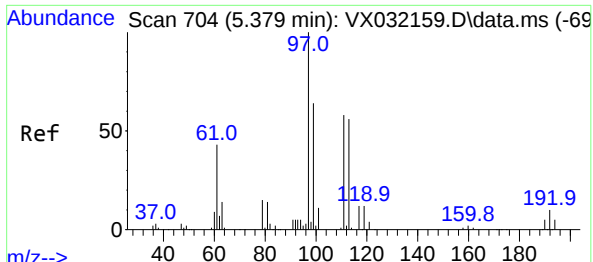

#35
Dibromofluoromethane
Concen: 59.538 ug/l
RT: 5.385 min Scan# 704
Delta R.T. 0.006 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11




Instrument :
MSVOA_X
ClientSampleId :
SB-43


Tgt Ion:113 Resp: 71721
Ion Ratio Lower Upper
113 100
111 104.4 82.4 123.6
192 17.9 14.1 21.1

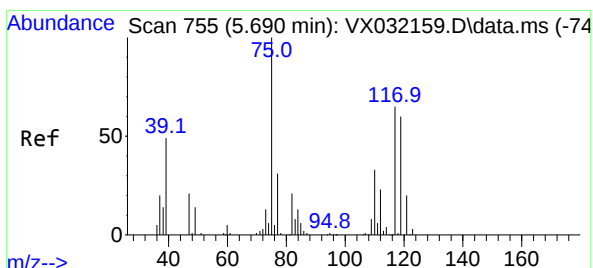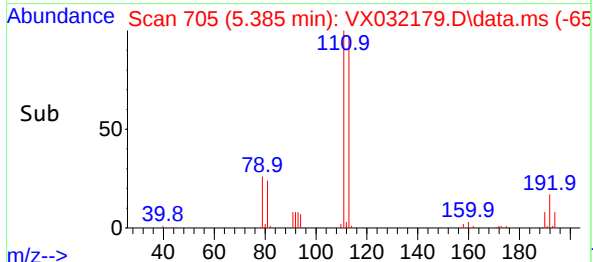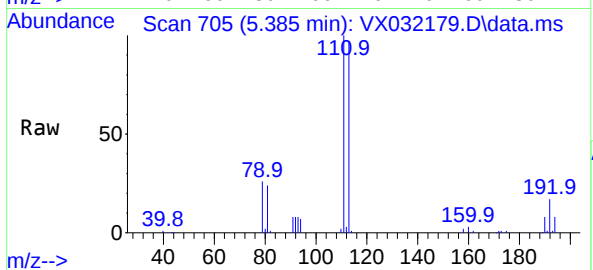

#36
1,1-Dichloropropene
Concen: 6.401 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.140 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11

Tgt Ion: 75 Resp: 11155
Ion Ratio Lower Upper
75 100
110 9.3 17.5 52.5#
77 0.0 24.9 37.3#


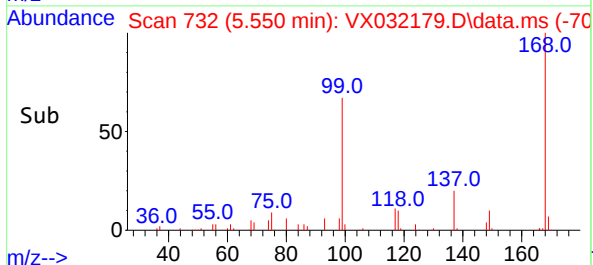

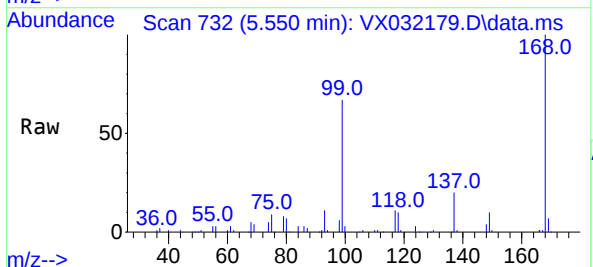




#37
Ethyl Acetate
Concen: 11.311 ug/l
RT: 4.715 min Scan# 594
Delta R.T. 0.006 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11




Instrument :
MSVOA_X
ClientSampleId :
SB-43


Tgt Ion:	43	Resp:	19782
Ion	Ratio	Lower	Upper
43	100		
61	14.3	11.1	16.7
70	11.0	8.6	13.0



#38
Carbon Tetrachloride
Concen: 7.502 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.116 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11

Tgt Ion:	117	Resp:	13847
Ion	Ratio	Lower	Upper
117	100		
119	4.3	74.6	112.0#
121	0.0	25.3	37.9#



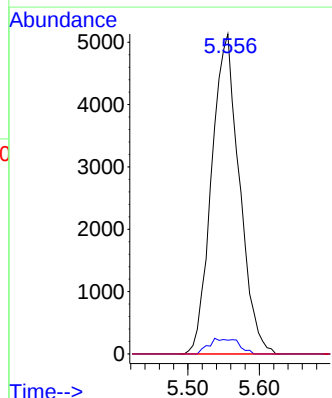





#40
Benzene
Concen: 0.796 ug/l
RT: 6.050 min Scan# 812
Delta R.T. 0.012 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11




Instrument :
MSVOA_X
ClientSampleId :
SB-43


Tgt Ion: 78 Resp: 3882
Ion Ratio Lower Upper
78 100
77 17.3 18.7 28.1#

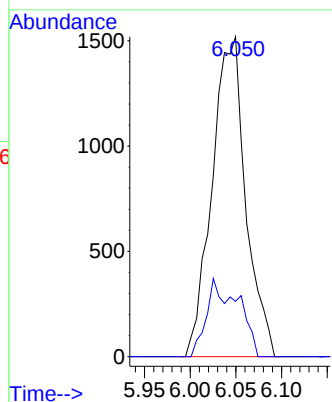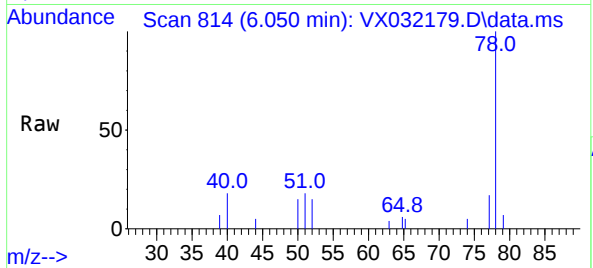

#43
Isopropyl Acetate
Concen: 26.351 ug/l
RT: 6.342 min Scan# 862
Delta R.T. 0.006 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11

Tgt Ion: 43 Resp: 69449
Ion Ratio Lower Upper
43 100
61 19.6 15.3 22.9
87 14.0 10.6 15.8


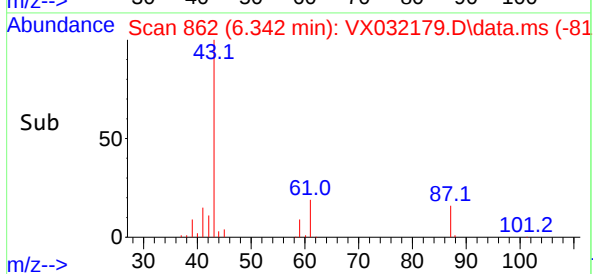






#48
Methyl methacrylate
Concen: 50.275 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.109 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11




Instrument :
MSVOA_X
ClientSampleId :
SB-43


Tgt Ion: 41 Resp: 67151
Ion Ratio Lower Upper
41 100
69 0.1 64.6 96.8#
39 57.4 51.4 77.0

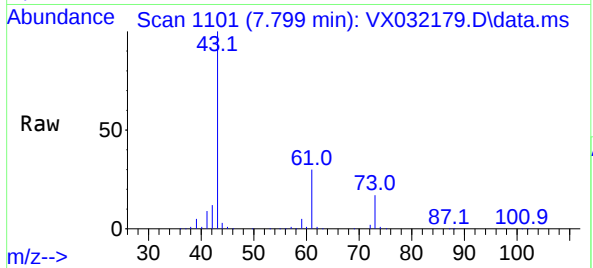

#49
1,4-Dioxane
Concen: 2.666 ug/l
RT: 7.793 min Scan# 1100
Delta R.T. 0.109 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11

Tgt Ion: 88 Resp: 73
Ion Ratio Lower Upper
88 100
43 942028.8 27.1 40.7#
58 4049.3 53.9 80.9#

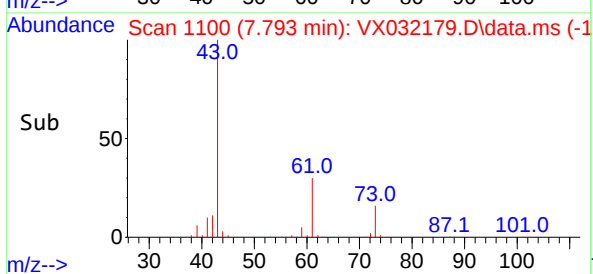



#50

Toluene-d8

Concen: 63.985 ug/l

RT: 8.647 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX032179.D

Acq: 18 Oct 2022 01:11

Instrument :

MSVOA_X

ClientSampleId :





SB-43

Tgt Ion: 98 Resp: 270353

Ion Ratio Lower Upper

98 100

100 66.1 52.5 78.7

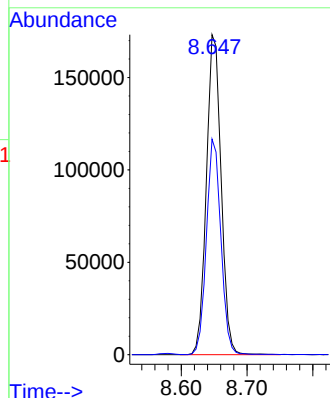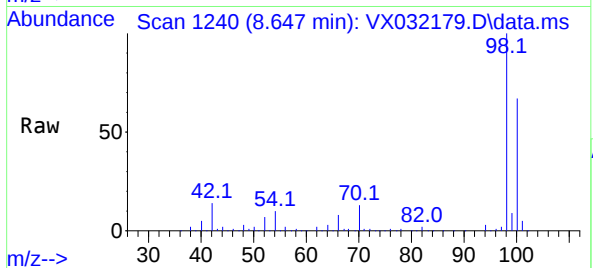

#51

4-Methyl-2-Pentanone

Concen: 47.893 ug/l

RT: 8.549 min Scan# 1224

Delta R.T. -0.025 min

Lab File: VX032179.D




Acq: 18 Oct 2022 01:11


Tgt Ion: 43 Resp: 77401

Ion Ratio Lower Upper

43 100

58 6.1 30.6 46.0#

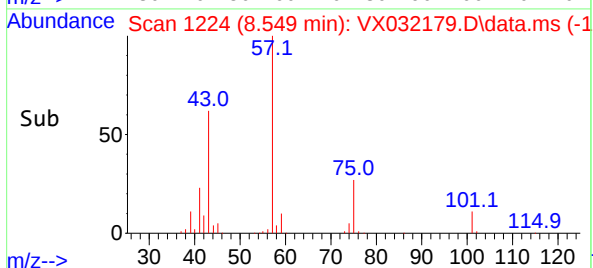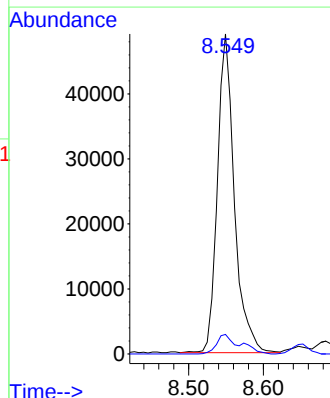



#52

Toluene

Concen: 1.321 ug/l

RT: 8.720 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX032179.D

Acq: 18 Oct 2022 01:11

Instrument :

MSVOA_X

ClientSampleId :


SB-43

Tgt Ion: 92 Resp: 4103




Ion Ratio Lower Upper

92 100

91 168.2 137.1 205.7

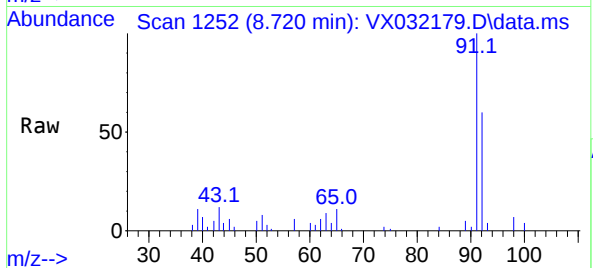

Abundance

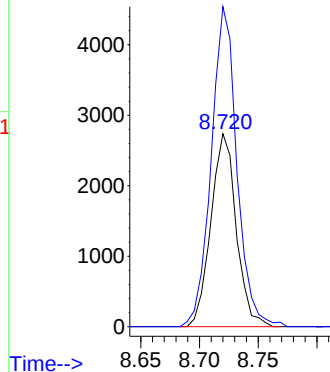

#53

t-1,3-Dichloropropene

Concen: 0.347 ug/l

RT: 8.952 min Scan# 1290

Delta R.T. -0.024 min

Lab File: VX032179.D


Acq: 18 Oct 2022 01:11

Tgt Ion: 75 Resp: 538



Ion Ratio Lower Upper


75 100

77 0.0 24.8 37.2#



Abundance



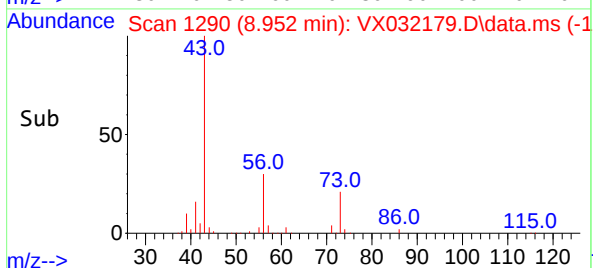
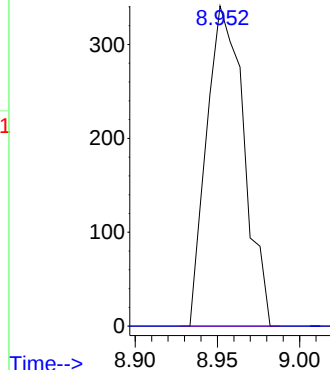




#54
cis-1,3-Dichloropropene
Concen: 17.569 ug/l
RT: 8.549 min Scan# 1194
Delta R.T. 0.183 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11




Instrument :
MSVOA_X
ClientSampleId :
SB-43


Tgt Ion: 75 Resp: 31984
Ion Ratio Lower Upper
75 100
77 0.6 24.4 36.6#
39 41.4 43.7 65.5#

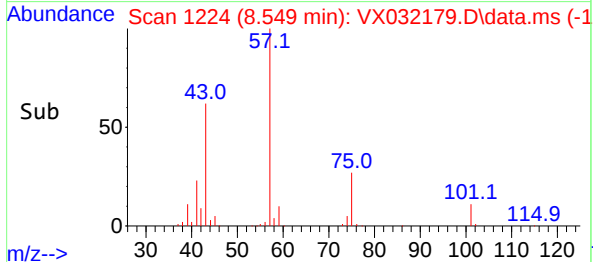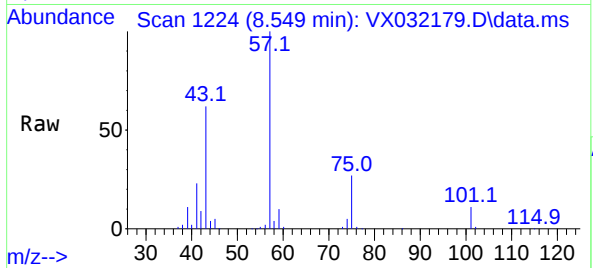

#56
Ethyl methacrylate
Concen: 0.427 ug/l
RT: 9.244 min Scan# 1338
Delta R.T. 0.128 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11

Tgt Ion: 69 Resp: 719
Ion Ratio Lower Upper
69 100
41 6816.6 54.2 81.4#
39 3070.2 34.2 51.2#


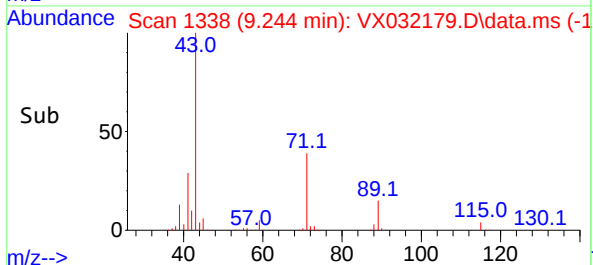
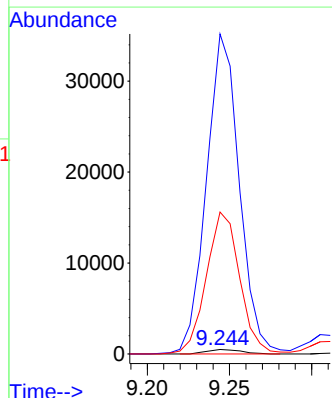
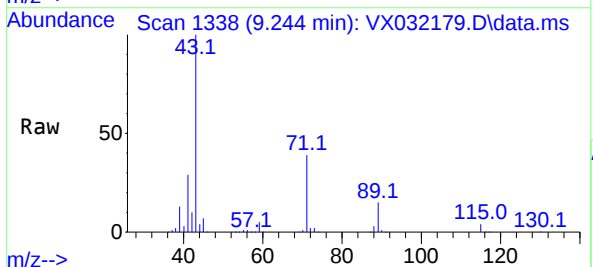


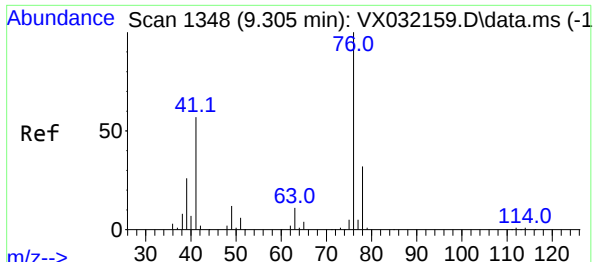

#57
1,3-Dichloropropane
Concen: 2.160 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.177 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11




Instrument :
MSVOA_X
ClientSampleId :
SB-43


Tgt Ion: 76 Resp: 4466
Ion Ratio Lower Upper
76 100
78 0.0 25.5 38.3#

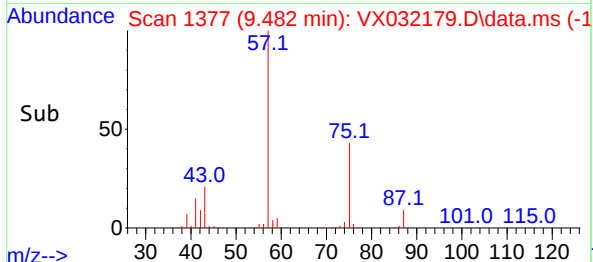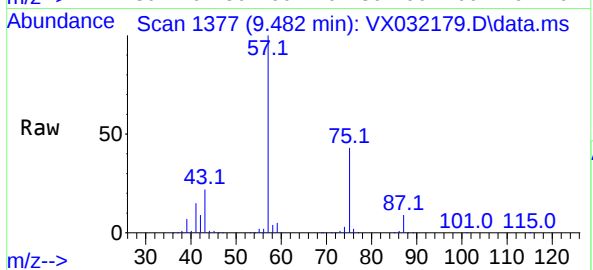

#59
2-Hexanone
Concen: 50.475 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.055 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11

Tgt Ion: 43 Resp: 60433
Ion Ratio Lower Upper
43 100
58 18.9 26.7 80.0#


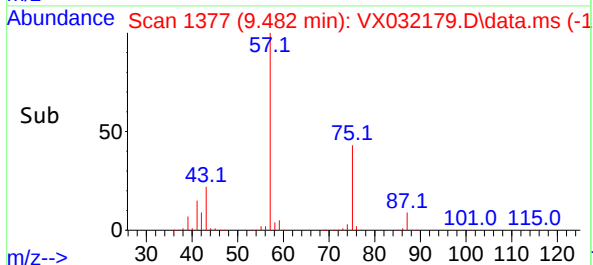

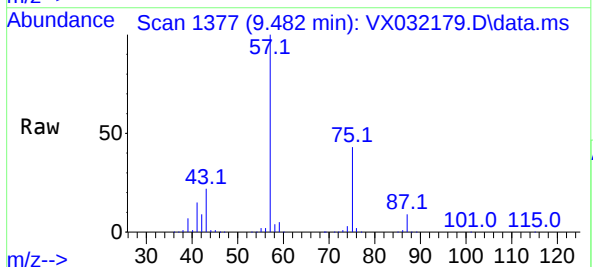




#62
4-Bromofluorobenzene
Concen: 62.561 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11




Instrument :
MSVOA_X
ClientSampleId :
SB-43


Tgt Ion: 95 Resp: 100643
Ion Ratio Lower Upper
95 100
174 72.6 0.0 153.2
176 71.8 0.0 144.0

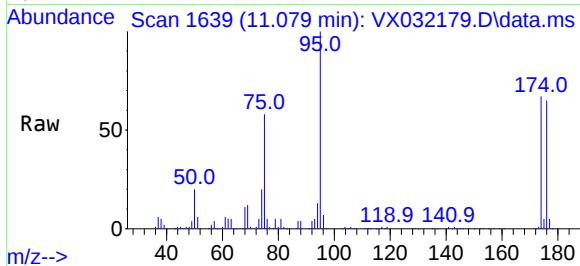

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11

Tgt Ion: 117 Resp: 202901
Ion Ratio Lower Upper
117 100
82 58.3 46.8 70.2
119 31.0 26.4 39.6



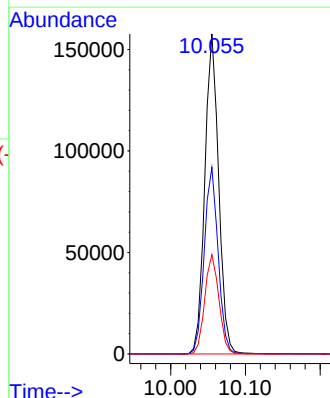
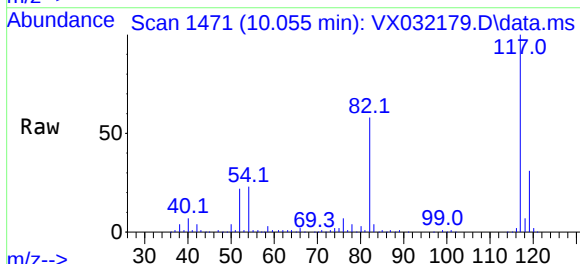




#68
m/p-Xylenes
Concen: 0.568 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11




Instrument :
MSVOA_X
ClientSampleId :
SB-43


Tgt Ion:106 Resp: 1708
Ion Ratio Lower Upper
106 100
91 211.1 161.0 241.4

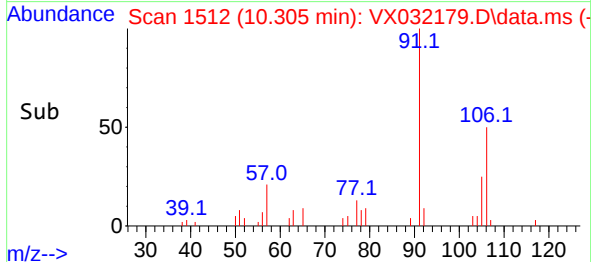

#69
o-Xylene
Concen: 0.368 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.006 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11

Tgt Ion:106 Resp: 1087
Ion Ratio Lower Upper
106 100
91 241.8 107.2 321.6


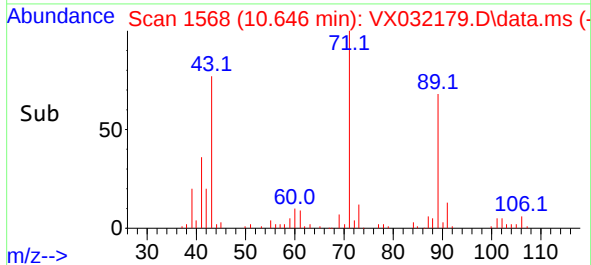

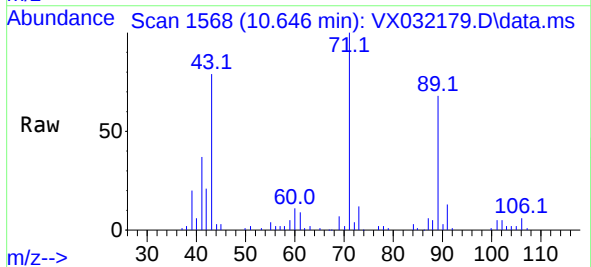




#70
Styrene
Concen: 0.305 ug/l
RT: 10.659 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11




Instrument :
MSVOA_X
ClientSampleId :
SB-43


Tgt Ion:104 Resp: 1456
Ion Ratio Lower Upper
104 100
78 57.9 41.4 62.2
103 61.7 43.8 65.8

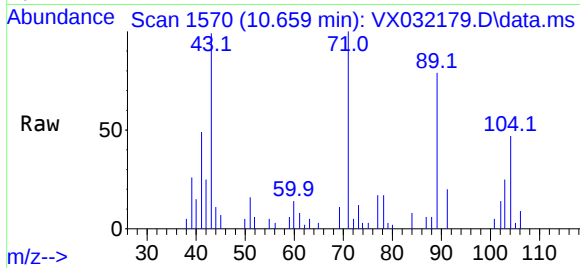

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11

Tgt Ion:152 Resp: 91483
Ion Ratio Lower Upper
152 100
115 62.4 43.4 130.1
150 155.0 0.0 346.8


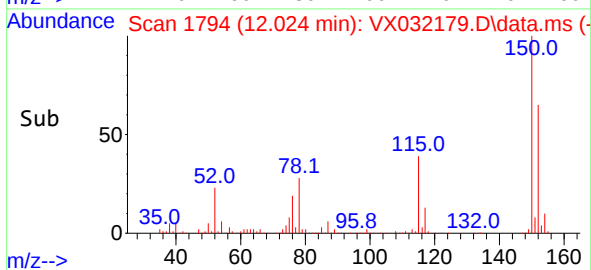

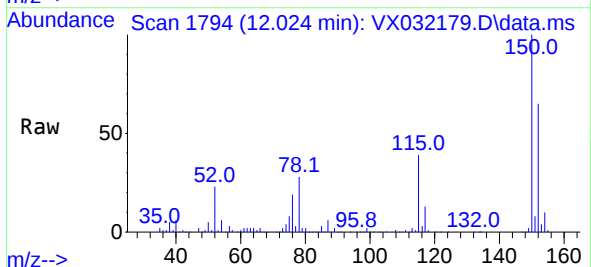




#74
N-amy1 acetate
Concen: 7.731 ug/l
RT: 10.640 min Scan# 1639
Delta R.T. -0.202 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11




Instrument :
MSVOA_X
ClientSampleId :
SB-43


Tgt Ion: 43	Resp: 18721
Ion Ratio	Lower Upper
43	100
70	1.8 33.4 50.2#
55	5.0 18.2 27.2#
61	10.2 19.3 28.9#

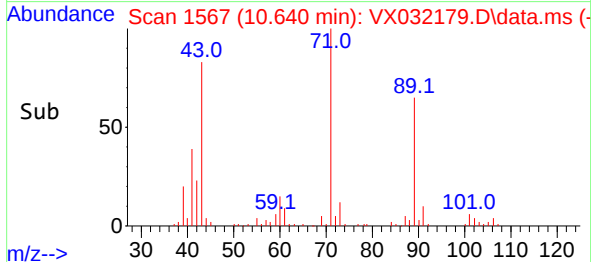

#76
1,2,3-Trichloropropane
Concen: 28.829 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11

Tgt Ion: 75	Resp: 57186
Ion Ratio	Lower Upper
75	100
77	1.2 20.3 60.9#


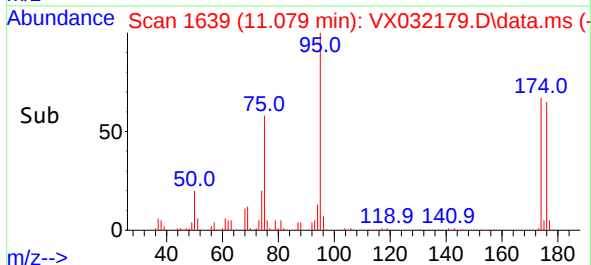
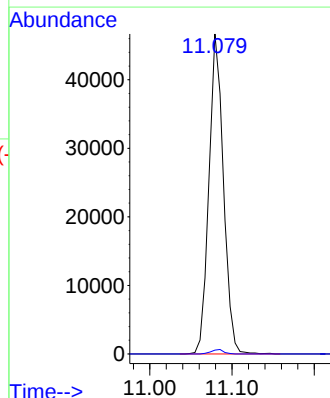
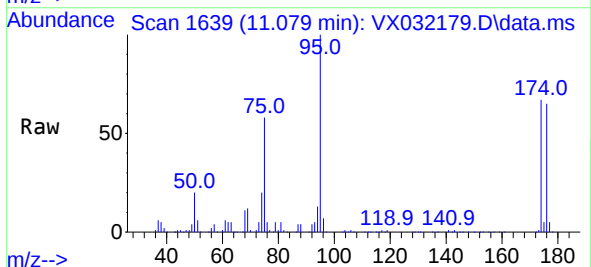




#81
trans-1,4-Dichloro-2-butene
Concen: 110.984 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11




Instrument :
MSVOA_X
ClientSampleId :
SB-43


Tgt Ion: 75 Resp: 57186
Ion Ratio Lower Upper
75 100
53 0.0 77.6 116.4#
89 0.0 37.4 56.0#

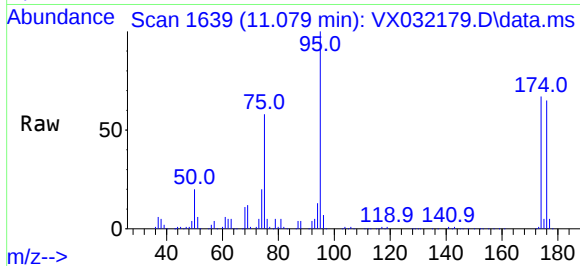

#84
1,2,4-Trimethylbenzene
Concen: 0.261 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11

Tgt Ion: 105 Resp: 1602
Ion Ratio Lower Upper
105 100
120 18.7 22.6 67.8#




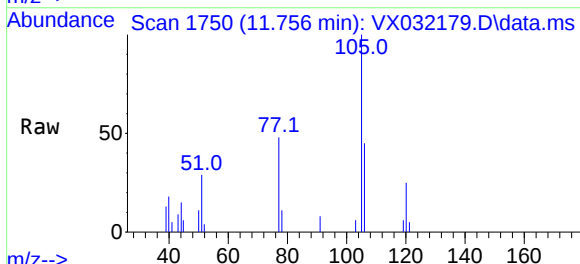




#85
sec-Butylbenzene
Concen: 0.213 ug/l
RT: 11.756 min Scan# 11
Delta R.T. -0.134 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11

Instrument :
MSVOA_X
ClientSampleId :
SB-43

Tgt Ion:105 Resp: 1602
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#



#95
Naphthalene
Concen: 2.238 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX032179.D
Acq: 18 Oct 2022 01:11

Tgt Ion:128 Resp: 12918
Ion Ratio Lower Upper
128 100
127 12.4 10.4 15.6
129 11.3 8.8 13.2

