

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101722\
 Data File : VX032180.D
 Acq On : 18 Oct 2022 01:34
 Operator : JC/MD
 Sample : N5159-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-44

Quant Time: Oct 18 04:35:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 18 04:18:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	108426	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	147656	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	195662	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	85558	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	73059	42.307	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	84.620%		
35) Dibromofluoromethane	5.385	113	67148	66.649	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	133.300%#		
50) Toluene-d8	8.647	98	218740	61.900	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	123.800%#		
62) 4-Bromofluorobenzene	11.079	95	100773	74.899	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	149.800%#		
Target Compounds						Qvalue
5) Bromomethane	1.618	94	219	0.230	ug/l #	73
11) Tert butyl alcohol	2.940	59	4097	17.250	ug/l #	73
13) Acrolein	2.227	56	243	1.215	ug/l #	42
16) Acetone	2.386	43	14899	35.882	ug/l	96
18) Methyl Acetate	2.709	43	2624	1.552	ug/l	94
20) Methylene Chloride	2.788	84	6806	5.331	ug/l	96
25) 2-Butanone	4.587	43	2930	3.303	ug/l	90
29) Tetrahydrofuran	5.025	42	681	1.280	ug/l #	56
31) Cyclohexane	5.556	56	2775	1.442	ug/l #	36
36) 1,1-Dichloropropene	5.556	75	9620	6.600	ug/l #	50
37) Ethyl Acetate	4.715	43	20333	13.901	ug/l #	93
38) Carbon Tetrachloride	5.556	117	11828	7.663	ug/l #	16
40) Benzene	6.044	78	8239	2.021	ug/l	99
41) Methacrylonitrile	5.032	41	393	0.521	ug/l #	48
43) Isopropyl Acetate	6.342	43	73525	33.357	ug/l	99
48) Methyl methacrylate	7.799	41	63468	56.815	ug/l #	45
49) 1,4-Dioxane	7.799	88	49	2.139	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	57248	42.354	ug/l #	51
52) Toluene	8.720	92	6163	2.373	ug/l	94
53) t-1,3-Dichloropropene	8.952	75	572	0.441	ug/l #	44
54) cis-1,3-Dichloropropene	8.549	75	25988	17.069	ug/l #	63
57) 1,3-Dichloropropane	9.482	76	4307	2.491	ug/l #	43
59) 2-Hexanone	9.482	43	60455	60.373	ug/l #	51
67) Ethyl Benzene	10.195	91	1655	0.219	ug/l #	87
68) m/p-Xylenes	10.305	106	2606	0.899	ug/l	95
69) o-Xylene	10.646	106	1763	0.618	ug/l	100
70) Styrene	10.659	104	2003	0.435	ug/l	96
74) N-amyl acetate	10.640	43	19066	8.418	ug/l #	53
76) 1,2,3-Trichloropropane	11.079	75	55934	30.151	ug/l #	37
81) trans-1,4-Dichloro-2-b...	11.079	75	55934	116.072	ug/l #	11
84) 1,2,4-Trimethylbenzene	11.756	105	3029	0.527	ug/l #	61
85) sec-Butylbenzene	11.756	105	3029	0.431	ug/l #	56
90) Hexachloroethane	12.408	117	219	0.270	ug/l #	15
95) Naphthalene	13.780	128	20151	3.733	ug/l	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101722\
Data File : VX032180.D
Acq On : 18 Oct 2022 01:34
Operator : JC/MD
Sample : N5159-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-44

Quant Time: Oct 18 04:35:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101722W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 18 04:18:35 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101722\
Data File : VX032180.D
Acq On : 18 Oct 2022 01:34
Operator : JC/MD
Sample : N5159-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-44

Quant Time: Oct 18 04:35:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101722W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 18 04:18:35 2022
Response via : Initial Calibration




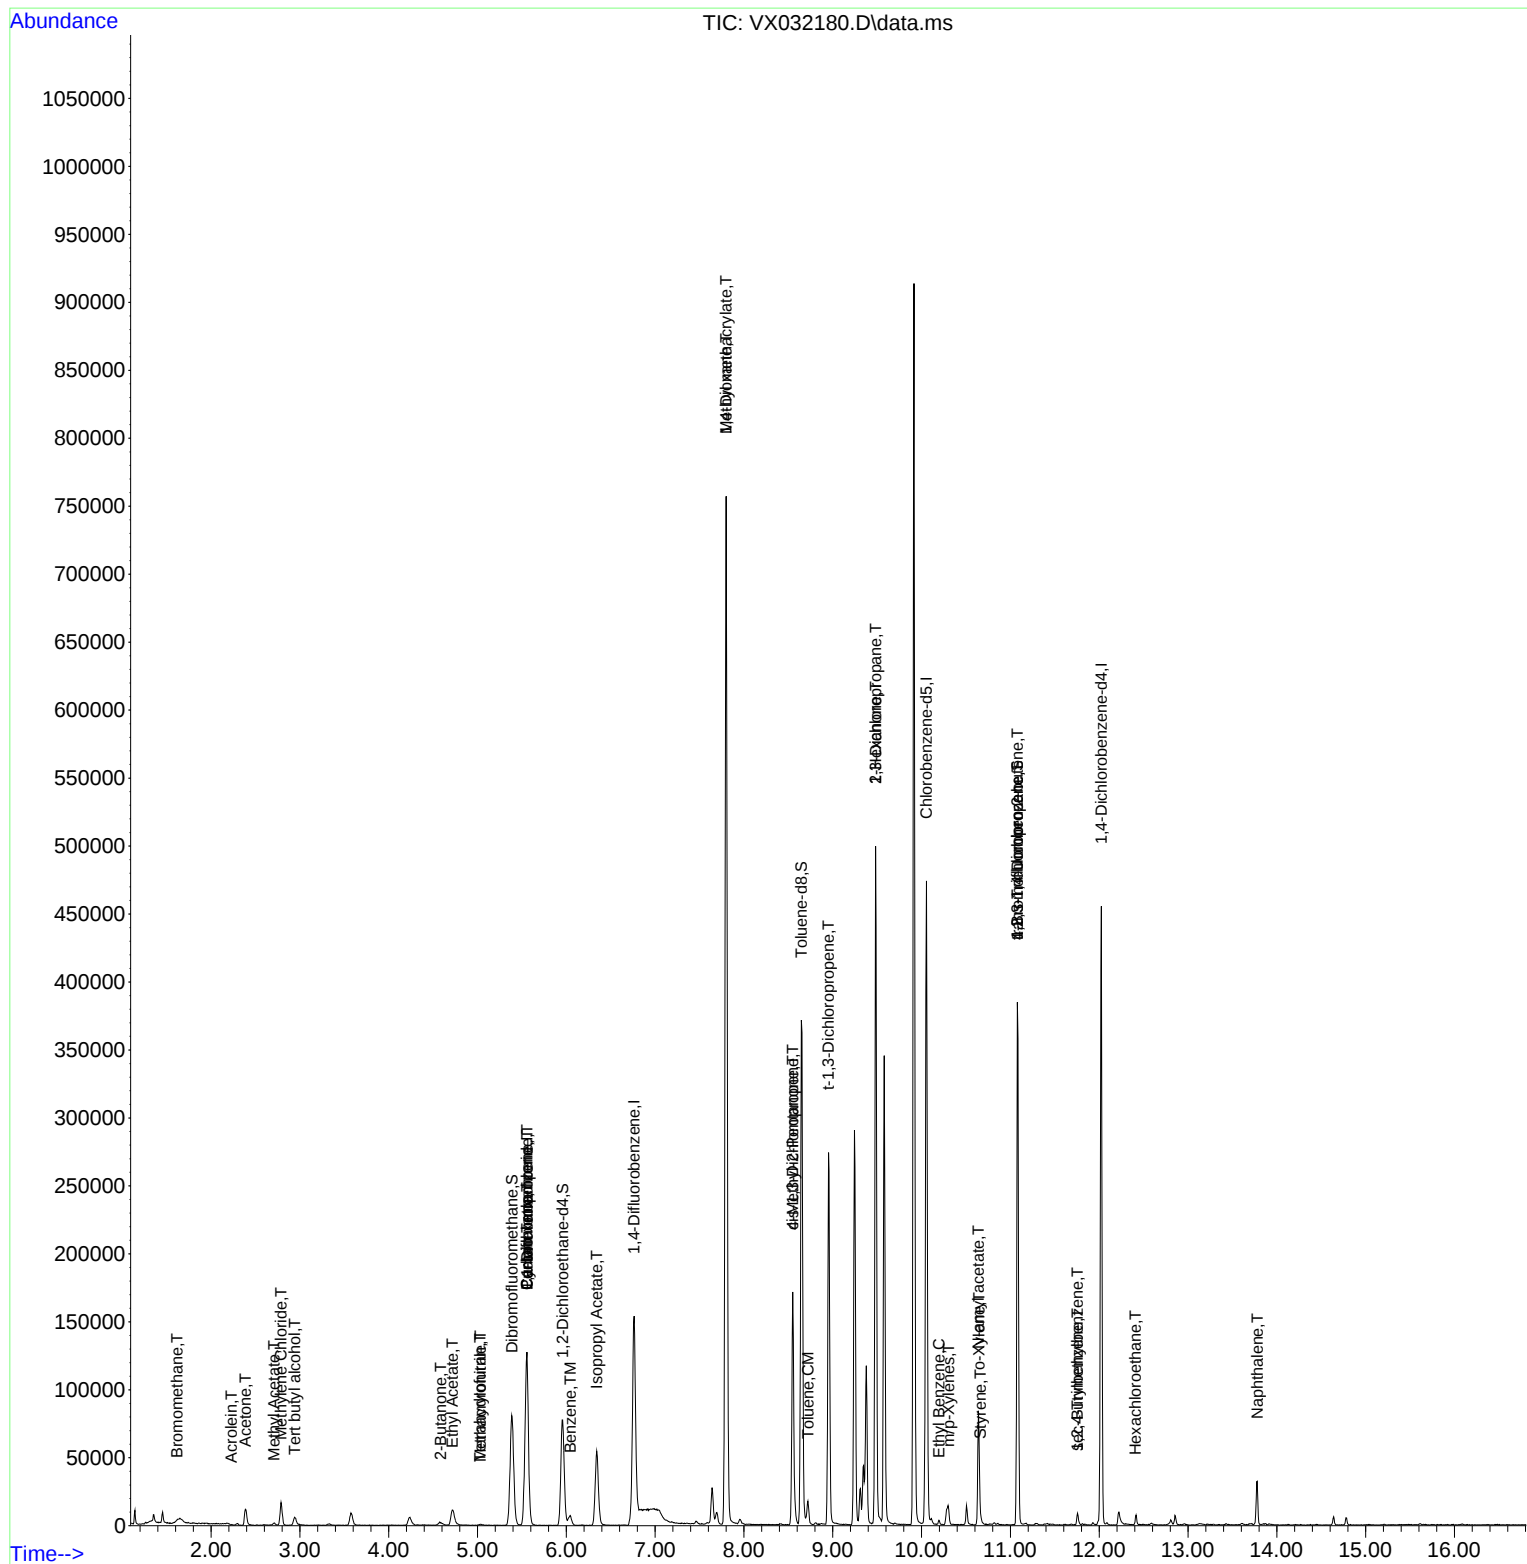




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34




Instrument :
MSVOA_X
ClientSampleId :
SB-44


Tgt Ion:168 Resp: 108426
Ion Ratio Lower Upper
168 100
99 62.6 48.8 73.2



#5
Bromomethane
Concen: 0.230 ug/l
RT: 1.618 min Scan# 87
Delta R.T. 0.006 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34

Tgt Ion: 94 Resp: 219
Ion Ratio Lower Upper
94 100
96 118.8 74.4 111.6#

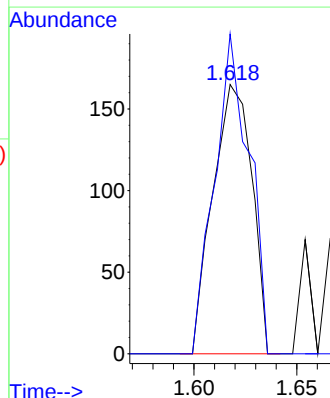



#11

Tert butyl alcohol

Concen: 17.250 ug/l

RT: 2.940 min Scan# 304

Delta R.T. -0.055 min

Lab File: VX032180.D

Acq: 18 Oct 2022 01:34

Instrument :

MSVOA_X

ClientSampleId :





SB-44

Tgt Ion: 59 Resp: 4097

Ion Ratio Lower Upper

59 100

57 0.0 8.2 12.2#

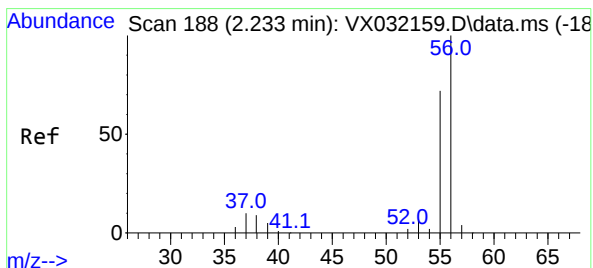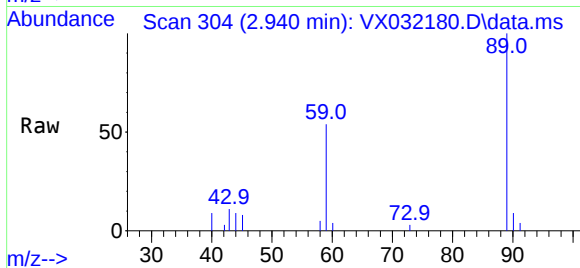

#13

Acrolein

Concen: 1.215 ug/l

RT: 2.227 min Scan# 187

Delta R.T. -0.006 min

Lab File: VX032180.D




Acq: 18 Oct 2022 01:34


Tgt Ion: 56 Resp: 243

Ion Ratio Lower Upper

56 100

55 22.2 56.0 84.0#


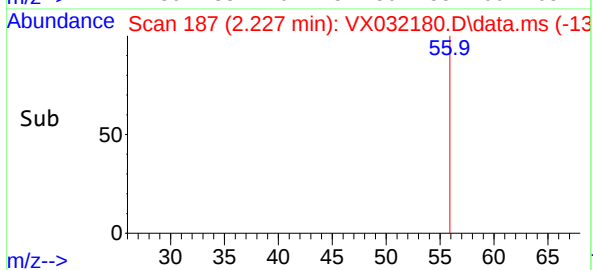

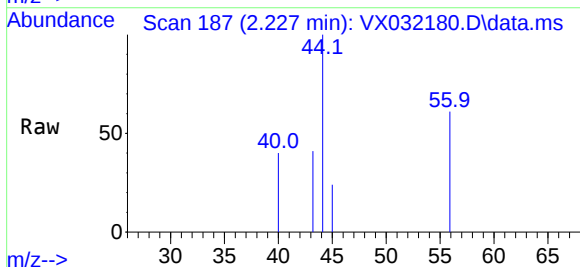




#16
Acetone
Concen: 35.882 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34




Instrument :
MSVOA_X
ClientSampleId :
SB-44


Tgt Ion: 43 Resp: 14899
Ion Ratio Lower Upper
43 100
58 27.5 23.8 35.8



#18
Methyl Acetate
Concen: 1.552 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.006 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34

Tgt Ion: 43 Resp: 2624
Ion Ratio Lower Upper
43 100
74 20.5 18.6 27.8

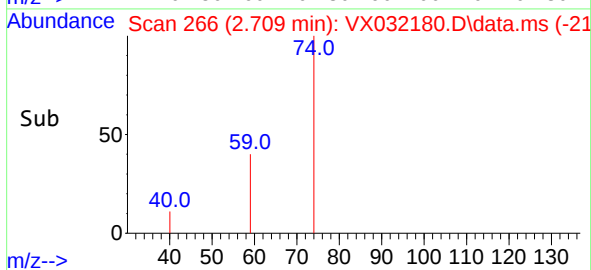







#20
Methylene Chloride
Concen: 5.331 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34

Instrument :
MSVOA_X
ClientSampleId :
SB-44

Tgt Ion: 84 Resp: 6806




Ion	Ratio	Lower	Upper
84	100		
49	124.7	105.9	158.9
51	42.9	32.2	48.2
86	63.7	50.8	76.2

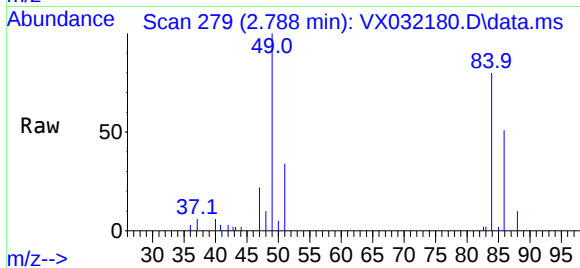


#25
2-Butanone
Concen: 3.303 ug/l
RT: 4.587 min Scan# 574
Delta R.T. 0.030 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34

Tgt Ion: 43 Resp: 2930

Ion	Ratio	Lower	Upper
43	100		
72	31.6	21.1	31.7

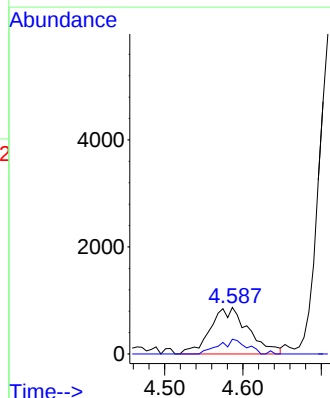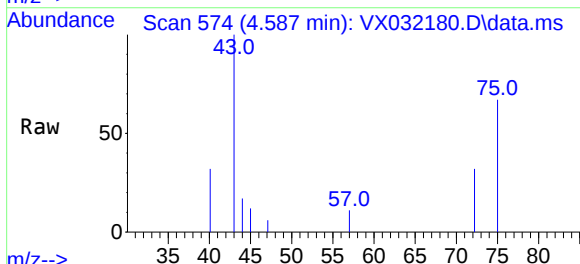



#29

Tetrahydrofuran

Concen: 1.280 ug/l

RT: 5.025 min Scan# 64

Delta R.T. 0.024 min

Lab File: VX032180.D

Acq: 18 Oct 2022 01:34

Instrument :

MSVOA_X

ClientSampleId :

SB-44





Tgt Ion: 42 Resp: 681

Ion Ratio Lower Upper

42 100

72 13.4 36.4 54.6#

71 17.3 33.5 50.3#

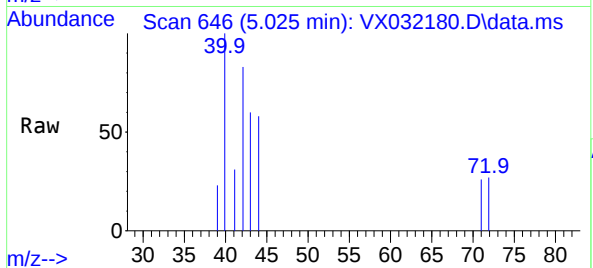

#31

Cyclohexane

Concen: 1.442 ug/l

RT: 5.556 min Scan# 733

Delta R.T. 0.085 min

Lab File: VX032180.D

Acq: 18 Oct 2022 01:34




Tgt Ion: 56 Resp: 2775


Ion Ratio Lower Upper

56 100

69 129.0 25.1 37.7#

84 110.5 70.2 105.4#

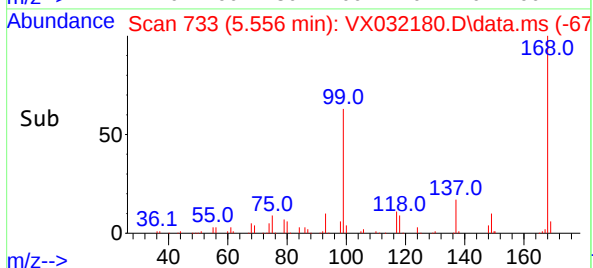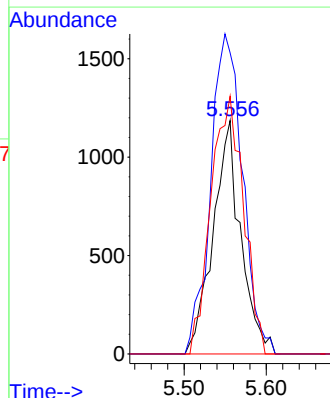



#33

1,2-Dichloroethane-d4

Concen: 42.307 ug/l

RT: 5.958 min Scan# 798

Delta R.T. 0.006 min

Lab File: VX032180.D

Acq: 18 Oct 2022 01:34

Instrument :

MSVOA_X

ClientSampleId :





SB-44

Tgt Ion: 65 Resp: 73059

Ion Ratio Lower Upper

65 100

67 51.9 0.0 102.4

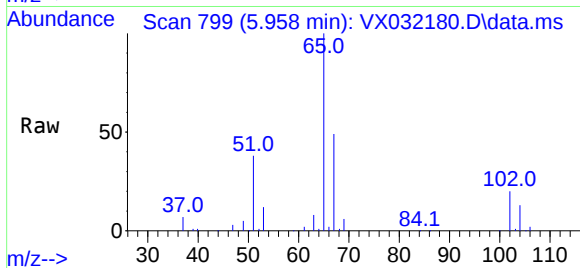

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.006 min

Lab File: VX032180.D

Acq: 18 Oct 2022 01:34




Tgt Ion: 114 Resp: 147656


Ion Ratio Lower Upper

114 100

63 18.1 0.0 42.6

88 15.3 0.0 33.0


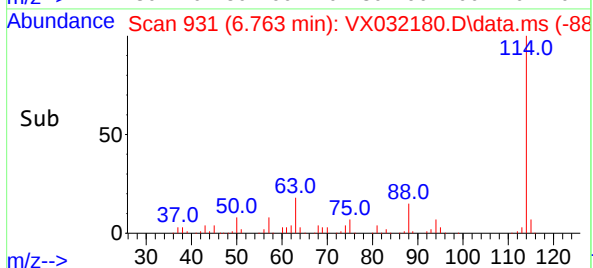
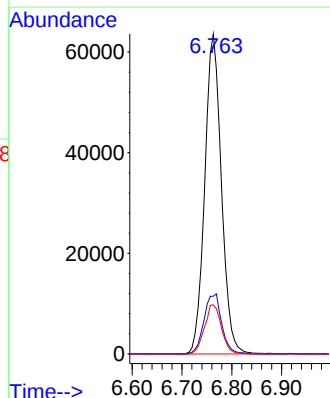
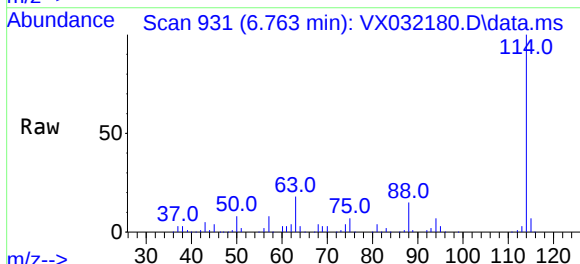


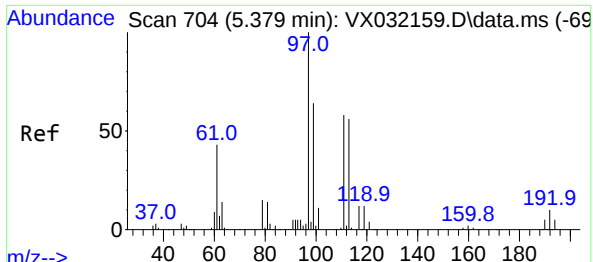

#35
Dibromofluoromethane
Concen: 66.649 ug/l
RT: 5.385 min Scan# 704
Delta R.T. 0.006 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34




Instrument :
MSVOA_X
ClientSampleId :
SB-44


Tgt Ion:113 Resp: 67148
Ion Ratio Lower Upper
113 100
111 103.3 82.4 123.6
192 18.7 14.1 21.1

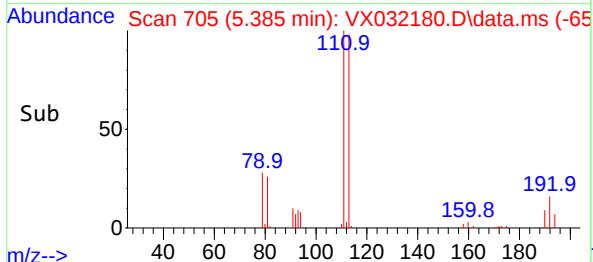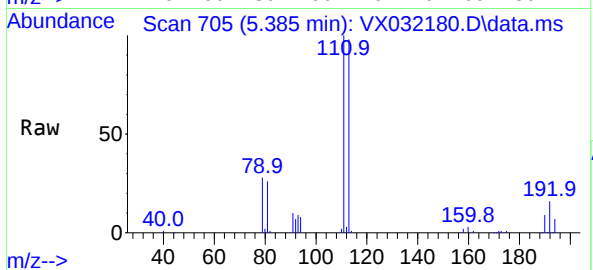

#36
1,1-Dichloropropene
Concen: 6.600 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.134 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34

Tgt Ion: 75 Resp: 9620
Ion Ratio Lower Upper
75 100
110 9.1 17.5 52.5#
77 0.0 24.9 37.3#

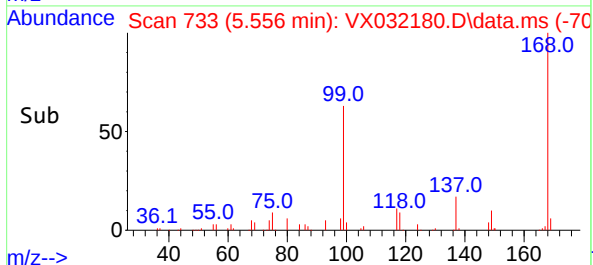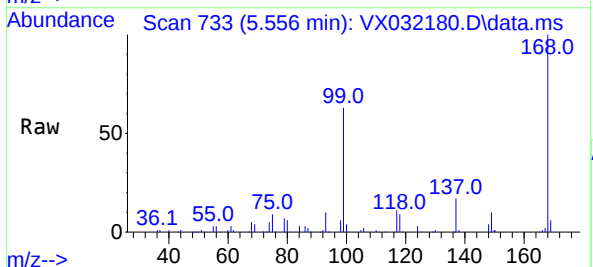



#37

Ethyl Acetate

Concen: 13.901 ug/l

RT: 4.715 min Scan# 594

Delta R.T. 0.006 min

Lab File: VX032180.D

Acq: 18 Oct 2022 01:34





Instrument :

MSVOA_X

ClientSampleId :

SB-44

Tgt Ion: 43	Resp: 20333
Ion Ratio	Lower Upper
43 100	
61 13.2	11.1 16.7
70 5.7	8.6 13.0



#38

Carbon Tetrachloride

Concen: 7.663 ug/l




RT: 5.556 min Scan# 733


Delta R.T. -0.116 min

Lab File: VX032180.D

Acq: 18 Oct 2022 01:34

Tgt Ion: 117	Resp: 11828
Ion Ratio	Lower Upper
117 100	
119 4.1	74.6 112.0
121 0.0	25.3 37.9



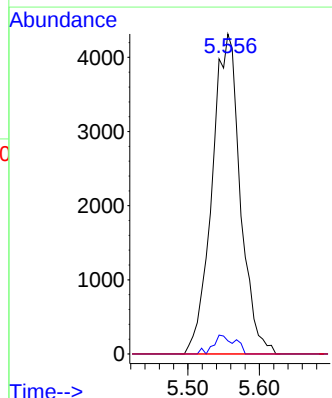





#40
Benzene
Concen: 2.021 ug/l
RT: 6.044 min Scan# 812
Delta R.T. 0.006 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34




Instrument :
MSVOA_X
ClientSampleId :
SB-44


Tgt Ion: 78 Resp: 8239
Ion Ratio Lower Upper
78 100
77 23.7 18.7 28.1



#41
Methacrylonitrile
Concen: 0.521 ug/l
RT: 5.032 min Scan# 647
Delta R.T. 0.116 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34

Tgt Ion: 41 Resp: 393
Ion Ratio Lower Upper
41 100
39 53.2 45.0 67.6
67 0.0 58.2 87.4#
52 0.0 25.0 37.6#


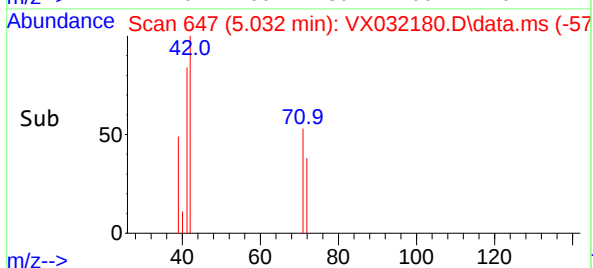
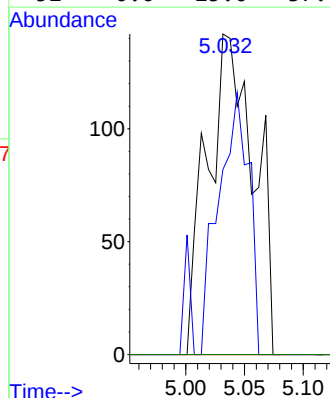





#43
Isopropyl Acetate
Concen: 33.357 ug/l
RT: 6.342 min Scan# 81
Delta R.T. 0.006 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34




Instrument :
MSVOA_X
ClientSampleId :
SB-44


Tgt Ion: 43	Resp: 73525
Ion Ratio	Lower Upper
43	100
61	19.2 15.3 22.9
87	13.6 10.6 15.8

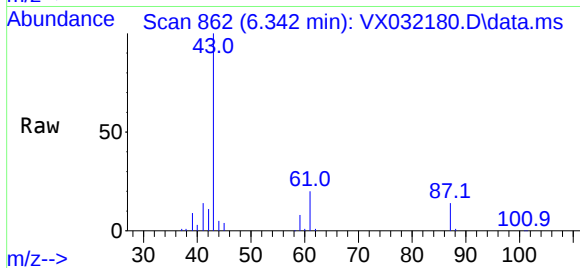

#48
Methyl methacrylate
Concen: 56.815 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.109 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34

Tgt Ion: 41	Resp: 63468
Ion Ratio	Lower Upper
41	100
69	0.0 64.6 96.8#
39	56.6 51.4 77.0


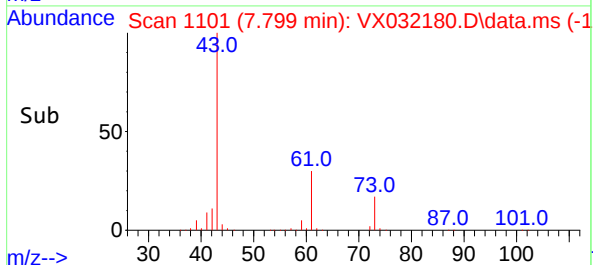
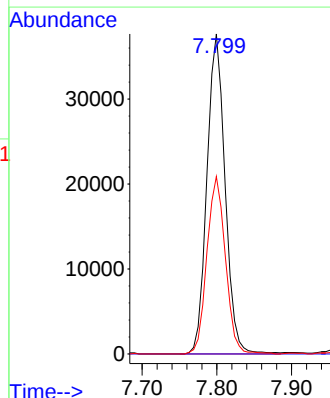
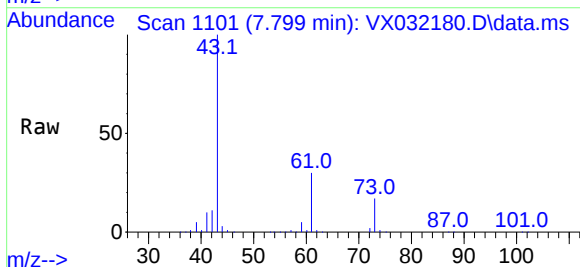




#49
1,4-Dioxane
Concen: 2.139 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.115 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34




Instrument :
MSVOA_X
ClientSampleId :
SB-44


Tgt Ion: 88 Resp: 49
Ion Ratio Lower Upper
88 100
43 1362771.4 27.1 40.7#
58 6667.3 53.9 80.9#

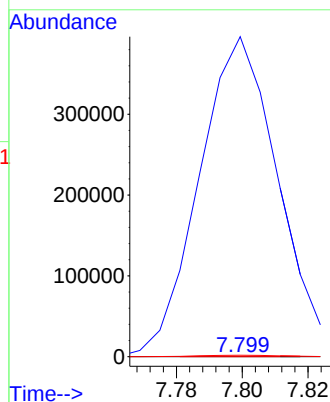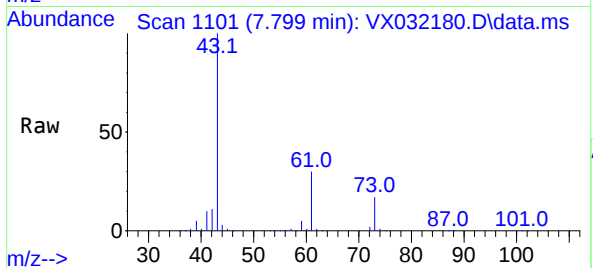

#50
Toluene-d8
Concen: 61.900 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34

Tgt Ion: 98 Resp: 218740
Ion Ratio Lower Upper
98 100
100 66.3 52.5 78.7

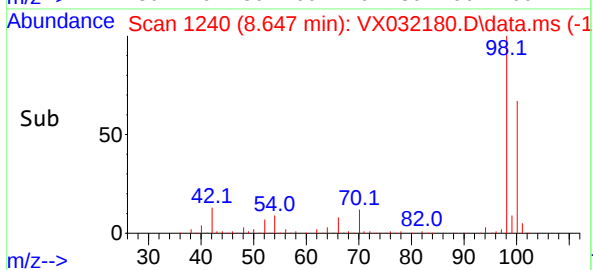



#51

4-Methyl-2-Pentanone

Concen: 42.354 ug/l

RT: 8.549 min Scan# 11

Delta R.T. -0.025 min

Lab File: VX032180.D

Acq: 18 Oct 2022 01:34

Instrument :

MSVOA_X

ClientSampleId :





SB-44

Tgt Ion: 43 Resp: 57248

Ion Ratio Lower Upper

43 100

58 8.8 30.6 46.0#

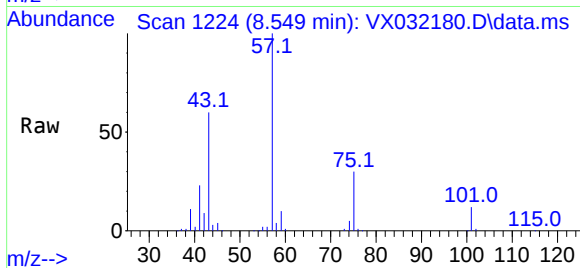

#52

Toluene

Concen: 2.373 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX032180.D




Acq: 18 Oct 2022 01:34


Tgt Ion: 92 Resp: 6163

Ion Ratio Lower Upper

92 100

91 163.2 137.1 205.7

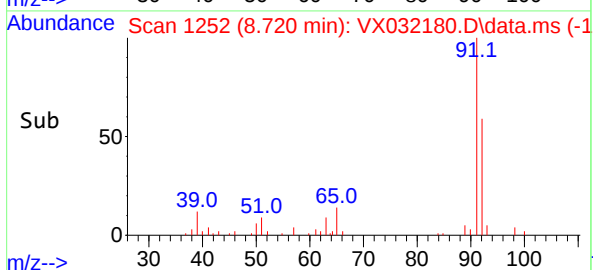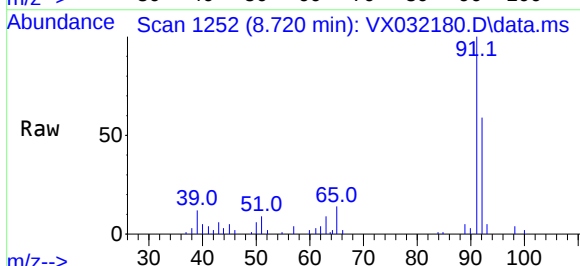



#53

t-1,3-Dichloropropene

Concen: 0.441 ug/l

RT: 8.952 min Scan# 11

Delta R.T. -0.024 min

Lab File: VX032180.D

Acq: 18 Oct 2022 01:34

Instrument :

MSVOA_X

ClientSampleId :





SB-44

Tgt Ion: 75 Resp: 572

Ion Ratio Lower Upper

75 100

77 0.0 24.8 37.2#

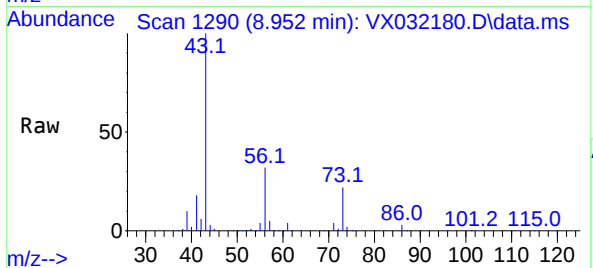

#54

cis-1,3-Dichloropropene

Concen: 17.069 ug/l

RT: 8.549 min Scan# 1224

Delta R.T. 0.183 min

Lab File: VX032180.D

Acq: 18 Oct 2022 01:34




Tgt Ion: 75 Resp: 25988


Ion Ratio Lower Upper

75 100

77 0.6 24.4 36.6#

39 35.4 43.7 65.5#


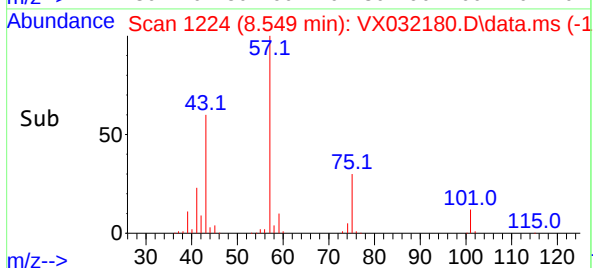
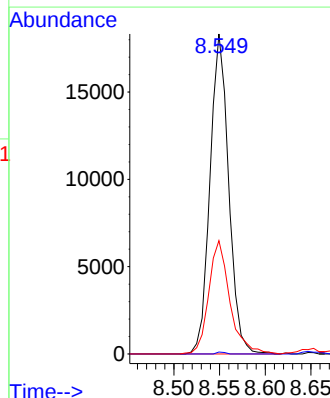





#57
1,3-Dichloropropane
Concen: 2.491 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.177 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34




Instrument :
MSVOA_X
ClientSampleId :
SB-44


Tgt Ion: 76 Resp: 4307
Ion Ratio Lower Upper
76 100
78 0.0 25.5 38.3#



#59
2-Hexanone
Concen: 60.373 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.055 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34

Tgt Ion: 43 Resp: 60455
Ion Ratio Lower Upper
43 100
58 18.6 26.7 80.0#


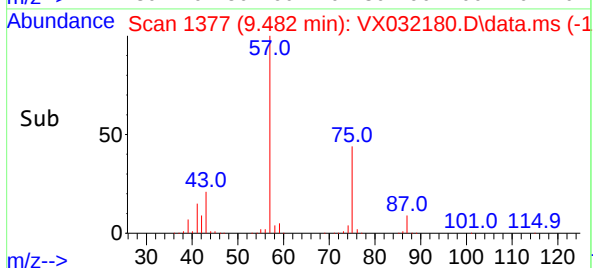






#62
4-Bromofluorobenzene
Concen: 74.899 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34




Instrument :
MSVOA_X
ClientSampleId :
SB-44


Tgt Ion: 95 Resp: 100773
Ion Ratio Lower Upper
95 100
174 72.8 0.0 153.2
176 70.3 0.0 144.0

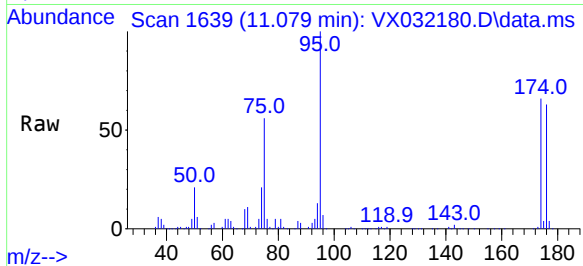

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34

Tgt Ion: 117 Resp: 195662
Ion Ratio Lower Upper
117 100
82 59.2 46.8 70.2
119 31.8 26.4 39.6



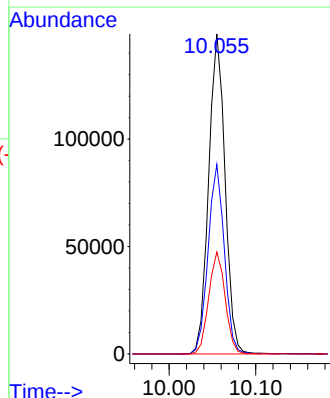
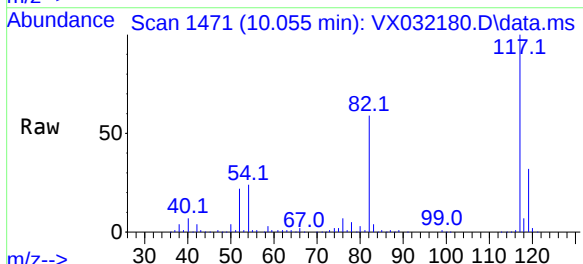




#67
Ethyl Benzene
Concen: 0.219 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34




Instrument :
MSVOA_X
ClientSampleId :
SB-44


Tgt Ion: 91 Resp: 1655
Ion Ratio Lower Upper
91 100
106 24.1 25.2 37.8#

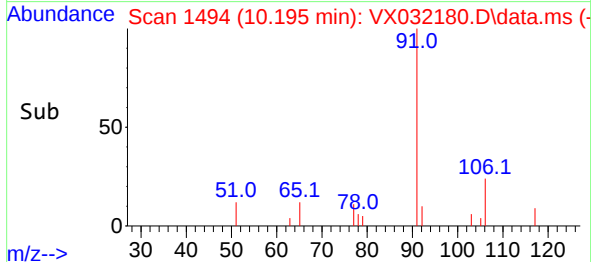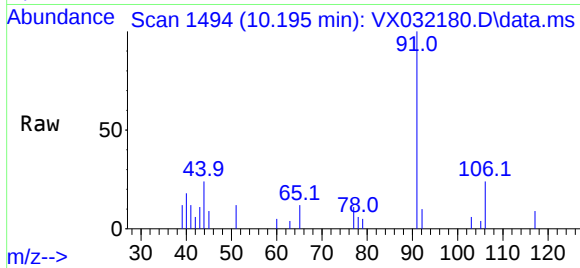

#68
m/p-Xylenes
Concen: 0.899 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34

Tgt Ion: 106 Resp: 2606
Ion Ratio Lower Upper
106 100
91 209.4 161.0 241.4


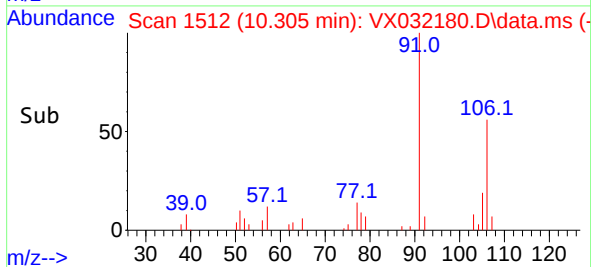

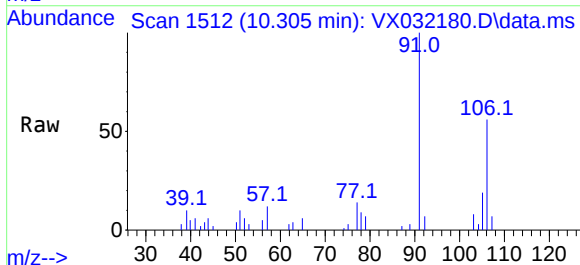




#69
o-Xylene
Concen: 0.618 ug/l
RT: 10.646 min Scan# 1567
Delta R.T. 0.006 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34




Instrument :
MSVOA_X
ClientSampleId :
SB-44


Tgt Ion:106 Resp: 1763
Ion Ratio Lower Upper
106 100
91 214.2 107.2 321.6

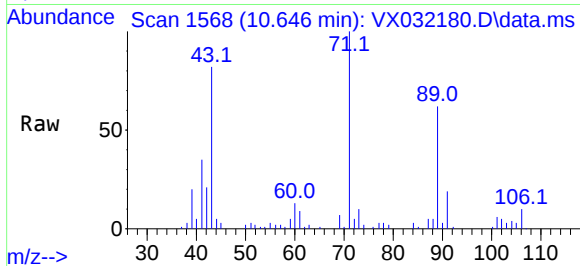

#70
Styrene
Concen: 0.435 ug/l
RT: 10.659 min Scan# 1570
Delta R.T. 0.006 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34

Tgt Ion:104 Resp: 2003
Ion Ratio Lower Upper
104 100
78 53.7 41.4 62.2
103 58.4 43.8 65.8


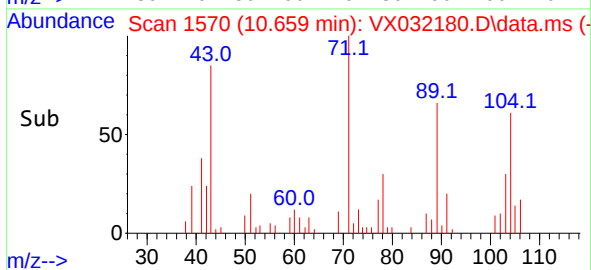

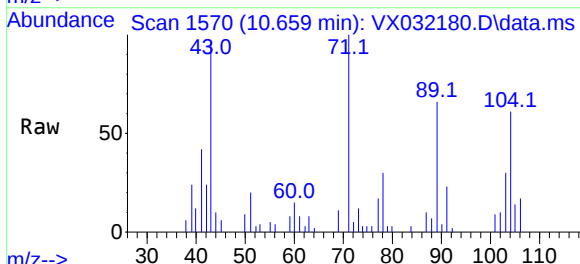




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34




Instrument :
MSVOA_X
ClientSampleId :
SB-44


Tgt Ion:152 Resp: 85558
Ion Ratio Lower Upper
152 100
115 65.3 43.4 130.1
150 159.1 0.0 346.8

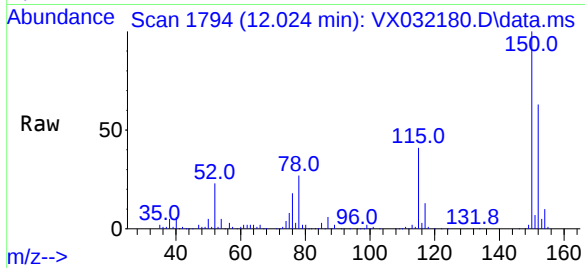

#74
N-ethyl acetate
Concen: 8.418 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.202 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34

Tgt Ion: 43 Resp: 19066
Ion Ratio Lower Upper
43 100
70 1.8 33.4 50.2#
55 5.1 18.2 27.2#
61 9.8 19.3 28.9#



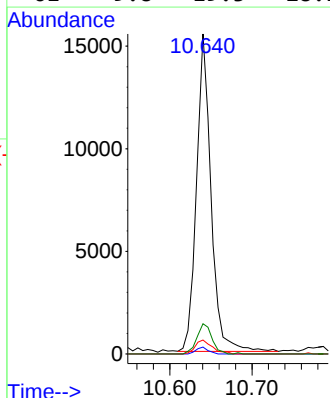
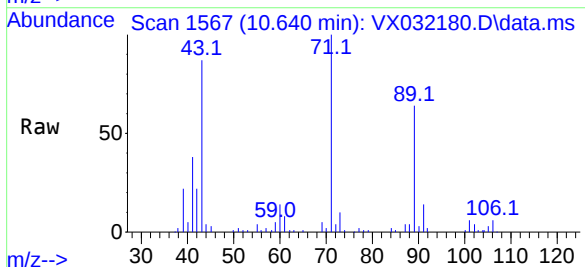




#76
1,2,3-Trichloropropane
Concen: 30.151 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34




Instrument :
MSVOA_X
ClientSampleId :
SB-44


Tgt Ion: 75 Resp: 55934
Ion Ratio Lower Upper
75 100
77 1.2 20.3 60.9#

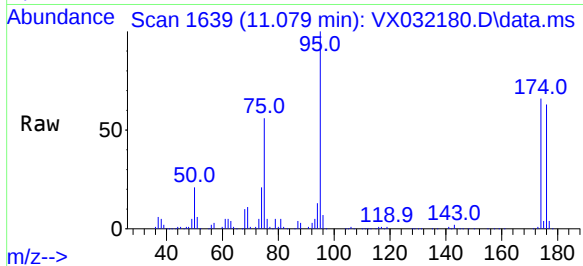

#81
trans-1,4-Dichloro-2-butene
Concen: 116.072 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34

Tgt Ion: 75 Resp: 55934
Ion Ratio Lower Upper
75 100
53 0.0 77.6 116.4#
89 0.0 37.4 56.0#



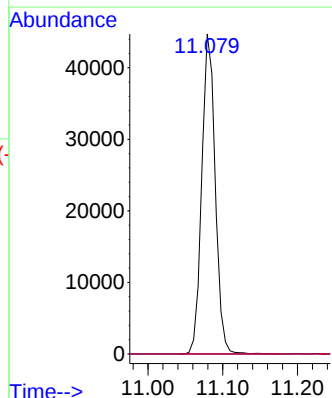
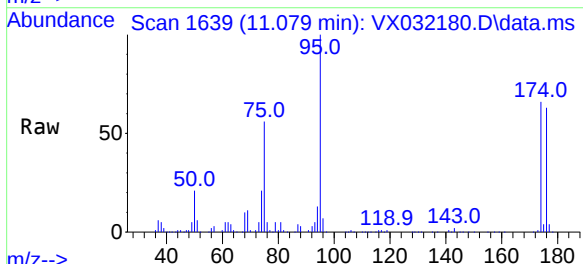




#84
1,2,4-Trimethylbenzene
Concen: 0.527 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34




Instrument :
MSVOA_X
ClientSampleId :
SB-44


Tgt Ion:105 Resp: 3029
Ion Ratio Lower Upper
105 100
120 19.3 22.6 67.8#

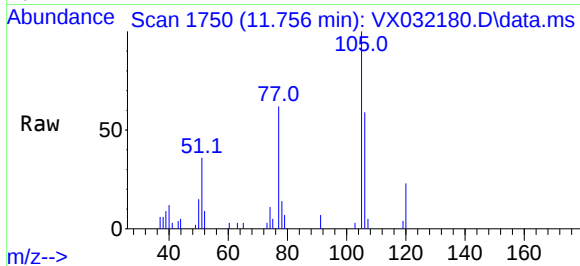

#85
sec-Butylbenzene
Concen: 0.431 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.134 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34

Tgt Ion:105 Resp: 3029
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#




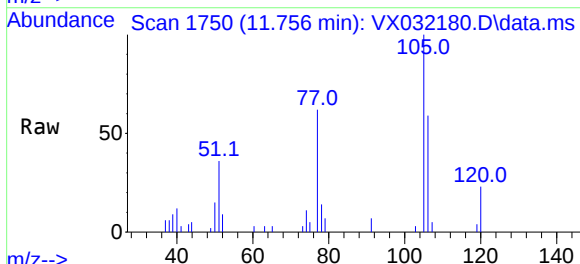




#90
Hexachloroethane
Concen: 0.270 ug/l
RT: 12.408 min Scan# 117
Delta R.T. -0.135 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34

Instrument :
MSVOA_X
ClientSampleId :
SB-44

Tgt Ion:117 Resp: 219
Ion Ratio Lower Upper
117 100
201 0.0 34.8 104.4#

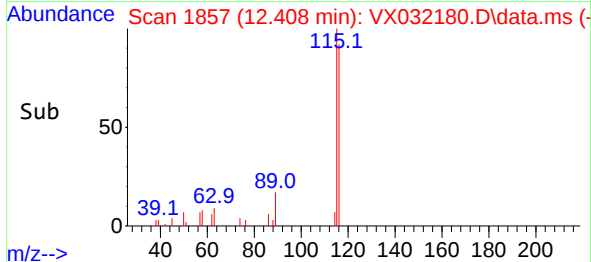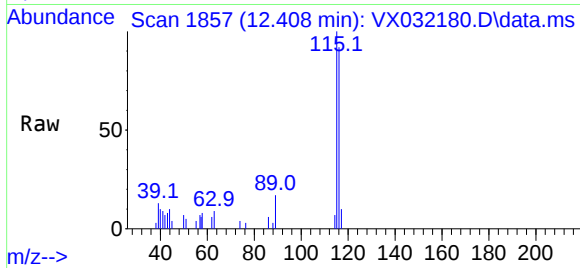

#95
Naphthalene
Concen: 3.733 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX032180.D
Acq: 18 Oct 2022 01:34

Tgt Ion:128 Resp: 20151
Ion Ratio Lower Upper
128 100
127 12.5 10.4 15.6
129 11.8 8.8 13.2

