

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101722\
 Data File : VX032181.D
 Acq On : 18 Oct 2022 01:57
 Operator : JC/MD
 Sample : N5159-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-45

Quant Time: Oct 18 04:35:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 18 04:18:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	124916	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	218551	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	202313	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	91812	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	100668	50.599	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	101.200%		
35) Dibromofluoromethane	5.385	113	71945	48.246	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	96.500%		
50) Toluene-d8	8.647	98	214319	40.975	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	81.940%#		
62) 4-Bromofluorobenzene	11.079	95	99030	49.728	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	99.460%		
Target Compounds					Qvalue	
5) Bromomethane	1.611	94	272	0.248	ug/l #	80
11) Tert butyl alcohol	2.940	59	4302	15.722	ug/l #	73
13) Acrolein	2.233	56	215	0.933	ug/l	83
16) Acetone	2.386	43	20859	43.604	ug/l	93
18) Methyl Acetate	2.709	43	2391	1.227	ug/l	94
20) Methylene Chloride	2.788	84	6833	4.646	ug/l	99
25) 2-Butanone	4.586	43	2920	2.857	ug/l	98
29) Tetrahydrofuran	5.038	42	511	0.834	ug/l #	64
31) Cyclohexane	5.544	56	3201	1.444	ug/l #	28
36) 1,1-Dichloropropene	5.556	75	11310	5.242	ug/l #	50
37) Ethyl Acetate	4.721	43	20069	9.270	ug/l	99
38) Carbon Tetrachloride	5.550	117	14392	6.299	ug/l #	17
40) Benzene	6.037	78	8176	1.355	ug/l	92
41) Methacrylonitrile	5.031	41	310	0.278	ug/l #	37
43) Isopropyl Acetate	6.342	43	91848	28.153	ug/l	99
48) Methyl methacrylate	7.799	41	70656	42.732	ug/l #	46
49) 1,4-Dioxane	7.799	88	24	0.708	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	58687	29.335	ug/l #	52
52) Toluene	8.720	92	5875	1.528	ug/l	98
53) t-1,3-Dichloropropene	8.958	75	524	0.273	ug/l #	44
54) cis-1,3-Dichloropropene	8.549	75	27236	12.086	ug/l #	63
56) Ethyl methacrylate	9.244	69	567	0.272	ug/l #	1
57) 1,3-Dichloropropane	9.482	76	4358	1.703	ug/l #	43
59) 2-Hexanone	9.482	43	60248	40.649	ug/l #	50
67) Ethyl Benzene	10.195	91	1655	0.212	ug/l	97
68) m/p-Xylenes	10.305	106	2580	0.861	ug/l	91
69) o-Xylene	10.646	106	1546	0.524	ug/l	90
70) Styrene	10.658	104	1716	0.360	ug/l	90
74) N-amyl acetate	10.640	43	19619	8.072	ug/l #	53
76) 1,2,3-Trichloropropane	11.079	75	56292	28.277	ug/l #	37
81) trans-1,4-Dichloro-2-b...	11.079	75	56292	108.857	ug/l #	11
84) 1,2,4-Trimethylbenzene	11.756	105	2963	0.481	ug/l #	62
85) sec-Butylbenzene	11.756	105	2963	0.393	ug/l #	56
90) Hexachloroethane	12.408	117	183	0.210	ug/l #	15
95) Naphthalene	13.780	128	19794	3.417	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101722\
Data File : VX032181.D
Acq On : 18 Oct 2022 01:57
Operator : JC/MD
Sample : N5159-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-45

Quant Time: Oct 18 04:35:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101722W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 18 04:18:35 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101722\
Data File : VX032181.D
Acq On : 18 Oct 2022 01:57
Operator : JC/MD
Sample : N5159-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-45

Quant Time: Oct 18 04:35:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101722W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 18 04:18:35 2022
Response via : Initial Calibration




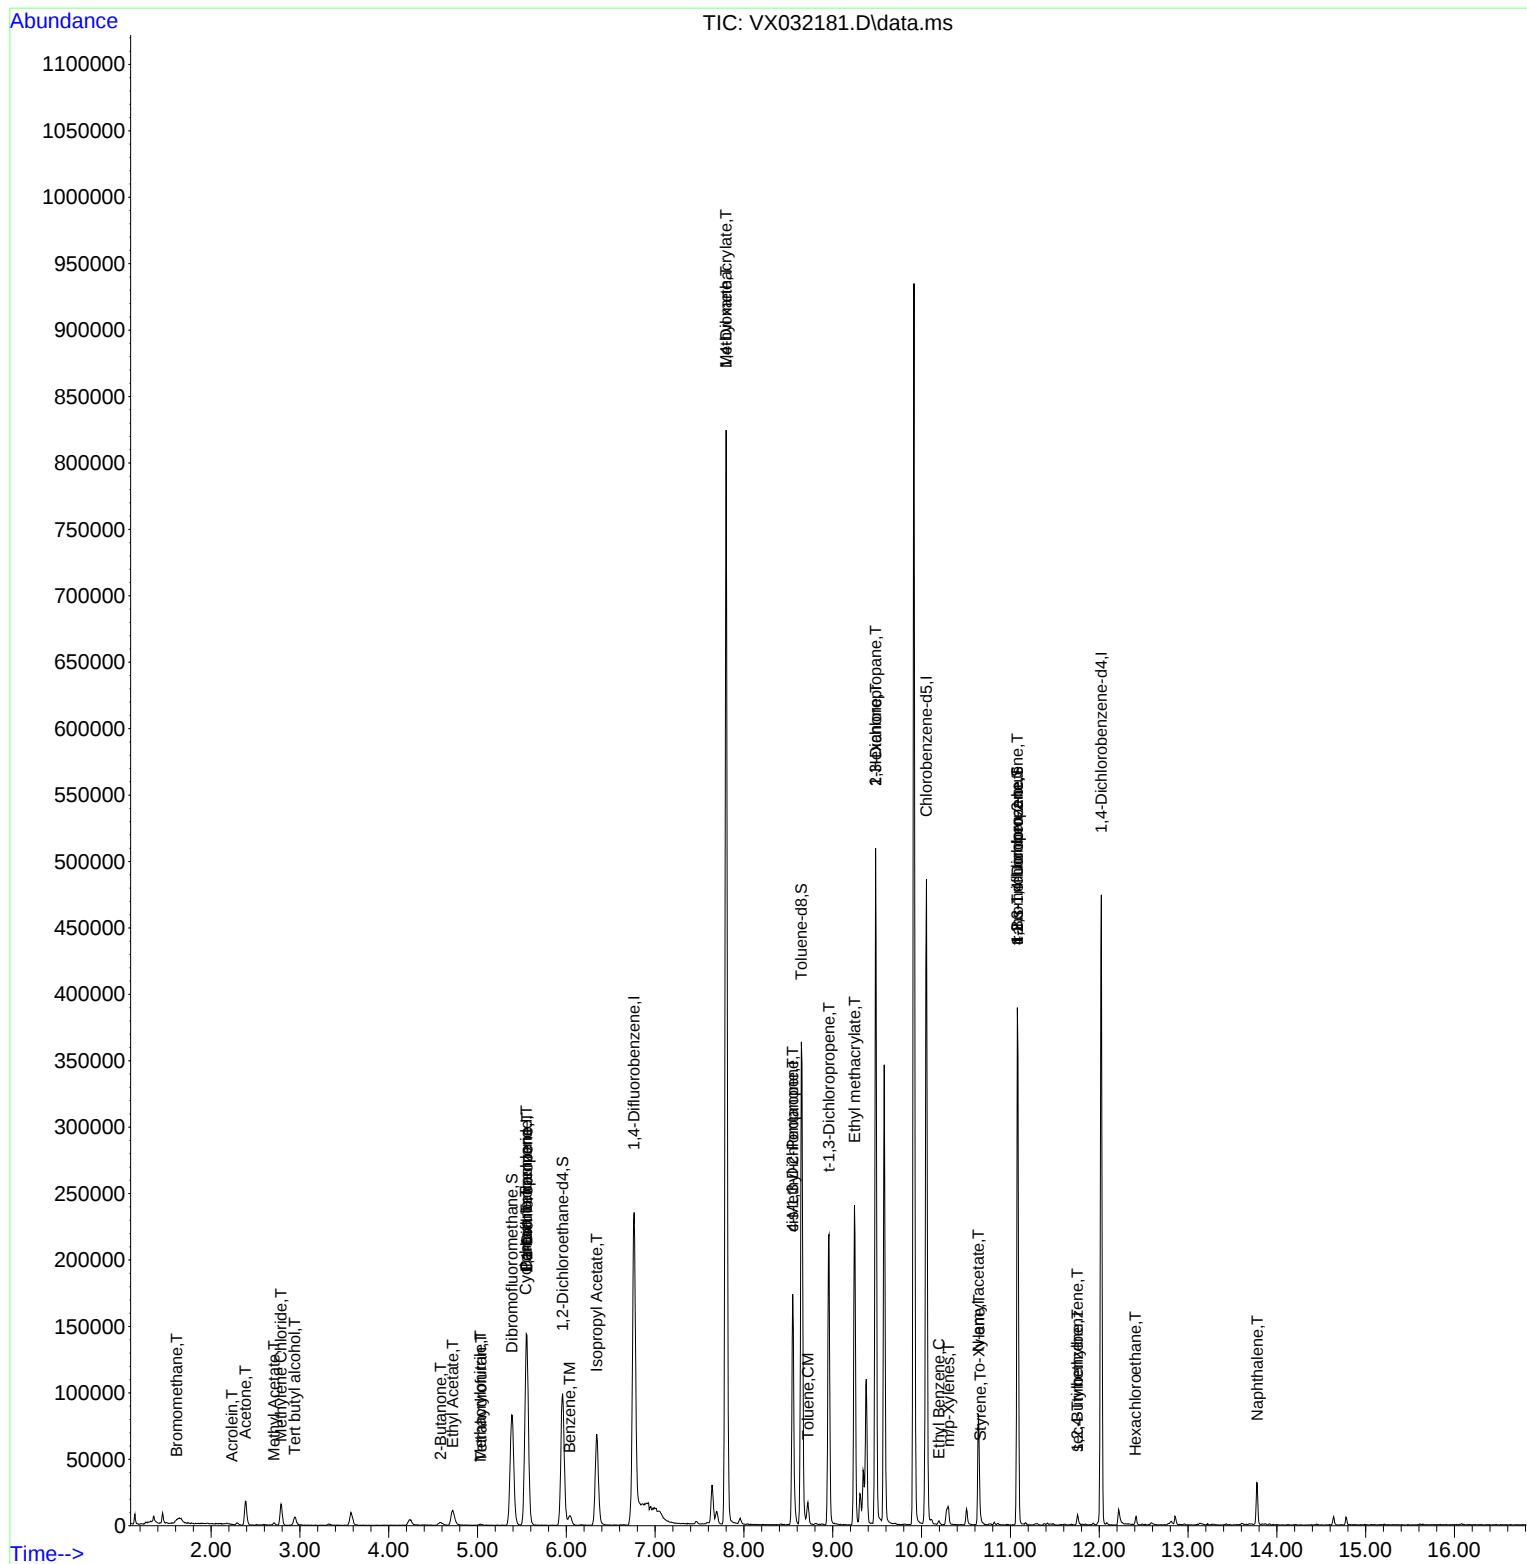




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57




Instrument :
MSVOA_X
ClientSampleId :
SB-45


Tgt Ion:168 Resp: 124916
Ion Ratio Lower Upper
168 100
99 65.9 48.8 73.2

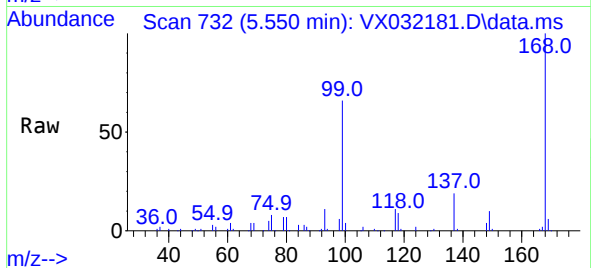

#5
Bromomethane
Concen: 0.248 ug/l
RT: 1.611 min Scan# 86
Delta R.T. -0.001 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57

Tgt Ion: 94 Resp: 272
Ion Ratio Lower Upper
94 100
96 73.8 74.4 111.6#


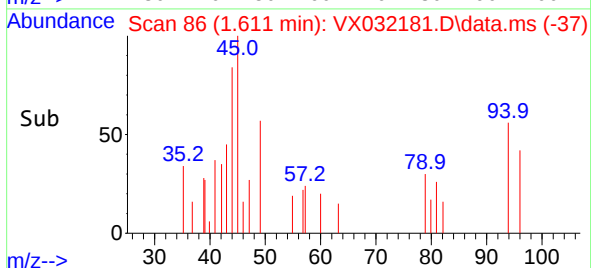
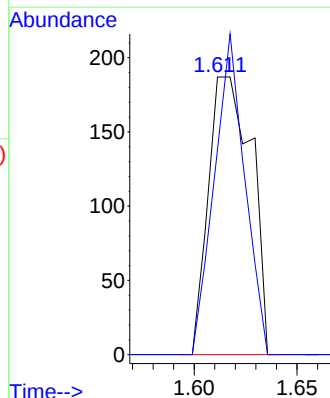





#11
Tert butyl alcohol
Concen: 15.722 ug/l
RT: 2.940 min Scan# 304
Delta R.T. -0.055 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57




Instrument :
MSVOA_X
ClientSampleId :
SB-45


Tgt Ion: 59 Resp: 4302
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#



#13
Acrolein
Concen: 0.933 ug/l
RT: 2.233 min Scan# 188
Delta R.T. 0.000 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57

Tgt Ion: 56 Resp: 215
Ion Ratio Lower Upper
56 100
55 83.7 56.0 84.0


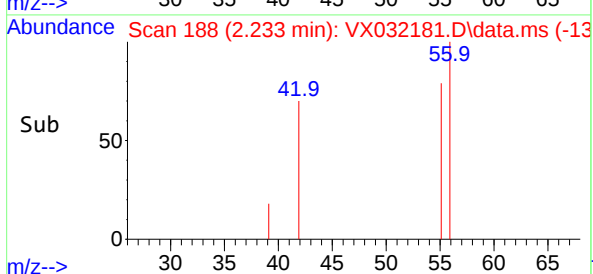






#16
Acetone
Concen: 43.604 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57




Instrument :
MSVOA_X
ClientSampleId :
SB-45


Tgt Ion: 43 Resp: 20859
Ion Ratio Lower Upper
43 100
58 26.2 23.8 35.8

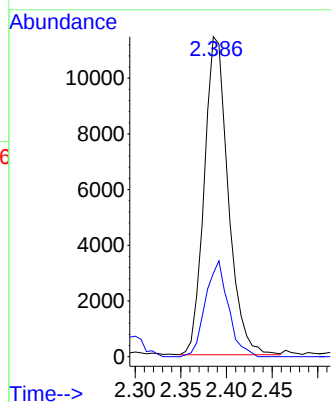

#18
Methyl Acetate
Concen: 1.227 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.006 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57

Tgt Ion: 43 Resp: 2391
Ion Ratio Lower Upper
43 100
74 20.2 18.6 27.8

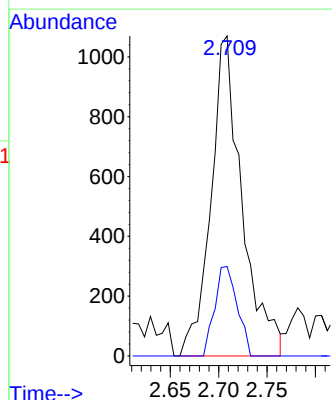







#20
Methylene Chloride
Concen: 4.646 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57

Instrument :
MSVOA_X
ClientSampleId :
SB-45

Tgt Ion: 84 Resp: 6833




Ion	Ratio	Lower	Upper
84	100		
49	133.4	105.9	158.9
51	39.9	32.2	48.2
86	63.5	50.8	76.2

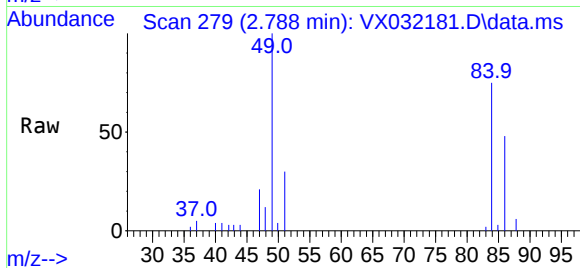


#25
2-Butanone
Concen: 2.857 ug/l
RT: 4.586 min Scan# 574
Delta R.T. 0.030 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57

Tgt Ion: 43 Resp: 2920

Ion	Ratio	Lower	Upper
43	100		
72	25.3	21.1	31.7

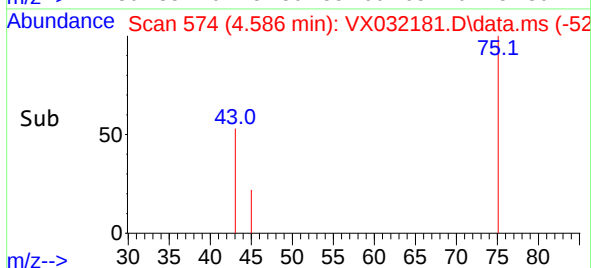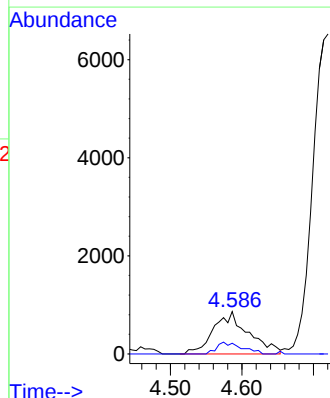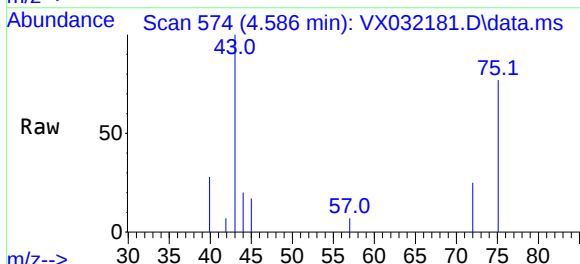



#29

Tetrahydrofuran

Concen: 0.834 ug/l

RT: 5.038 min Scan# 642

Delta R.T. 0.037 min

Lab File: VX032181.D

Acq: 18 Oct 2022 01:57

Instrument :

MSVOA_X

ClientSampleId :

SB-45





Tgt Ion: 42 Resp: 511

Ion Ratio Lower Upper

42 100

72 27.2 36.4 54.6#

71 13.3 33.5 50.3#

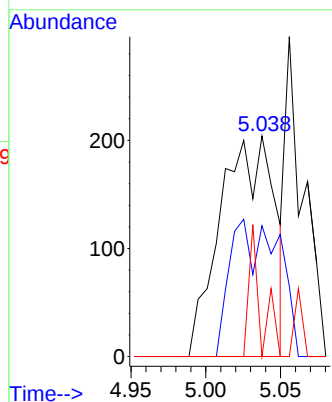

#31

Cyclohexane

Concen: 1.444 ug/l

RT: 5.544 min Scan# 731

Delta R.T. 0.073 min

Lab File: VX032181.D

Acq: 18 Oct 2022 01:57




Tgt Ion: 56 Resp: 3201


Ion Ratio Lower Upper

56 100

69 160.5 25.1 37.7#

84 101.2 70.2 105.4

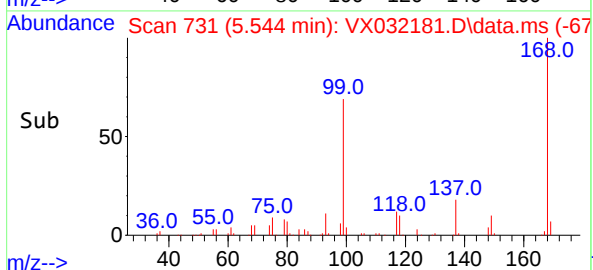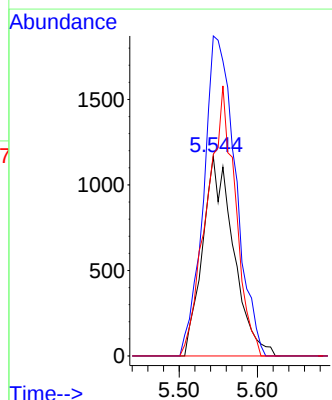



#33

1,2-Dichloroethane-d4

Concen: 50.599 ug/l

RT: 5.958 min Scan# 798

Delta R.T. 0.006 min

Lab File: VX032181.D

Acq: 18 Oct 2022 01:57

Instrument :

MSVOA_X

ClientSampleId :





SB-45

Tgt Ion: 65 Resp: 100668

Ion Ratio Lower Upper

65 100

67 49.4 0.0 102.4

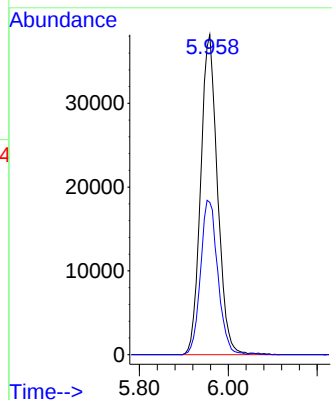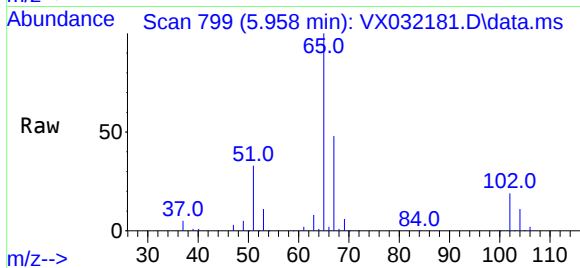

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.006 min

Lab File: VX032181.D

Acq: 18 Oct 2022 01:57




Tgt Ion: 114 Resp: 218551


Ion Ratio Lower Upper

114 100

63 21.0 0.0 42.6

88 16.7 0.0 33.0

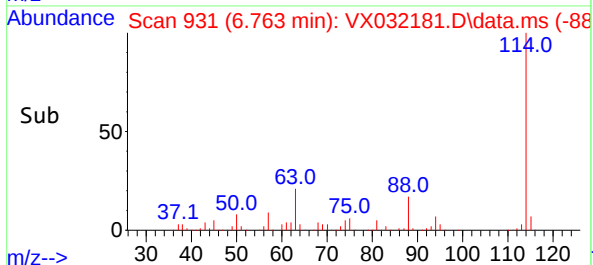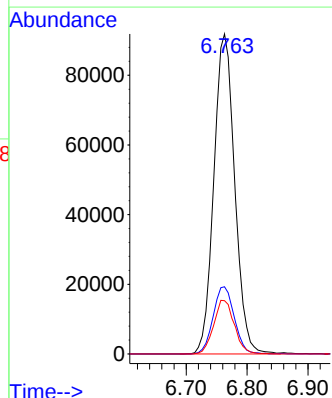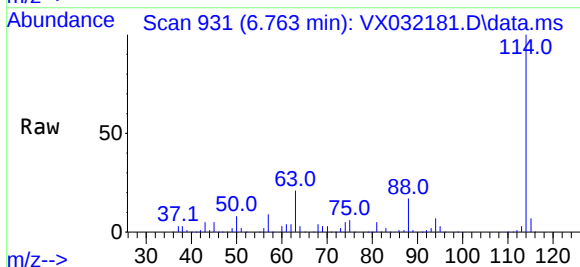

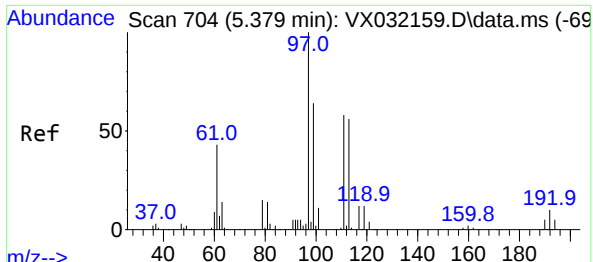

#35

Dibromofluoromethane

Concen: 48.246 ug/l

RT: 5.385 min Scan# 704

Delta R.T. 0.006 min

Lab File: VX032181.D

Acq: 18 Oct 2022 01:57

Instrument :

MSVOA_X

ClientSampleId :

SB-45





Tgt Ion:113 Resp: 71945

Ion Ratio Lower Upper

113 100

111 101.3 82.4 123.6

192 17.6 14.1 21.1

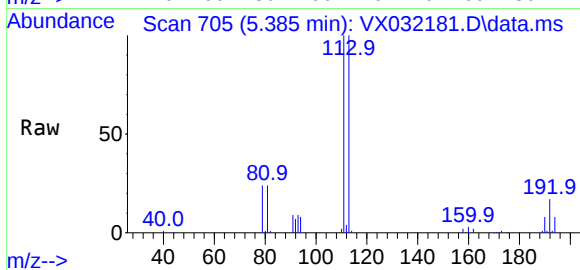

#36

1,1-Dichloropropene

Concen: 5.242 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.134 min

Lab File: VX032181.D

Acq: 18 Oct 2022 01:57




Tgt Ion: 75 Resp: 11310


Ion Ratio Lower Upper

75 100

110 9.8 17.5 52.5#

77 0.0 24.9 37.3#

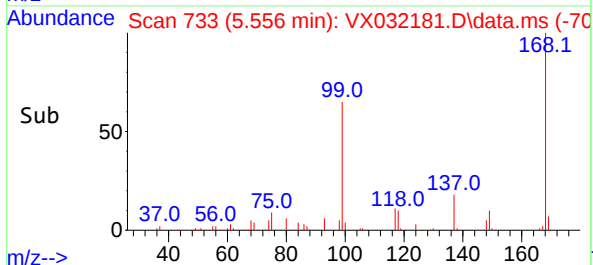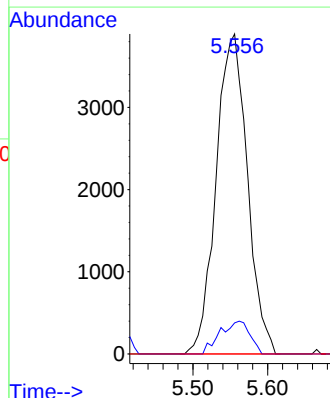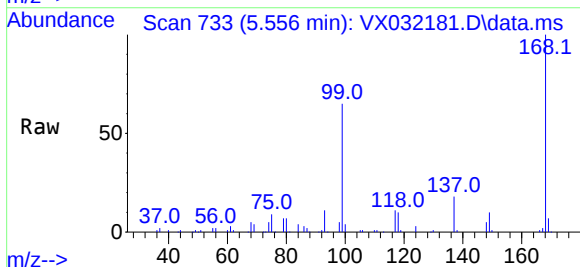



#37

Ethyl Acetate

Concen: 9.270 ug/l

RT: 4.721 min Scan# 596

Delta R.T. 0.012 min

Lab File: VX032181.D

Acq: 18 Oct 2022 01:57

Instrument :

MSVOA_X

ClientSampleId :

SB-45





Tgt Ion: 43 Resp: 20069

Ion Ratio Lower Upper

43 100

61 13.7 11.1 16.7

70 11.8 8.6 13.0

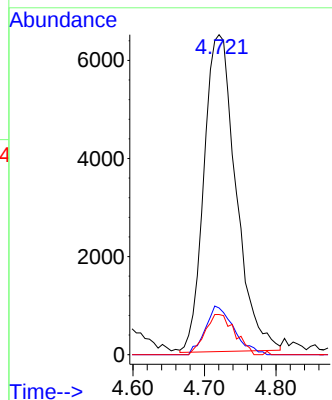

#38

Carbon Tetrachloride

Concen: 6.299 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.122 min

Lab File: VX032181.D

Acq: 18 Oct 2022 01:57




Tgt Ion: 117 Resp: 14392


Ion Ratio Lower Upper

117 100

119 4.4 74.6 112.0#

121 0.0 25.3 37.9#


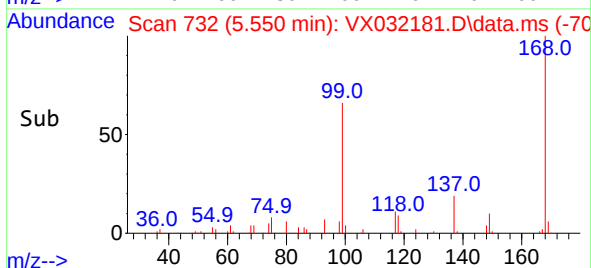
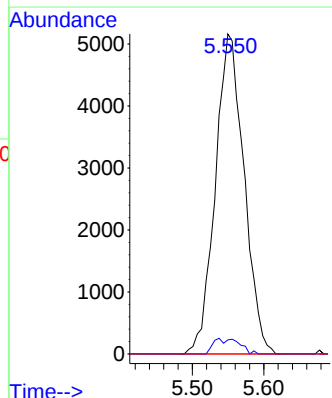





#40
Benzene
Concen: 1.355 ug/l
RT: 6.037 min Scan# 812
Delta R.T. -0.001 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57




Instrument :
MSVOA_X
ClientSampleId :
SB-45


Tgt Ion: 78 Resp: 8176
Ion Ratio Lower Upper
78 100
77 27.1 18.7 28.1

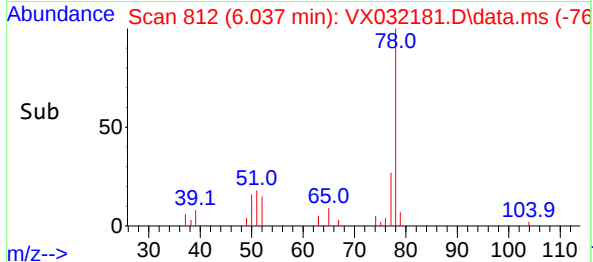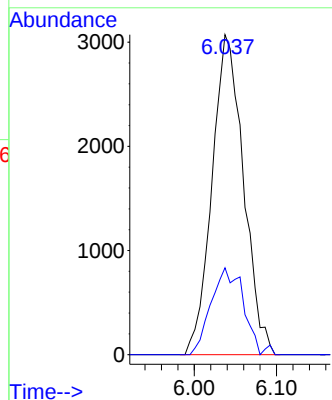

#41
Methacrylonitrile
Concen: 0.278 ug/l
RT: 5.031 min Scan# 647
Delta R.T. 0.115 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57

Tgt Ion: 41 Resp: 310
Ion Ratio Lower Upper
41 100
39 29.4 45.0 67.6#
67 0.0 58.2 87.4#
52 0.0 25.0 37.6#



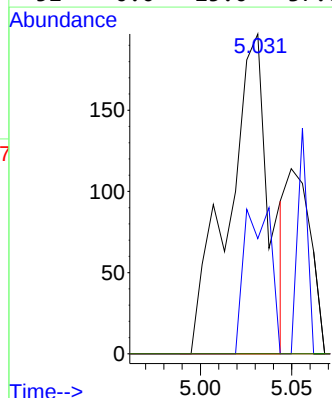





#43
Isopropyl Acetate
Concen: 28.153 ug/l
RT: 6.342 min Scan# 81
Delta R.T. 0.006 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57




Instrument :
MSVOA_X
ClientSampleId :
SB-45


Tgt Ion: 43 Resp: 91848
Ion Ratio Lower Upper
43 100
61 18.7 15.3 22.9
87 13.8 10.6 15.8

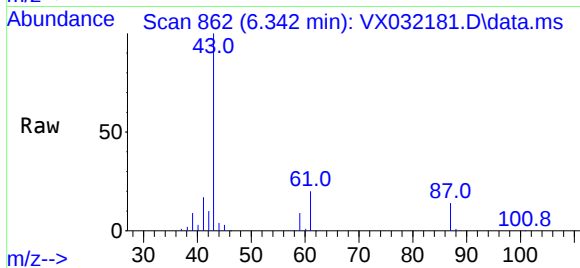

#48
Methyl methacrylate
Concen: 42.732 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.109 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57

Tgt Ion: 41 Resp: 70656
Ion Ratio Lower Upper
41 100
69 0.1 64.6 96.8#
39 58.1 51.4 77.0


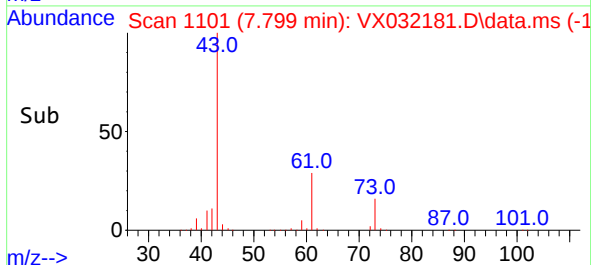
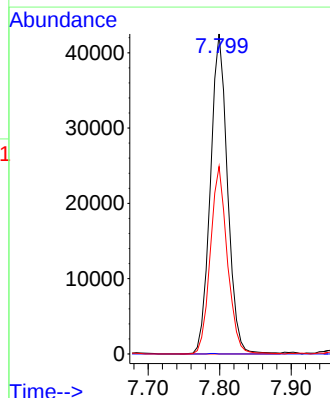
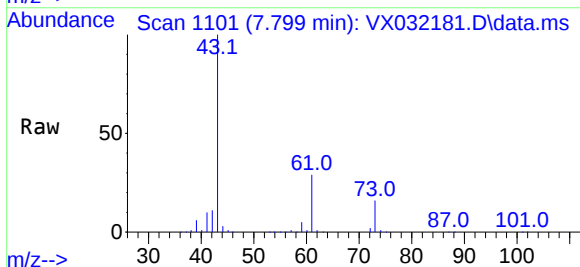




#49
1,4-Dioxane
Concen: 0.708 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.115 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57




Instrument :
MSVOA_X
ClientSampleId :
SB-45


Tgt Ion: 88 Resp: 24
Ion Ratio Lower Upper
88 100
43 2986995.8 27.1 40.7#
58 13091.7 53.9 80.9#

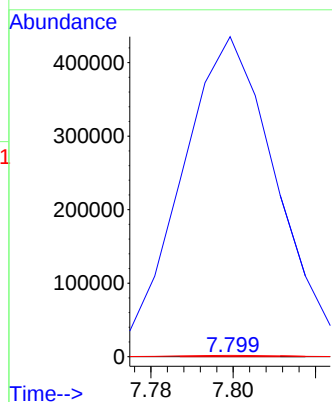

#50
Toluene-d8
Concen: 40.975 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57

Tgt Ion: 98 Resp: 214319
Ion Ratio Lower Upper
98 100
100 66.8 52.5 78.7


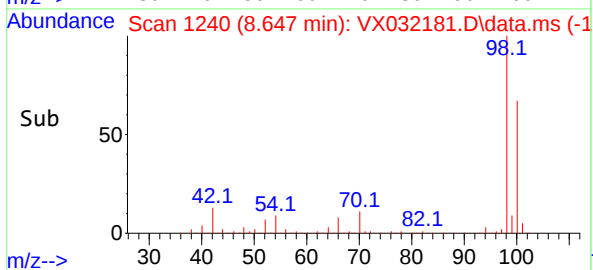
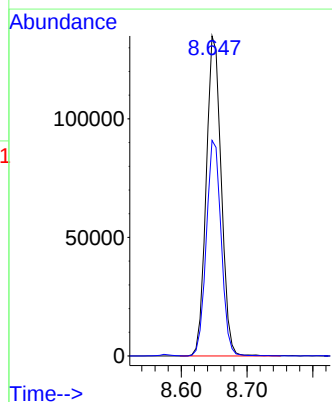





#51
4-Methyl-2-Pentanone
Concen: 29.335 ug/l
RT: 8.549 min Scan# 11
Delta R.T. -0.025 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57




Instrument :
MSVOA_X
ClientSampleId :
SB-45


Tgt Ion: 43 Resp: 58687
Ion Ratio Lower Upper
43 100
58 9.2 30.6 46.0#

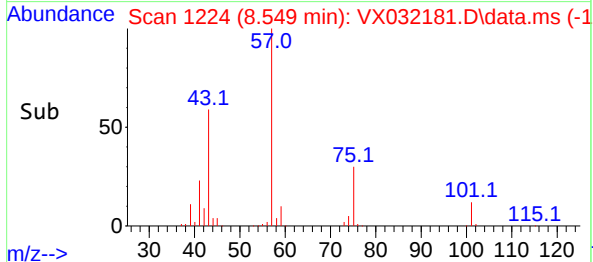

#52
Toluene
Concen: 1.528 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57

Tgt Ion: 92 Resp: 5875
Ion Ratio Lower Upper
92 100
91 169.2 137.1 205.7





#53

t-1,3-Dichloropropene

Concen: 0.273 ug/l

RT: 8.958 min Scan# 11

Delta R.T. -0.018 min

Lab File: VX032181.D

Acq: 18 Oct 2022 01:57

Instrument :

MSVOA_X

ClientSampleId :





SB-45

Tgt Ion: 75 Resp: 524

Ion Ratio Lower Upper

75 100

77 0.0 24.8 37.2#

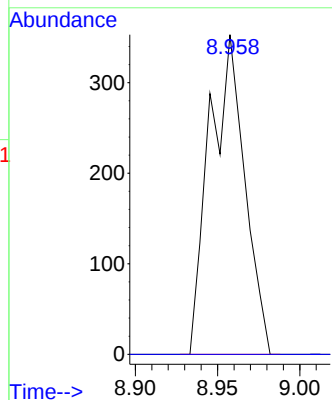

#54

cis-1,3-Dichloropropene

Concen: 12.086 ug/l

RT: 8.549 min Scan# 1224

Delta R.T. 0.183 min

Lab File: VX032181.D

Acq: 18 Oct 2022 01:57




Tgt Ion: 75 Resp: 27236


Ion Ratio Lower Upper

75 100

77 0.5 24.4 36.6#

39 35.3 43.7 65.5#

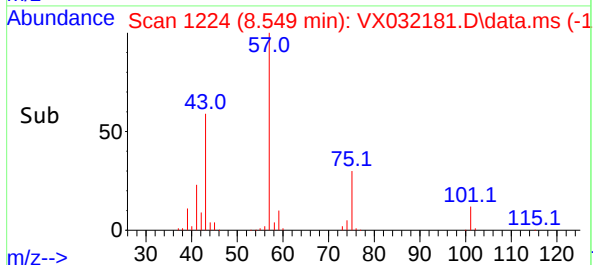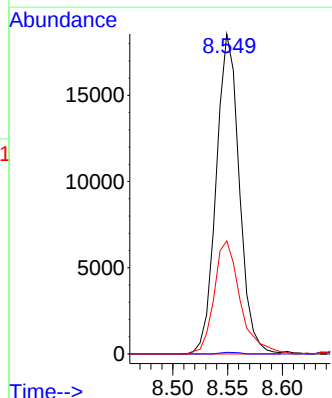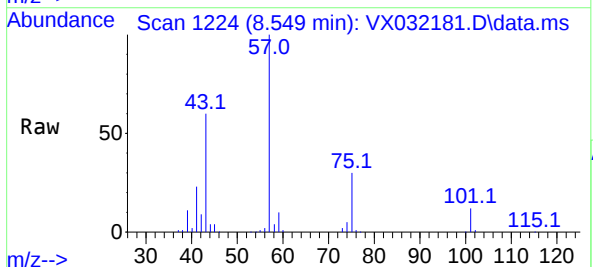



#56

Ethyl methacrylate

Concen: 0.272 ug/l

RT: 9.244 min Scan# 11

Delta R.T. 0.128 min

Lab File: VX032181.D

Acq: 18 Oct 2022 01:57

Instrument :

MSVOA_X

ClientSampleId :

SB-45


Tgt Ion: 69 Resp: 567

Ion Ratio Lower Upper




69 100

41 6966.7 54.2 81.4#

39 3277.4 34.2 51.2#



Abundance

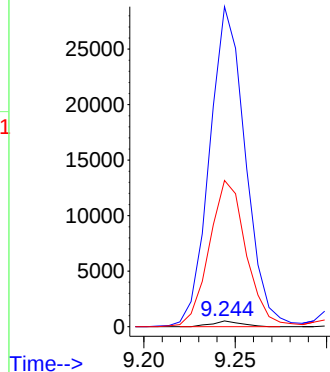

#57

1,3-Dichloropropane

Concen: 1.703 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.177 min

Lab File: VX032181.D


Acq: 18 Oct 2022 01:57

Tgt Ion: 76 Resp: 4358



Ion Ratio Lower Upper


76 100

78 0.0 25.5 38.3#



Abundance




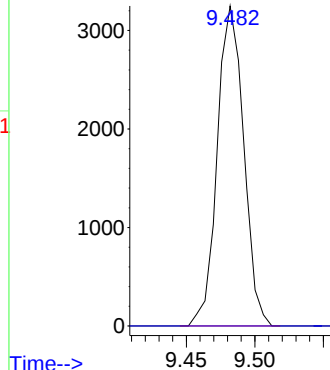




#59
2-Hexanone
Concen: 40.649 ug/l
RT: 9.482 min Scan# 11
Delta R.T. 0.055 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57




Instrument :
MSVOA_X
ClientSampleId :
SB-45


Tgt Ion: 43 Resp: 60248
Ion Ratio Lower Upper
43 100
58 18.0 26.7 80.0#

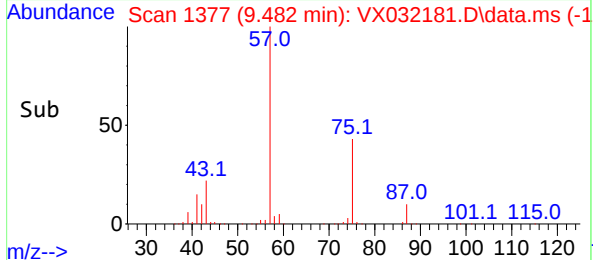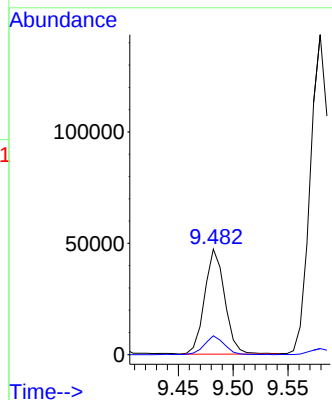

#62
4-Bromofluorobenzene
Concen: 49.728 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57

Tgt Ion: 95 Resp: 99030
Ion Ratio Lower Upper
95 100
174 73.3 0.0 153.2
176 71.9 0.0 144.0


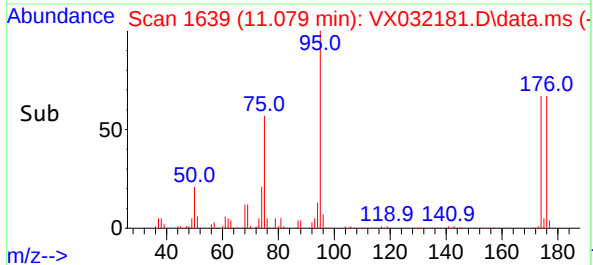
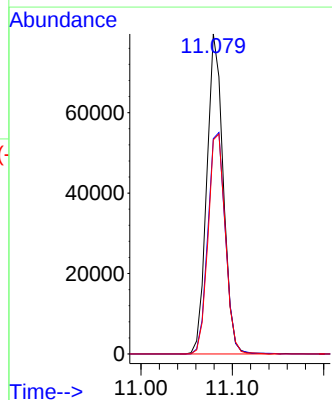
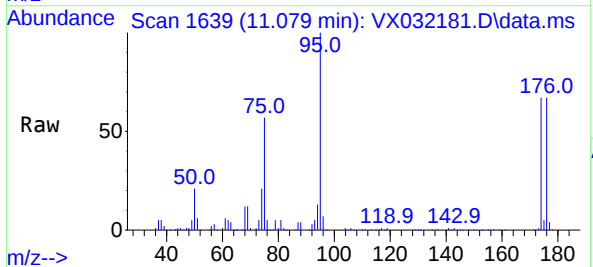




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57




Instrument :
MSVOA_X
ClientSampleId :
SB-45


Tgt Ion:117 Resp: 202313
Ion Ratio Lower Upper
117 100
82 58.0 46.8 70.2
119 32.5 26.4 39.6

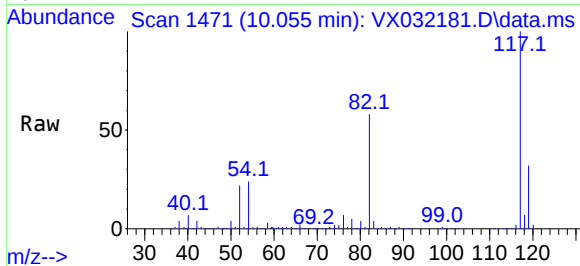

#67
Ethyl Benzene
Concen: 0.212 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57

Tgt Ion: 91 Resp: 1655
Ion Ratio Lower Upper
91 100
106 30.0 25.2 37.8


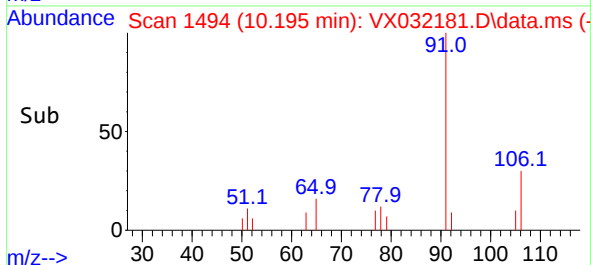
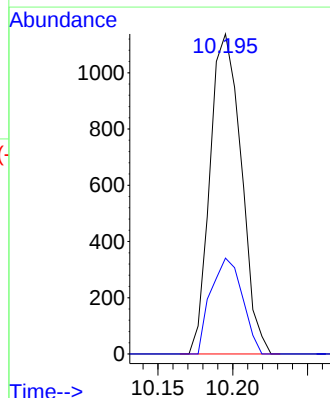
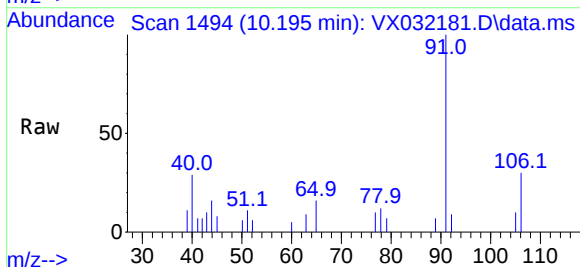




#68
m/p-Xylenes
Concen: 0.861 ug/l
RT: 10.305 min Scan# 1511
Delta R.T. 0.006 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57




Instrument :
MSVOA_X
ClientSampleId :
SB-45


Tgt Ion:106 Resp: 2580
Ion Ratio Lower Upper
106 100
91 215.3 161.0 241.4

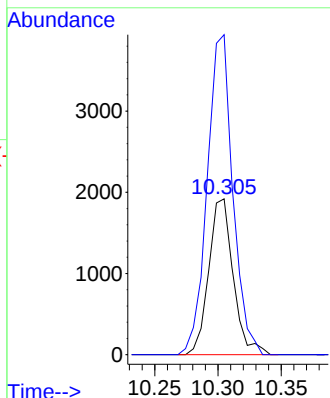

#69
o-Xylene
Concen: 0.524 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.006 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57

Tgt Ion:106 Resp: 1546
Ion Ratio Lower Upper
106 100
91 229.8 107.2 321.6


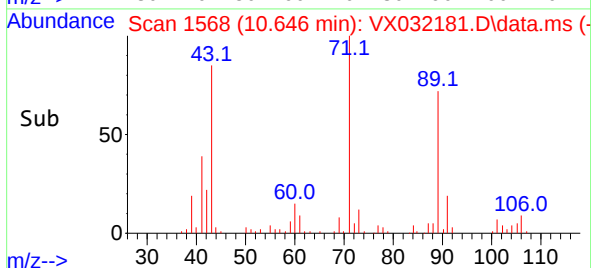






#70
Styrene
Concen: 0.360 ug/l
RT: 10.658 min Scan# 11
Delta R.T. 0.005 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57




Instrument :
MSVOA_X
ClientSampleId :
SB-45


Tgt Ion:104 Resp: 1716
Ion Ratio Lower Upper
104 100
78 61.8 41.4 62.2
103 59.7 43.8 65.8

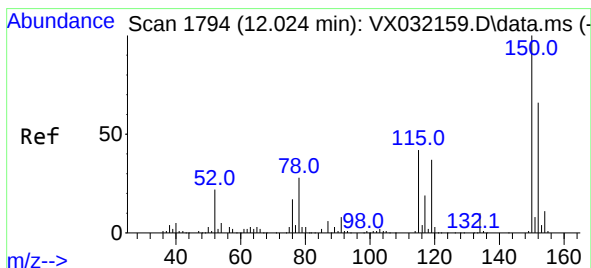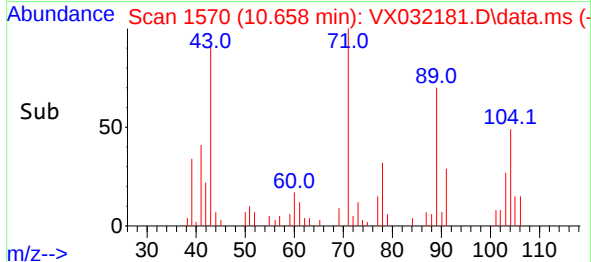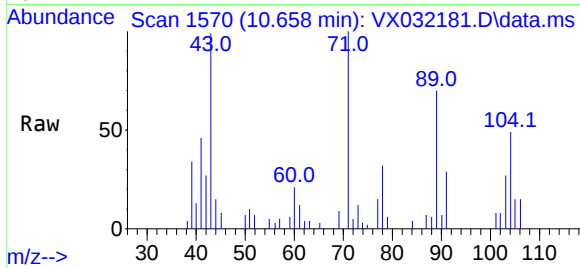

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57

Tgt Ion:152 Resp: 91812
Ion Ratio Lower Upper
152 100
115 63.2 43.4 130.1
150 157.5 0.0 346.8


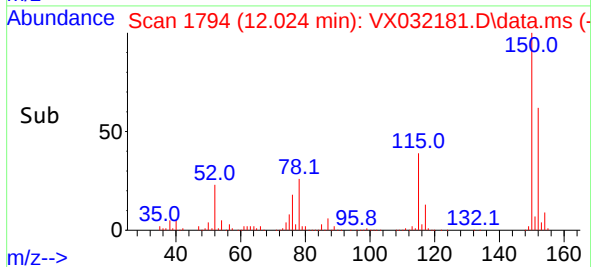

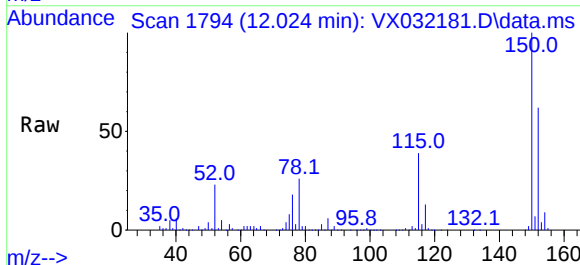




#74
N-amy1 acetate
Concen: 8.072 ug/l
RT: 10.640 min Scan# 11
Delta R.T. -0.202 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57




Instrument :
MSVOA_X
ClientSampleId :
SB-45


Tgt Ion: 43	Resp: 19619
Ion Ratio	Lower Upper
43 100	
70 2.0	33.4 50.2#
55 5.0	18.2 27.2#
61 9.6	19.3 28.9#

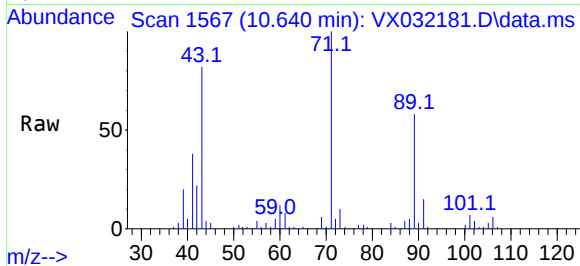

#76
1,2,3-Trichloropropane
Concen: 28.277 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57

Tgt Ion: 75	Resp: 56292
Ion Ratio	Lower Upper
75 100	
77 1.1	20.3 60.9#


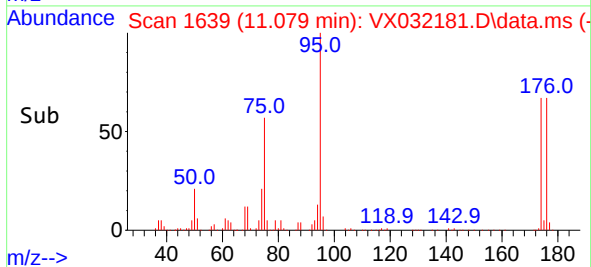

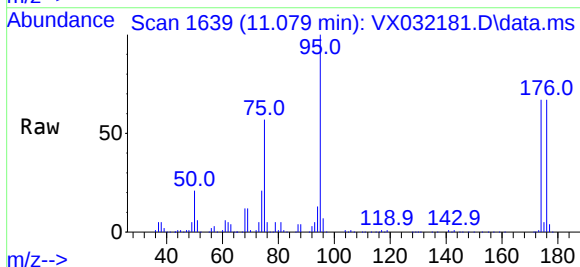




#81
trans-1,4-Dichloro-2-butene
Concen: 108.857 ug/l
RT: 11.079 min Scan# 11
Delta R.T. 0.061 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57




Instrument :
MSVOA_X
ClientSampleId :
SB-45


Tgt Ion: 75 Resp: 56292
Ion Ratio Lower Upper
75 100
53 0.0 77.6 116.4#
89 0.0 37.4 56.0#

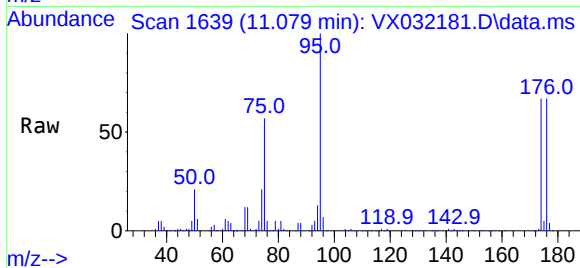

#84
1,2,4-Trimethylbenzene
Concen: 0.481 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57

Tgt Ion:105 Resp: 2963
Ion Ratio Lower Upper
105 100
120 20.3 22.6 67.8#


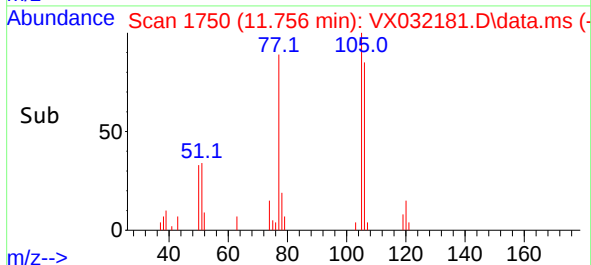

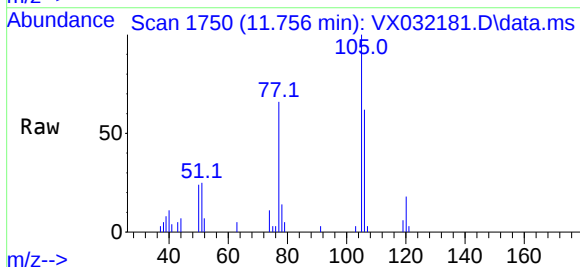




#85
sec-Butylbenzene
Concen: 0.393 ug/l
RT: 11.756 min Scan# 11
Delta R.T. -0.134 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57




Instrument :
MSVOA_X
ClientSampleId :
SB-45


Tgt Ion:105 Resp: 2963
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#

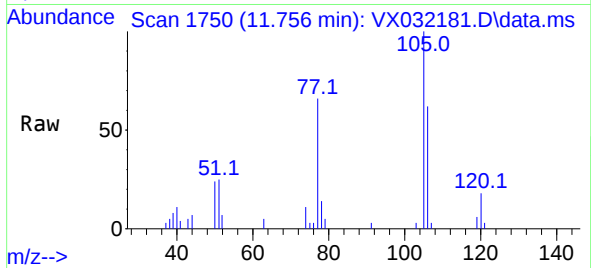

#90
Hexachloroethane
Concen: 0.210 ug/l
RT: 12.408 min Scan# 1857
Delta R.T. -0.135 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57


Tgt Ion:117 Resp: 183
Ion Ratio Lower Upper
117 100
201 0.0 34.8 104.4#

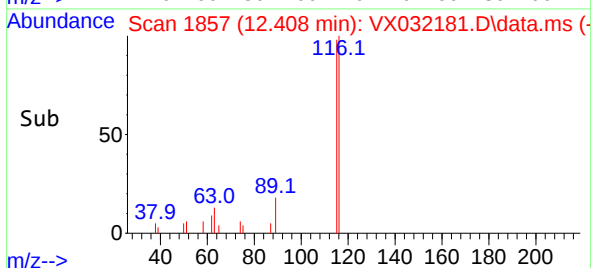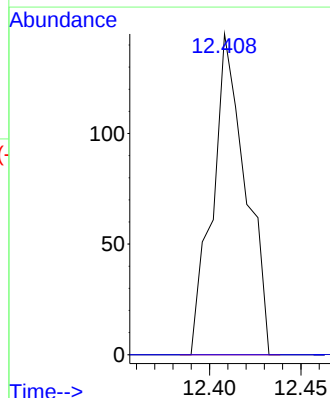



#95
Naphthalene
Concen: 3.417 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX032181.D
Acq: 18 Oct 2022 01:57

Instrument :
MSVOA_X
ClientSampleId :
SB-45

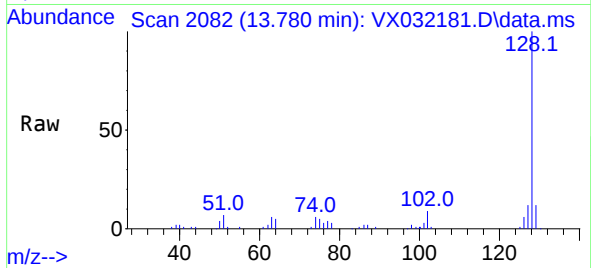

Tgt Ion:128 Resp: 19794

Ion	Ratio	Lower	Upper
128	100		
127	12.3	10.4	15.6
129	10.8	8.8	13.2

