
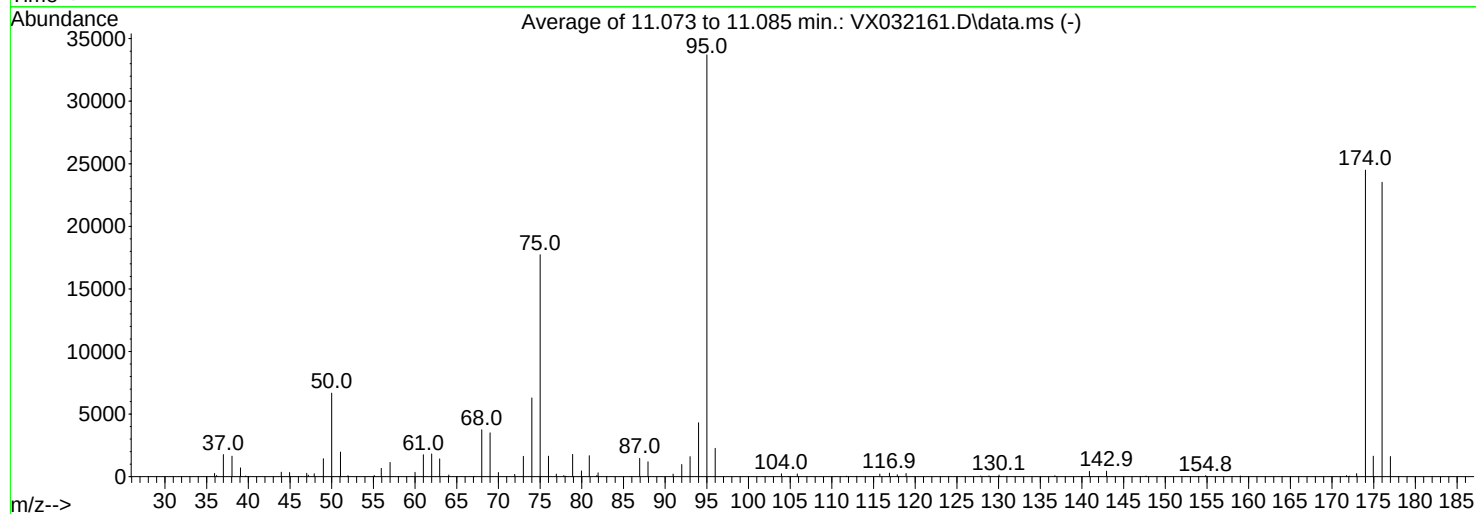


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101722\
 Data File : VX032161.D
 Acq On : 17 Oct 2022 17:44
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101722W.M
 Title : SW846 8260
 Last Update : Tue Oct 18 04:18:35 2022

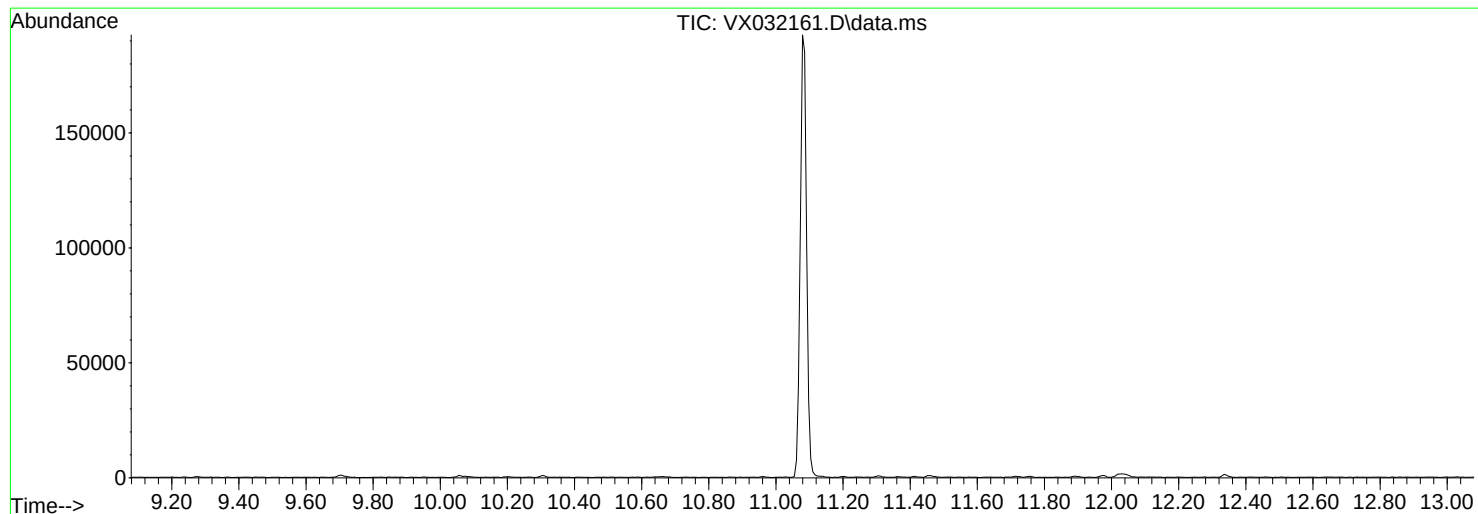

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	6676	PASS
75	95	30	60	52.6	17734	PASS
95	95	100	100	100.0	33704	PASS
96	95	5	9	6.7	2268	PASS
173	174	0.00	2	1.0	243	PASS
174	95	50	100	72.7	24502	PASS
175	174	5	9	6.7	1638	PASS
176	174	95	101	96.0	23529	PASS
177	176	5	9	6.8	1611	PASS