

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101823\
 Data File : VX038359.D
 Acq On : 18 Oct 2023 13:53
 Operator : JC/MD
 Sample : 04924-03 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 50102

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
 Title : SW846 8260

Signal : TIC: VX038359.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	51	rBV2	7068	8756	1.22%	0.192%
2	2.056	151	159	165	rBV4	4734	11129	1.55%	0.244%
3	2.215	181	185	190	rVB3	5313	7969	1.11%	0.175%
4	3.117	326	333	340	rBV2	5175	12173	1.70%	0.267%
5	4.568	560	571	579	rBV2	4486	14918	2.08%	0.327%
6	5.391	693	706	721	rBV2	77575	230254	32.13%	5.047%
7	5.556	722	733	747	rVB	125877	354148	49.42%	7.763%
8	5.952	788	798	806	rBV	87265	231200	32.26%	5.068%
9	6.037	806	812	827	rVB	43215	119460	16.67%	2.619%
10	6.763	922	931	944	rBV	205822	492712	68.75%	10.800%
11	8.647	1234	1240	1247	rBV	445500	699625	97.63%	15.336%
12	8.720	1247	1252	1267	rVB	188951	299519	41.80%	6.565%
13	10.055	1465	1471	1486	rVB	491652	668258	93.25%	14.648%
14	10.195	1486	1494	1500	rBV	17155	23000	3.21%	0.504%
15	10.299	1506	1511	1520	rBV	50596	71799	10.02%	1.574%
16	10.640	1561	1567	1575	rBV	26036	36676	5.12%	0.804%
17	11.079	1634	1639	1649	rBV	411846	531334	74.14%	11.647%
18	11.378	1684	1688	1691	rBV	5878	8051	1.12%	0.176%
19	11.750	1745	1749	1756	rBV	13172	16630	2.32%	0.365%
20	12.018	1788	1793	1801	rBV	532794	716638	100.00%	15.709%
21	12.085	1801	1804	1811	rVB	5054	7819	1.09%	0.171%




Sum of corrected areas: 4562068

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101823\
Data File : VX038359.D
Acq On : 18 Oct 2023 13:53
Operator : JC/MD
Sample : 04924-03 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50102

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

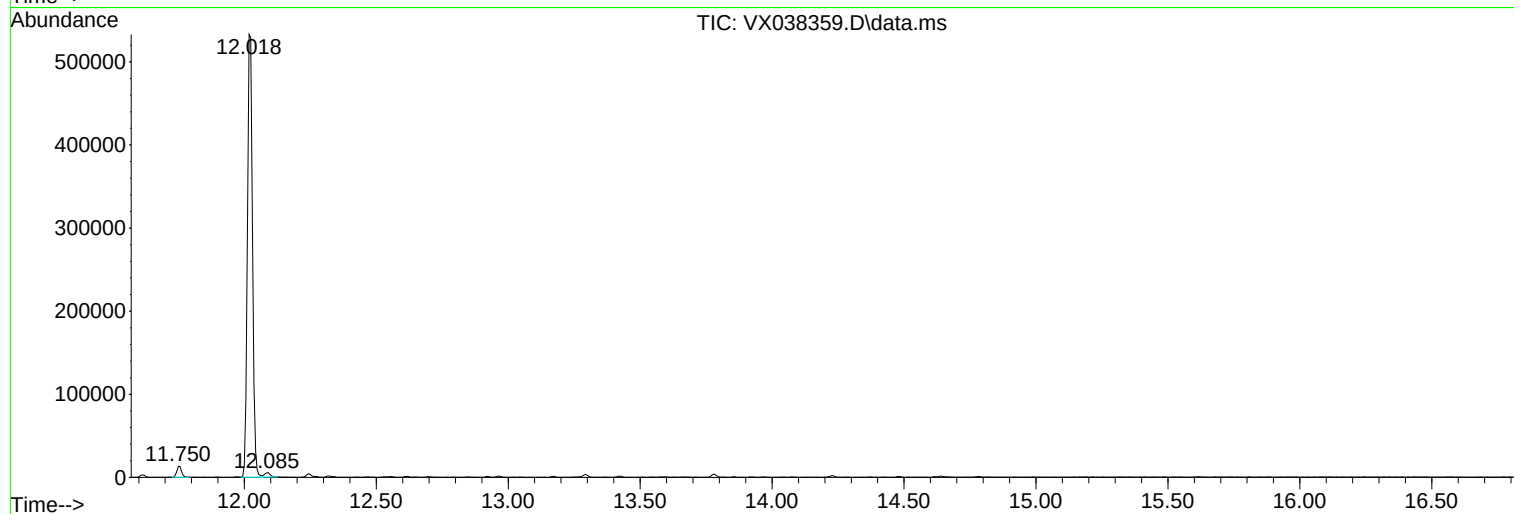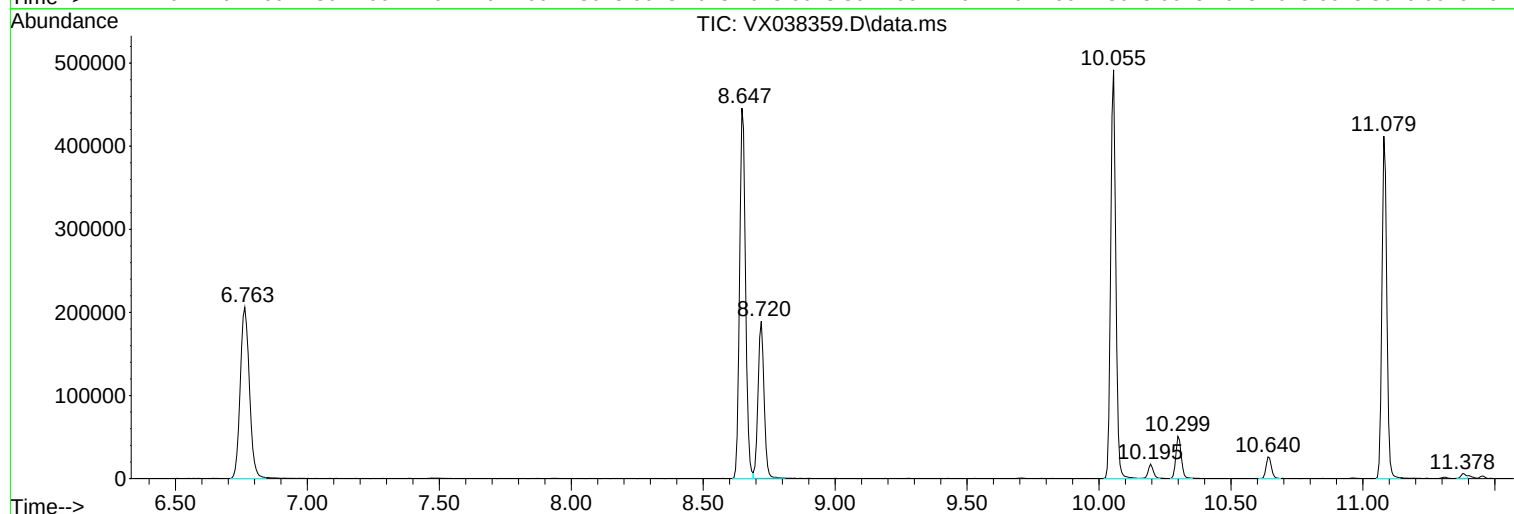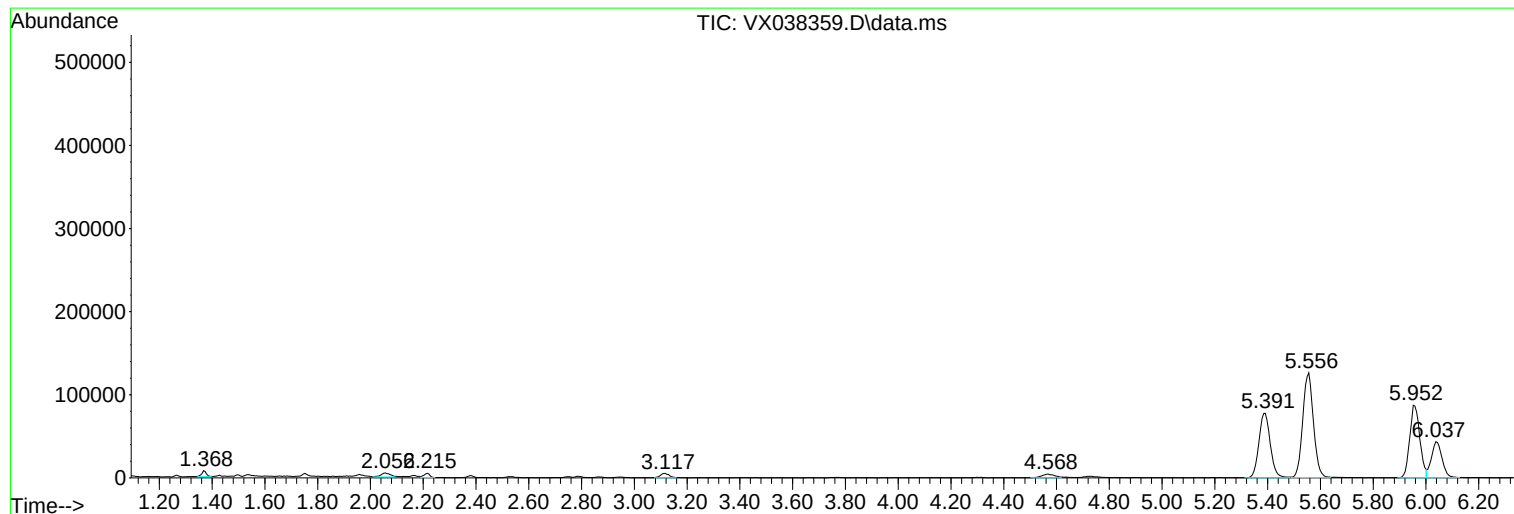

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101823\
Data File : VX038359.D
Acq On : 18 Oct 2023 13:53
Operator : JC/MD
Sample : 04924-03 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50102

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101823\
Data File : VX038359.D
Acq On : 18 Oct 2023 13:53
Operator : JC/MD
Sample : 04924-03 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
50102

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------