

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101921\
 Data File : VX024844.D
 Acq On : 19 Oct 2021 13:33
 Operator : JC/MD
 Sample : M4181-02ME
 Misc : 6.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B07ME

Quant Time: Oct 20 04:22:45 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 20 04:21:44 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	290208	50.00	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	262462	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	133326	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	61818	34.40	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 68.80%			
7) Chloroethane-d5	1.648	69	38546	32.59	ug/L	-0.02
Spiked Amount 50.000	Range 70 - 130		Recovery = 65.18%#			
11) 1,1-Dichloroethene-d2	2.282	63	94739	26.85	ug/L	-0.03
Spiked Amount 50.000	Range 60 - 125		Recovery = 53.70%#			
21) 2-Butanone-d5	4.489	46	152232	103.05	ug/L	0.03
Spiked Amount 100.000	Range 40 - 130		Recovery = 103.05%			
24) Chloroform-d	5.062	84	143161	39.34	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 78.68%			
26) 1,2-Dichloroethane-d4	5.958	65	103385	40.17	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 80.34%			
32) Benzene-d6	5.977	84	273272	36.96	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 73.92%			
36) 1,2-Dichloropropane-d6	7.312	67	96173	41.59	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 83.18%			
41) Toluene-d8	8.647	98	251677	34.94	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 69.88%#			
43) trans-1,3-Dichloroprop...	8.952	79	42004	36.66	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 73.32%			
47) 2-Hexanone-d5	9.397	63	100672	92.73	ug/L	0.01
Spiked Amount 100.000	Range 45 - 130		Recovery = 92.73%			
56) 1,1,2,2-Tetrachloroeth...	11.195	84	137744	43.25	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 86.50%			
66) 1,2-Dichlorobenzene-d4	12.323	152	107112	41.06	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 82.12%			
Target Compounds						Qvalue
16) Methylene chloride	2.782	84	1257	0.63	ug/L	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101921\
Data File : VX024844.D
Acq On : 19 Oct 2021 13:33
Operator : JC/MD
Sample : M4181-02ME
Misc : 6.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B07ME


Quant Time: Oct 20 04:22:45 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM100721WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 20 04:21:44 2021
Response via : Initial Calibration

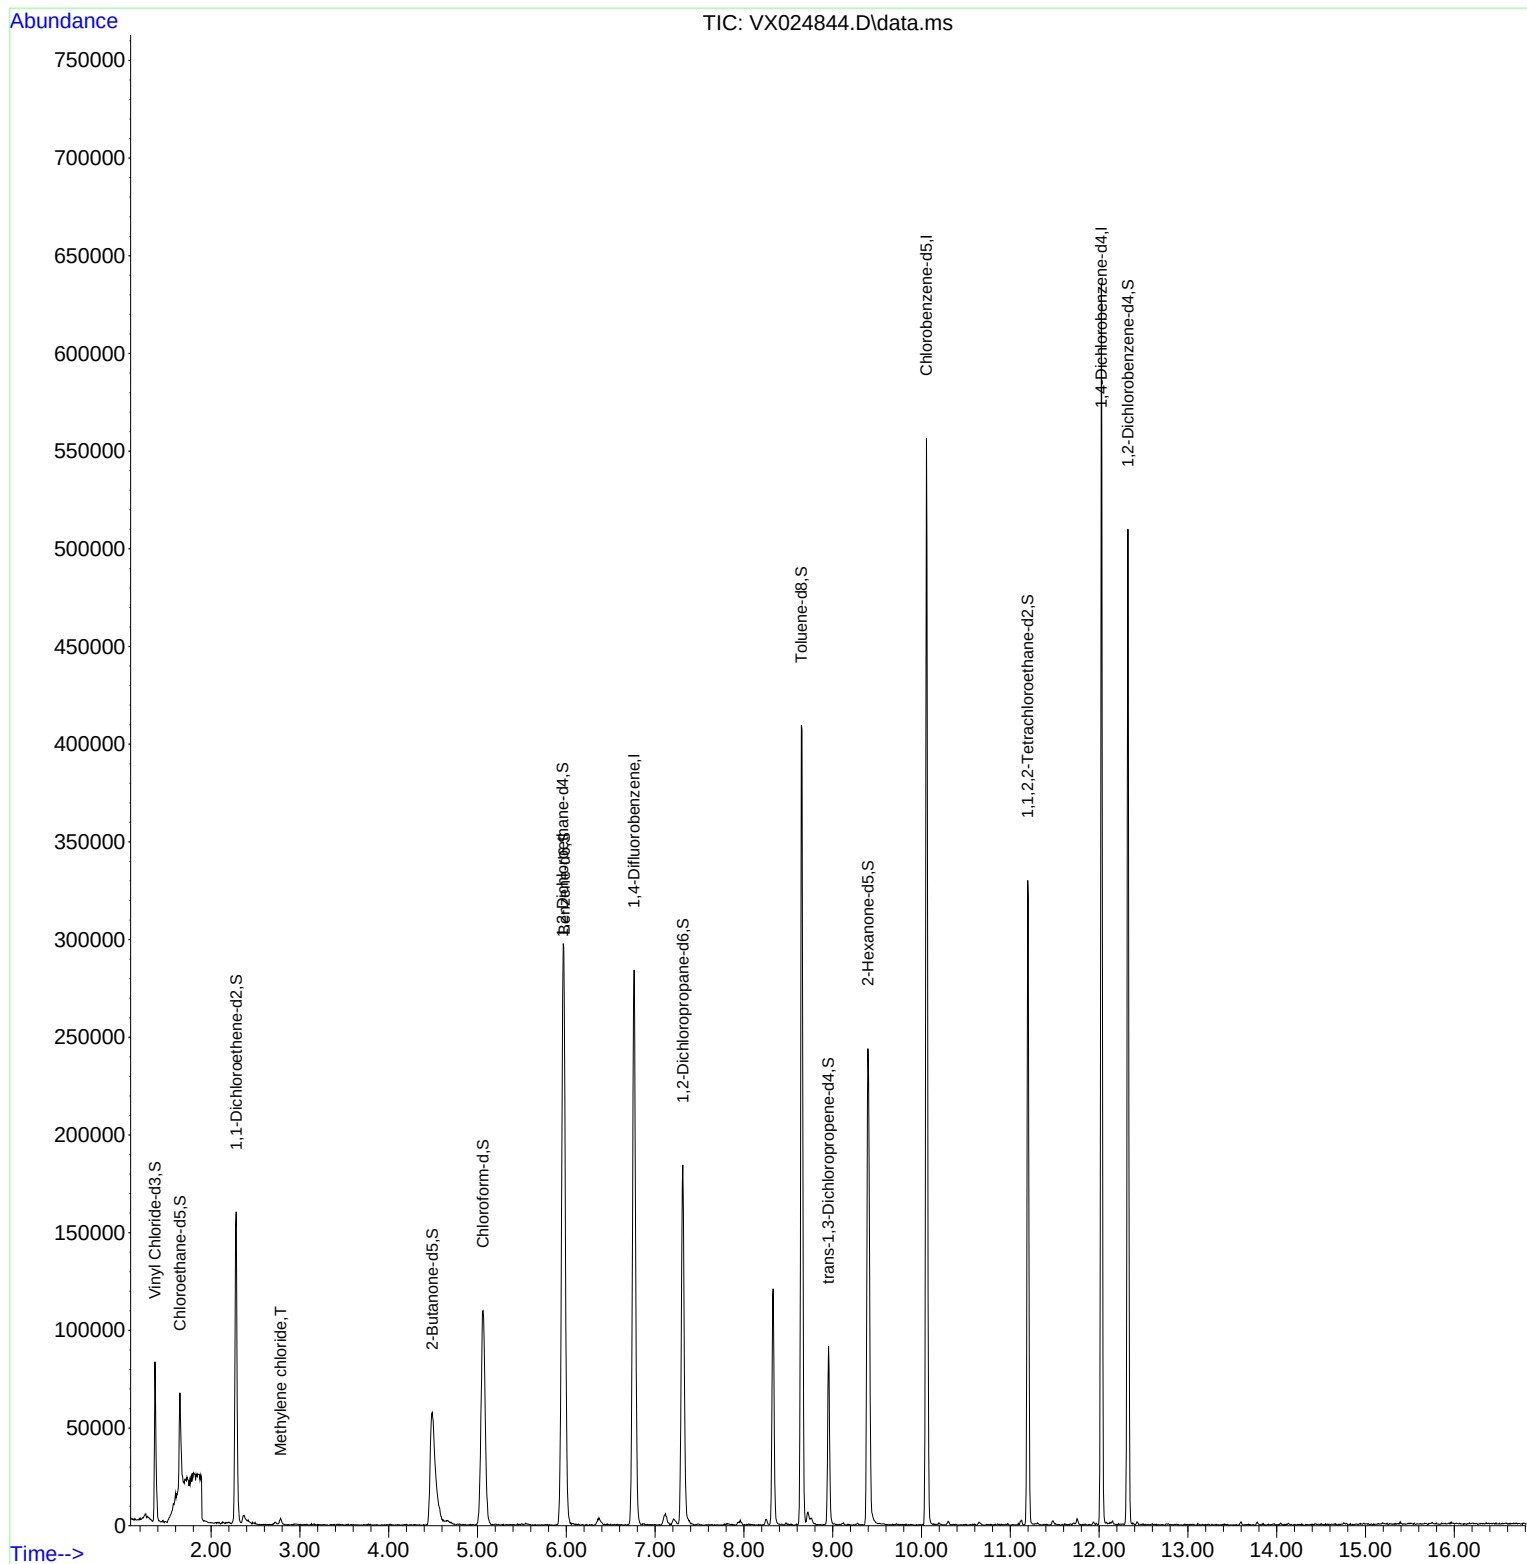

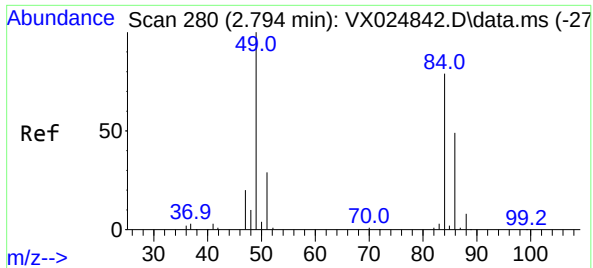

#16
Methylene chloride
Concen: 0.63 ug/L
RT: 2.782 min Scan# 278
Delta R.T. -0.012 min
Lab File: VX024844.D
Acq: 19 Oct 2021 13:33

Instrument :
MSVOA_X
ClientSampleId :
C0B07ME

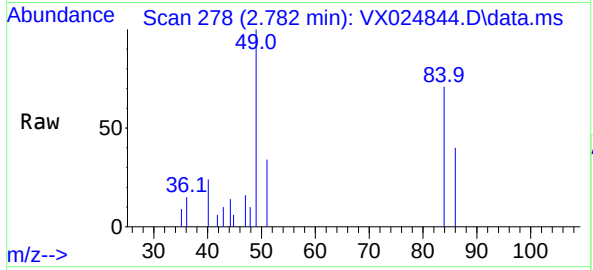

Tgt Ion: 84 Resp: 1257

Ion	Ratio	Lower	Upper
84	100		
86	56.4	44.2	82.0
49	141.5	77.8	144.6

