

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101921\
 Data File : VX024843.D
 Acq On : 19 Oct 2021 13:04
 Operator : JC/MD
 Sample : VX1019MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK611

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M

Title : VOC Analysis

Signal : TIC: VX024843.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	55	rVB	101390	103472	12.24%	1.530%
2	1.672	91	96	103	rVB	74809	93633	11.07%	1.385%
3	2.312	194	201	212	rVB	158812	269937	31.92%	3.993%
4	2.520	229	235	242	rBV3	1325	3151	0.37%	0.047%
5	2.703	263	265	271	rVB3	696	1038	0.12%	0.015%
6	2.794	273	280	286	rBV3	1478	3181	0.38%	0.047%
7	3.081	324	327	328	rBV	947	838	0.10%	0.012%
8	3.196	344	346	348	rBV2	393	437	0.05%	0.006%
9	3.300	361	363	367	rVB	376	412	0.05%	0.006%
10	3.367	369	374	376	rBV	487	695	0.08%	0.010%
11	3.538	401	402	407	rBV2	344	548	0.06%	0.008%
12	3.587	409	410	415	rVB2	602	730	0.09%	0.011%
13	3.623	415	416	421	rBV2	377	551	0.07%	0.008%
14	3.678	421	425	426	rBV2	367	394	0.05%	0.006%
15	3.824	447	449	453	rVB2	535	549	0.06%	0.008%
16	4.464	544	554	571	rBV	88338	250302	29.60%	3.702%
17	4.696	591	592	595	rVB2	524	407	0.05%	0.006%
18	4.794	605	608	610	rBV2	512	707	0.08%	0.010%
19	5.062	637	652	670	rBV2	113026	349843	41.37%	5.174%
20	5.385	702	705	707	rBV	784	703	0.08%	0.010%
21	5.446	714	715	720	rBV2	346	600	0.07%	0.009%
22	5.543	728	731	733	rBV2	836	1020	0.12%	0.015%
23	5.678	751	753	755	rBV2	419	418	0.05%	0.006%
24	5.976	790	802	817	rBV2	285958	845627	100.00%	12.507%
25	6.287	851	853	854	rBV2	724	415	0.05%	0.006%
26	6.482	883	885	889	rVB2	545	633	0.07%	0.009%
27	6.556	893	897	898	rBV	328	455	0.05%	0.007%
28	6.763	920	931	944	rBV	251182	596752	70.57%	8.826%
29	6.854	944	946	949	rVB3	798	872	0.10%	0.013%
30	6.964	960	964	967	rVB3	428	595	0.07%	0.009%
31	7.007	969	971	973	rVB	531	499	0.06%	0.007%
32	7.055	976	979	982	rBV	593	766	0.09%	0.011%
33	7.116	982	989	995	rBV4	6373	14838	1.75%	0.219%
34	7.311	1012	1021	1036	rBV2	182601	400041	47.31%	5.917%
35	7.476	1045	1048	1052	rVB2	651	1049	0.12%	0.016%
36	7.519	1052	1055	1057	rBV	433	383	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101921\
 Data File : VX024843.D
 Acq On : 19 Oct 2021 13:04
 Operator : JC/MD
 Sample : VX1019MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK611

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM100721WMA.M
 Title : VOC Analysis

37	7.677	1079	1081	1087	rVB2	391	372	0.04%	0.006%
38	7.738	1087	1091	1096	rVB2	577	875	0.10%	0.013%
39	7.775	1096	1097	1100	rBV	602	757	0.09%	0.011%
40	7.878	1113	1114	1118	rVB2	404	377	0.04%	0.006%
41	7.927	1118	1122	1129	rVB3	1284	2102	0.25%	0.031%
42	8.250	1173	1175	1178	rBV2	455	562	0.07%	0.008%
43	8.330	1181	1188	1201	rBV	124229	210170	24.85%	3.109%
44	8.470	1209	1211	1213	rBV3	939	639	0.08%	0.009%
45	8.653	1234	1241	1249	rBV	406317	635561	75.16%	9.400%
46	8.811	1265	1267	1269	rBV	405	407	0.05%	0.006%
47	8.951	1284	1290	1298	rBV	97275	137724	16.29%	2.037%
48	9.116	1315	1317	1319	rBV2	723	505	0.06%	0.007%
49	9.281	1342	1344	1347	rVB2	648	508	0.06%	0.008%
50	9.384	1356	1361	1381	rVB	329480	497031	58.78%	7.351%
51	9.902	1444	1446	1447	rBV2	358	367	0.04%	0.005%
52	10.055	1465	1471	1481	rBV	513414	672044	79.47%	9.940%
53	10.201	1489	1495	1497	rBV4	851	1483	0.18%	0.022%
54	10.305	1509	1512	1515	rVB2	1884	2078	0.25%	0.031%
55	10.354	1519	1520	1524	rVV3	425	384	0.05%	0.006%
56	10.463	1535	1538	1541	rVB	323	514	0.06%	0.008%
57	10.658	1565	1570	1574	rBV4	1432	2640	0.31%	0.039%
58	10.921	1611	1613	1615	rBV	424	469	0.06%	0.007%
59	10.963	1618	1620	1623	rBV	770	891	0.11%	0.013%
60	11.085	1637	1640	1642	rBV2	469	571	0.07%	0.008%
61	11.116	1642	1645	1652	rVV3	1363	2264	0.27%	0.033%
62	11.195	1653	1658	1670	rVB	340888	425691	50.34%	6.296%
63	11.280	1670	1672	1675	rBV2	535	489	0.06%	0.007%
64	11.378	1685	1688	1690	rBV2	573	536	0.06%	0.008%
65	11.427	1694	1696	1698	rBV	421	389	0.05%	0.006%
66	11.451	1698	1700	1704	rBV2	957	1227	0.15%	0.018%
67	11.579	1717	1721	1724	rBV3	407	592	0.07%	0.009%
68	11.616	1725	1727	1730	rVB2	701	697	0.08%	0.010%
69	11.677	1734	1737	1740	rBV2	592	891	0.11%	0.013%
70	11.750	1746	1749	1754	rVB5	2442	2865	0.34%	0.042%
71	11.890	1769	1772	1775	rBV2	644	636	0.08%	0.009%
72	11.933	1777	1779	1782	rBV2	837	944	0.11%	0.014%
73	11.975	1783	1786	1789	rVB2	1163	1285	0.15%	0.019%
74	12.024	1789	1794	1802	rBV	504834	618152	73.10%	9.143%
75	12.268	1832	1834	1836	rBV2	379	436	0.05%	0.006%
76	12.323	1837	1843	1851	rVV	448999	568150	67.19%	8.403%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101921\
 Data File : VX024843.D
 Acq On : 19 Oct 2021 13:04
 Operator : JC/MD
 Sample : VX1019MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK611

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
 Title : VOC Analysis

77	12.445	1860	1863	1865	rBV	408	446	0.05%	0.007%
78	12.725	1907	1909	1911	rBV2	436	399	0.05%	0.006%
79	12.804	1920	1922	1926	rBV2	428	437	0.05%	0.006%
80	13.091	1967	1969	1970	rVV	474	367	0.04%	0.005%
81	13.115	1970	1973	1978	rVB2	1241	1705	0.20%	0.025%
82	13.256	1993	1996	1997	rBV	440	376	0.04%	0.006%
83	13.396	2016	2019	2023	rBV	678	624	0.07%	0.009%
84	13.469	2027	2031	2033	rBV	375	457	0.05%	0.007%
85	13.591	2047	2051	2055	rVB4	2150	2947	0.35%	0.044%
86	13.780	2078	2082	2086	rVB	1321	1977	0.23%	0.029%
87	13.816	2086	2088	2092	rVB2	501	762	0.09%	0.011%
88	13.890	2095	2100	2102	rBV	318	427	0.05%	0.006%
89	13.969	2109	2113	2118	rVB3	1254	1711	0.20%	0.025%
90	14.152	2141	2143	2146	rBV3	795	804	0.10%	0.012%
91	14.469	2193	2195	2198	rBV2	368	380	0.04%	0.006%
92	14.835	2251	2255	2259	rBV2	774	1515	0.18%	0.022%
93	14.950	2272	2274	2275	rBV2	750	682	0.08%	0.010%
94	15.426	2350	2352	2355	rBV2	682	765	0.09%	0.011%
95	15.450	2355	2356	2359	rVB3	755	609	0.07%	0.009%
96	15.578	2375	2377	2378	rBV2	648	421	0.05%	0.006%
97	15.810	2414	2415	2419	rVB3	821	664	0.08%	0.010%
98	16.133	2464	2468	2469	rBV	767	780	0.09%	0.012%
99	16.194	2477	2478	2480	rBV2	451	463	0.05%	0.007%
100	16.566	2537	2539	2542	rVB	661	480	0.06%	0.007%

Sum of corrected areas: 6760964




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101921\
Data File : VX024843.D
Acq On : 19 Oct 2021 13:04
Operator : JC/MD
Sample : VX1019MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK611

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM100721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

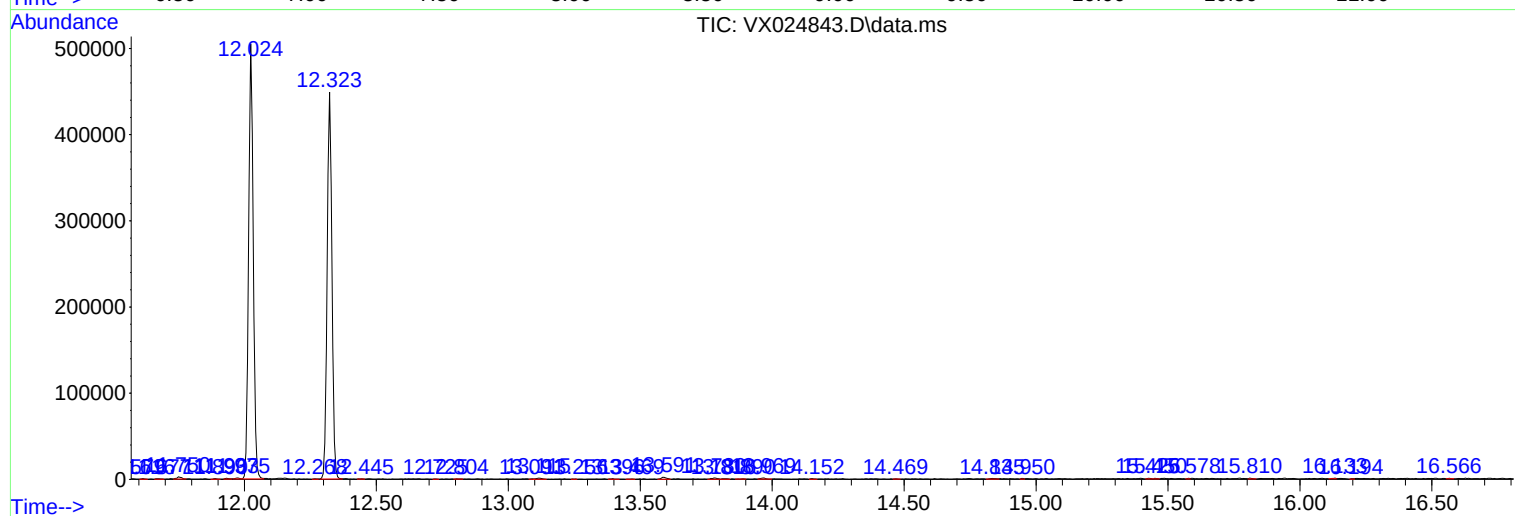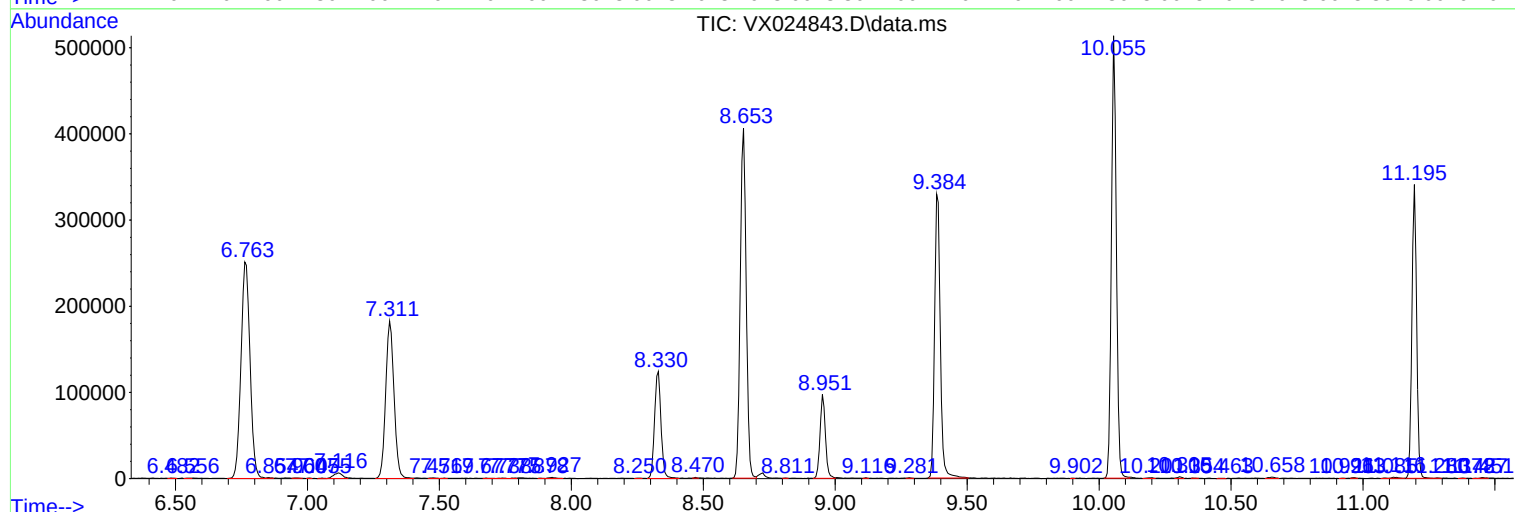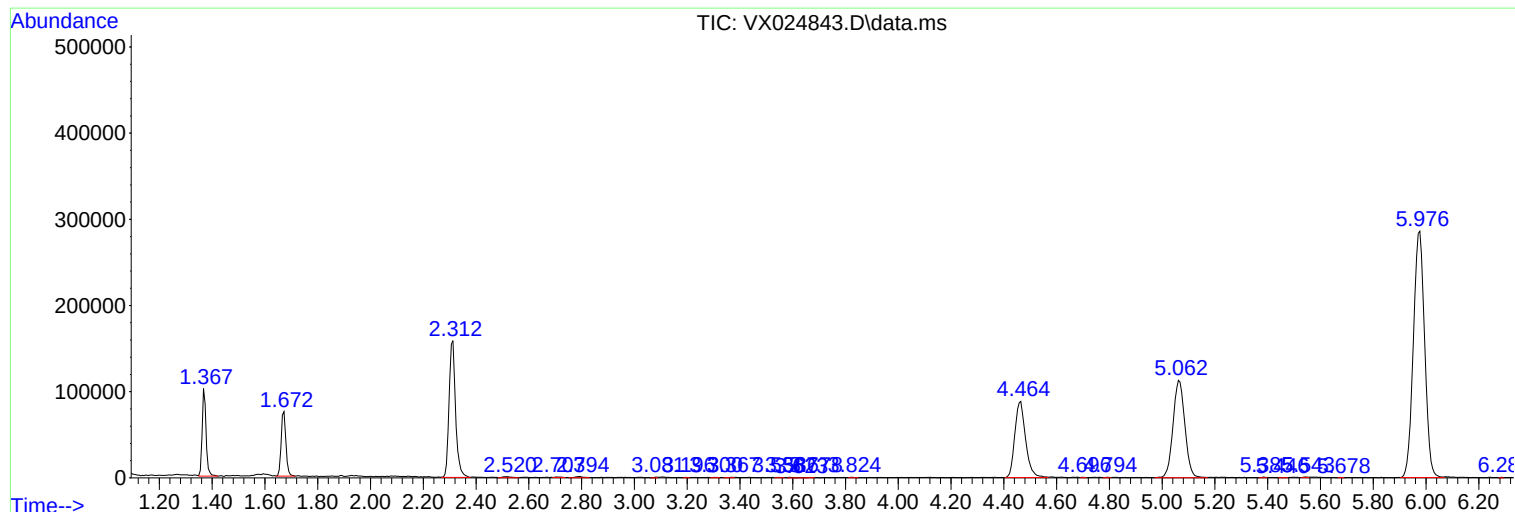

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101921\
Data File : VX024843.D
Acq On : 19 Oct 2021 13:04
Operator : JC/MD
Sample : VX1019MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK611

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101921\
Data File : VX024843.D
Acq On : 19 Oct 2021 13:04
Operator : JC/MD
Sample : VX1019MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK611

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc