
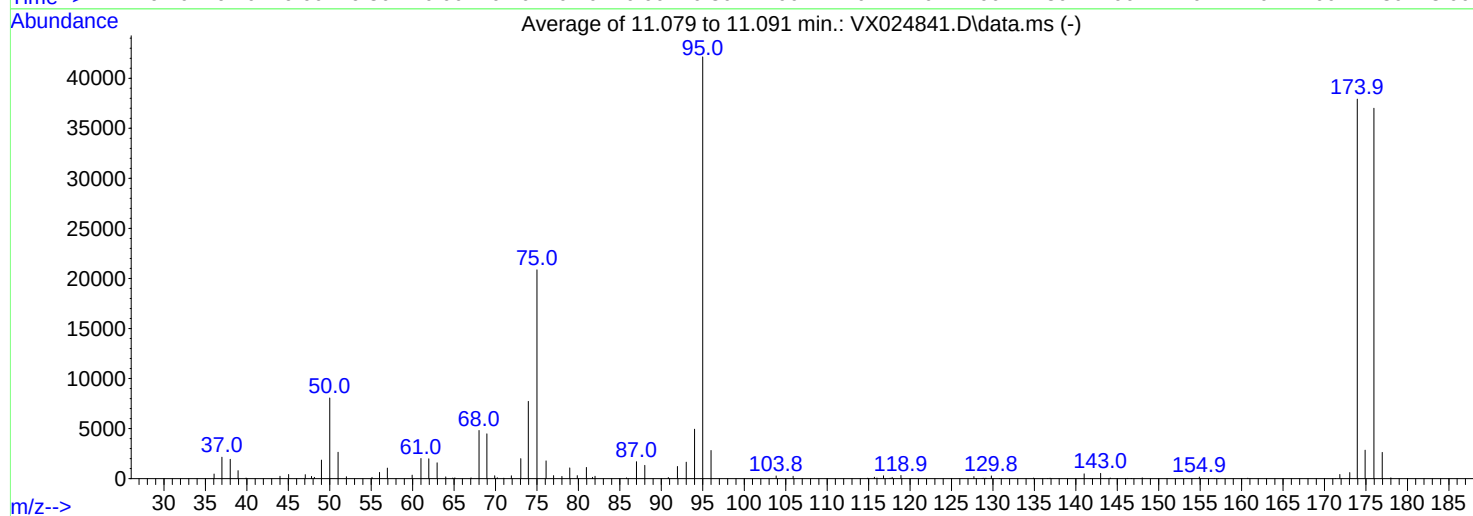


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101921\
 Data File : VX024841.D
 Acq On : 19 Oct 2021 10:48
 Operator : JC/MD
 Sample : BFB605
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB605

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM100721WMA.M
 Title : VOC Analysis
 Last Update : Wed Oct 20 14:52:57 2021

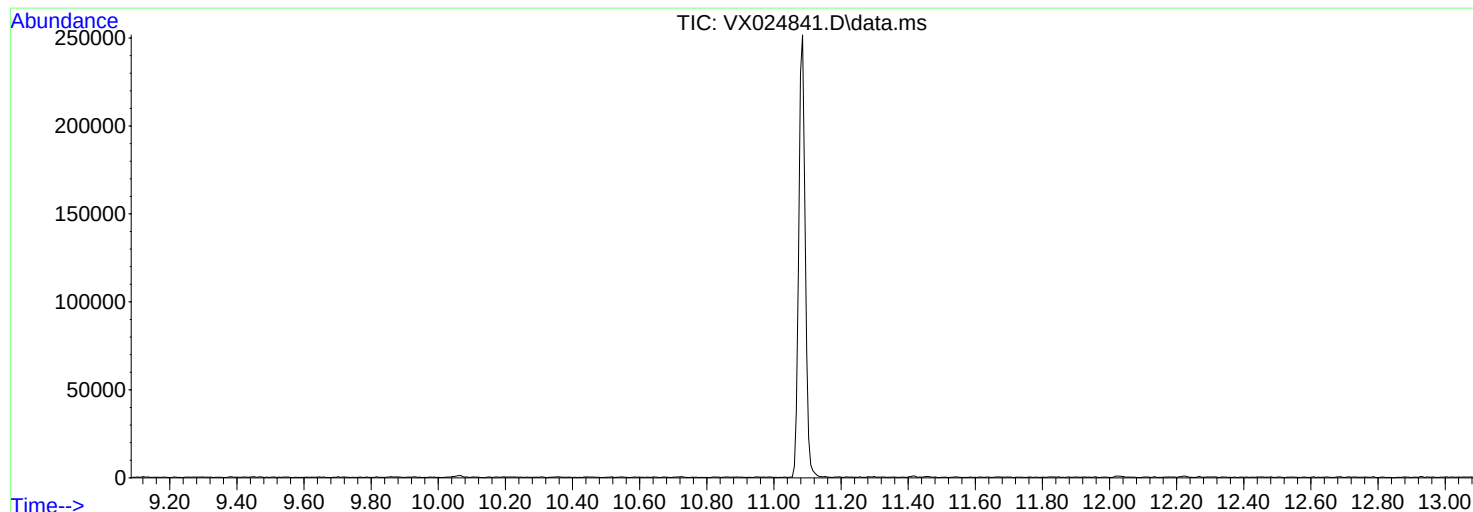

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1634

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	8063	PASS
75	95	30	80	49.5	20859	PASS
95	95	100	100	100.0	42139	PASS
96	95	5	9	6.7	2806	PASS
173	174	0.00	2	1.6	606	PASS
174	95	50	120	90.0	37925	PASS
175	174	5	9	7.5	2846	PASS
176	174	95	101	97.6	37013	PASS
177	176	5	9	7.1	2619	PASS

m/z	Abundance
38.80	69.0
39.80	114.0
41.20	51.0
44.00	76.0
46.40	56.0
73.90	54.0
88.10	52.0

Instrument :
MSVOA_X
ClientSampleId :
BFB605

m/z	Abundance
36.10	584.0
37.00	2364.0
38.00	2122.0
39.10	873.0
40.10	248.0
43.90	418.0
45.00	596.0
47.10	518.0
47.80	317.0
49.00	2267.0
50.00	9946.0
51.00	3078.0
52.00	245.0
55.10	201.0
56.00	855.0
57.00	1080.0
60.00	352.0
61.00	2228.0
62.00	2423.0
63.00	2103.0
64.00	309.0
64.80	124.0
67.10	68.0
68.00	5767.0
68.90	4986.0
69.90	474.0
72.00	373.0
73.10	2049.0
74.00	9027.0
75.00	22944.0
76.20	1797.0
77.00	306.0
78.00	214.0
79.00	1346.0
79.90	460.0
81.00	1275.0
81.70	405.0
85.80	171.0
87.00	1920.0
88.00	1547.0
90.80	170.0
91.90	1629.0
93.00	1890.0
94.00	5843.0
95.00	46088.0
96.00	3488.0
103.90	356.0
105.90	286.0
115.70	188.0
116.80	305.0
117.90	170.0
118.90	456.0
127.80	305.0
128.70	89.0
129.20	59.0
129.90	379.0
134.90	219.0
136.90	137.0
141.00	520.0
143.00	577.0
146.20	67.0
146.70	58.0
148.00	105.0
154.90	98.0
156.70	52.0
157.20	51.0
171.30	76.0
172.00	251.0
173.00	567.0
173.90	35888.0
174.90	2727.0
175.90	35752.0
176.90	2297.0
178.00	108.0

Instrument :
MSVOA_X
ClientSampleId :
BFB605

m/z	Abundance
36.00	581.0
37.00	2652.0
38.00	2182.0
39.00	1054.0
39.90	130.0
44.00	332.0
45.10	466.0
47.00	507.0
47.80	198.0
48.20	195.0
49.00	2077.0
50.00	8956.0
51.00	3111.0
51.90	204.0
55.10	171.0
56.00	724.0
56.90	1259.0
59.90	423.0
61.00	2501.0
61.90	2370.0
62.90	1592.0
64.10	110.0
65.10	229.0
67.00	198.0
68.00	5435.0
69.00	5351.0
69.90	380.0
71.80	316.0
73.00	2411.0
74.00	9079.0
75.00	23104.0
76.10	2170.0
77.10	394.0
77.90	128.0
78.90	1102.0
79.80	332.0
80.90	1188.0
82.10	313.0
85.80	61.0
87.00	2160.0
88.00	1873.0
90.90	126.0
92.00	1203.0
93.00	2080.0
94.00	5497.0
95.00	49792.0
96.00	2896.0
103.80	232.0
105.90	285.0
114.90	57.0
115.70	246.0
116.80	401.0
117.80	195.0
119.00	262.0
127.70	234.0
129.10	103.0
129.70	291.0
130.80	56.0
136.60	73.0
140.90	566.0
141.80	51.0
143.00	649.0
144.10	71.0
146.30	52.0
148.00	127.0
154.90	274.0
160.70	98.0
171.80	635.0
173.10	704.0
174.00	45608.0
174.90	3317.0
176.00	44184.0
177.00	3237.0
178.00	72.0

Instrument :
MSVOA_X
ClientSampleId :
BFB605

m/z	Abundance
35.90	232.0
37.00	1430.0
38.00	1488.0
38.90	695.0
39.90	165.0
44.10	200.0
45.00	184.0
47.00	199.0
47.70	151.0
48.10	200.0
49.00	1229.0
50.00	5287.0
51.00	1707.0
52.10	133.0
55.90	312.0
56.90	815.0
60.00	297.0
60.90	1322.0
61.90	1162.0
62.90	1071.0
63.90	117.0
64.90	92.0
68.00	3252.0
69.00	3090.0
70.20	300.0
71.00	129.0
71.90	175.0
73.10	1529.0
74.00	5218.0
75.00	16528.0
76.00	1346.0
76.90	205.0
78.00	354.0
78.90	753.0
80.00	132.0
80.90	906.0
81.90	390.0
87.00	1020.0
88.10	709.0
90.90	68.0
92.00	820.0
93.00	951.0
94.00	3476.0
95.00	30536.0
96.00	2033.0
103.90	223.0
106.00	151.0
114.90	90.0
116.00	178.0
116.80	163.0
117.60	133.0
118.80	234.0
127.60	113.0
128.90	151.0
129.80	133.0
141.10	382.0
142.90	373.0
144.20	106.0
155.00	105.0
160.80	62.0
171.90	347.0
173.00	547.0
173.90	32280.0
174.90	2493.0
175.90	31104.0
176.90	2323.0
178.00	67.0

Instrument :
MSVOA_X
ClientSampleId :
BFB605