

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101922\
 Data File : VX032218.D
 Acq On : 19 Oct 2022 19:18
 Operator : JC/MD
 Sample : N5170-05 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TRE-1663

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
 Title : SW846 8260

Signal : TIC: VX032218.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.453	56	60	66	rVB	14684	16403	2.18%	0.375%
2	2.105	155	167	182	rBV3	20754	80285	10.69%	1.836%
3	2.380	205	212	222	rVB	6245	11486	1.53%	0.263%
4	2.940	297	304	319	rVB2	5097	12024	1.60%	0.275%
5	3.111	324	332	342	rVB2	21264	50638	6.75%	1.158%
6	4.562	560	570	583	rBV3	3209	11506	1.53%	0.263%
7	5.385	694	705	721	rBV	89624	261036	34.77%	5.970%
8	5.556	721	733	748	rVB	147678	415410	55.33%	9.500%
9	5.958	788	799	818	rBV	100654	263152	35.05%	6.018%
10	6.763	921	931	943	rBV	220462	519334	69.18%	11.877%
11	8.647	1234	1240	1249	rBV	473900	750720	100.00%	17.169%
12	10.055	1465	1471	1481	rBV	457846	605860	80.70%	13.856%
13	10.299	1504	1511	1518	rBV	11279	15530	2.07%	0.355%
14	10.640	1563	1567	1573	rVB	7090	8935	1.19%	0.204%
15	11.079	1634	1639	1650	rBV	400634	521984	69.53%	11.938%
16	11.378	1684	1688	1692	rBV2	7304	11787	1.57%	0.270%
17	11.750	1745	1749	1757	rVB	18464	24031	3.20%	0.550%
18	12.024	1788	1794	1800	rBV	462048	587993	78.32%	13.447%
19	12.097	1800	1806	1815	rVB2	12219	24523	3.27%	0.561%
20	12.219	1822	1826	1828	rBV2	10931	15641	2.08%	0.358%
21	12.244	1828	1830	1838	rVV3	12242	19836	2.64%	0.454%
22	12.317	1838	1842	1848	rVB5	4704	8958	1.19%	0.205%
23	13.170	1978	1982	1986	rVB2	6265	8496	1.13%	0.194%
24	13.268	1993	1998	1999	rBV2	6451	7913	1.05%	0.181%
25	13.292	1999	2002	2006	rVB3	13786	18127	2.41%	0.415%
26	13.420	2019	2023	2028	rBV	12519	17058	2.27%	0.390%
27	13.774	2078	2081	2088	rVB	5185	7637	1.02%	0.175%
28	14.036	2120	2124	2127	rBV2	7178	7555	1.01%	0.173%
29	14.231	2147	2156	2161	rBV3	9661	17987	2.40%	0.411%
30	14.481	2192	2197	2207	rVB5	6796	11272	1.50%	0.258%
31	14.615	2215	2219	2221	rBV5	6150	8466	1.13%	0.194%
32	15.182	2307	2312	2315	rBV4	6449	10753	1.43%	0.246%
33	15.487	2355	2362	2368	rBV4	7177	12107	1.61%	0.277%
34	16.377	2502	2508	2515	rVB5	4076	8127	1.08%	0.186%

Sum of corrected areas: 4372570


Instrument :
MSVOA_X
ClientSampleId :
TRE-1663

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101922\
Data File : VX032218.D
Acq On : 19 Oct 2022 19:18
Operator : JC/MD
Sample : N5170-05 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRE-1663

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

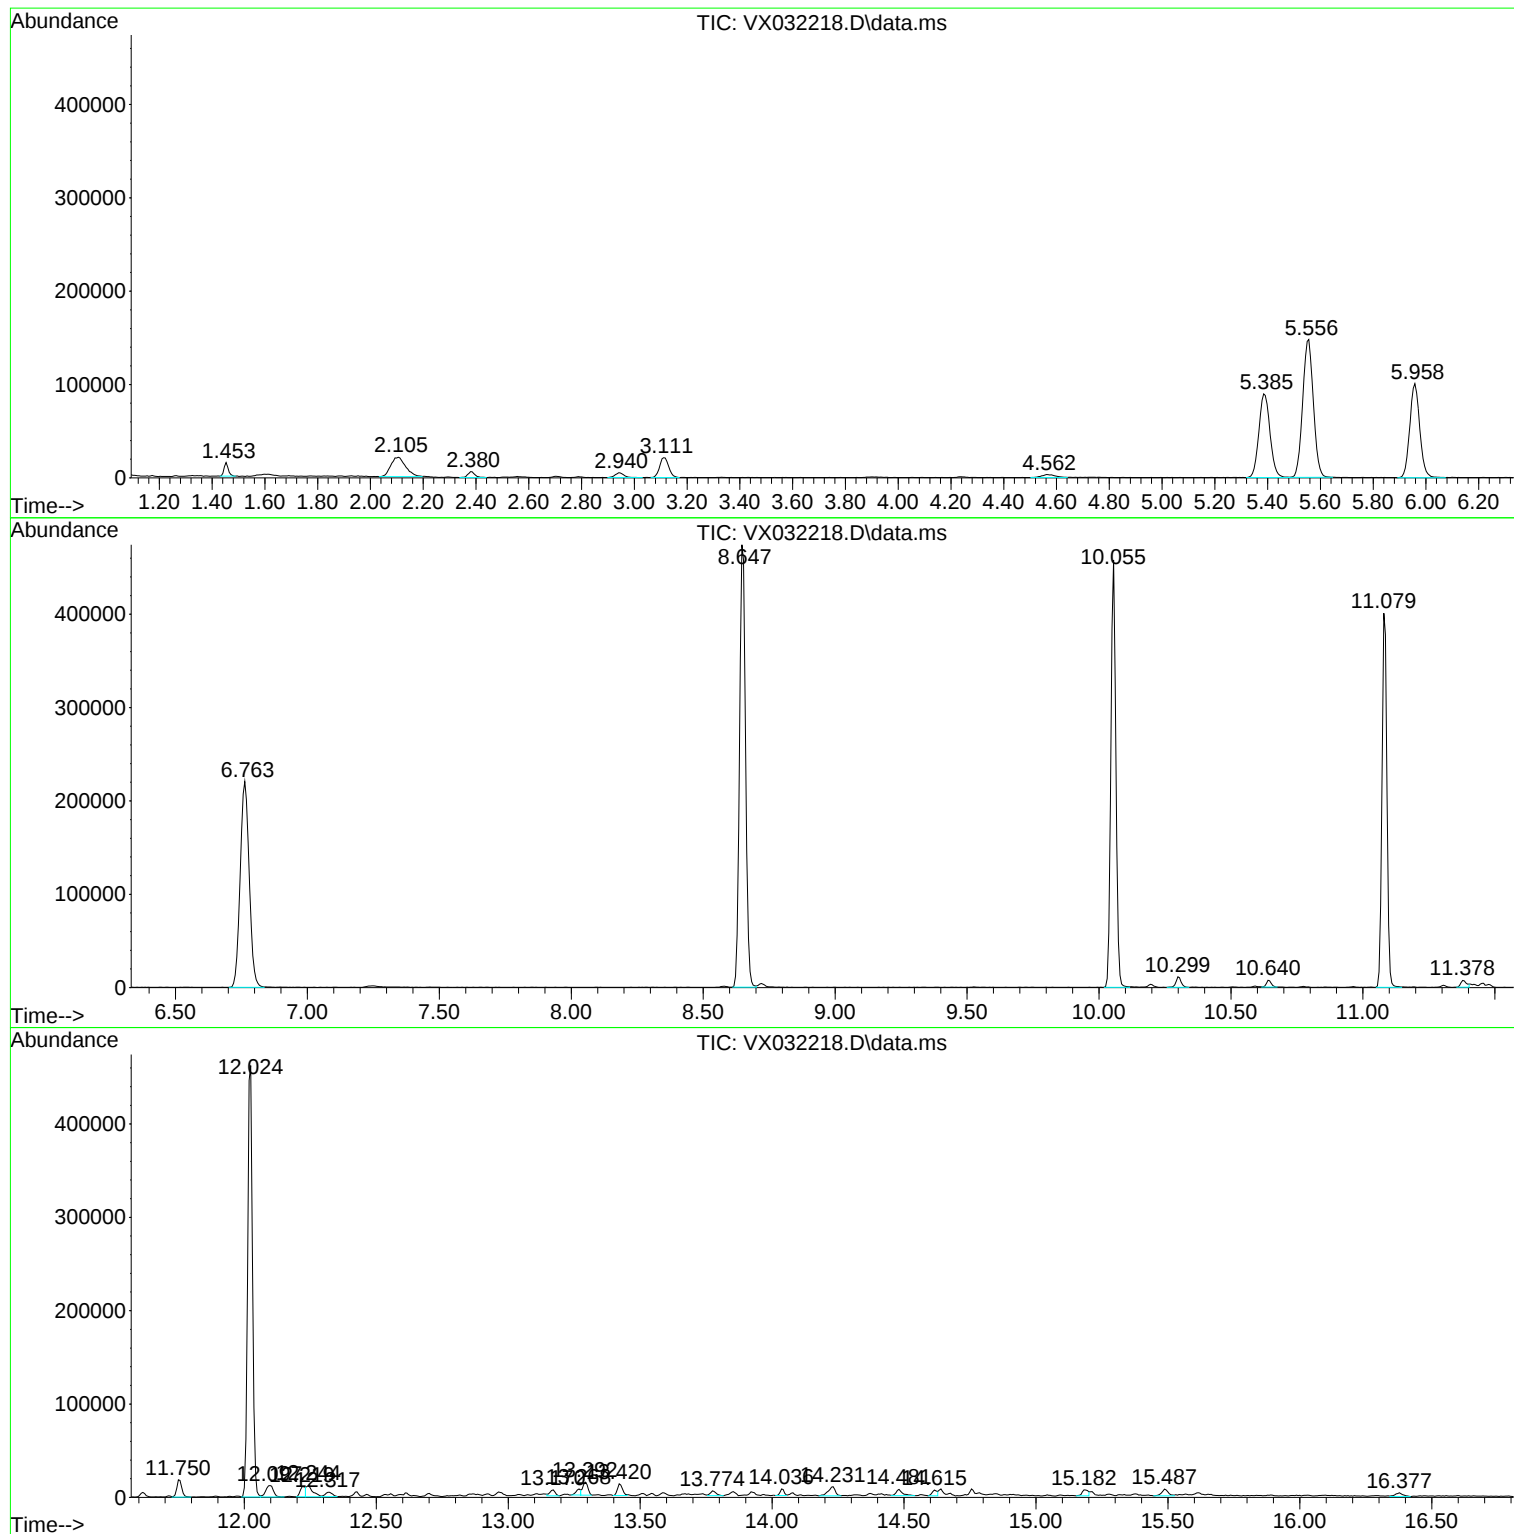

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101922\
Data File : VX032218.D
Acq On : 19 Oct 2022 19:18
Operator : JC/MD
Sample : N5170-05 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRE-1663










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.105	9.66 ug/l	80285	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol	46	C2H6O	000064-17-5	78
2			Dimethyl ether	46	C2H6O	000115-10-6	9
3			Methane, nitroso-	45	CH3NO	000865-40-7	4
4			3-Nitropropanoic acid	119	C3H5NO4	000504-88-1	4
5			Formic acid	46	CH2O2	000064-18-6	4

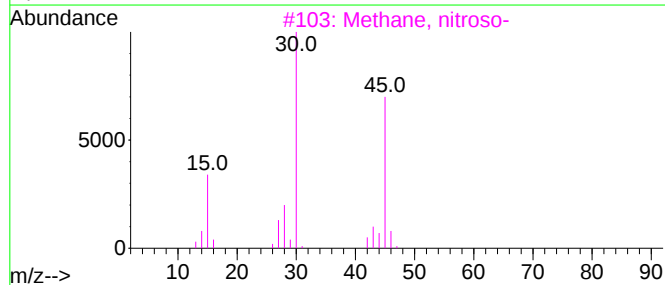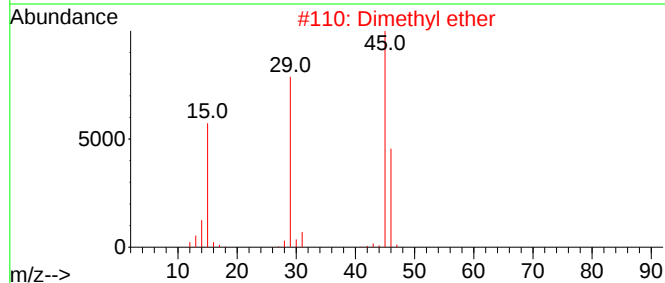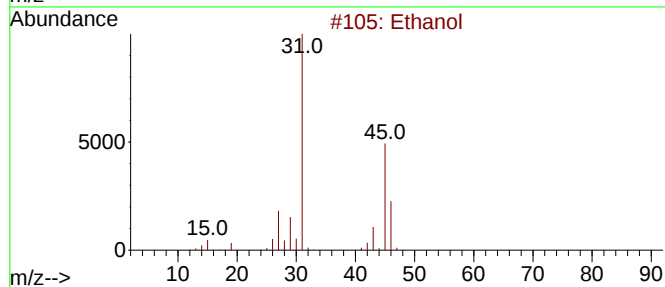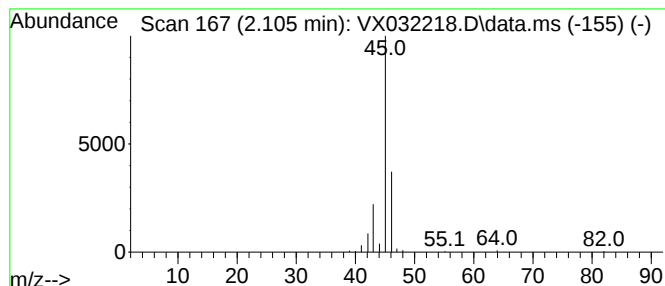

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101922\
Data File : VX032218.D
Acq On : 19 Oct 2022 19:18
Operator : JC/MD
Sample : N5170-05 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRE-1663

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol	2.105	9.7	ug/l	80285	1	5.556	415410	50.0