

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101922\
 Data File : VX032221.D
 Acq On : 19 Oct 2022 20:28
 Operator : JC/MD
 Sample : N5170-08 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TRE-1666

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
 Title : SW846 8260

Signal : TIC: VX032221.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.453	56	60	68	rVB	16078	18055	2.42%	0.390%
2	2.117	155	169	182	rBV3	20149	85853	11.52%	1.856%
3	2.386	206	213	221	rBV	6204	11115	1.49%	0.240%
4	2.940	297	304	315	rVB	5500	12565	1.69%	0.272%
5	3.111	321	332	343	rBV	65899	151045	20.27%	3.265%
6	4.568	560	571	580	rBV	4026	14119	1.89%	0.305%
7	5.385	691	705	721	rBV2	88251	259594	34.83%	5.612%
8	5.556	721	733	747	rVB	149116	418709	56.18%	9.052%
9	5.958	789	799	812	rBV	100184	264253	35.45%	5.713%
10	6.763	922	931	943	rBV	221622	523621	70.25%	11.320%
11	8.647	1234	1240	1248	rBV	476816	745332	100.00%	16.113%
12	8.720	1248	1252	1262	rVB	6599	11393	1.53%	0.246%
13	10.055	1465	1471	1481	rBV	464208	607351	81.49%	13.130%
14	10.195	1488	1494	1499	rVB	5609	7507	1.01%	0.162%
15	10.299	1505	1511	1519	rBV	19213	27525	3.69%	0.595%
16	10.640	1563	1567	1572	rBV	12970	16548	2.22%	0.358%
17	11.079	1634	1639	1653	rVB	409542	514196	68.99%	11.116%
18	11.378	1682	1688	1697	rBV	12852	25947	3.48%	0.561%
19	11.616	1721	1727	1733	rBV	7387	10622	1.43%	0.230%
20	11.750	1745	1749	1757	rVB	27594	35133	4.71%	0.760%
21	12.024	1788	1794	1800	rBV	470137	591307	79.33%	12.783%
22	12.091	1800	1805	1812	rVB2	13940	25654	3.44%	0.555%
23	12.244	1827	1830	1833	rVB	10510	12052	1.62%	0.261%
24	12.317	1838	1842	1849	rVB4	6384	10902	1.46%	0.236%
25	12.420	1851	1859	1863	rBV	7630	9998	1.34%	0.216%
26	12.695	1899	1904	1909	rBV	5015	7931	1.06%	0.171%
27	12.963	1944	1948	1955	rVB3	6676	11048	1.48%	0.239%
28	13.170	1978	1982	1986	rVB2	7428	9831	1.32%	0.213%
29	13.268	1993	1998	1999	rBV2	10160	11277	1.51%	0.244%
30	13.292	1999	2002	2007	rVB3	18672	23205	3.11%	0.502%
31	13.420	2019	2023	2032	rVB	15799	22649	3.04%	0.490%
32	13.664	2055	2063	2069	rBV3	2783	7883	1.06%	0.170%
33	13.774	2077	2081	2088	rVB2	5818	8884	1.19%	0.192%
34	13.847	2088	2093	2098	rVV7	5600	9909	1.33%	0.214%
35	13.926	2100	2106	2111	rVB5	4883	8713	1.17%	0.188%
36	14.036	2117	2124	2128	rBV	11003	13075	1.75%	0.283%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101922\
Data File : VX032221.D
Acq On : 19 Oct 2022 20:28
Operator : JC/MD
Sample : N5170-08 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRE-1666

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Title : SW846 8260

37	14.231	2147	2156	2163	rVB	11895	21362	2.87%	0.462%
38	14.481	2191	2197	2207	rVB7	8111	13569	1.82%	0.293%
39	14.615	2215	2219	2221	rBV2	8072	10635	1.43%	0.230%
40	14.755	2238	2242	2245	rBV	10059	11207	1.50%	0.242%
41	15.182	2308	2312	2315	rBV4	6096	9377	1.26%	0.203%
42	15.493	2357	2363	2367	rBV3	9151	14721	1.98%	0.318%




Sum of corrected areas: 4625672

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101922\
Data File : VX032221.D
Acq On : 19 Oct 2022 20:28
Operator : JC/MD
Sample : N5170-08 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRE-1666

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

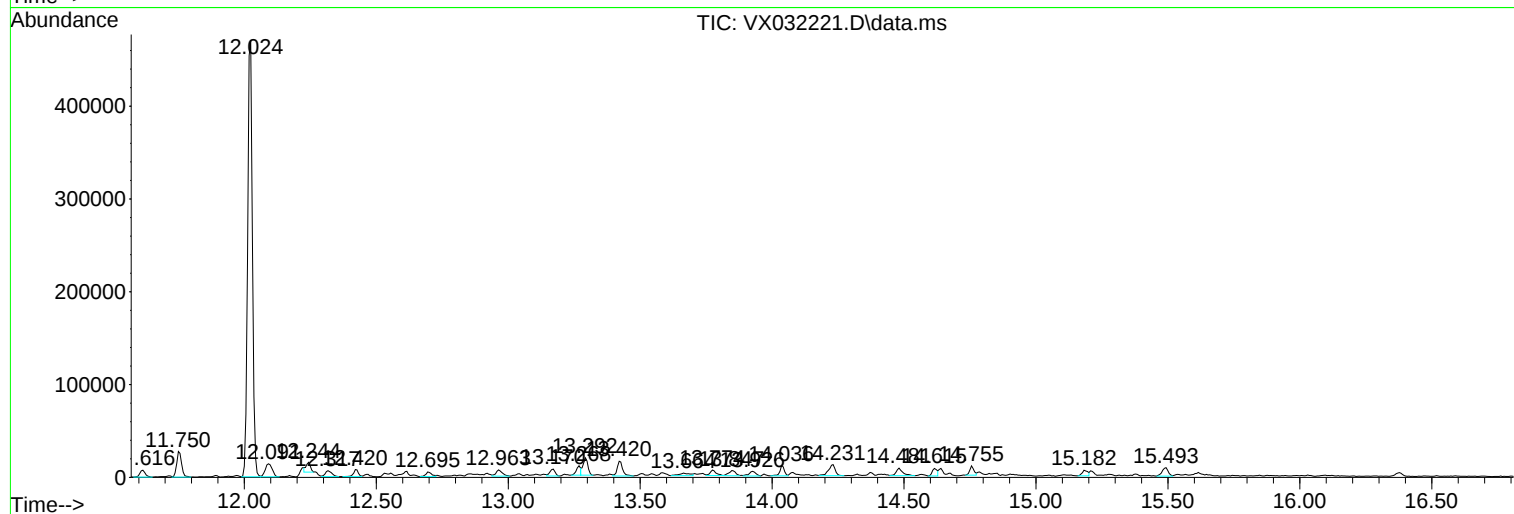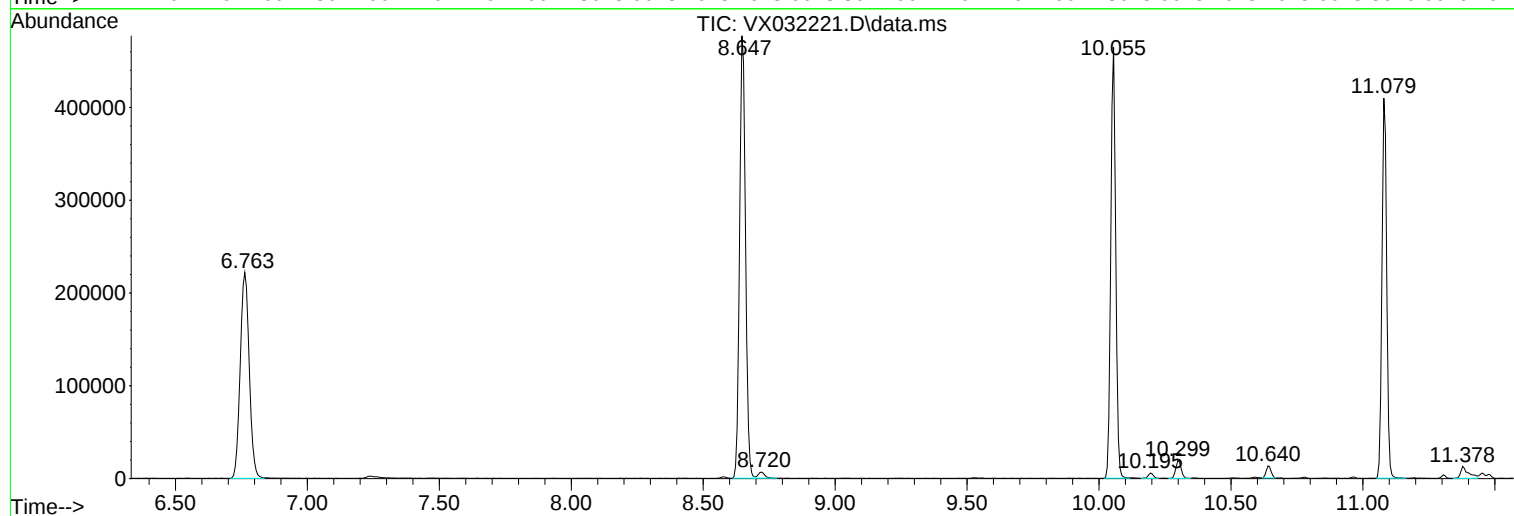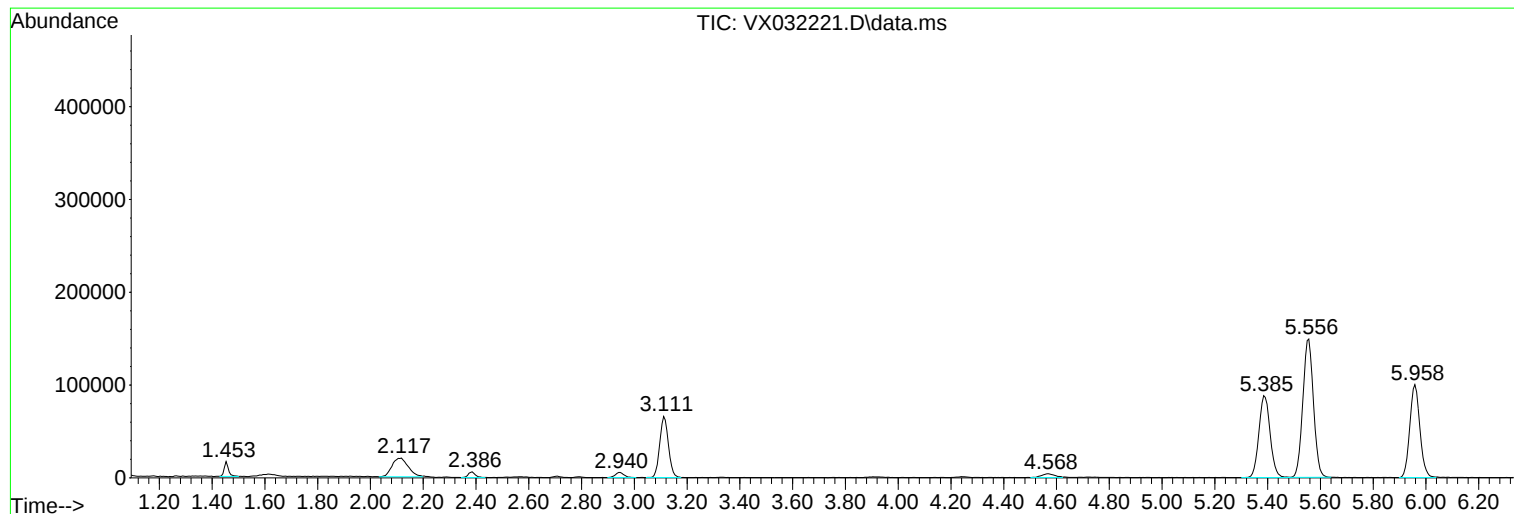

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101922\
Data File : VX032221.D
Acq On : 19 Oct 2022 20:28
Operator : JC/MD
Sample : N5170-08 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRE-1666










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.117	10.25 ug/l	85853	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol	46	C2H6O	000064-17-5	64
2			Dimethyl ether	46	C2H6O	000115-10-6	9
3			Formic acid	46	CH2O2	000064-18-6	4
4			Propanedioic acid, dihydroxy-	136	C3H4O6	000560-27-0	4
5			Methoxyacetyl chloride	108	C3H5ClO2	038870-89-2	4

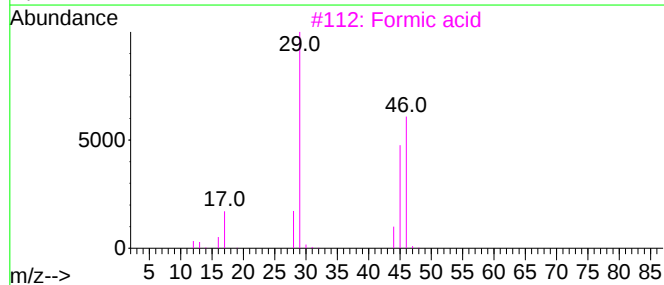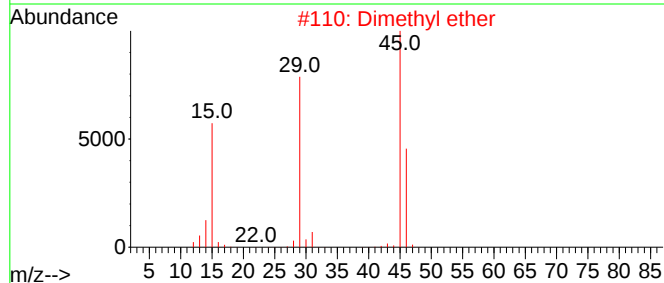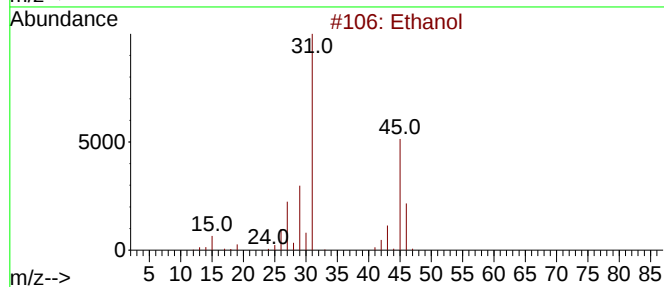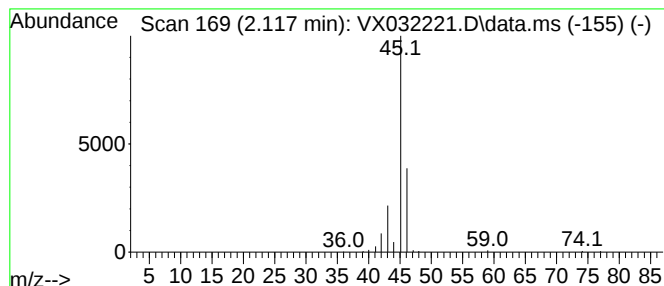

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101922\
Data File : VX032221.D
Acq On : 19 Oct 2022 20:28
Operator : JC/MD
Sample : N5170-08 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRE-1666

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol	2.117	10.3	ug/l	85853	1	5.556	418709	50.0