
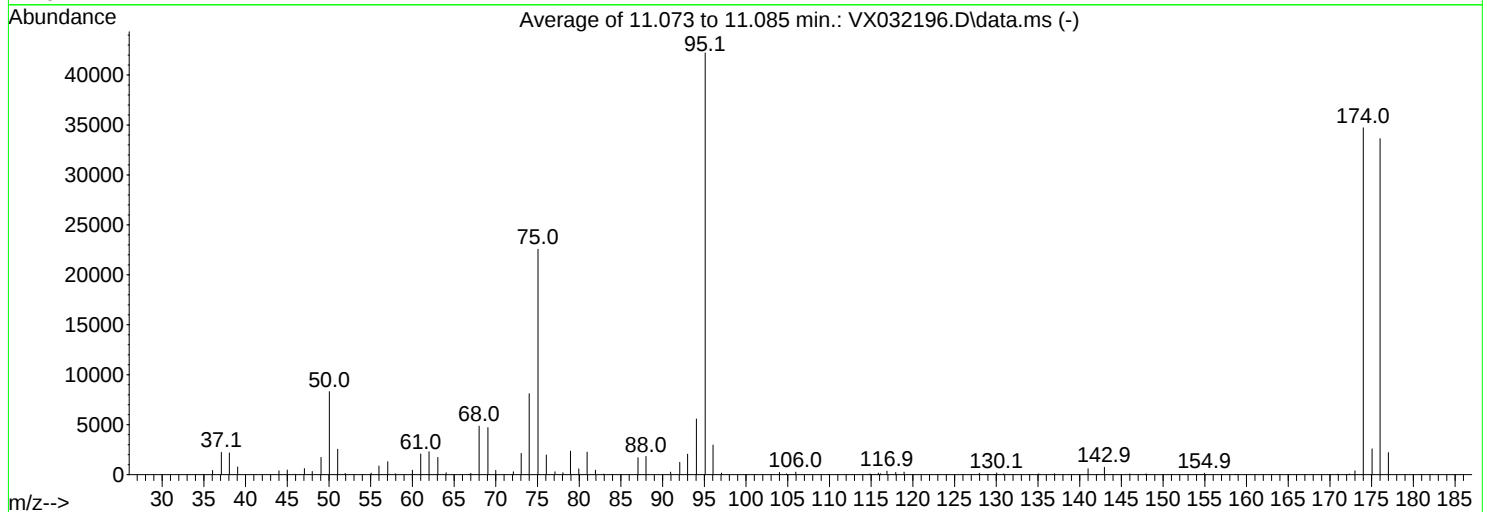


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101922\
Data File : VX032196.D
Acq On : 19 Oct 2022 09:32
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Title : SW846 8260
Last Update : Wed Oct 19 16:51:09 2022

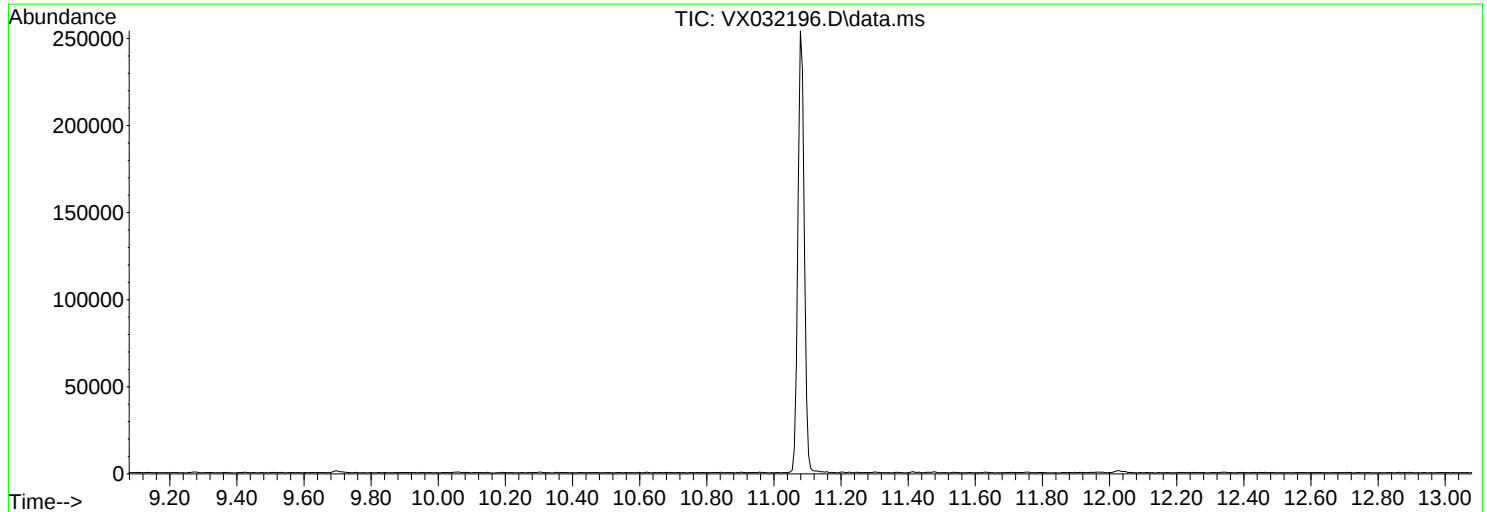

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	8315	PASS
75	95	30	60	53.5	22573	PASS
95	95	100	100	100.0	42219	PASS
96	95	5	9	7.0	2962	PASS
173	174	0.00	2	1.1	391	PASS
174	95	50	100	82.2	34720	PASS
175	174	5	9	7.4	2586	PASS
176	174	95	101	96.9	33632	PASS
177	176	5	9	6.6	2216	PASS