


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101922\
 Data File : VX032225.D
 Acq On : 19 Oct 2022 22:23
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
 Title : SW846 8260
 Last Update : Wed Oct 19 16:51:09 2022

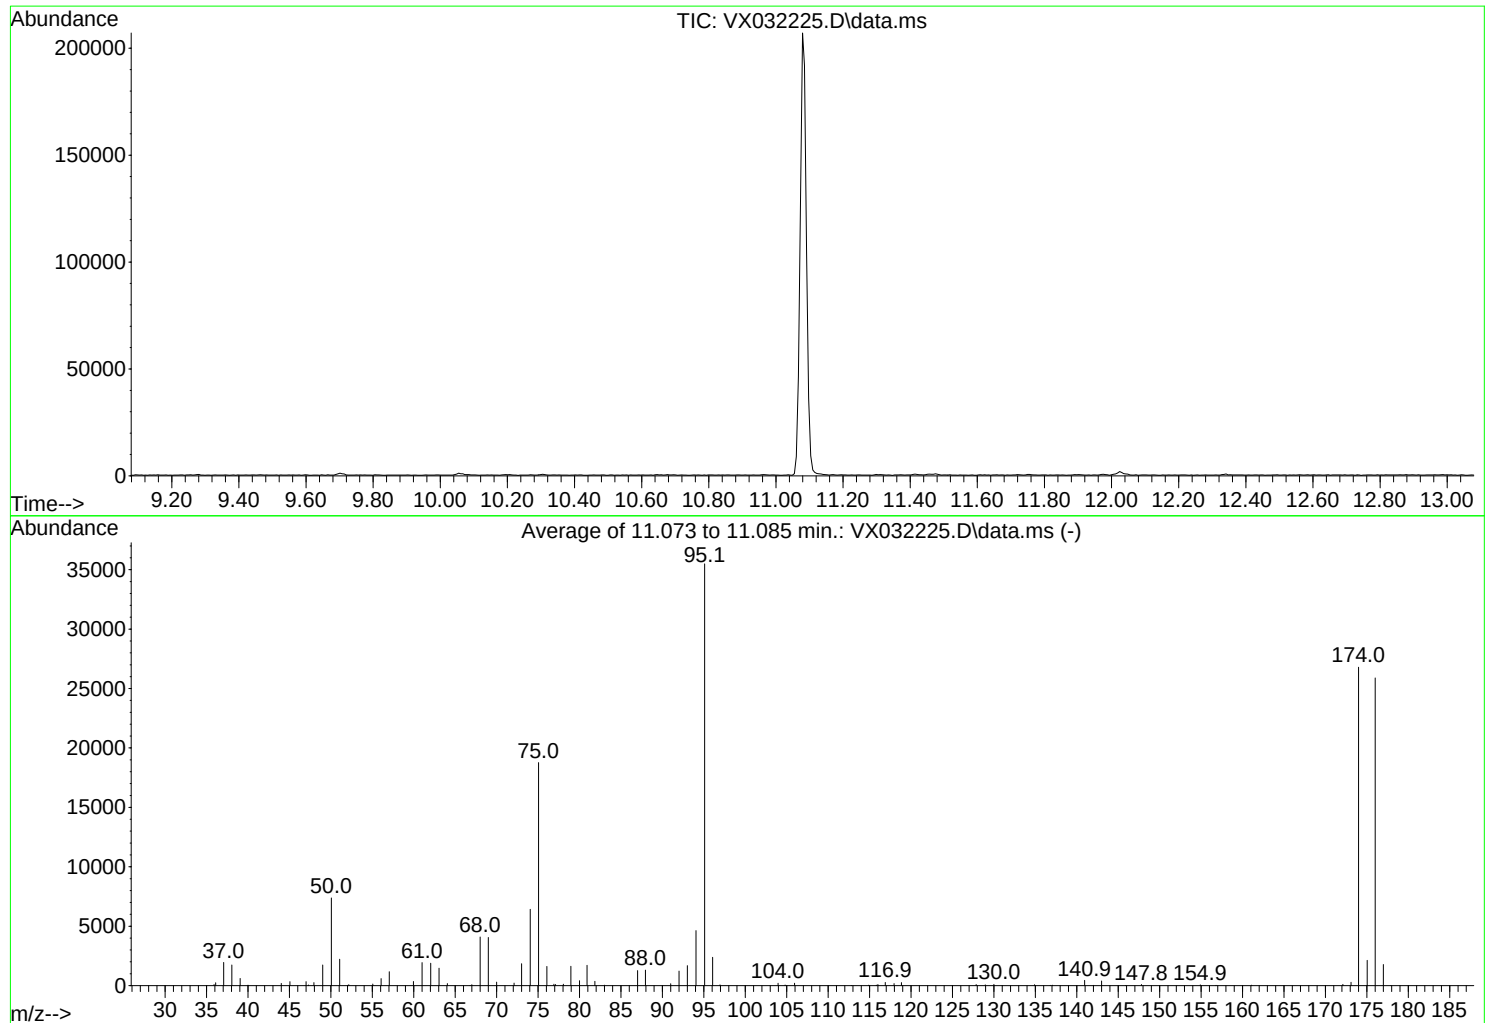

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	7380	PASS
75	95	30	60	52.9	18772	PASS
95	95	100	100	100.0	35491	PASS
96	95	5	9	6.7	2379	PASS
173	174	0.00	2	1.1	283	PASS
174	95	50	100	75.5	26797	PASS
175	174	5	9	7.9	2127	PASS
176	174	95	101	96.6	25889	PASS
177	176	5	9	6.9	1784	PASS