

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101923\
Data File : VX038380.D
Acq On : 19 Oct 2023 13:05
Operator : JC/MD
Sample : 04957-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-H

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038380.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.148	6	10	19	rVB	42447	53740	7.40%	1.333%
2	1.471	56	63	69	rBV	12353	16214	2.23%	0.402%
3	2.050	151	158	164	rBV2	4134	7696	1.06%	0.191%
4	2.532	230	237	243	rBV	5551	10461	1.44%	0.259%
5	5.013	637	644	654	rBV4	4039	12805	1.76%	0.318%
6	5.385	694	705	722	rBV3	78090	228349	31.43%	5.663%
7	5.556	722	733	746	rVV	123344	350982	48.31%	8.704%
8	5.958	787	799	815	rBV	89445	233365	32.12%	5.787%
9	6.763	922	931	951	rBV	203663	485770	66.86%	12.046%
10	8.646	1234	1240	1258	rBV	437428	699318	96.26%	17.342%
11	10.055	1465	1471	1486	rBV	502550	673819	92.75%	16.709%
12	11.079	1634	1639	1661	rBV	406947	533559	73.44%	13.231%
13	12.024	1788	1794	1804	rBV	563278	726524	100.00%	18.016%




Sum of corrected areas: 4032602

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101923\
Data File : VX038380.D
Acq On : 19 Oct 2023 13:05
Operator : JC/MD
Sample : 04957-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-H

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

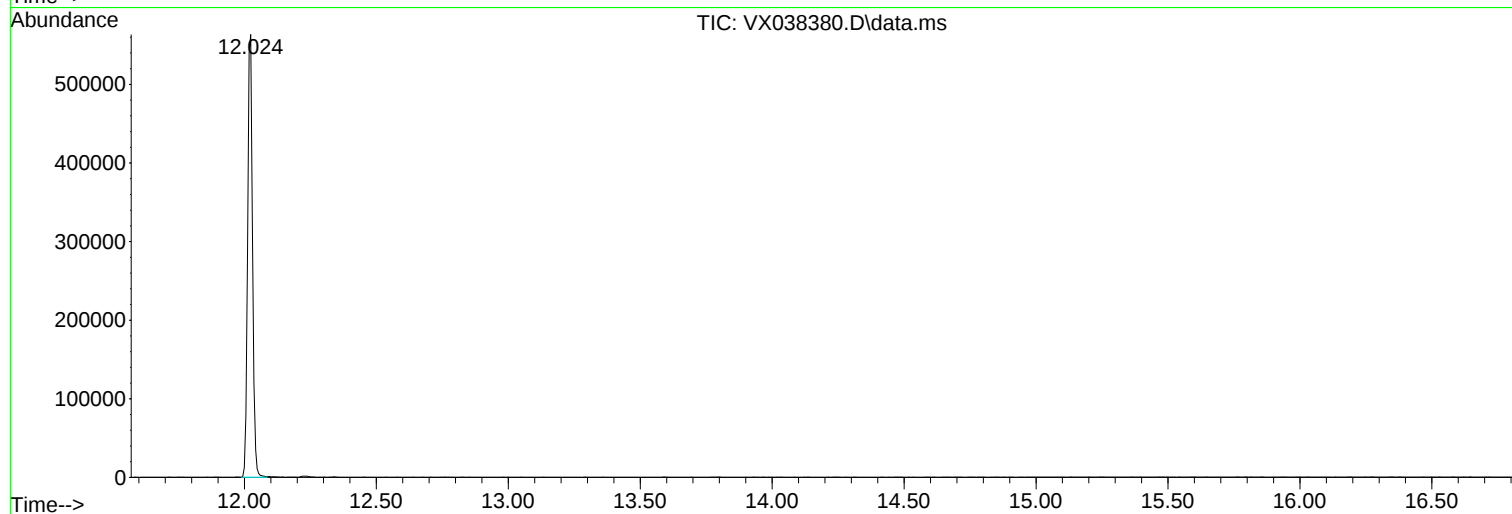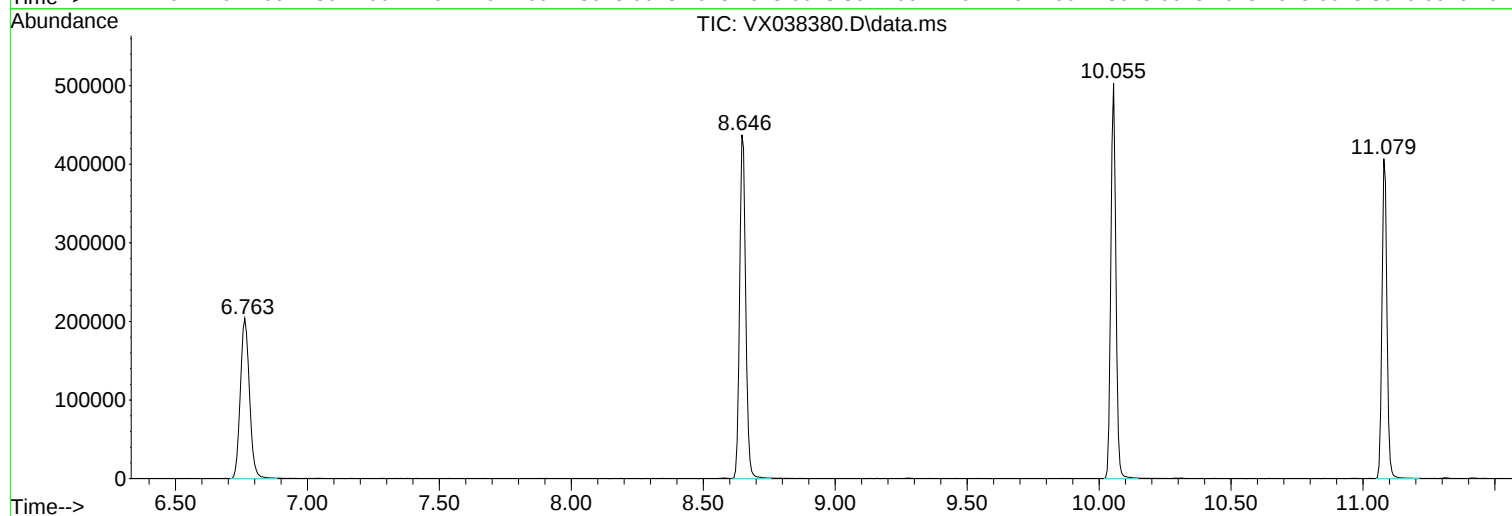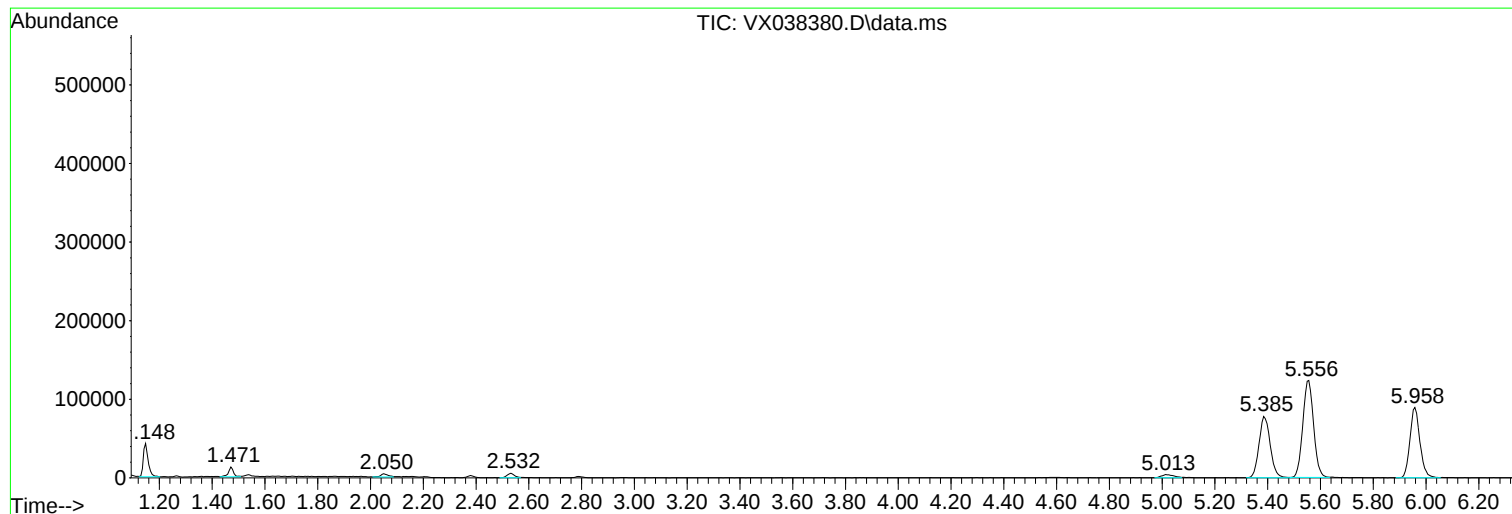

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101923\
Data File : VX038380.D
Acq On : 19 Oct 2023 13:05
Operator : JC/MD
Sample : 04957-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-H










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethane, 1,1-difluoro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.148	7.66 ug/l	53740	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 1,1-difluoro-	66	C2H4F2	000075-37-6	91
2			Propiolonitrile	51	C3HN	001070-71-9	3
3			Propane, 2,2-difluoro-	80	C3H6F2	000420-45-1	2
4			Difluoromethane	52	CH2F2	000075-10-5	1
5			2-Chloroethanol	80	C2H5ClO	000107-07-3	1

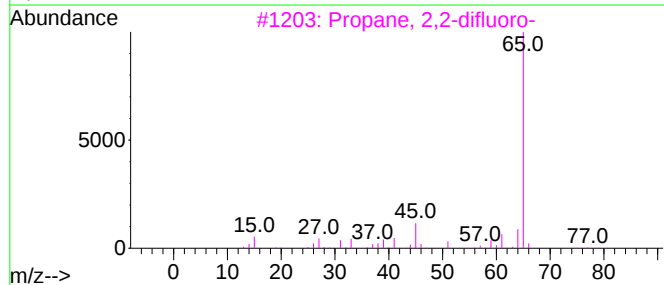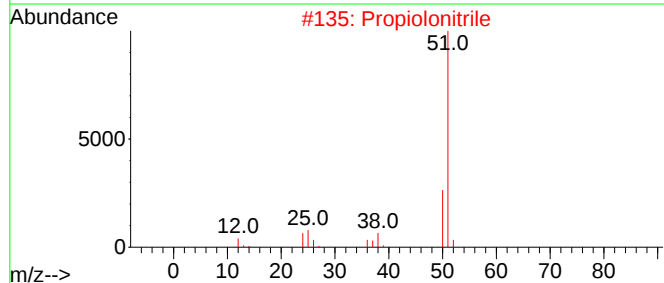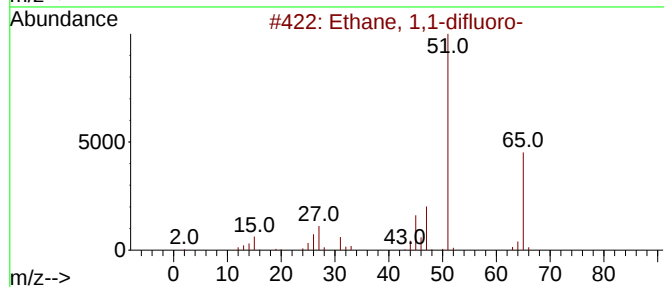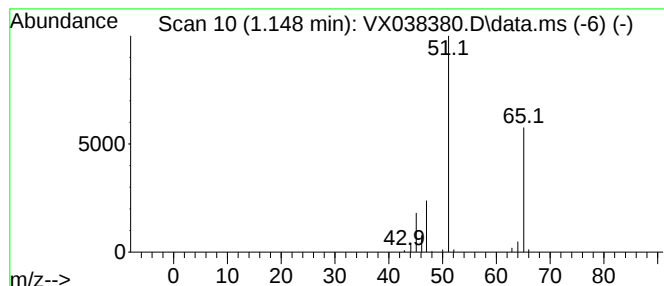

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101923\
Data File : VX038380.D
Acq On : 19 Oct 2023 13:05
Operator : JC/MD
Sample : 04957-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-H

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethane, 1,1-dif...	1.148	7.7	ug/l	53740	1	5.556	350982	50.0