



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX101923\
Data File : VX038369.D
Acq On : 19 Oct 2023 08:31
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Title : SW846 8260
Last Update : Thu Oct 05 15:27:13 2023

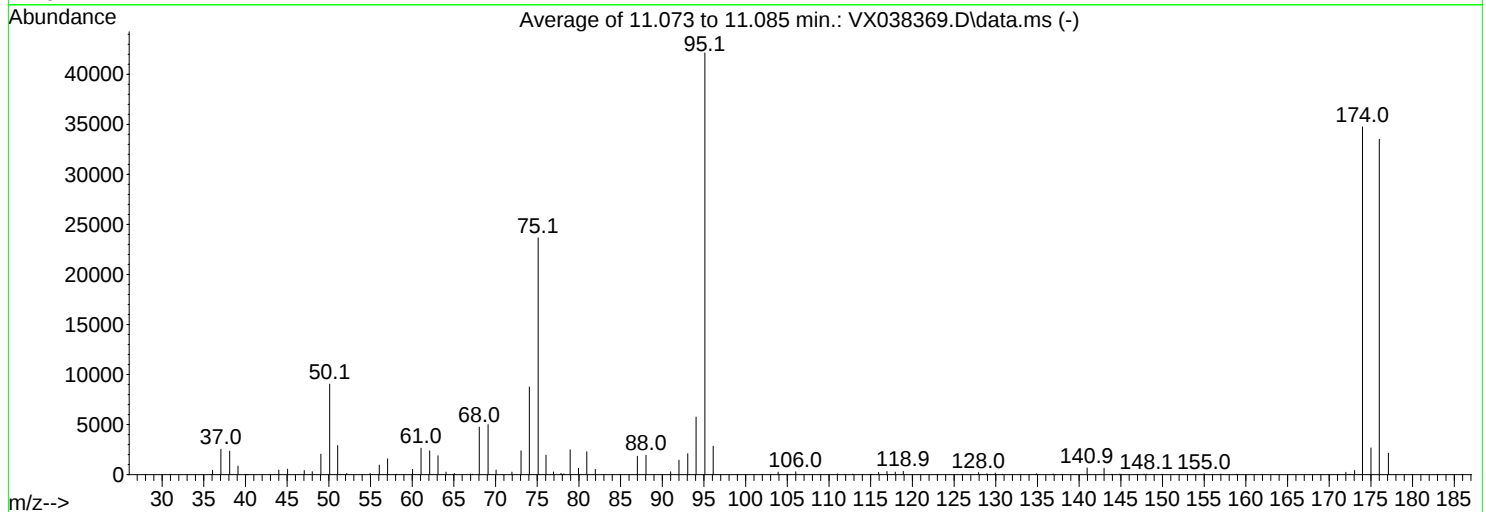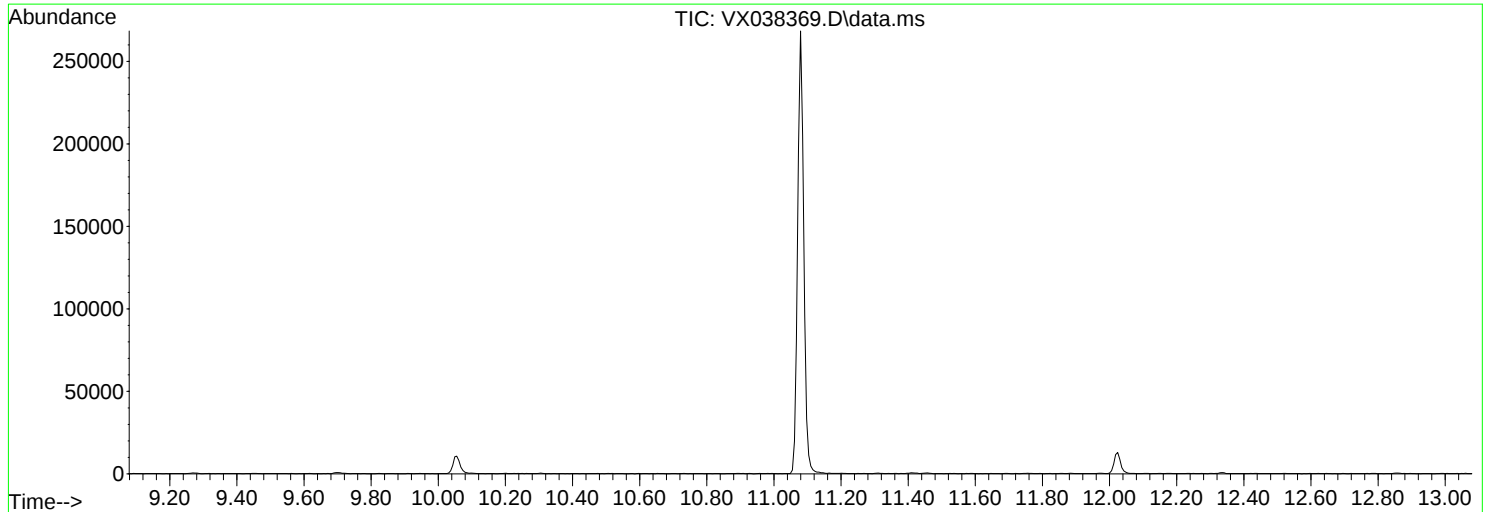

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	9051	PASS
75	95	30	60	56.2	23664	PASS
95	95	100	100	100.0	42144	PASS
96	95	5	9	6.8	2854	PASS
173	174	0.00	2	1.2	424	PASS
174	95	50	100	82.5	34755	PASS
175	174	5	9	7.7	2678	PASS
176	174	95	101	96.4	33501	PASS
177	176	5	9	6.4	2147	PASS