

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX102020\
 Data File : VX018995.D
 Acq On : 20 Oct 2020 23:47
 Operator : JC/SP
 Sample : L4457-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SUTTON-PR-2152-SED

Quant Time: Oct 21 03:29:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102020W.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 20 19:16:32 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	162004	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	301370	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	296187	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	145453	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.03	65	111953	52.57	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.14%	
35) Dibromofluoromethane	5.46	113	91401	47.99	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.98%	
50) Toluene-d8	8.70	98	391480	51.58	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.16%	
62) 4-Bromofluorobenzene	11.12	95	145182	48.97	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.94%	
Target Compounds						
					Qvalue	
5) Bromomethane	1.64	94	343	0.204	ug/l	99
11) Tert butyl alcohol	3.01	59	1703	3.487	ug/l	97
12) 1,1-Dichloroethene	2.31	96	95	Below Cal	#	1
13) Acrolein	2.29	56	277	Below Cal	#	15
16) Acetone	2.42	43	16456	22.193	ug/l	99
18) Methyl Acetate	2.75	43	1679	0.934	ug/l	90
20) Methylene Chloride	2.83	84	4427	2.310	ug/l	97
25) 2-Butanone	4.64	43	8196	6.842	ug/l	97
29) Tetrahydrofuran	5.10	42	1059	1.500	ug/l #	63
31) Cyclohexane	5.63	56	3549	1.426	ug/l #	1
36) 1,1-Dichloropropene	5.63	75	13789	4.896	ug/l #	48
37) Ethyl Acetate	4.64	43	8196	3.366	ug/l #	68
38) Carbon Tetrachloride	5.63	117	16268	5.740	ug/l #	17
43) Isopropyl Acetate	6.41	43	32119	7.829	ug/l	99
48) Methyl methacrylate	7.65	41	2850	1.407	ug/l #	15
49) 1,4-Dioxane	7.84	88	26	0.484	ug/l #	1
51) 4-Methyl-2-Pentanone	8.59	43	36282	14.322	ug/l #	46
54) cis-1,3-Dichloropropene	8.59	75	20036	5.682	ug/l #	60
57) 1,3-Dichloropropane	9.52	76	2555	0.711	ug/l #	44
59) 2-Hexanone	9.42	43	34658	17.617	ug/l #	17
60) Dibromochloromethane	9.32	129	1106	0.449	ug/l #	11
64) Tetrachloroethene	9.32	164	1111	0.532	ug/l	90
68) m/p-Xylenes	10.34	106	1157	0.271	ug/l	96
76) 1,2,3-Trichloropropane	11.12	75	73353	24.537	ug/l #	36
81) trans-1,4-Dichloro-2-buten	11.12	75	73353	64.723	ug/l #	16
95) Naphthalene	13.82	128	22828	2.118	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX102020\
Data File : VX018995.D
Acq On : 20 Oct 2020 23:47
Operator : JC/SP
Sample : L4457-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SUTTON-PR-2152-SED

Quant Time: Oct 21 03:29:43 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X102020W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 20 19:16:32 2020
Response via : Initial Calibration

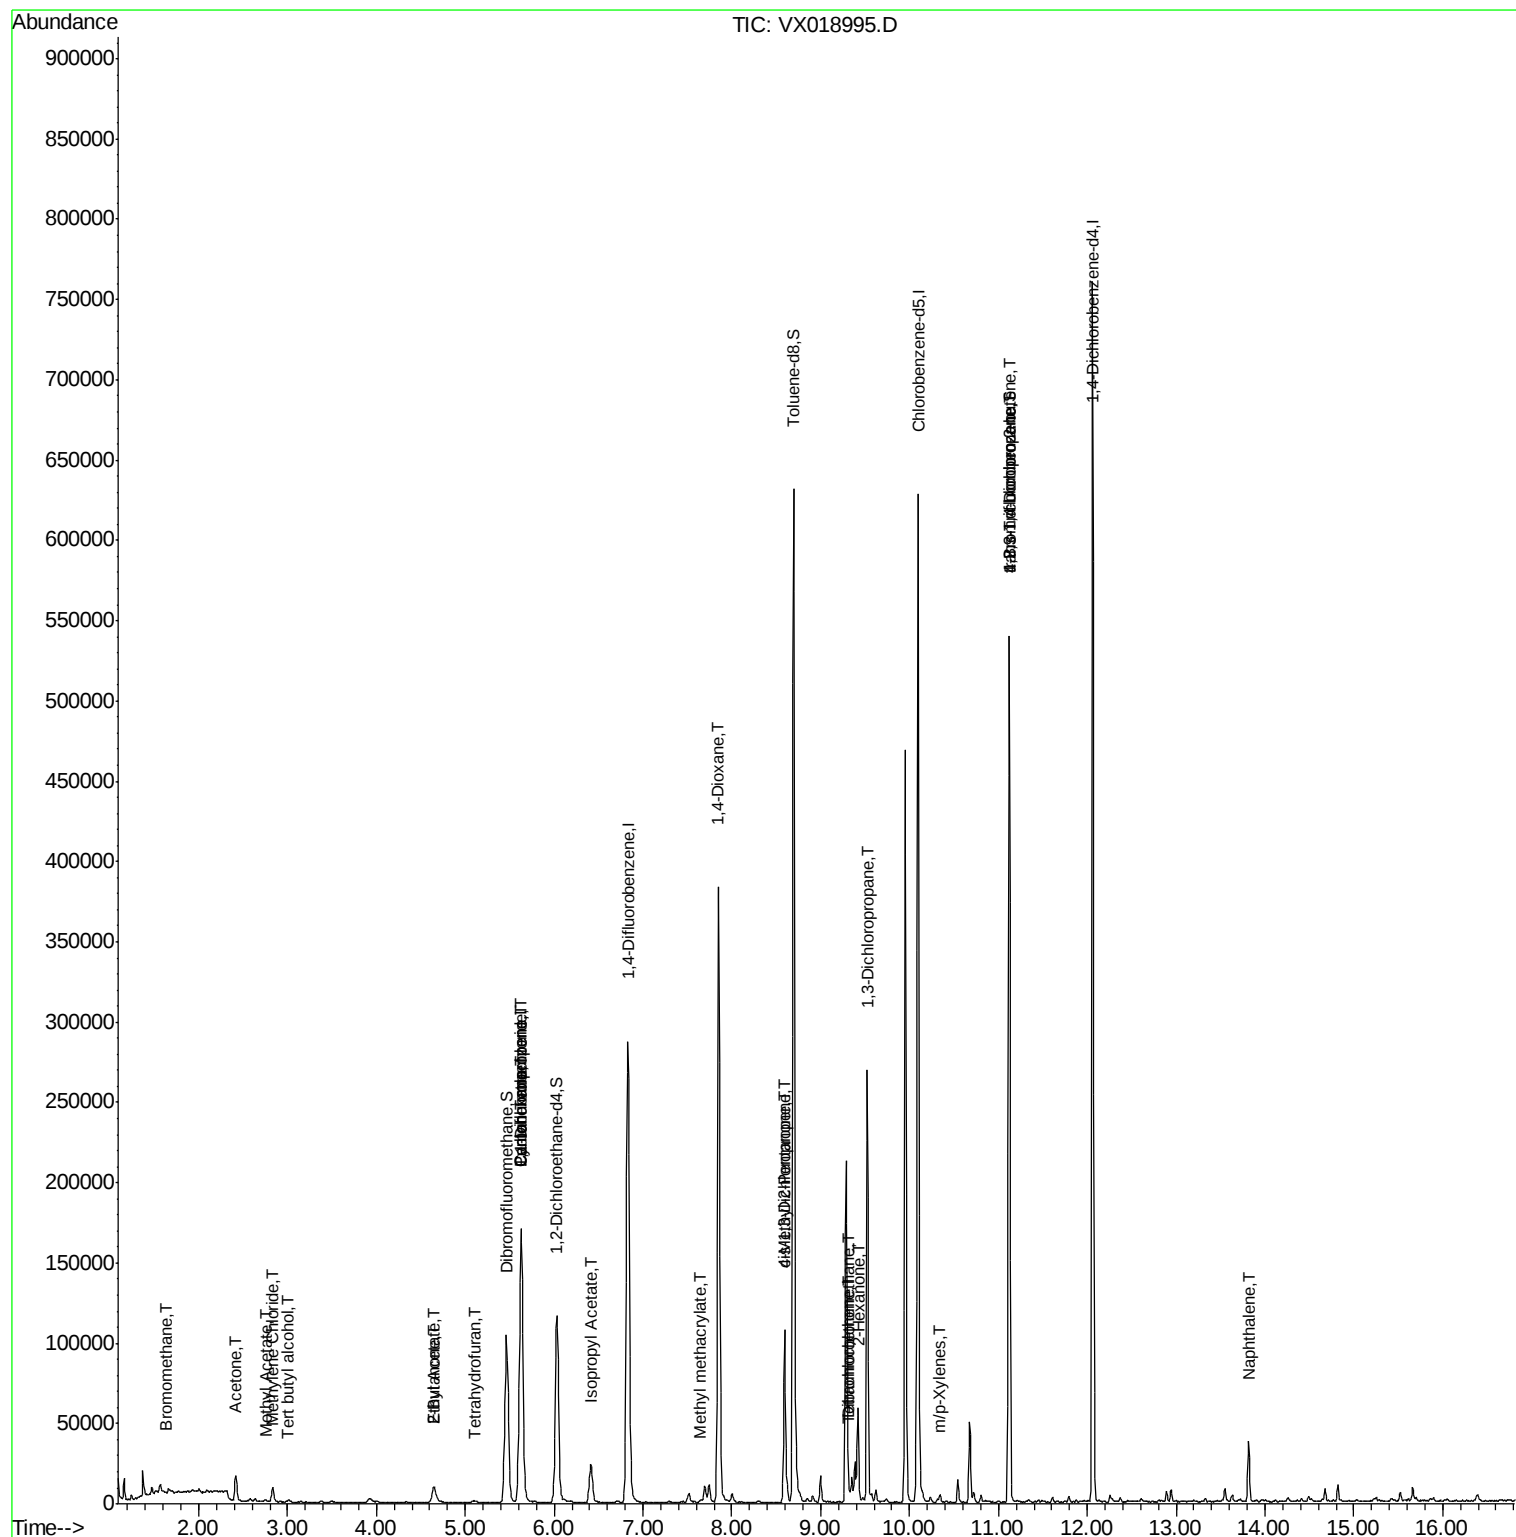

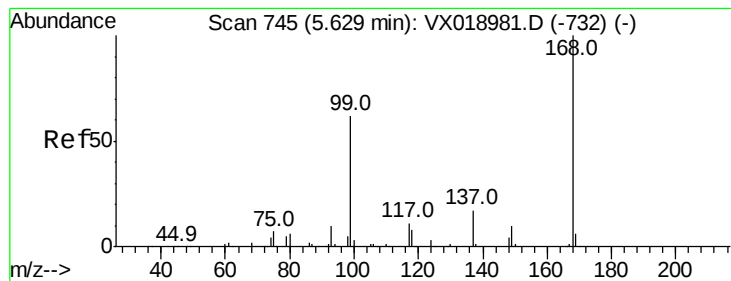

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.00 min

Lab File: VX018995.D

Acq: 20 Oct 2020 23:47

Instrument :

MSVOA_X

ClientSampleId :


SUTTON-PR-2152-SED

Tot Ion:168 Resp: 162004

Ion Ratio Lower Upper




168 100

99 57.8 49.7 74.5



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

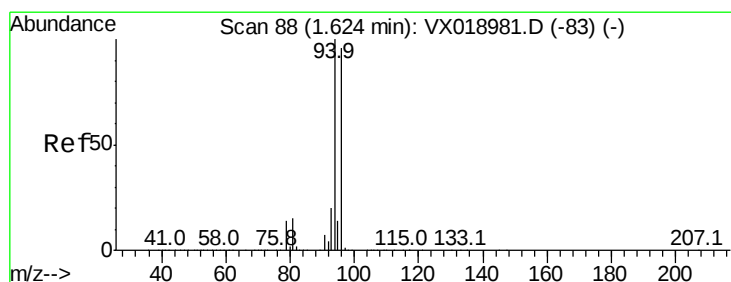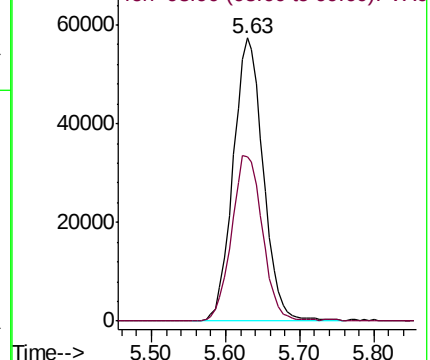

#5

Bromomethane

Concen: 0.204 ug/l

RT: 1.64 min Scan# 91

Delta R.T. 0.02 min

Lab File: VX018995.D


Acq: 20 Oct 2020 23:47

Tgt Ion: 94 Resp: 343

Ion Ratio Lower Upper



94 100


96 94.3 76.4 114.6



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

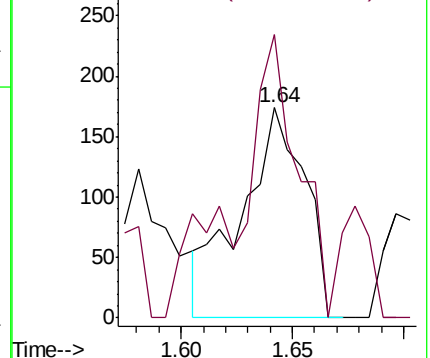







#11

Tert butyl alcohol
Concen: 3.487 ug/l
RT: 3.01 min Scan# 315
Delta R.T. -0.01 min
Lab File: VX018995.D
Acq: 20 Oct 2020 23:47

Instrument :
MSVOA_X
ClientSampleId :
SUTTON-PR-2152-SED




Tot Ion: 59 Resp: 1703
Ion Ratio Lower Upper
59 100
57 9.1 8.3 12.5

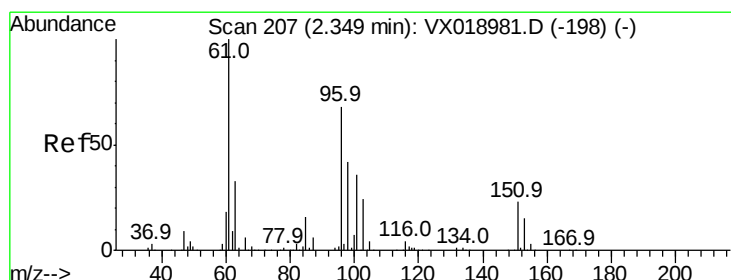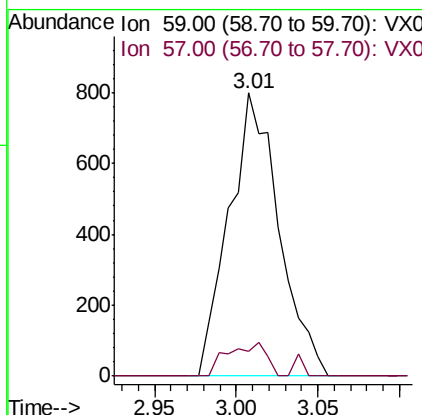


#12

1,1-Dichloroethene
Concen: Below Cal
RT: 2.31 min Scan# 200
Delta R.T. -0.04 min
Lab File: VX018995.D
Acq: 20 Oct 2020 23:47

Tgt Ion: 96 Resp: 95
Ion Ratio Lower Upper
96 100
61 0.0 117.4 176.0#
98 0.0 48.9 73.3#

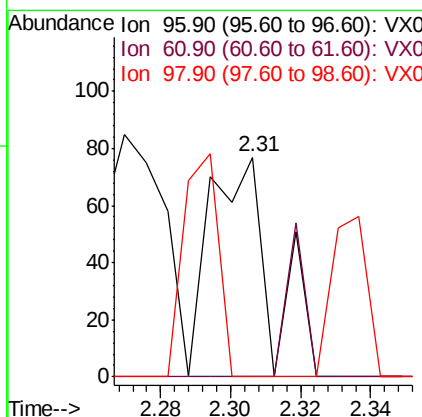



#13

Acrolein

Concen: Below Cal

RT: 2.29 min Scan# 197

Delta R.T. 0.02 min

Lab File: VX018995.D

Acq: 20 Oct 2020 23:47

Instrument :

MSVOA_X

ClientSampleId :





SUTTON-PR-2152-SED

Tot Ion: 56 Resp: 277

Ion Ratio Lower Upper

56 100

55 0.0 55.4 83.2#

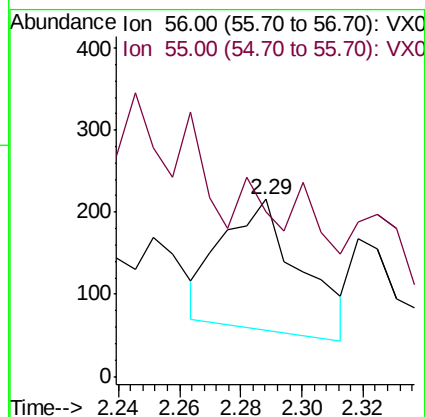

#16

Acetone

Concen: 22.193 ug/l

RT: 2.42 min Scan# 218

Delta R.T. -0.00 min

Lab File: VX018995.D




Acq: 20 Oct 2020 23:47


Tgt Ion: 43 Resp: 16456

Ion Ratio Lower Upper

43 100

58 34.3 27.9 41.9



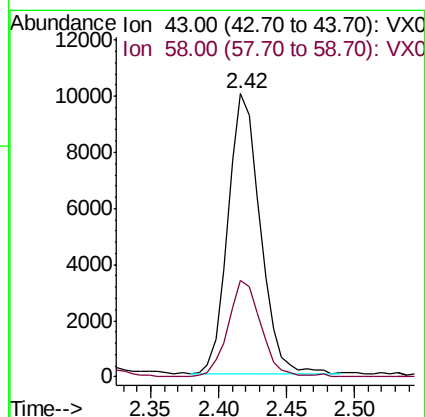





#18
Methvl Acetate
Concen: 0.934 ug/l
RT: 2.75 min Scan# 272
Delta R.T. -0.00 min
Lab File: VX018995.D
Acq: 20 Oct 2020 23:47




Instrument :
MSVOA_X
ClientSampleId :
SUTTON-PR-2152-SED


Tot Ion: 43 Resp: 1679
Ion Ratio Lower Upper
43 100
74 35.7 24.1 36.1

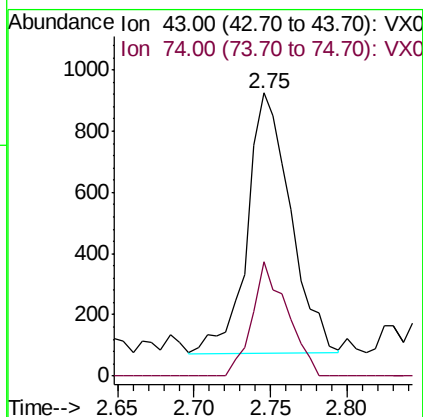

#20
Methylene Chloride
Concen: 2.310 ug/l
RT: 2.83 min Scan# 286
Delta R.T. -0.00 min
Lab File: VX018995.D
Acq: 20 Oct 2020 23:47

Tgt Ion: 84 Resp: 4427
Ion Ratio Lower Upper
84 100
49 100.5 82.9 124.3
51 30.8 26.4 39.6
86 66.1 51.8 77.6



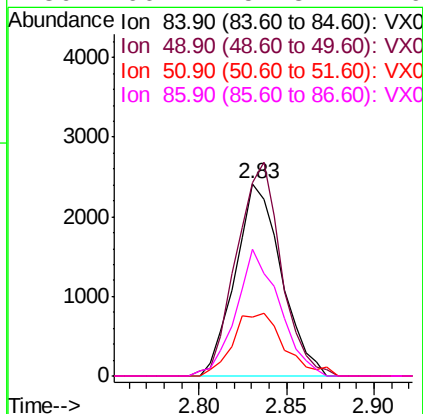





#25
2-Butanone
Concen: 6.842 ug/l
RT: 4.64 min Scan# 583
Delta R.T. 0.01 min
Lab File: VX018995.D
Acq: 20 Oct 2020 23:47




Instrument :
MSVOA_X
ClientSampleId :
SUTTON-PR-2152-SED


Tot Ion: 43 Resp: 8196
Ion Ratio Lower Upper
43 100
72 32.7 27.3 40.9

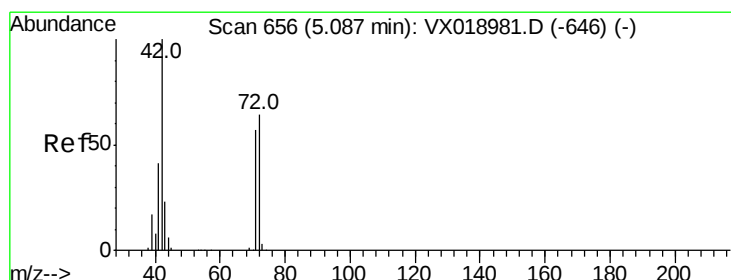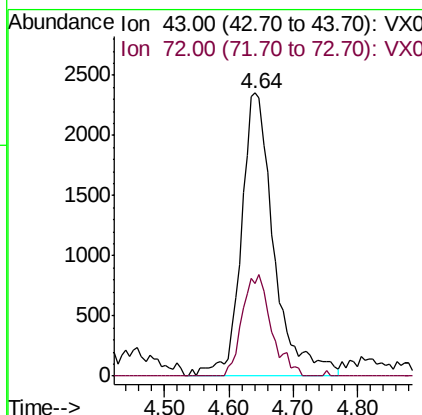

#29
Tetrahydrofuran
Concen: 1.500 ug/l
RT: 5.10 min Scan# 659
Delta R.T. 0.02 min
Lab File: VX018995.D
Acq: 20 Oct 2020 23:47

Tgt Ion: 42 Resp: 1059
Ion Ratio Lower Upper
42 100
72 43.9 49.2 73.8#
71 18.9 45.3 67.9#

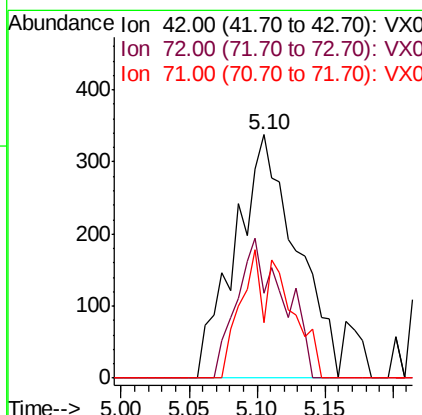







#31
Cvclohexane
Concen: 1.426 ug/l
RT: 5.63 min Scan# 745
Delta R.T. 0.09 min
Lab File: VX018995.D
Acq: 20 Oct 2020 23:47

Instrument :
MSVOA_X
ClientSampleId :
SUTTON-PR-2152-SED

Tot Ion: 56 Resp: 3549
Ion Ratio Lower Upper
56 100
69 186.6 27.1 40.7#
84 153.0 80.4 120.6#




Abundance Ion 56.00 (55.70 to 56.70): VX0
Ion 69.00 (68.70 to 69.70): VX0
Ion 84.00 (83.70 to 84.70): VX0

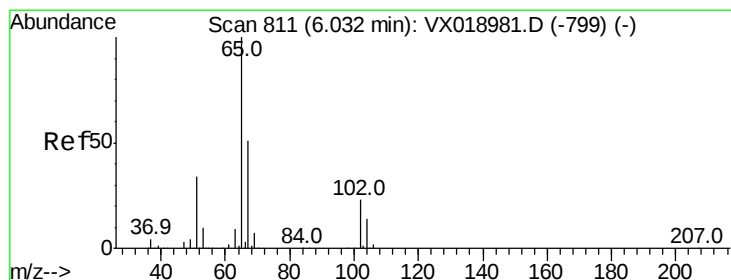
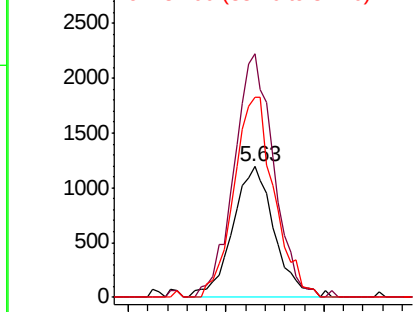



#33
1,2-Dichloroethane-d4
Concen: 52.572 ug/l
RT: 6.03 min Scan# 811
Delta R.T. -0.00 min
Lab File: VX018995.D
Acq: 20 Oct 2020 23:47

Tgt Ion: 65 Resp: 111953
Ion Ratio Lower Upper
65 100
67 52.0 0.0 105.4



Abundance Ion 64.90 (64.60 to 65.60): VX0
Ion 66.90 (66.60 to 67.60): VX0

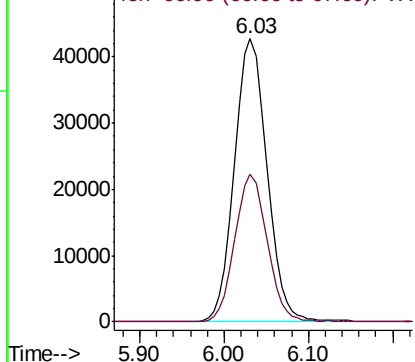


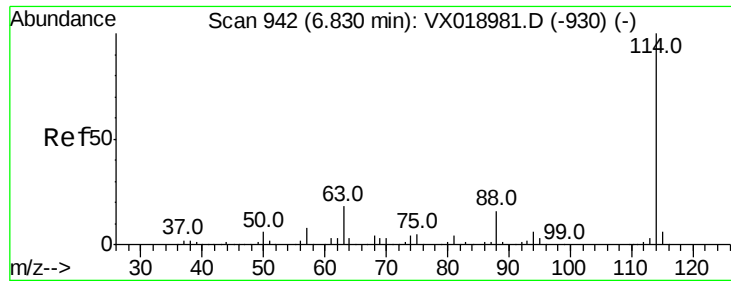




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.83 min Scan# 942
 Delta R.T. -0.00 min
 Lab File: VX018995.D
 Acq: 20 Oct 2020 23:47

Instrument :
 MSVOA_X
 ClientSampleId :
 SUTTON-PR-2152-SED

Tot Ion:114 Resp: 301370
 Ion Ratio Lower Upper
 114 100
 63 19.7 0.0 36.8
 88 16.1 0.0 31.8




Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VX0
 Ion 87.90 (87.60 to 88.60): VX0

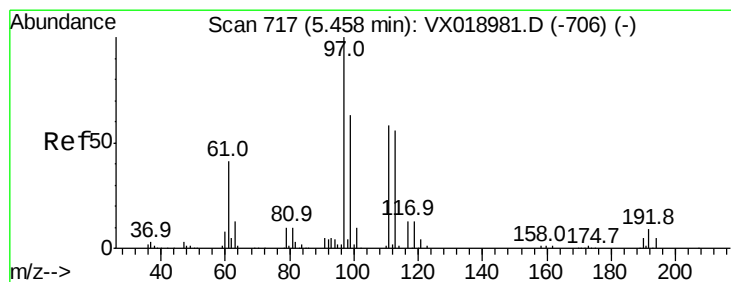
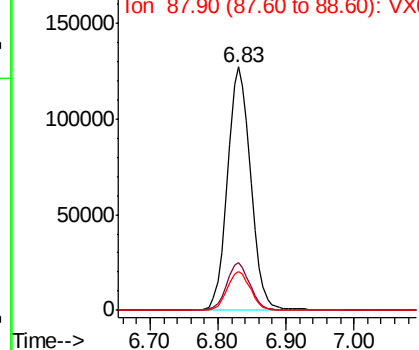



#35
 Dibromofluoromethane
 Concen: 47.987 ug/l
 RT: 5.46 min Scan# 718
 Delta R.T. 0.01 min
 Lab File: VX018995.D
 Acq: 20 Oct 2020 23:47

Tgt Ion:113 Resp: 91401
 Ion Ratio Lower Upper
 113 100
 111 103.4 84.1 126.1
 192 17.8 14.7 22.1



Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V




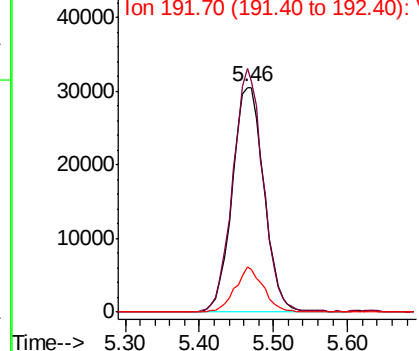




#36
 1,1-Dichloropropene
 Concen: 4.896 ug/l
 RT: 5.63 min Scan# 745
 Delta R.T. -0.14 min
 Lab File: VX018995.D
 Acq: 20 Oct 2020 23:47




Instrument :
 MSVOA_X
 ClientSampleId :
 SUTTON-PR-2152-SED


Tot Ion: 75 Resp: 13789
 Ion Ratio Lower Upper
 75 100
 110 8.7 18.6 55.6#
 77 0.0 25.0 37.4#

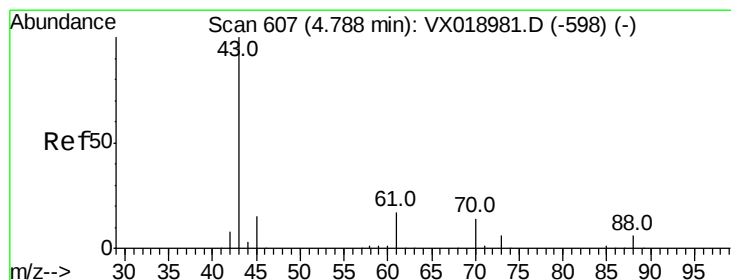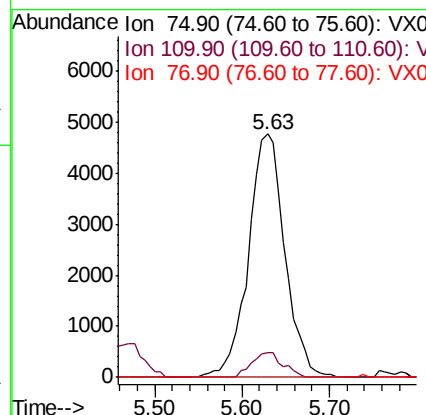

#37
 Ethyl Acetate
 Concen: 3.366 ug/l
 RT: 4.64 min Scan# 583
 Delta R.T. -0.15 min
 Lab File: VX018995.D
 Acq: 20 Oct 2020 23:47

Tgt Ion: 43 Resp: 8196
 Ion Ratio Lower Upper
 43 100
 61 4.0 13.5 20.3#
 70 0.0 11.4 17.2#

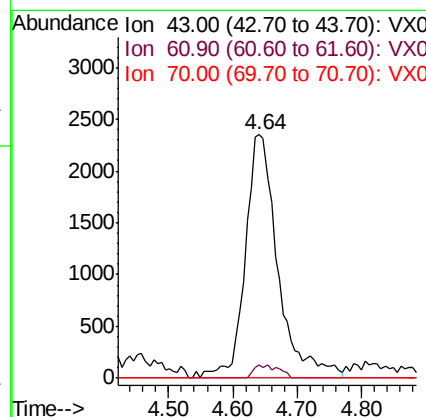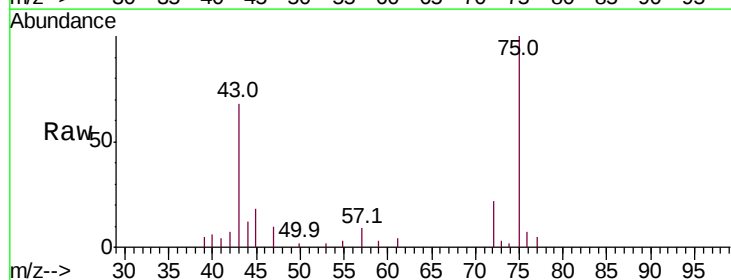



#38

Carbon Tetrachloride

Concen: 5.740 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.12 min

Lab File: VX018995.D

Acq: 20 Oct 2020 23:47

Instrument :

MSVOA_X

ClientSampleId :

SUTTON-PR-2152-SED


Tot Ion:117 Resp: 16268

Ion Ratio Lower Upper

117 100

119 6.5 77.6 116.4#




121 0.0 23.9 35.9#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

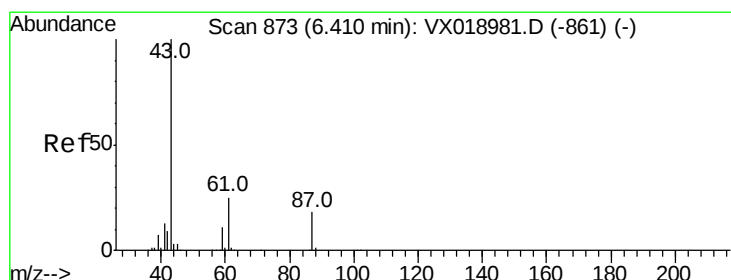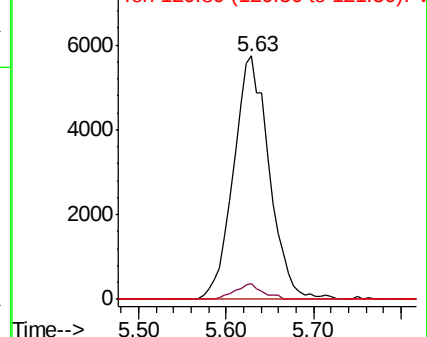

#43

Isopropyl Acetate

Concen: 7.829 ug/l

RT: 6.41 min Scan# 873

Delta R.T. -0.00 min

Lab File: VX018995.D

Acq: 20 Oct 2020 23:47


Tgt Ion: 43 Resp: 32119

Ion Ratio Lower Upper

43 100

61 23.3 19.3 28.9



87 17.6 14.3 21.5




Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0




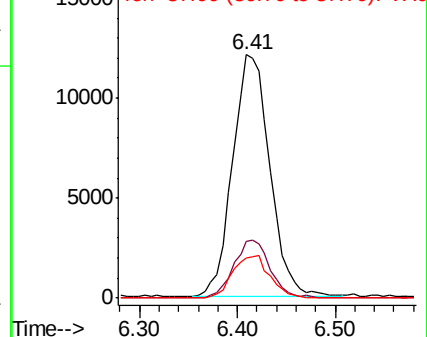




#48
Methvl methacrylate
Concen: 1.407 ug/l
RT: 7.65 min Scan# 1077
Delta R.T. -0.09 min
Lab File: VX018995.D
Acq: 20 Oct 2020 23:47




Instrument :
MSVOA_X
ClientSampleId :
SUTTON-PR-2152-SED


Tot Ion: 41 Resp: 2850
Ion Ratio Lower Upper
41 100
69 0.0 88.0 132.0#
39 22.4 49.9 74.9#

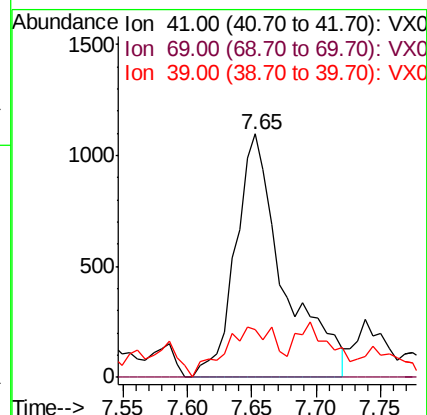

#49
1,4-Dioxane
Concen: 0.484 ug/l
RT: 7.84 min Scan# 1108
Delta R.T. 0.13 min
Lab File: VX018995.D
Acq: 20 Oct 2020 23:47

Tgt Ion: 88 Resp: 26
Ion Ratio Lower Upper
88 100
43 1295892.3 20.4 30.6#
58 6496.2 49.3 73.9#



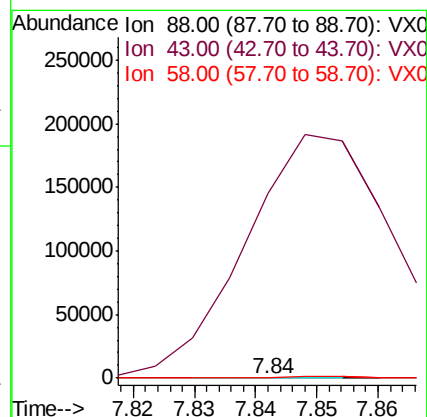





#50
Toluene-d8
Concen: 51.580 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. -0.00 min
Lab File: VX018995.D
Acq: 20 Oct 2020 23:47




Instrument :
MSVOA_X
ClientSampleId :
SUTTON-PR-2152-SED


Tot Ion: 98 Resp: 391480
Ion Ratio Lower Upper
98 100
100 64.5 52.6 78.8

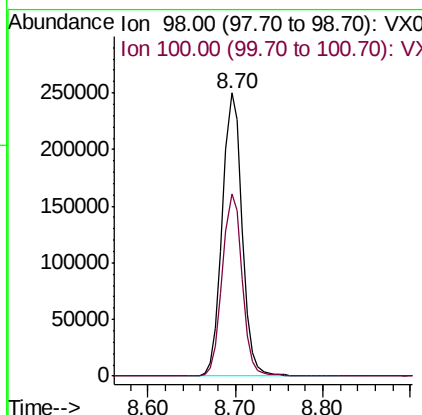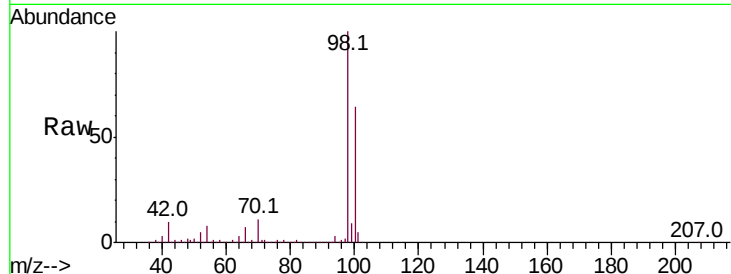

#51
4-Methyl-2-Pentanone
Concen: 14.322 ug/l
RT: 8.59 min Scan# 1231
Delta R.T. -0.03 min
Lab File: VX018995.D
Acq: 20 Oct 2020 23:47

Tgt Ion: 43 Resp: 36282
Ion Ratio Lower Upper
43 100
58 11.4 37.8 56.8#



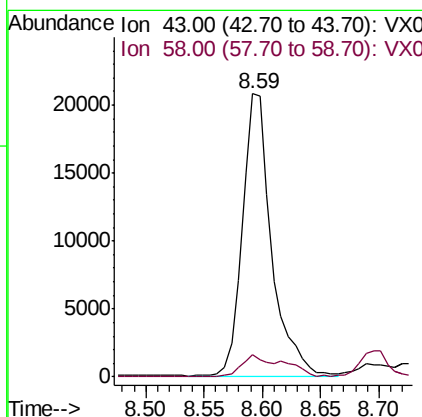





#54
 cis-1,3-Dichloropropene
 Concen: 5.682 ug/l
 RT: 8.59 min Scan# 1231
 Delta R.T. 0.18 min
 Lab File: VX018995.D
 Acq: 20 Oct 2020 23:47




Instrument :
 MSVOA_X
 ClientSampleId :
 SUTTON-PR-2152-SED


Tot Ion: 75 Resp: 20036
 Ion Ratio Lower Upper
 75 100
 77 0.5 25.4 38.0#
 39 23.0 31.3 46.9#

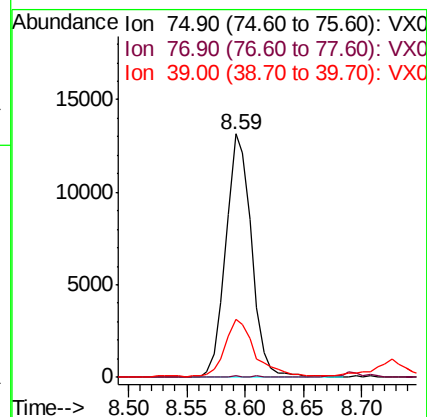

#57
 1,3-Dichloropropane
 Concen: 0.711 ug/l
 RT: 9.52 min Scan# 1384
 Delta R.T. 0.17 min
 Lab File: VX018995.D
 Acq: 20 Oct 2020 23:47

Tgt Ion: 76 Resp: 2555
 Ion Ratio Lower Upper
 76 100
 78 0.9 26.1 39.1#

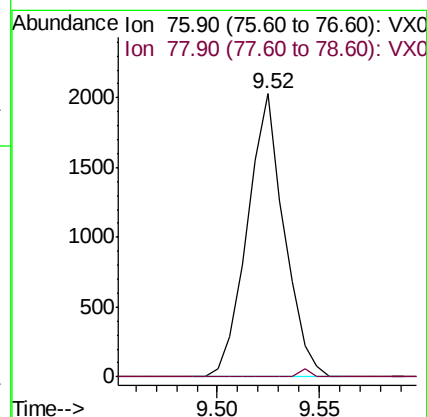







#59
2-Hexanone
Concen: 17.617 ug/l
RT: 9.42 min Scan# 1367
Delta R.T. -0.05 min
Lab File: VX018995.D
Acq: 20 Oct 2020 23:47

Instrument :
MSVOA_X
ClientSampleId :
SUTTON-PR-2152-SED

Tot Ion: 43 Resp: 34658
Ion Ratio Lower Upper
43 100
58 0.0 33.0 99.0#




Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 58.00 (57.70 to 58.70): VX0


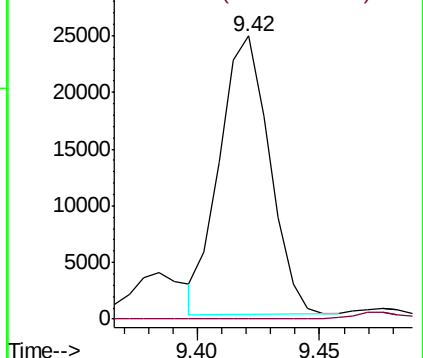



#60
Dibromochloromethane
Concen: 0.449 ug/l
RT: 9.32 min Scan# 1350
Delta R.T. -0.25 min
Lab File: VX018995.D
Acq: 20 Oct 2020 23:47

Tgt Ion:129 Resp: 1106
Ion Ratio Lower Upper
129 100
127 0.0 38.8 116.4#



Abundance Ion 128.80 (128.50 to 129.50): V
Ion 126.80 (126.50 to 127.50): V

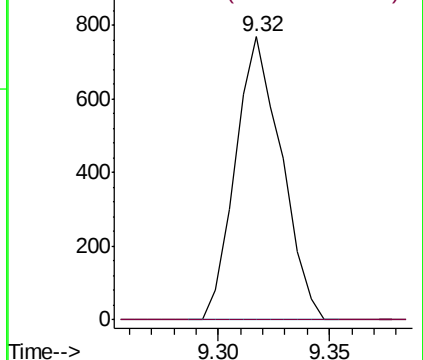

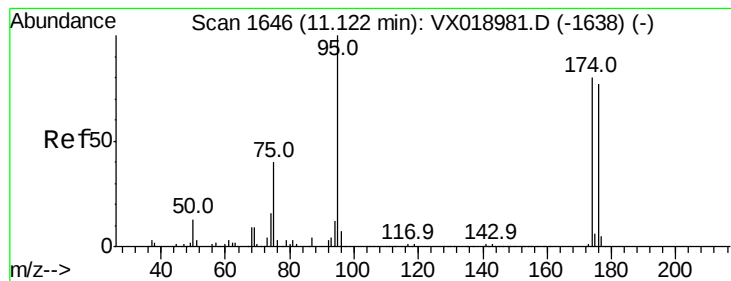

#62

4-Bromofluorobenzene

Concen: 48.973 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX018995.D

Acq: 20 Oct 2020 23:47

Instrument :

MSVOA_X

ClientSampleId :

SUTTON-PR-2152-SED


Tot Ion: 95 Resp: 145182

Ion Ratio Lower Upper




95 100

174 74.3 0.0 159.8

176 71.3 0.0 152.8



Abundance Ion 94.90 (94.60 to 95.60): VX018995.D (-1597) (-)

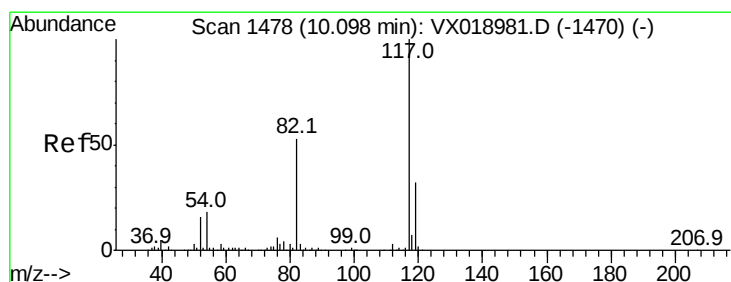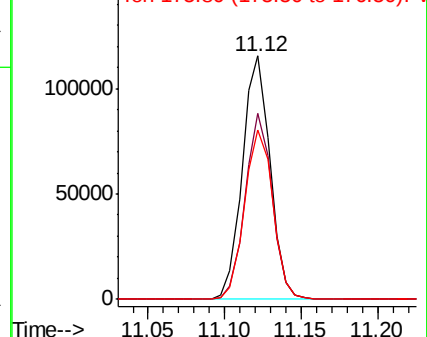

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.10 min Scan# 1478

Delta R.T. -0.00 min

Lab File: VX018995.D

Acq: 20 Oct 2020 23:47


Tgt Ion: 117 Resp: 296187

Ion Ratio Lower Upper



117 100


82 55.1 42.2 63.4

119 31.2 25.8 38.8



Abundance Ion 116.90 (116.60 to 117.60): VX018995.D (-1429) (-)

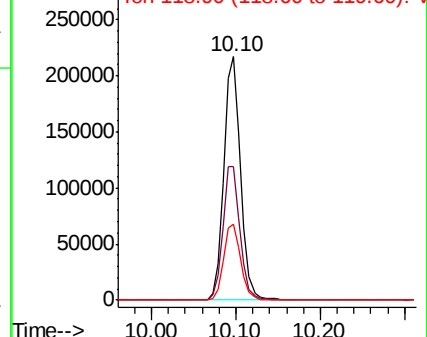

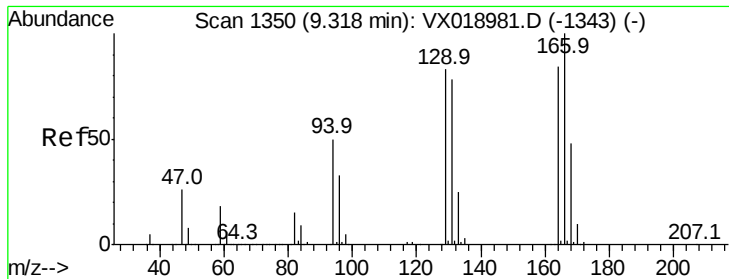

#64

Tetrachloroethene

Concen: 0.532 ug/l

RT: 9.32 min Scan# 1351

Delta R.T. 0.01 min

Lab File: VX018995.D

Acq: 20 Oct 2020 23:47

Instrument :

MSVOA_X

ClientSampleId :

SUTTON-PR-2152-SED

Tot Ion:164 Resp: 1111


Ion Ratio Lower Upper

164 100




166 125.4 95.2 142.8

129 87.8 79.4 119.0

131 79.6 74.2 111.2

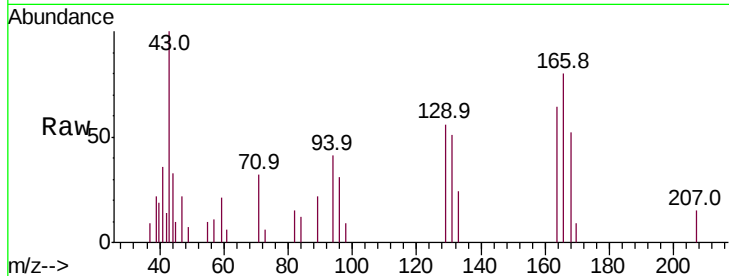

Abundance Ion 163.80 (163.50 to 164.50): V
Ion 165.80 (165.50 to 166.50): V
Ion 128.80 (128.50 to 129.50): V
Ion 130.80 (130.50 to 131.50): V

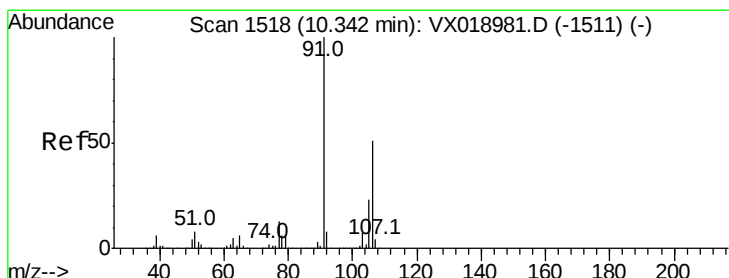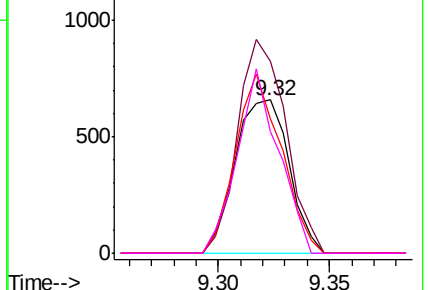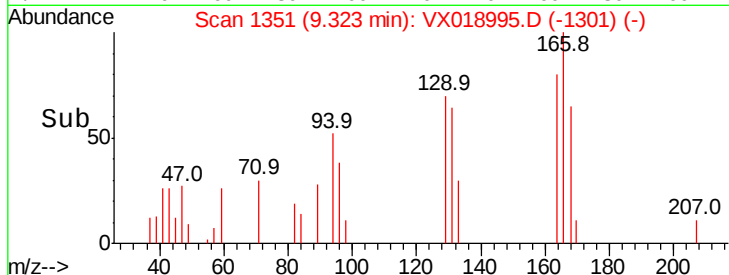

#68

m/p-Xylenes

Concen: 0.271 ug/l

RT: 10.34 min Scan# 1518

Delta R.T. -0.00 min

Lab File: VX018995.D


Acq: 20 Oct 2020 23:47

Tgt Ion:106 Resp: 1157



Ion Ratio Lower Upper


106 100

91 191.4 157.9 236.9

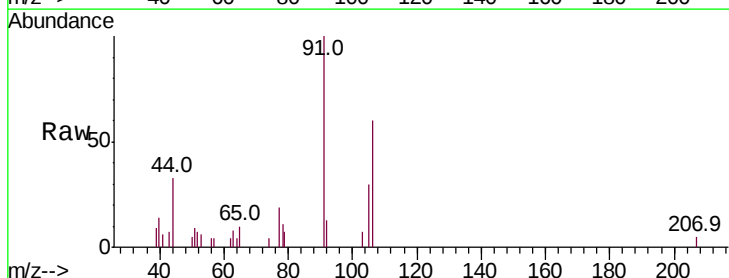

Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): V

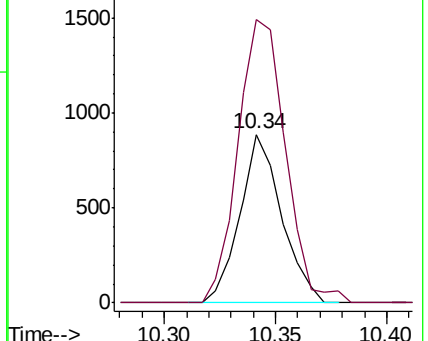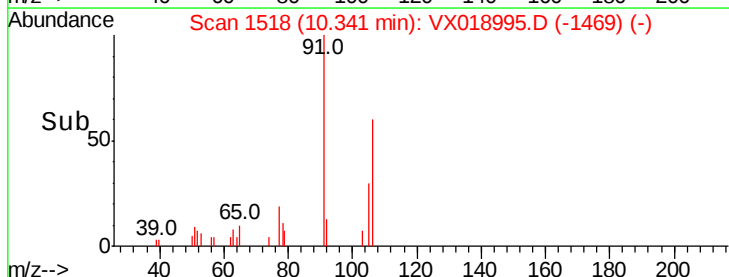

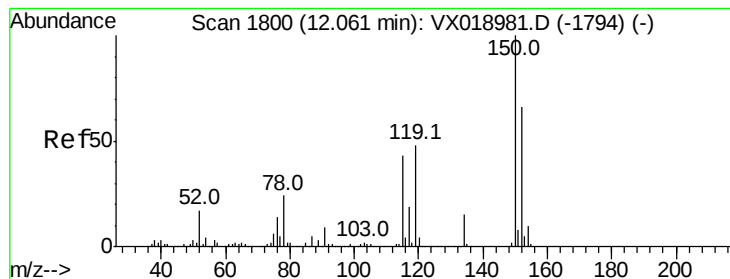

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX018995.D

Acq: 20 Oct 2020 23:47

Instrument :

MSVOA_X

ClientSampleId :

SUTTON-PR-2152-SED


Tot Ion:152 Resp: 145453

Ion Ratio Lower Upper

152 100

115 63.2 41.2 123.6




150 159.4 0.0 345.6

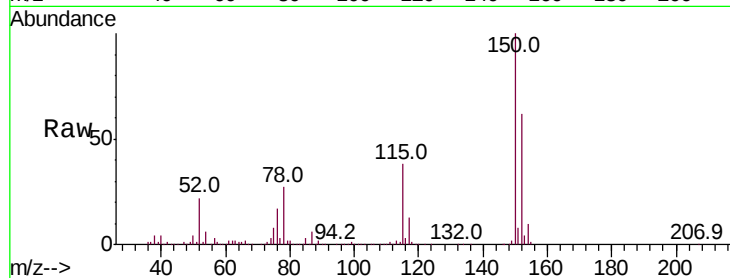

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

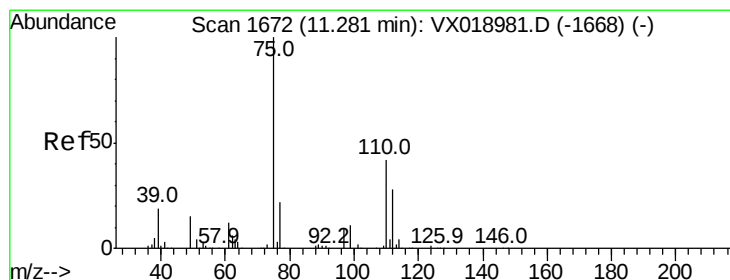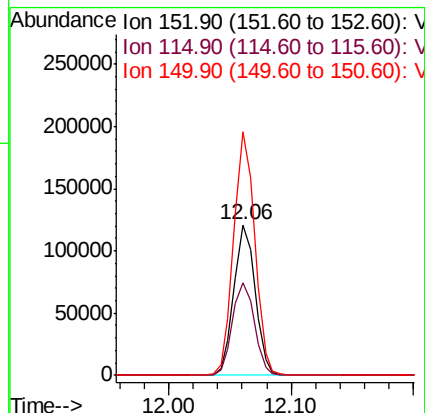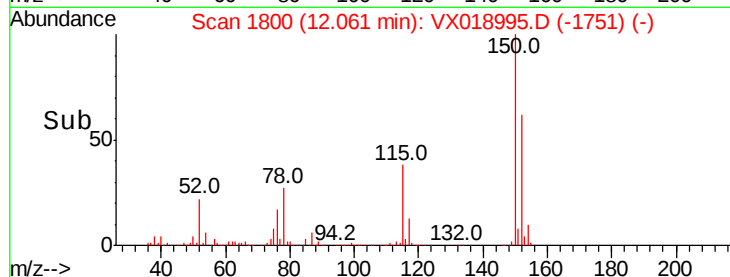

#76

1,2,3-Trichloropropane

Concen: 24.537 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX018995.D


Acq: 20 Oct 2020 23:47

Tgt Ion: 75 Resp: 73353

Ion Ratio Lower Upper



75 100


77 1.3 20.6 61.9#

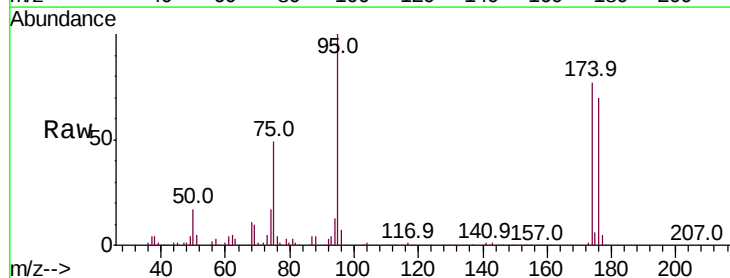

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

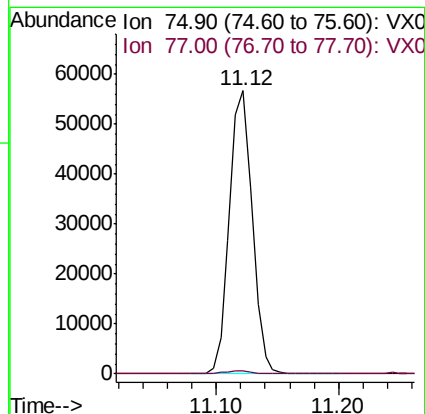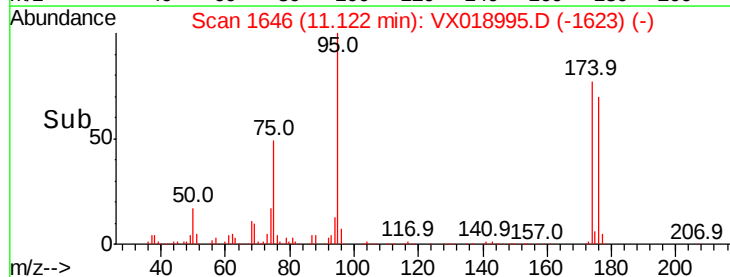



#81

trans-1,4-Dichloro-2-butene

Concen: 64.723 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.07 min

Lab File: VX018995.D

Acq: 20 Oct 2020 23:47

Instrument :

MSVOA_X

ClientSampleId :

SUTTON-PR-2152-SED


Tot Ion: 75 Resp: 73353

Ion Ratio Lower Upper

75 100

53 0.0 63.9 95.9#




89 0.0 39.9 59.9#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

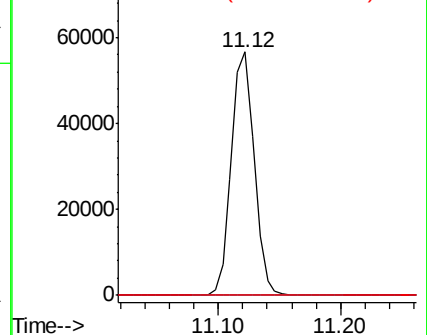

#95

Naphthalene

Concen: 2.118 ug/l

RT: 13.82 min Scan# 2088

Delta R.T. -0.00 min

Lab File: VX018995.D

Acq: 20 Oct 2020 23:47


Tgt Ion:128 Resp: 22828

Ion Ratio Lower Upper

128 100

127 13.0 10.3 15.5

129 10.5 8.6 12.8



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

