


1,1,2-Trichlorotrifluoroethane

Response Ratio

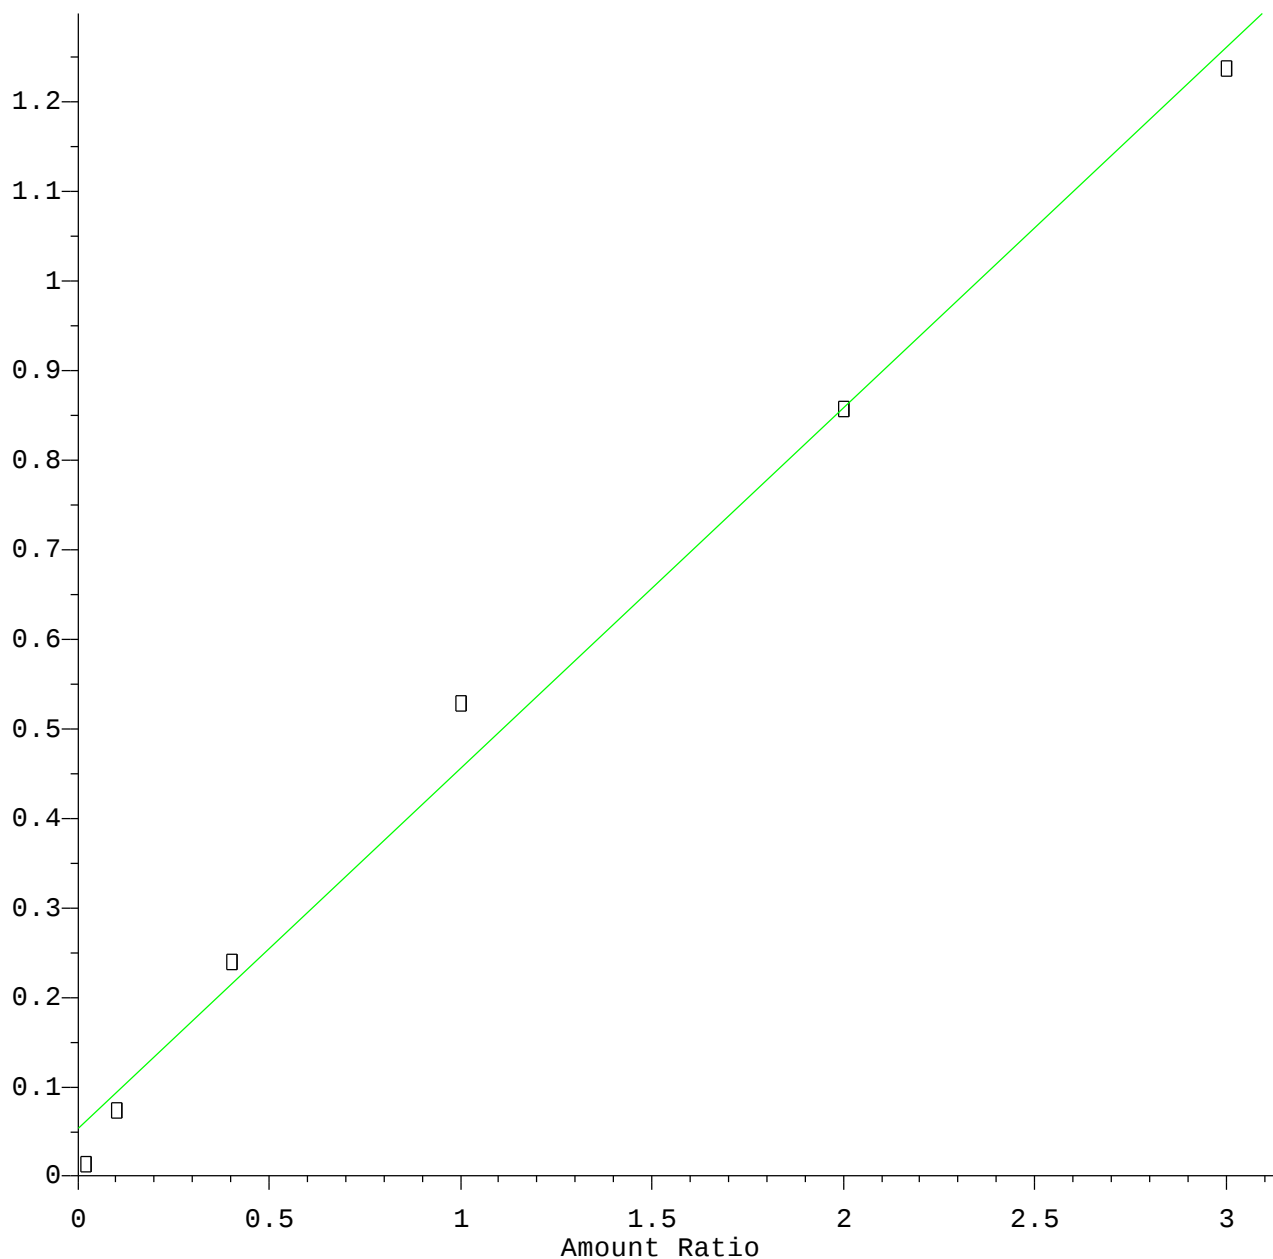


Resp Ratio = $4.03e-001 * Amt + 5.32e-002$
Coef of Det (r^2) = 0.992 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102020W.M
Calibration Table Last Updated: Tue Oct 20 19:16:32 2020

1,1-Dichloroethene

Response Ratio

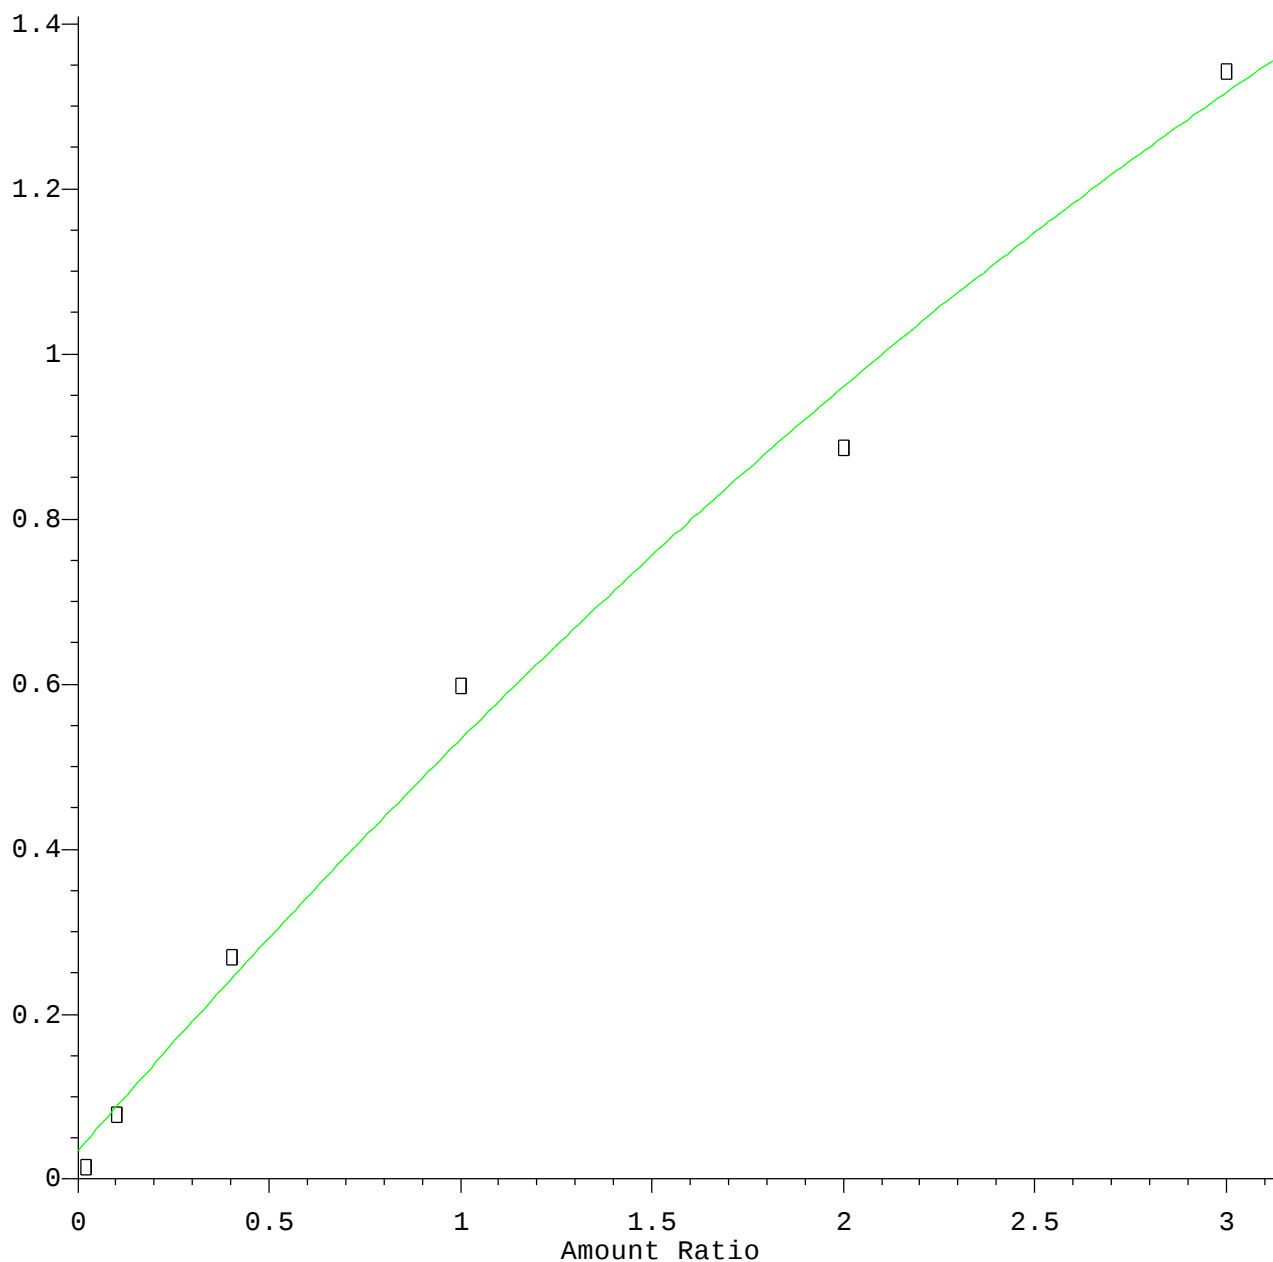


$R = -3.56e-002 A^2 + 5.34e-001 A + 3.45e-002$
Coef of Det (r^2) = 0.991 Curve Fit: Quadratic

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102020W.M
Calibration Table Last Updated: Tue Oct 20 19:16:32 2020


Acrolein

Response Ratio

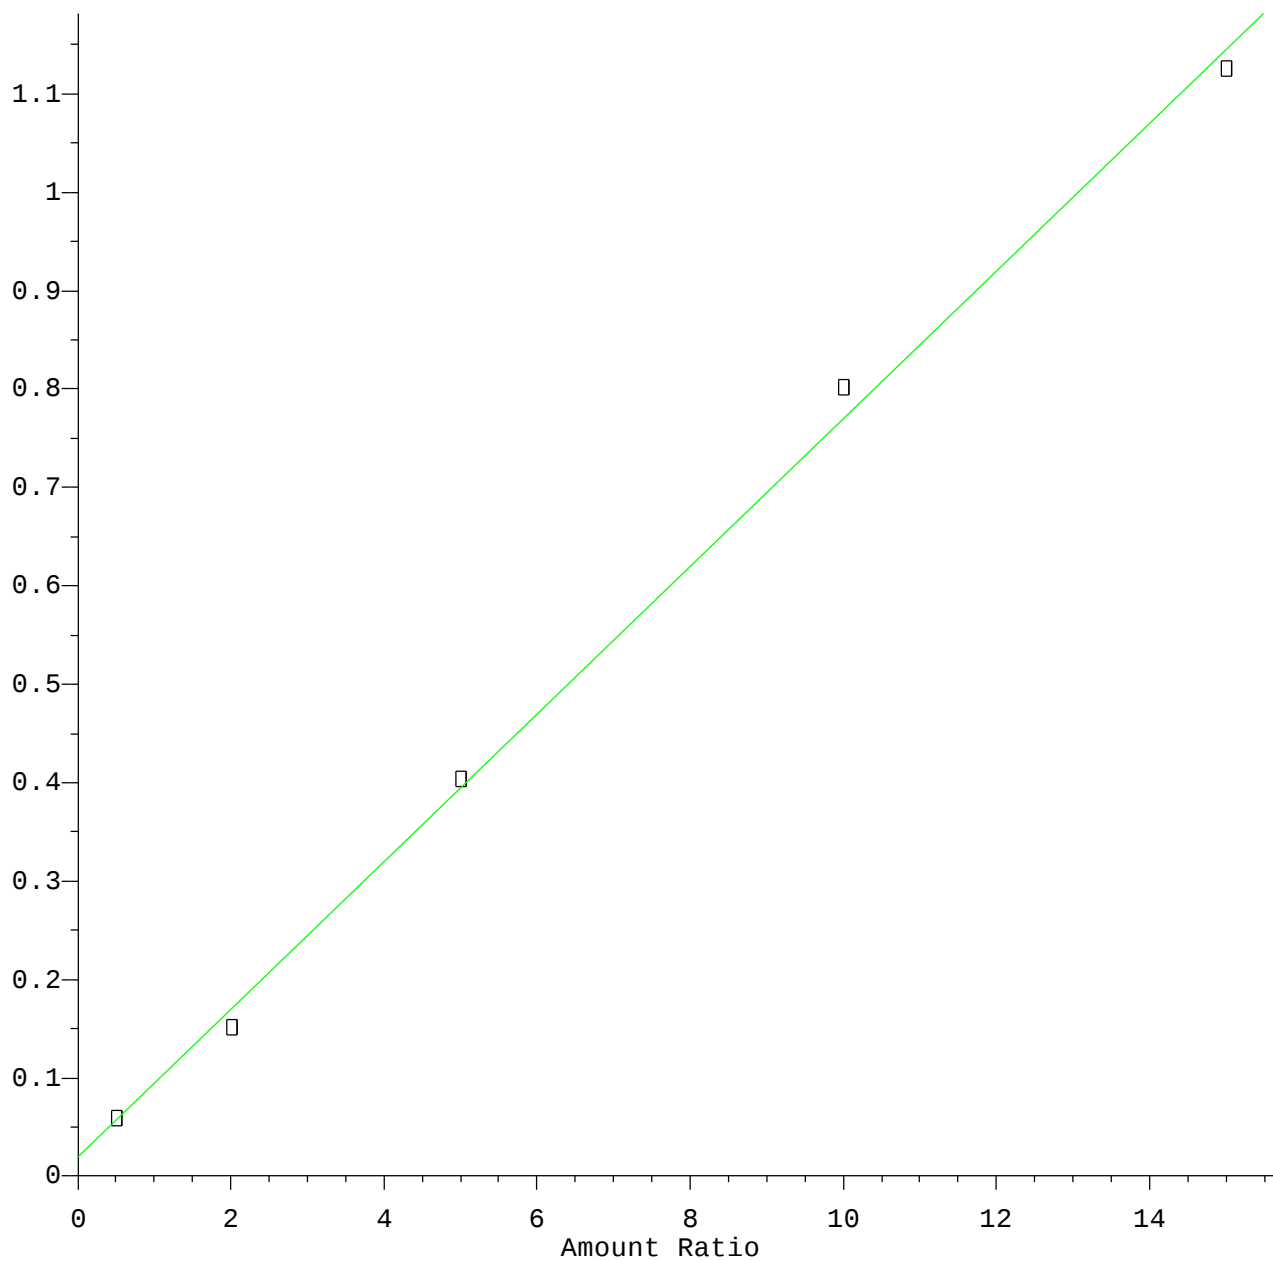

Resp Ratio = $7.50 \times 10^{-2} \times \text{Amt} + 2.03 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102020W.M
Calibration Table Last Updated: Tue Oct 20 19:16:32 2020

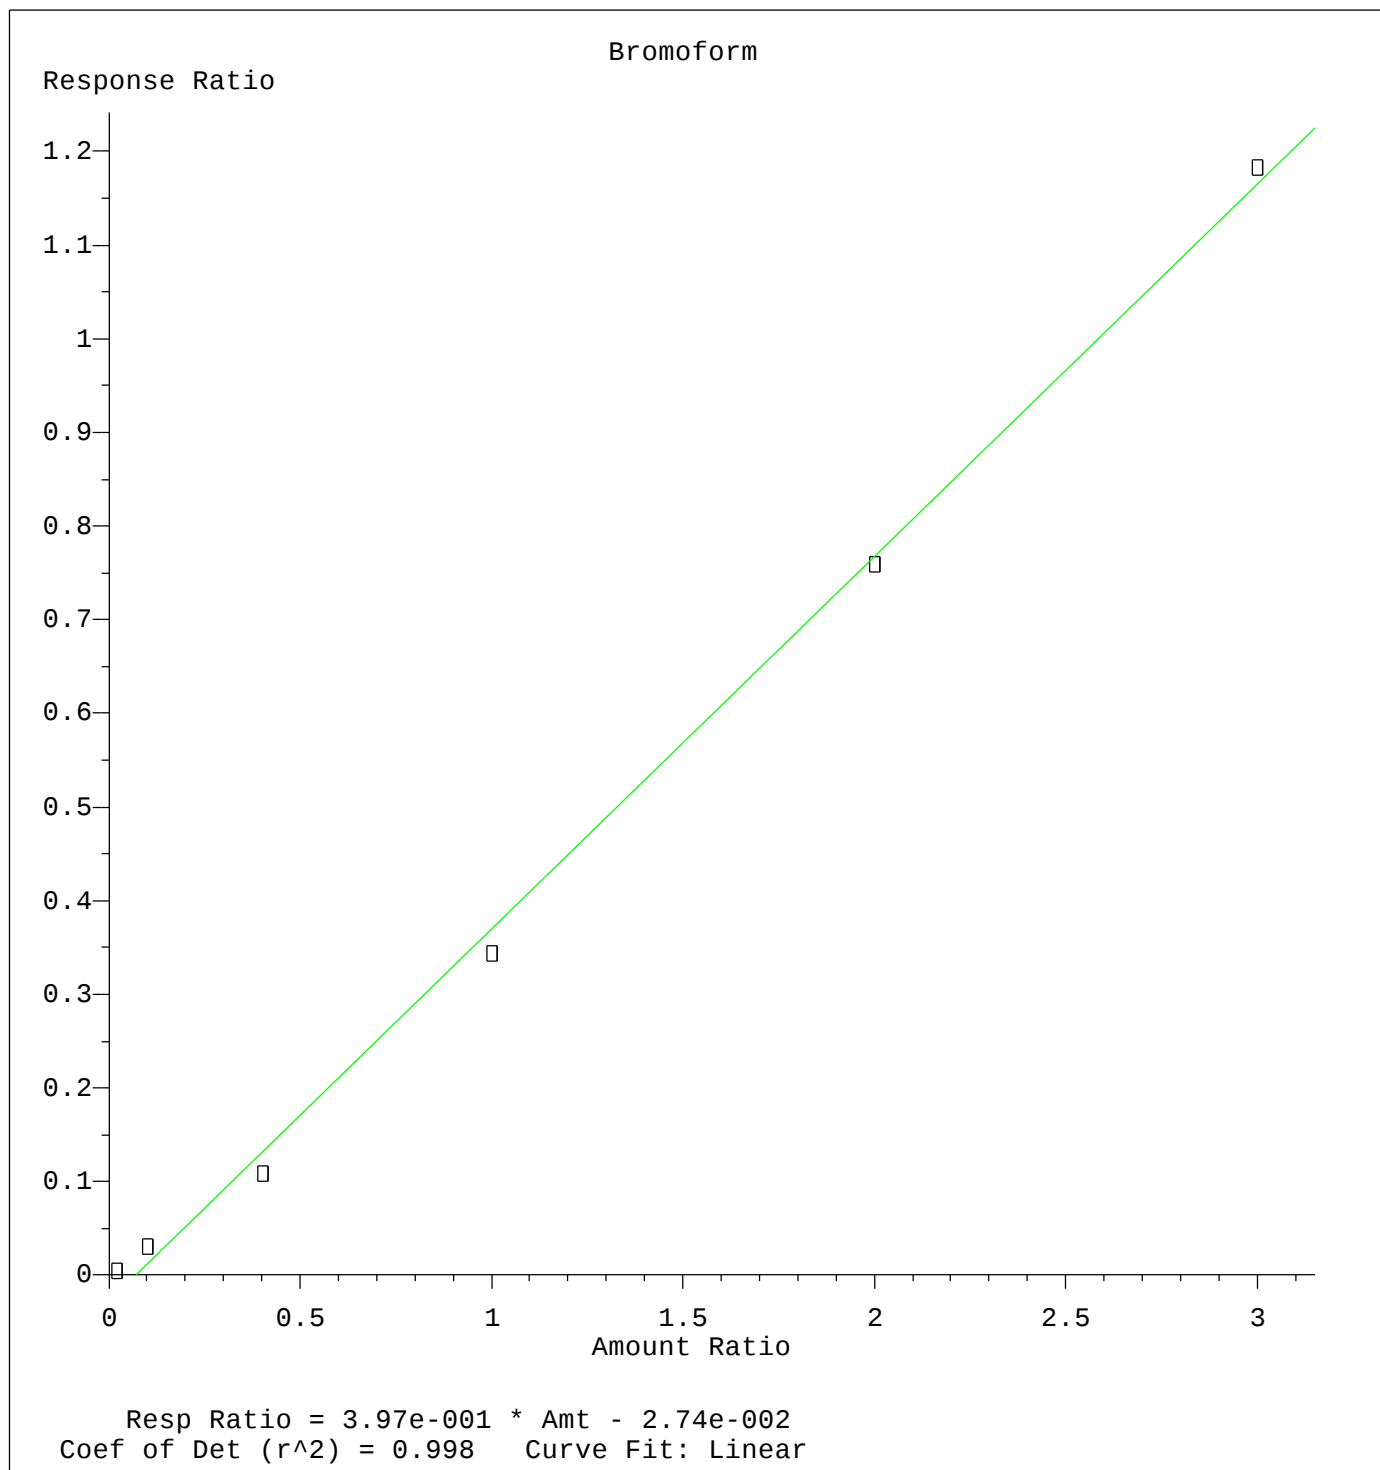

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102020W.M
Calibration Table Last Updated: Tue Oct 20 19:16:32 2020