

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102022\
 Data File : VX032271.D
 Acq On : 20 Oct 2022 18:24
 Operator : JC/MD
 Sample : N5185-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-04

Quant Time: Oct 21 02:15:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 19 16:51:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	148663	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	229631	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	198352	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	91424	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	94476	48.851	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	97.700%		
35) Dibromofluoromethane	5.385	113	71700	44.871	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	89.740%		
50) Toluene-d8	8.647	98	270348	47.000	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	94.000%		
62) 4-Bromofluorobenzene	11.079	95	94951	45.079	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	90.160%		
Target Compounds						Qvalue
3) Chloromethane	1.288	50	200	Below Cal	#	44
6) Chloroethane	1.679	64	82	2.007	ug/l #	41
11) Tert butyl alcohol	2.934	59	120	Below Cal	#	74
13) Acrolein	2.337	56	1310	5.564	ug/l	84
14) Allyl chloride	2.776	41	8872	4.257	ug/l #	66
15) Acrylonitrile	3.105	53	854	1.177	ug/l #	33
16) Acetone	2.386	43	4074	6.491	ug/l	99
18) Methyl Acetate	2.782	43	19666	9.230	ug/l #	50
25) 2-Butanone	4.574	43	2136	2.180	ug/l	96
31) Cyclohexane	5.477	56	4682	2.118	ug/l	92
36) 1,1-Dichloropropene	5.550	75	11923	5.801	ug/l #	50
38) Carbon Tetrachloride	5.550	117	15492	7.139	ug/l #	17
39) Methylcyclohexane	7.379	83	3131	1.275	ug/l #	87
40) Benzene	6.044	78	8197	1.376	ug/l	96
48) Methyl methacrylate	7.653	41	519	0.329	ug/l #	74
52) Toluene	8.720	92	1364	0.353	ug/l	90
55) 1,1,2-Trichloroethane	9.104	97	371	0.237	ug/l #	15
67) Ethyl Benzene	10.195	91	50459	7.008	ug/l	99
68) m/p-Xylenes	10.305	106	4004	1.408	ug/l	87
73) Isopropylbenzene	10.964	105	6311	0.967	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	52124	28.774	ug/l #	45
78) n-propylbenzene	11.305	91	14298	1.914	ug/l	99
79) 2-Chlorotoluene	11.305	91	14298	3.176	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.402	105	2215	0.393	ug/l	77
81) trans-1,4-Dichloro-2-b...	11.079	75	52124	88.167	ug/l #	6
82) 4-Chlorotoluene	11.305	91	14298	2.728	ug/l #	45
84) 1,2,4-Trimethylbenzene	11.756	105	1877	0.343	ug/l	98
89) n-Butylbenzene	12.335	91	1366	0.268	ug/l #	67
90) Hexachloroethane	12.646	117	693	0.770	ug/l #	11
95) Naphthalene	13.780	128	5846	0.928	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102022\
Data File : VX032271.D
Acq On : 20 Oct 2022 18:24
Operator : JC/MD
Sample : N5185-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-04

Quant Time: Oct 21 02:15:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 19 16:51:09 2022
Response via : Initial Calibration



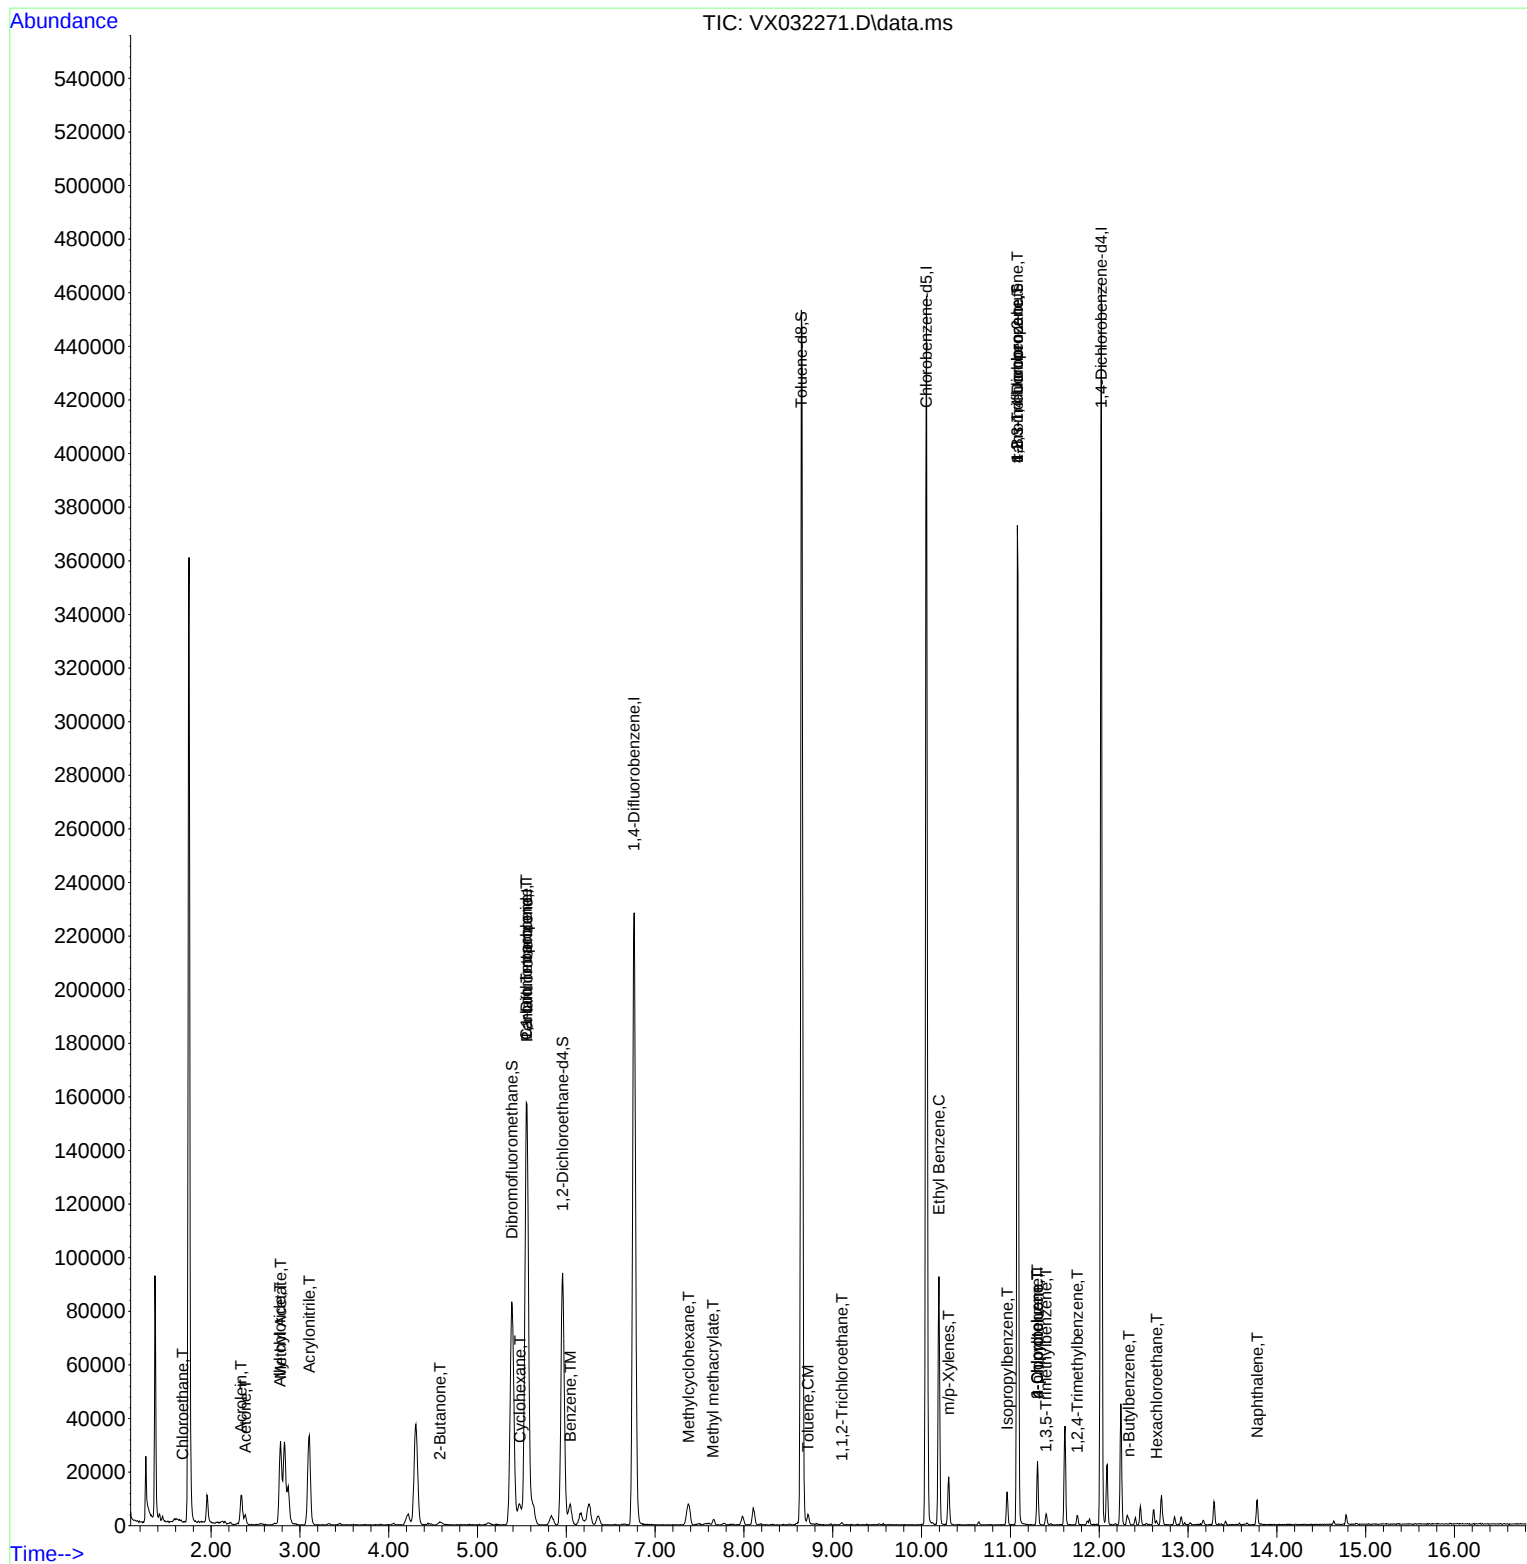




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24




Instrument :
MSVOA_X
ClientSampleId :
MW-04

Tgt Ion:168 Resp: 148663
Ion Ratio Lower Upper
168 100
99 56.4 44.8 67.2




#3
Chloromethane
Concen: Below Cal
RT: 1.288 min Scan# 33
Delta R.T. -0.007 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24

Tgt Ion: 50 Resp: 200
Ion Ratio Lower Upper
50 100
52 0.0 24.7 37.1#

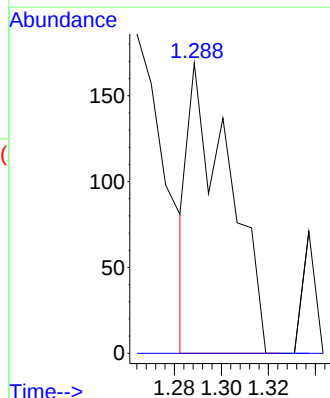


Abundance Scan 98 (1.685 min): VX032201.D\data.ms (-89)

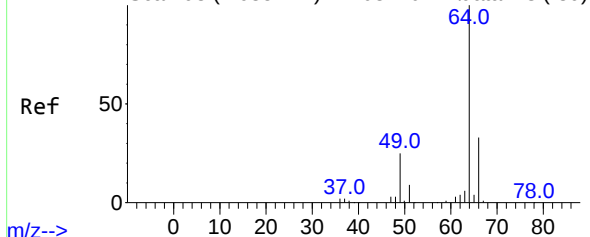


m/z-->

Abundance Scan 97 (1.679 min): VX032271.D\data.ms

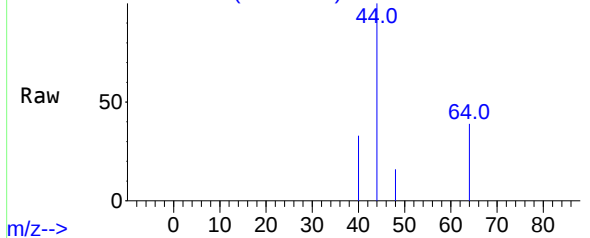

m/z-->

Abundance Scan 97 (1.679 min): VX032271.D\data.ms (-49)

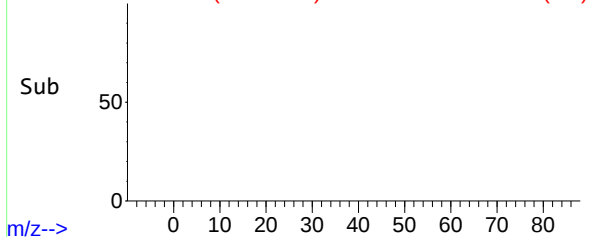


m/z-->


#6
Chloroethane
Concen: 2.007 ug/l
RT: 1.679 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24

Instrument :
MSVOA_X
ClientSampleId :
MW-04

Tgt Ion: 64 Resp: 82
Ion Ratio Lower Upper
64 100
66 0.0 26.6 39.8#




Abundance Scan 310 (2.977 min): VX032201.D\data.ms (-29)

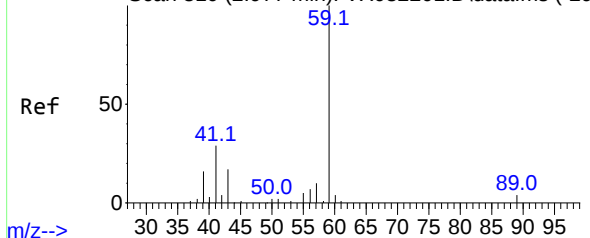


m/z-->

Abundance Scan 303 (2.934 min): VX032271.D\data.ms

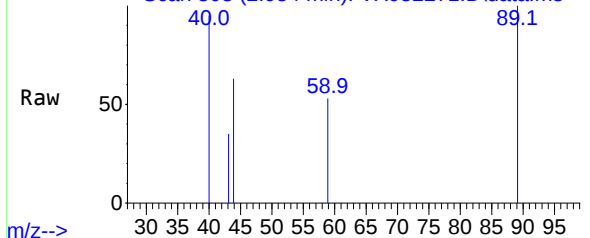

m/z-->


Abundance Scan 303 (2.934 min): VX032271.D\data.ms (-26)

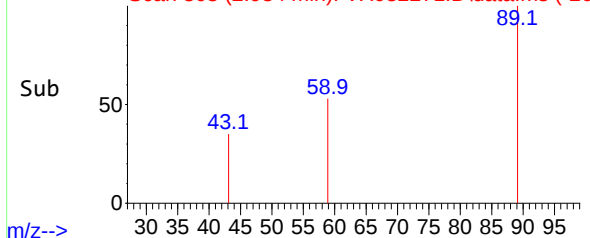


m/z-->

#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.934 min Scan# 303
Delta R.T. -0.043 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24

Tgt Ion: 59 Resp: 120
Ion Ratio Lower Upper
59 100
57 0.0 7.5 11.3#

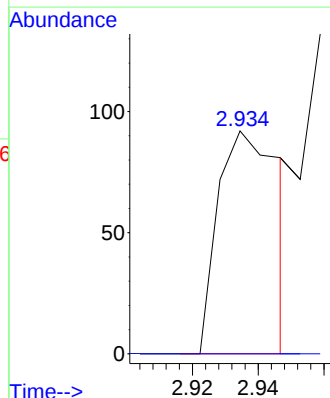



#13

Acrolein

Concen: 5.564 ug/l

RT: 2.337 min Scan# 205

Delta R.T. 0.104 min

Lab File: VX032271.D

Acq: 20 Oct 2022 18:24

Instrument :

MSVOA_X

ClientSampleId :





MW-04

Tgt Ion: 56 Resp: 1310

Ion Ratio Lower Upper

56 100

55 57.0 56.4 84.6

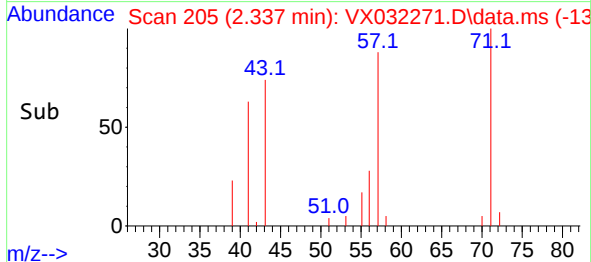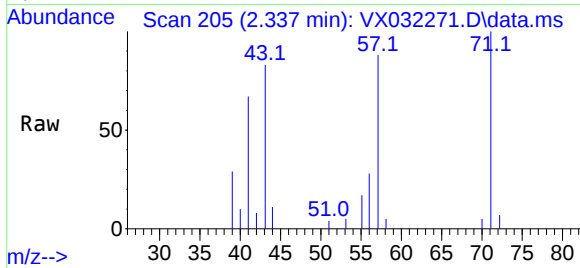

#14

Allyl chloride

Concen: 4.257 ug/l

RT: 2.776 min Scan# 277

Delta R.T. 0.110 min

Lab File: VX032271.D

Acq: 20 Oct 2022 18:24




Tgt Ion: 41 Resp: 8872


Ion Ratio Lower Upper

41 100

39 56.1 59.5 89.3#

76 0.0 28.6 42.8#


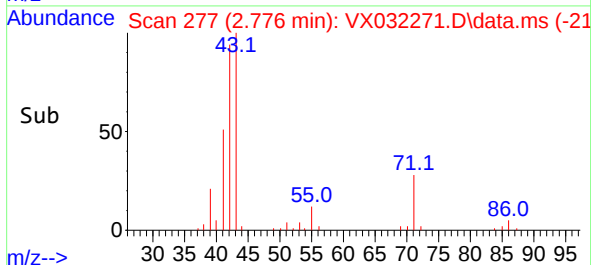
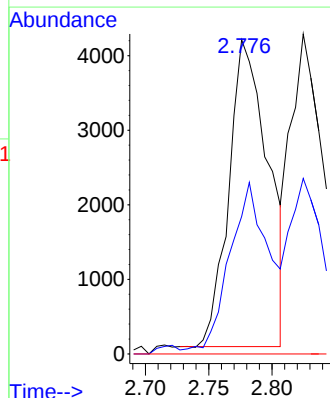
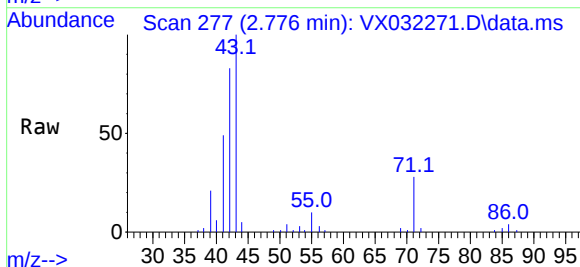




#15
Acrylonitrile
Concen: 1.177 ug/l
RT: 3.105 min Scan# 31
Delta R.T. 0.042 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24




Instrument :
MSVOA_X
ClientSampleId :
MW-04


Tgt Ion: 53 Resp: 854
Ion Ratio Lower Upper
53 100
52 13.1 65.9 98.9#
51 63.8 29.7 44.5#



#16
Acetone
Concen: 6.491 ug/l
RT: 2.386 min Scan# 213
Delta R.T. 0.006 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24

Tgt Ion: 43 Resp: 4074
Ion Ratio Lower Upper
43 100
58 29.9 24.2 36.2

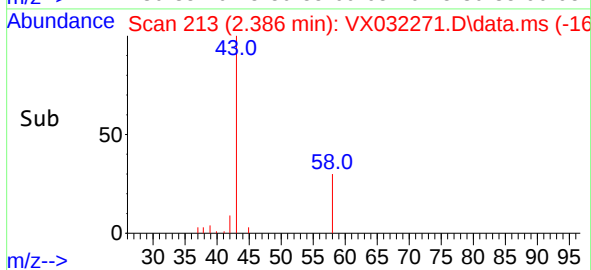



#18

Methyl Acetate

Concen: 9.230 ug/l

RT: 2.782 min Scan# 21

Delta R.T. 0.079 min

Lab File: VX032271.D

Acq: 20 Oct 2022 18:24

Instrument :

MSVOA_X

ClientSampleId :





MW-04

Tgt Ion: 43 Resp: 19666

Ion Ratio Lower Upper

43 100

74 0.0 19.8 29.8#

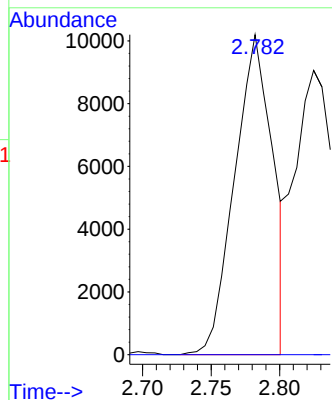

#25

2-Butanone

Concen: 2.180 ug/l

RT: 4.574 min Scan# 572

Delta R.T. 0.018 min

Lab File: VX032271.D




Acq: 20 Oct 2022 18:24


Tgt Ion: 43 Resp: 2136

Ion Ratio Lower Upper

43 100

72 29.2 21.7 32.5

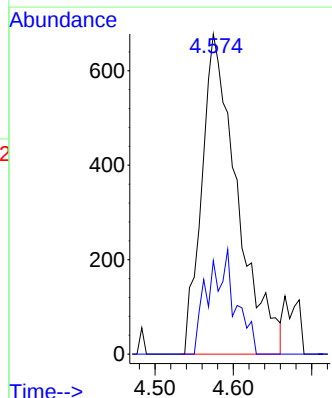







#31
Cyclohexane
Concen: 2.118 ug/l
RT: 5.477 min Scan# 719
Delta R.T. -0.000 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24

Instrument :
MSVOA_X
ClientSampleId :
MW-04

Tgt Ion: 56 Resp: 4682




Ion	Ratio	Lower	Upper
56	100		
69	30.3	25.4	38.0
84	98.2	71.2	106.8

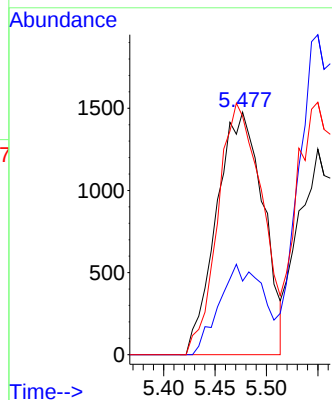


#33
1,2-Dichloroethane-d4
Concen: 48.851 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.006 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24

Tgt Ion: 65 Resp: 94476

Ion	Ratio	Lower	Upper
65	100		
67	49.9	0.0	103.6


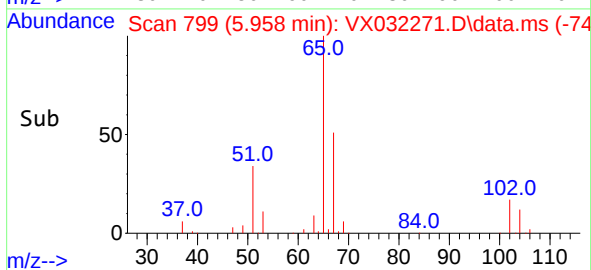
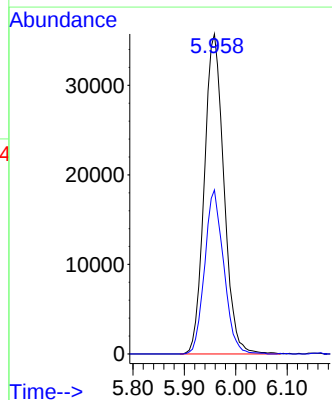
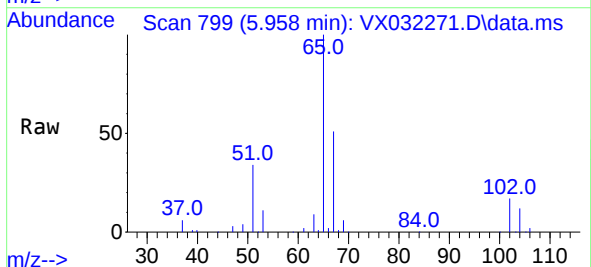




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24




Instrument :
MSVOA_X
ClientSampleId :
MW-04


Tgt Ion:114 Resp: 229631
Ion Ratio Lower Upper
114 100
63 21.0 0.0 38.6
88 16.2 0.0 32.6

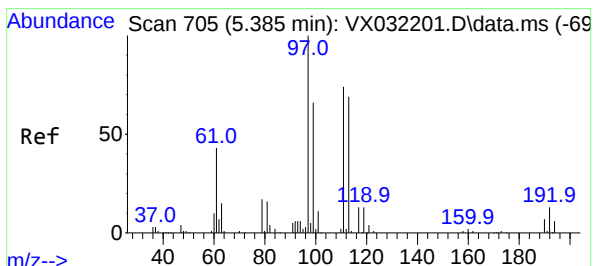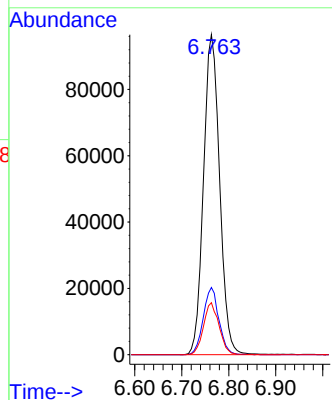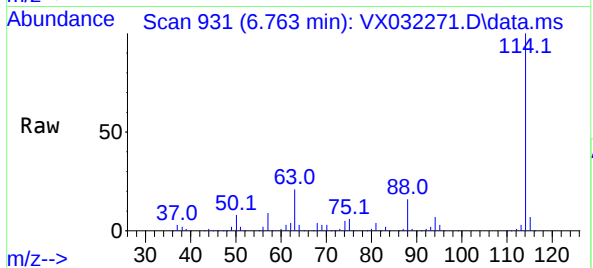

#35
Dibromofluoromethane
Concen: 44.871 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24

Tgt Ion:113 Resp: 71700
Ion Ratio Lower Upper
113 100
111 103.2 82.8 124.2
192 19.3 15.5 23.3


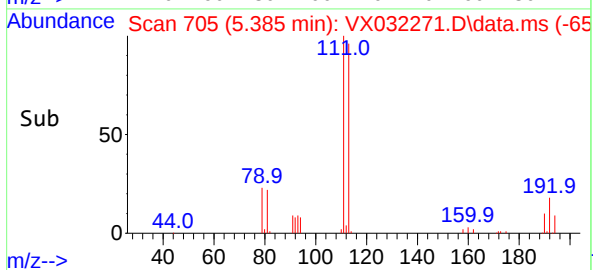
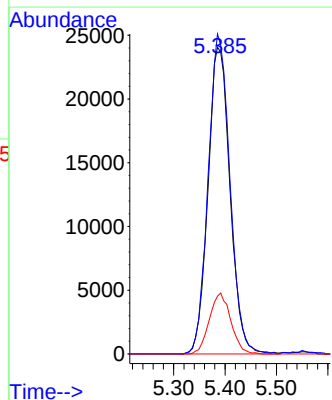





#36
1,1-Dichloropropene
Concen: 5.801 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.146 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24




Instrument :
MSVOA_X
ClientSampleId :
MW-04


Tgt Ion: 75 Resp: 11923
Ion Ratio Lower Upper
75 100
110 10.1 18.4 55.0#
77 0.0 24.7 37.1#

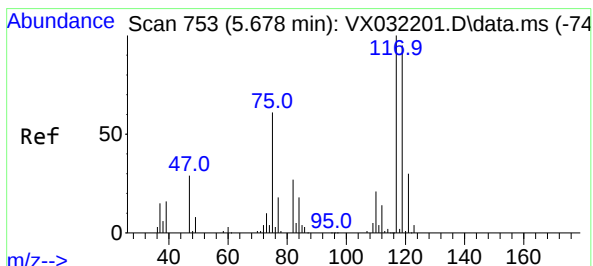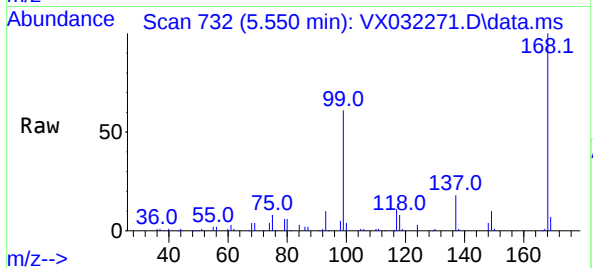

#38
Carbon Tetrachloride
Concen: 7.139 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.128 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24

Tgt Ion: 117 Resp: 15492
Ion Ratio Lower Upper
117 100
119 5.8 75.4 113.0#
121 0.0 23.9 35.9#

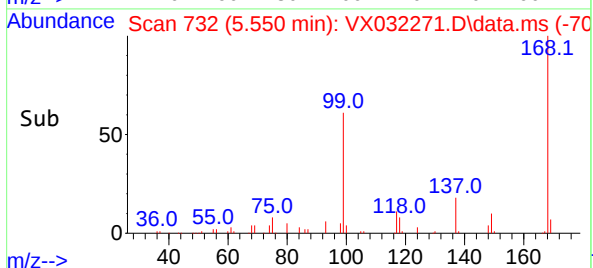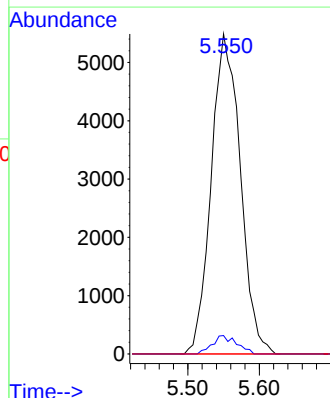

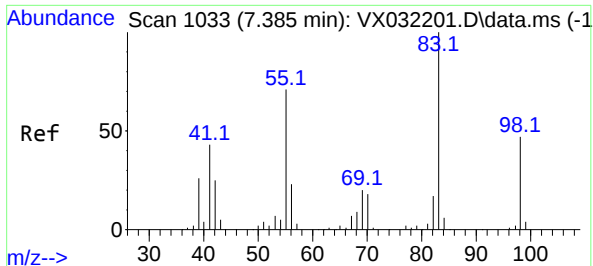

#39

Methylcyclohexane

Concen: 1.275 ug/l

RT: 7.379 min Scan# 1032

Delta R.T. -0.006 min

Lab File: VX032271.D

Acq: 20 Oct 2022 18:24

Instrument :

MSVOA_X

ClientSampleId :

MW-04





Tgt Ion: 83 Resp: 3131

Ion Ratio Lower Upper

83 100

55 86.9 56.6 85.0#

98 45.1 37.4 56.0

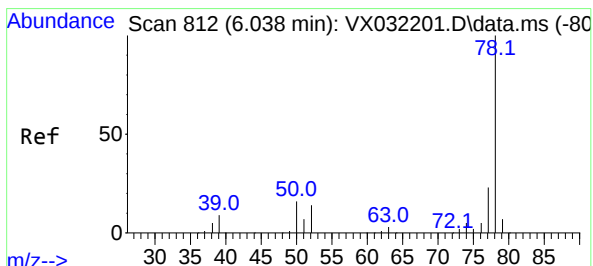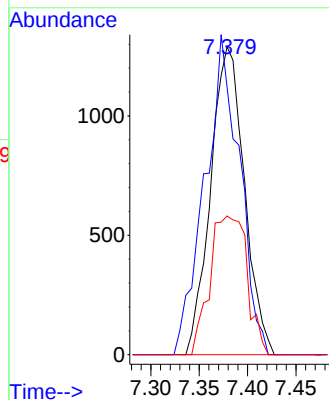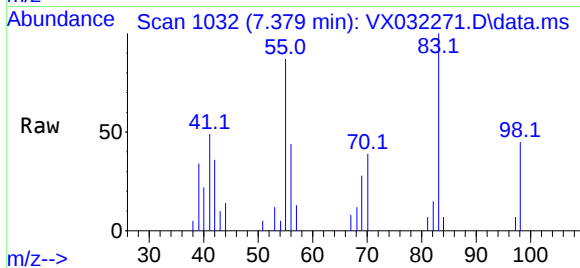

#40

Benzene

Concen: 1.376 ug/l

RT: 6.044 min Scan# 813

Delta R.T. 0.006 min

Lab File: VX032271.D




Acq: 20 Oct 2022 18:24


Tgt Ion: 78 Resp: 8197

Ion Ratio Lower Upper

78 100

77 21.1 18.6 27.8

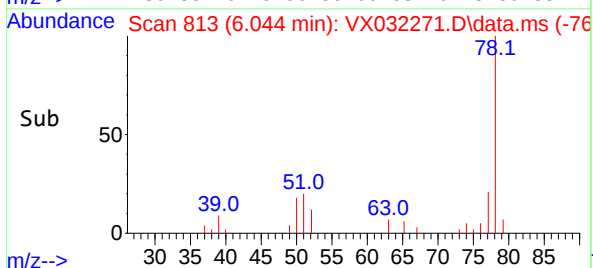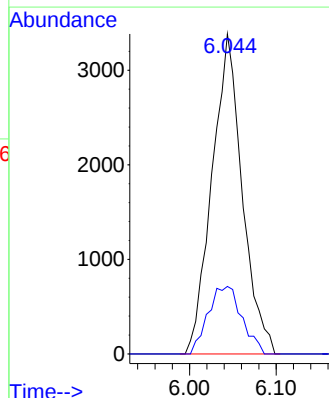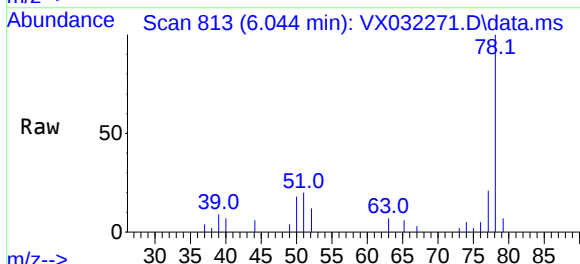

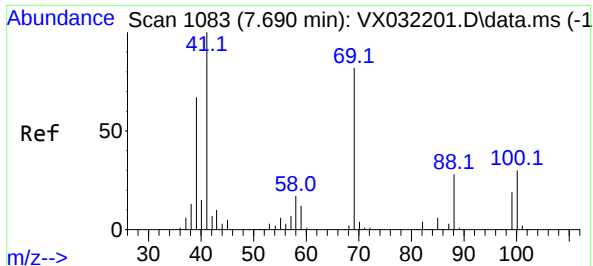

#48

Methyl methacrylate

Concen: 0.329 ug/l

RT: 7.653 min Scan# 1

Delta R.T. -0.037 min

Lab File: VX032271.D

Acq: 20 Oct 2022 18:24

Instrument :

MSVOA_X

ClientSampleId :

MW-04





Tgt Ion: 41 Resp: 519

Ion Ratio Lower Upper

41 100

69 109.4 67.3 100.9#

39 49.1 53.8 80.8#

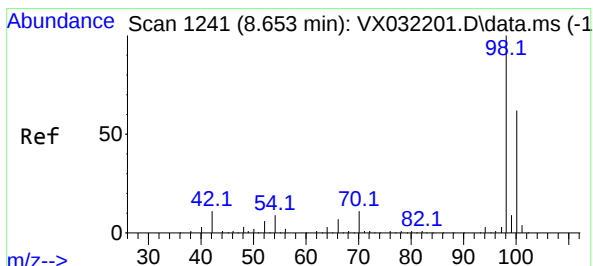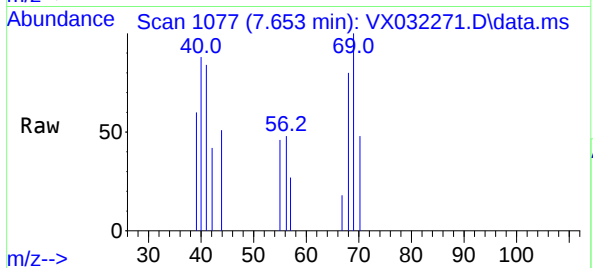

#50

Toluene-d8

Concen: 47.000 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.006 min

Lab File: VX032271.D




Acq: 20 Oct 2022 18:24


Tgt Ion: 98 Resp: 270348

Ion Ratio Lower Upper

98 100

100 63.8 50.7 76.1

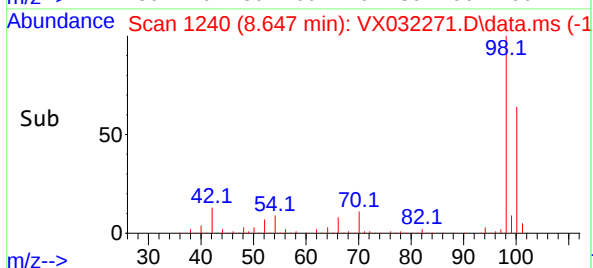

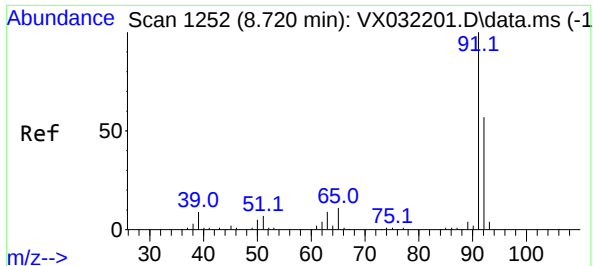

#52

Toluene

Concen: 0.353 ug/l

RT: 8.720 min Scan# 1315

Delta R.T. 0.000 min

Lab File: VX032271.D

Acq: 20 Oct 2022 18:24

Instrument :

MSVOA_X

ClientSampleId :





MW-04

Tgt Ion: 92 Resp: 1364

Ion Ratio Lower Upper

92 100

91 189.4 140.3 210.5

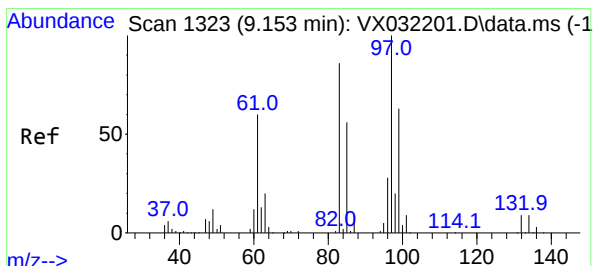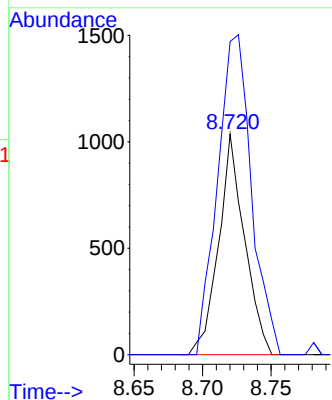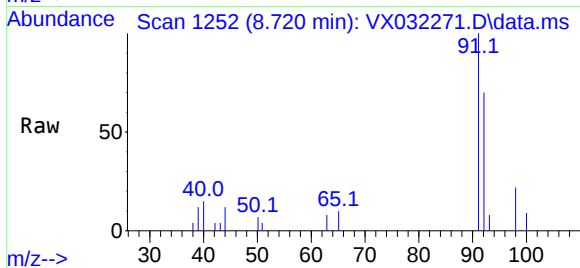

#55

1,1,2-Trichloroethane

Concen: 0.237 ug/l

RT: 9.104 min Scan# 1315

Delta R.T. -0.049 min

Lab File: VX032271.D

Acq: 20 Oct 2022 18:24

Tgt Ion: 97 Resp: 371




Ion Ratio Lower Upper


97 100

83 0.0 68.8 103.2#

85 0.0 44.7 67.1#

99 0.0 50.6 76.0#

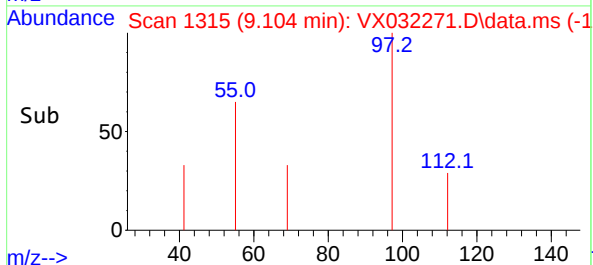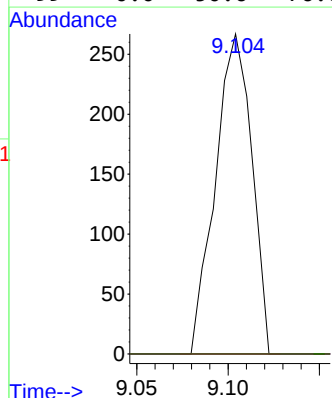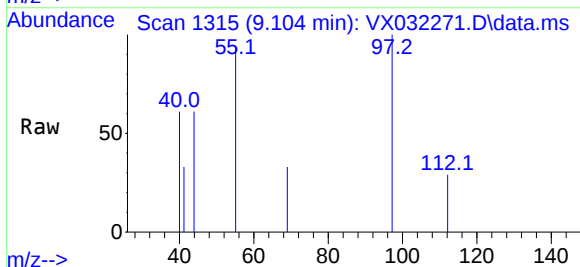



#62

4-Bromofluorobenzene

Concen: 45.079 ug/l

RT: 11.079 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX032271.D

Acq: 20 Oct 2022 18:24

Instrument :

MSVOA_X

ClientSampleId :

MW-04





Tgt Ion: 95 Resp: 94951

Ion Ratio Lower Upper

95 100

174 80.9 0.0 166.8

176 78.9 0.0 161.4



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX032271.D

Acq: 20 Oct 2022 18:24




Tgt Ion: 117 Resp: 198352


Ion Ratio Lower Upper

117 100

82 54.5 44.2 66.4

119 32.4 25.8 38.8


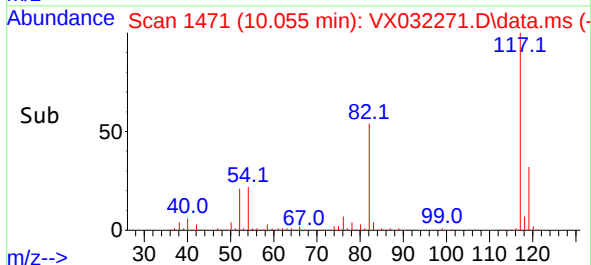
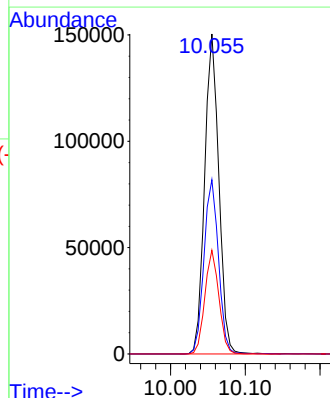
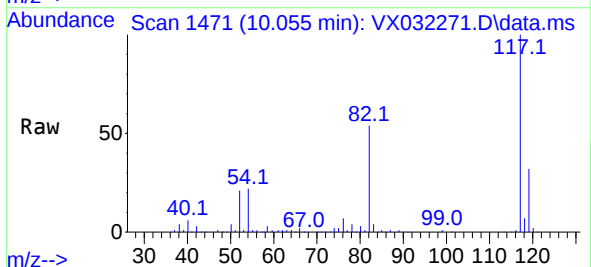




#67
Ethyl Benzene
Concen: 7.008 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24




Instrument :
MSVOA_X
ClientSampleId :
MW-04


Tgt Ion: 91 Resp: 50459
Ion Ratio Lower Upper
91 100
106 31.7 25.0 37.4

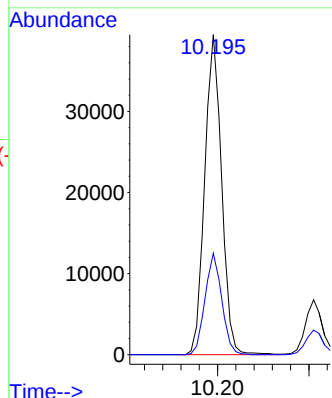

#68
m/p-Xylenes
Concen: 1.408 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24

Tgt Ion: 106 Resp: 4004
Ion Ratio Lower Upper
106 100
91 222.8 162.6 244.0



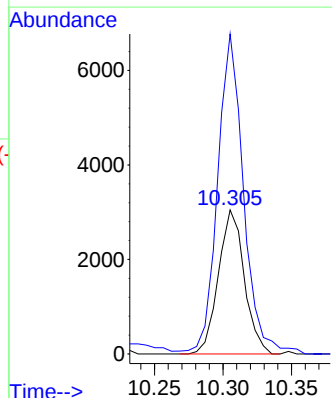
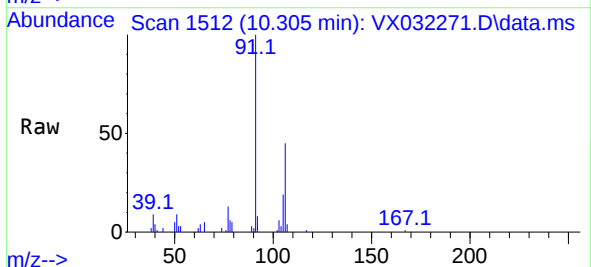




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24




Instrument :
MSVOA_X
ClientSampleId :
MW-04


Tgt Ion:152 Resp: 91424
Ion Ratio Lower Upper
152 100
115 61.7 43.1 129.4
150 158.3 0.0 348.6

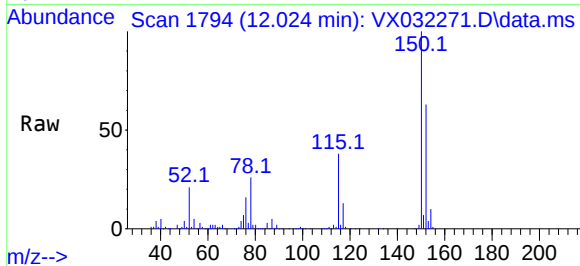

#73
Isopropylbenzene
Concen: 0.967 ug/l
RT: 10.964 min Scan# 1620
Delta R.T. -0.000 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24

Tgt Ion:105 Resp: 6311
Ion Ratio Lower Upper
105 100
120 27.0 13.2 39.6


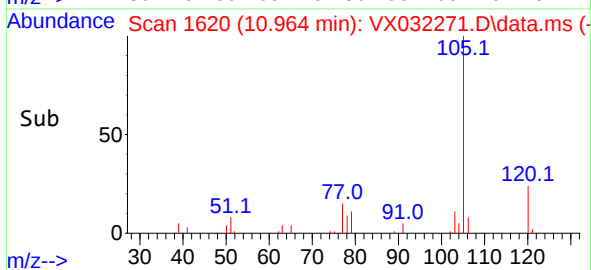

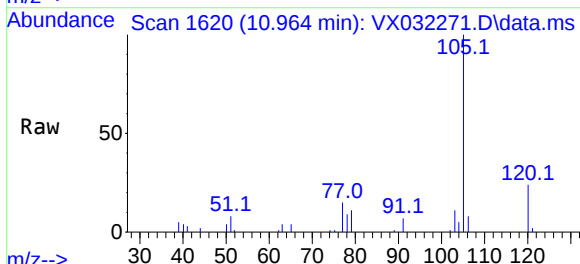




#76
1,2,3-Trichloropropane
Concen: 28.774 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24




Instrument :
MSVOA_X
ClientSampleId :
MW-04


Tgt Ion: 75 Resp: 52124
Ion Ratio Lower Upper
75 100
77 1.0 16.0 47.9#

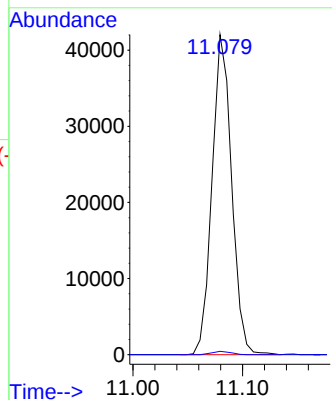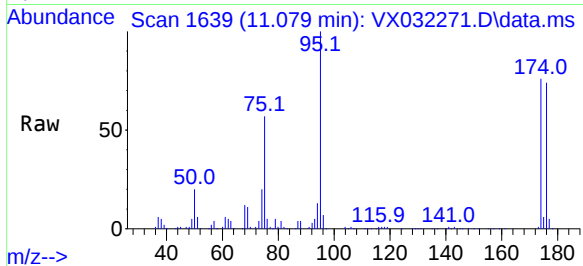

#78
n-propylbenzene
Concen: 1.914 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24

Tgt Ion: 91 Resp: 14298
Ion Ratio Lower Upper
91 100
120 22.8 11.6 34.8



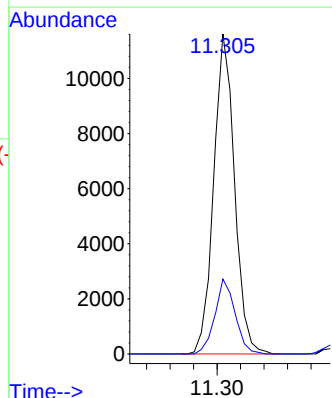
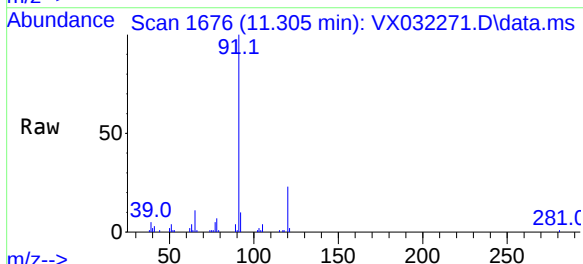




#79
2-Chlorotoluene
Concen: 3.176 ug/l
RT: 11.305 min Scan# 1692
Delta R.T. -0.061 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24




Instrument :
MSVOA_X
ClientSampleId :
MW-04


Tgt Ion: 91 Resp: 14298
Ion Ratio Lower Upper
91 100
126 0.0 17.3 51.9#

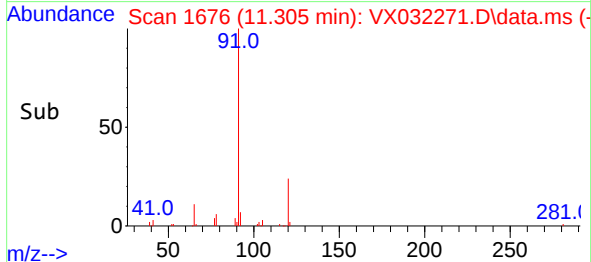

#80
1,3,5-Trimethylbenzene
Concen: 0.393 ug/l
RT: 11.402 min Scan# 1692
Delta R.T. -0.049 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24

Tgt Ion: 105 Resp: 2215
Ion Ratio Lower Upper
105 100
120 32.0 23.5 70.6



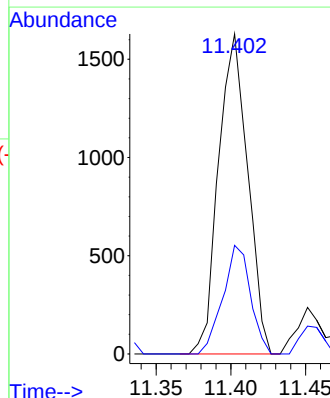





#81
trans-1,4-Dichloro-2-butene
Concen: 88.167 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24




Instrument :
MSVOA_X
ClientSampleId :
MW-04


Tgt Ion: 75 Resp: 52124
Ion Ratio Lower Upper
75 100
53 0.0 87.8 131.8#
89 0.0 37.8 56.8#

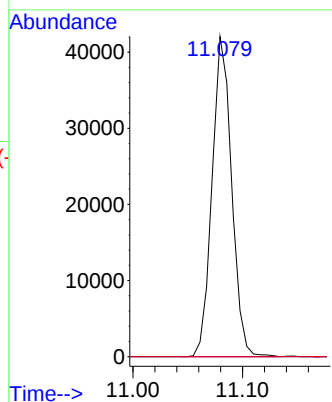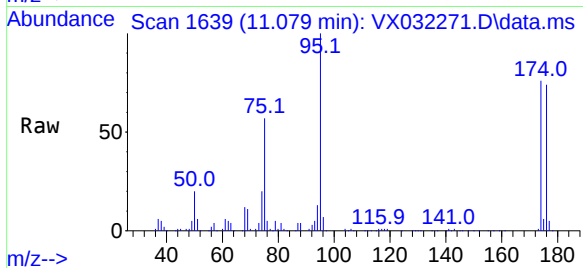

#82
4-Chlorotoluene
Concen: 2.728 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.152 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24

Tgt Ion: 91 Resp: 14298
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#


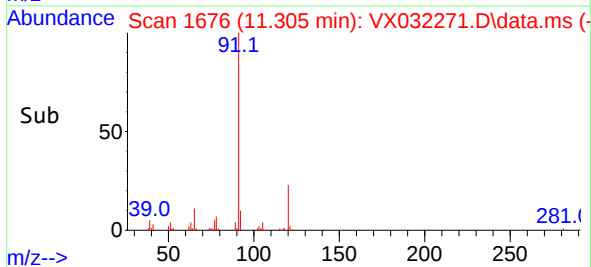
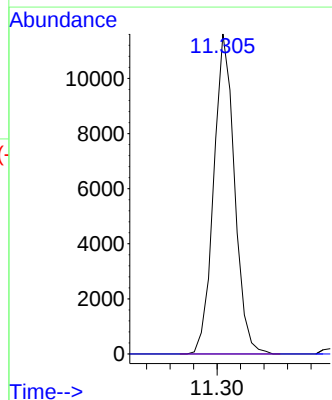
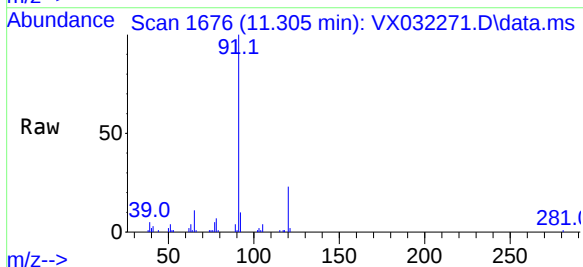




#84
1,2,4-Trimethylbenzene
Concen: 0.343 ug/l
RT: 11.756 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24




Instrument :
MSVOA_X
ClientSampleId :
MW-04


Tgt Ion:105 Resp: 1877
Ion Ratio Lower Upper
105 100
120 45.3 22.1 66.1

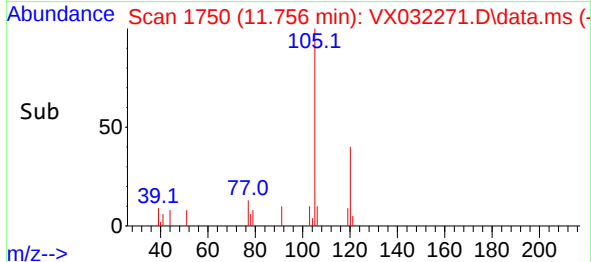

#89
n-Butylbenzene
Concen: 0.268 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24

Tgt Ion: 91 Resp: 1366
Ion Ratio Lower Upper
91 100
92 40.8 26.3 78.9
134 60.1 13.0 39.0#


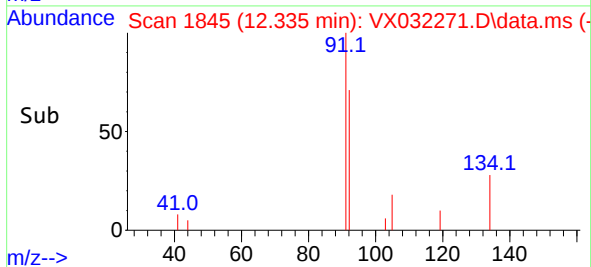

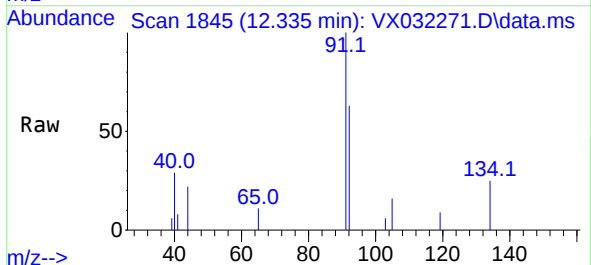




#90
Hexachloroethane
Concen: 0.770 ug/l
RT: 12.646 min Scan# 1896
Delta R.T. 0.103 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24

Instrument :
MSVOA_X
ClientSampleId :
MW-04

Tgt Ion:117 Resp: 693
Ion Ratio Lower Upper
117 100
201 0.0 38.5 115.3#

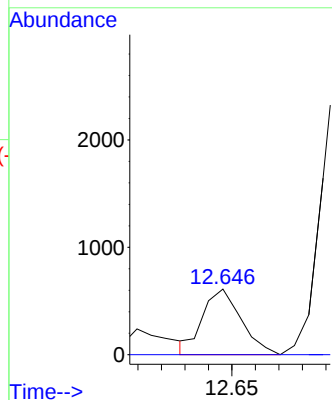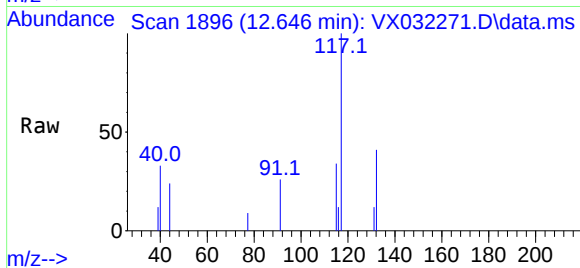

#95
Naphthalene
Concen: 0.928 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX032271.D
Acq: 20 Oct 2022 18:24

Tgt Ion:128 Resp: 5846
Ion Ratio Lower Upper
128 100
127 12.9 10.3 15.5
129 11.8 8.7 13.1

