

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102022\
 Data File : VX032253.D
 Acq On : 20 Oct 2022 11:24
 Operator : JC/MD
 Sample : VX1020MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1020MBL01

Quant Time: Oct 21 01:21:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 19 16:51:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	189603	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	293621	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	252798	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	120358	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	123505	50.072	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	100.140%
35) Dibromofluoromethane	5.379	113	94238	46.122	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.240%
50) Toluene-d8	8.647	98	356387	48.456	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	96.920%
62) 4-Bromofluorobenzene	11.079	95	128016	47.532	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	95.060%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102022\
Data File : VX032253.D
Acq On : 20 Oct 2022 11:24
Operator : JC/MD
Sample : VX1020MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1020MBL01

Quant Time: Oct 21 01:21:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X101922W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 19 16:51:09 2022
Response via : Initial Calibration




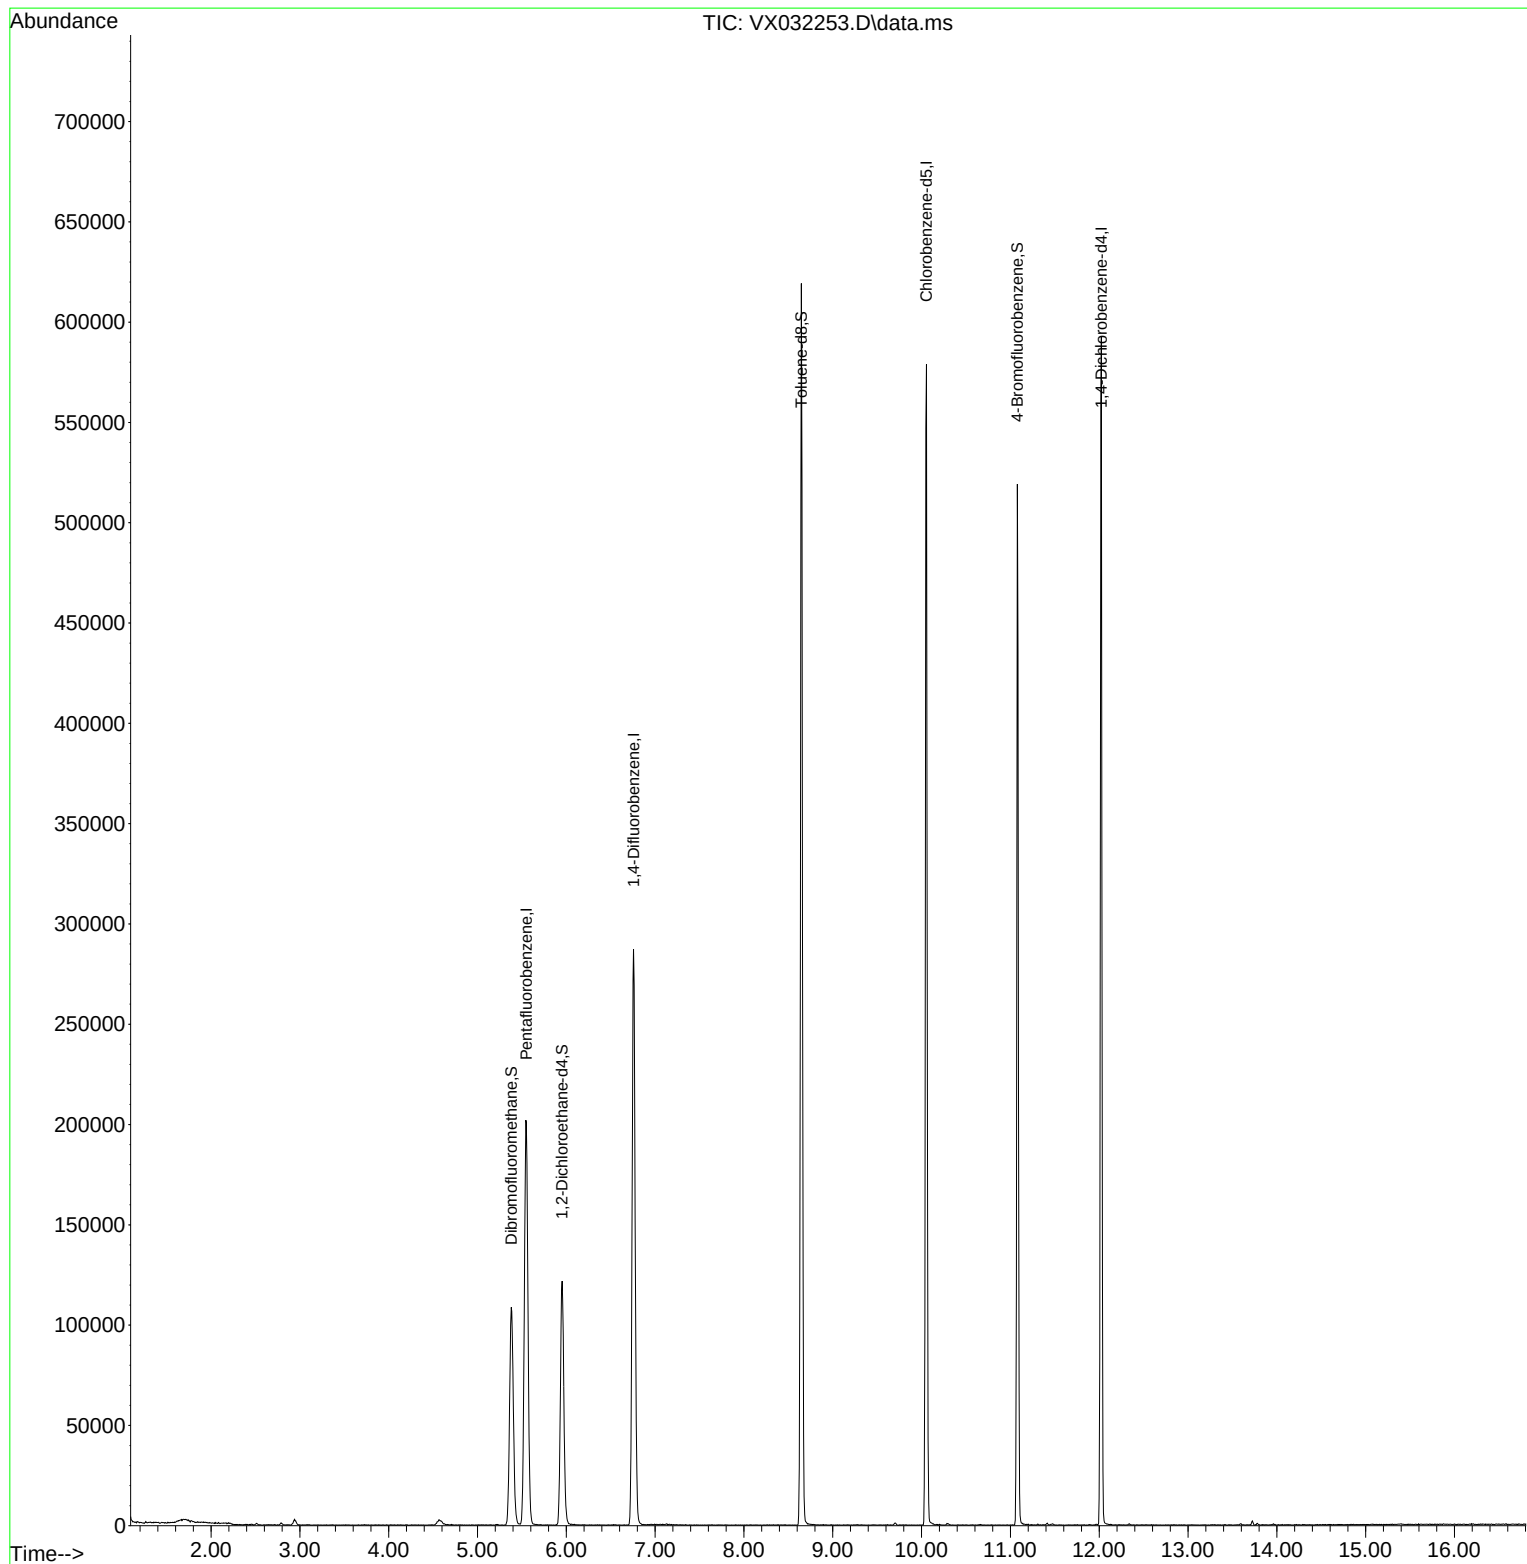


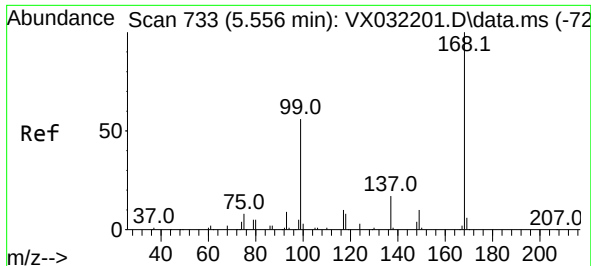

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 713
Delta R.T. -0.006 min
Lab File: VX032253.D
Acq: 20 Oct 2022 11:24




Instrument :
MSVOA_X
ClientSampleId :
VX1020MBL01


Tgt Ion:168 Resp: 189603
Ion Ratio Lower Upper
168 100
99 58.3 44.8 67.2

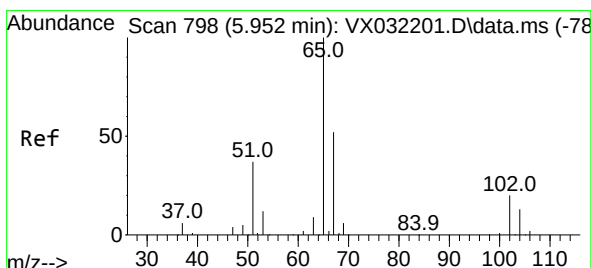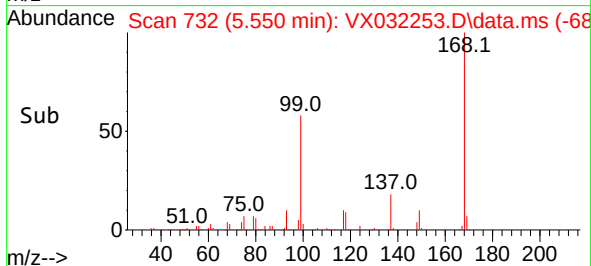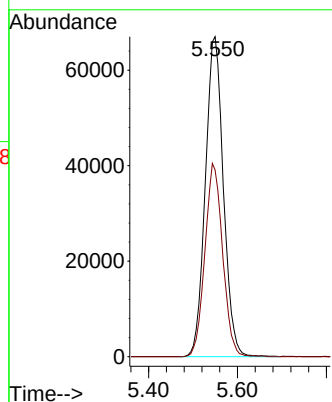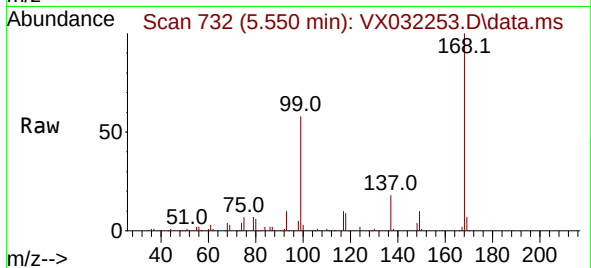

#33
1,2-Dichloroethane-d4
Concen: 50.072 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX032253.D
Acq: 20 Oct 2022 11:24

Tgt Ion: 65 Resp: 123505
Ion Ratio Lower Upper
65 100
67 50.4 0.0 103.6


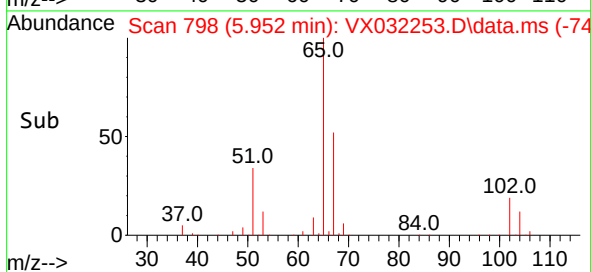
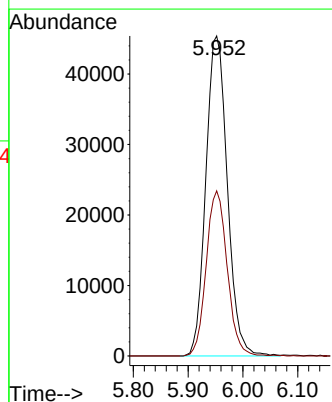
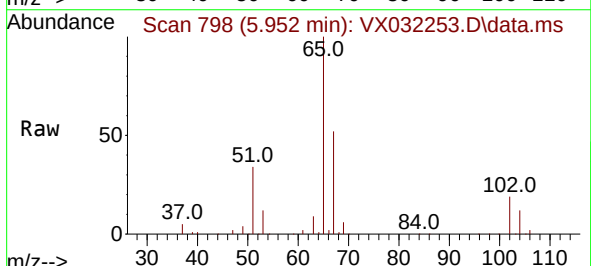


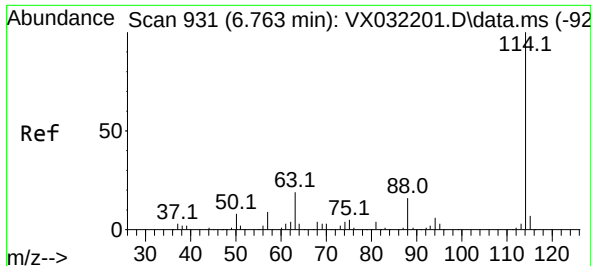

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX032253.D
Acq: 20 Oct 2022 11:24




Instrument :
MSVOA_X
ClientSampleId :
VX1020MBL01


Tgt Ion:114 Resp: 293621
Ion Ratio Lower Upper
114 100
63 19.8 0.0 38.6
88 16.0 0.0 32.6

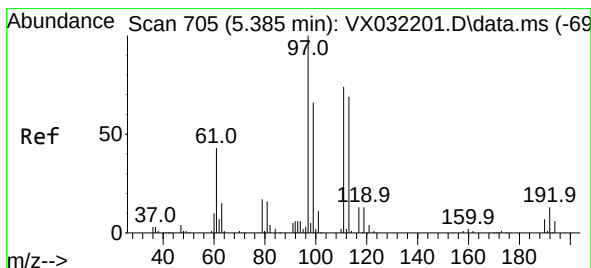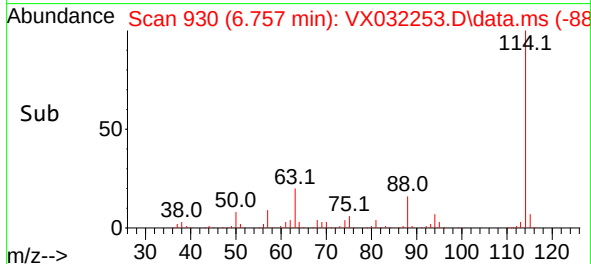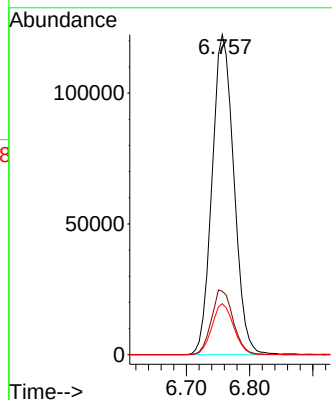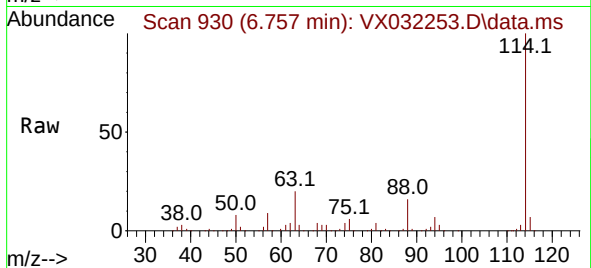

#35
Dibromofluoromethane
Concen: 46.122 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.006 min
Lab File: VX032253.D
Acq: 20 Oct 2022 11:24

Tgt Ion:113 Resp: 94238
Ion Ratio Lower Upper
113 100
111 101.9 82.8 124.2
192 19.2 15.5 23.3


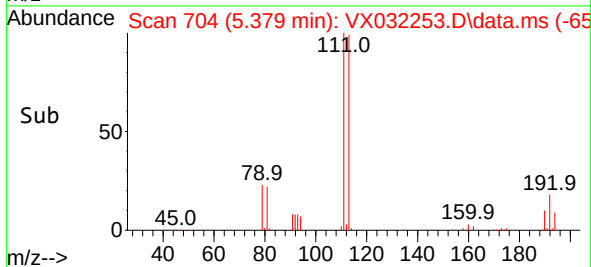
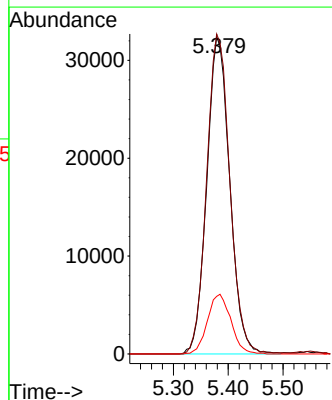
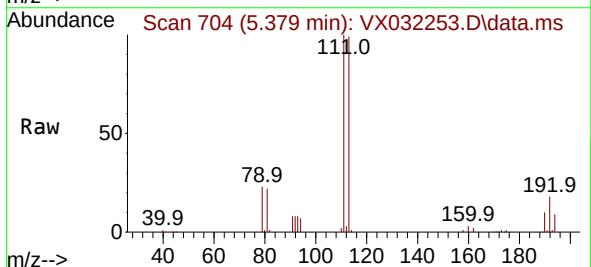


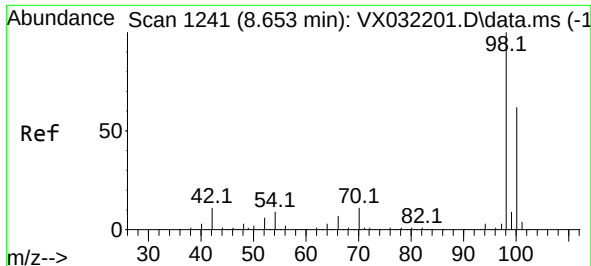

#50
Toluene-d8
Concen: 48.456 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX032253.D
Acq: 20 Oct 2022 11:24




Instrument :
MSVOA_X
ClientSampleId :
VX1020MBL01


Tgt Ion: 98 Resp: 356387
Ion Ratio Lower Upper
98 100
100 63.7 50.7 76.1

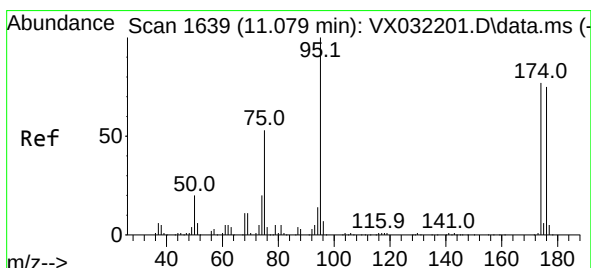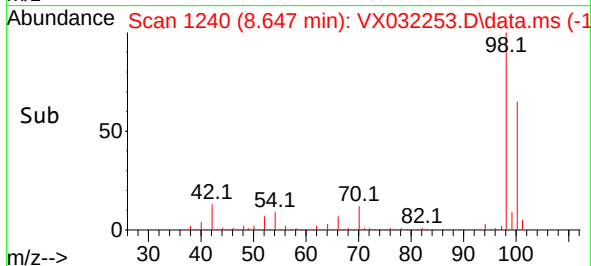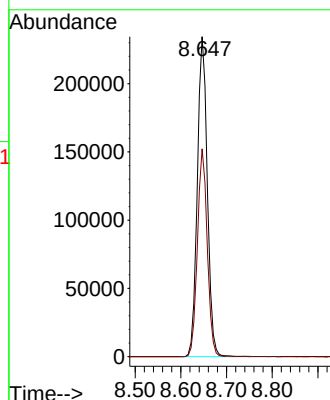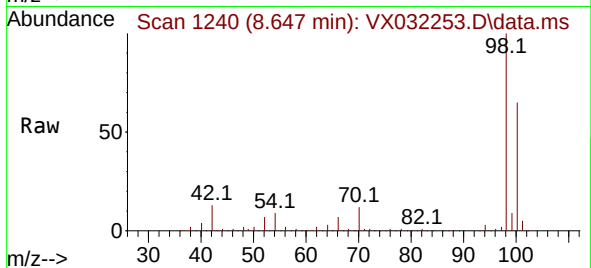

#62
4-Bromofluorobenzene
Concen: 47.532 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX032253.D
Acq: 20 Oct 2022 11:24

Tgt Ion: 95 Resp: 128016
Ion Ratio Lower Upper
95 100
174 78.1 0.0 166.8
176 77.1 0.0 161.4

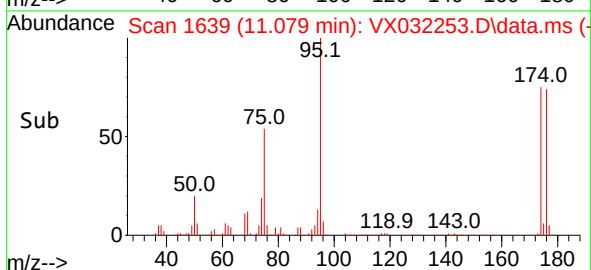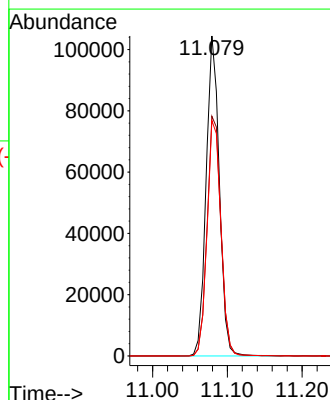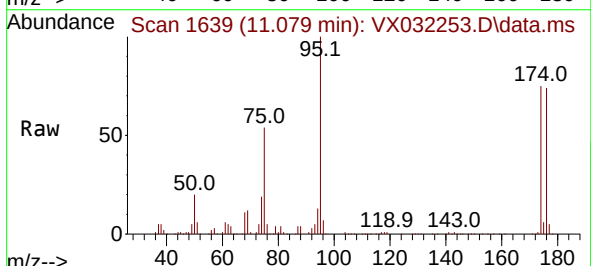

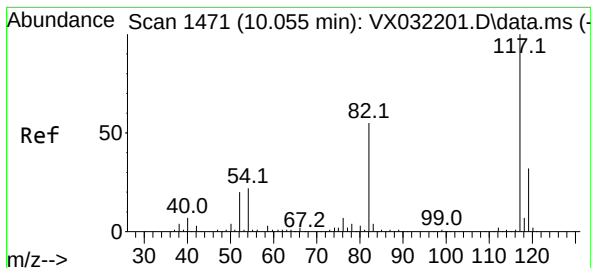

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX032253.D

Acq: 20 Oct 2022 11:24

Instrument :

MSVOA_X

ClientSampleId :

VX1020MBL01





Tgt Ion:117 Resp: 252798

Ion Ratio Lower Upper

117 100

82 55.0 44.2 66.4

119 32.4 25.8 38.8

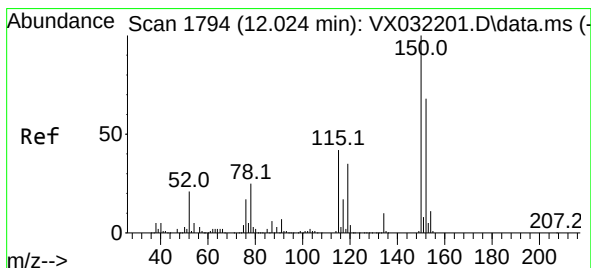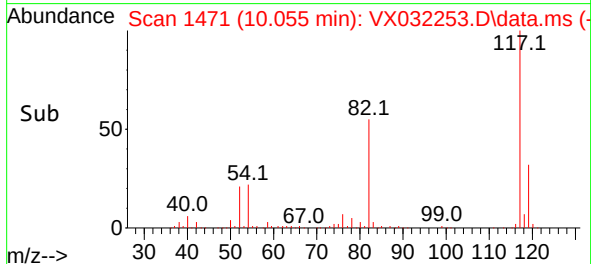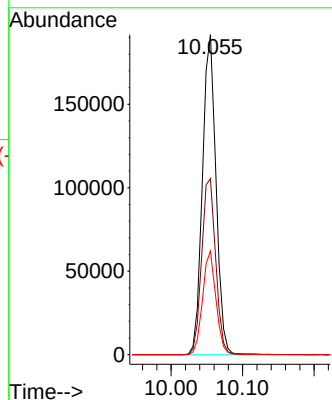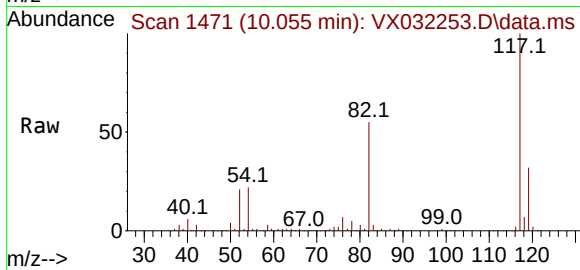

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX032253.D

Acq: 20 Oct 2022 11:24

Tgt Ion:152 Resp: 120358

Ion Ratio Lower Upper

152 100

115 61.3 43.1 129.4

150 155.7 0.0 348.6

